

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS010821\
 Data File : PS013707.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jan 2021 18:03
 Operator : DD\AJ
 Sample : PB134013BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 08 22:29:34 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010421.M
 Quant Title : 8080.M
 QLast Update : Tue Jan 05 01:51:07 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.210	6.912	465.5E6	231.7E6	487.163	576.291
Target Compounds							
1) T	Dalapon	2.988f	2.587	78244908	102.1E6	71.941	196.312 #
2) T	3,5-DICHL...	0.000	6.094	0	31565703	N.D.	50.104
3) T	4-Nitroph...	6.983f	0.000	8101966	0	17.041	N.D. #
5) T	DICAMBA	0.000	7.045	0	6676905	N.D.	3.888
7) T	MCPA	0.000	7.369	0	27948353	N.D.	13.824
10) T	Pentachlo...	8.682f	0.000	12908368	0	<MDL	N.D. #
11) T	2,4,5-TP ...	0.000	8.760	0	11131209	N.D.	4.660
12) T	2,4,5-T	9.399f	0.000	36064621	0	6.378	N.D. #
14) T	DINOSEB	11.145	10.017	39176966	5368669	8.880	3.208 #
15) T	Picloram	11.048f	11.037f	97215962	70250022	13.460	20.213 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS010821\
Data File : PS013707.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Jan 2021 18:03
Operator : DD\AJ
Sample : PB134013BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 08 22:29:34 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010421.M
Quant Title : 8080.M
QLast Update : Tue Jan 05 01:51:07 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

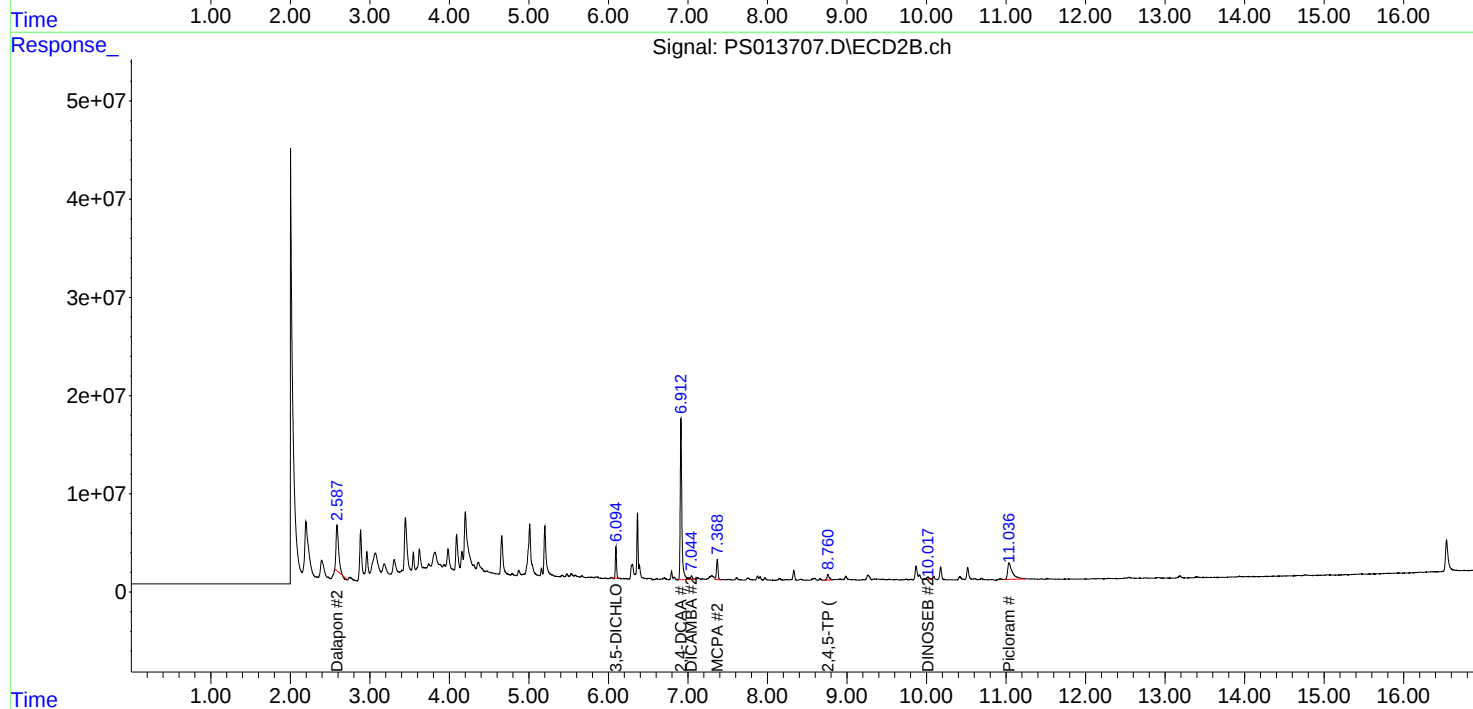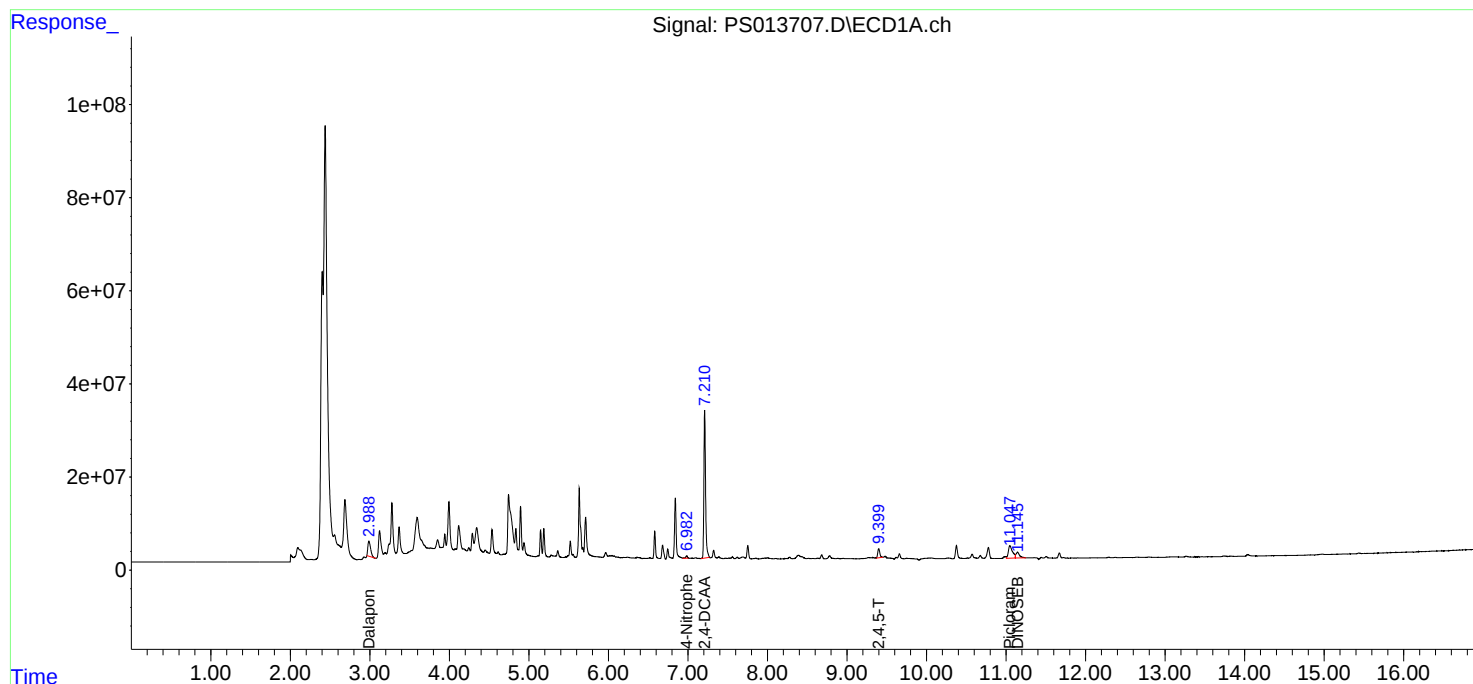


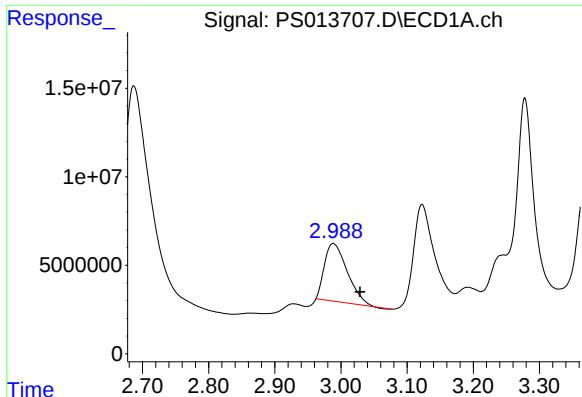

#1 Dalapon


R.T.: 2.988 min
Delta R.T.: -0.041 min
Response: 78244908
Conc: 71.94 ng/ml

Instrument :
ECD_S
ClientSampleId :

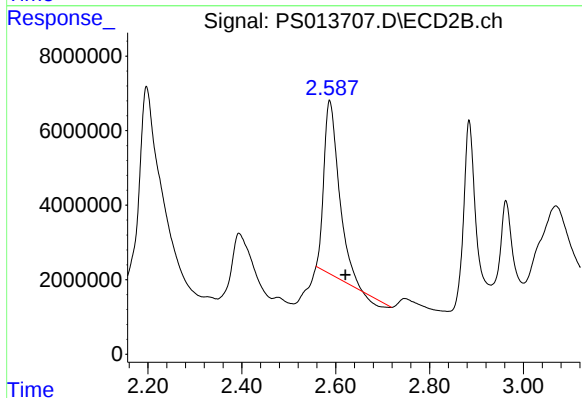


#1 Dalapon

R.T.: 2.587 min
Delta R.T.: -0.034 min
Response: 102072204
Conc: 196.31 ng/ml

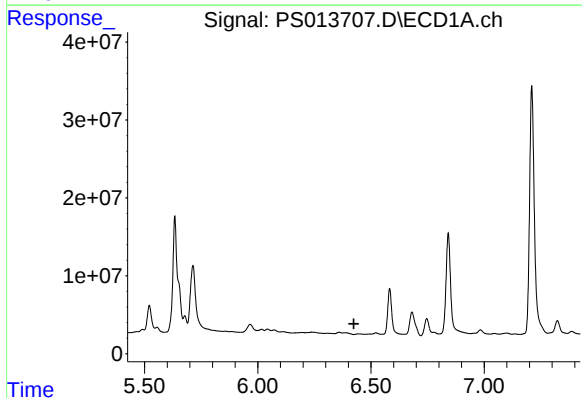


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.425 min
Response: 0
Conc: N.D.

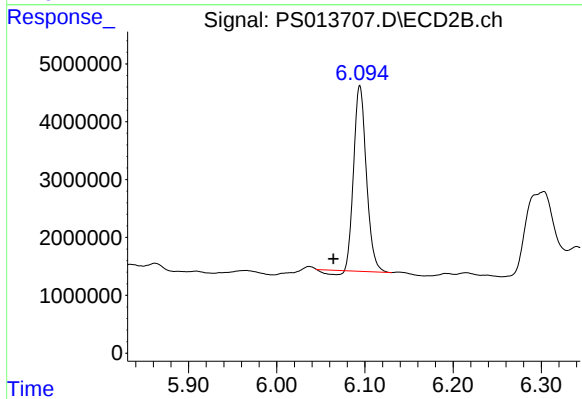

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.094 min
Delta R.T.: 0.030 min
Response: 31565703
Conc: 50.10 ng/ml

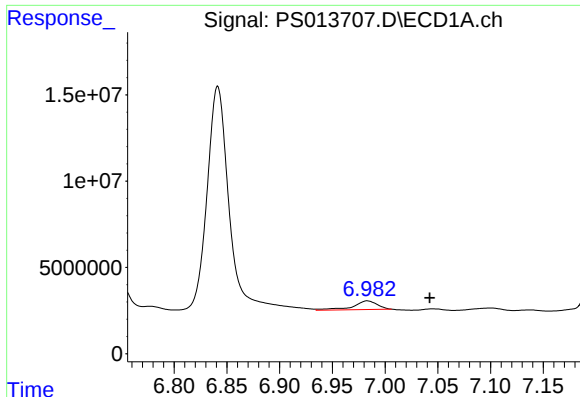

#3 4-Nitrophenol


R.T.: 6.983 min
Delta R.T.: -0.059 min
Response: 8101966
Conc: 17.04 ng/ml

Instrument :
ECD_S
ClientSampleId :

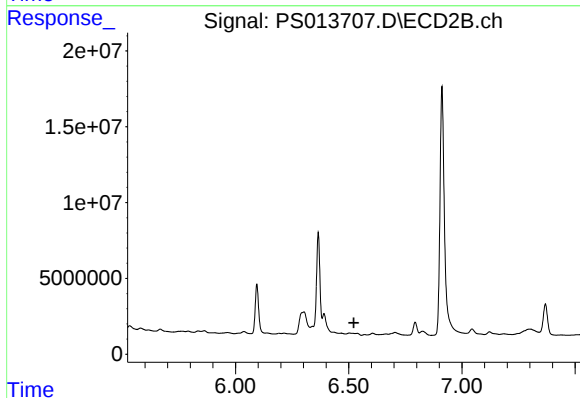


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.523 min
Response: 0
Conc: N.D.

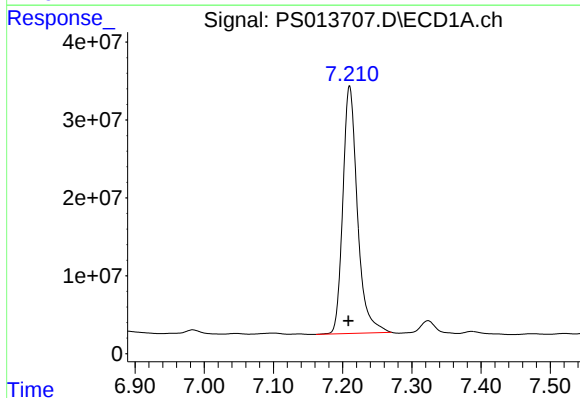


#4 2,4-DCAA

R.T.: 7.210 min
Delta R.T.: 0.002 min
Response: 465529552
Conc: 487.16 ng/ml

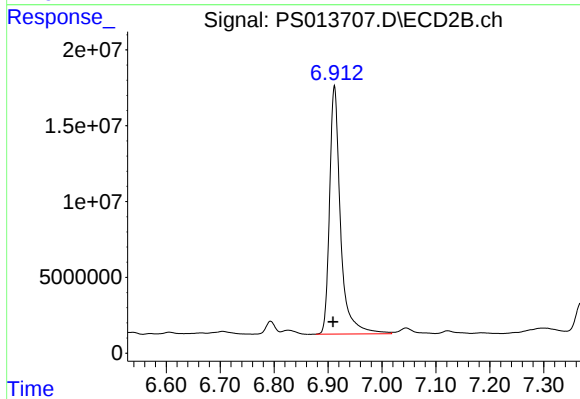

#4 2,4-DCAA


R.T.: 6.912 min
Delta R.T.: 0.002 min
Response: 231735426
Conc: 576.29 ng/ml

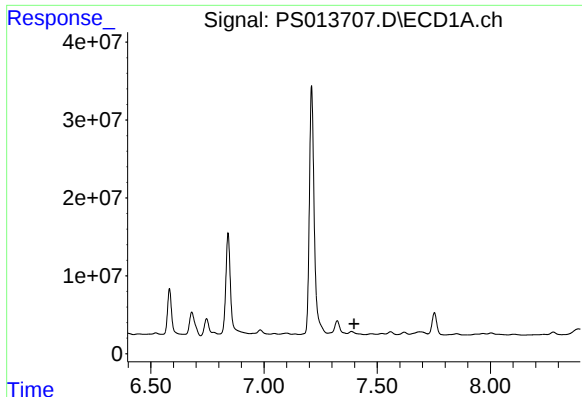

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 7.397 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

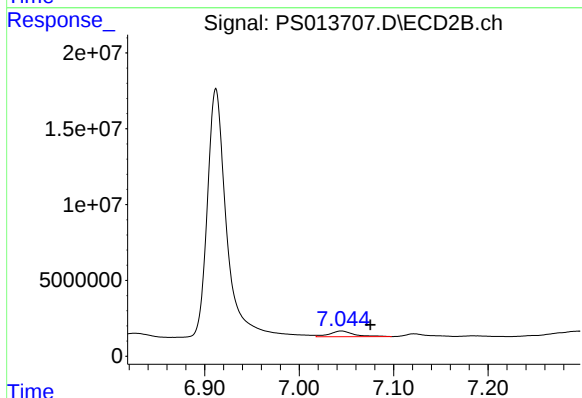


#5 DICAMBA

R.T.: 7.045 min
Delta R.T.: -0.031 min
Response: 6676905
Conc: 3.89 ng/ml

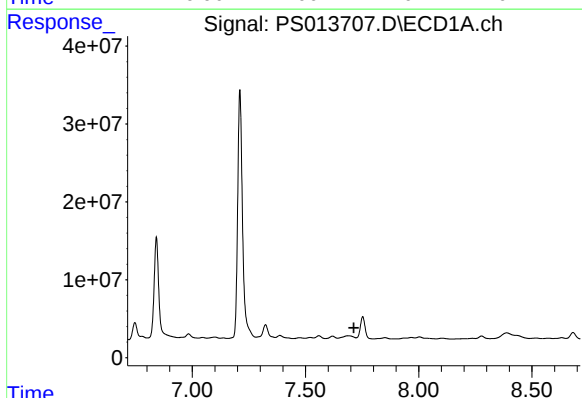


#7 MCPA

R.T.: 0.000 min
Exp R.T.: 7.713 min
Response: 0
Conc: N.D.

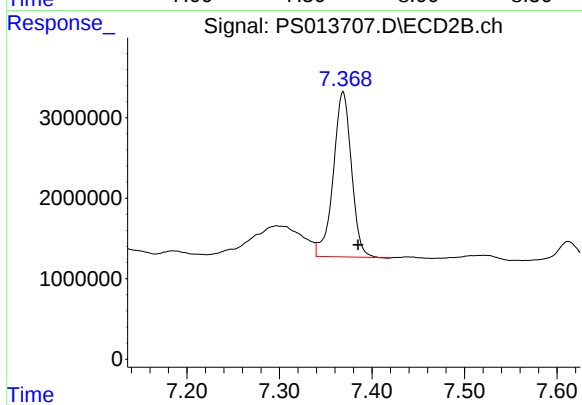

#7 MCPA


R.T.: 7.369 min
Delta R.T.: -0.016 min
Response: 27948353
Conc: 13.82 ug/ml

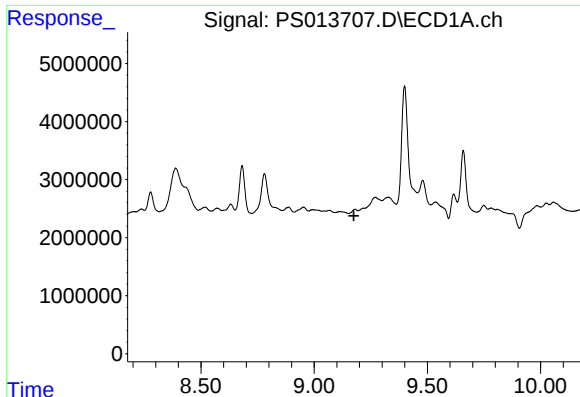

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 9.175 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

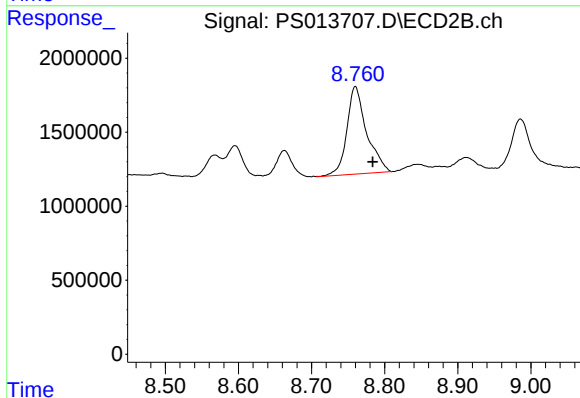


#11 2,4,5-TP (SILVEX)

R.T.: 8.760 min
Delta R.T.: -0.024 min
Response: 11131209
Conc: 4.66 ng/ml

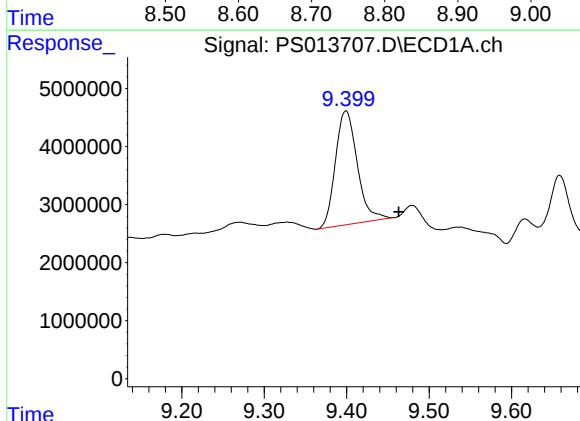


#12 2,4,5-T

R.T.: 9.399 min
Delta R.T.: -0.064 min
Response: 36064621
Conc: 6.38 ng/ml

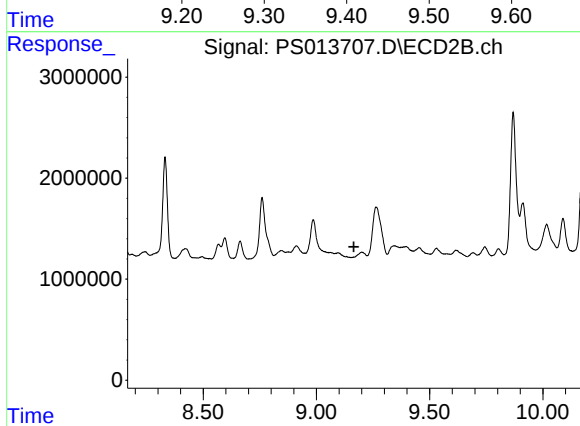

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 9.165 min
Response: 0
Conc: N.D.

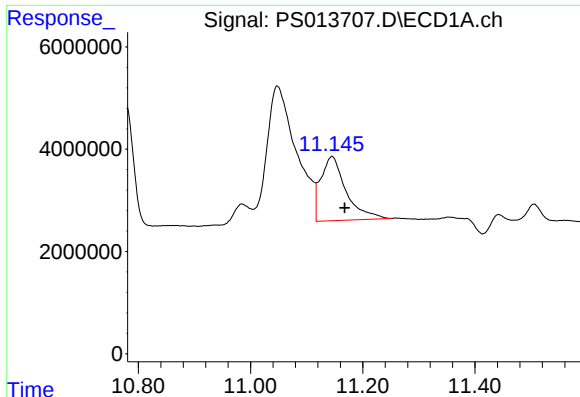

#14 DINOSEB


R.T.: 11.145 min
Delta R.T.: -0.022 min
Response: 39176966
Conc: 8.88 ng/ml

Instrument :
ECD_S
ClientSampleId :

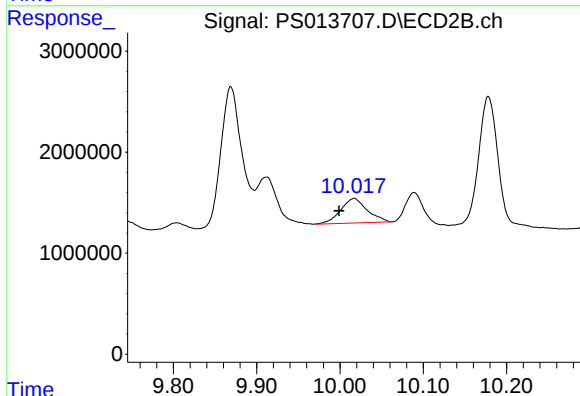


#14 DINOSEB

R.T.: 10.017 min
Delta R.T.: 0.018 min
Response: 5368669
Conc: 3.21 ng/ml

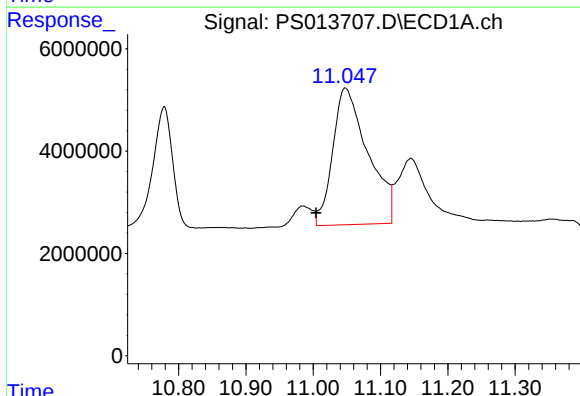

#15 Picloram

R.T.: 11.048 min
Delta R.T.: 0.044 min
Response: 97215962
Conc: 13.46 ng/ml

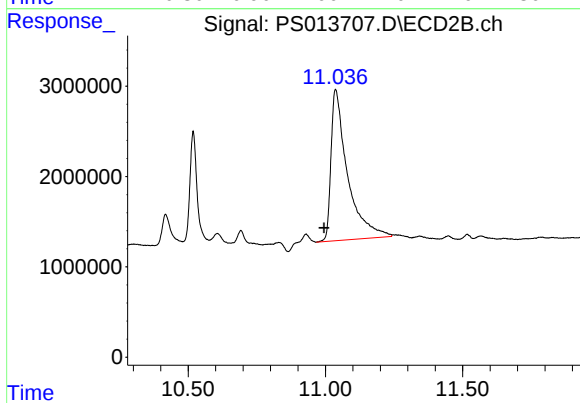

#15 Picloram

R.T.: 11.037 min
Delta R.T.: 0.042 min
Response: 70250022
Conc: 20.21 ng/ml