

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS010923\
 Data File : PS021660.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Jan 2023 13:43
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 09 16:48:28 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010923.M
 Quant Title : 8080.M
 QLast Update : Mon Jan 09 16:45:07 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.382	6.814	1235.1E6	993.6E6	443.729	553.030
Target Compounds							
1) T	Dalapon	2.520f	0.000	589196	0	1.709	N.D. #
2) T	3,5-DICHL...	5.804f	0.000	745268	0	<MDL	N.D. #
3) T	4-Nitroph...	6.236	0.000	5000145	0	3.430	N.D. #
7) T	MCPA	6.780	7.225f	-2225961	39483722	N.D.	4.353
10) T	Pentachlo...	7.571	0.000	406899	0	<MDL	N.D. #
11) T	2,4,5-TP ...	8.063	8.693	5498484	1840238	<MDL	<MDL #
12) T	2,4,5-T	8.371	0.000	7095272	0	<MDL	N.D. #
13) T	2,4-DB	8.859	0.000	4743120	0	1.498	N.D. #
14) T	DINOSEB	9.882	0.000	31286138	0	1.906	N.D. #
15) T	Picloram	9.774	10.926f	568364	32666857	<MDL	1.845 #
16) T	DCPA	10.172	0.000	695616	0	<MDL	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS010923\
Data File : PS021660.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Jan 2023 13:43
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 09 16:48:28 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010923.M
Quant Title : 8080.M
QLast Update : Mon Jan 09 16:45:07 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

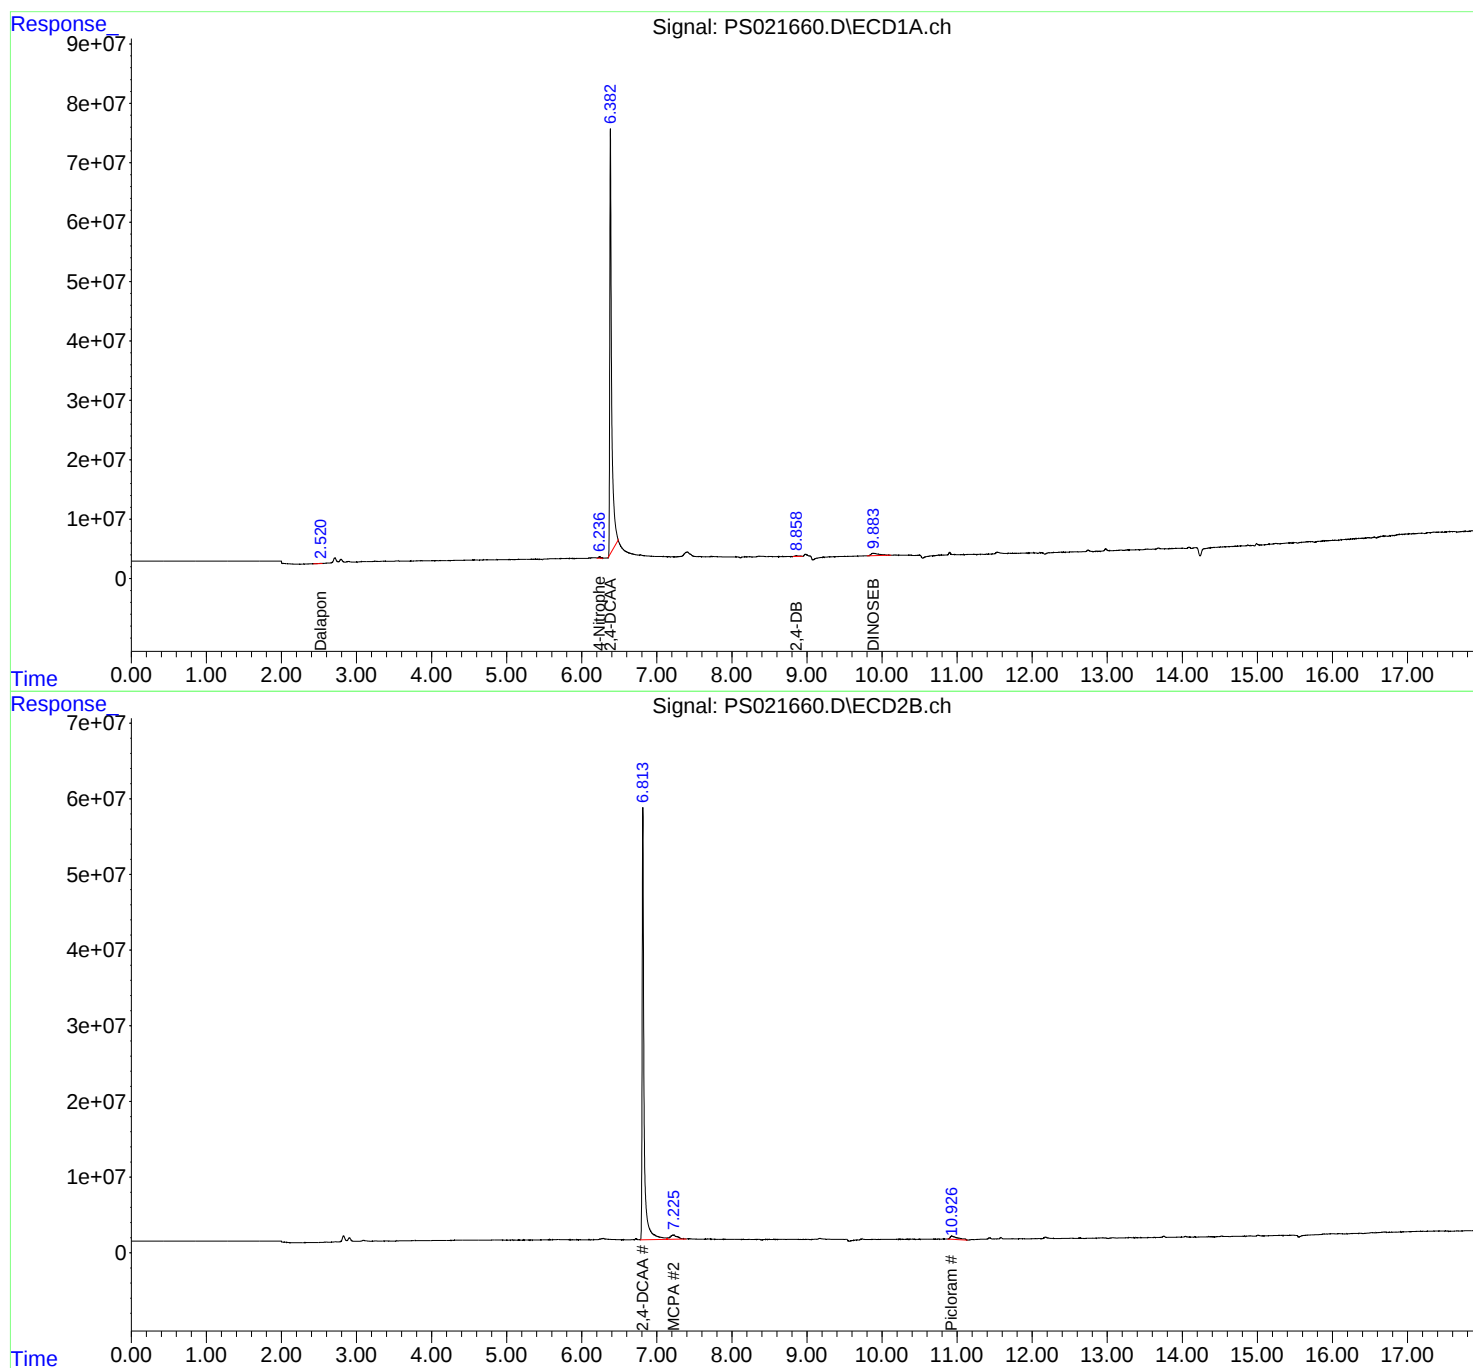


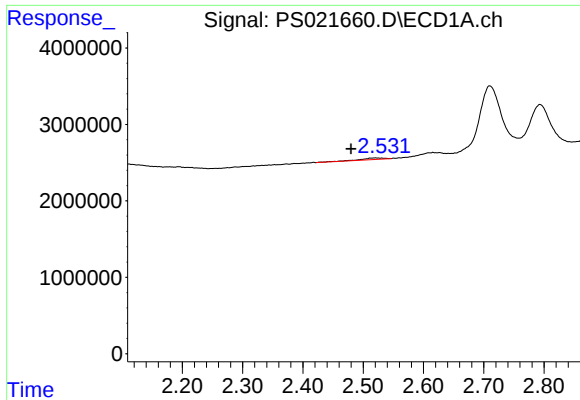

#1 Dalapon


R.T.: 2.520 min
Delta R.T.: 0.040 min
Response: 589196
Conc: 1.71 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

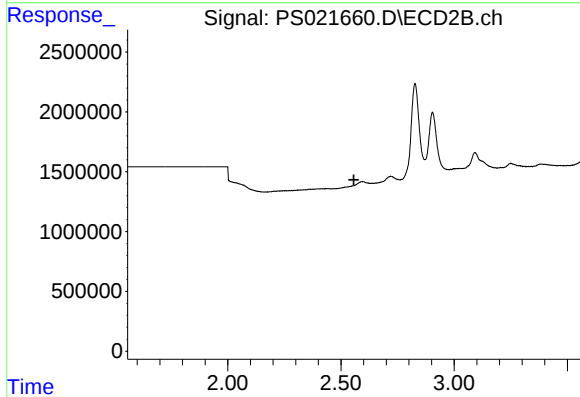


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 2.557 min
Response: 0
Conc: N.D.

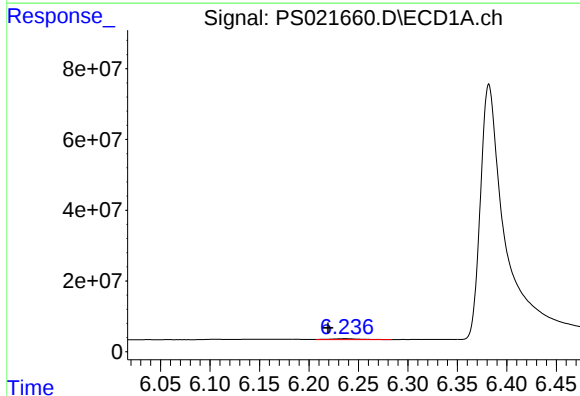


#3 4-Nitrophenol

R.T.: 6.236 min
Delta R.T.: 0.017 min
Response: 5000145
Conc: 3.43 ng/ml

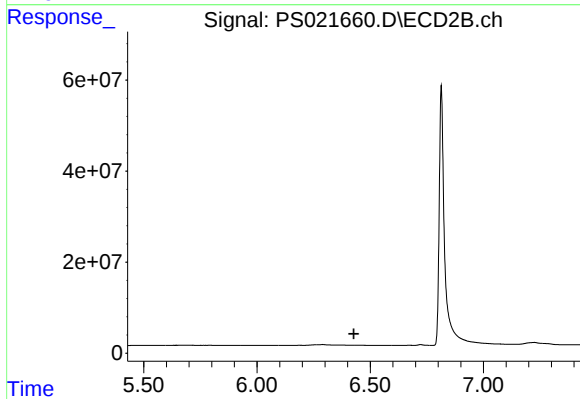

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T. : 6.428 min
Response: 0
Conc: N.D.

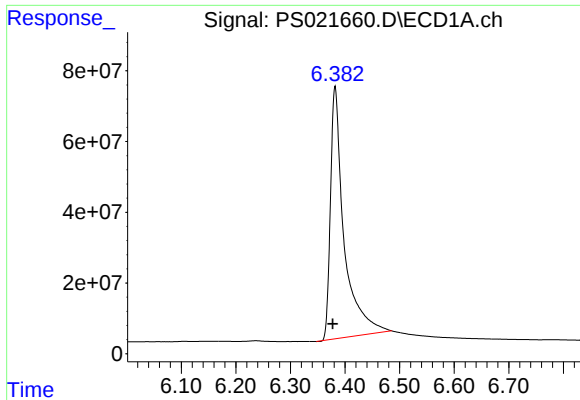

#4 2,4-DCAA


R.T.: 6.382 min
Delta R.T.: 0.005 min
Response: 1235149218
Conc: 443.73 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

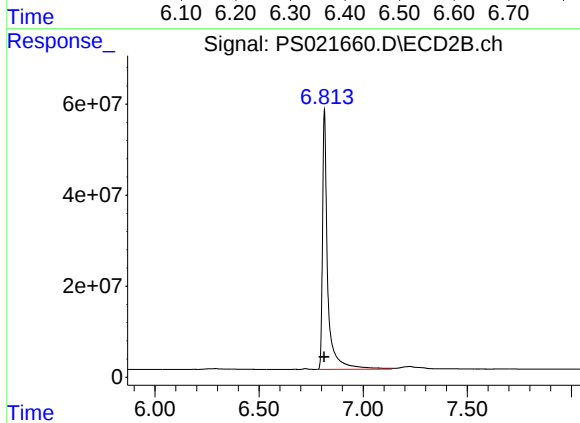


#4 2,4-DCAA

R.T.: 6.814 min
Delta R.T.: 0.002 min
Response: 993623121
Conc: 553.03 ng/ml

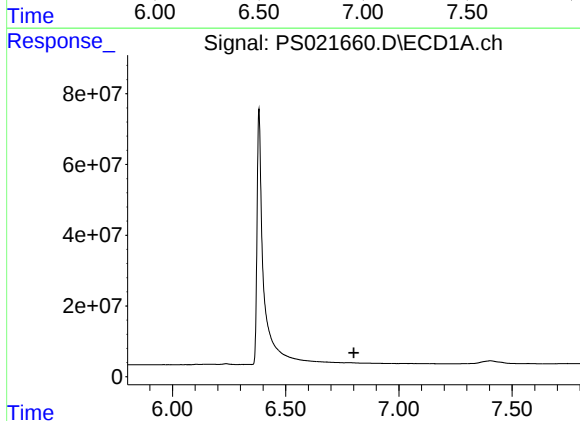


#7 MCPA

R.T.: 6.780 min
Delta R.T.: -0.021 min
Response: -2225961
Conc: N.D.

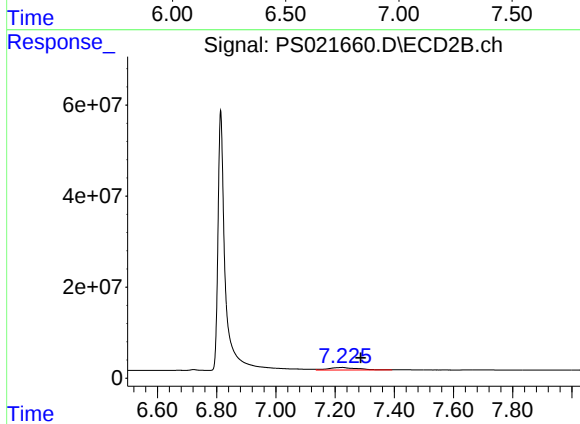

#7 MCPA


R.T.: 7.225 min
Delta R.T.: -0.062 min
Response: 39483722
Conc: 4.35 ug/ml

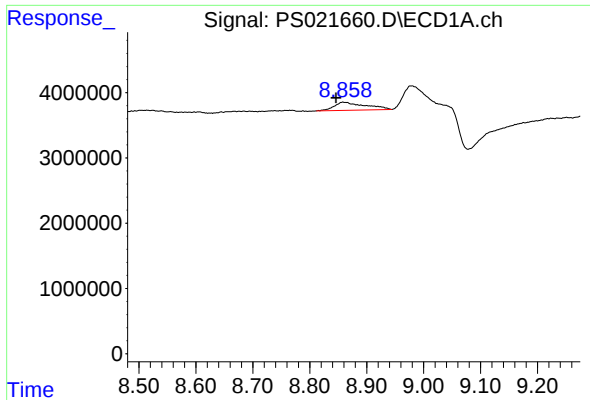

#13 2,4-DB


R.T.: 8.859 min
Delta R.T.: 0.013 min
Response: 4743120
Conc: 1.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

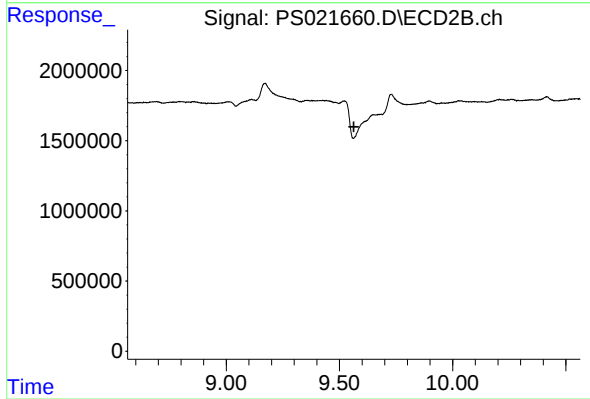


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 9.564 min
Response: 0
Conc: N.D.

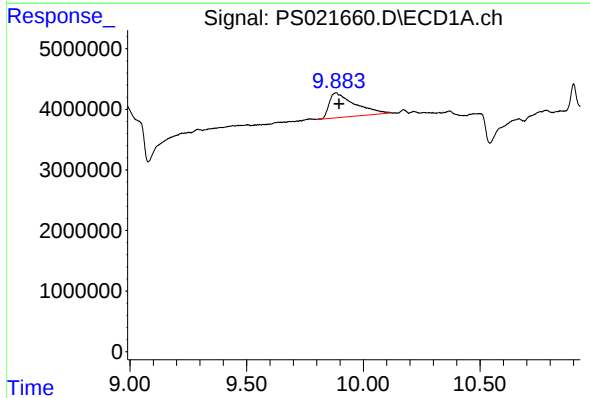


#14 DINOSEB

R.T.: 9.882 min
Delta R.T.: -0.014 min
Response: 31286138
Conc: 1.91 ng/ml

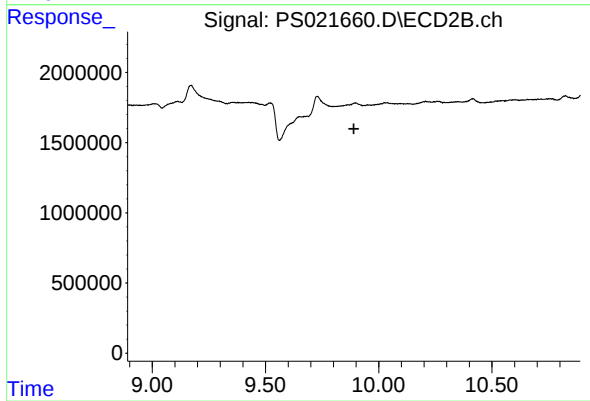

#14 DINOSEB


R.T.: 0.000 min
Exp R.T. : 9.890 min
Response: 0
Conc: N.D.

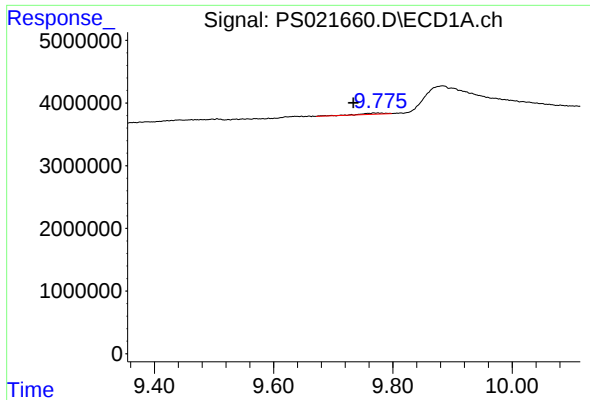

#15 Picloram

R.T.: 9.774 min
Delta R.T.: 0.040 min
Response: 568364
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

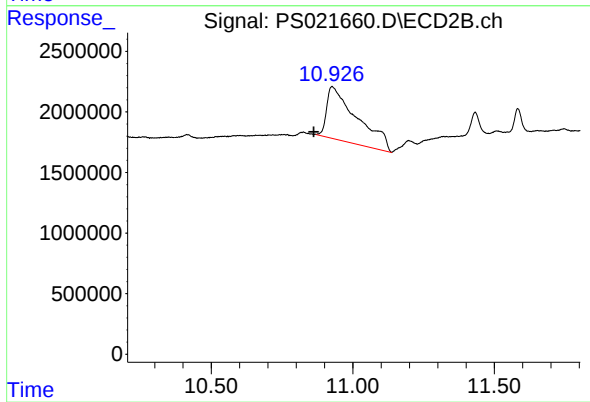

#15 Picloram

R.T.: 10.926 min
Delta R.T.: 0.064 min
Response: 32666857
Conc: 1.84 ng/ml