

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS010923\
 Data File : PS021679.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Jan 2023 21:22
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 10 05:53:17 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010923.M
 Quant Title : 8080.M
 QLast Update : Mon Jan 09 16:45:07 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.379	6.813	1304.9E6	995.5E6	468.791	554.099
Target Compounds							
1) T	Dalapon	2.521f	0.000	611316	0	1.717	N.D. #
2) T	3,5-DICHL...	5.807f	0.000	178615	0	<MDL	N.D. #
3) T	4-Nitroph...	6.229	0.000	6734892	0	4.620	N.D. #
7) T	MCPA	6.767	7.219f	1945891	33799360	<MDL	3.727 #
8) T	DICHLORPROP	7.061f	0.000	146290	0	<MDL	N.D. #
10) T	Pentachlo...	7.559	8.327	1174022	3398553	<MDL	<MDL #
11) T	2,4,5-TP ...	8.088	8.700	4093271	13710129	<MDL	1.153 #
12) T	2,4,5-T	8.339	9.096	14244932	23011855	<MDL	2.060 #
13) T	2,4-DB	8.856	9.516f	782044	3660142	<MDL	2.443 #
14) T	DINOSEB	9.884	9.900	10033676	4829508	<MDL	<MDL #
15) T	Picloram	0.000	10.862	0	5183734	N.D.	<MDL
16) T	DCPA	10.169	10.823	754307	6624261	<MDL	<MDL #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS010923\
Data File : PS021679.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Jan 2023 21:22
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 10 05:53:17 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010923.M
Quant Title : 8080.M
QLast Update : Mon Jan 09 16:45:07 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

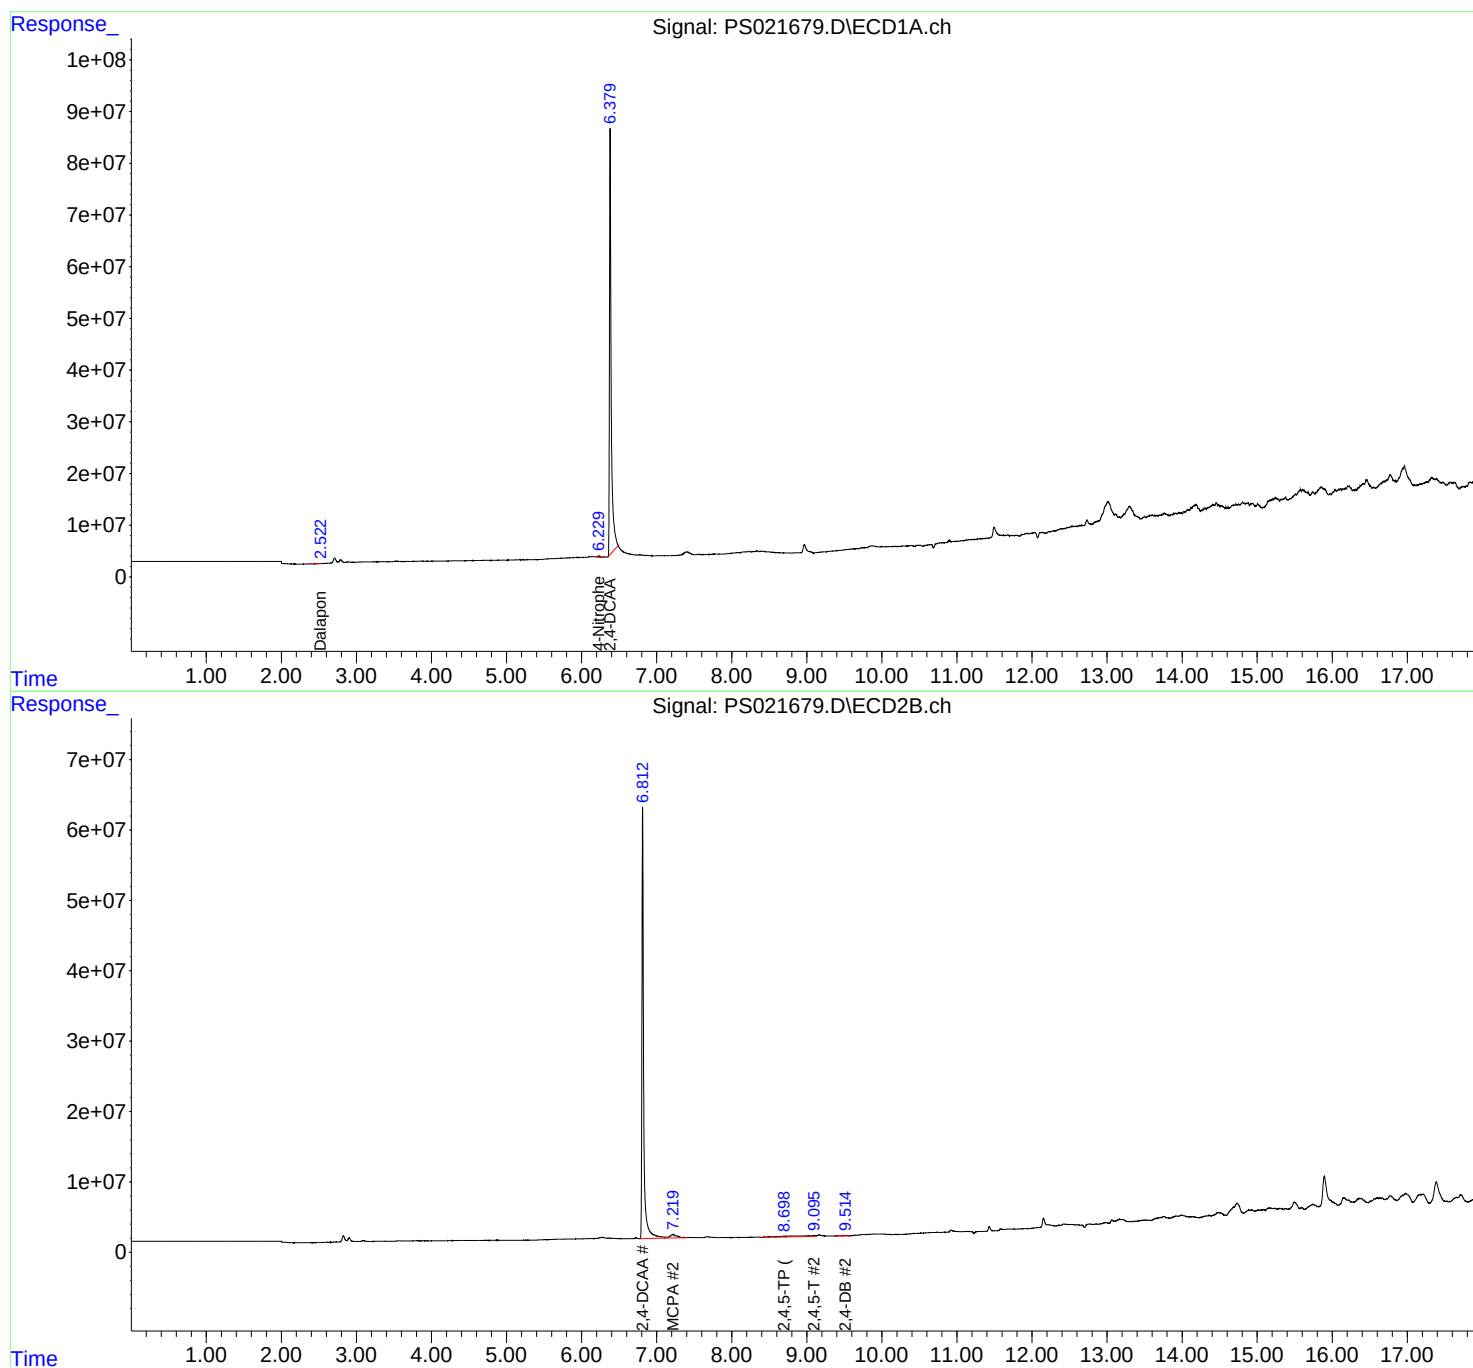


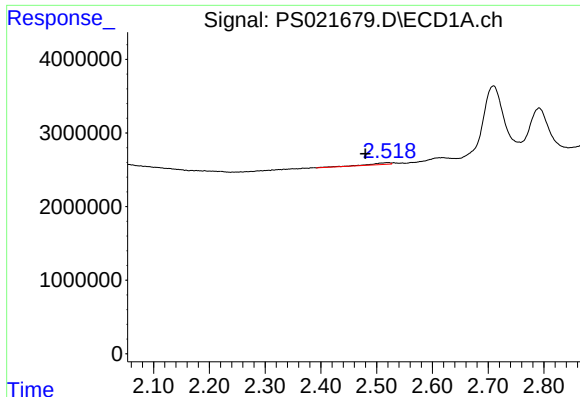

#1 Dalapon


R.T.: 2.521 min
Delta R.T.: 0.041 min
Response: 611316
Conc: 1.72 ng/ml

Instrument :
ECD_S
ClientSampleId :

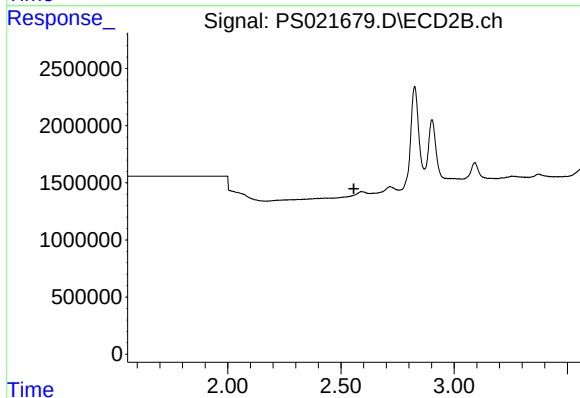


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 2.557 min
Response: 0
Conc: N.D.

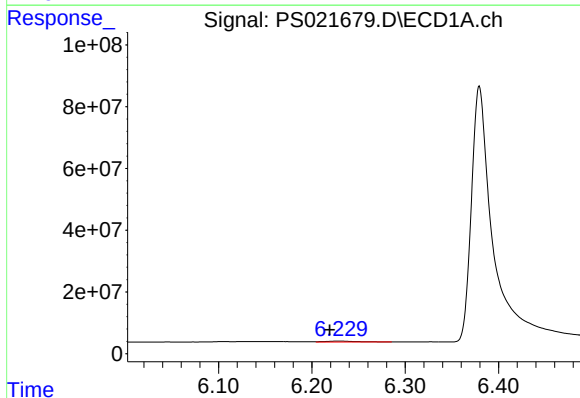


#3 4-Nitrophenol

R.T.: 6.229 min
Delta R.T.: 0.010 min
Response: 6734892
Conc: 4.62 ng/ml

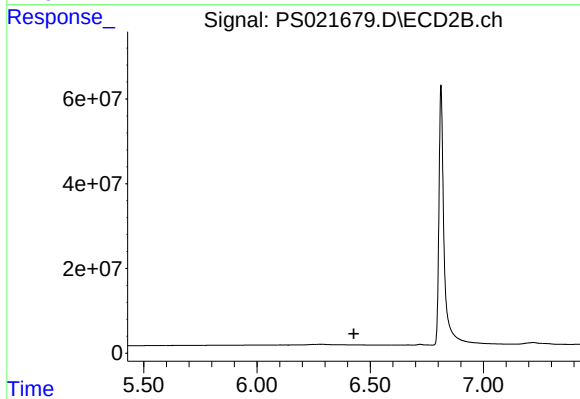

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T. : 6.428 min
Response: 0
Conc: N.D.

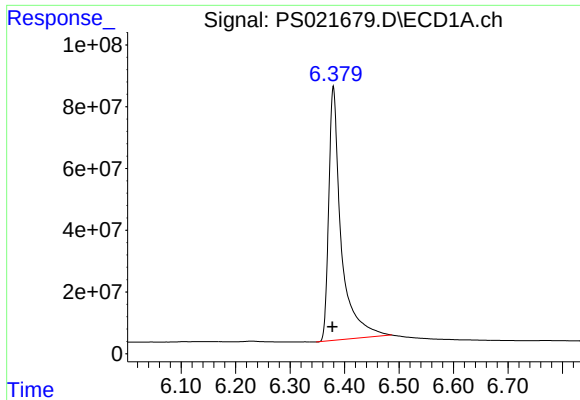

#4 2,4-DCAA


R.T.: 6.379 min
Delta R.T.: 0.002 min
Response: 1304909889
Conc: 468.79 ng/ml

Instrument :
ECD_S
ClientSampleId :

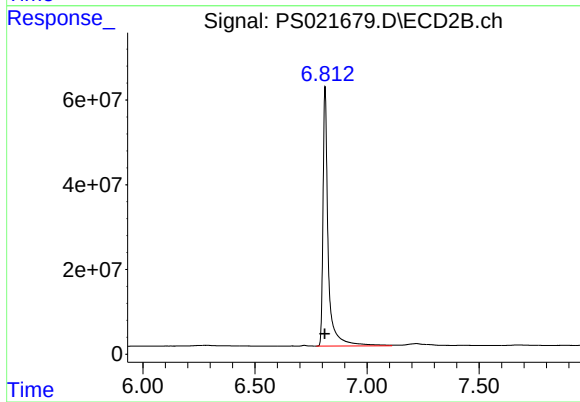


#4 2,4-DCAA

R.T.: 6.813 min
Delta R.T.: 0.001 min
Response: 995544133
Conc: 554.10 ng/ml

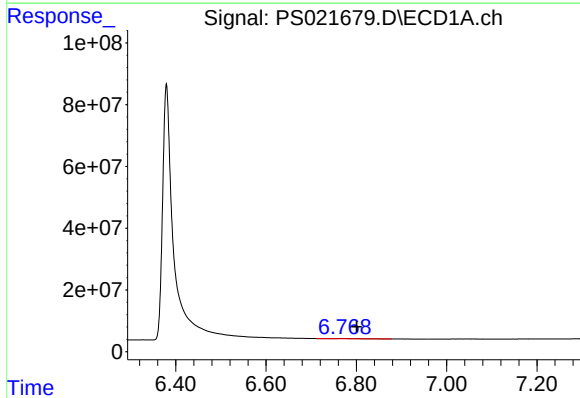


#7 MCPA

R.T.: 6.767 min
Delta R.T.: -0.034 min
Response: 1945891
Conc: N.D.

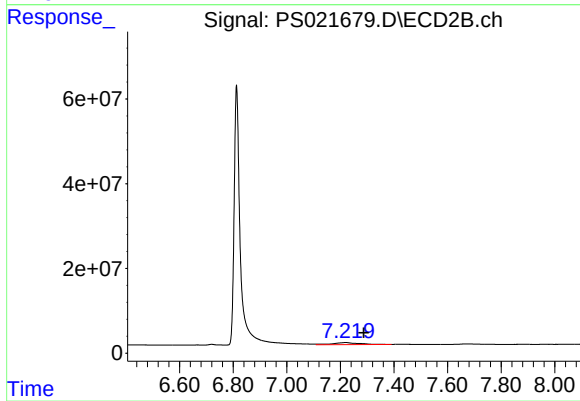

#7 MCPA


R.T.: 7.219 min
Delta R.T.: -0.067 min
Response: 33799360
Conc: 3.73 ug/ml

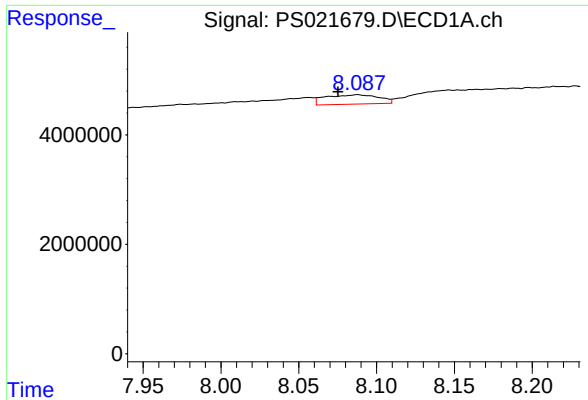

#11 2,4,5-TP (SILVEX)


R.T.: 8.088 min
Delta R.T.: 0.012 min
Response: 4093271
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

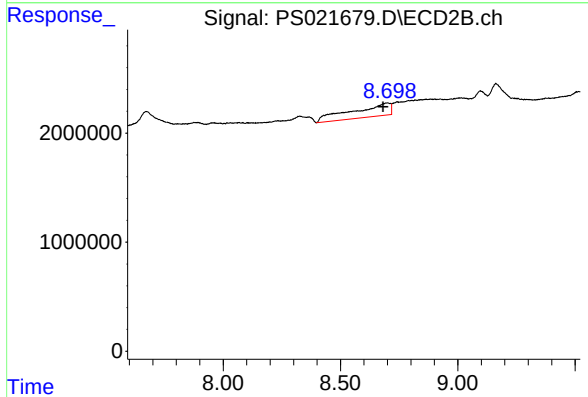


#11 2,4,5-TP (SILVEX)

R.T.: 8.700 min
Delta R.T.: 0.019 min
Response: 13710129
Conc: 1.15 ng/ml

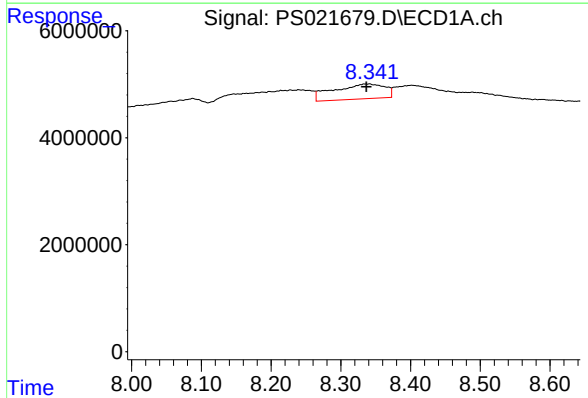


#12 2,4,5-T

R.T.: 8.339 min
Delta R.T.: 0.002 min
Response: 14244932
Conc: N.D.

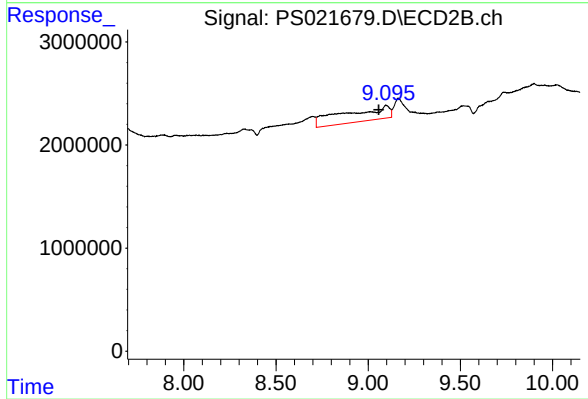

#12 2,4,5-T


R.T.: 9.096 min
Delta R.T.: 0.039 min
Response: 23011855
Conc: 2.06 ng/ml

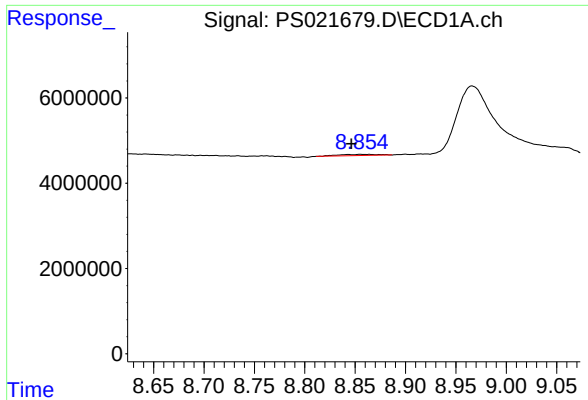

#13 2,4-DB

R.T.: 8.856 min
Delta R.T.: 0.010 min
Response: 782044
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

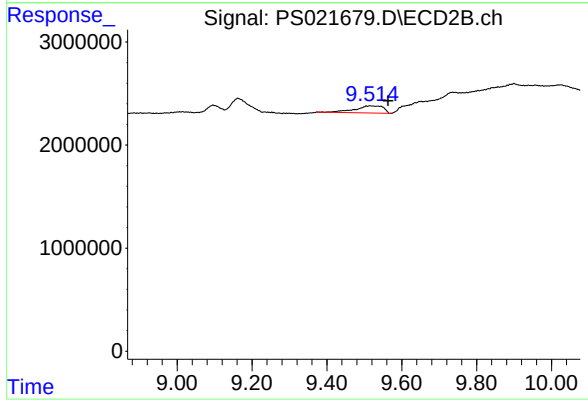

#13 2,4-DB

R.T.: 9.516 min
Delta R.T.: -0.048 min
Response: 3660142
Conc: 2.44 ng/ml