

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS010923\
 Data File : PS021671.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Jan 2023 18:09
 Operator : AR\AJ
 Sample : N6245-02
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 WASTE-COMP

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 01/10/2023
 Supervised By :Ankita Jodhani 01/10/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 10 05:50:33 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010923.M
 Quant Title : 8080.M
 QLast Update : Mon Jan 09 16:45:07 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
4) S 2,4-DCAA	6.741f	7.396f	572.1E6	381.5E6	205.531m	212.314m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS010923\
Data File : PS021671.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Jan 2023 18:09
Operator : AR\AJ
Sample : N6245-02
Misc :
ALS Vial : 12 Sample Multiplier: 1



Instrument :
ECD_S
ClientSampleId :
WASTE-COMP


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 01/10/2023
Supervised By : Ankita Jodhani 01/10/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 10 05:50:33 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010923.M
Quant Title : 8080.M
QLast Update : Mon Jan 09 16:45:07 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

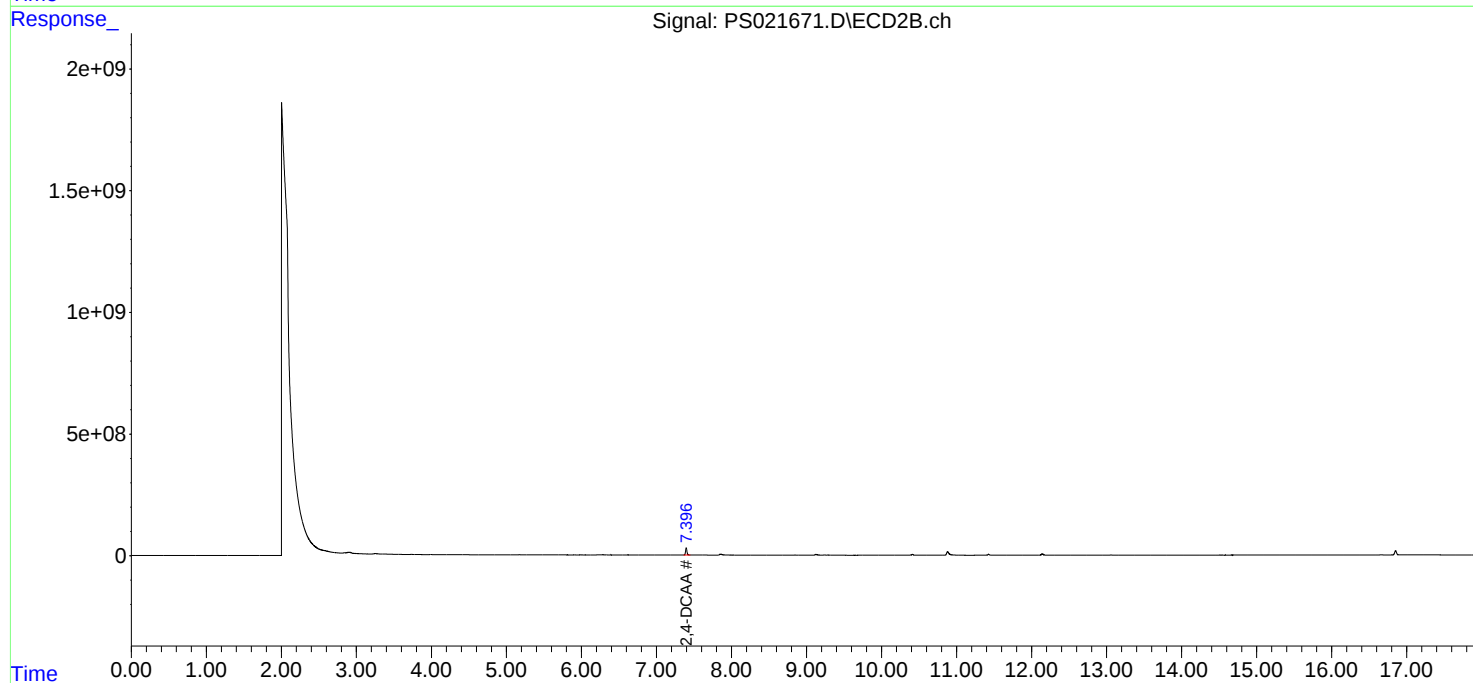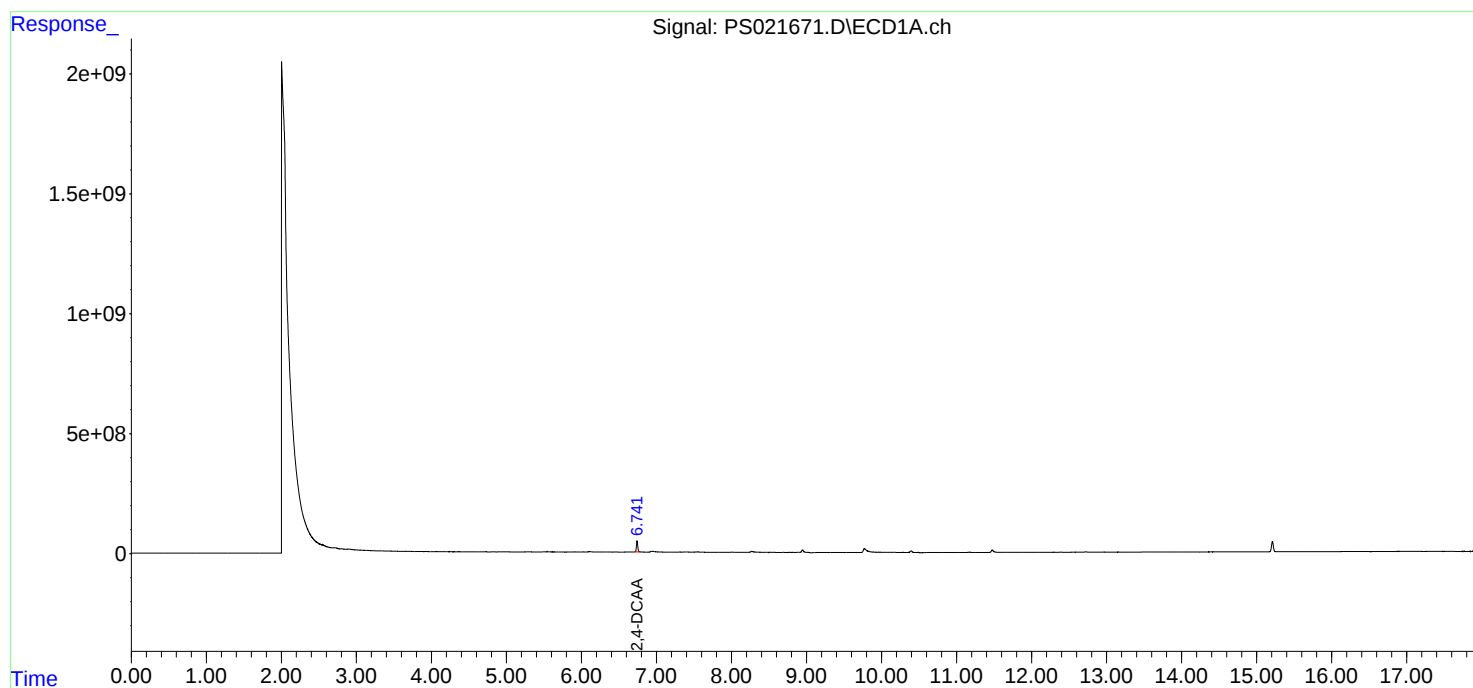

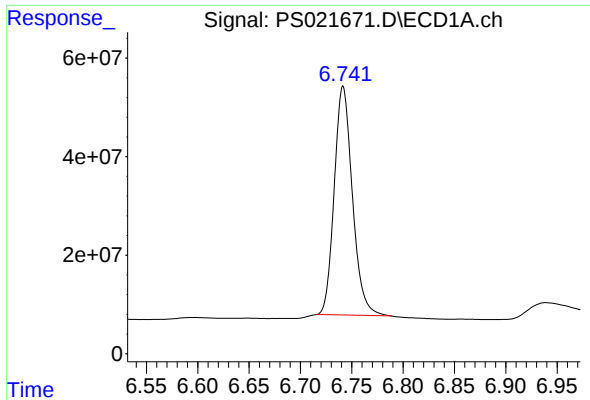

#4 2,4-DCAA

R.T.: 6.741 min
Delta R.T.: 0.364 min
Response: 572109515
Conc: 205.53 ng/ml

Instrument :

ECD_S

ClientSampleId :


WASTE-COMP

Manual Integrations

APPROVED

Reviewed By :Abdul Mirza 01/10/2023

Supervised By :Ankita Jodhani 01/10/2023

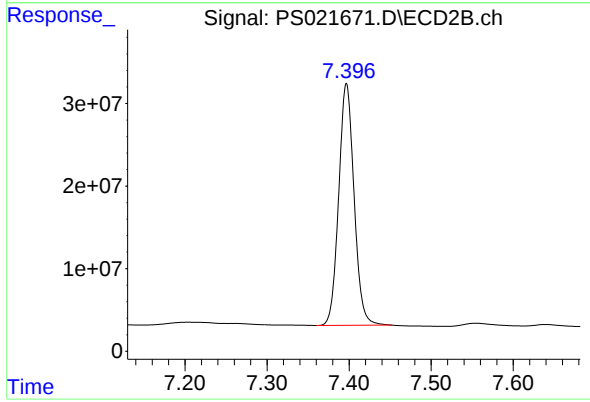

#4 2,4-DCAA

R.T.: 7.396 min
Delta R.T.: 0.585 min
Response: 381462351
Conc: 212.31 ng/ml m