

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS011020\
 Data File : PS008379.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Jan 2020 22:10
 Operator : DD\AJ
 Sample : L1064-07
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 11 01:29:35 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010820.M
 Quant Title : 8080.M
 QLast Update : Wed Jan 08 11:00:59 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.271	5.967	964.3E6	463.6E6	546.139	489.293
Target Compounds							
1) T	Dalapon	2.505	2.191	47226183	56832766	18.420	44.830 #
2) T	3,5-DICHL...	0.000	5.153	0	114.1E6	N.D.	81.699
3) T	4-Nitroph...	6.142	5.629	-11891650	9116357	N.D.	15.354
5) T	DICAMBA	6.535	0.000	26854708	0	3.907	N.D. #
6) T	MCPD	6.710	0.000	365.9E6	0	71.794	N.D. #
7) T	MCPA	0.000	6.489	0	70611583	N.D.	16.537
8) T	DICHLORPROP	0.000	6.787	0	11087142	N.D.	11.476
10) T	Pentachlo...	7.755	0.000	32531459	0	1.338	N.D. #
12) T	2,4,5-T	8.601	0.000	23154931	0	2.510	N.D. #
14) T	DINOSEB	10.208	0.000	1675359	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS011020\
Data File : PS008379.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Jan 2020 22:10
Operator : DD\AJ
Sample : L1064-07
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 11 01:29:35 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010820.M
Quant Title : 8080.M
QLast Update : Wed Jan 08 11:00:59 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

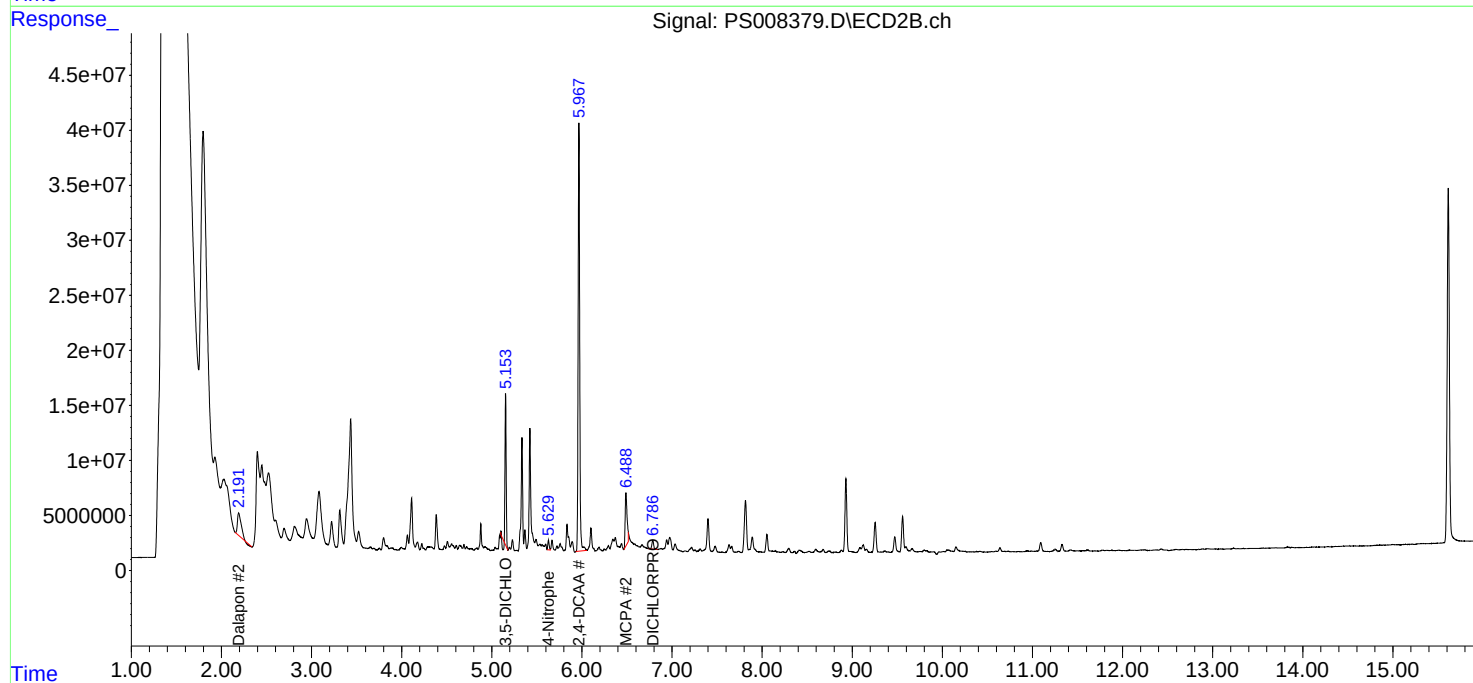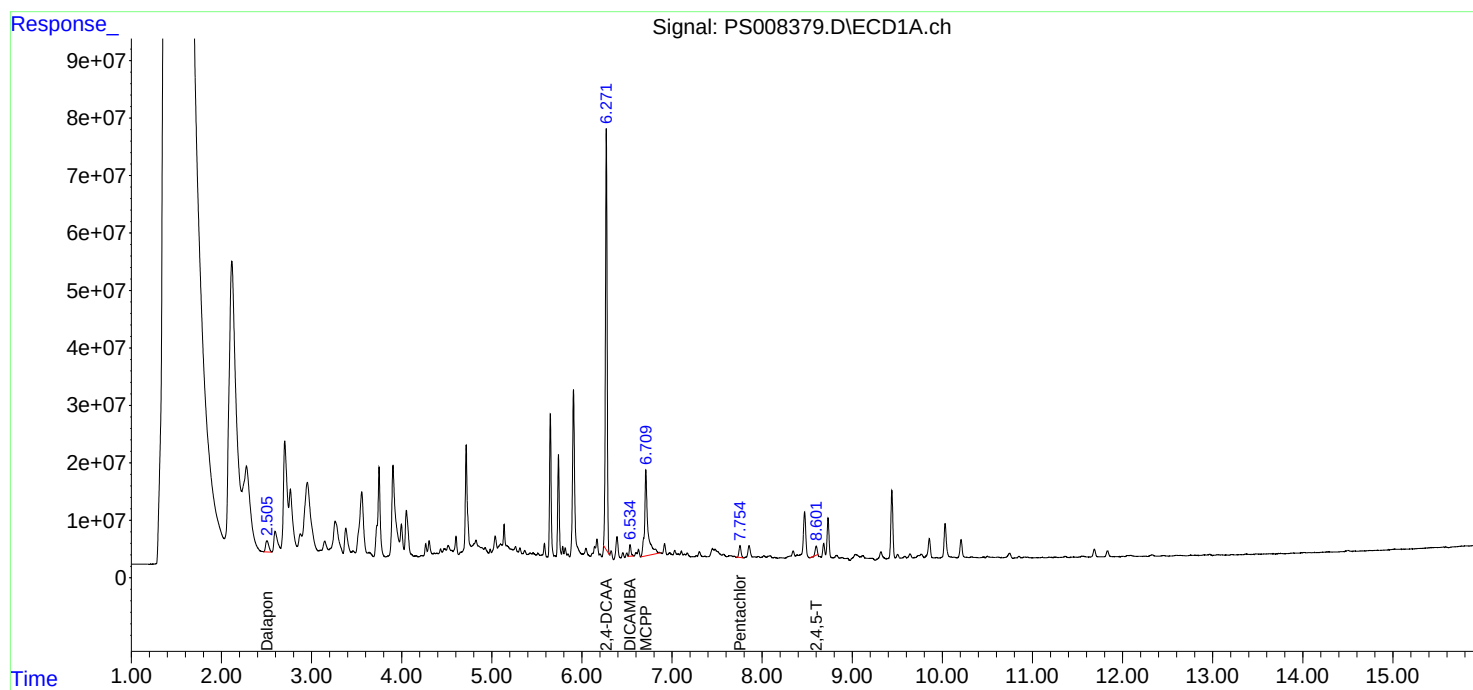


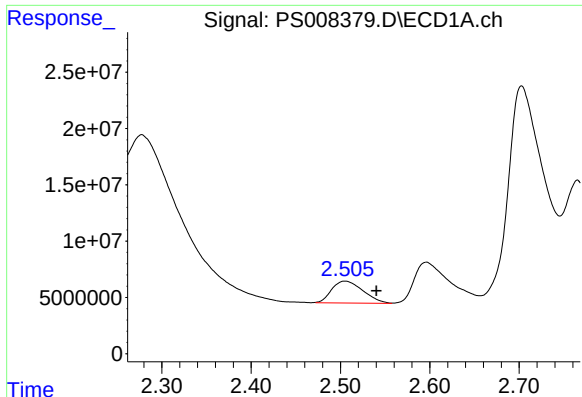

#1 Dalapon


R.T.: 2.505 min
Delta R.T.: -0.035 min
Response: 47226183
Conc: 18.42 ng/ml

Instrument :
ECD_S
ClientSampleId :

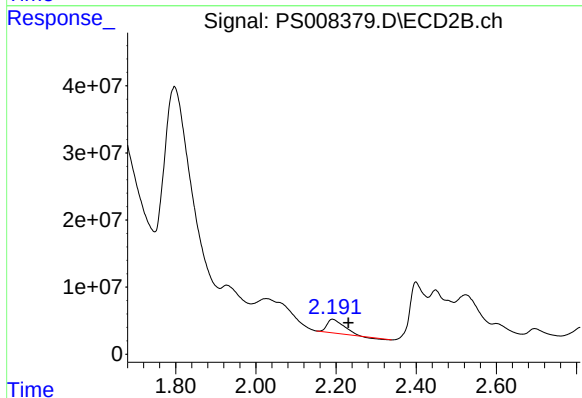


#1 Dalapon

R.T.: 2.191 min
Delta R.T.: -0.040 min
Response: 56832766
Conc: 44.83 ng/ml

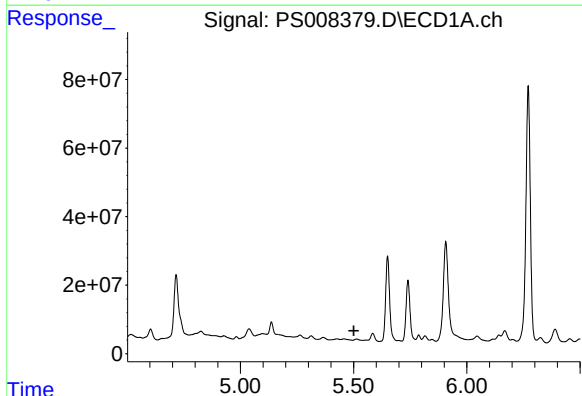


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 5.501 min
Response: 0
Conc: N.D.

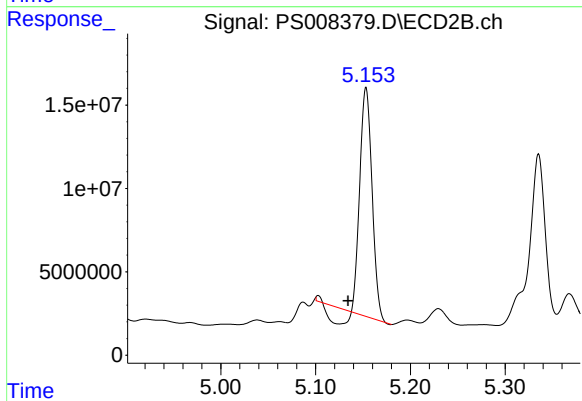

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 5.153 min
Delta R.T.: 0.019 min
Response: 114147905
Conc: 81.70 ng/ml

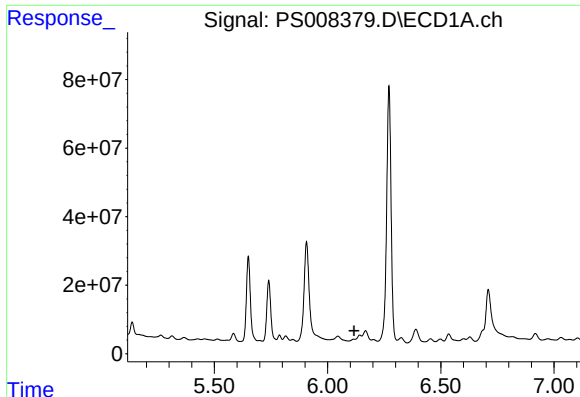

#3 4-Nitrophenol


R.T.: 6.142 min
Delta R.T.: 0.026 min
Response: -11891650
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

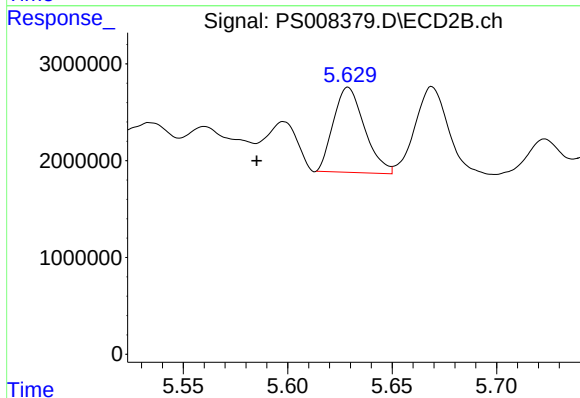


#3 4-Nitrophenol

R.T.: 5.629 min
Delta R.T.: 0.044 min
Response: 9116357
Conc: 15.35 ng/ml

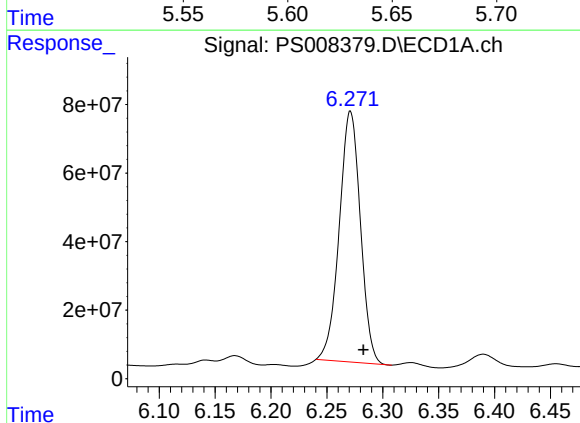


#4 2,4-DCAA

R.T.: 6.271 min
Delta R.T.: -0.012 min
Response: 964319149
Conc: 546.14 ng/ml

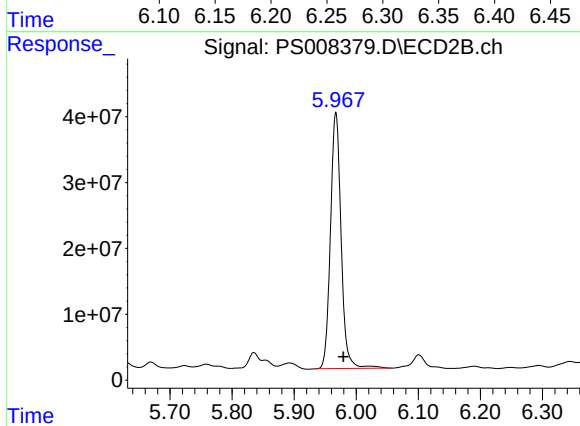

#4 2,4-DCAA


R.T.: 5.967 min
Delta R.T.: -0.012 min
Response: 463586602
Conc: 489.29 ng/ml

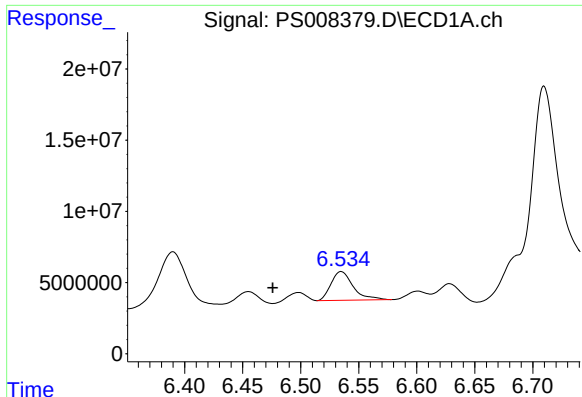

#5 DICAMBA


R.T.: 6.535 min
Delta R.T.: 0.059 min
Response: 26854708
Conc: 3.91 ng/ml

Instrument :
ECD_S
ClientSampleId :

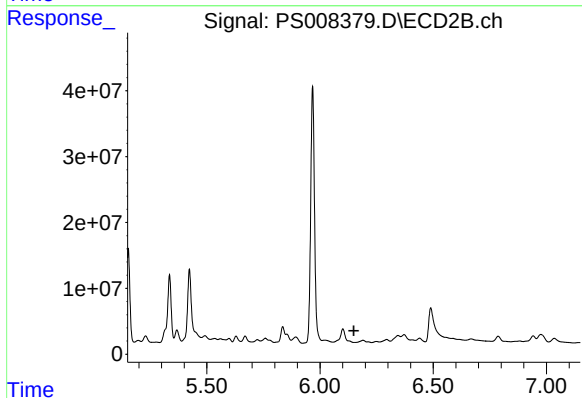


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 6.150 min
Response: 0
Conc: N.D.

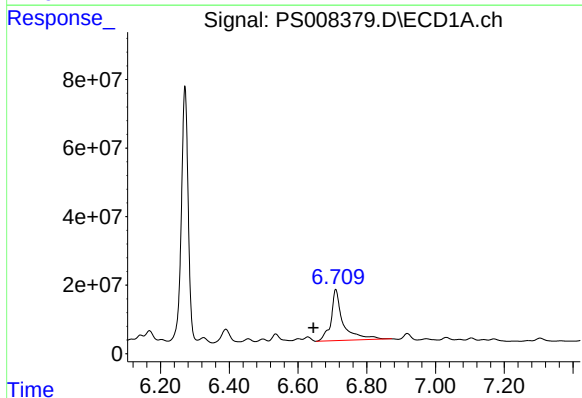


#6 MCP

R.T.: 6.710 min
Delta R.T.: 0.064 min
Response: 365920929
Conc: 71.79 ug/ml

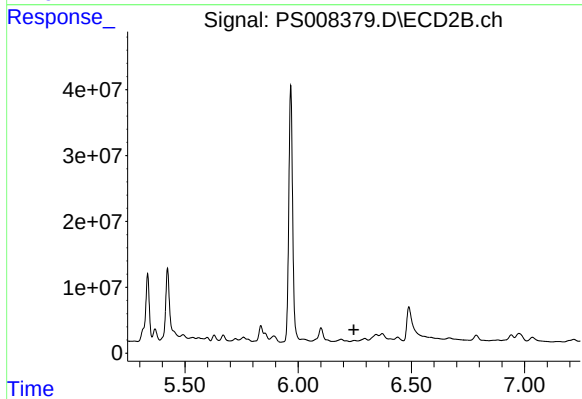

#6 MCP


R.T.: 0.000 min
Exp R.T. : 6.246 min
Response: 0
Conc: N.D.

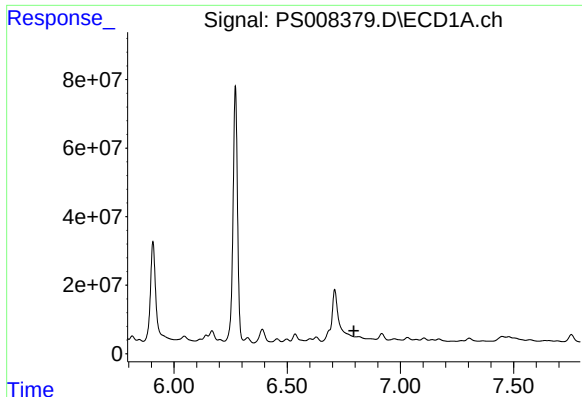

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 6.794 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

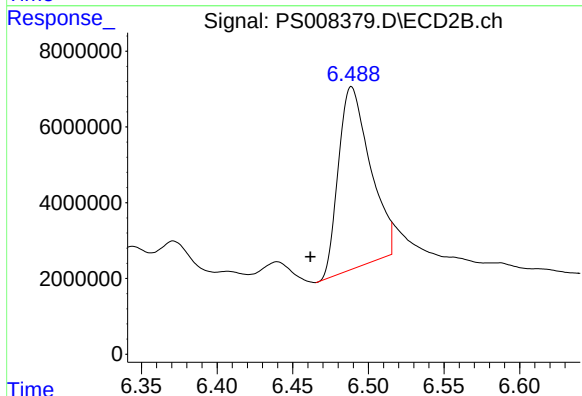


#7 MCPA

R.T.: 6.489 min
Delta R.T.: 0.028 min
Response: 70611583
Conc: 16.54 ug/ml

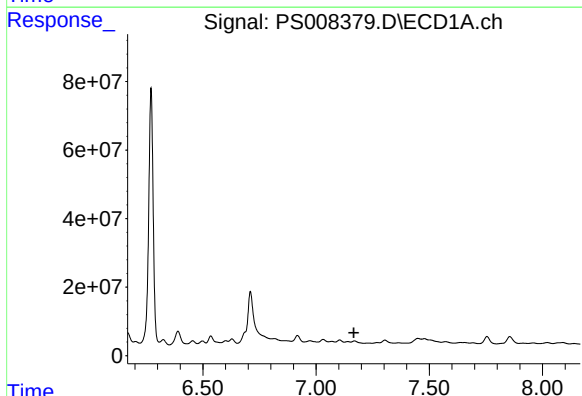


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 7.167 min
Response: 0
Conc: N.D.

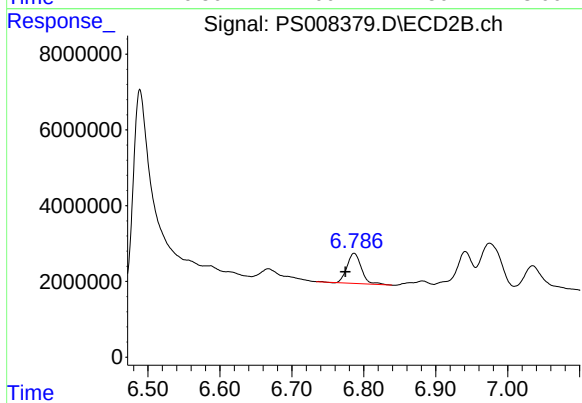

#8 DICHLORPROP


R.T.: 6.787 min
Delta R.T.: 0.012 min
Response: 11087142
Conc: 11.48 ng/ml

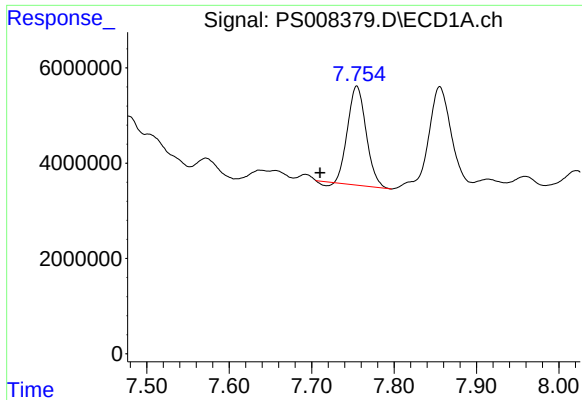

#10 Pentachlorophenol


R.T.: 7.755 min
Delta R.T.: 0.045 min
Response: 32531459
Conc: 1.34 ng/ml

Instrument :
ECD_S
ClientSampleId :

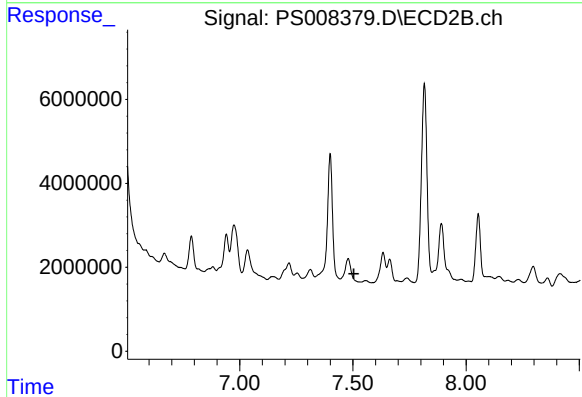


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T. : 7.505 min
Response: 0
Conc: N.D.

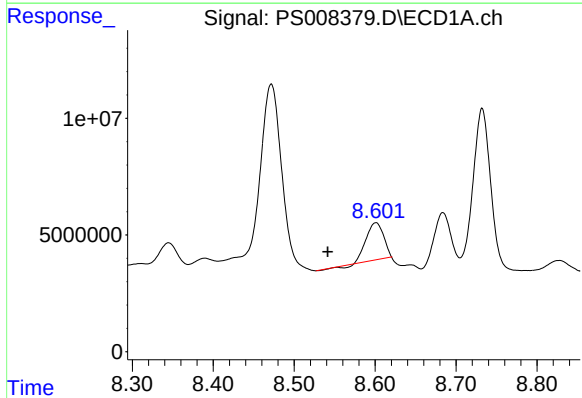

#12 2,4,5-T

R.T.: 8.601 min
Delta R.T.: 0.059 min
Response: 23154931
Conc: 2.51 ng/ml

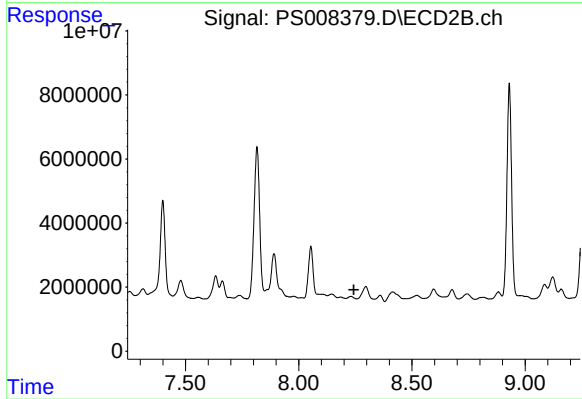

#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 8.243 min
Response: 0
Conc: N.D.