

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS011023\
 Data File : PS021691.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Jan 2023 08:56
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 11 06:54:25 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010923.M
 Quant Title : 8080.M
 QLast Update : Tue Jan 10 10:34:52 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.380	6.813	1296.7E6	1026.4E6	465.846	571.275
Target Compounds							
1) T	Dalapon	2.518	0.000	557931	0	<MDL	N.D. #
2) T	3,5-DICHL...	5.737	0.000	553869	0	<MDL	N.D. #
3) T	4-Nitroph...	6.232	0.000	5078171	0	3.484	N.D. #
7) T	MCPA	6.770	7.223f	1146054	24124784	<MDL	2.660 #
10) T	Pentachlo...	7.558	0.000	1210542	0	<MDL	N.D. #
11) T	2,4,5-TP ...	8.058	8.696	2830173	643196	<MDL	<MDL #
12) T	2,4,5-T	0.000	9.105f	0	1371569	N.D.	<MDL
13) T	2,4-DB	8.849	0.000	960451	0	<MDL	N.D. #
14) T	DINOSEB	9.882	0.000	37211524	0	2.267	N.D. #
15) T	Picloram	9.754	10.819f	10955115	16660242	<MDL	<MDL #
16) T	DCPA	10.168	10.819	1227014	16660242	<MDL	1.195 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS011023\
Data File : PS021691.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Jan 2023 08:56
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 11 06:54:25 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010923.M
Quant Title : 8080.M
QLast Update : Tue Jan 10 10:34:52 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

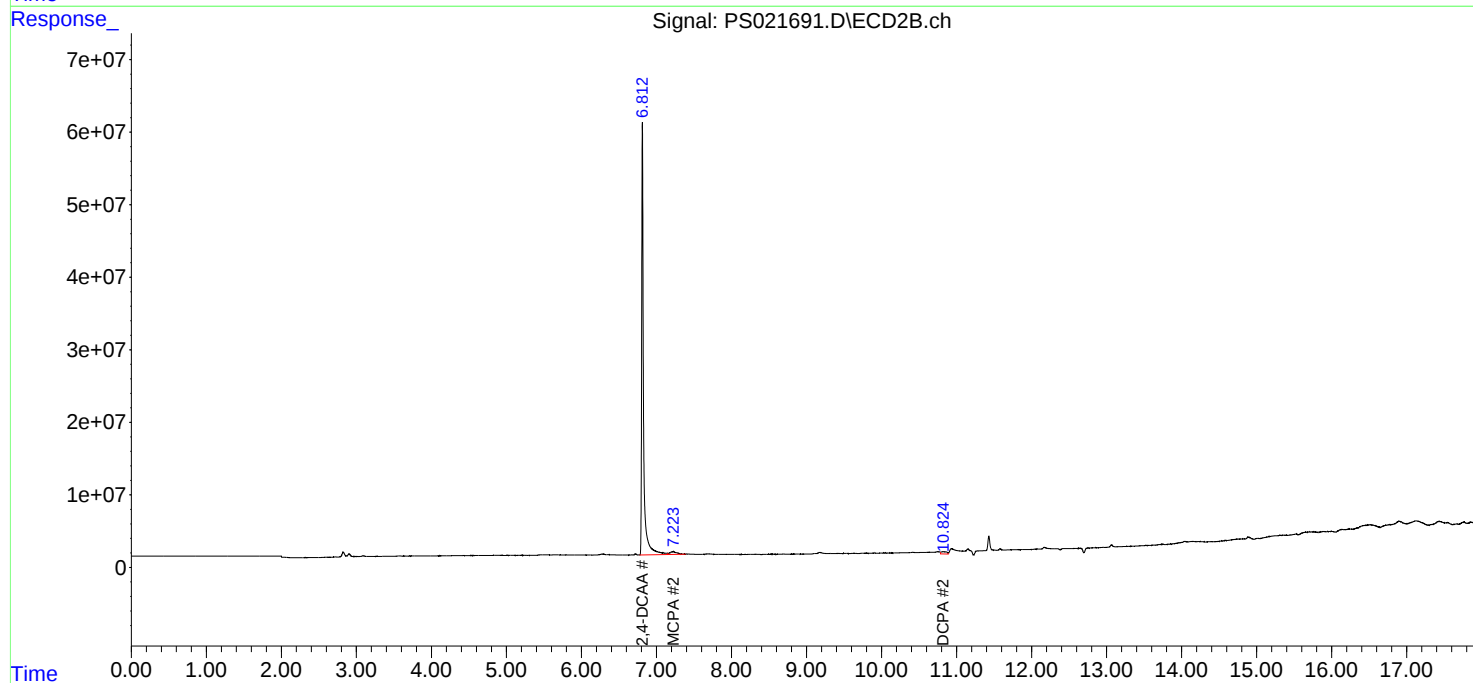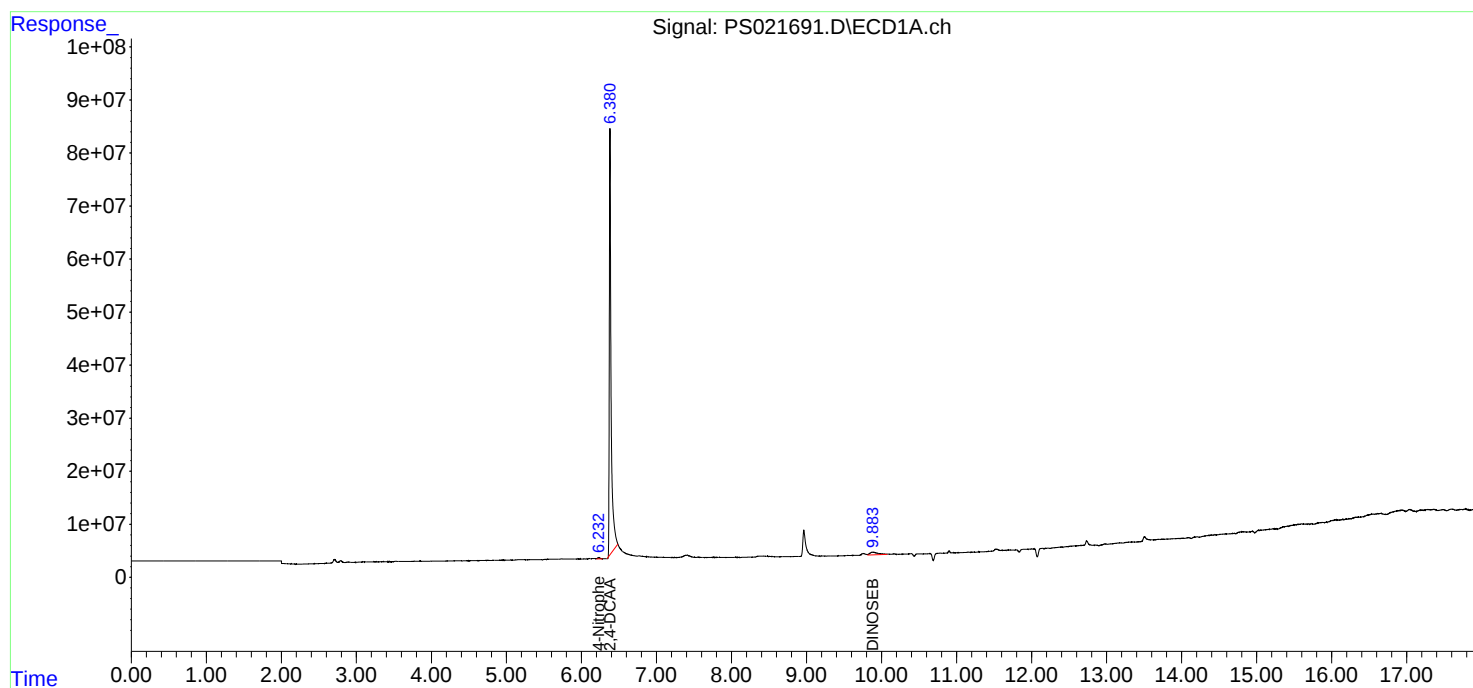


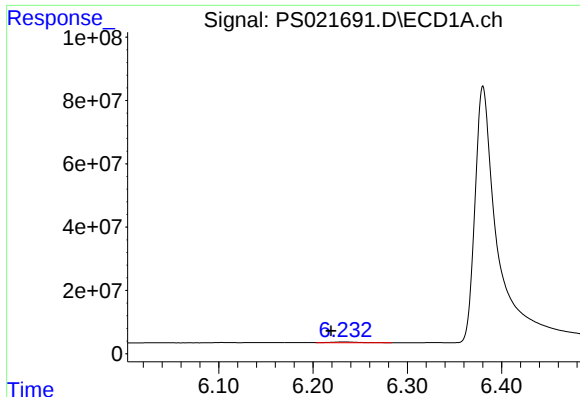

#3 4-Nitrophenol


R.T.: 6.232 min
Delta R.T.: 0.013 min
Response: 5078171
Conc: 3.48 ng/ml

Instrument :
ECD_S
ClientSampleId :

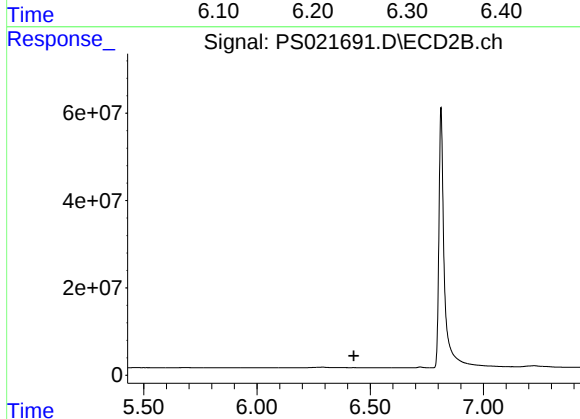


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.428 min
Response: 0
Conc: N.D.

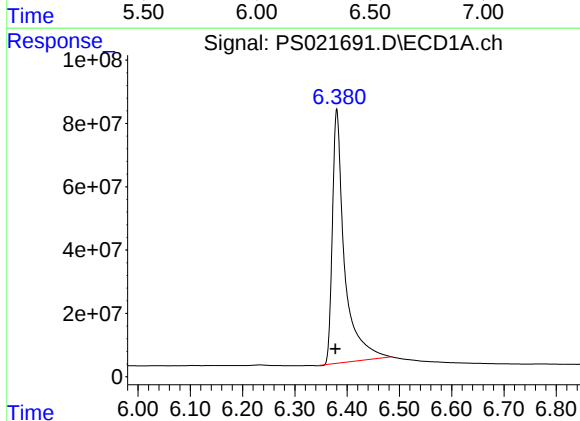


#4 2,4-DCAA

R.T.: 6.380 min
Delta R.T.: 0.003 min
Response: 1296713456
Conc: 465.85 ng/ml

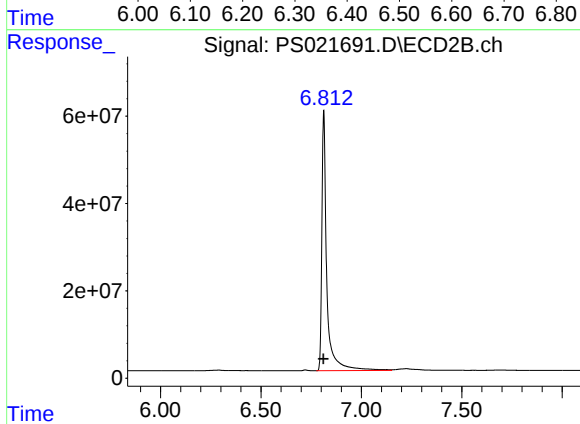

#4 2,4-DCAA


R.T.: 6.813 min
Delta R.T.: 0.001 min
Response: 1026403372
Conc: 571.27 ng/ml

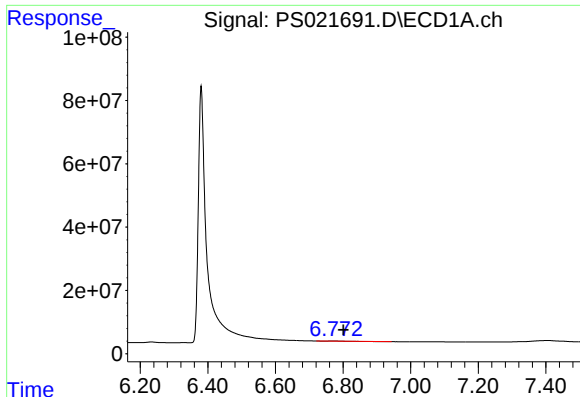

#7 MCPA


R.T.: 6.770 min
Delta R.T.: -0.031 min
Response: 1146054
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

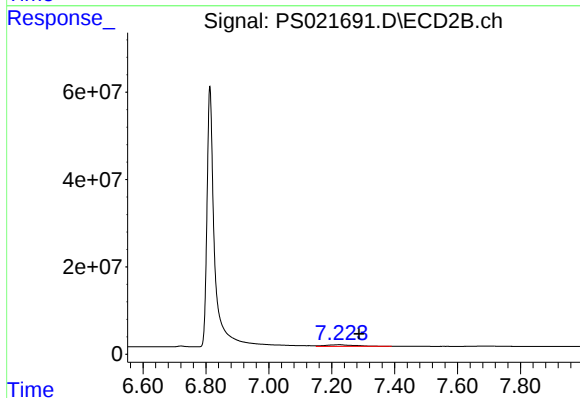


#7 MCPA

R.T.: 7.223 min
Delta R.T.: -0.064 min
Response: 24124784
Conc: 2.66 ug/ml

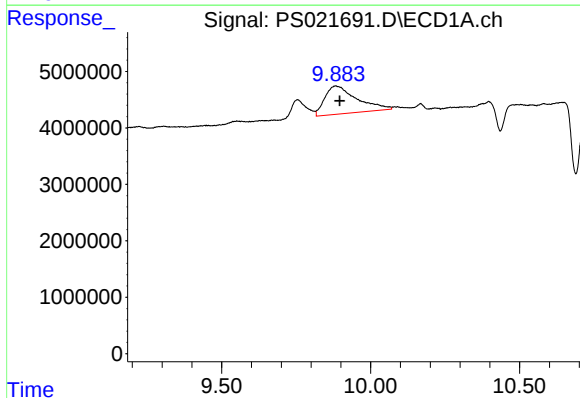


#14 DINOSEB

R.T.: 9.882 min
Delta R.T.: -0.014 min
Response: 37211524
Conc: 2.27 ng/ml

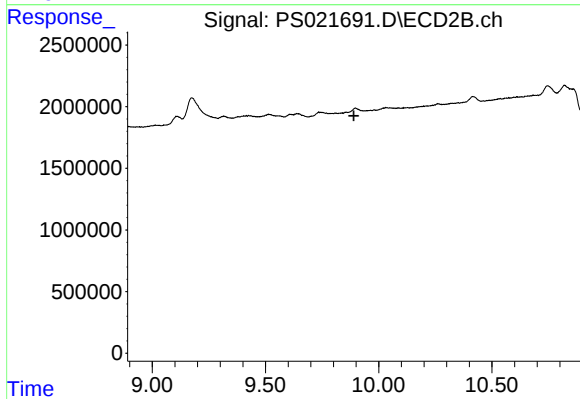

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 9.890 min
Response: 0
Conc: N.D.

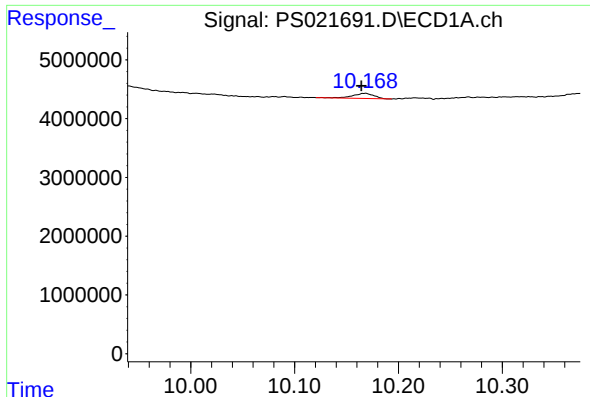

#16 DCPA

R.T.: 10.168 min
Delta R.T.: 0.003 min
Response: 1227014
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

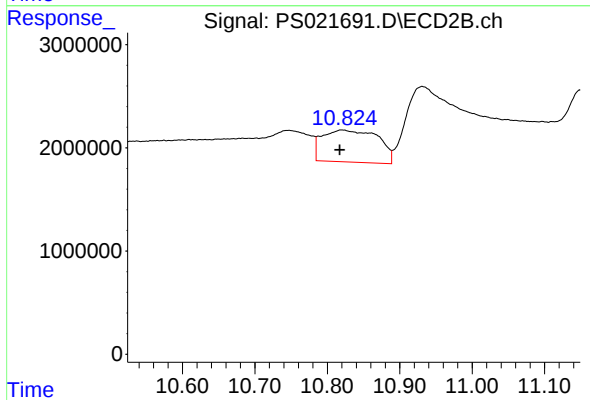

#16 DCPA

R.T.: 10.819 min
Delta R.T.: 0.002 min
Response: 16660242
Conc: 1.20 ng/ml