

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS011023\
 Data File : PS021703.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Jan 2023 18:16
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 11 06:58:35 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010923.M
 Quant Title : 8080.M
 QLast Update : Tue Jan 10 10:34:52 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.377	6.811	1392.5E6	1000.5E6	500.247	556.850
Target Compounds							
1) T	Dalapon	2.512	2.593	578200	554162	<MDL	<MDL #
3) T	4-Nitroph...	6.221	6.421	5707394	489255	3.916	<MDL #
5) T	DICAMBA	0.000	7.024f	0	3745280	N.D.	<MDL
6) T	MCP	0.000	7.024f	0	3745280	N.D.	<MDL
7) T	MCPA	6.751f	0.000	7033429	0	<MDL	N.D. #
8) T	DICHLORPROP	7.123	7.642f	433785	4764460	<MDL	2.233 #
9) T	2,4-D	7.305	7.864	2413795	1238238	<MDL	<MDL #
10) T	Pentachlo...	7.546	0.000	1870685	0	<MDL	N.D. #
11) T	2,4,5-TP ...	8.081	8.689	10640907	3598206	<MDL	<MDL #
12) T	2,4,5-T	8.367	9.079	7210439	5166746	<MDL	<MDL #
13) T	2,4-DB	0.000	9.592	0	1001905	N.D.	<MDL
14) T	DINOSEB	9.897	0.000	27370687	0	1.668	N.D. #
15) T	Picloram	9.722	10.822f	25104938	100.3E6	<MDL	5.666 #
16) T	DCPA	10.157	10.822	2433666	100.3E6	<MDL	7.197 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS011023\
Data File : PS021703.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Jan 2023 18:16
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 11 06:58:35 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010923.M
Quant Title : 8080.M
QLast Update : Tue Jan 10 10:34:52 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

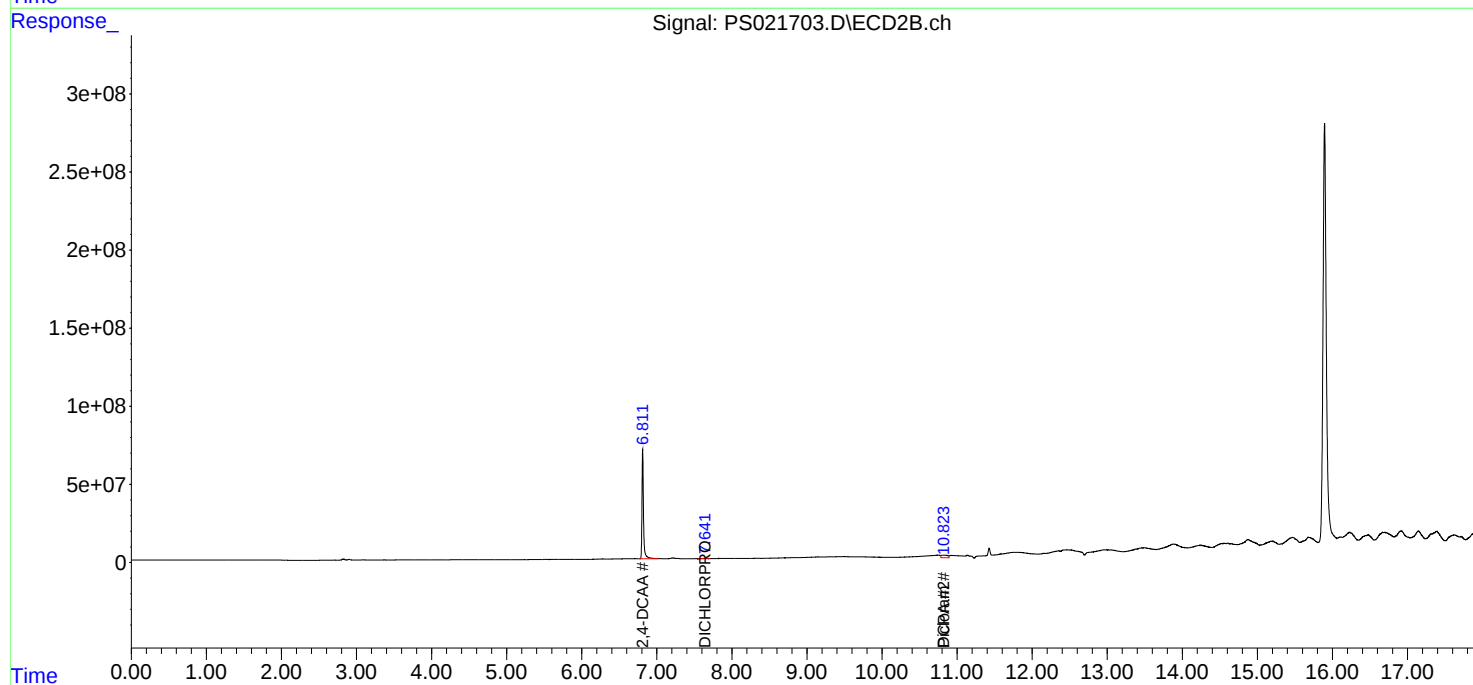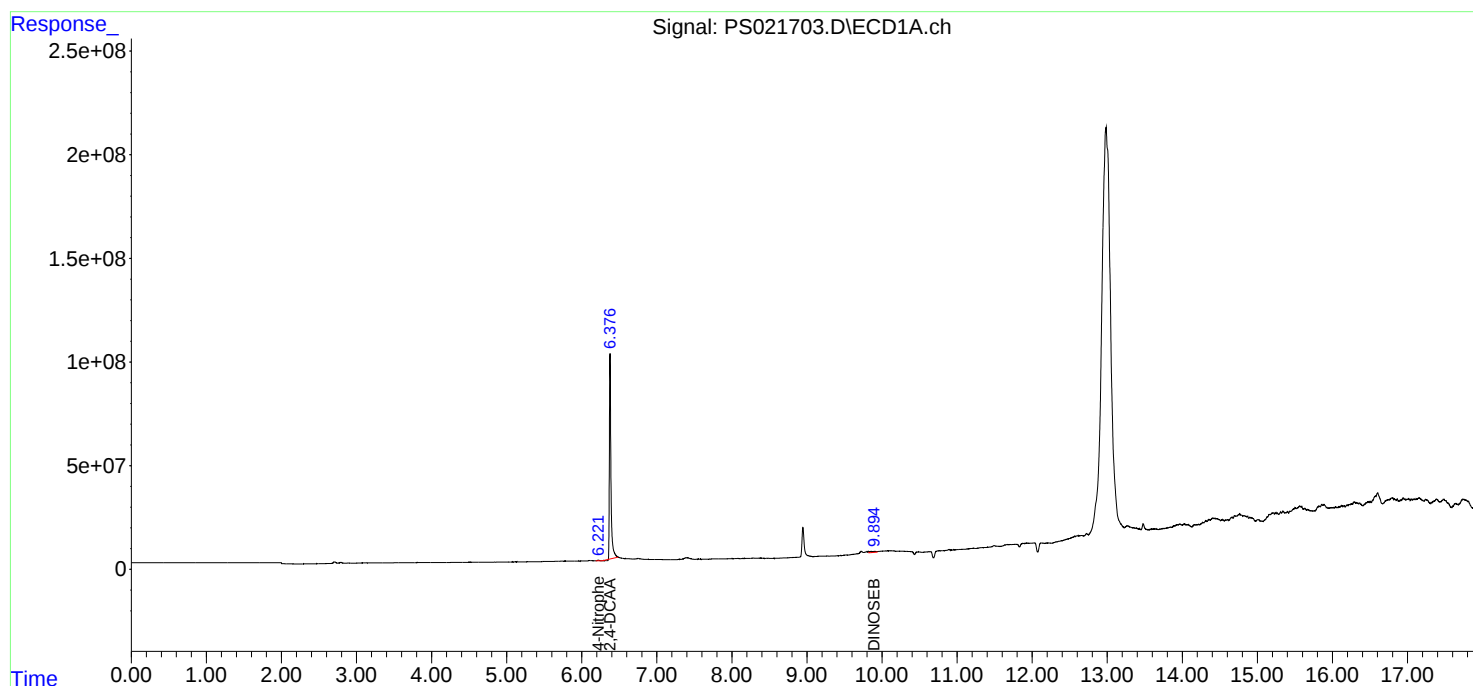


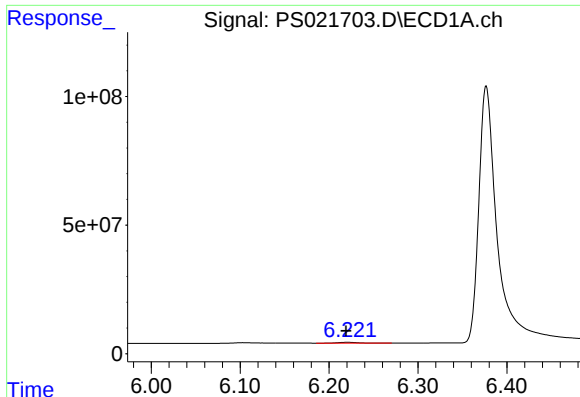

#3 4-Nitrophenol


R.T.: 6.221 min
Delta R.T.: 0.001 min
Response: 5707394
Conc: 3.92 ng/ml

Instrument :
ECD_S
ClientSampleId :

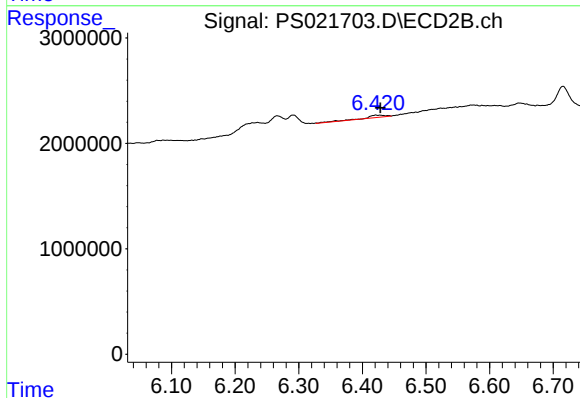


#3 4-Nitrophenol

R.T.: 6.421 min
Delta R.T.: -0.007 min
Response: 489255
Conc: N.D.

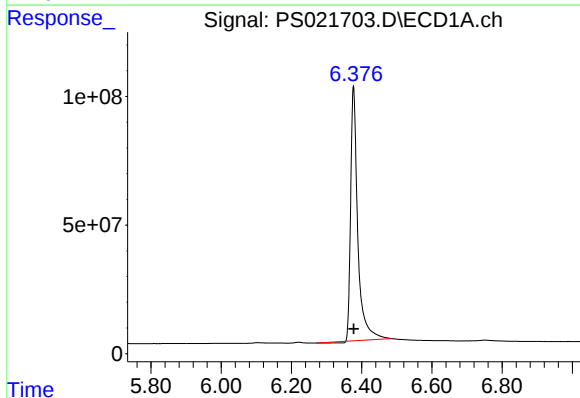


#4 2,4-DCAA

R.T.: 6.377 min
Delta R.T.: 0.000 min
Response: 1392469718
Conc: 500.25 ng/ml

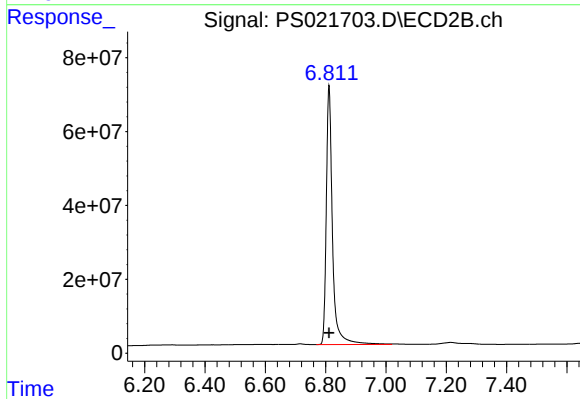

#4 2,4-DCAA


R.T.: 6.811 min
Delta R.T.: 0.000 min
Response: 1000486490
Conc: 556.85 ng/ml

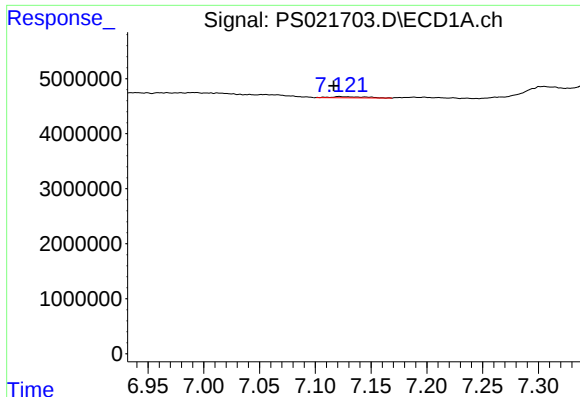

#8 DICHLORPROP


R.T.: 7.123 min
Delta R.T.: 0.006 min
Response: 433785
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

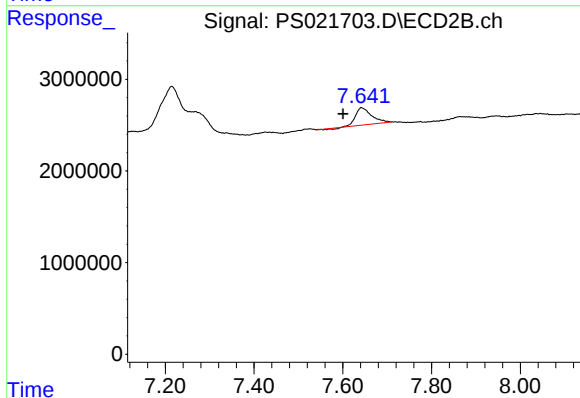


#8 DICHLORPROP

R.T.: 7.642 min
Delta R.T.: 0.042 min
Response: 4764460
Conc: 2.23 ng/ml

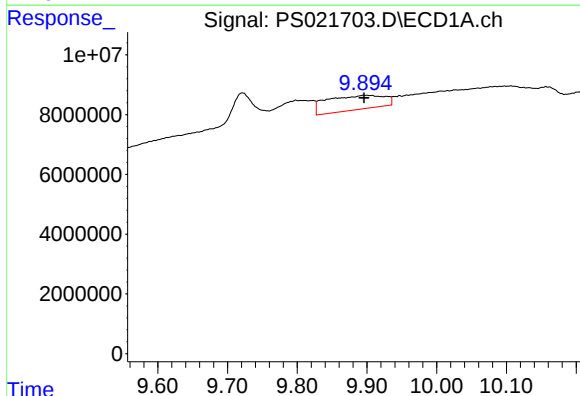


#14 DINOSEB

R.T.: 9.897 min
Delta R.T.: 0.001 min
Response: 27370687
Conc: 1.67 ng/ml

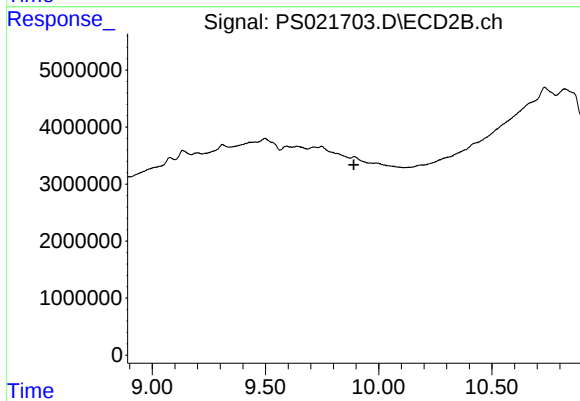

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 9.890 min
Response: 0
Conc: N.D.

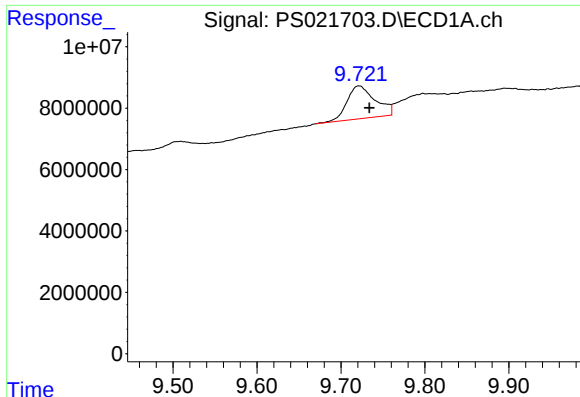

#15 Picloram


R.T.: 9.722 min
Delta R.T.: -0.012 min
Response: 25104938
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

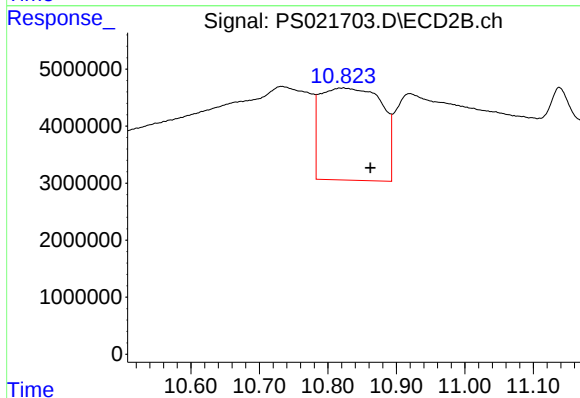


#15 Picloram

R.T.: 10.822 min
Delta R.T.: -0.040 min
Response: 100330018
Conc: 5.67 ng/ml

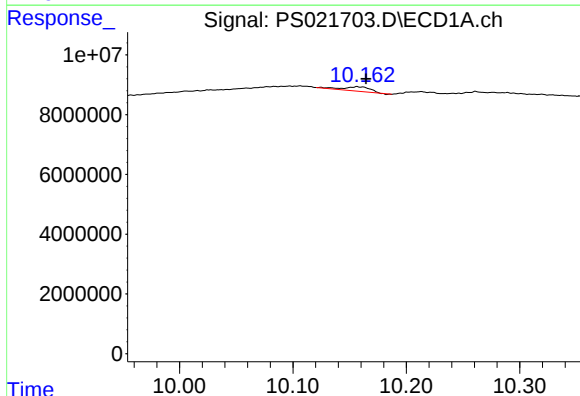

#16 DCPA

R.T.: 10.157 min
Delta R.T.: -0.007 min
Response: 2433666
Conc: N.D.

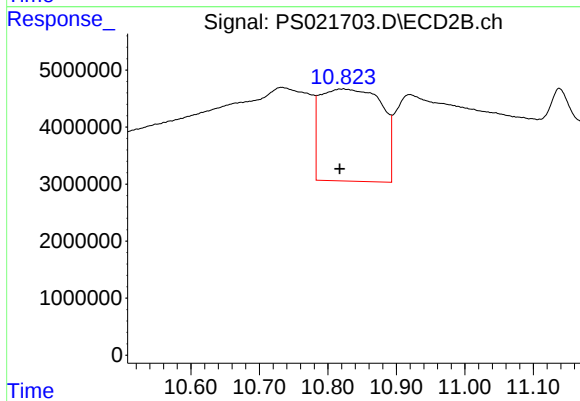

#16 DCPA

R.T.: 10.822 min
Delta R.T.: 0.004 min
Response: 100330018
Conc: 7.20 ng/ml