

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS011025\
 Data File : PS028876.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Jan 2025 08:46
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 11 01:44:52 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS122324.M
 Quant Title : 8080.M
 QLast Update : Mon Dec 23 13:44:25 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds							
1)	T	Dalapon	2.659f	0.000	4289295	0	1.523 N.D. #
2)	T	3,5-DICHL...	6.365	0.000	2721704	0	<MDL N.D. #
3)	T	4-Nitroph...	6.989	0.000	5910049	0	3.935 N.D. #
5)	T	DICAMBA	7.408	7.888	559185	3685524	<MDL <MDL #
6)	T	MCP	7.530f	7.982	1967193	2743381	<MDL <MDL #
8)	T	DICHLORPROP	0.000	8.644f	0	2397843	N.D. 1.738
9)	T	2,4-D	8.349	0.000	5366905	0	1.883 N.D. #
10)	T	Pentachlo...	8.661f	0.000	1433771	0	<MDL N.D. #
11)	T	2,4,5-TP ...	9.177f	0.000	852954	0	<MDL N.D. #
12)	T	2,4,5-T	9.449f	0.000	7987694	0	<MDL N.D. #
13)	T	2,4-DB	10.075	0.000	1837225	0	<MDL N.D. #
14)	T	DINOSEB	11.251	0.000	795329	0	<MDL N.D. #
15)	T	Picloram	11.101	12.281	6508264	2250125	<MDL <MDL #
16)	T	DCPA	11.546	12.281f	889217	2250125	<MDL <MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS011025\
Data File : PS028876.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Jan 2025 08:46
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 11 01:44:52 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS122324.M
Quant Title : 8080.M
QLast Update : Mon Dec 23 13:44:25 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

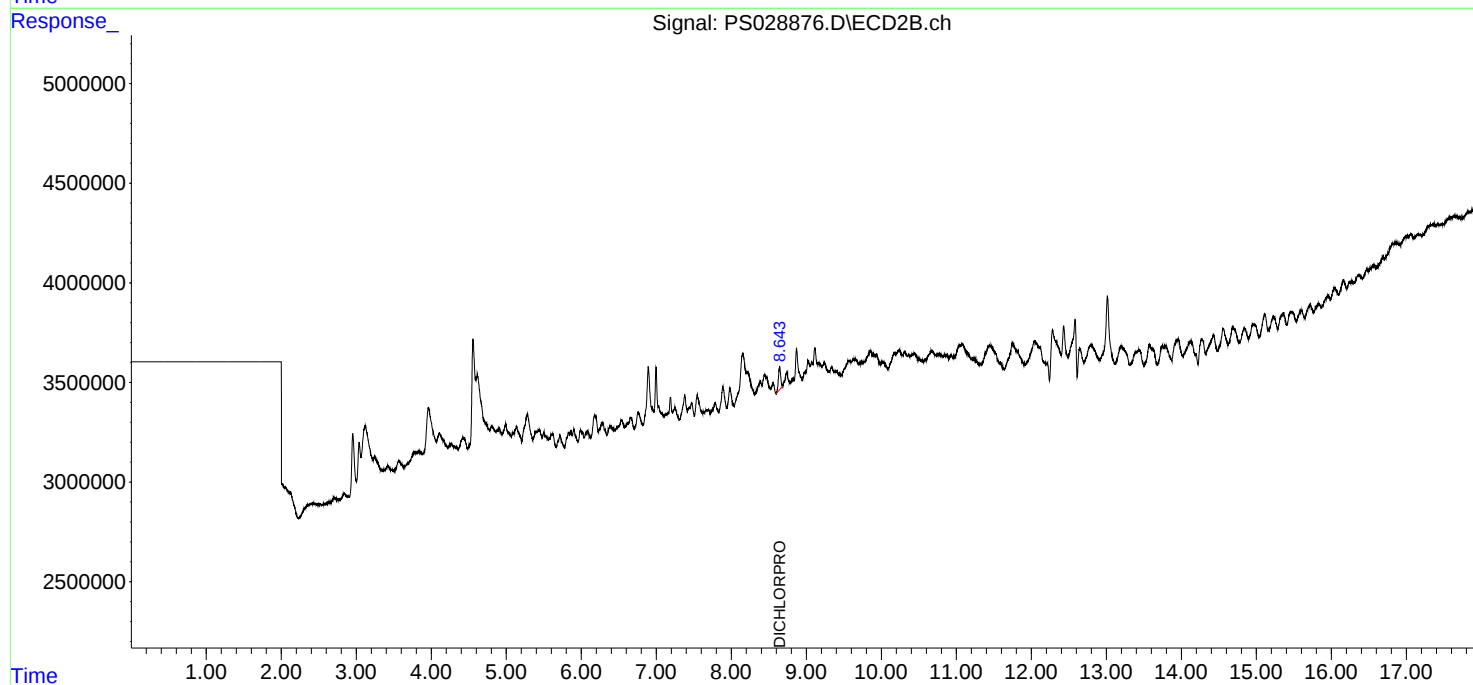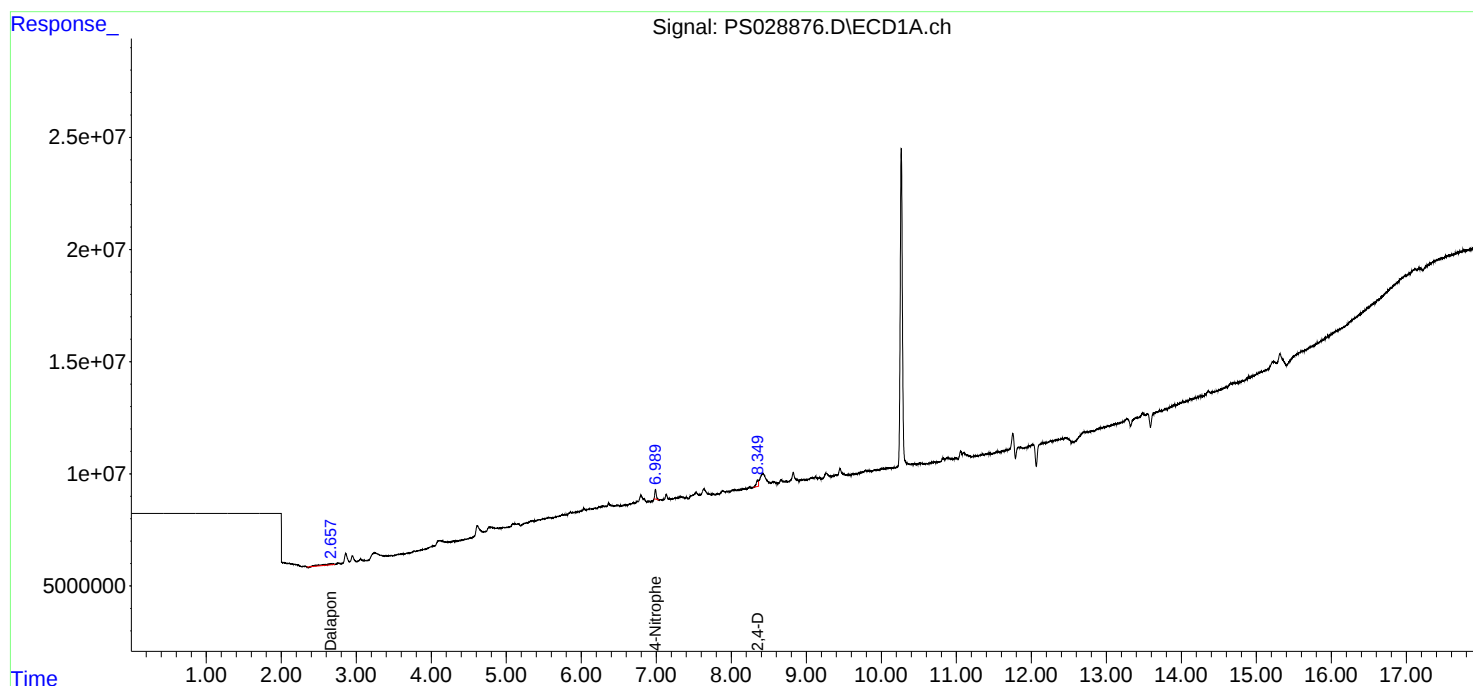


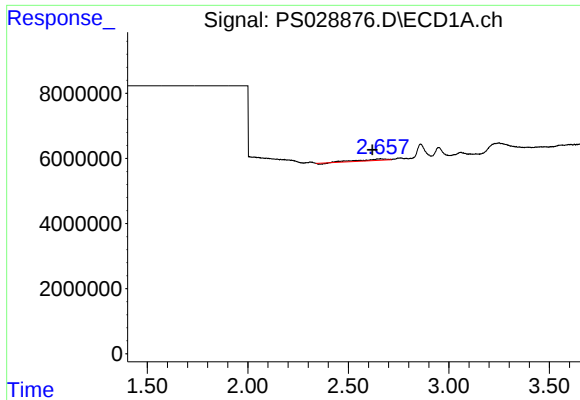

#1 Dalapon


R.T.: 2.659 min
Delta R.T.: 0.039 min
Response: 4289295
Conc: 1.52 ng/ml

Instrument :
ECD_S
ClientSampleId :

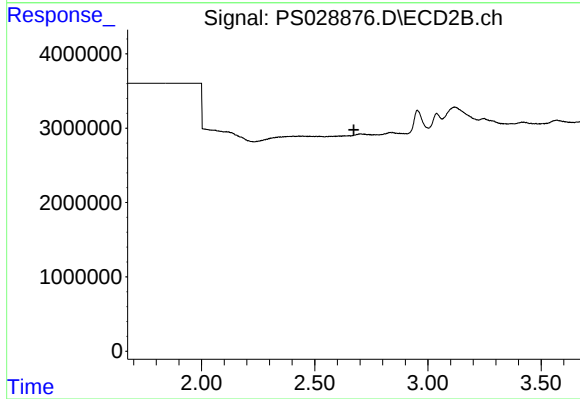


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 2.673 min
Response: 0
Conc: N.D.

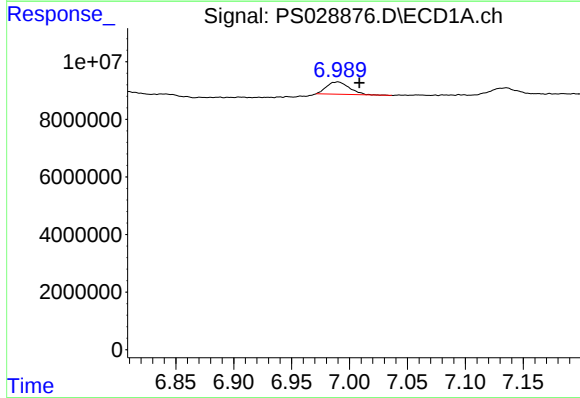


#3 4-Nitrophenol

R.T.: 6.989 min
Delta R.T.: -0.019 min
Response: 5910049
Conc: 3.93 ng/ml

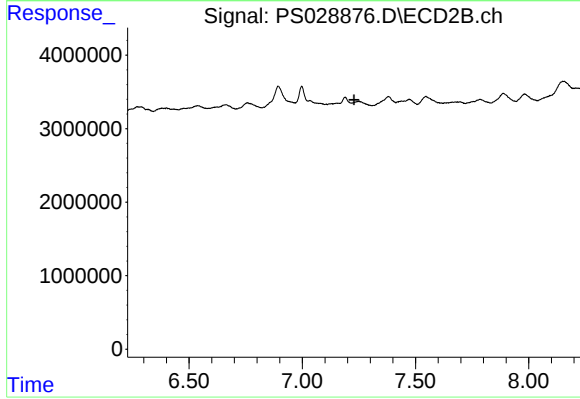

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T. : 7.228 min
Response: 0
Conc: N.D.

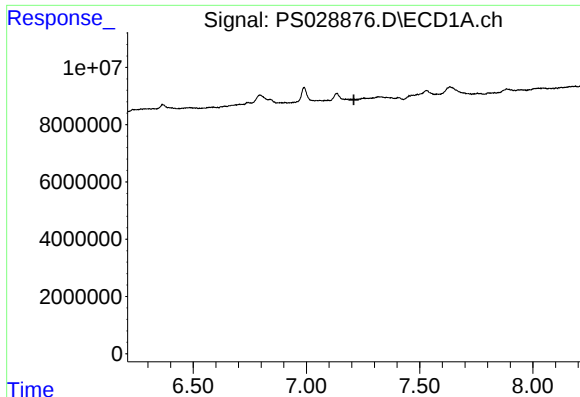

#4 2,4-DCAA


R.T.: 7.254 min
Delta R.T.: 0.044 min
Response: -143256
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

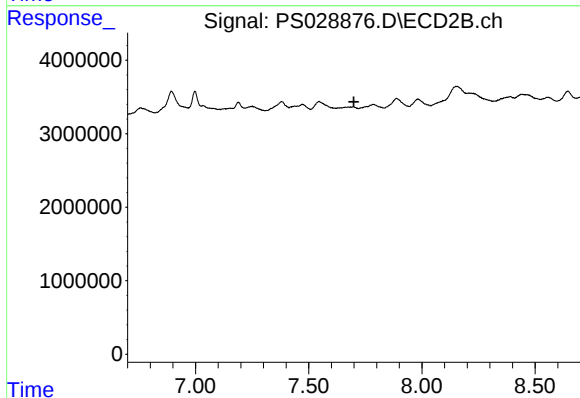


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 7.699 min
Response: 0
Conc: N.D.

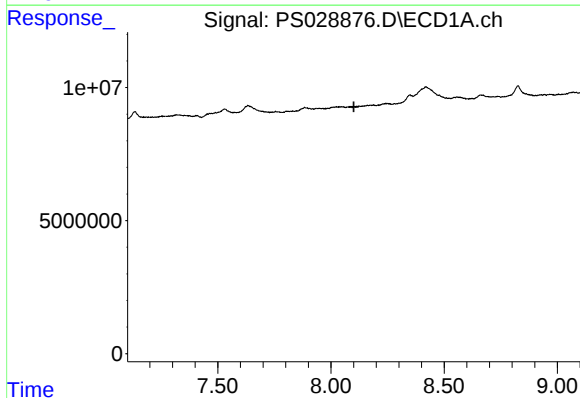


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.101 min
Response: 0
Conc: N.D.

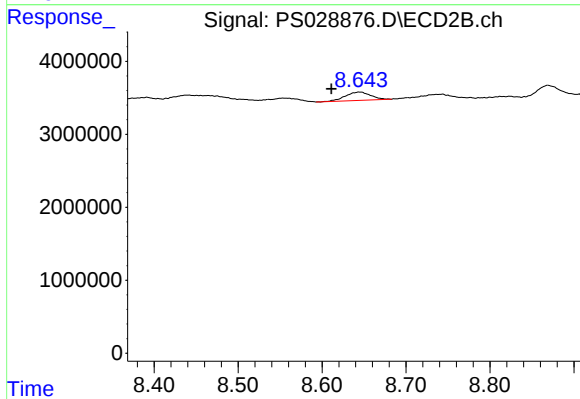

#8 DICHLORPROP


R.T.: 8.644 min
Delta R.T.: 0.033 min
Response: 2397843
Conc: 1.74 ng/ml

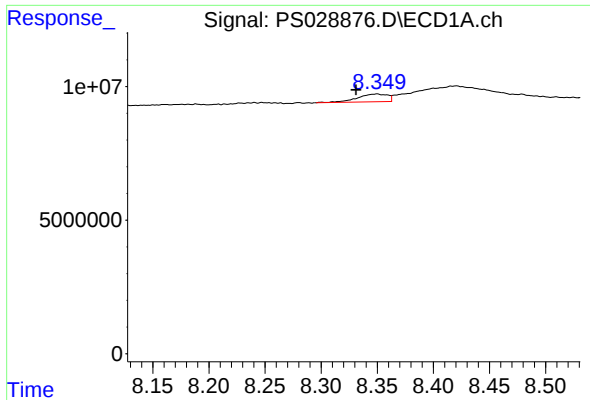

#9 2,4-D

R.T.: 8.349 min
Delta R.T.: 0.018 min
Response: 5366905
Conc: 1.88 ng/ml

Instrument :
ECD_S
ClientSampleId :

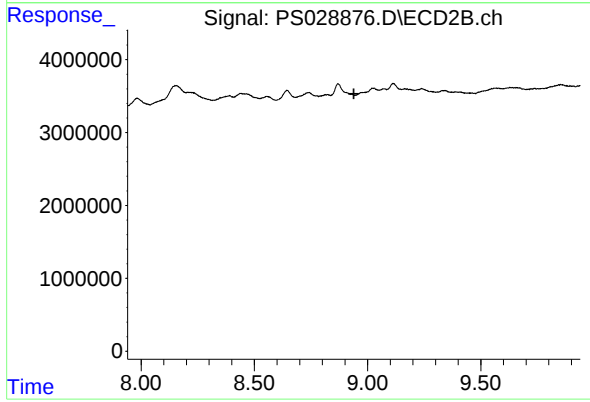

#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 8.939 min
Response: 0
Conc: N.D.