

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS011025\
 Data File : PS028877.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Jan 2025 09:10
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 11 01:45:13 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS122324.M
 Quant Title : 8080.M
 QLast Update : Mon Dec 23 13:44:25 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.204	7.684	1191.4E6	486.0E6	526.700	431.783
Target Compounds							
1) T	Dalapon	2.661f	0.000	3235044	0	1.149	N.D. #
2) T	3,5-DICHL...	6.396	0.000	1090115	0	<MDL	N.D. #
3) T	4-Nitroph...	6.990	0.000	15535993	0	10.343	N.D. #
5) T	DICAMBA	7.421	7.880	-1087332	9186711	N.D.	1.673
6) T	MCPD	7.526f	0.000	4713792	0	<MDL	N.D. #
7) T	MCPA	7.758f	8.235	200017	114106	<MDL	<MDL #
8) T	DICHLORPROP	8.128f	8.640f	2434748	3444364	<MDL	2.497 #
9) T	2,4-D	8.346	8.965f	6309919	325290	2.214	<MDL #
10) T	Pentachlo...	8.656f	0.000	10874266	0	<MDL	N.D. #
11) T	2,4,5-TP ...	9.178f	9.837	3979402	11851934	<MDL	1.319 #
12) T	2,4,5-T	9.547f	10.238	1401209	2543325	<MDL	<MDL #
13) T	2,4-DB	10.050	0.000	3284140	0	1.052	N.D. #
15) T	Picloram	11.088	12.274	12791031	3163650	<MDL	<MDL #
16) T	DCPA	11.559	12.274f	1587631	3163650	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS011025\
Data File : PS028877.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Jan 2025 09:10
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 11 01:45:13 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS122324.M
Quant Title : 8080.M
QLast Update : Mon Dec 23 13:44:25 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

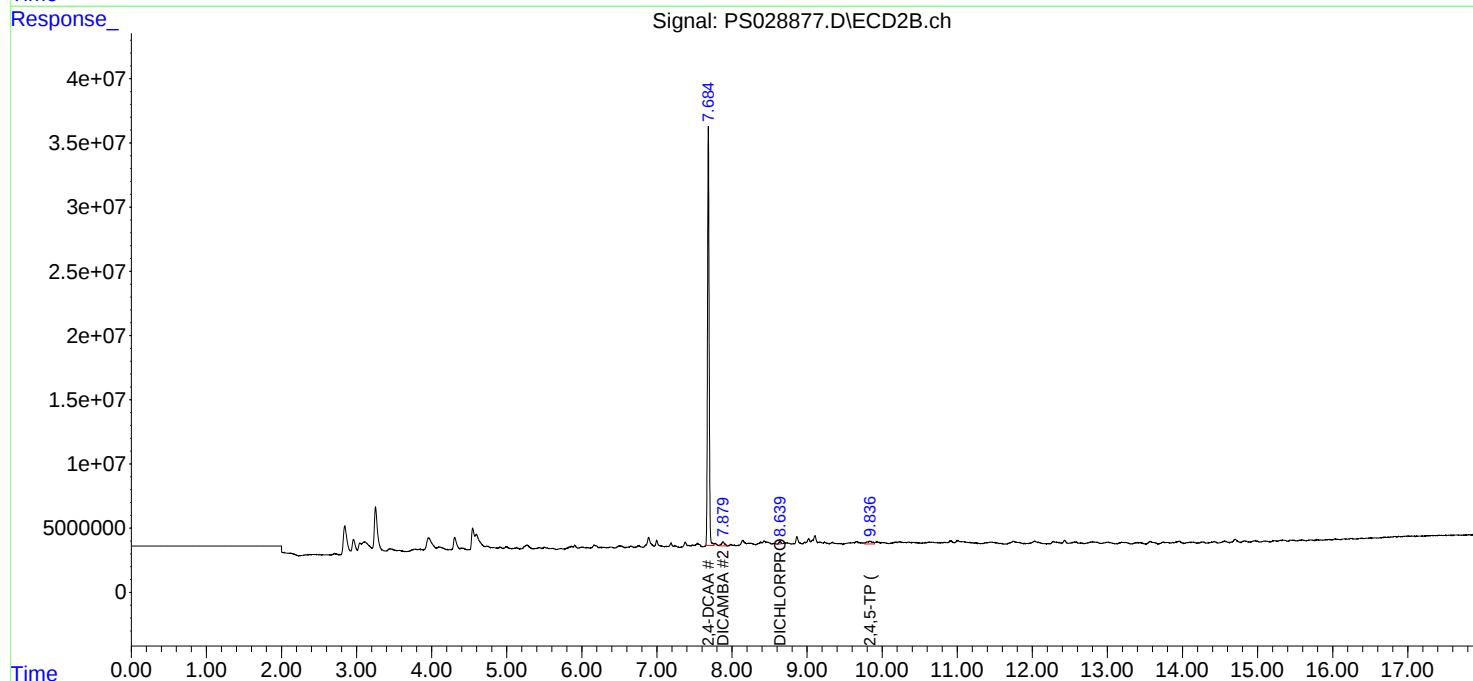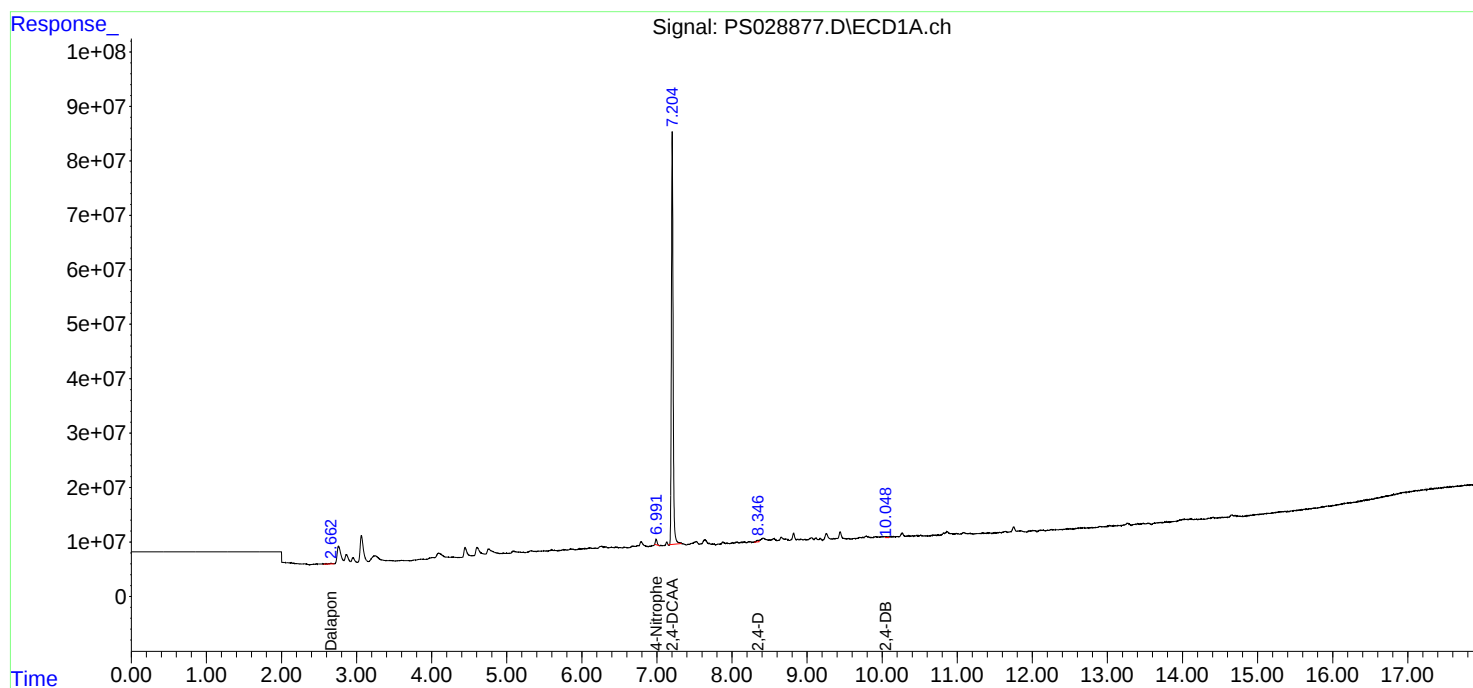


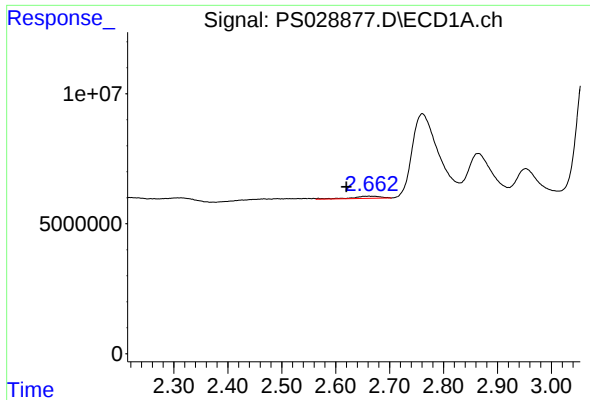

#1 Dalapon


R.T.: 2.661 min
Delta R.T.: 0.041 min
Response: 3235044
Conc: 1.15 ng/ml

Instrument :
ECD_S
ClientSampleId :

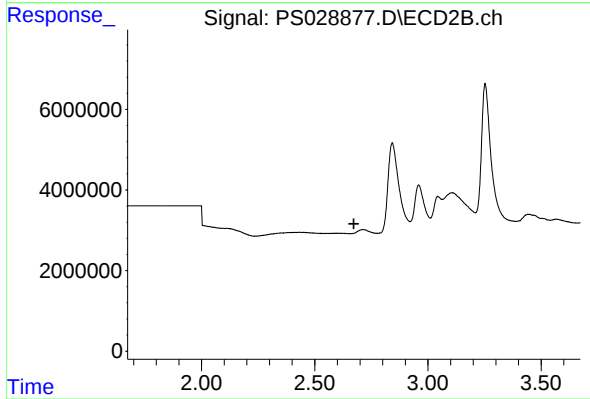


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 2.673 min
Response: 0
Conc: N.D.

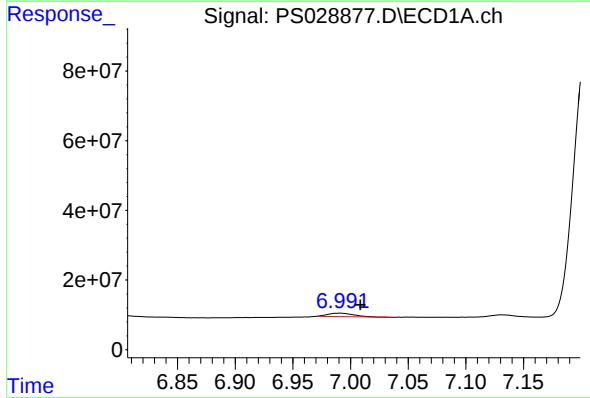


#3 4-Nitrophenol

R.T.: 6.990 min
Delta R.T.: -0.018 min
Response: 15535993
Conc: 10.34 ng/ml

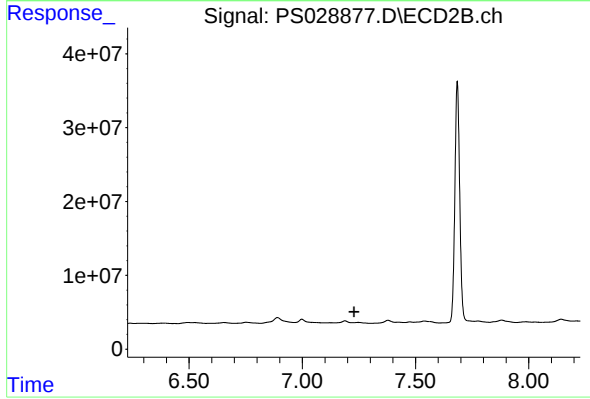

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T. : 7.228 min
Response: 0
Conc: N.D.

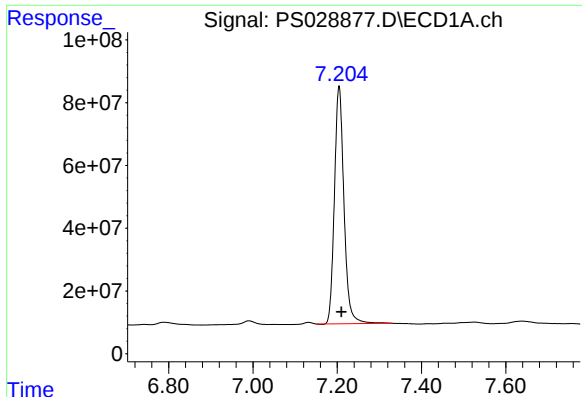

#4 2,4-DCAA


R.T.: 7.204 min
Delta R.T.: -0.005 min
Response: 1191408771
Conc: 526.70 ng/ml

Instrument :
ECD_S
ClientSampleId :

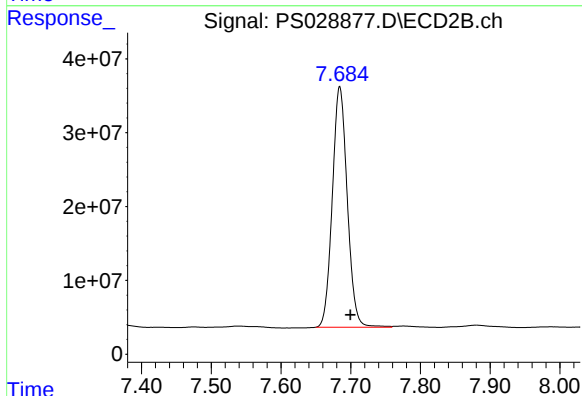


#4 2,4-DCAA

R.T.: 7.684 min
Delta R.T.: -0.015 min
Response: 485988408
Conc: 431.78 ng/ml

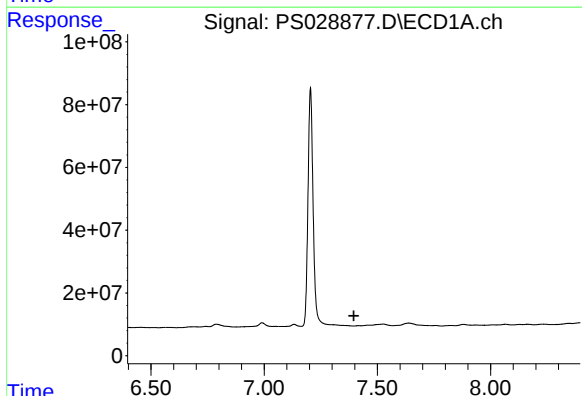


#5 DICAMBA

R.T.: 7.421 min
Delta R.T.: 0.025 min
Response: -1087332
Conc: N.D.

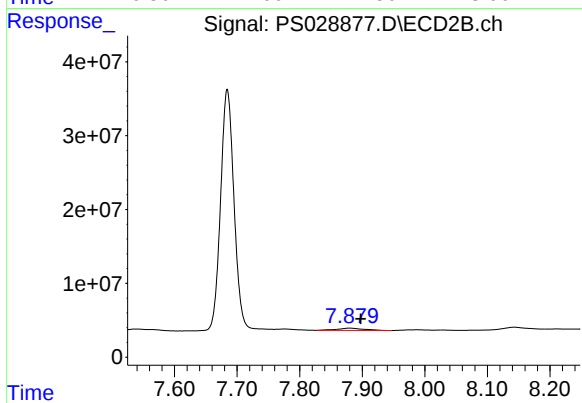

#5 DICAMBA


R.T.: 7.880 min
Delta R.T.: -0.018 min
Response: 9186711
Conc: 1.67 ng/ml

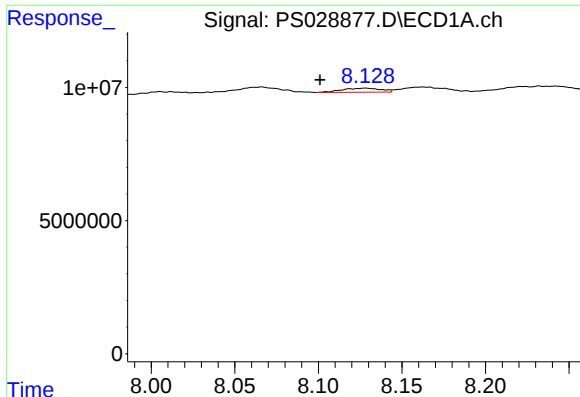

#8 DICHLORPROP


R.T.: 8.128 min
Delta R.T.: 0.027 min
Response: 2434748
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

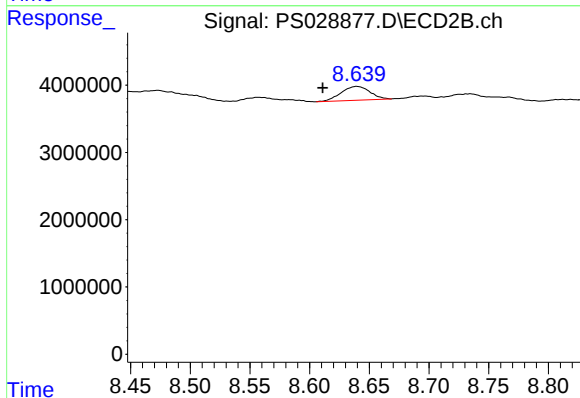


#8 DICHLORPROP

R.T.: 8.640 min
Delta R.T.: 0.028 min
Response: 3444364
Conc: 2.50 ng/ml

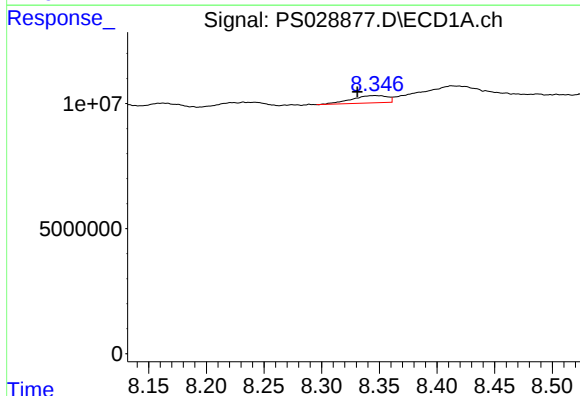


#9 2,4-D

R.T.: 8.346 min
Delta R.T.: 0.015 min
Response: 6309919
Conc: 2.21 ng/ml

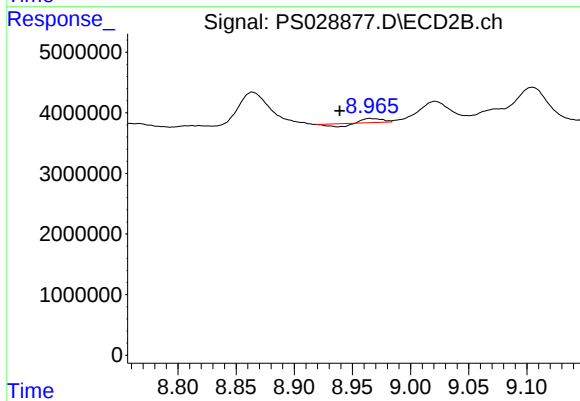

#9 2,4-D


R.T.: 8.965 min
Delta R.T.: 0.026 min
Response: 325290
Conc: N.D.

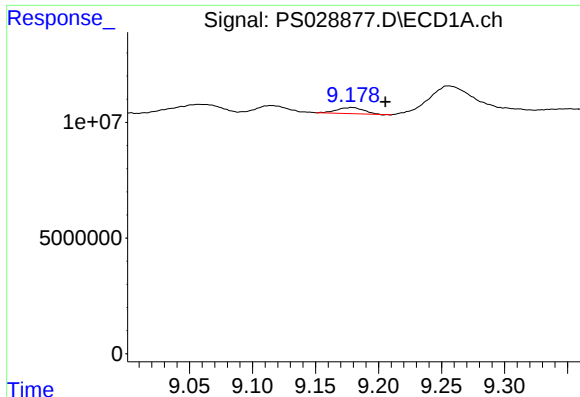

#11 2,4,5-TP (SILVEX)


R.T.: 9.178 min
Delta R.T.: -0.027 min
Response: 3979402
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

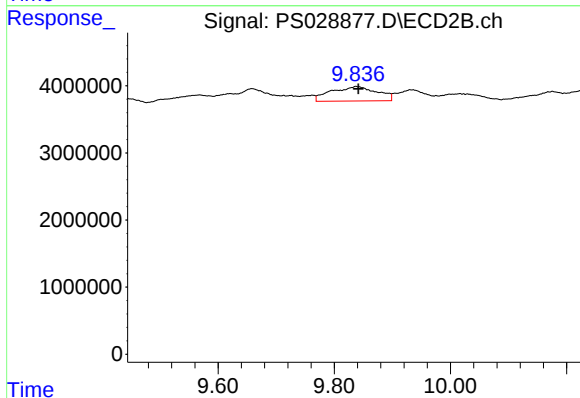


#11 2,4,5-TP (SILVEX)

R.T.: 9.837 min
Delta R.T.: -0.005 min
Response: 11851934
Conc: 1.32 ng/ml

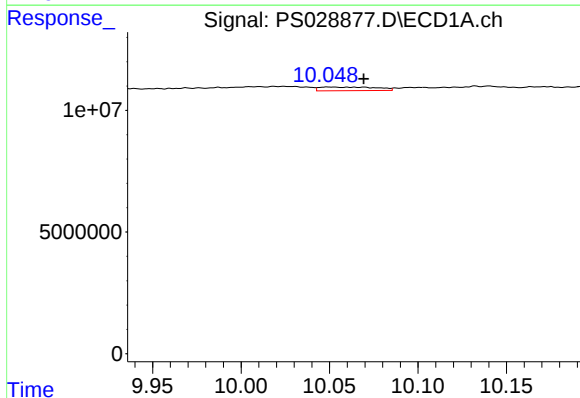

#13 2,4-DB

R.T.: 10.050 min
Delta R.T.: -0.019 min
Response: 3284140
Conc: 1.05 ng/ml

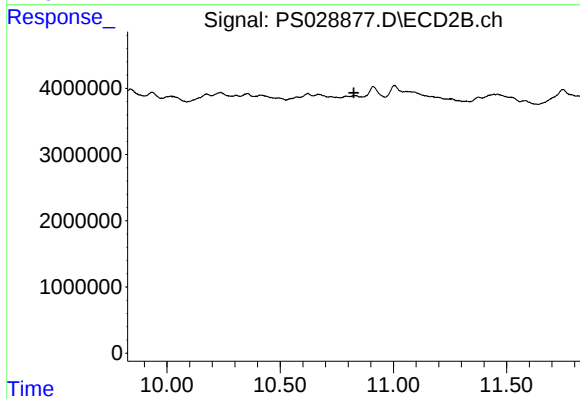

#13 2,4-DB

R.T.: 0.000 min
Exp R.T.: 10.826 min
Response: 0
Conc: N.D.