

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS011025\
 Data File : PS028884.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Jan 2025 14:07
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 11 01:47:41 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS122324.M
 Quant Title : 8080.M
 QLast Update : Mon Dec 23 13:44:25 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.205	7.686	1174.9E6	488.4E6	519.381	433.951
Target Compounds							
1) T	Dalapon	2.665f	0.000	2503473	0	<MDL	N.D. #
2) T	3,5-DICHL...	6.394	0.000	465547	0	<MDL	N.D. #
3) T	4-Nitroph...	6.993	0.000	7141270	0	4.754	N.D. #
5) T	DICAMBA	0.000	7.883	0	5749619	N.D.	1.047
6) T	MCPD	7.527f	7.991	2522584	1981933	<MDL	<MDL #
7) T	MCPA	0.000	8.230	0	4838853	N.D.	1.044
8) T	DICHLORPROP	8.068f	8.644f	5026688	12123677	1.895	8.787 #
10) T	Pentachlo...	8.623	0.000	96993	0	<MDL	N.D. #
11) T	2,4,5-TP ...	9.184	9.889f	1679505	10295366	<MDL	1.146 #
12) T	2,4,5-T	9.499	0.000	6527260	0	<MDL	N.D. #
13) T	2,4-DB	10.055	0.000	2863376	0	<MDL	N.D. #
14) T	DINOSEB	11.264	11.229	5481960	8415971	<MDL	1.366 #
15) T	Picloram	11.094	12.279	57892396	11155674	2.159	<MDL #
16) T	DCPA	11.545f	12.279f	2657137	11155674	<MDL	1.038 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS011025\
Data File : PS028884.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Jan 2025 14:07
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 11 01:47:41 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS122324.M
Quant Title : 8080.M
QLast Update : Mon Dec 23 13:44:25 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

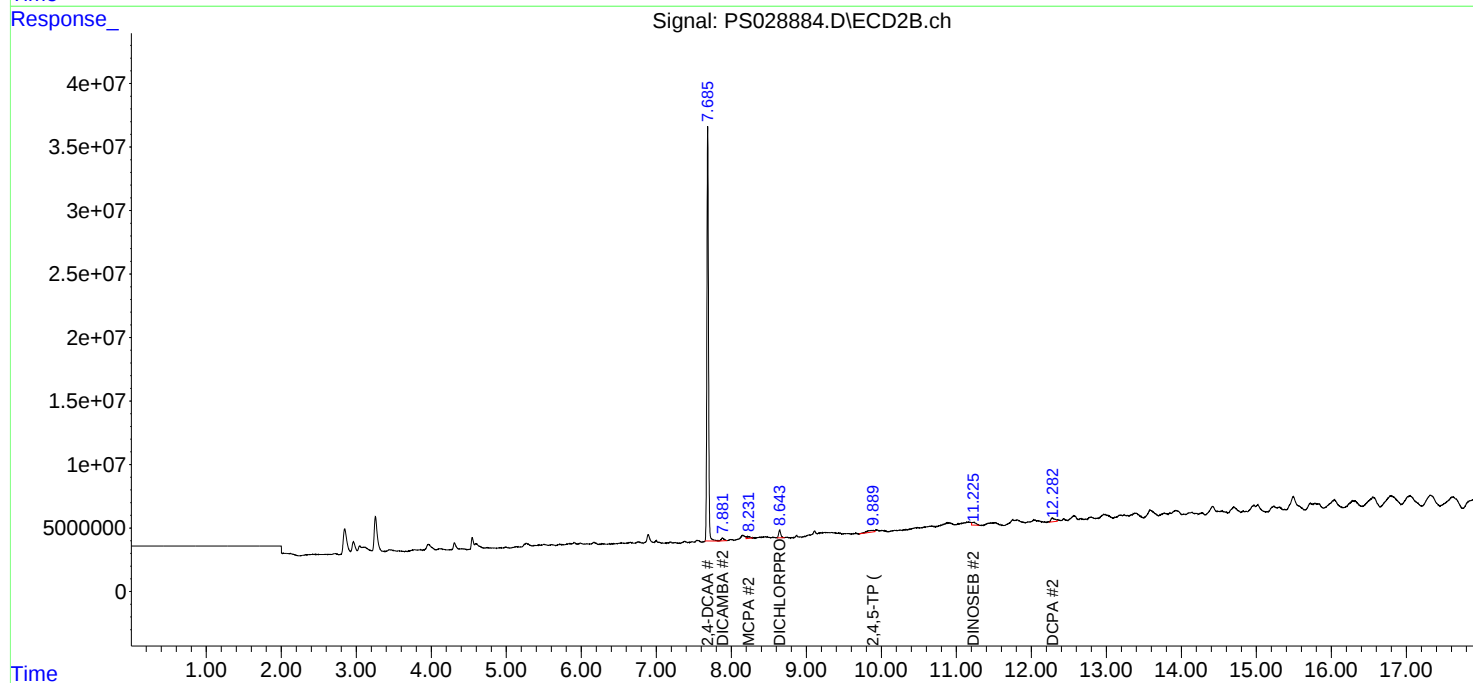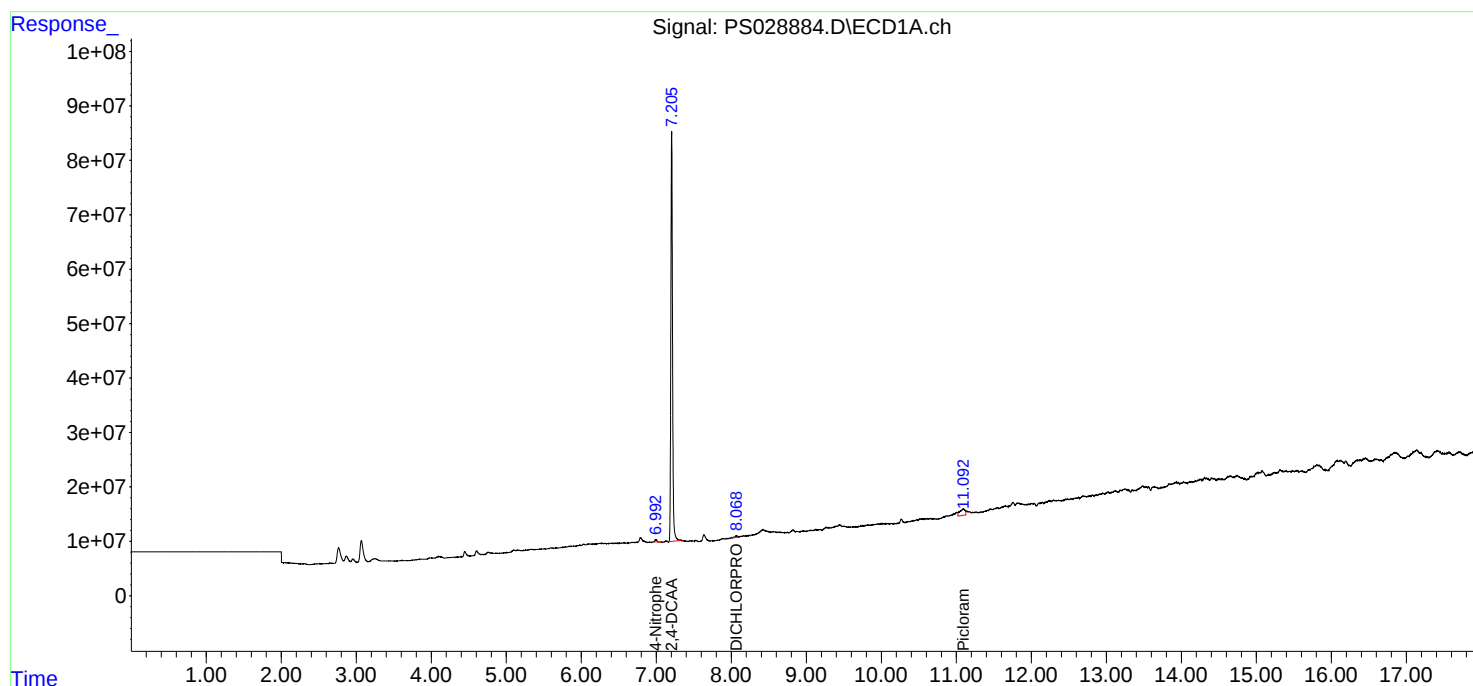


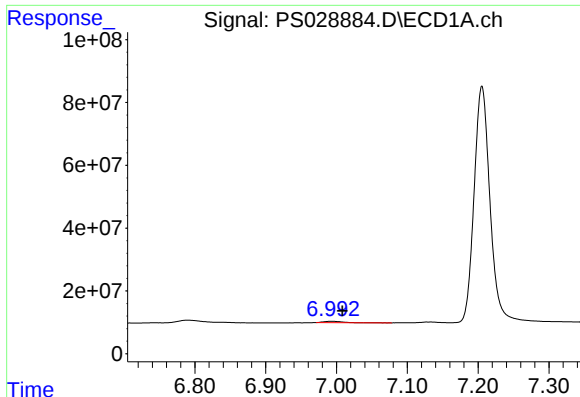

#3 4-Nitrophenol


R.T.: 6.993 min
Delta R.T.: -0.016 min
Response: 7141270
Conc: 4.75 ng/ml

Instrument :
ECD_S
ClientSampleId :

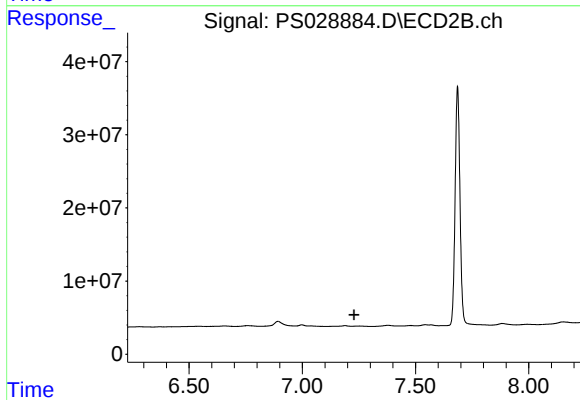


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 7.228 min
Response: 0
Conc: N.D.

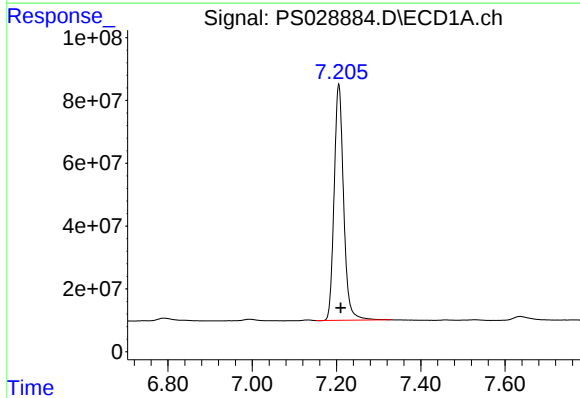


#4 2,4-DCAA

R.T.: 7.205 min
Delta R.T.: -0.005 min
Response: 1174852035
Conc: 519.38 ng/ml

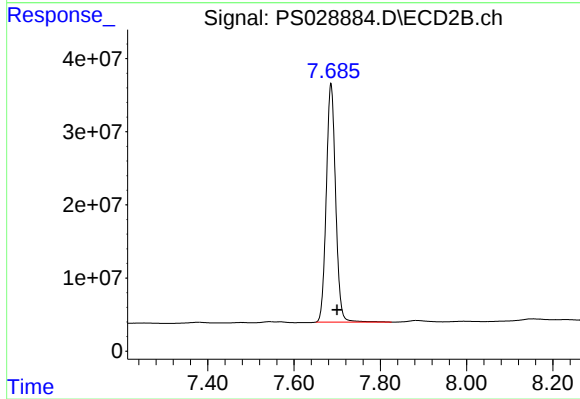

#4 2,4-DCAA


R.T.: 7.686 min
Delta R.T.: -0.014 min
Response: 488428249
Conc: 433.95 ng/ml

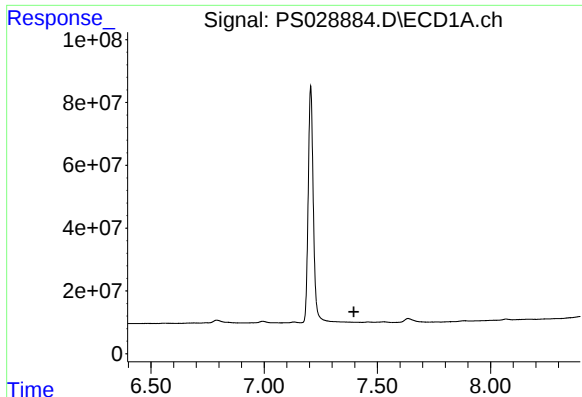

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 7.396 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

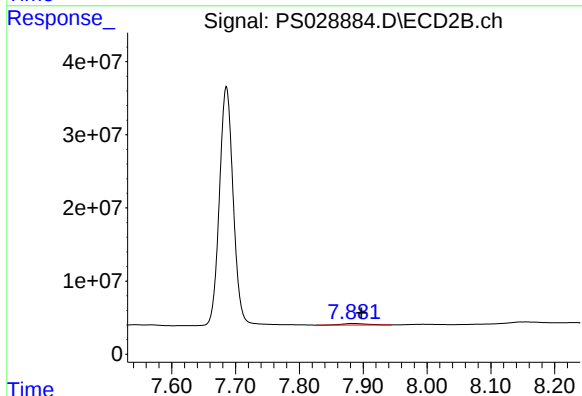


#5 DICAMBA

R.T.: 7.883 min
Delta R.T.: -0.014 min
Response: 5749619
Conc: 1.05 ng/ml

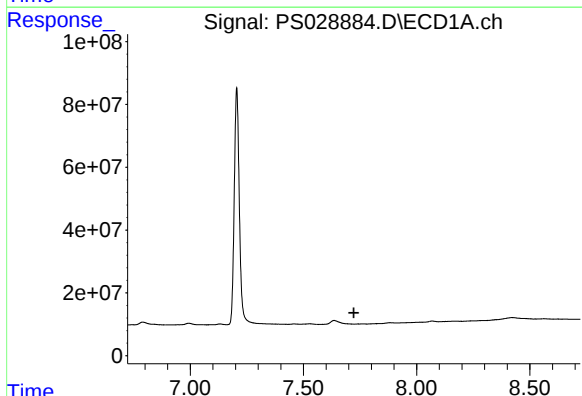


#7 MCPA

R.T.: 0.000 min
Exp R.T.: 7.723 min
Response: 0
Conc: N.D.

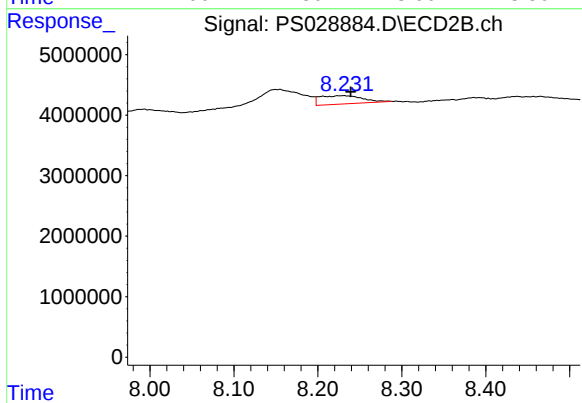

#7 MCPA


R.T.: 8.230 min
Delta R.T.: -0.009 min
Response: 4838853
Conc: 1.04 ug/ml

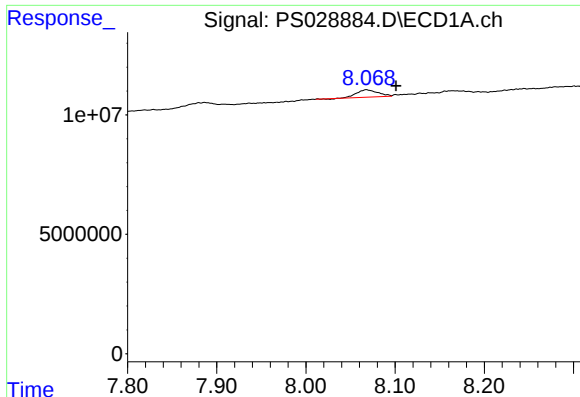

#8 DICHLORPROP


R.T.: 8.068 min
Delta R.T.: -0.033 min
Response: 5026688
Conc: 1.89 ng/ml

Instrument :
ECD_S
ClientSampleId :

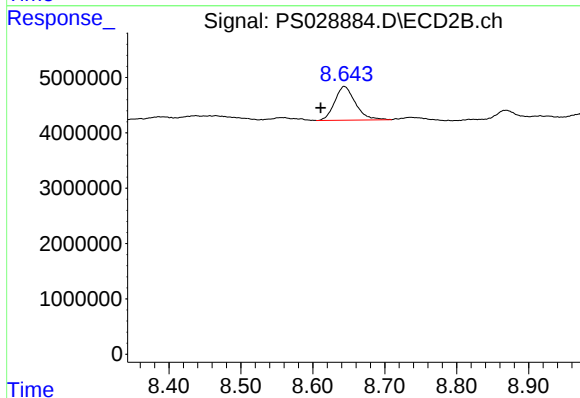


#8 DICHLORPROP

R.T.: 8.644 min
Delta R.T.: 0.033 min
Response: 12123677
Conc: 8.79 ng/ml

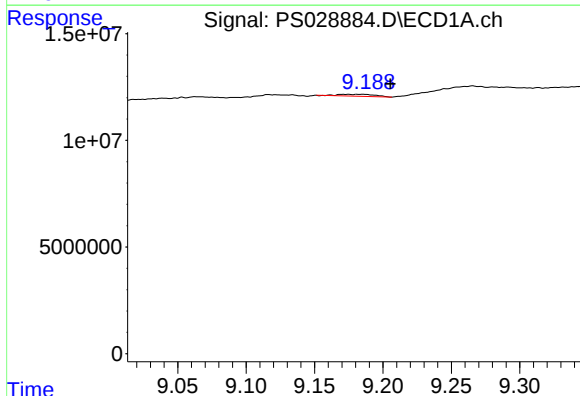


#11 2,4,5-TP (SILVEX)

R.T.: 9.184 min
Delta R.T.: -0.021 min
Response: 1679505
Conc: N.D.

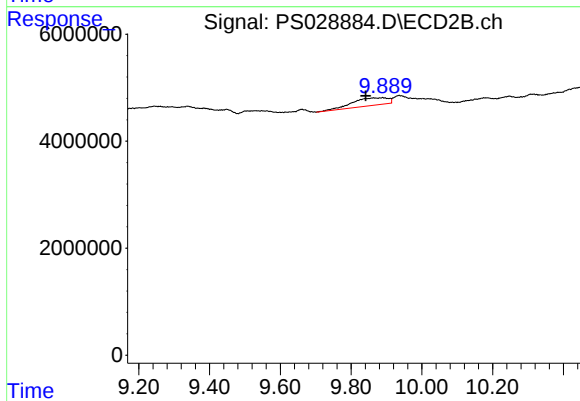

#11 2,4,5-TP (SILVEX)


R.T.: 9.889 min
Delta R.T.: 0.047 min
Response: 10295366
Conc: 1.15 ng/ml

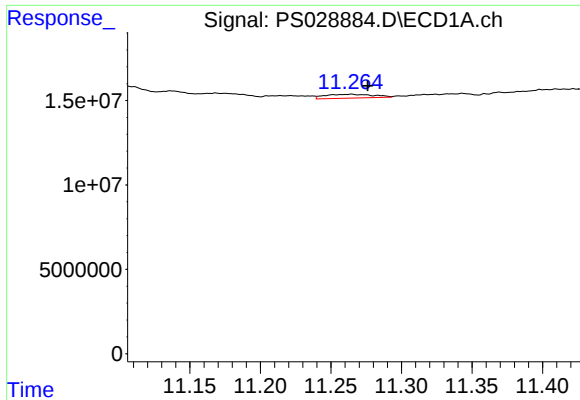

#14 DINOSEB


R.T.: 11.264 min
Delta R.T.: -0.012 min
Response: 5481960
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

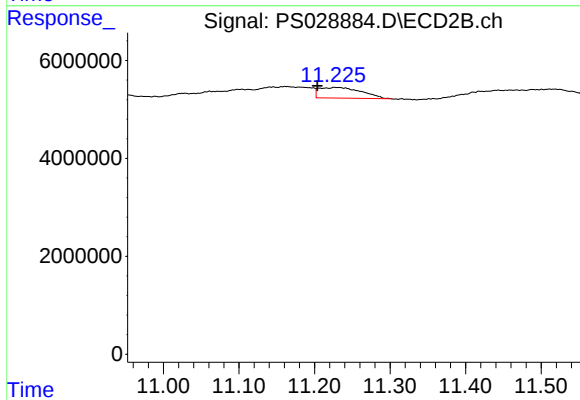


#14 DINOSEB

R.T.: 11.229 min
Delta R.T.: 0.025 min
Response: 8415971
Conc: 1.37 ng/ml

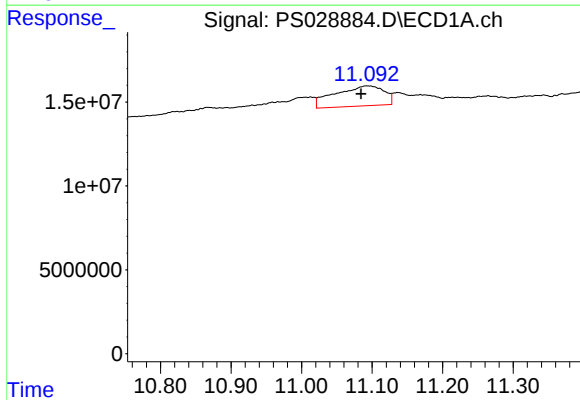


#15 Picloram

R.T.: 11.094 min
Delta R.T.: 0.009 min
Response: 57892396
Conc: 2.16 ng/ml

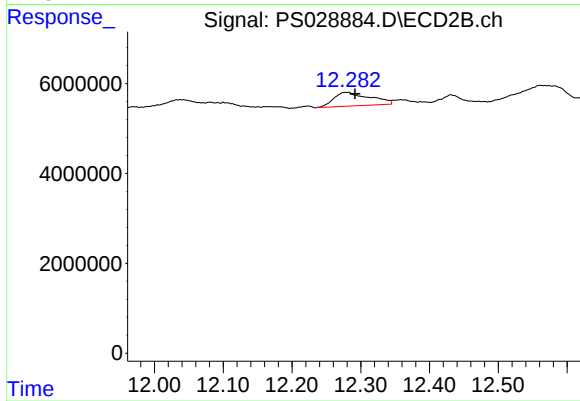

#15 Picloram


R.T.: 12.279 min
Delta R.T.: -0.012 min
Response: 11155674
Conc: N.D.

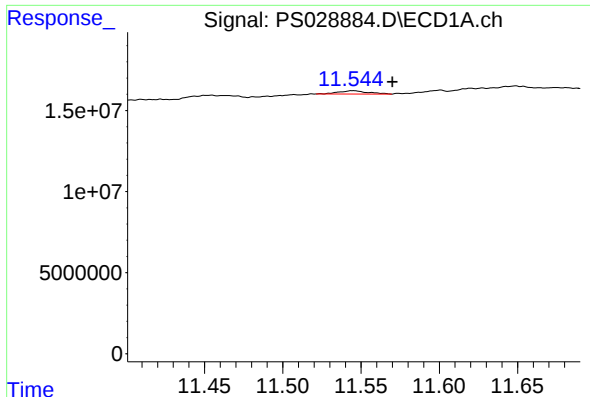

#16 DCPA

R.T.: 11.545 min
Delta R.T.: -0.025 min
Response: 2657137
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

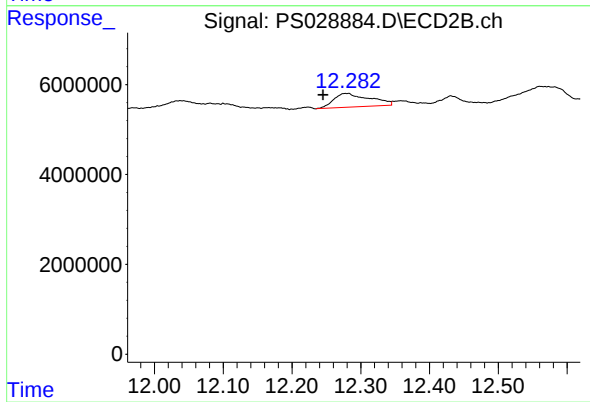

#16 DCPA

R.T.: 12.279 min
Delta R.T.: 0.034 min
Response: 11155674
Conc: 1.04 ng/ml