

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS011121\
 Data File : PS013736.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Jan 2021 16:19
 Operator : DD\AJ
 Sample : PB133994BL
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 11 17:15:58 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010421.M
 Quant Title : 8080.M
 QLast Update : Tue Jan 05 01:51:07 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.208	6.910	537.6E6	235.5E6	562.544	585.772
Target Compounds							
1) T	Dalapon	2.988f	2.589	87807456	142.4E6	80.733	273.842 #
2) T	3,5-DICHL...	0.000	6.093	0	34517020	N.D.	54.789
3) T	4-Nitroph...	6.981f	0.000	14620272	0	30.751	N.D. #
5) T	DICAMBA	0.000	7.044	0	4774606	N.D.	2.780
7) T	MCPA	7.685	7.368	12129962	27168935	2.951	13.439 #
10) T	Pentachlo...	8.679f	0.000	18645705	0	1.316	N.D. #
11) T	2,4,5-TP ...	0.000	8.757	0	24106521	N.D.	10.092
12) T	2,4,5-T	9.395f	0.000	36833448	0	6.514	N.D. #
13) T	2,4-DB	10.052	0.000	5800901	0	5.937	N.D. #
14) T	DINOSEB	11.143	0.000	18076193	0	4.097	N.D. #
15) T	Picloram	0.000	11.007	0	7034280	N.D.	2.024



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS011121\
Data File : PS013736.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Jan 2021 16:19
Operator : DD\AJ
Sample : PB133994BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 11 17:15:58 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010421.M
Quant Title : 8080.M
QLast Update : Tue Jan 05 01:51:07 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

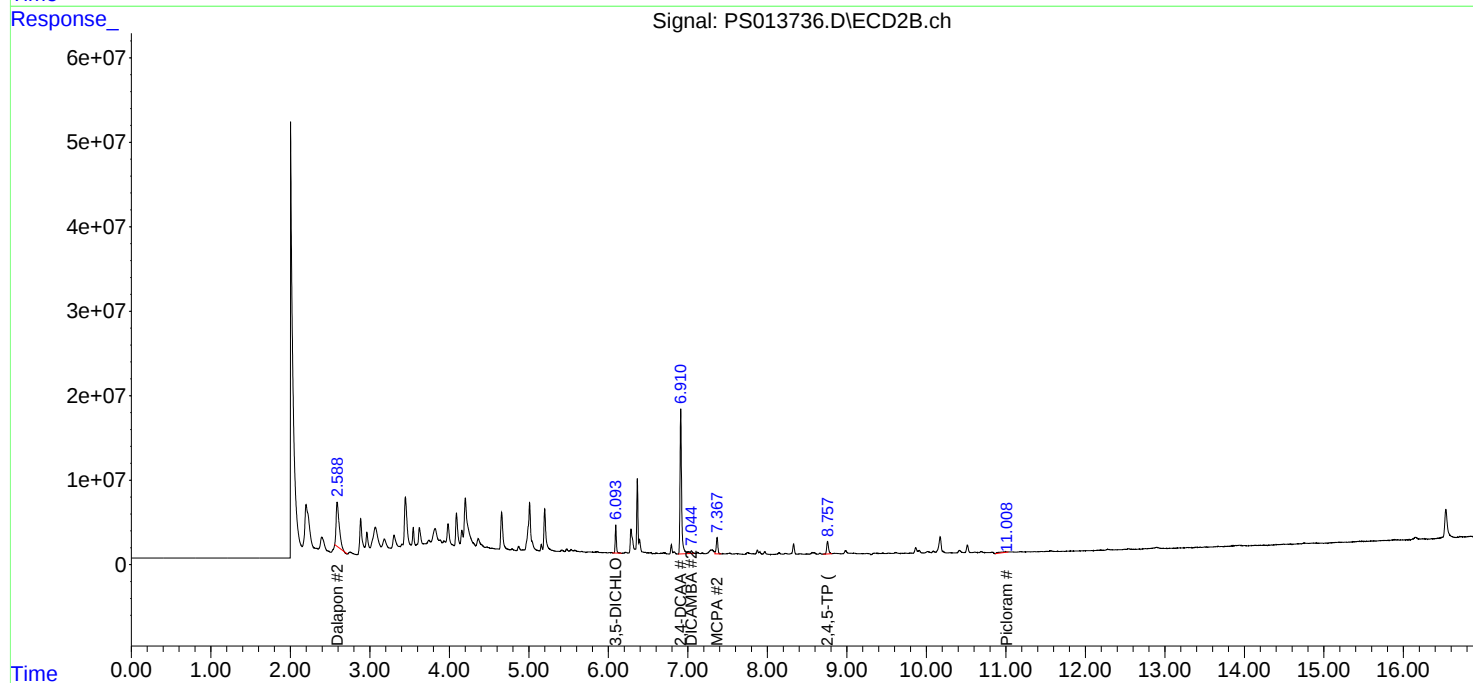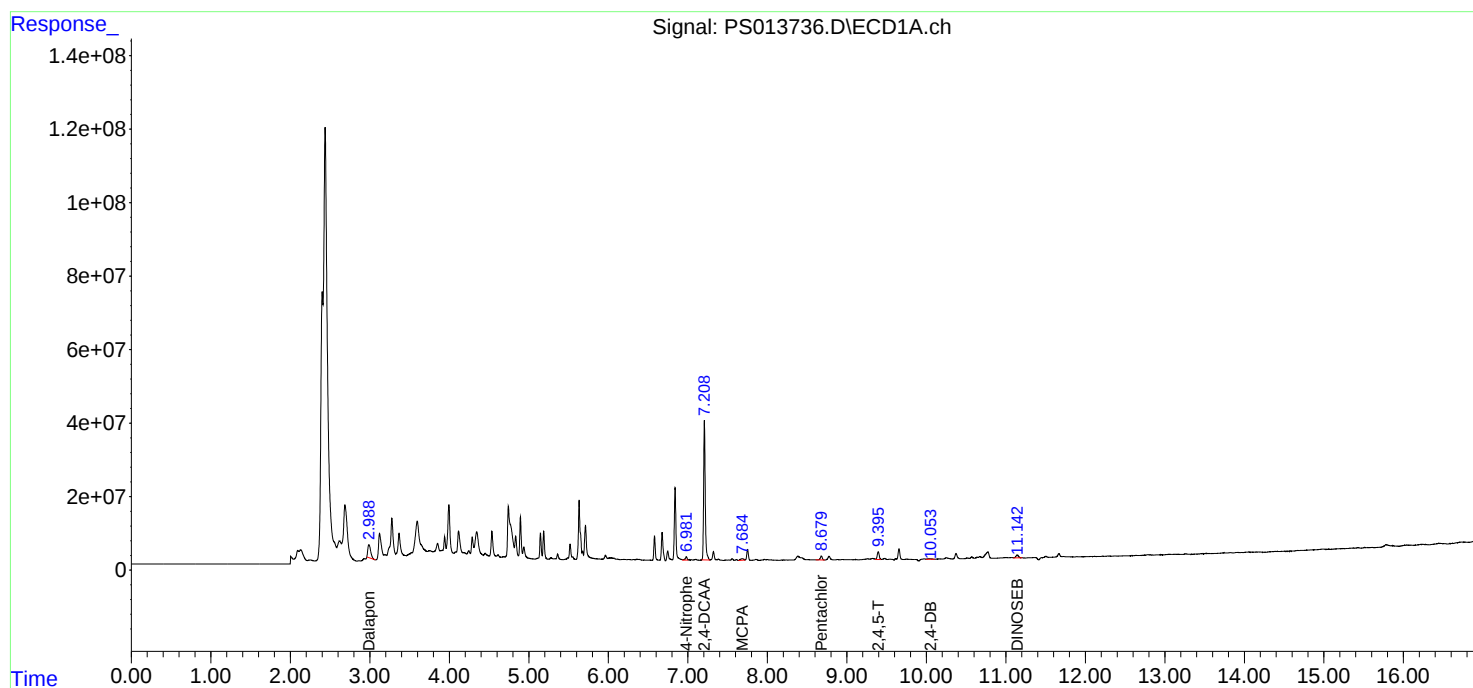


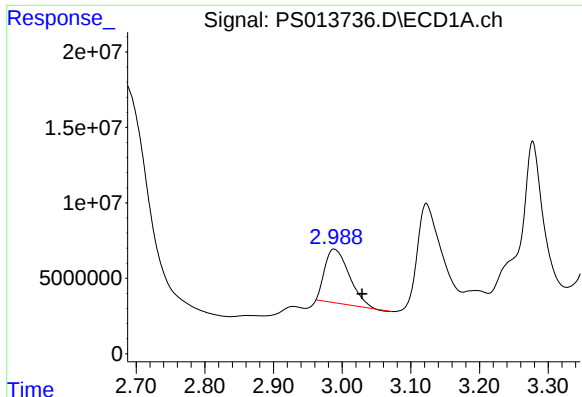

#1 Dalapon


R.T.: 2.988 min
Delta R.T.: -0.041 min
Response: 87807456
Conc: 80.73 ng/ml

Instrument :
ECD_S
ClientSampleId :

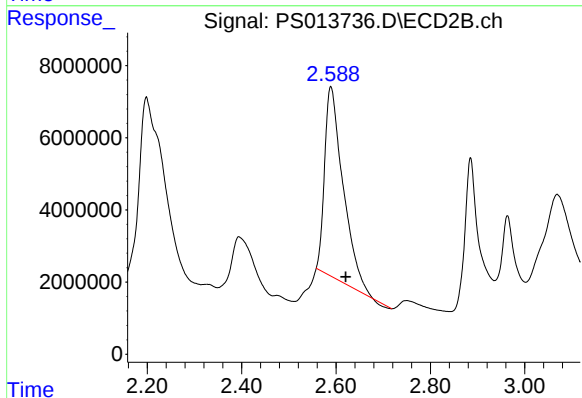


#1 Dalapon

R.T.: 2.589 min
Delta R.T.: -0.032 min
Response: 142383918
Conc: 273.84 ng/ml

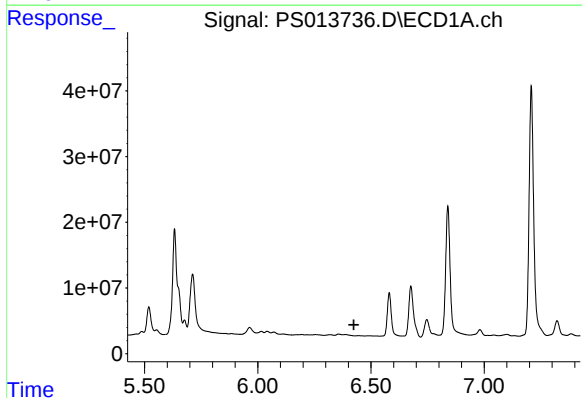


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.425 min
Response: 0
Conc: N.D.

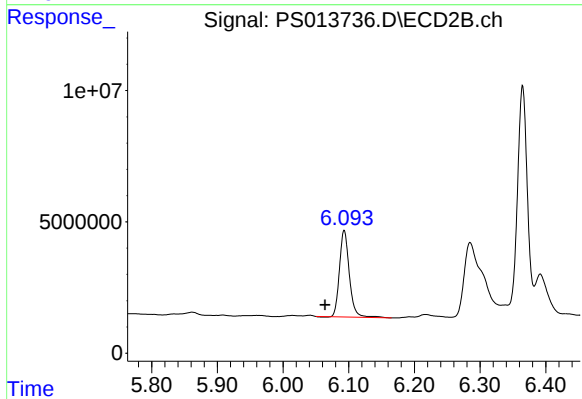

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.093 min
Delta R.T.: 0.029 min
Response: 34517020
Conc: 54.79 ng/ml

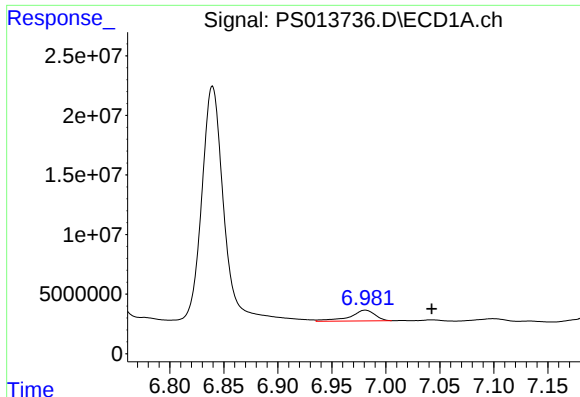

#3 4-Nitrophenol


R.T.: 6.981 min
Delta R.T.: -0.062 min
Response: 14620272
Conc: 30.75 ng/ml

Instrument :
ECD_S
ClientSampleId :

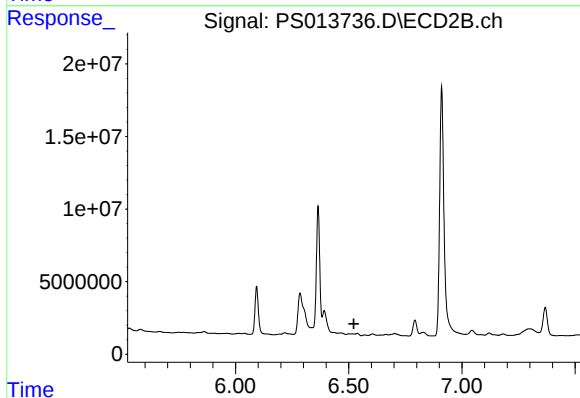


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.523 min
Response: 0
Conc: N.D.

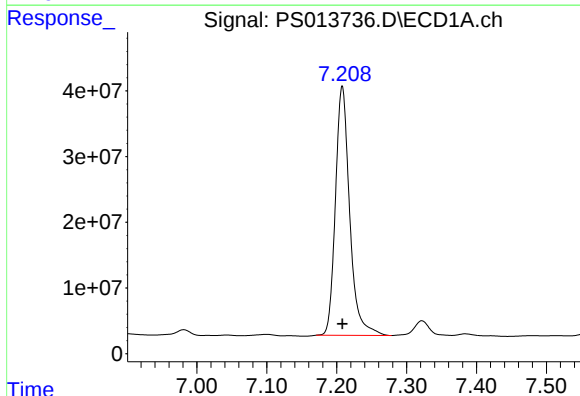


#4 2,4-DCAA

R.T.: 7.208 min
Delta R.T.: 0.000 min
Response: 537562679
Conc: 562.54 ng/ml

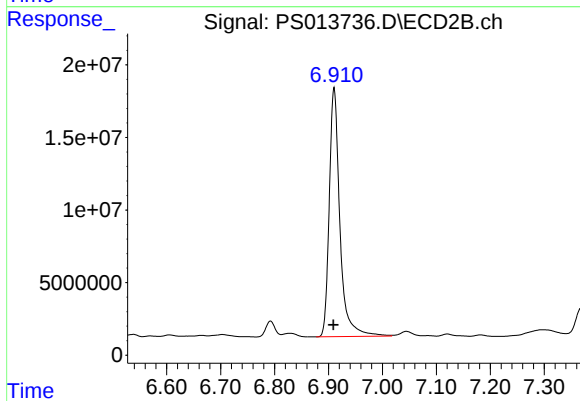

#4 2,4-DCAA


R.T.: 6.910 min
Delta R.T.: 0.000 min
Response: 235547658
Conc: 585.77 ng/ml

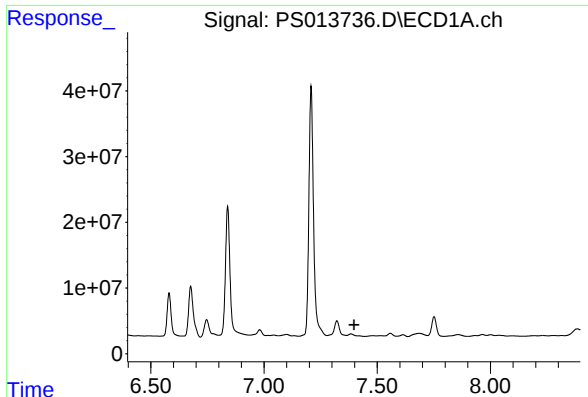

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 7.397 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

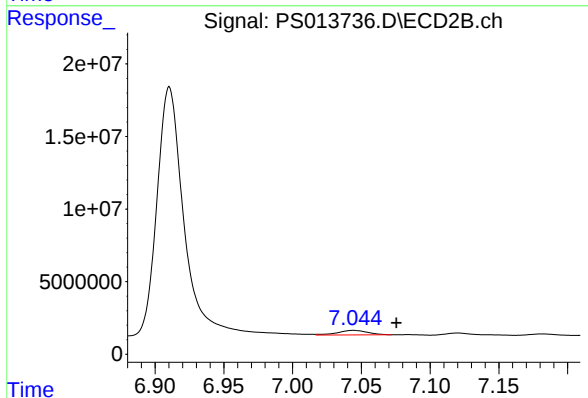


#5 DICAMBA

R.T.: 7.044 min
Delta R.T.: -0.031 min
Response: 4774606
Conc: 2.78 ng/ml

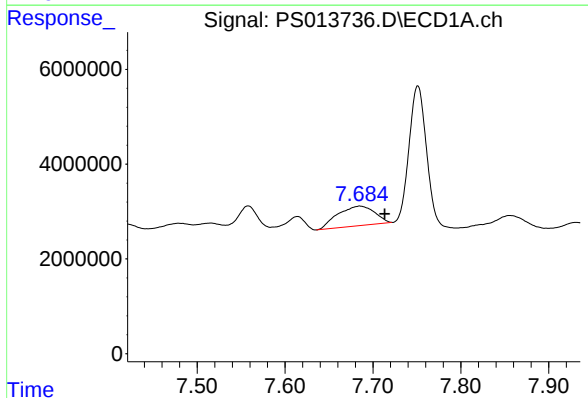


#7 MCPA

R.T.: 7.685 min
Delta R.T.: -0.028 min
Response: 12129962
Conc: 2.95 ug/ml

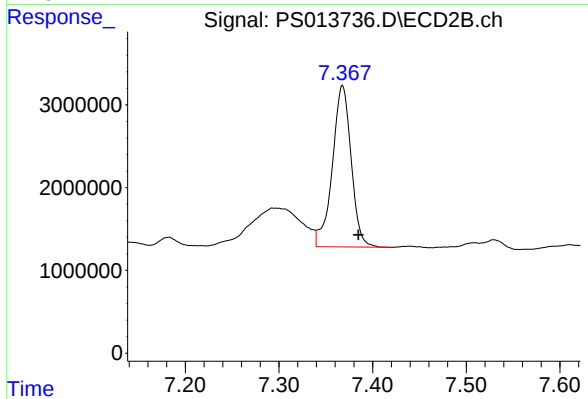

#7 MCPA


R.T.: 7.368 min
Delta R.T.: -0.017 min
Response: 27168935
Conc: 13.44 ug/ml

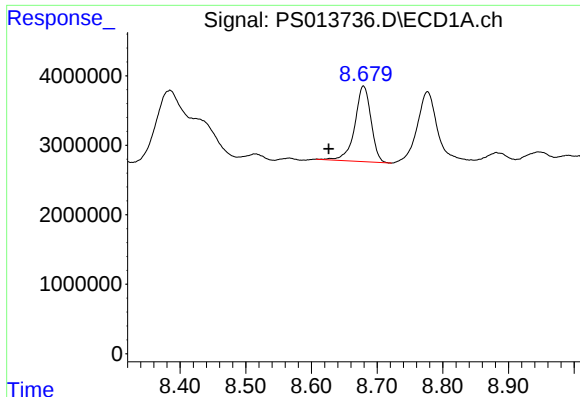

#10 Pentachlorophenol


R.T.: 8.679 min
Delta R.T.: 0.053 min
Response: 18645705
Conc: 1.32 ng/ml

Instrument :
ECD_S
ClientSampleId :

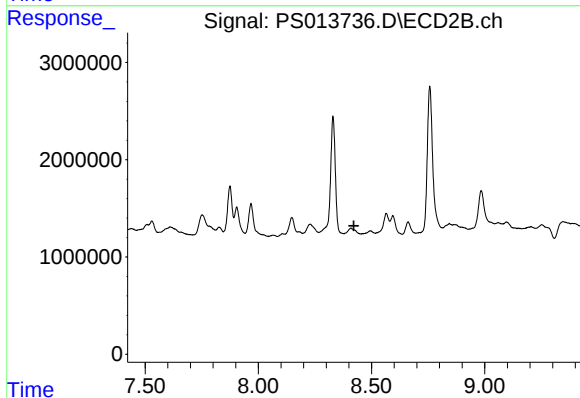


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T. : 8.422 min
Response: 0
Conc: N.D.

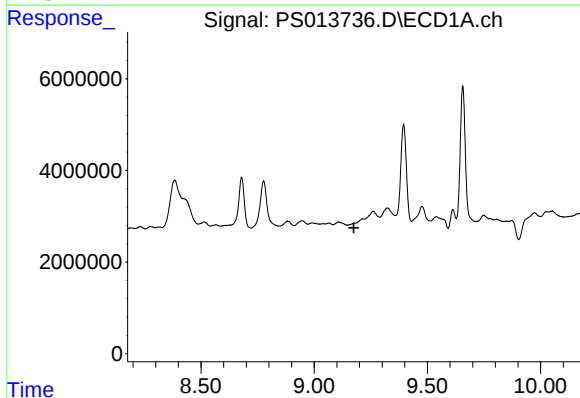


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 9.175 min
Response: 0
Conc: N.D.

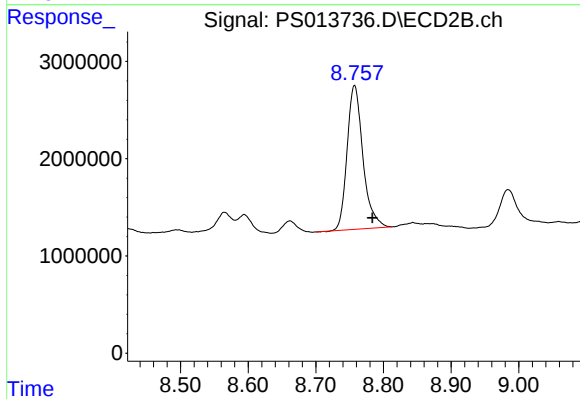

#11 2,4,5-TP (SILVEX)


R.T.: 8.757 min
Delta R.T.: -0.026 min
Response: 24106521
Conc: 10.09 ng/ml

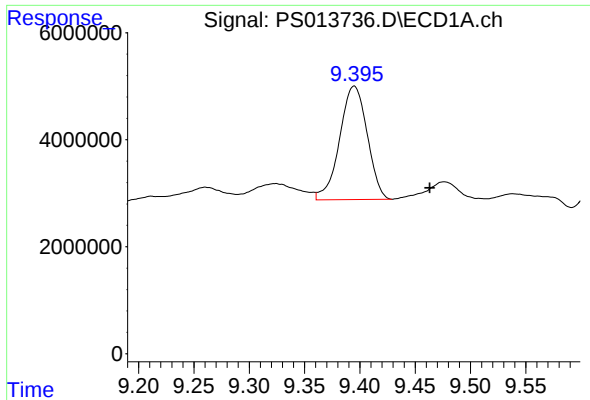

#12 2,4,5-T


R.T.: 9.395 min
Delta R.T.: -0.069 min
Response: 36833448
Conc: 6.51 ng/ml

Instrument :
ECD_S
ClientSampleId :

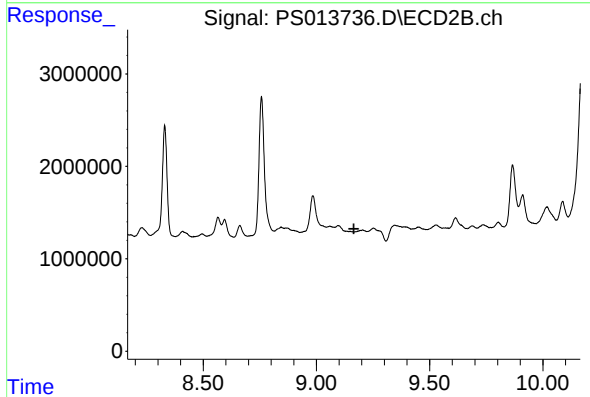


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 9.165 min
Response: 0
Conc: N.D.

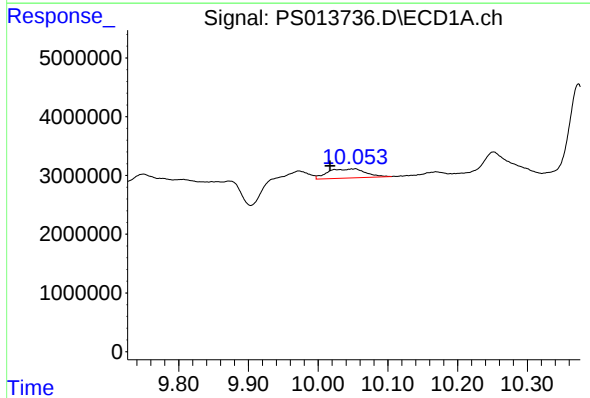


#13 2,4-DB

R.T.: 10.052 min
Delta R.T.: 0.034 min
Response: 5800901
Conc: 5.94 ng/ml

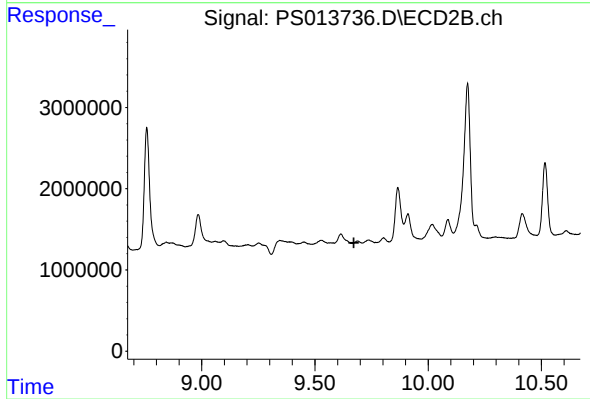

#13 2,4-DB


R.T.: 0.000 min
Exp R.T. : 9.672 min
Response: 0
Conc: N.D.

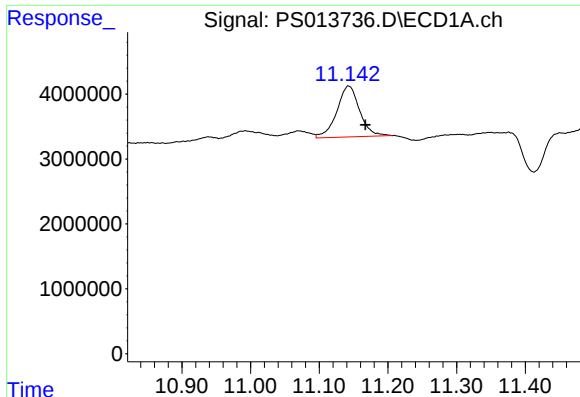

#14 DINOSEB


R.T.: 11.143 min
Delta R.T.: -0.025 min
Response: 18076193
Conc: 4.10 ng/ml

Instrument :
ECD_S
ClientSampleId :

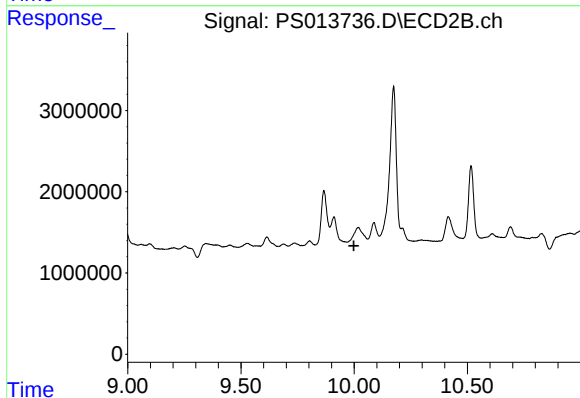


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 9.999 min
Response: 0
Conc: N.D.

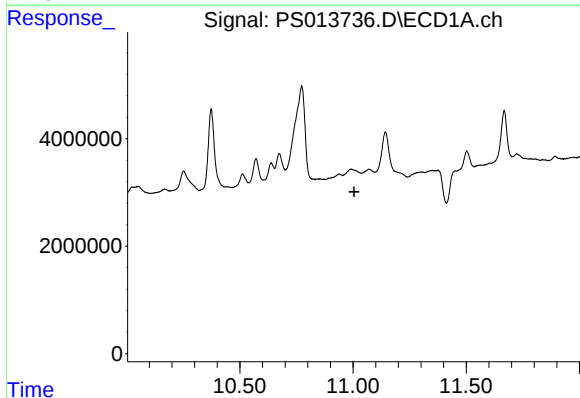

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 11.004 min
Response: 0
Conc: N.D.

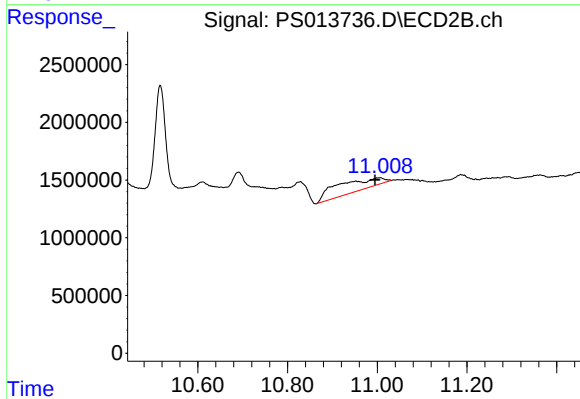

#15 Picloram

R.T.: 11.007 min
Delta R.T.: 0.012 min
Response: 7034280
Conc: 2.02 ng/ml