

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS011121\
 Data File : PS013724.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Jan 2021 11:44
 Operator : DD\AJ
 Sample : M1043-01
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 BALL-1

Manual Integrations
 APPROVED

Ankita
 1/12/2021 5:40:05 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 11 12:02:30 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010421.M
 Quant Title : 8080.M
 QLast Update : Tue Jan 05 01:51:07 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.207	6.911	246.7E6	110.1E6	258.202m	273.797m
Target Compounds							
10) T	Pentachlo...	8.626	8.423	380.2E6	158.5E6	26.837	27.428

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS011121\
Data File : PS013724.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Jan 2021 11:44
Operator : DD\AJ
Sample : M1043-01
Misc :
ALS Vial : 6 Sample Multiplier: 1



Instrument :
ECD_S
ClientSampleId :
BALL-1


Manual Integrations
APPROVED

Ankita
1/12/2021 5:40:05 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 11 12:02:30 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010421.M
Quant Title : 8080.M
QLast Update : Tue Jan 05 01:51:07 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

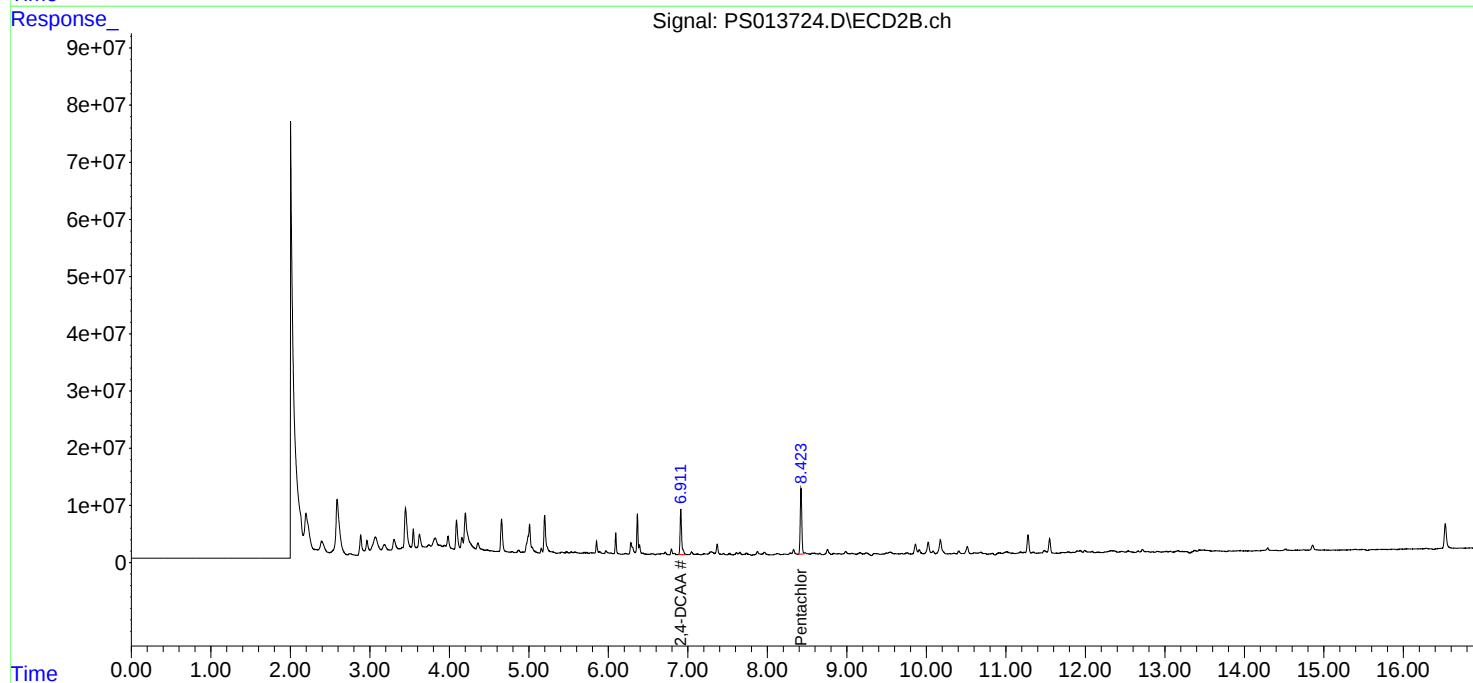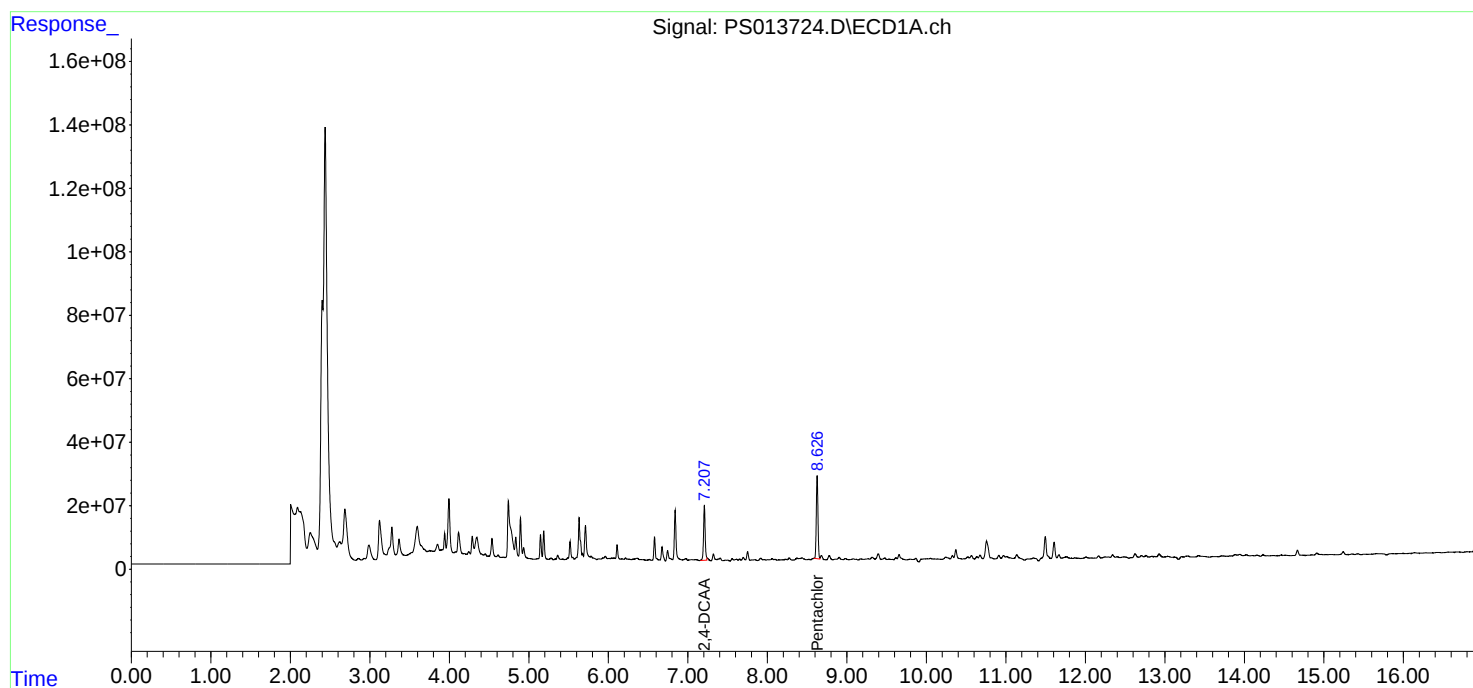

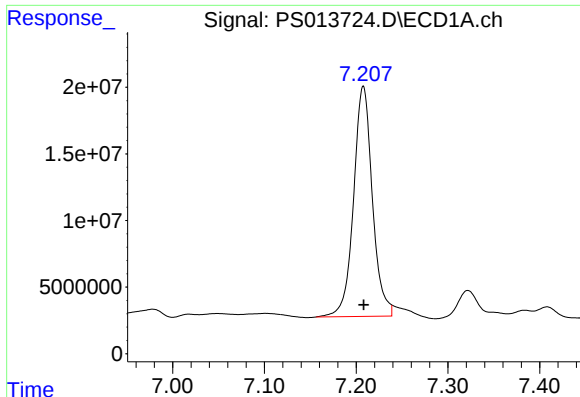


#4 2,4-DCAA

R.T.: 7.207 min
Delta R.T.: 0.000 min
Response: 246735563
Conc: 258.20 ng/ml m

Instrument :
ECD_S
ClientSampleId :
BALL-1


Manual Integrations
APPROVED

Ankita
1/12/2021 5:40:05 PM

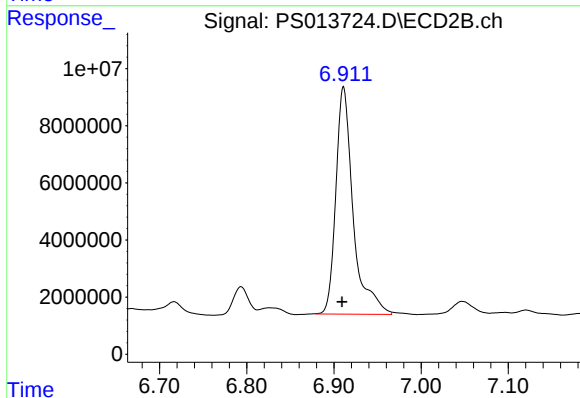


#4 2,4-DCAA

R.T.: 6.911 min
Delta R.T.: 0.001 min
Response: 110098035
Conc: 273.80 ng/ml m

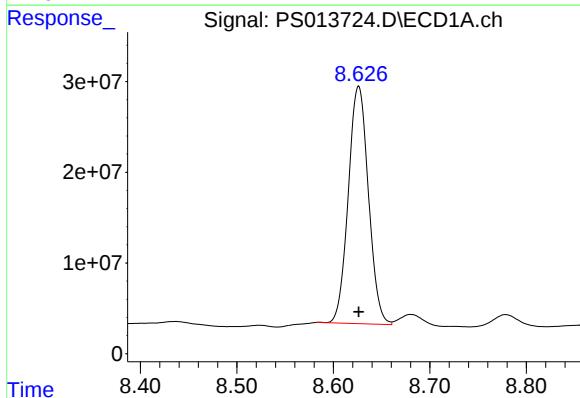

#10 Pentachlorophenol

R.T.: 8.626 min
Delta R.T.: 0.000 min
Response: 380199191
Conc: 26.84 ng/ml

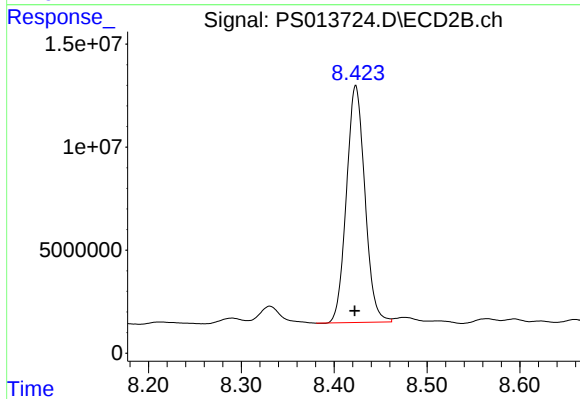

#10 Pentachlorophenol

R.T.: 8.423 min
Delta R.T.: 0.001 min
Response: 158549463
Conc: 27.43 ng/ml