

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS011122\
 Data File : PS017953.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Jan 2022 08:32
 Operator : AJ\MA
 Sample : HEXANE
 Misc : LOT#M03961
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 11 15:27:55 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010522.M
 Quant Title : 8080.M
 QLast Update : Thu Jan 06 10:21:08 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds							
2) T	3,5-DICHL...	6.291	0.000	671565	0	<MDL	N.D. #
5) T	DICAMBA	7.238	0.000	8297745	0	1.329	N.D. #
7) T	MCPA	7.482f	0.000	6085294	0	<MDL	N.D. #
8) T	DICHLORPROP	7.923	0.000	3312065	0	2.106	N.D. #
9) T	2,4-D	8.152	0.000	7688796	0	4.222	N.D. #
10) T	Pentachlo...	8.450	8.112	22179434	9712643	1.050	1.153
11) T	2,4,5-TP ...	9.002	8.473	17387748	4978777	2.055	1.397 #
12) T	2,4,5-T	9.284	8.851	26388116	10317643	2.977	3.154
13) T	2,4-DB	9.826	0.000	19758452	0	11.953	N.D. #
14) T	DINOSEB	10.979	9.674	12128636	7163814	1.847	2.871 #
15) T	Picloram	10.802	10.653	269.8E6	79291350	22.605	16.957
16) T	DCPA	11.249	10.600	26693550	10373658	2.471	2.349



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS011122\
Data File : PS017953.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Jan 2022 08:32
Operator : AJ\MA
Sample : HEXANE
Misc : LOT#M03961
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 11 15:27:55 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010522.M
Quant Title : 8080.M
QLast Update : Thu Jan 06 10:21:08 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

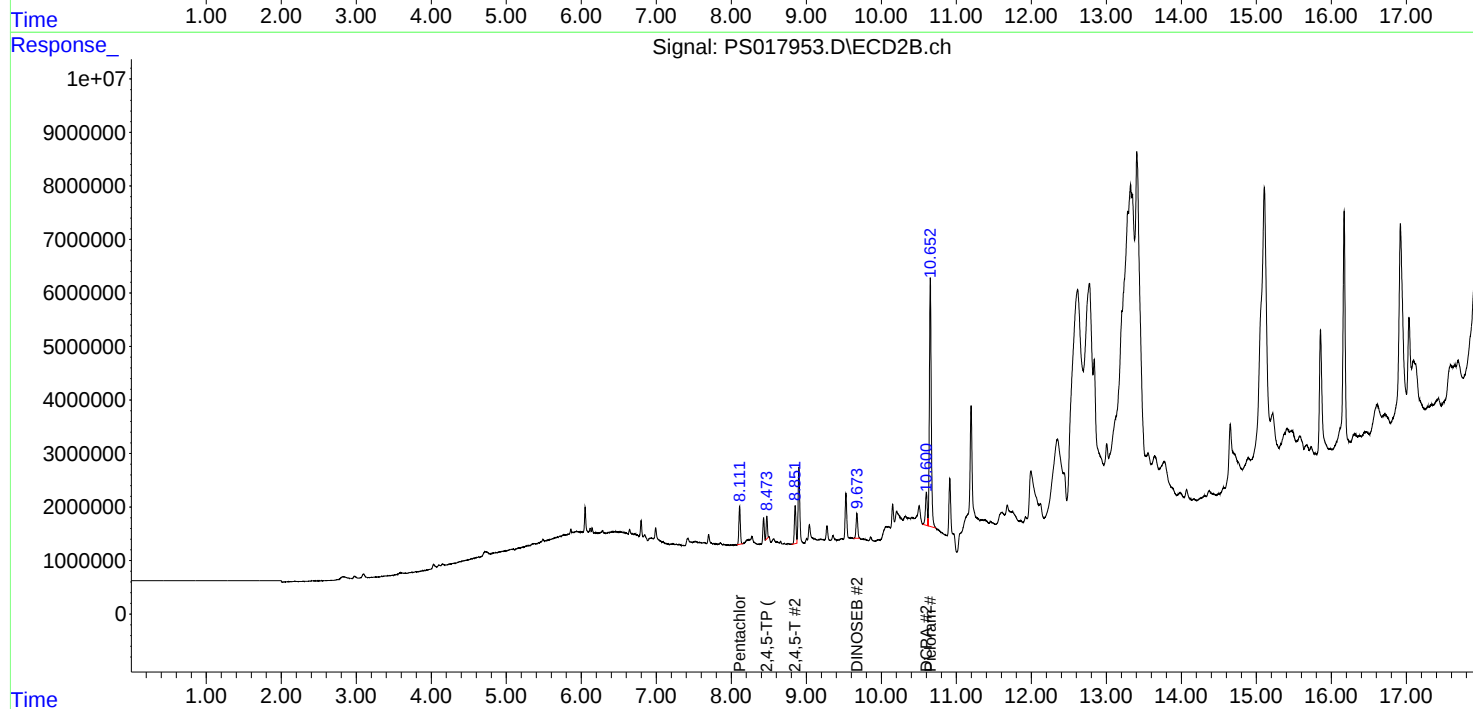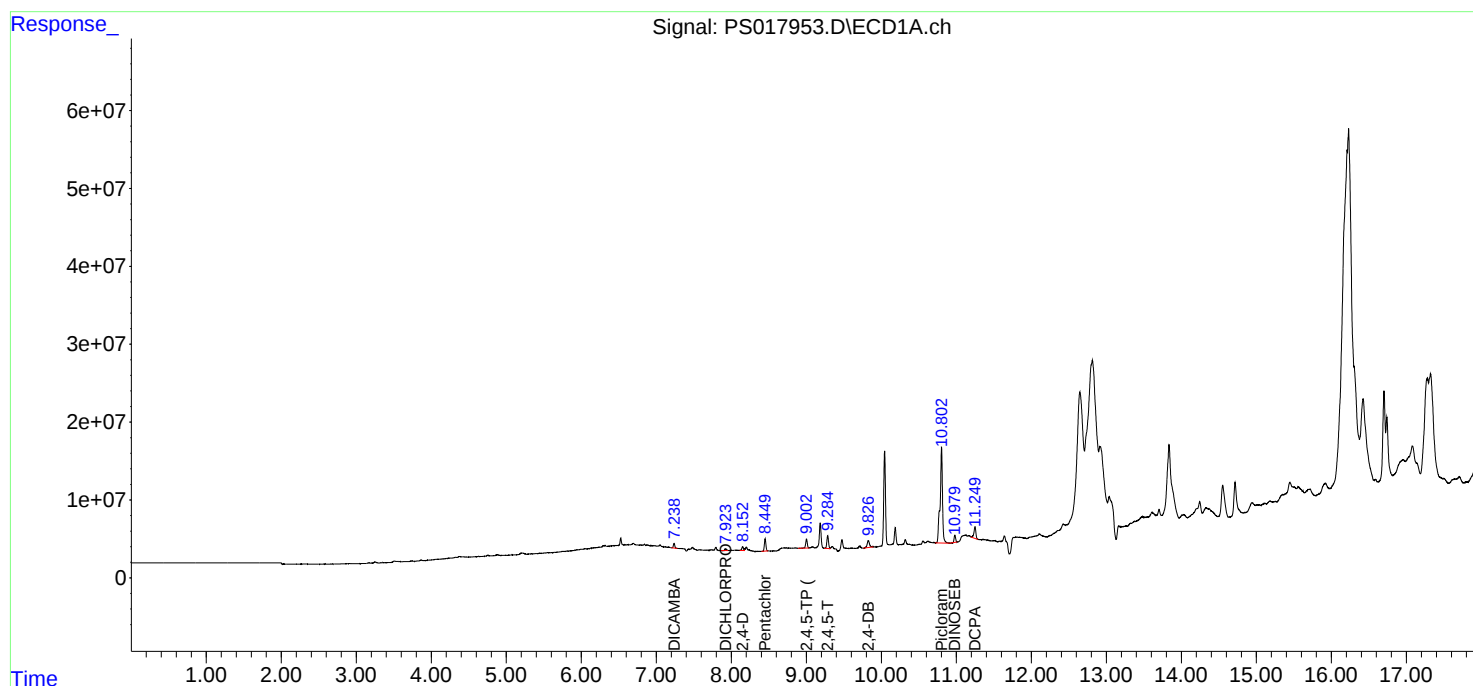


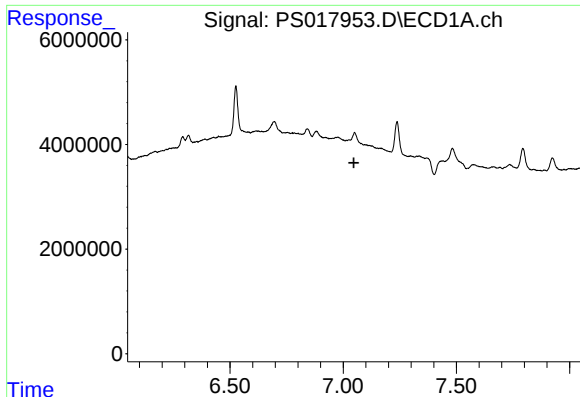

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T.: 7.047 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

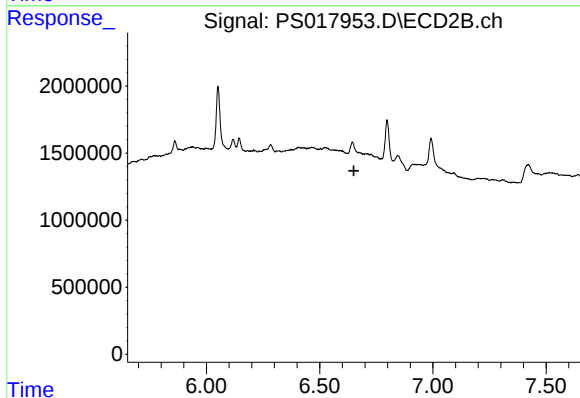


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T.: 6.651 min
Response: 0
Conc: N.D.

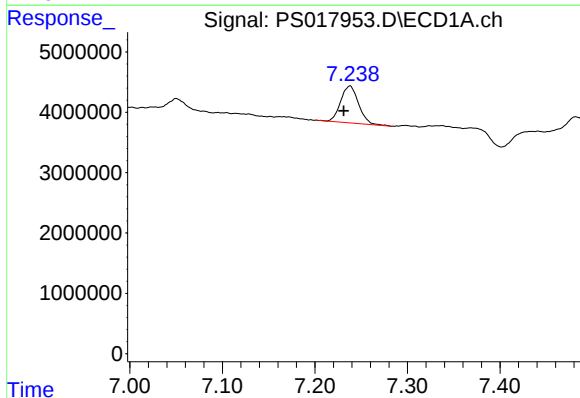


#5 DICAMBA

R.T.: 7.238 min
Delta R.T.: 0.007 min
Response: 8297745
Conc: 1.33 ng/ml

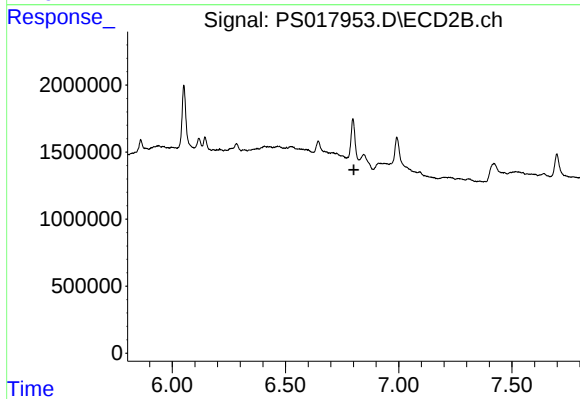

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 6.802 min
Response: 0
Conc: N.D.

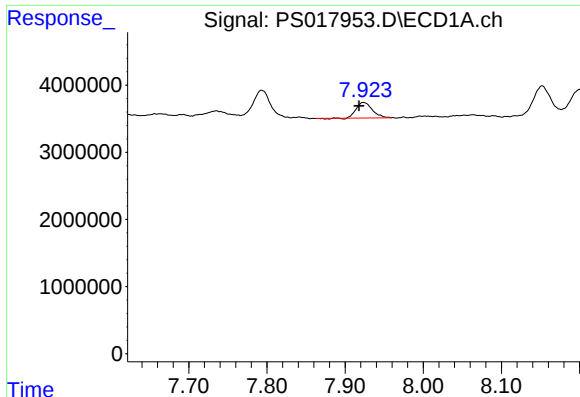

#8 DICHLORPROP


R.T.: 7.923 min
Delta R.T.: 0.005 min
Response: 3312065
Conc: 2.11 ng/ml

Instrument :
ECD_S
ClientSampleId :

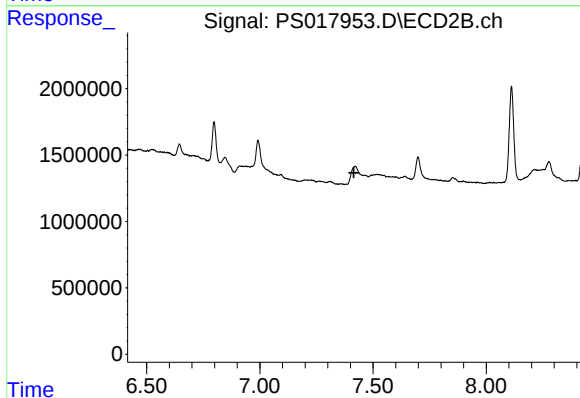


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 7.415 min
Response: 0
Conc: N.D.

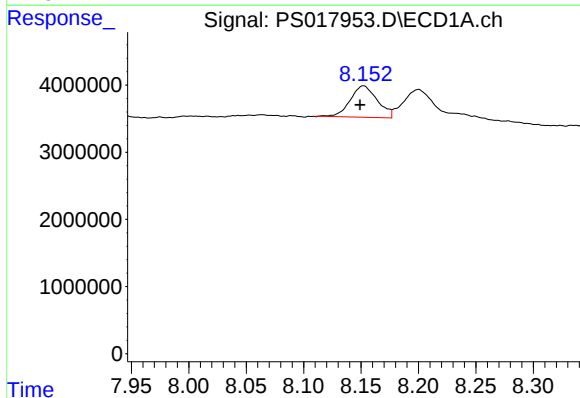


#9 2,4-D

R.T.: 8.152 min
Delta R.T.: 0.003 min
Response: 7688796
Conc: 4.22 ng/ml

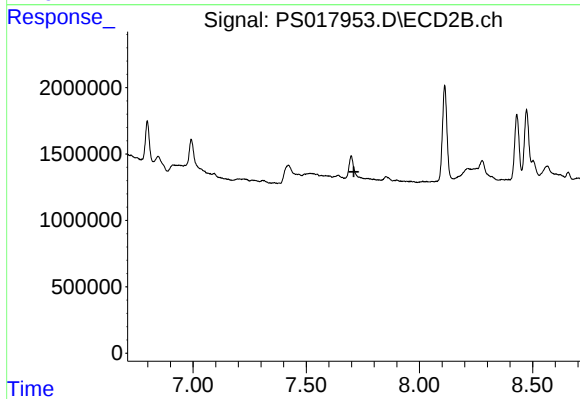

#9 2,4-D


R.T.: 0.000 min
Exp R.T. : 7.710 min
Response: 0
Conc: N.D.

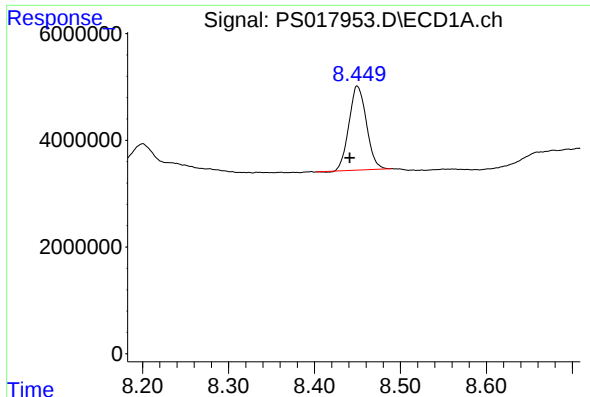

#10 Pentachlorophenol


R.T.: 8.450 min
Delta R.T.: 0.009 min
Response: 22179434
Conc: 1.05 ng/ml

Instrument :
ECD_S
ClientSampleId :

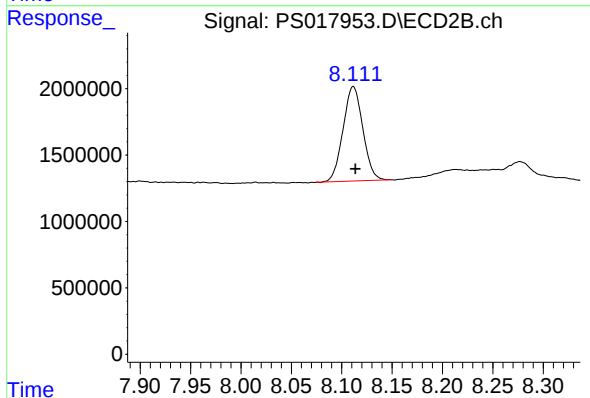


#10 Pentachlorophenol

R.T.: 8.112 min
Delta R.T.: -0.002 min
Response: 9712643
Conc: 1.15 ng/ml

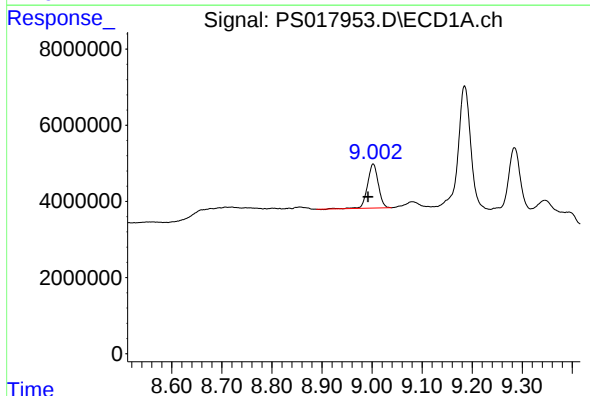


#11 2,4,5-TP (SILVEX)

R.T.: 9.002 min
Delta R.T.: 0.010 min
Response: 17387748
Conc: 2.05 ng/ml

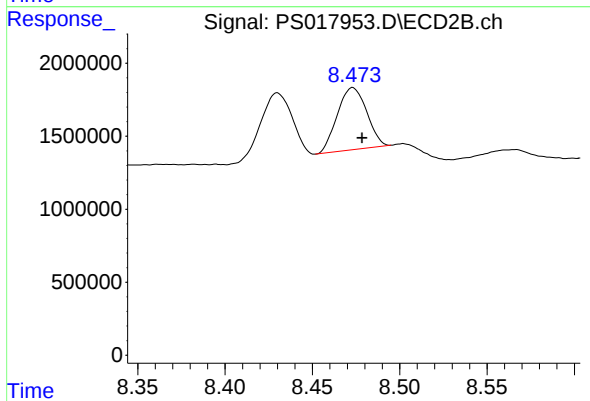

#11 2,4,5-TP (SILVEX)


R.T.: 8.473 min
Delta R.T.: -0.005 min
Response: 4978777
Conc: 1.40 ng/ml

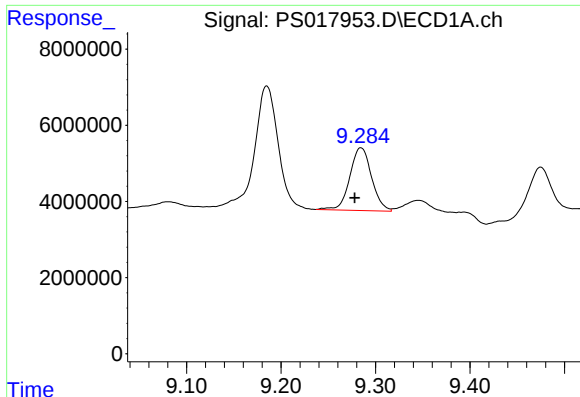

#12 2,4,5-T


R.T.: 9.284 min
Delta R.T.: 0.007 min
Response: 26388116
Conc: 2.98 ng/ml

Instrument :
ECD_S
ClientSampleId :

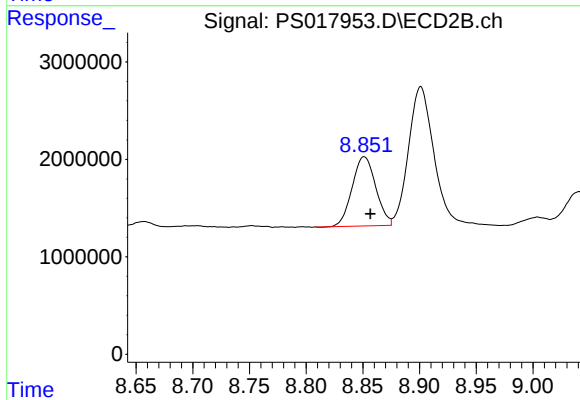


#12 2,4,5-T

R.T.: 8.851 min
Delta R.T.: -0.005 min
Response: 10317643
Conc: 3.15 ng/ml

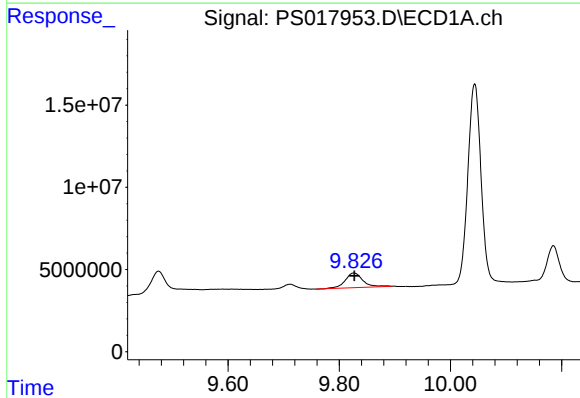


#13 2,4-DB

R.T.: 9.826 min
Delta R.T.: -0.001 min
Response: 19758452
Conc: 11.95 ng/ml

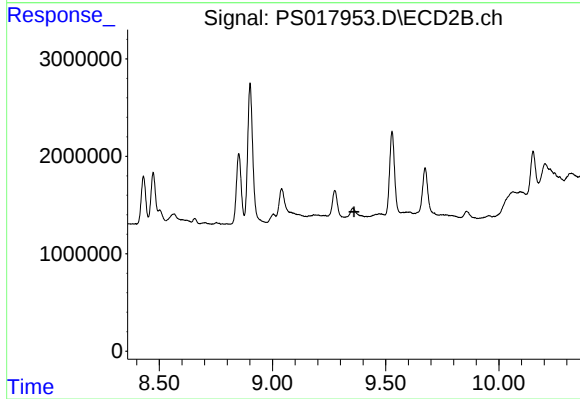

#13 2,4-DB


R.T.: 0.000 min
Exp R.T. : 9.360 min
Response: 0
Conc: N.D.

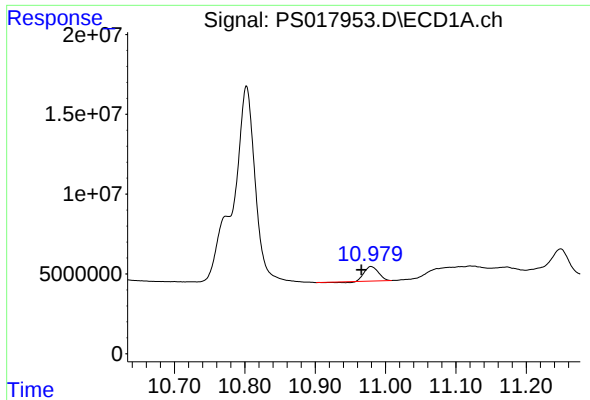

#14 DINOSEB


R.T.: 10.979 min
Delta R.T.: 0.014 min
Response: 12128636
Conc: 1.85 ng/ml

Instrument :
ECD_S
ClientSampleId :

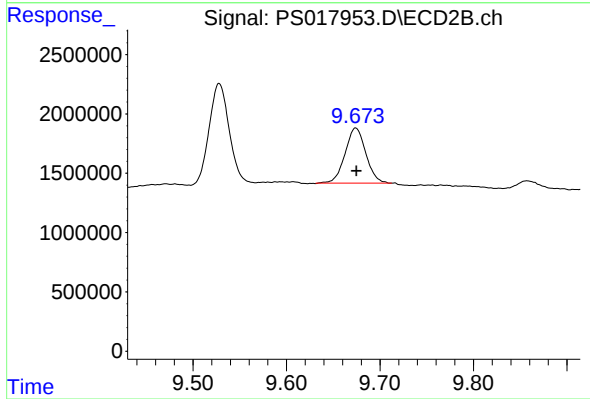


#14 DINOSEB

R.T.: 9.674 min
Delta R.T.: 0.000 min
Response: 7163814
Conc: 2.87 ng/ml

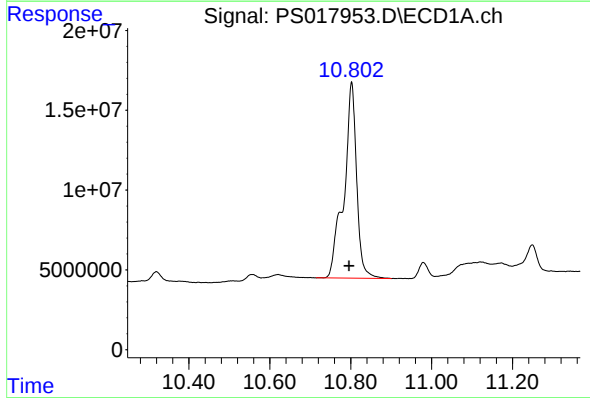


#15 Picloram

R.T.: 10.802 min
Delta R.T.: 0.006 min
Response: 269810539
Conc: 22.60 ng/ml

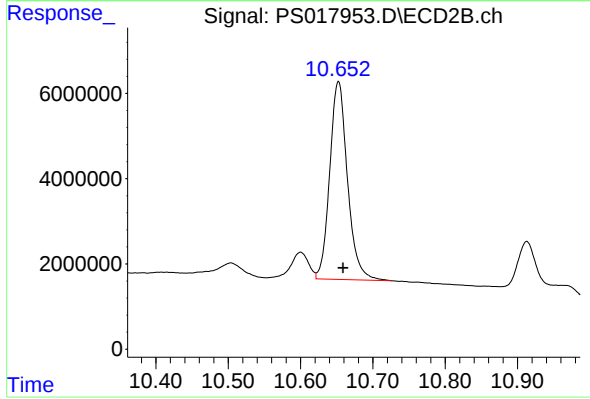

#15 Picloram


R.T.: 10.653 min
Delta R.T.: -0.006 min
Response: 79291350
Conc: 16.96 ng/ml

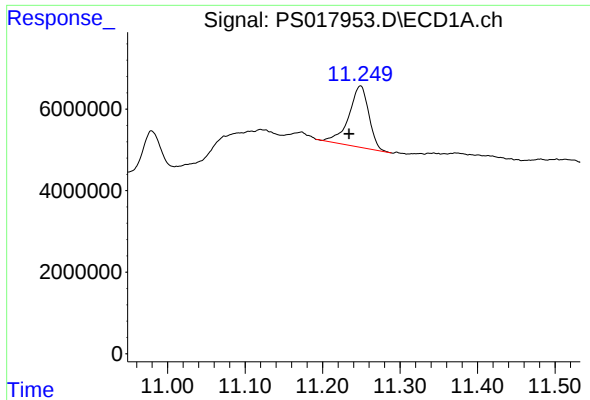

#16 DCPA

R.T.: 11.249 min
Delta R.T.: 0.015 min
Response: 26693550
Conc: 2.47 ng/ml

Instrument :
ECD_S
ClientSampleId :

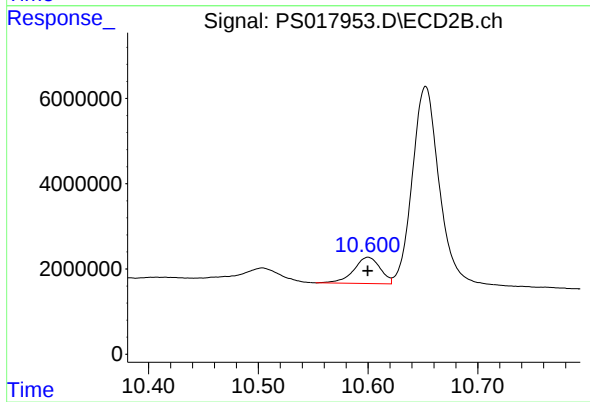

#16 DCPA

R.T.: 10.600 min
Delta R.T.: 0.000 min
Response: 10373658
Conc: 2.35 ng/ml