

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS011122\
 Data File : PS017963.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Jan 2022 16:05
 Operator : AJ\MA
 Sample : I.BLK
 Misc : LOT#M03961
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 11 18:02:35 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010522.M
 Quant Title : 8080.M
 QLast Update : Thu Jan 06 10:21:08 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.048	6.643	696.8E6	293.7E6	482.079	506.155
Target Compounds							
7) T	MCPA	7.489f	0.000	4254733	0	<MDL	N.D. #
9) T	2,4-D	8.208f	0.000	4627809	0	2.541	N.D. #
10) T	Pentachlo...	8.450	0.000	3564461	0	<MDL	N.D. #
11) T	2,4,5-TP ...	9.059f	8.431f	18148310	7817160	2.145	2.193
12) T	2,4,5-T	9.341f	0.000	27988485	0	3.157	N.D. #
14) T	DINOSEB	10.929	0.000	15444897	0	2.352	N.D. #
15) T	Picloram	10.801	10.665	11898913	21741868	<MDL	4.650 #
16) T	DCPA	11.231	10.665f	12469433	21741868	1.154	4.924 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS011122\
Data File : PS017963.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Jan 2022 16:05
Operator : AJ\MA
Sample : I.BLK
Misc : LOT#M03961
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 11 18:02:35 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010522.M
Quant Title : 8080.M
QLast Update : Thu Jan 06 10:21:08 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

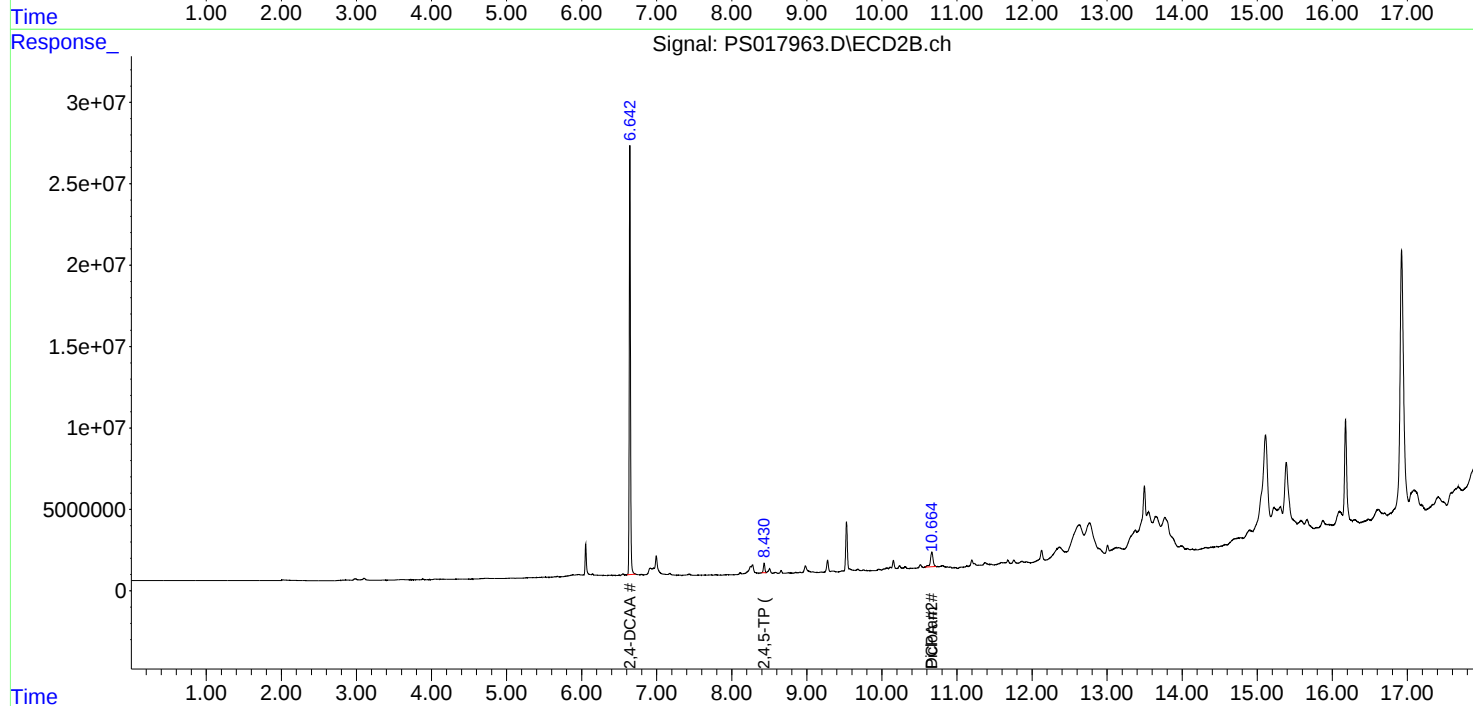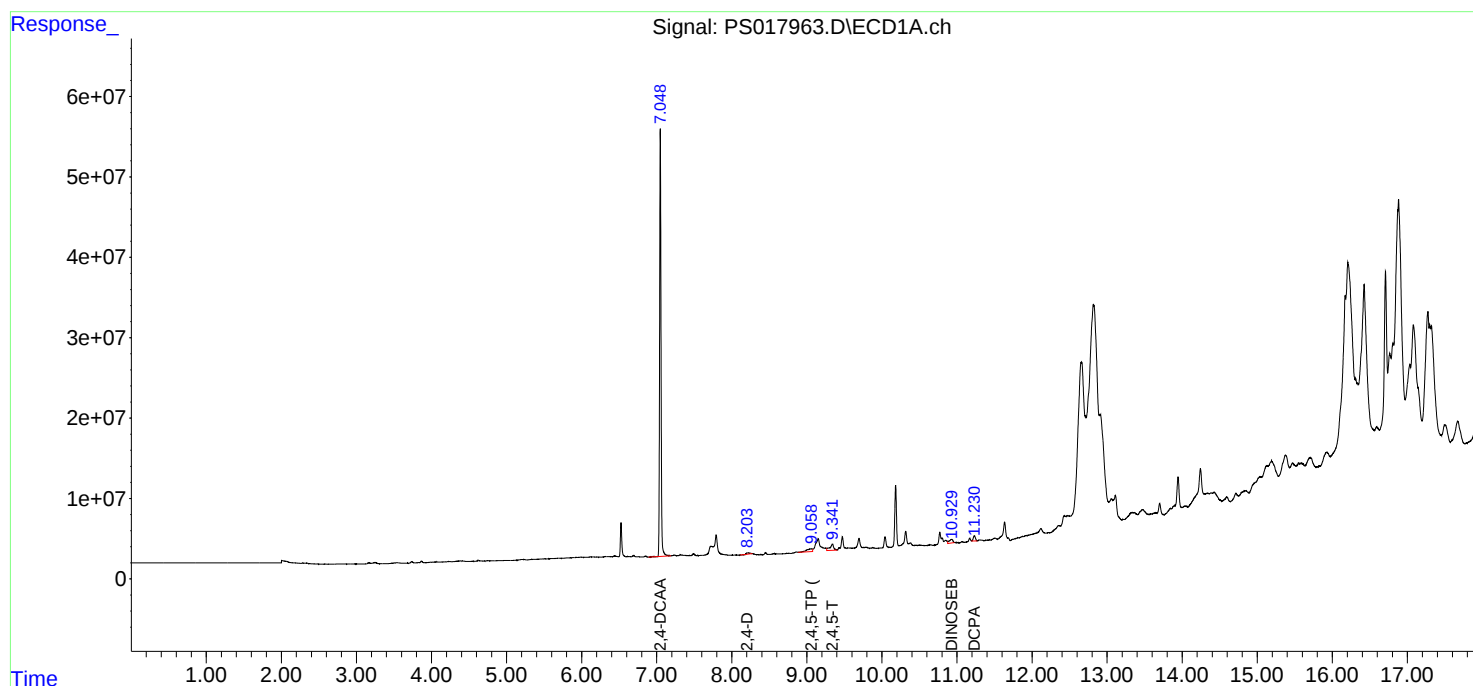


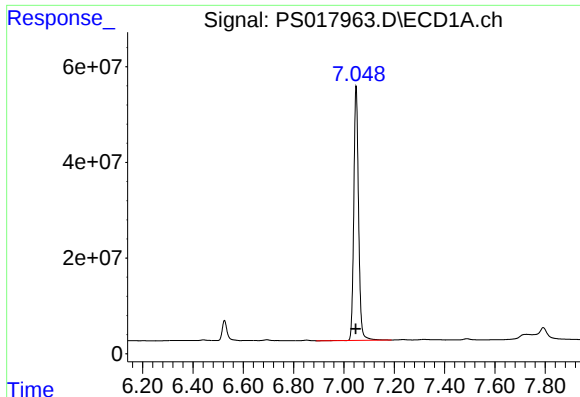

#4 2,4-DCAA


R.T.: 7.048 min
Delta R.T.: 0.000 min
Response: 696839277
Conc: 482.08 ng/ml

Instrument :
ECD_S
ClientSampleId :

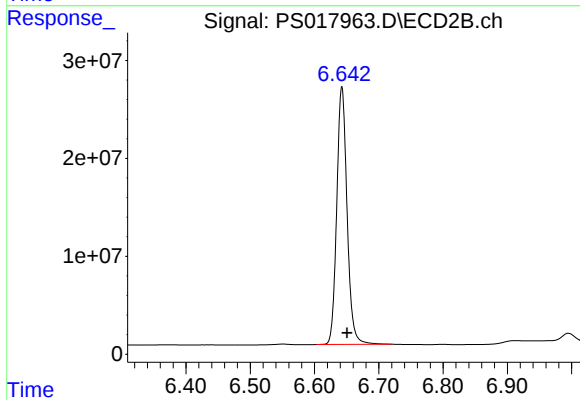


#4 2,4-DCAA

R.T.: 6.643 min
Delta R.T.: -0.008 min
Response: 293696037
Conc: 506.16 ng/ml

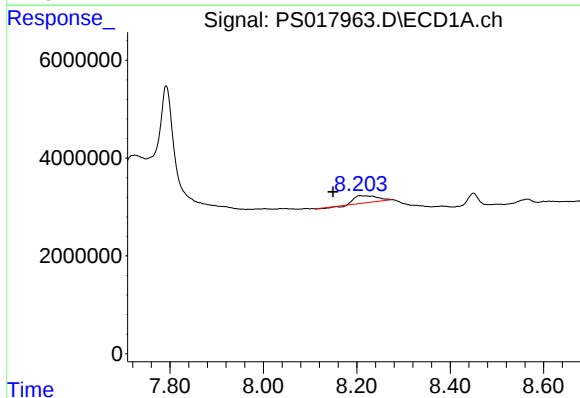


#9 2,4-D

R.T.: 8.208 min
Delta R.T.: 0.059 min
Response: 4627809
Conc: 2.54 ng/ml

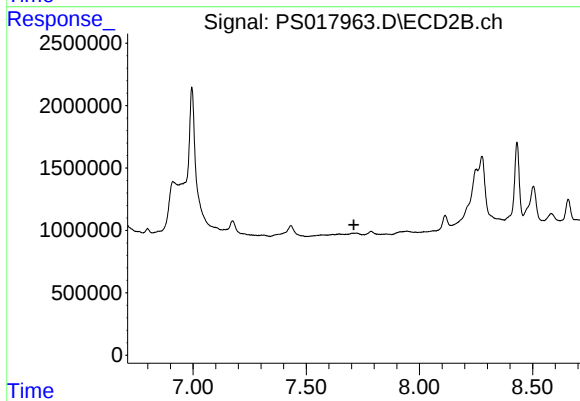

#9 2,4-D


R.T.: 0.000 min
Exp R.T. : 7.710 min
Response: 0
Conc: N.D.

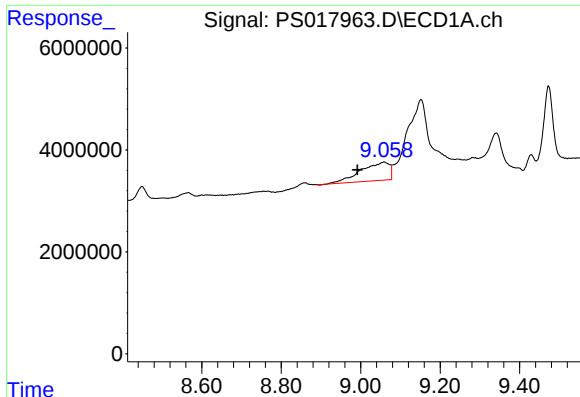

#11 2,4,5-TP (SILVEX)


R.T.: 9.059 min
Delta R.T.: 0.067 min
Response: 18148310
Conc: 2.14 ng/ml

Instrument :
ECD_S
ClientSampleId :

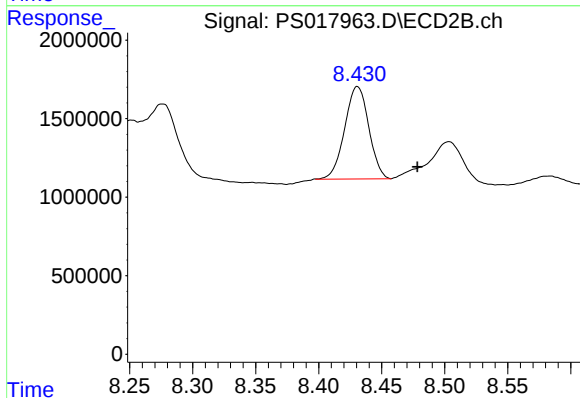


#11 2,4,5-TP (SILVEX)

R.T.: 8.431 min
Delta R.T.: -0.048 min
Response: 7817160
Conc: 2.19 ng/ml

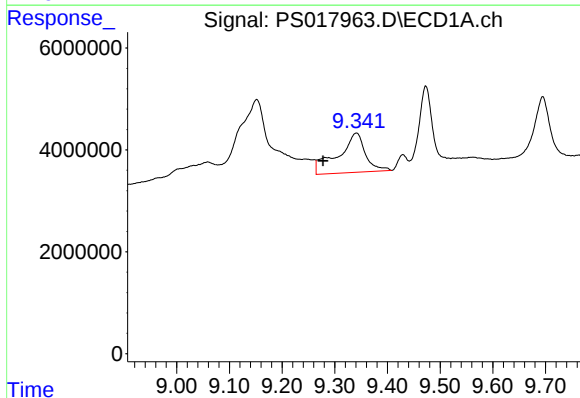


#12 2,4,5-T

R.T.: 9.341 min
Delta R.T.: 0.063 min
Response: 27988485
Conc: 3.16 ng/ml

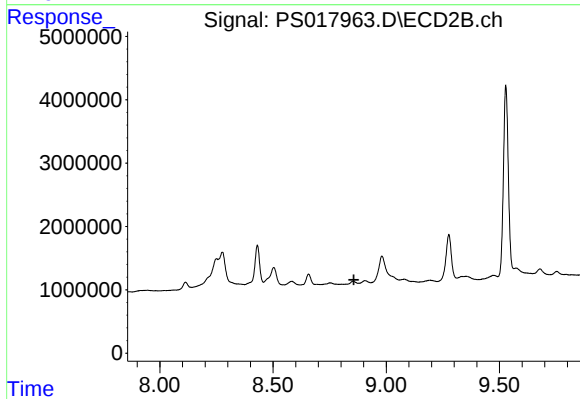

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T. : 8.857 min
Response: 0
Conc: N.D.

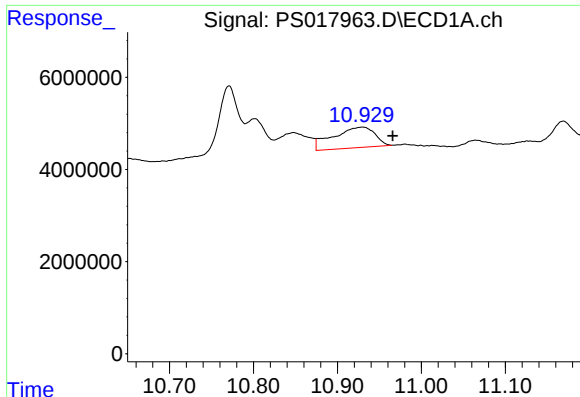

#14 DINOSEB


R.T.: 10.929 min
Delta R.T.: -0.036 min
Response: 15444897
Conc: 2.35 ng/ml

Instrument :
ECD_S
ClientSampleId :

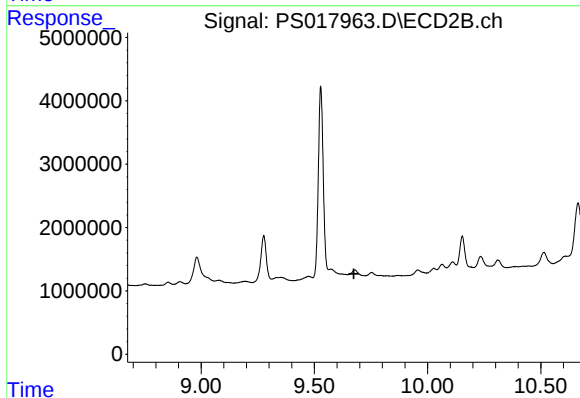


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 9.675 min
Response: 0
Conc: N.D.

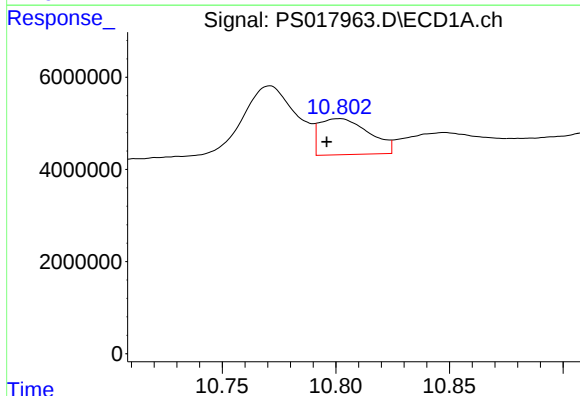


#15 Picloram

R.T.: 10.801 min
Delta R.T.: 0.005 min
Response: 11898913
Conc: N.D.

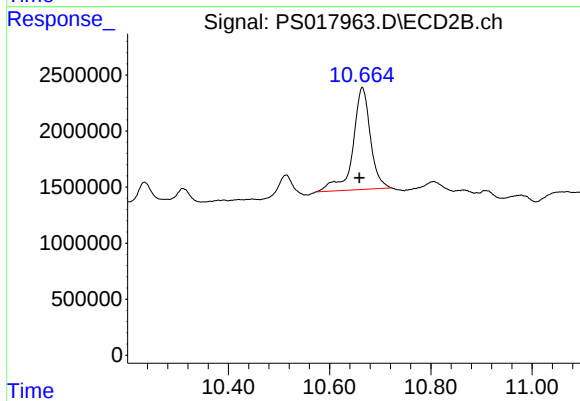

#15 Picloram


R.T.: 10.665 min
Delta R.T.: 0.006 min
Response: 21741868
Conc: 4.65 ng/ml

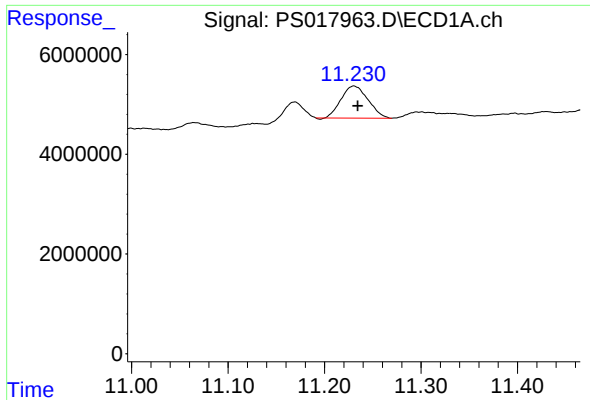

#16 DCPA

R.T.: 11.231 min
Delta R.T.: -0.004 min
Response: 12469433
Conc: 1.15 ng/ml

Instrument :
ECD_S
ClientSampleId :

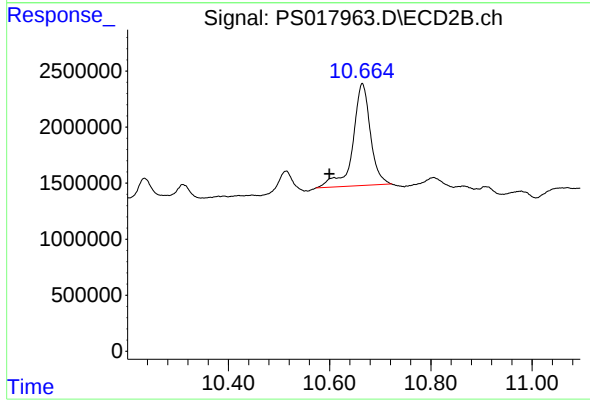

#16 DCPA

R.T.: 10.665 min
Delta R.T.: 0.065 min
Response: 21741868
Conc: 4.92 ng/ml