

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS011221\
 Data File : PS013739.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Jan 2021 09:31
 Operator : DD\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 12 10:36:12 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010421.M
 Quant Title : 8080.M
 QLast Update : Tue Jan 05 01:51:07 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds

2) T	3,5-DICHL...	6.469f	0.000	102.8E6	0	77.714	N.D.	#
5) T	DICAMBA	0.000	7.145f	0	52861928	N.D.	30.781	
6) T	MCCP	0.000	7.145	0	52861928	N.D.	37.407	
15) T	Picloram	10.982	11.064f	25754717	15892800	3.566	4.573	#



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS011221\
Data File : PS013739.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Jan 2021 09:31
Operator : DD\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 12 10:36:12 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010421.M
Quant Title : 8080.M
QLast Update : Tue Jan 05 01:51:07 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

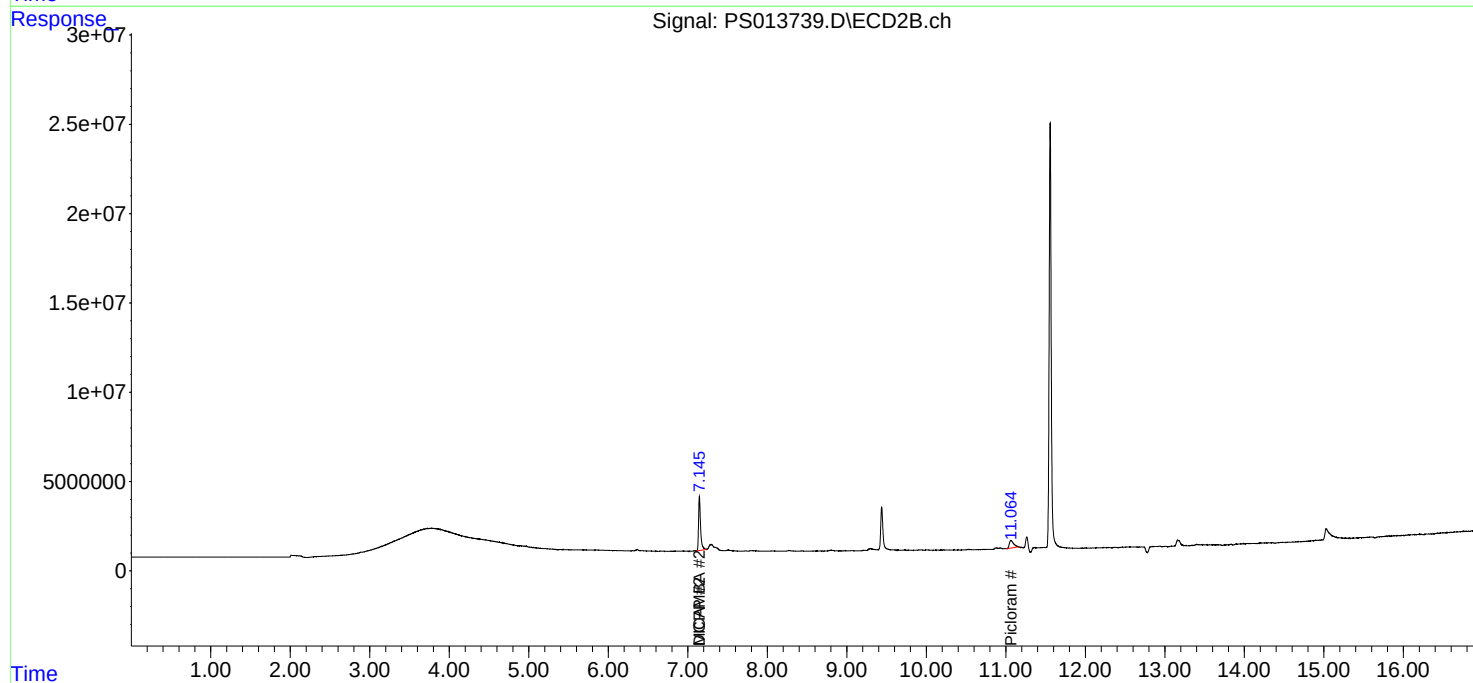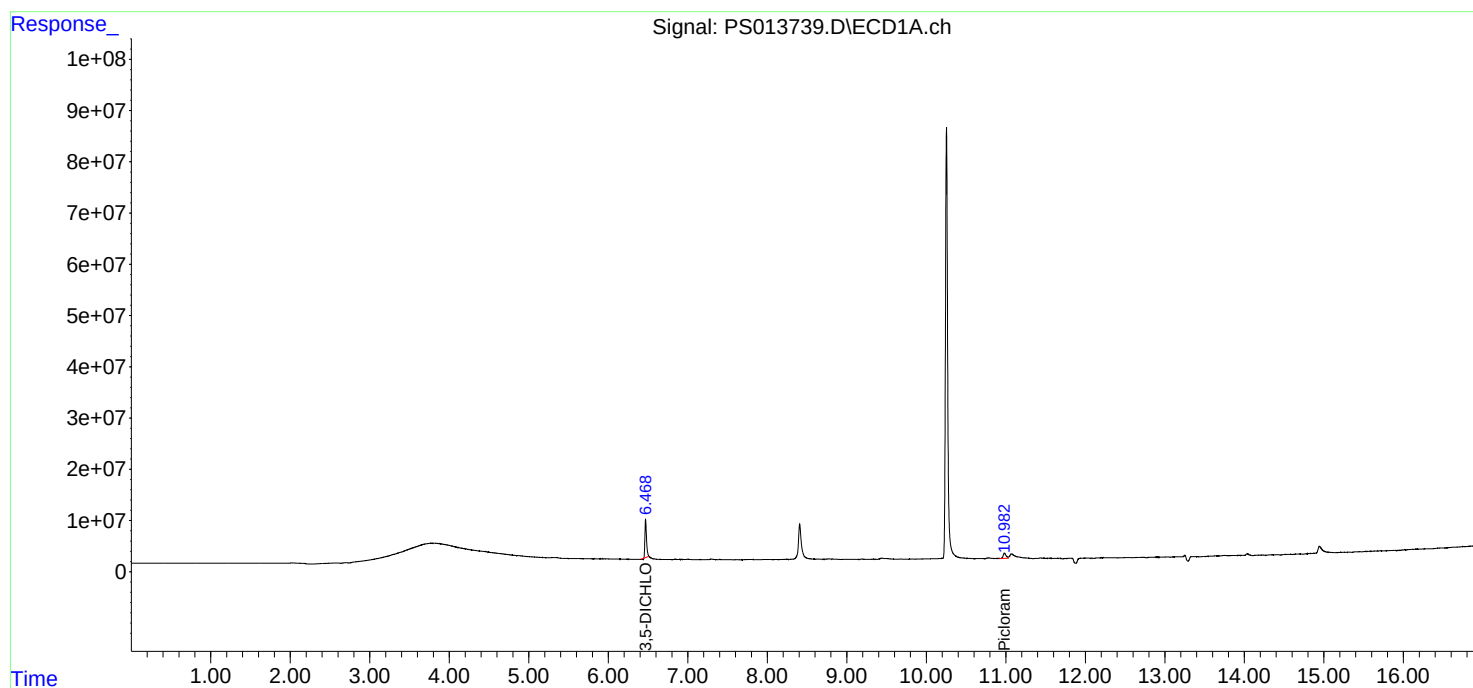


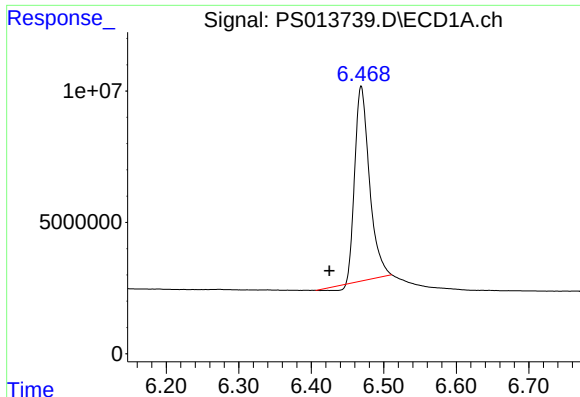

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.469 min
Delta R.T.: 0.044 min
Response: 102770716
Conc: 77.71 ng/ml

Instrument :
ECD_S
ClientSampleId :
HEXANE

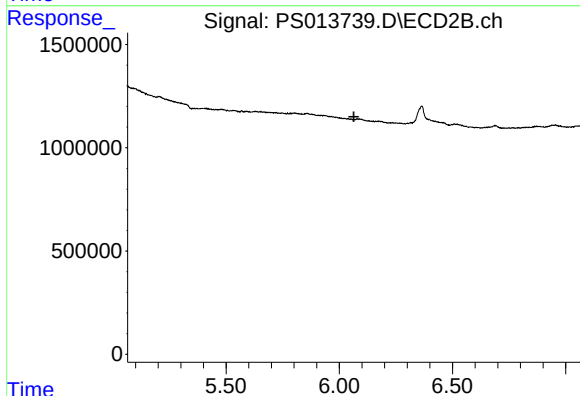


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.064 min
Response: 0
Conc: N.D.

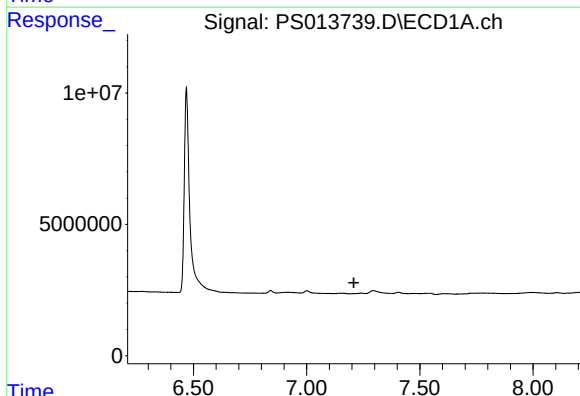


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 7.208 min
Response: 0
Conc: N.D.

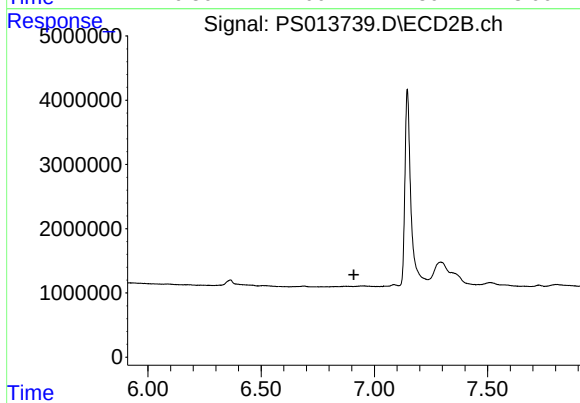

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T. : 6.909 min
Response: 0
Conc: N.D.

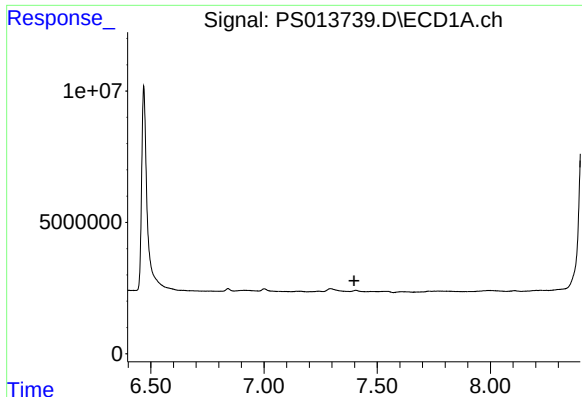

#5 DICAMBA


R.T.: 0.000 min
Exp R.T. : 7.397 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

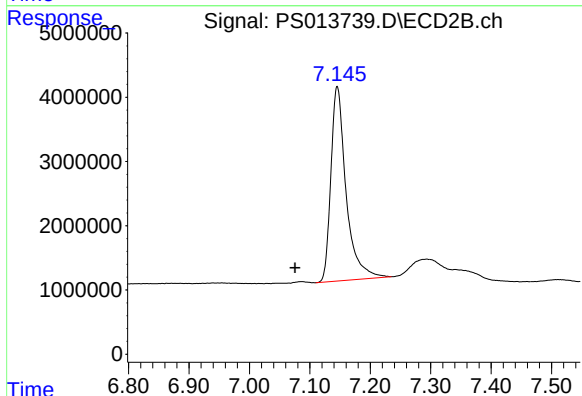


#5 DICAMBA

R.T.: 7.145 min
Delta R.T.: 0.070 min
Response: 52861928
Conc: 30.78 ng/ml

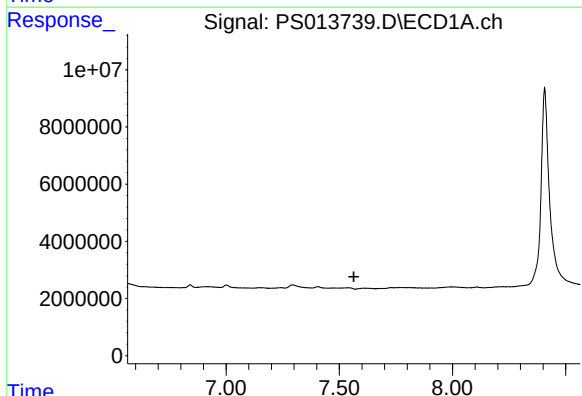


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 7.564 min
Response: 0
Conc: N.D.

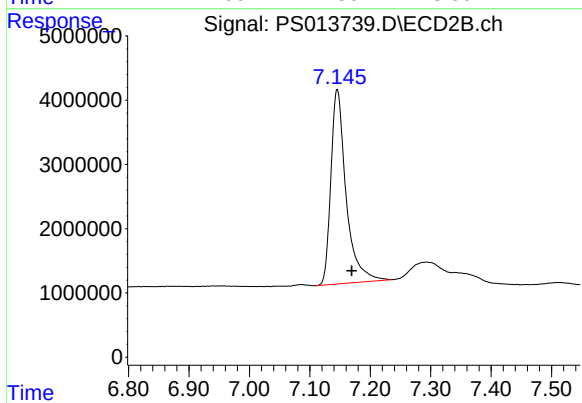

#6 MCPP


R.T.: 7.145 min
Delta R.T.: -0.024 min
Response: 52861928
Conc: 37.41 ug/ml

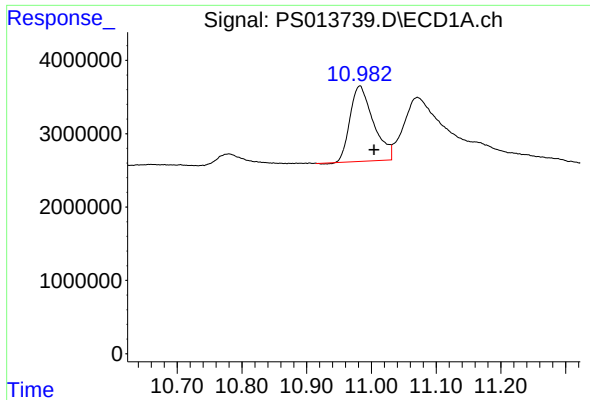

#15 Picloram

R.T.: 10.982 min
Delta R.T.: -0.022 min
Response: 25754717
Conc: 3.57 ng/ml

Instrument :
ECD_S
ClientSampleId :
HEXANE

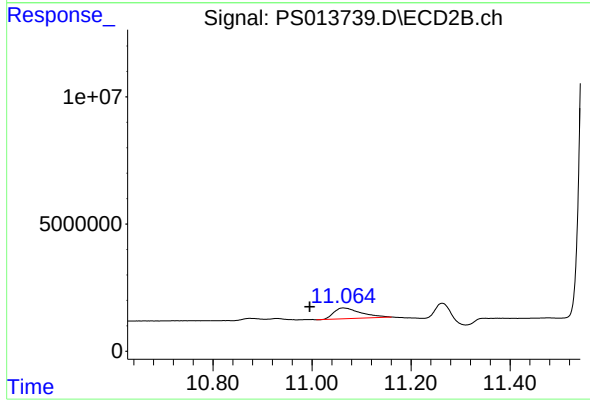

#15 Picloram

R.T.: 11.064 min
Delta R.T.: 0.068 min
Response: 15892800
Conc: 4.57 ng/ml