

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS011222\
 Data File : PS017965.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Jan 2022 08:18
 Operator : AJ\MA
 Sample : HEXANE
 Misc : LOT#M03961
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 13 00:02:03 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010522.M
 Quant Title : 8080.M
 QLast Update : Thu Jan 06 10:21:08 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds							
2) T	3,5-DICHL...	6.292	0.000	3044111	0	1.415	N.D. #
5) T	DICAMBA	7.239	0.000	7981909	0	1.278	N.D. #
7) T	MCPA	7.486f	0.000	6879811	0	1.031	N.D. #
8) T	DICHLORPROP	7.926	0.000	3511987	0	2.233	N.D. #
9) T	2,4-D	8.154	0.000	20260792	0	11.127	N.D. #
10) T	Pentachlo...	8.453	8.113	24716991	11344977	1.170	1.347
11) T	2,4,5-TP ...	9.005	8.475	31313109	2645643	3.700	<MDL #
12) T	2,4,5-T	9.288	8.852	34339698	10450645	3.874	3.195
13) T	2,4-DB	9.826	0.000	27913680	0	16.886	N.D. #
14) T	DINOSEB	10.948	0.000	8697734	0	1.324	N.D. #
15) T	Picloram	10.806	10.653	578.5E6	207.7E6	48.471	44.419
16) T	DCPA	11.253	10.601	21759360	15479821	2.014	3.506 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS011222\
Data File : PS017965.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Jan 2022 08:18
Operator : AJ\MA
Sample : HEXANE
Misc : LOT#M03961
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 13 00:02:03 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010522.M
Quant Title : 8080.M
QLast Update : Thu Jan 06 10:21:08 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

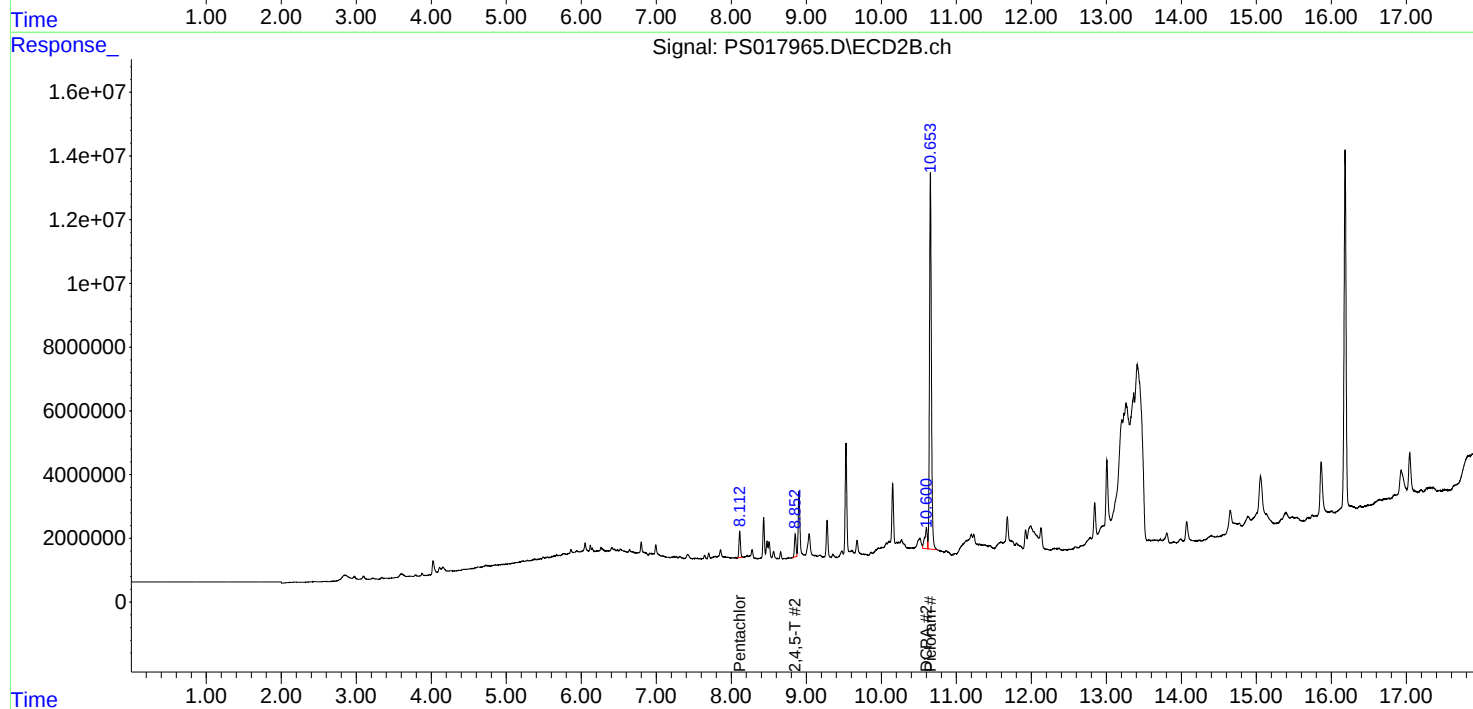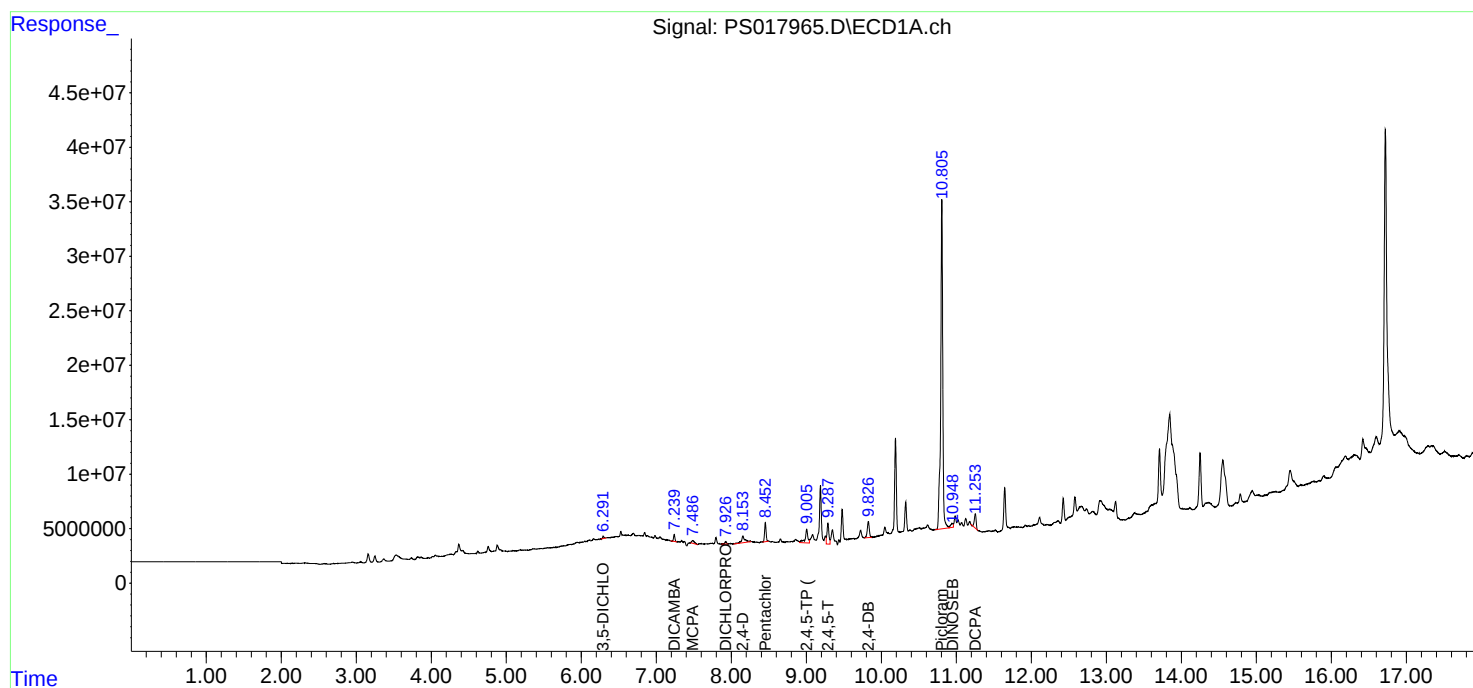


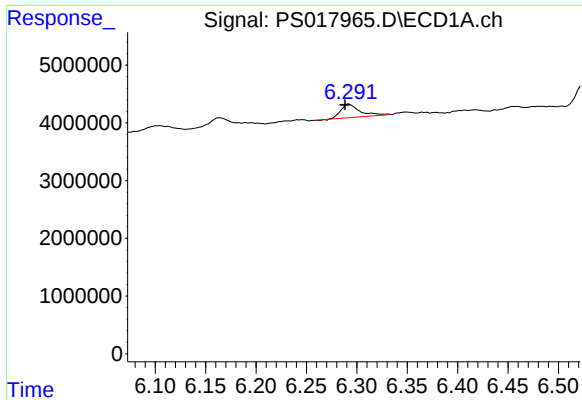

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.292 min
Delta R.T.: 0.004 min
Response: 3044111
Conc: 1.42 ng/ml

Instrument :
ECD_S
ClientSampleId :

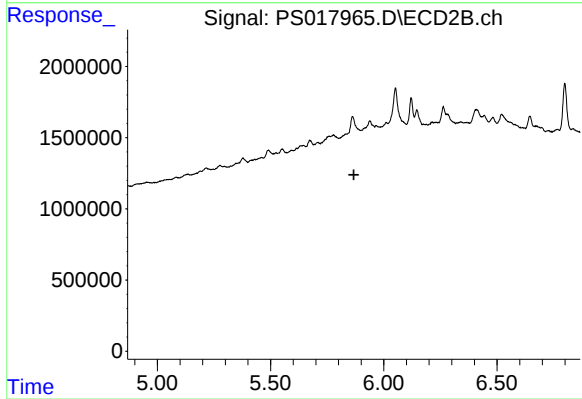


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 5.868 min
Response: 0
Conc: N.D.

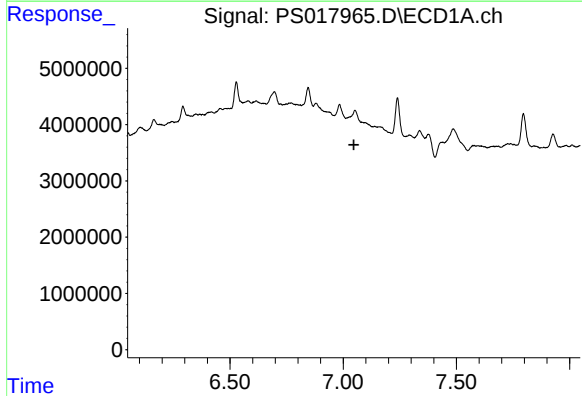


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 7.047 min
Response: 0
Conc: N.D.

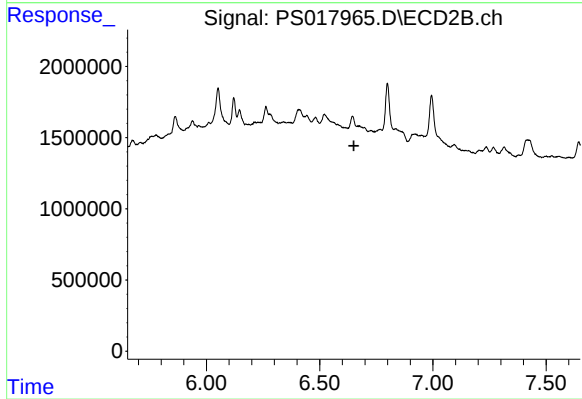

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T. : 6.651 min
Response: 0
Conc: N.D.

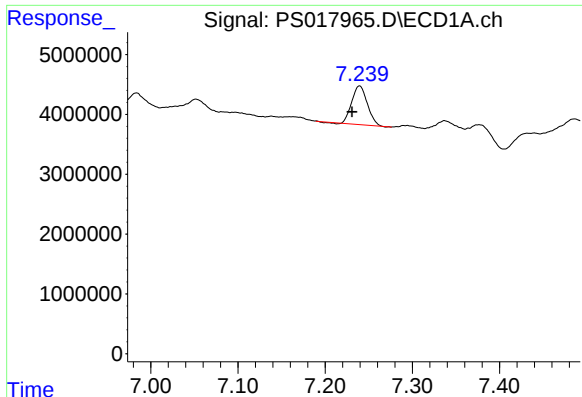

#5 DICAMBA


R.T.: 7.239 min
Delta R.T.: 0.008 min
Response: 7981909
Conc: 1.28 ng/ml

Instrument :
ECD_S
ClientSampleId :

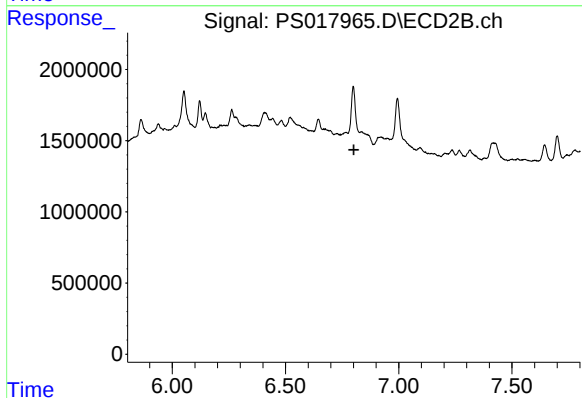


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 6.802 min
Response: 0
Conc: N.D.

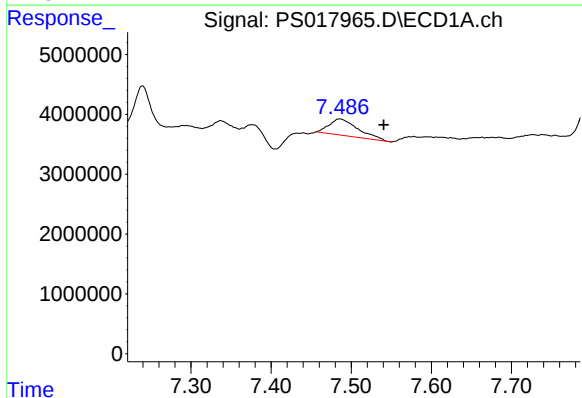


#7 MCPA

R.T.: 7.486 min
Delta R.T.: -0.055 min
Response: 6879811
Conc: 1.03 ug/ml

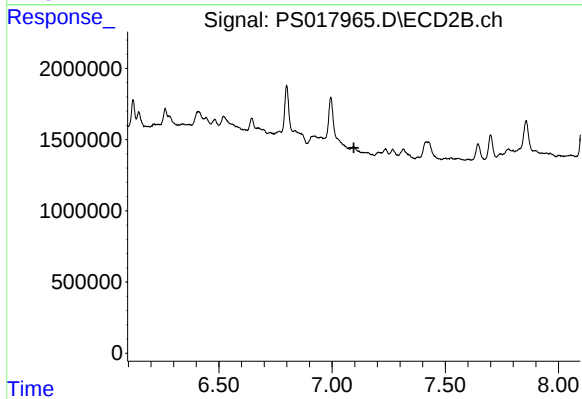

#7 MCPA


R.T.: 0.000 min
Exp R.T. : 7.096 min
Response: 0
Conc: N.D.

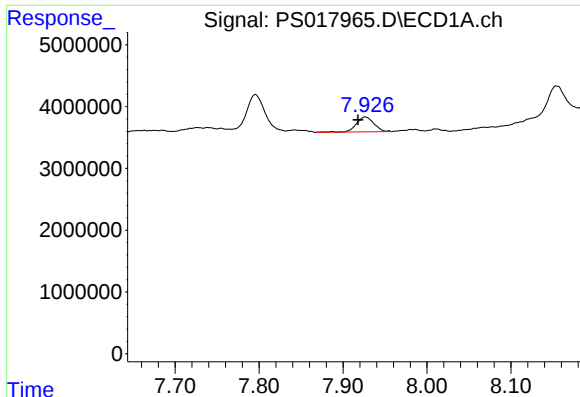

#8 DICHLORPROP


R.T.: 7.926 min
Delta R.T.: 0.009 min
Response: 3511987
Conc: 2.23 ng/ml

Instrument :
ECD_S
ClientSampleId :

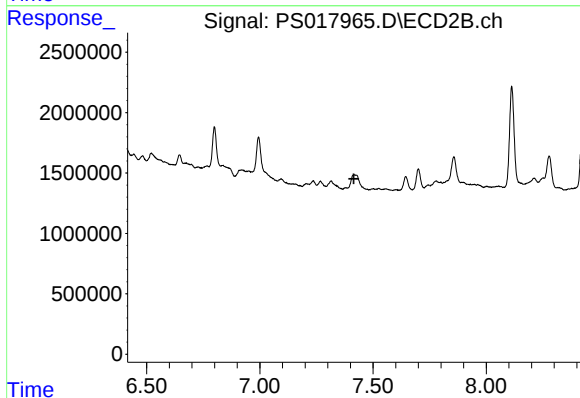


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 7.415 min
Response: 0
Conc: N.D.

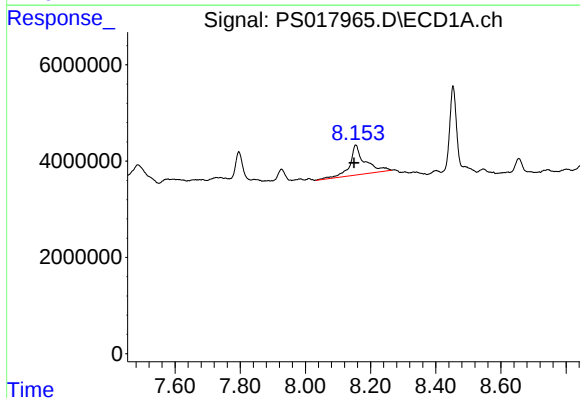


#9 2,4-D

R.T.: 8.154 min
Delta R.T.: 0.005 min
Response: 20260792
Conc: 11.13 ng/ml

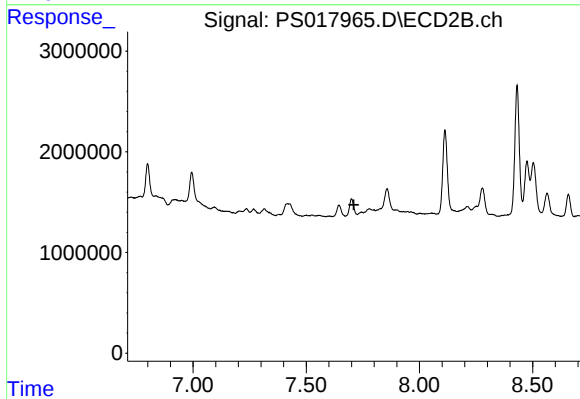

#9 2,4-D


R.T.: 0.000 min
Exp R.T. : 7.710 min
Response: 0
Conc: N.D.

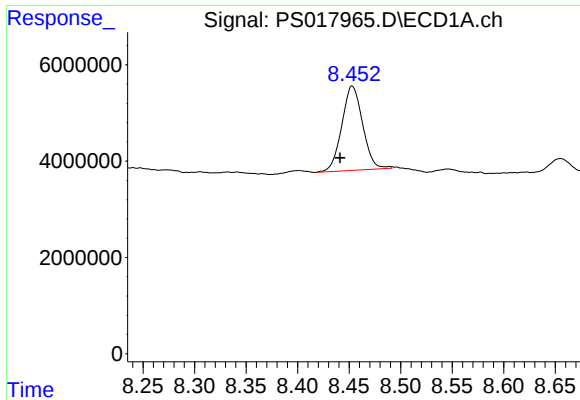

#10 Pentachlorophenol


R.T.: 8.453 min
Delta R.T.: 0.012 min
Response: 24716991
Conc: 1.17 ng/ml

Instrument :
ECD_S
ClientSampleId :

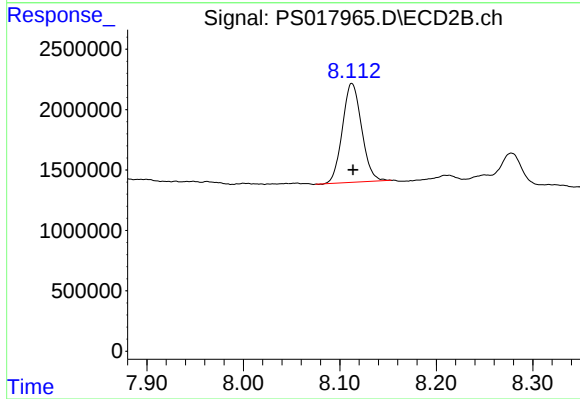


#10 Pentachlorophenol

R.T.: 8.113 min
Delta R.T.: -0.001 min
Response: 11344977
Conc: 1.35 ng/ml

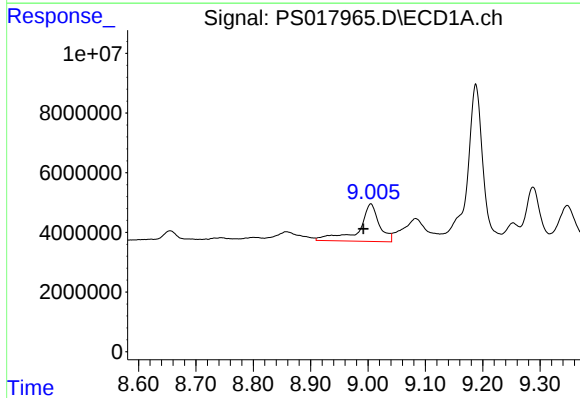


#11 2,4,5-TP (SILVEX)

R.T.: 9.005 min
Delta R.T.: 0.013 min
Response: 31313109
Conc: 3.70 ng/ml

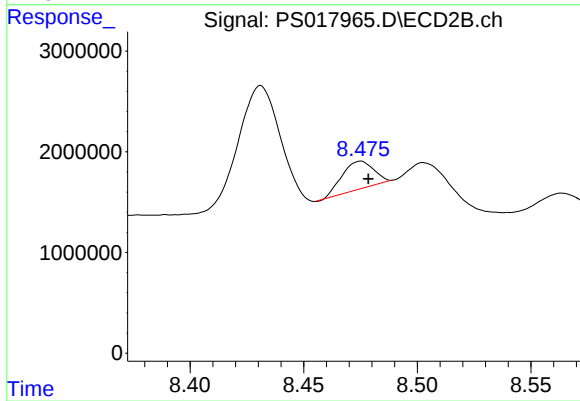

#11 2,4,5-TP (SILVEX)


R.T.: 8.475 min
Delta R.T.: -0.003 min
Response: 2645643
Conc: N.D.

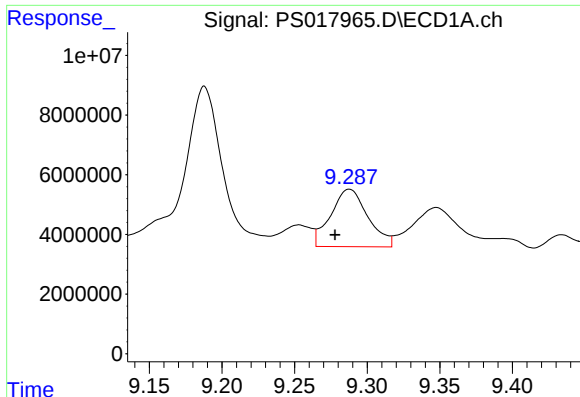

#12 2,4,5-T


R.T.: 9.288 min
Delta R.T.: 0.010 min
Response: 34339698
Conc: 3.87 ng/ml

Instrument :
ECD_S
ClientSampleId :

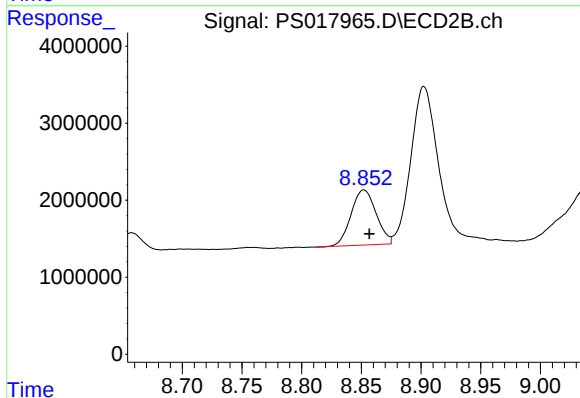


#12 2,4,5-T

R.T.: 8.852 min
Delta R.T.: -0.005 min
Response: 10450645
Conc: 3.19 ng/ml

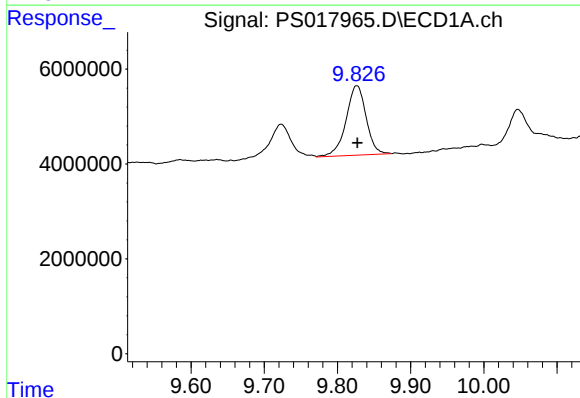


#13 2,4-DB

R.T.: 9.826 min
Delta R.T.: 0.000 min
Response: 27913680
Conc: 16.89 ng/ml

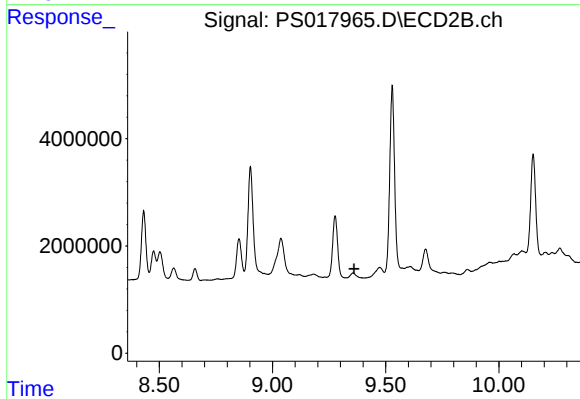

#13 2,4-DB


R.T.: 0.000 min
Exp R.T. : 9.360 min
Response: 0
Conc: N.D.

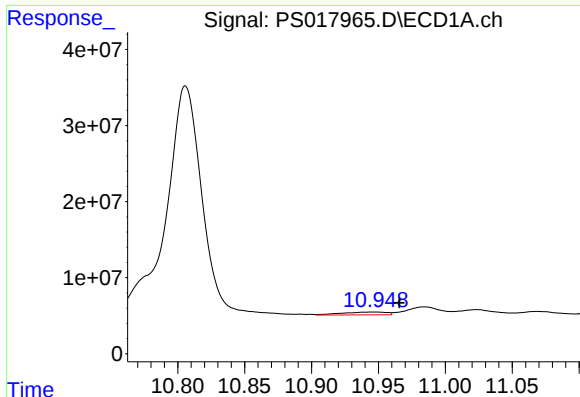

#14 DINOSEB


R.T.: 10.948 min
Delta R.T.: -0.018 min
Response: 8697734
Conc: 1.32 ng/ml

Instrument :
ECD_S
ClientSampleId :

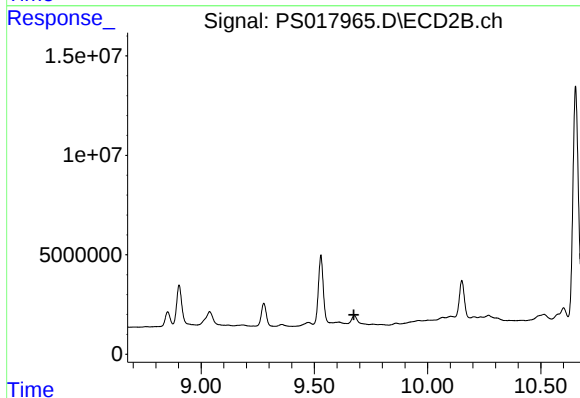


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 9.675 min
Response: 0
Conc: N.D.

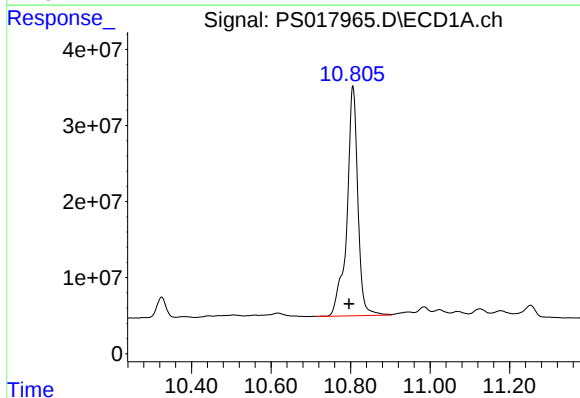


#15 Picloram

R.T.: 10.806 min
Delta R.T.: 0.010 min
Response: 578543887
Conc: 48.47 ng/ml

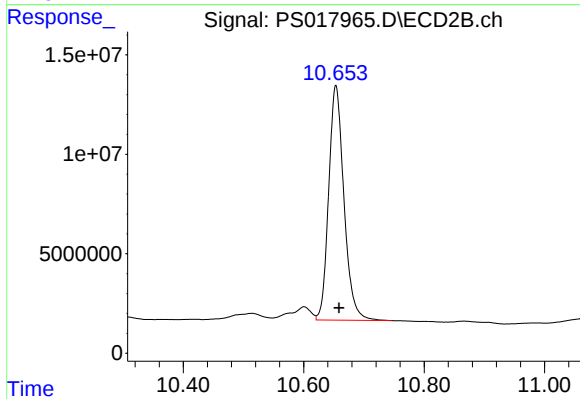

#15 Picloram


R.T.: 10.653 min
Delta R.T.: -0.006 min
Response: 207711839
Conc: 44.42 ng/ml

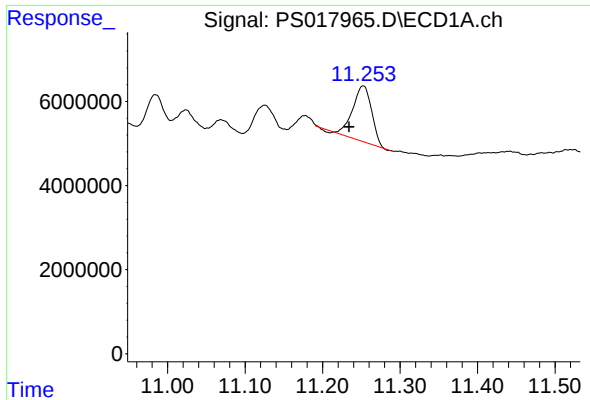

#16 DCPA

R.T.: 11.253 min
Delta R.T.: 0.018 min
Response: 21759360
Conc: 2.01 ng/ml

Instrument :
ECD_S
ClientSampleId :

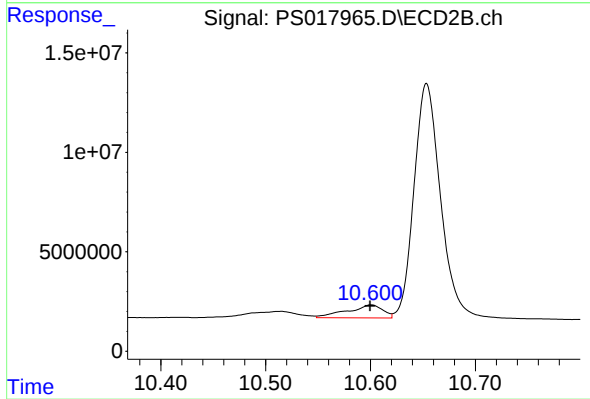

#16 DCPA

R.T.: 10.601 min
Delta R.T.: 0.000 min
Response: 15479821
Conc: 3.51 ng/ml