

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS011222\
 Data File : PS017966.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Jan 2022 08:45
 Operator : AJ\MA
 Sample : I.BLK
 Misc : LOT#M03961
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 13 00:02:34 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010522.M
 Quant Title : 8080.M
 QLast Update : Thu Jan 06 10:21:08 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.050	6.644	651.3E6	289.7E6	450.585	499.353
Target Compounds							
11) T	2,4,5-TP ...	0.000	8.433f	0	5756555	N.D.	1.615
12) T	2,4,5-T	9.285	8.910f	4683958	9252167	<MDL	2.829 #
13) T	2,4-DB	9.824	0.000	7816444	0	4.729	N.D. #
14) T	DINOSEB	10.924f	0.000	9525921	0	1.451	N.D. #
15) T	Picloram	10.802	10.656	369.8E6	131.8E6	30.982	28.191
16) T	DCPA	11.235	10.656f	6401465	131.8E6	<MDL	29.855 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS011222\
Data File : PS017966.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Jan 2022 08:45
Operator : AJ\MA
Sample : I.BLK
Misc : LOT#M03961
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 13 00:02:34 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010522.M
Quant Title : 8080.M
QLast Update : Thu Jan 06 10:21:08 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

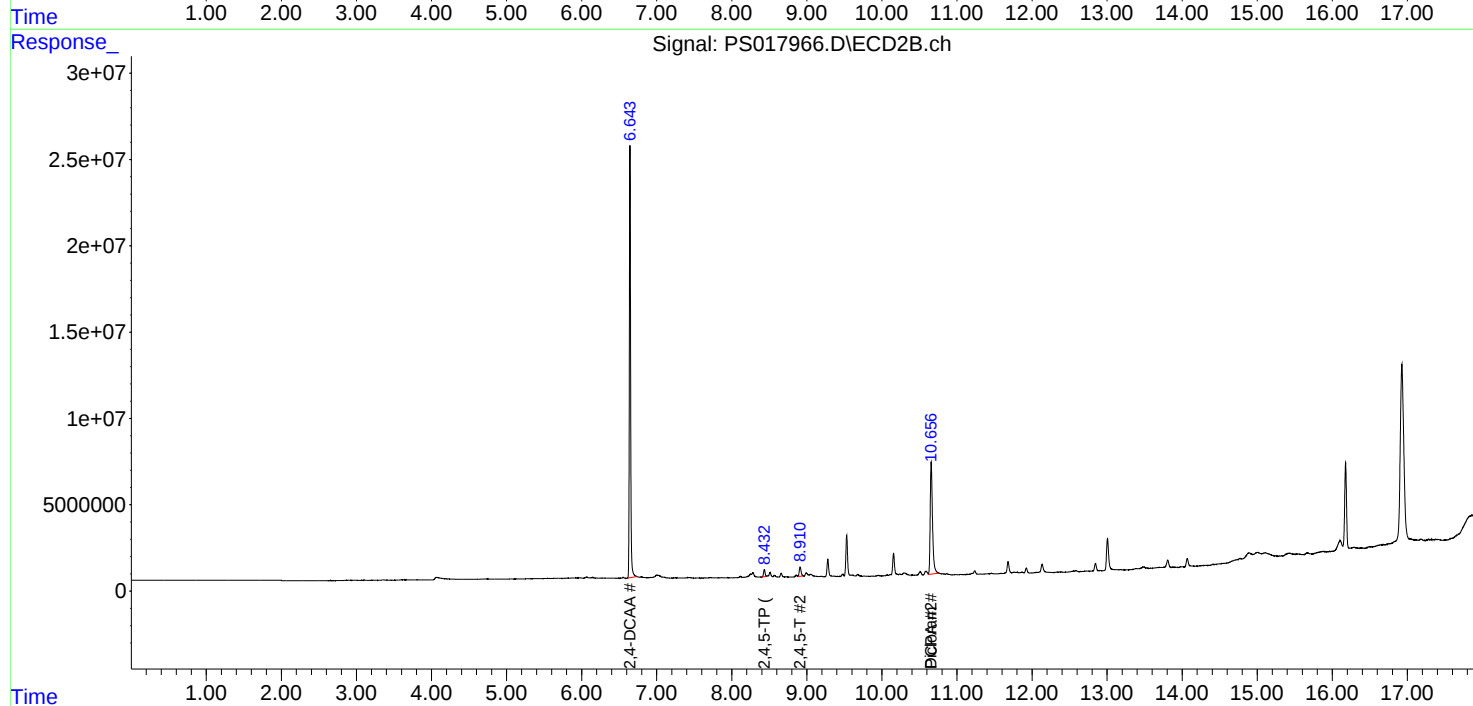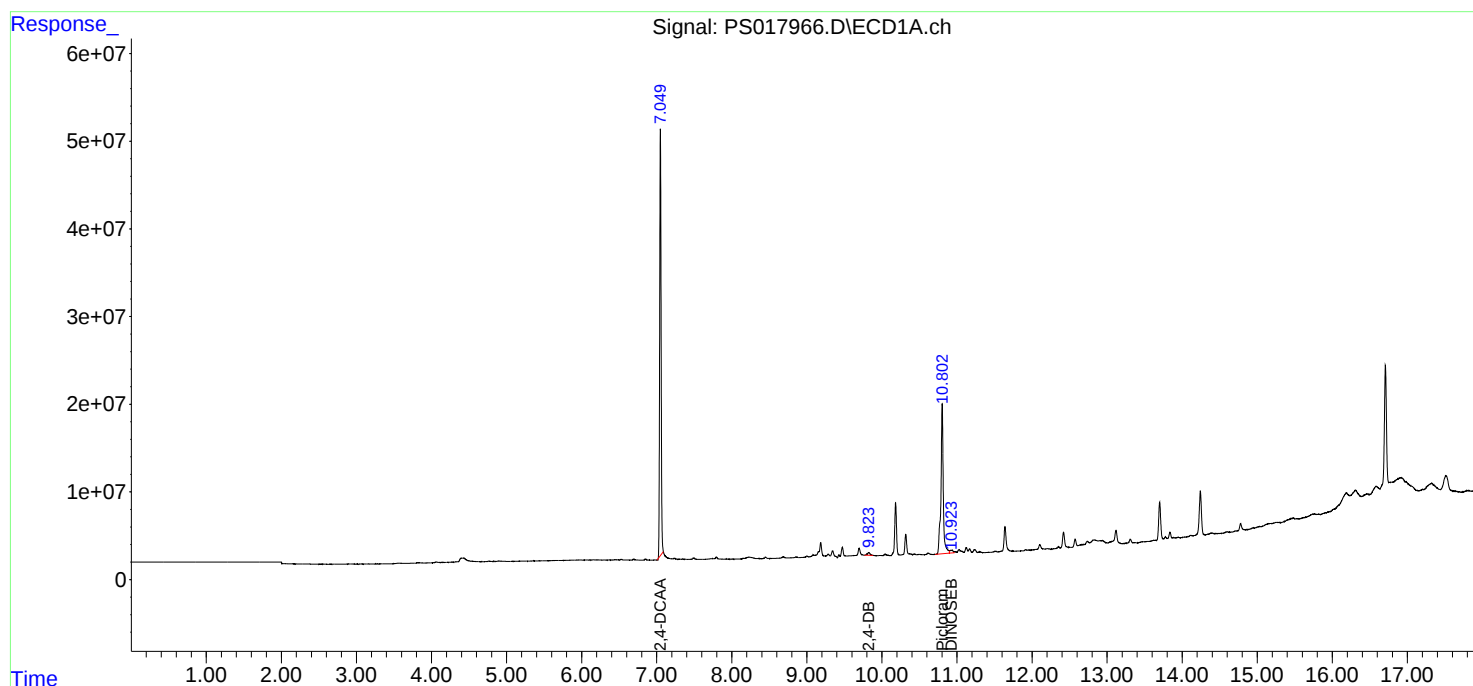


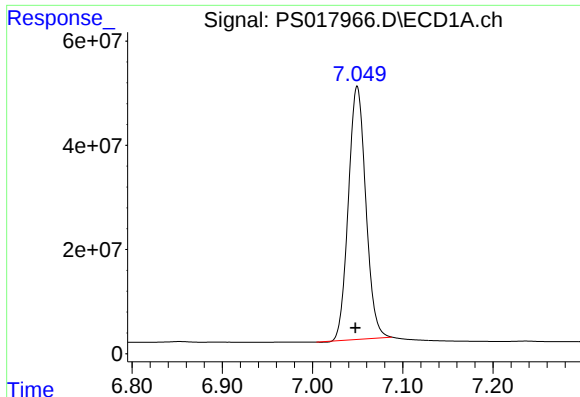

#4 2,4-DCAA


R.T.: 7.050 min
Delta R.T.: 0.002 min
Response: 651315530
Conc: 450.59 ng/ml

Instrument :
ECD_S
ClientSampleId :

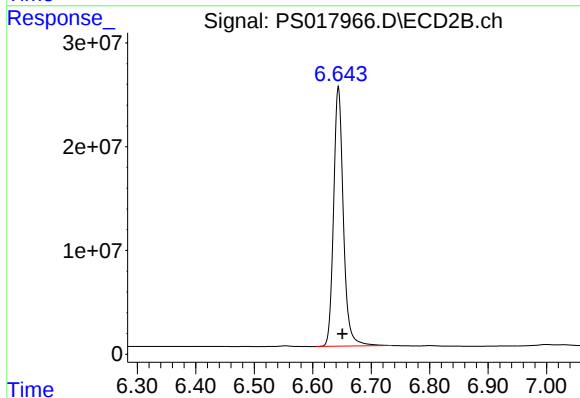


#4 2,4-DCAA

R.T.: 6.644 min
Delta R.T.: -0.007 min
Response: 289748707
Conc: 499.35 ng/ml

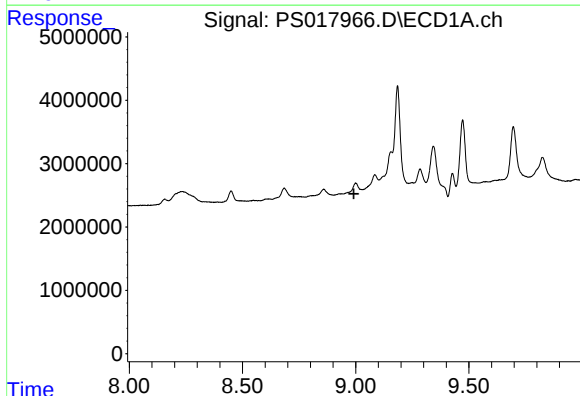


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 8.992 min
Response: 0
Conc: N.D.

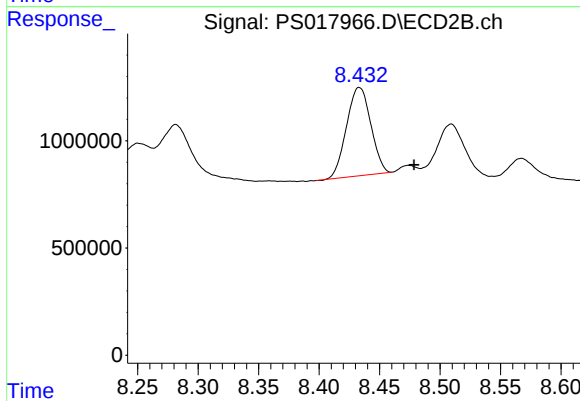

#11 2,4,5-TP (SILVEX)


R.T.: 8.433 min
Delta R.T.: -0.045 min
Response: 5756555
Conc: 1.61 ng/ml

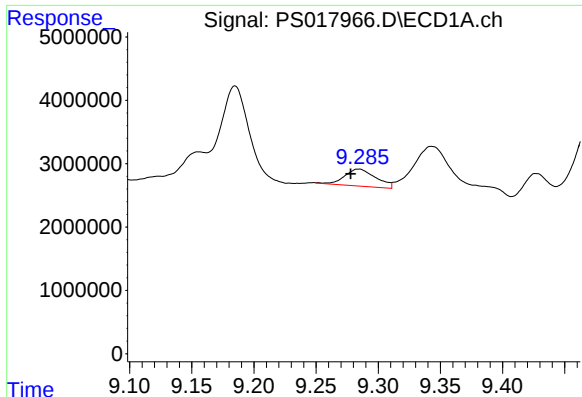

#12 2,4,5-T


R.T.: 9.285 min
Delta R.T.: 0.007 min
Response: 4683958
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

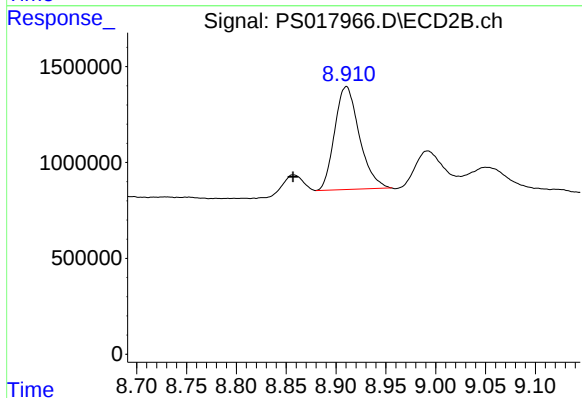


#12 2,4,5-T

R.T.: 8.910 min
Delta R.T.: 0.054 min
Response: 9252167
Conc: 2.83 ng/ml

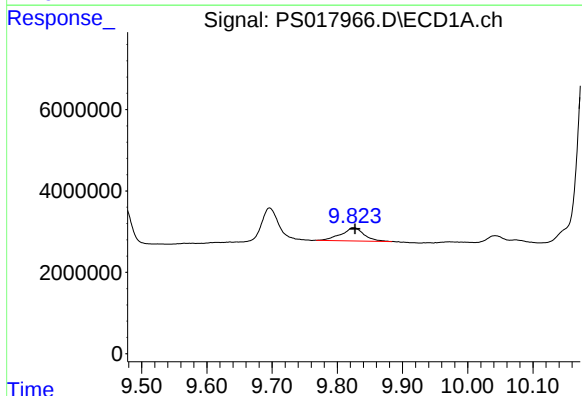


#13 2,4-DB

R.T.: 9.824 min
Delta R.T.: -0.003 min
Response: 7816444
Conc: 4.73 ng/ml

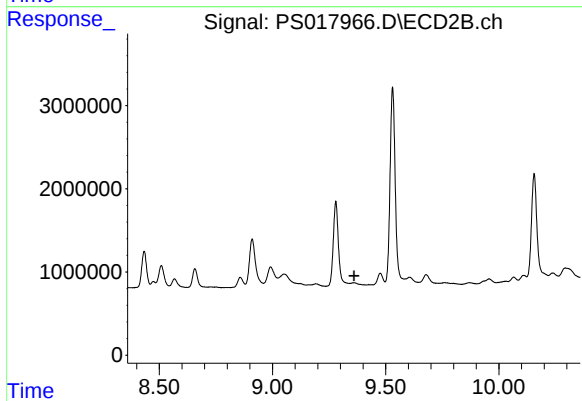

#13 2,4-DB


R.T.: 0.000 min
Exp R.T. : 9.360 min
Response: 0
Conc: N.D.

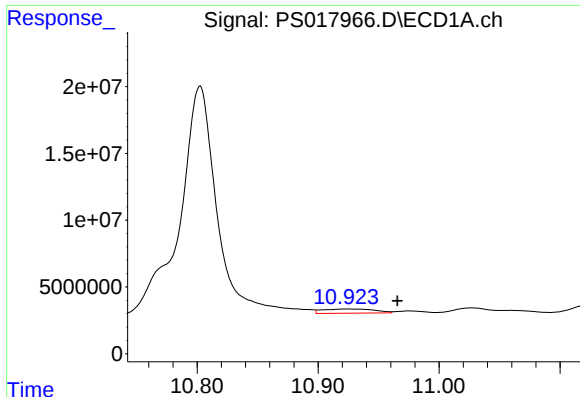

#14 DINOSEB


R.T.: 10.924 min
Delta R.T.: -0.042 min
Response: 9525921
Conc: 1.45 ng/ml

Instrument :
ECD_S
ClientSampleId :

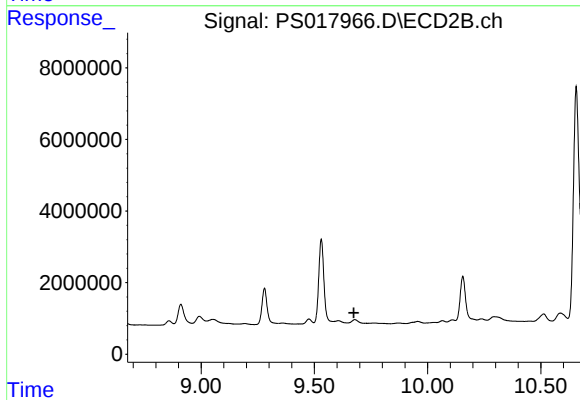


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 9.675 min
Response: 0
Conc: N.D.

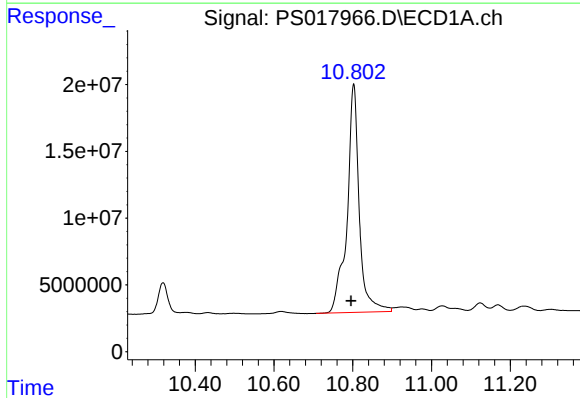


#15 Picloram

R.T.: 10.802 min
Delta R.T.: 0.007 min
Response: 369796732
Conc: 30.98 ng/ml

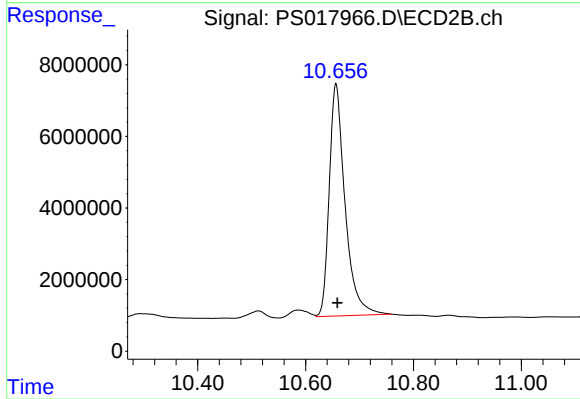

#15 Picloram


R.T.: 10.656 min
Delta R.T.: -0.003 min
Response: 131826334
Conc: 28.19 ng/ml

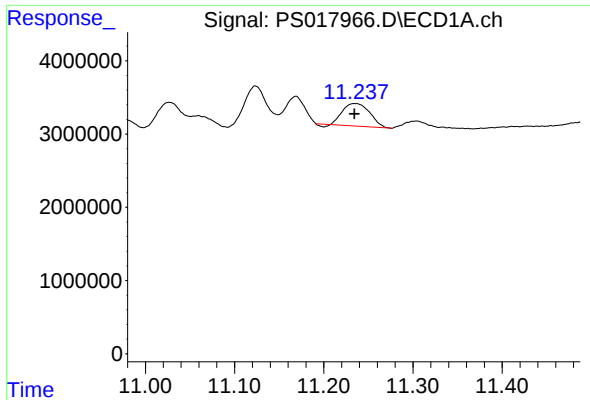

#16 DCPA

R.T.: 11.235 min
Delta R.T.: 0.001 min
Response: 6401465
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

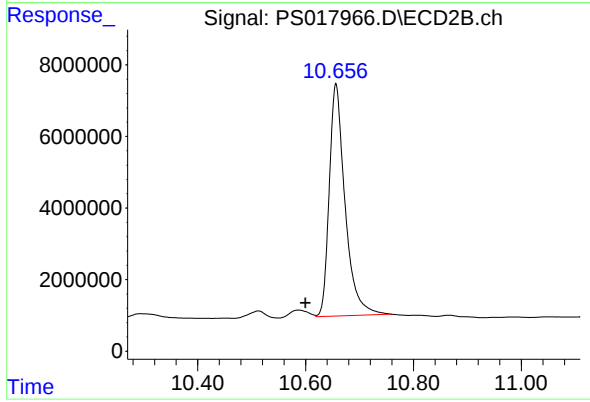

#16 DCPA

R.T.: 10.656 min
Delta R.T.: 0.057 min
Response: 131826334
Conc: 29.86 ng/ml