

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS011222\
 Data File : PS017971.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Jan 2022 14:15
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 13 00:05:09 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010522.M
 Quant Title : 8080.M
 QLast Update : Thu Jan 06 10:21:08 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.048	6.643	666.0E6	296.9E6	460.754	511.625
Target Compounds							
5) T	DICAMBA	7.236	0.000	4178909	0	<MDL	N.D. #
7) T	MCPA	7.487f	0.000	2847991	0	<MDL	N.D. #
9) T	2,4-D	8.199f	0.000	11828223	0	6.496	N.D. #
10) T	Pentachlo...	8.449	8.112	15804161	6178396	<MDL	<MDL #
11) T	2,4,5-TP ...	9.003	8.503	18214130	13713470	2.152	3.847 #
12) T	2,4,5-T	9.284	0.000	9592852	0	1.082	N.D. #
14) T	DINOSEB	10.922f	0.000	41186149	0	6.272	N.D. #
15) T	Picloram	10.770	10.663	173.1E6	56204507	14.499	12.019
16) T	DCPA	11.231	10.663f	25847678	56204507	2.392	12.729 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS011222\
Data File : PS017971.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Jan 2022 14:15
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 13 00:05:09 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010522.M
Quant Title : 8080.M
QLast Update : Thu Jan 06 10:21:08 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

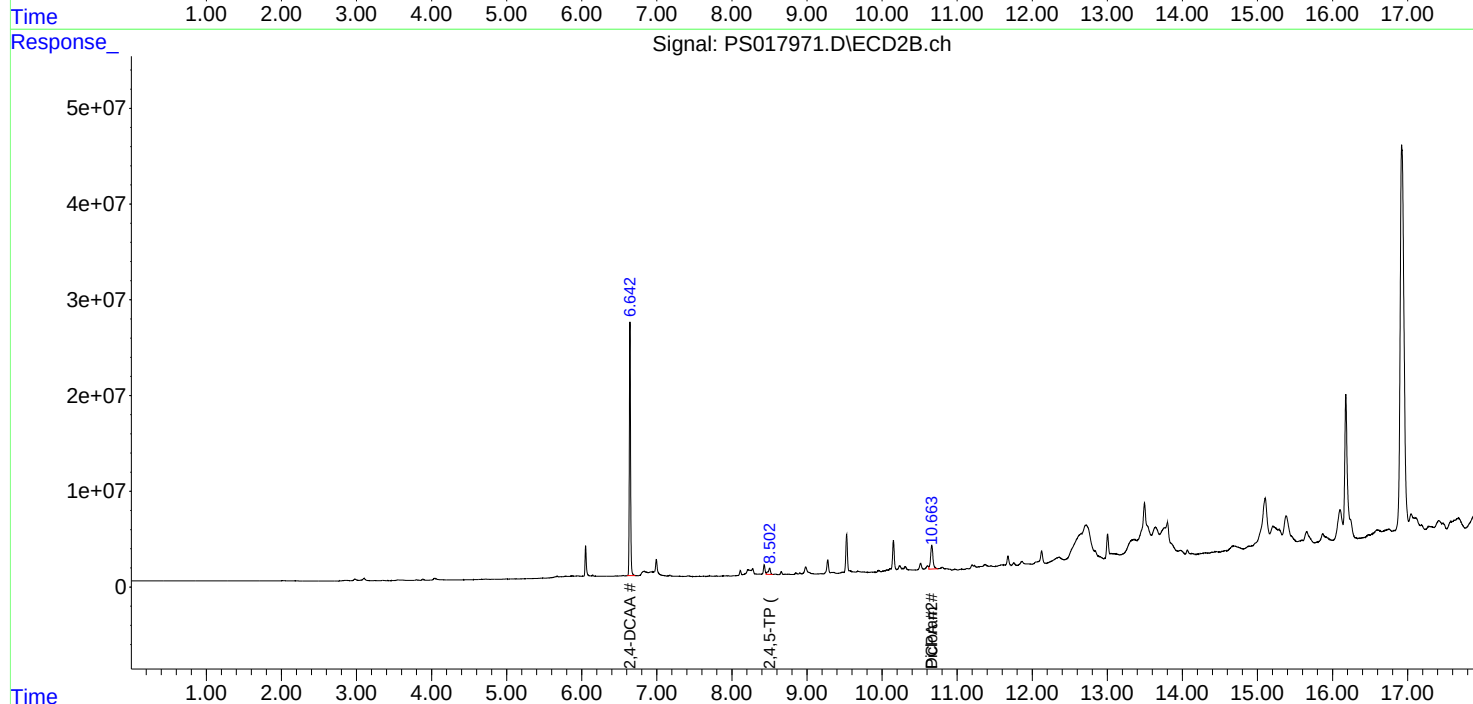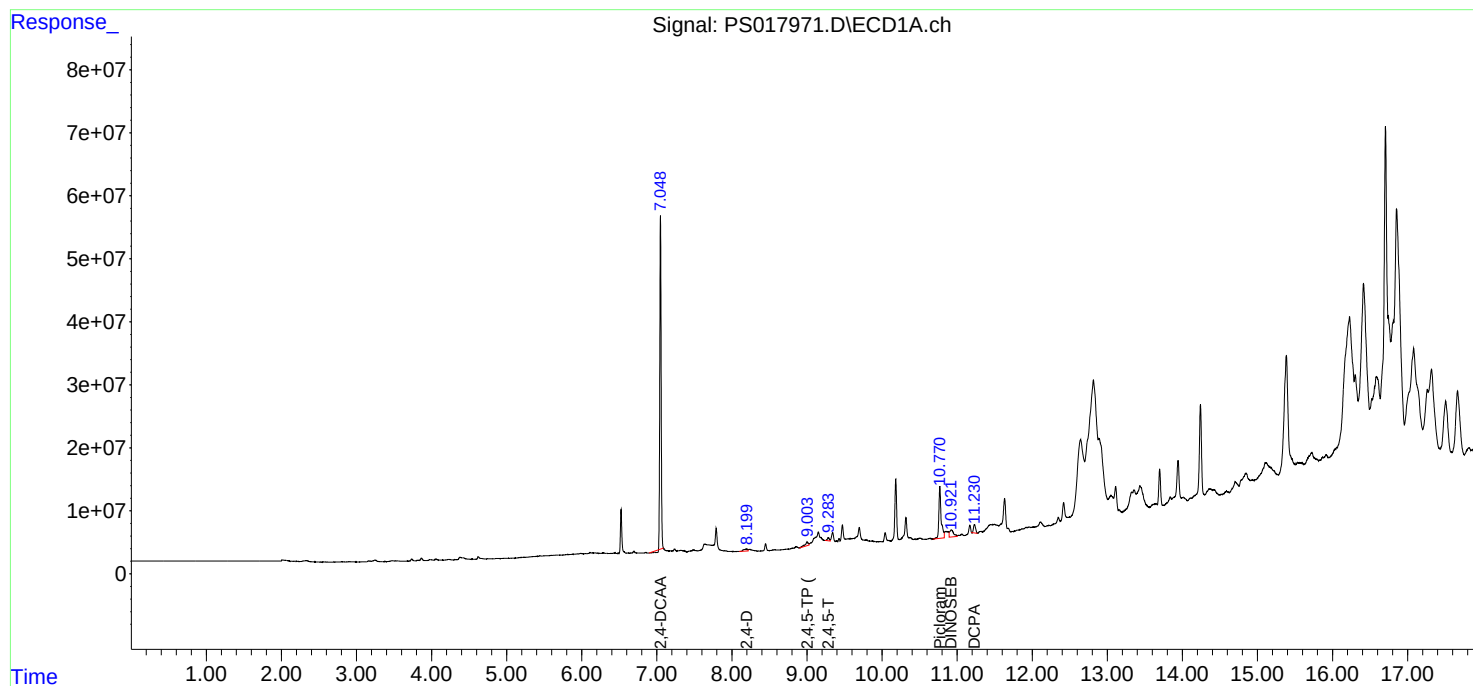


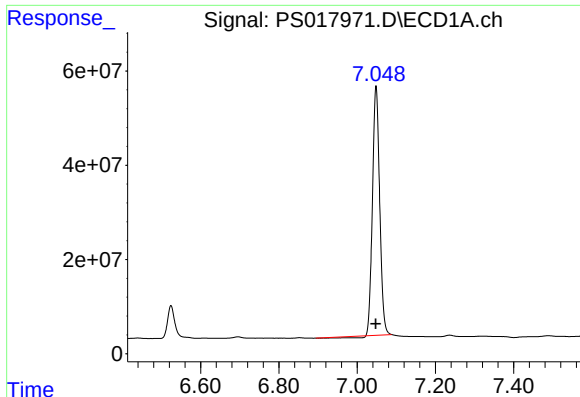

#4 2,4-DCAA


R.T.: 7.048 min
Delta R.T.: 0.000 min
Response: 666013706
Conc: 460.75 ng/ml

Instrument :
ECD_S
ClientSampleId :

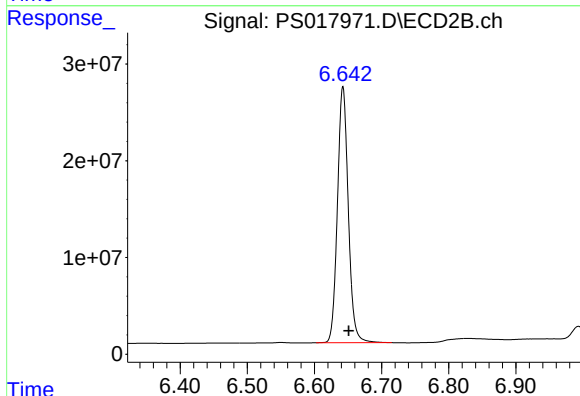


#4 2,4-DCAA

R.T.: 6.643 min
Delta R.T.: -0.008 min
Response: 296869741
Conc: 511.62 ng/ml

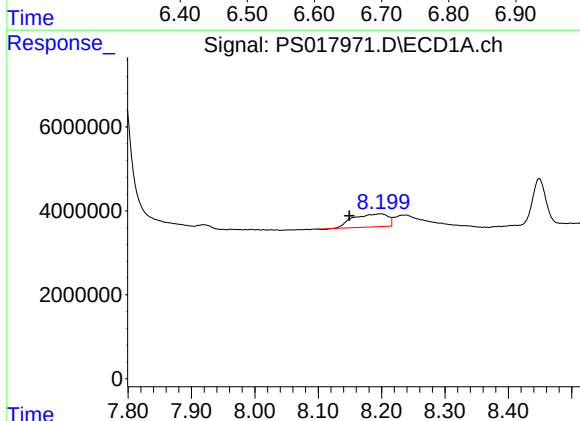


#9 2,4-D

R.T.: 8.199 min
Delta R.T.: 0.050 min
Response: 11828223
Conc: 6.50 ng/ml

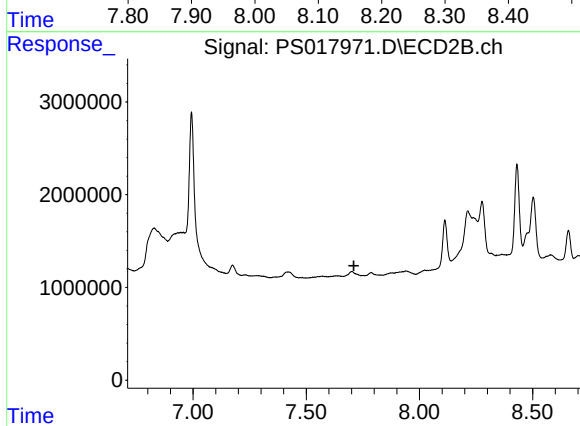

#9 2,4-D


R.T.: 0.000 min
Exp R.T. : 7.710 min
Response: 0
Conc: N.D.

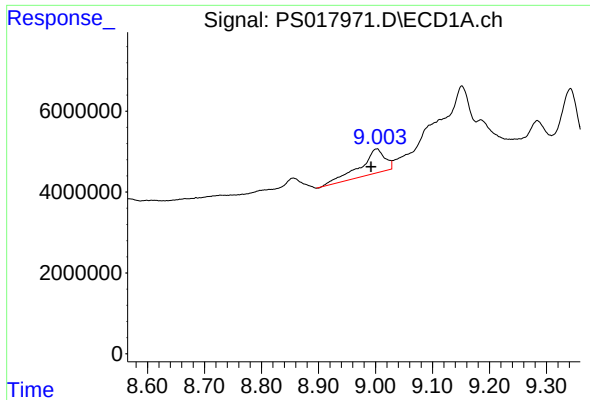

#11 2,4,5-TP (SILVEX)


R.T.: 9.003 min
Delta R.T.: 0.011 min
Response: 18214130
Conc: 2.15 ng/ml

Instrument :
ECD_S
ClientSampleId :

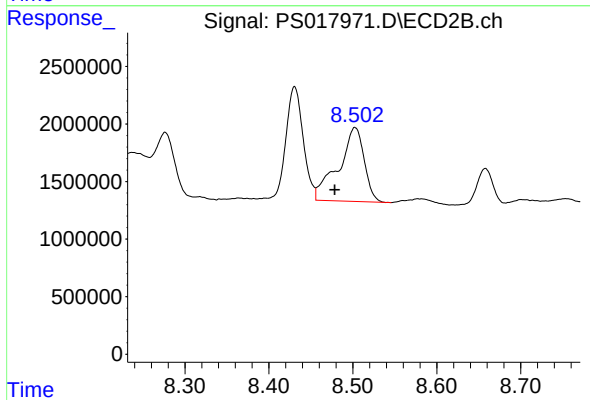


#11 2,4,5-TP (SILVEX)

R.T.: 8.503 min
Delta R.T.: 0.024 min
Response: 13713470
Conc: 3.85 ng/ml

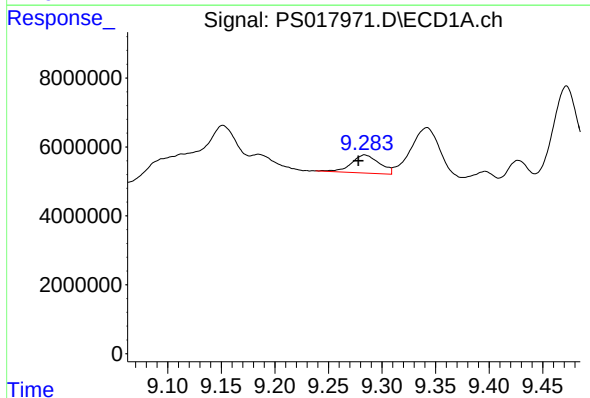


#12 2,4,5-T

R.T.: 9.284 min
Delta R.T.: 0.006 min
Response: 9592852
Conc: 1.08 ng/ml

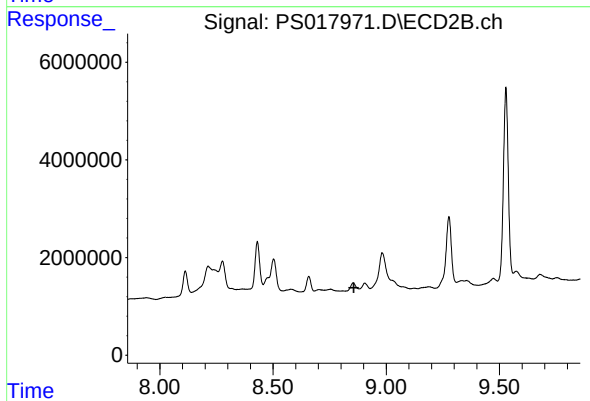

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T. : 8.857 min
Response: 0
Conc: N.D.

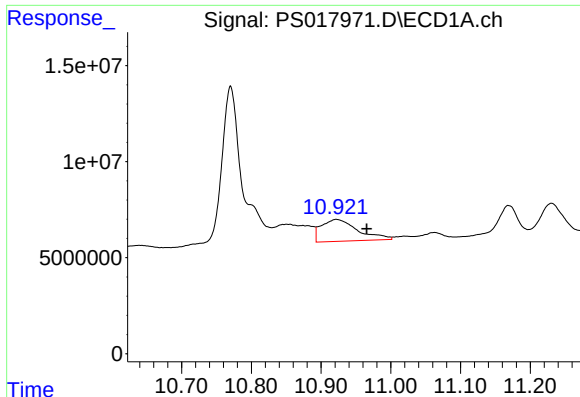

#14 DINoseb


R.T.: 10.922 min
Delta R.T.: -0.044 min
Response: 41186149
Conc: 6.27 ng/ml

Instrument :
ECD_S
ClientSampleId :

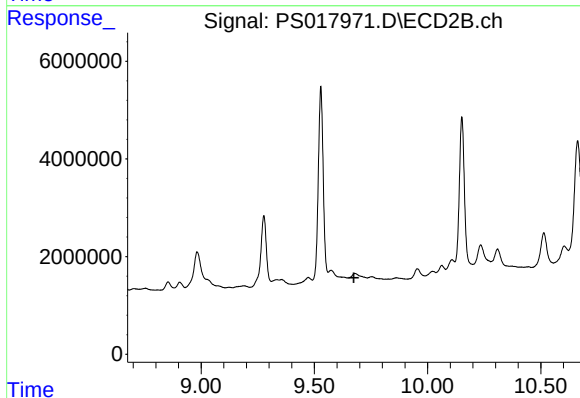


#14 DINoseb

R.T.: 0.000 min
Exp R.T. : 9.675 min
Response: 0
Conc: N.D.

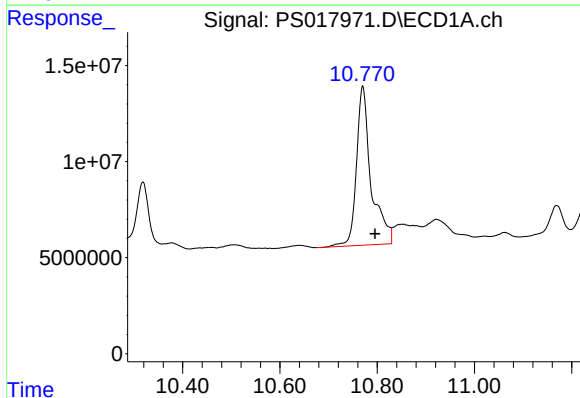


#15 Picloram

R.T.: 10.770 min
Delta R.T.: -0.026 min
Response: 173059042
Conc: 14.50 ng/ml

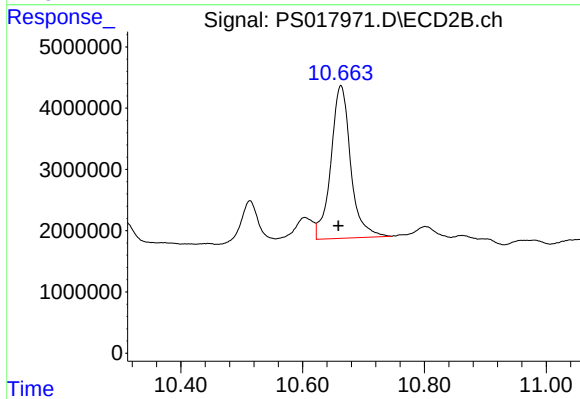

#15 Picloram


R.T.: 10.663 min
Delta R.T.: 0.004 min
Response: 56204507
Conc: 12.02 ng/ml

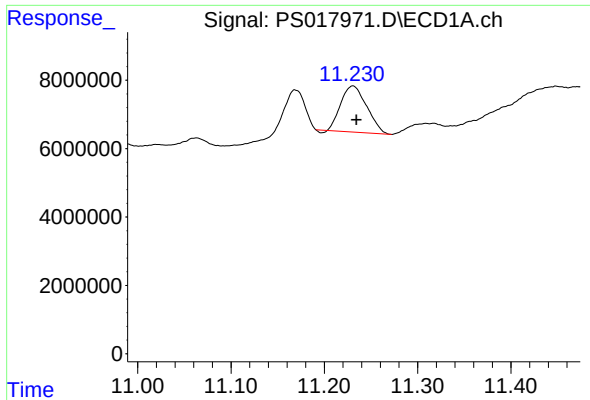

#16 DCPA

R.T.: 11.231 min
Delta R.T.: -0.004 min
Response: 25847678
Conc: 2.39 ng/ml

Instrument :
ECD_S
ClientSampleId :

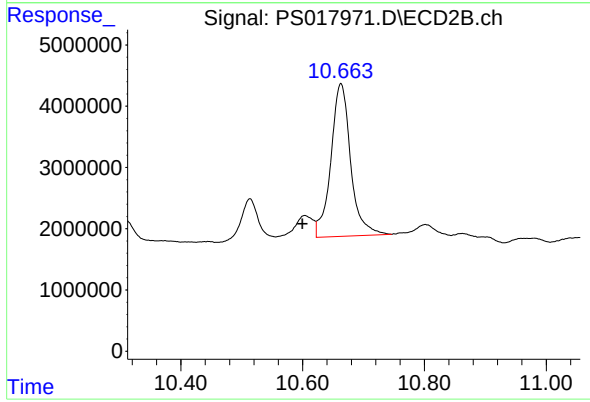

#16 DCPA

R.T.: 10.663 min
Delta R.T.: 0.063 min
Response: 56204507
Conc: 12.73 ng/ml