

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS011222\
 Data File : PS017977.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Jan 2022 18:33
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 13 00:07:47 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010522.M
 Quant Title : 8080.M
 QLast Update : Thu Jan 06 10:21:08 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.048	6.643	680.5E6	299.4E6	470.778	516.001
Target Compounds							
2) T	3,5-DICHL...	6.290	0.000	1728971	0	<MDL	N.D. #
5) T	DICAMBA	7.234	0.000	6521402	0	1.044	N.D. #
7) T	MCPA	7.488f	0.000	8511800	0	1.276	N.D. #
9) T	2,4-D	8.203f	0.000	2284061	0	1.254	N.D. #
10) T	Pentachlo...	8.448	8.114	21249850	9081882	1.006	1.078
11) T	2,4,5-TP ...	8.999	8.432f	9729257	6690612	1.150	1.877 #
12) T	2,4,5-T	9.282	0.000	18356401	0	2.071	N.D. #
14) T	DINOSEB	10.976	0.000	8760288	0	1.334	N.D. #
15) T	Picloram	10.803	10.665	48911449	20026567	4.098	4.283
16) T	DCPA	11.243	10.665f	18993160	20026567	1.758	4.536 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS011222\
Data File : PS017977.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Jan 2022 18:33
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 13 00:07:47 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010522.M
Quant Title : 8080.M
QLast Update : Thu Jan 06 10:21:08 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

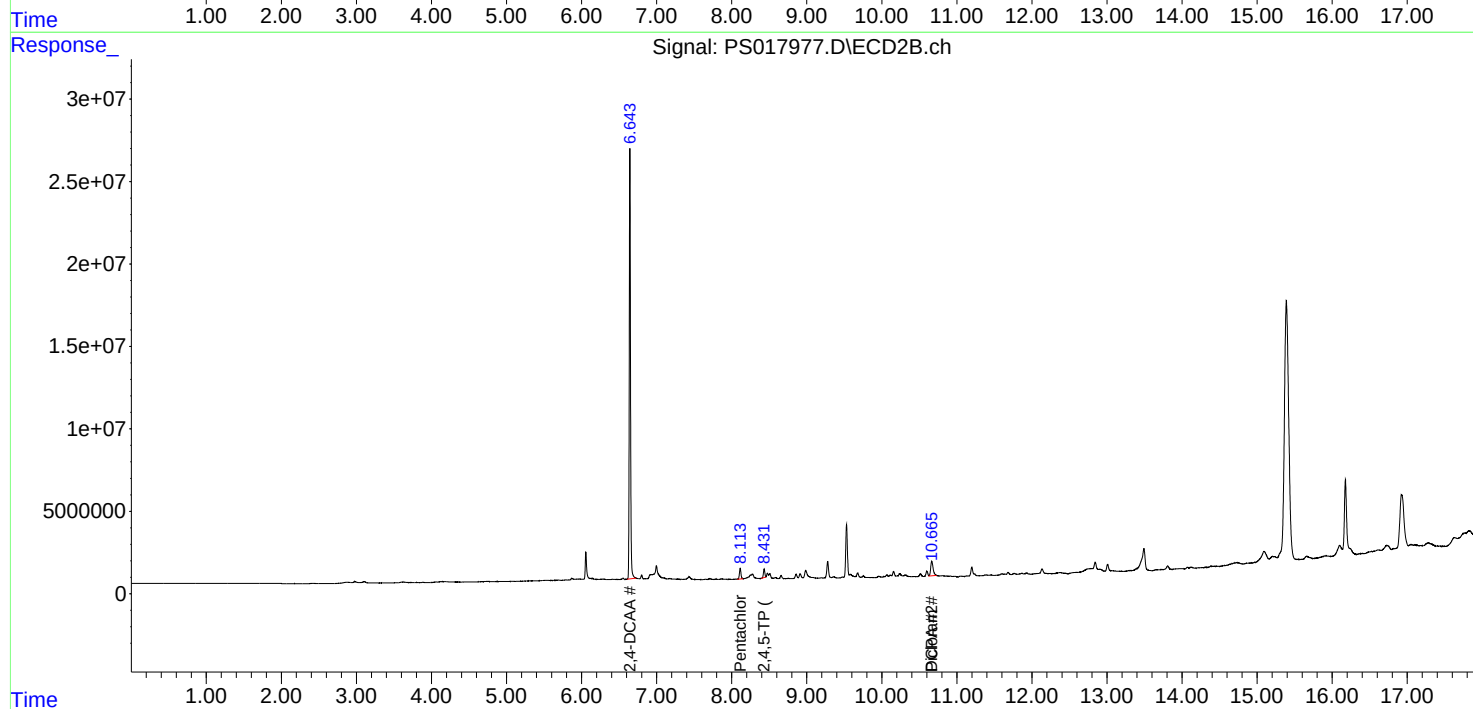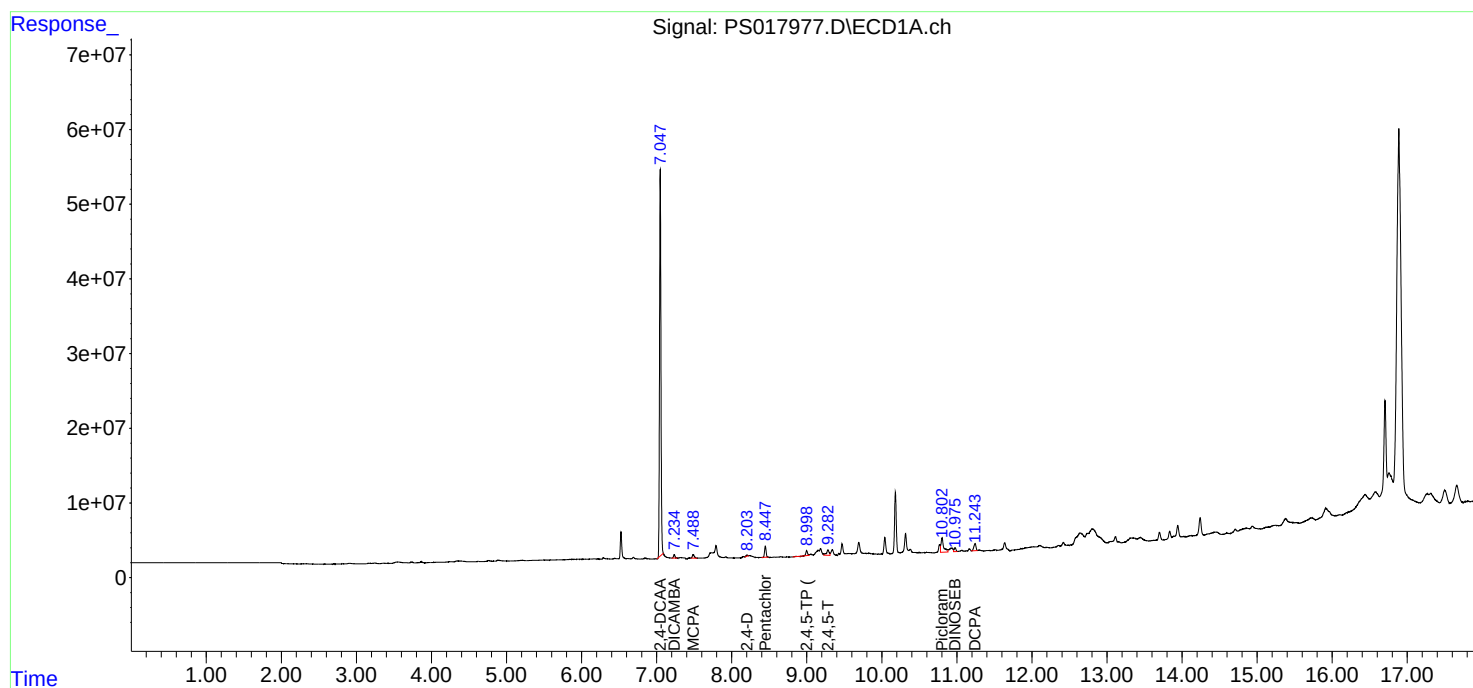


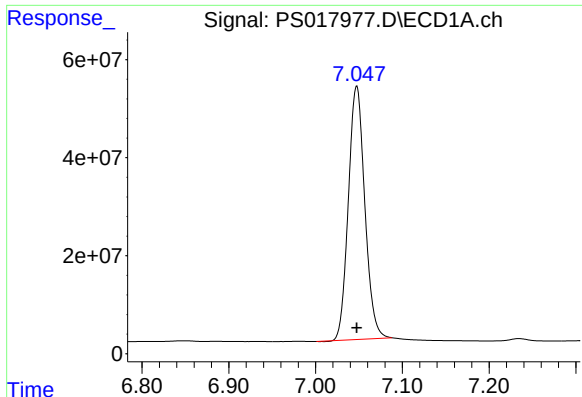

#4 2,4-DCAA


R.T.: 7.048 min
Delta R.T.: 0.000 min
Response: 680504244
Conc: 470.78 ng/ml

Instrument :
ECD_S
ClientSampleId :

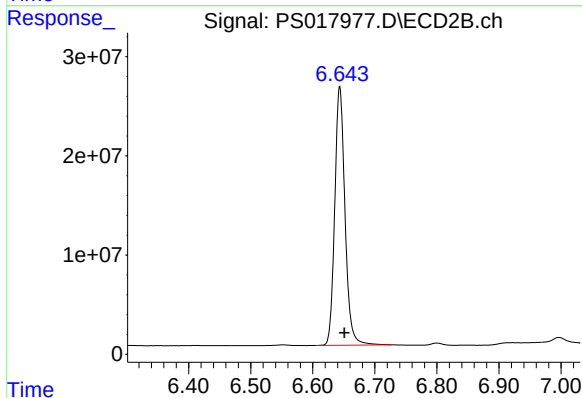


#4 2,4-DCAA

R.T.: 6.643 min
Delta R.T.: -0.007 min
Response: 299409043
Conc: 516.00 ng/ml

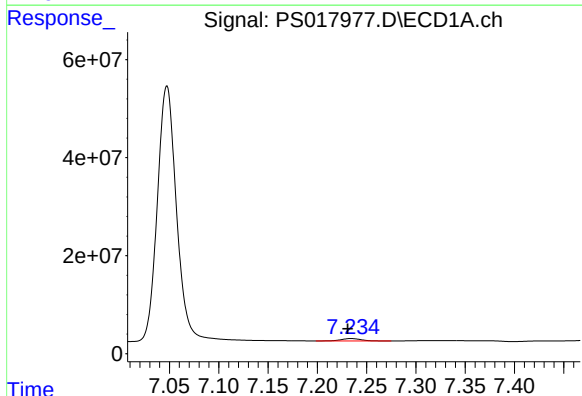


#5 DICAMBA

R.T.: 7.234 min
Delta R.T.: 0.003 min
Response: 6521402
Conc: 1.04 ng/ml

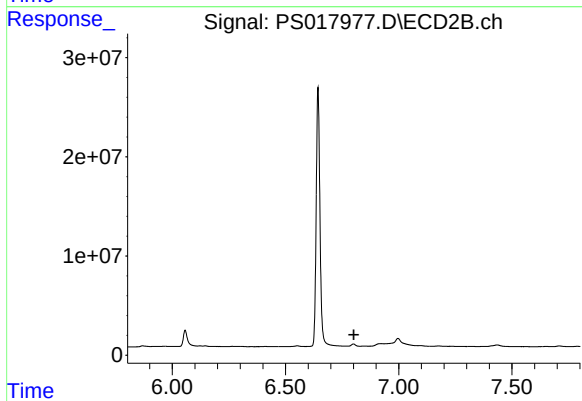

#5 DICAMBA


R.T.: 0.000 min
Exp R.T. : 6.802 min
Response: 0
Conc: N.D.

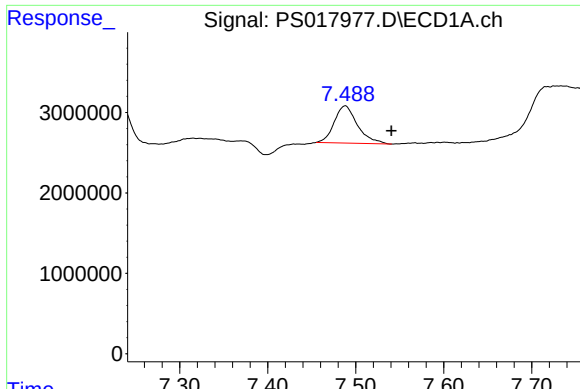

#7 MCPA


R.T.: 7.488 min
Delta R.T.: -0.052 min
Response: 8511800
Conc: 1.28 ug/ml

Instrument :
ECD_S
ClientSampleId :

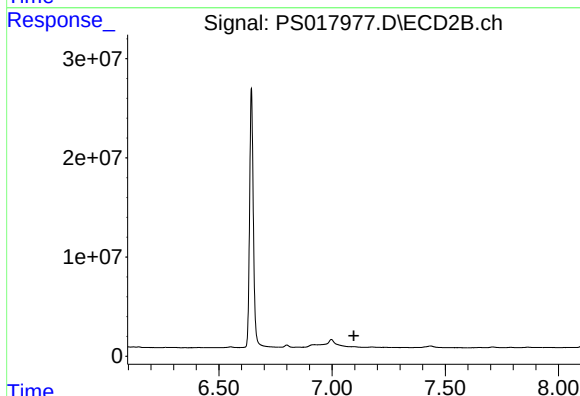


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 7.096 min
Response: 0
Conc: N.D.

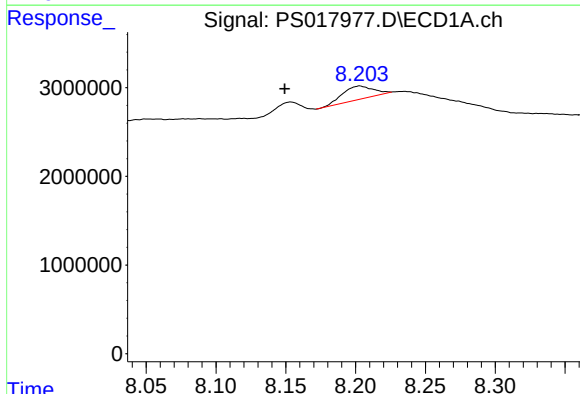


#9 2,4-D

R.T.: 8.203 min
Delta R.T.: 0.054 min
Response: 2284061
Conc: 1.25 ng/ml

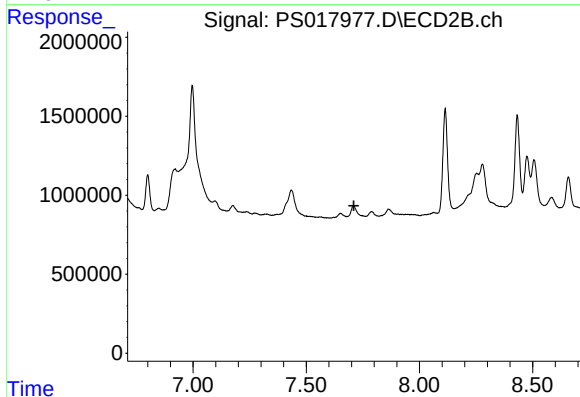

#9 2,4-D


R.T.: 0.000 min
Exp R.T. : 7.710 min
Response: 0
Conc: N.D.

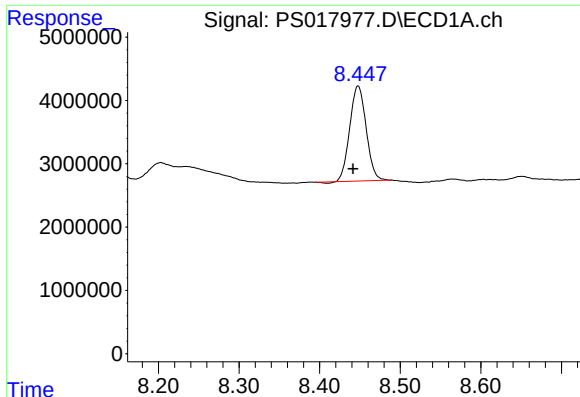

#10 Pentachlorophenol


R.T.: 8.448 min
Delta R.T.: 0.006 min
Response: 21249850
Conc: 1.01 ng/ml

Instrument :
ECD_S
ClientSampleId :

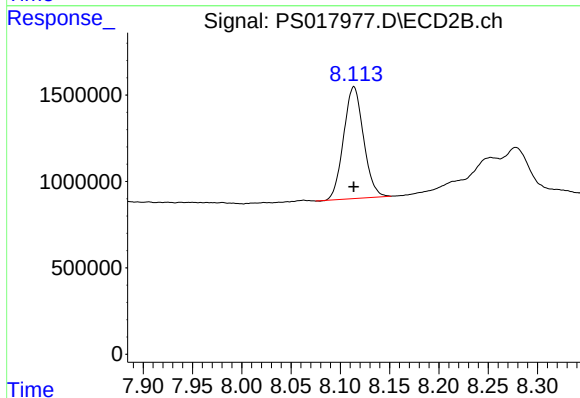


#10 Pentachlorophenol

R.T.: 8.114 min
Delta R.T.: 0.000 min
Response: 9081882
Conc: 1.08 ng/ml

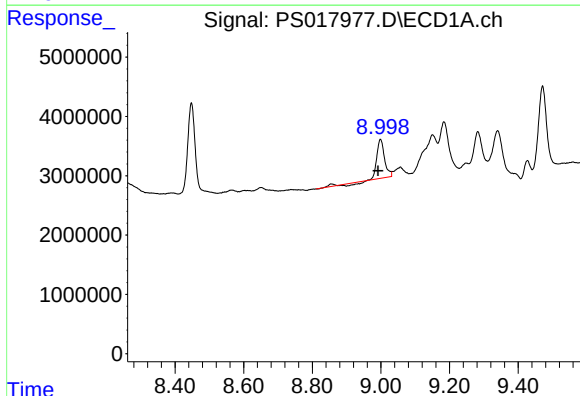


#11 2,4,5-TP (SILVEX)

R.T.: 8.999 min
Delta R.T.: 0.007 min
Response: 9729257
Conc: 1.15 ng/ml

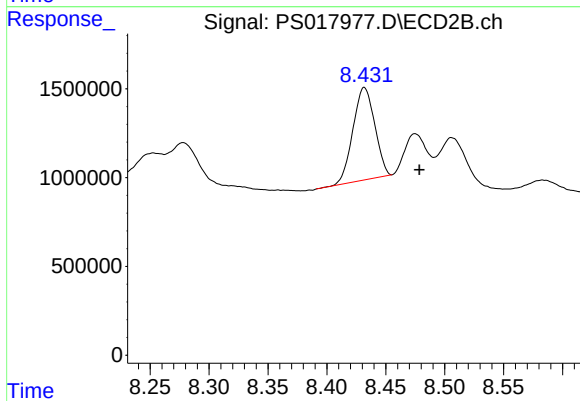

#11 2,4,5-TP (SILVEX)


R.T.: 8.432 min
Delta R.T.: -0.047 min
Response: 6690612
Conc: 1.88 ng/ml

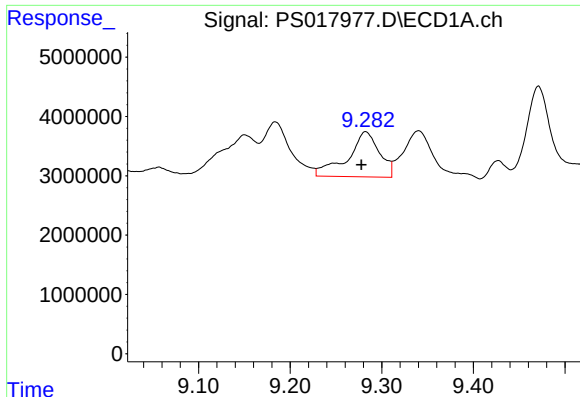

#12 2,4,5-T


R.T.: 9.282 min
Delta R.T.: 0.004 min
Response: 18356401
Conc: 2.07 ng/ml

Instrument :
ECD_S
ClientSampleId :

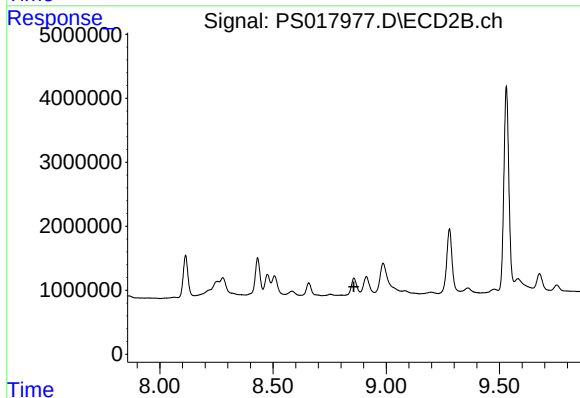


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 8.857 min
Response: 0
Conc: N.D.

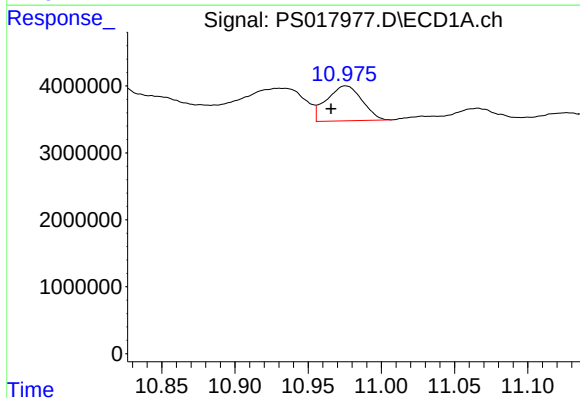


#14 DINOSEB

R.T.: 10.976 min
Delta R.T.: 0.010 min
Response: 8760288
Conc: 1.33 ng/ml

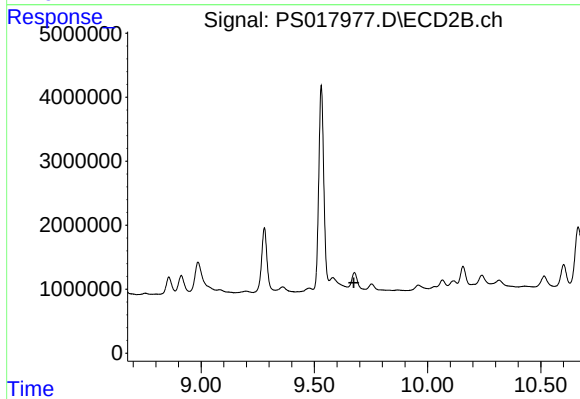

#14 DINOSEB


R.T.: 0.000 min
Exp R.T. : 9.675 min
Response: 0
Conc: N.D.

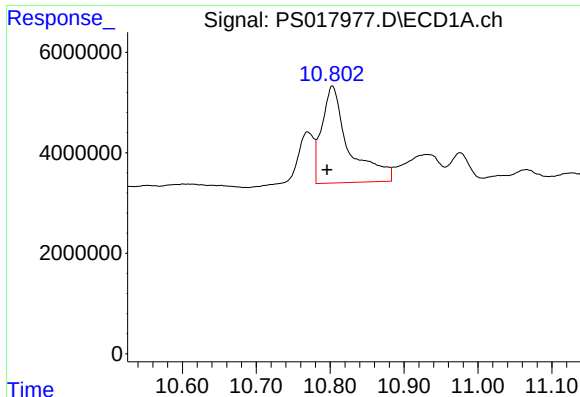

#15 Picloram


R.T.: 10.803 min
Delta R.T.: 0.007 min
Response: 48911449
Conc: 4.10 ng/ml

Instrument :
ECD_S
ClientSampleId :

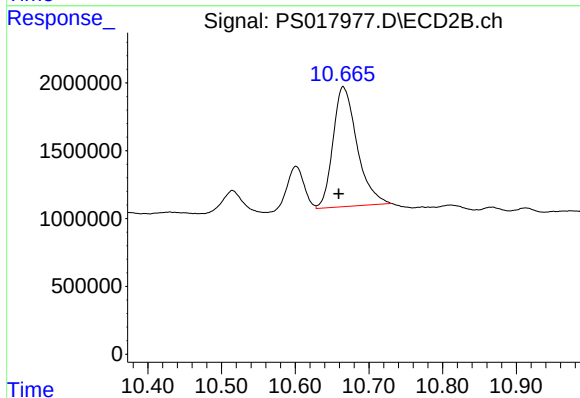


#15 Picloram

R.T.: 10.665 min
Delta R.T.: 0.006 min
Response: 20026567
Conc: 4.28 ng/ml

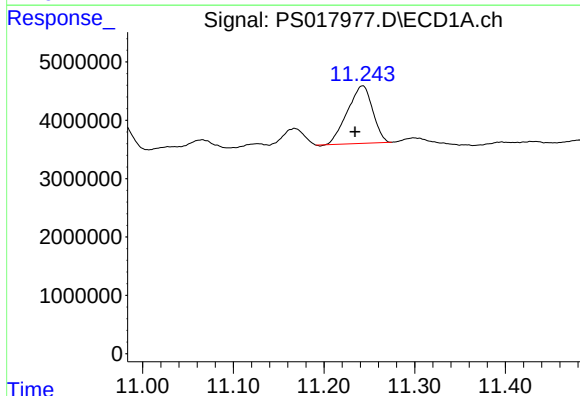

#16 DCPA

R.T.: 11.243 min
Delta R.T.: 0.008 min
Response: 18993160
Conc: 1.76 ng/ml

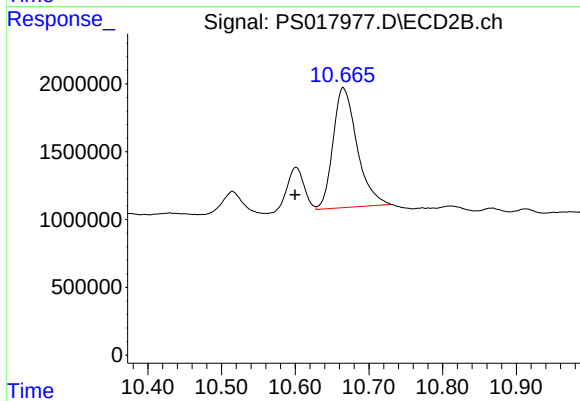

#16 DCPA

R.T.: 10.665 min
Delta R.T.: 0.065 min
Response: 20026567
Conc: 4.54 ng/ml