

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS011223\
 Data File : PS021736.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Jan 2023 08:42
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 12 11:46:59 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010923.M
 Quant Title : 8080.M
 QLast Update : Tue Jan 10 10:34:52 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.378	6.812	1422.4E6	1037.8E6	511.009	577.619
Target Compounds							
1) T	Dalapon	2.523f	0.000	625227	0	1.722	N.D. #
3) T	4-Nitroph...	6.224	0.000	6760900	0	4.638	N.D. #
5) T	DICAMBA	0.000	6.974	0	10240232	N.D.	1.204
6) T	MCP	6.700	7.032f	-848856	4645484	N.D.	<MDL
7) T	MCPA	6.761f	7.219f	5580267	13004177	<MDL	1.434 #
8) T	DICHLORPROP	7.135	7.653f	1219048	3126006	<MDL	1.465 #
9) T	2,4-D	7.310	7.941f	9677657	2757203	2.492	1.091 #
10) T	Pentachlo...	7.552	8.320	4956709	4608222	<MDL	<MDL #
11) T	2,4,5-TP ...	8.087	8.686	4083928	4514210	<MDL	<MDL #
12) T	2,4,5-T	8.374	9.082	37762550	7323988	1.959	<MDL #
13) T	2,4-DB	8.834	9.591	489051	925324	<MDL	<MDL #
14) T	DINOSEB	0.000	9.893	0	3850977	N.D.	<MDL
15) T	Picloram	9.727	10.889	25518997	290.7E6	<MDL	16.413 #
16) T	DCPA	10.164	10.818	6788361	19117683	<MDL	1.371 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS011223\
Data File : PS021736.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Jan 2023 08:42
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 12 11:46:59 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010923.M
Quant Title : 8080.M
QLast Update : Tue Jan 10 10:34:52 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

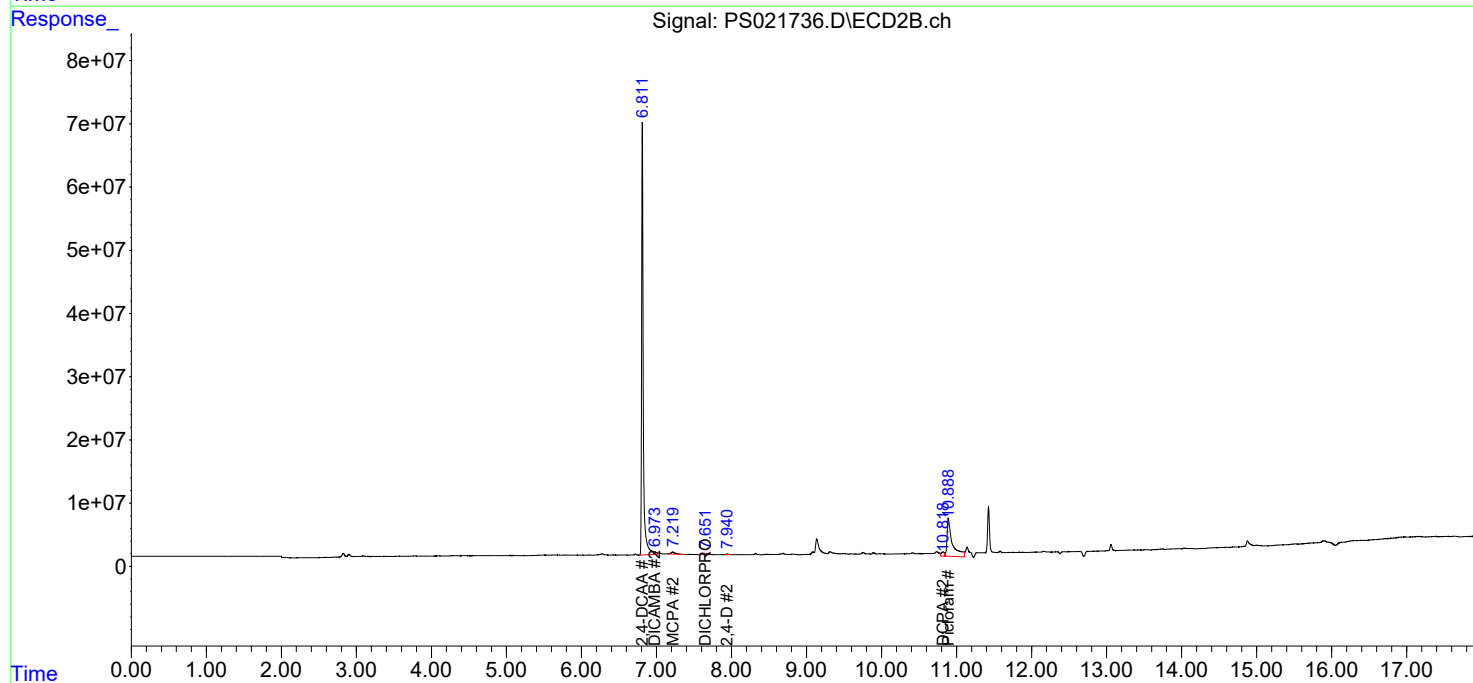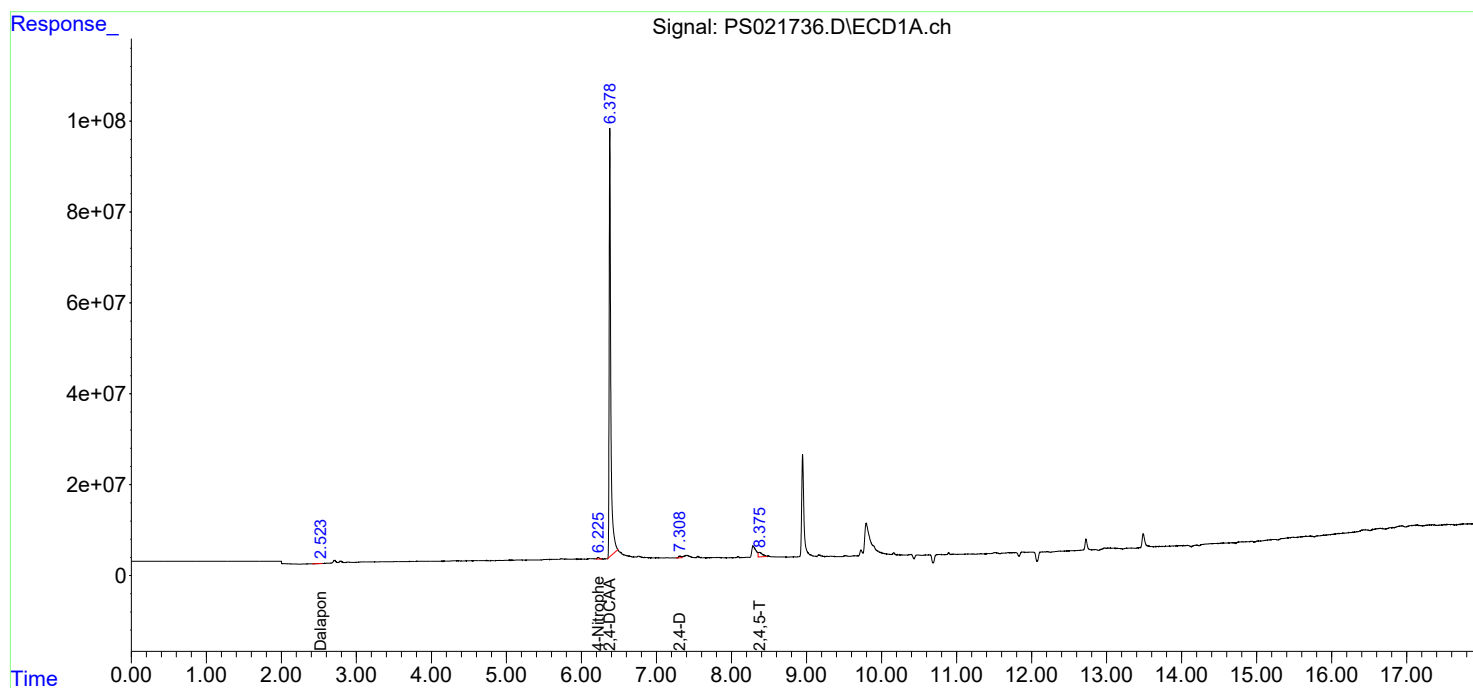


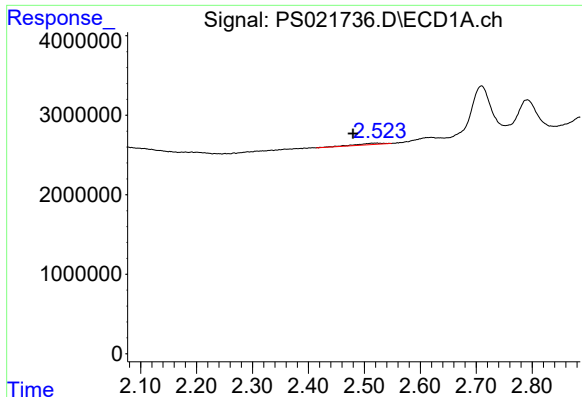

#1 Dalapon


R.T.: 2.523 min
Delta R.T.: 0.043 min
Response: 625227
Conc: 1.72 ng/ml

Instrument :
ECD_S
ClientSampleId :

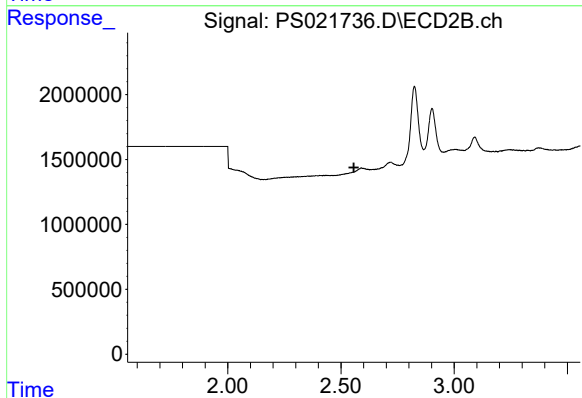


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 2.557 min
Response: 0
Conc: N.D.

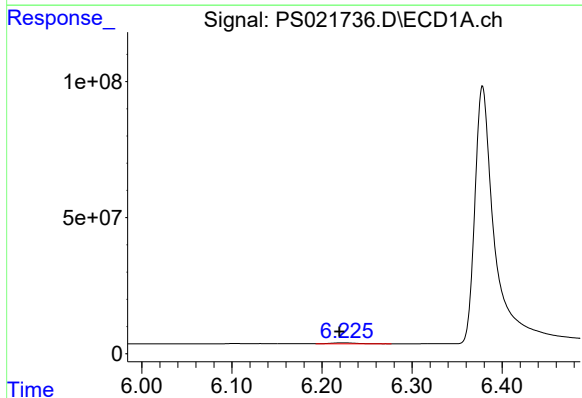


#3 4-Nitrophenol

R.T.: 6.224 min
Delta R.T.: 0.005 min
Response: 6760900
Conc: 4.64 ng/ml

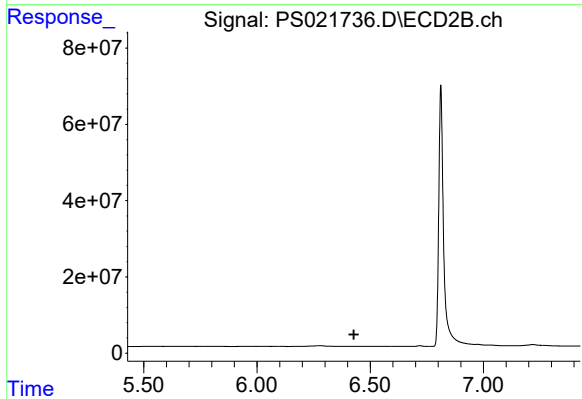

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T. : 6.428 min
Response: 0
Conc: N.D.

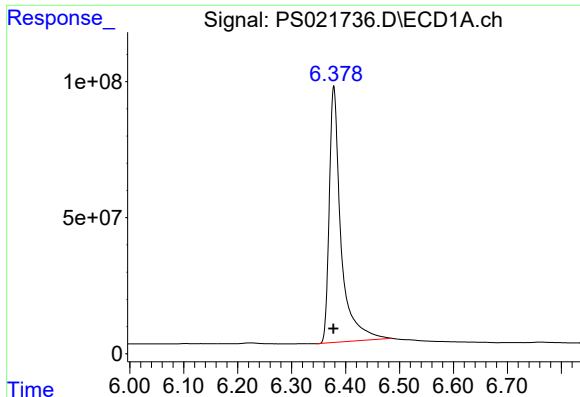

#4 2,4-DCAA


R.T.: 6.378 min
Delta R.T.: 0.000 min
Response: 1422427197
Conc: 511.01 ng/ml

Instrument :
ECD_S
ClientSampleId :

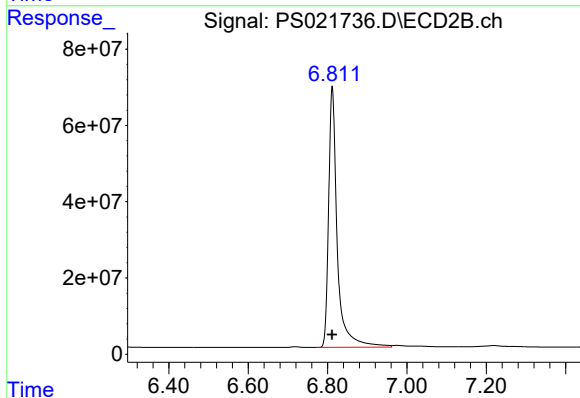


#4 2,4-DCAA

R.T.: 6.812 min
Delta R.T.: 0.000 min
Response: 1037801504
Conc: 577.62 ng/ml

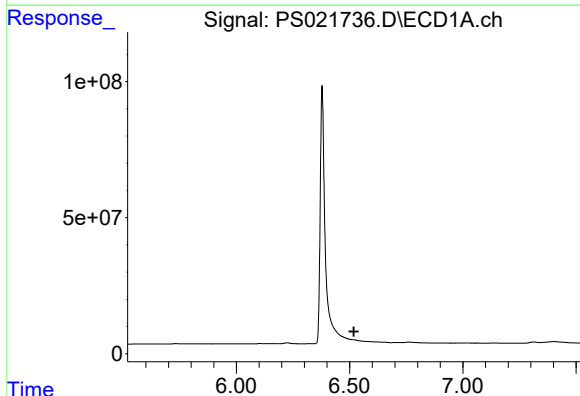


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 6.518 min
Response: 0
Conc: N.D.

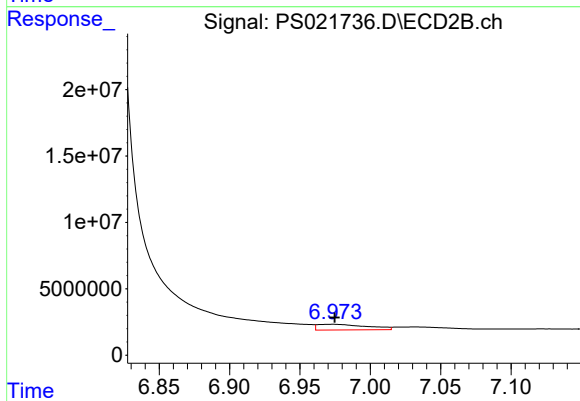

#5 DICAMBA


R.T.: 6.974 min
Delta R.T.: 0.000 min
Response: 10240232
Conc: 1.20 ng/ml

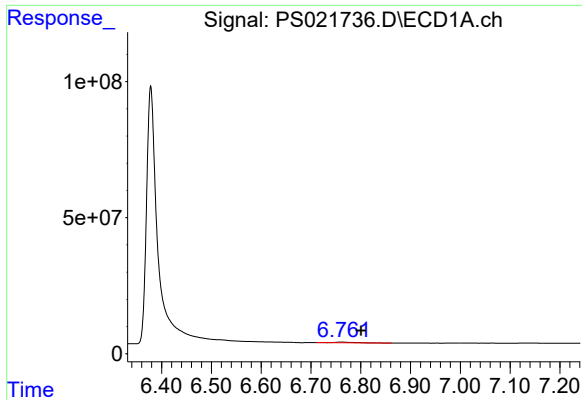

#7 MCPA


R.T.: 6.761 min
Delta R.T.: -0.041 min
Response: 5580267
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

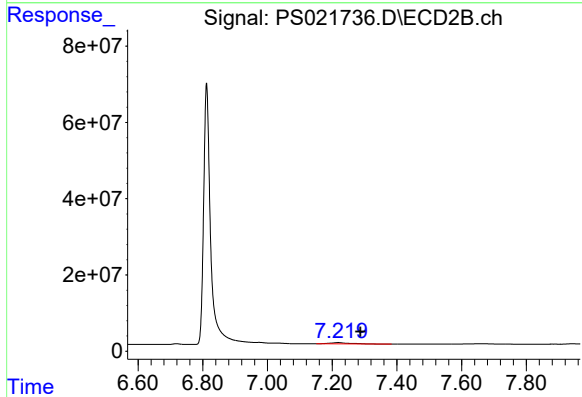


#7 MCPA

R.T.: 7.219 min
Delta R.T.: -0.068 min
Response: 13004177
Conc: 1.43 ug/ml

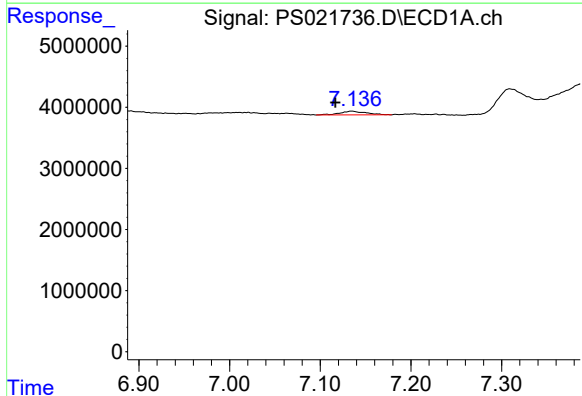


#8 DICHLORPROP

R.T.: 7.135 min
Delta R.T.: 0.018 min
Response: 1219048
Conc: N.D.

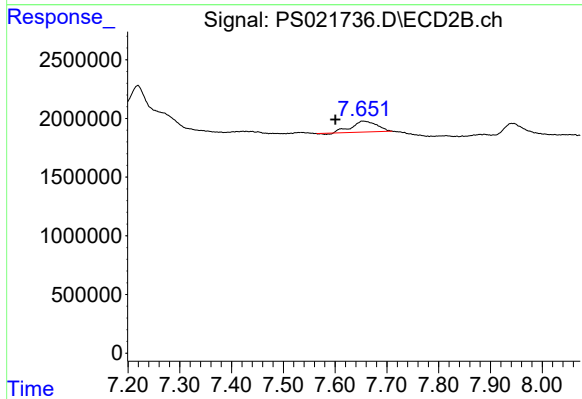

#8 DICHLORPROP


R.T.: 7.653 min
Delta R.T.: 0.053 min
Response: 3126006
Conc: 1.47 ng/ml

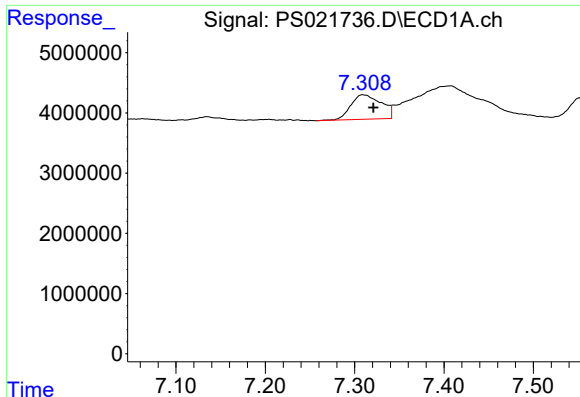

#9 2,4-D


R.T.: 7.310 min
Delta R.T.: -0.011 min
Response: 9677657
Conc: 2.49 ng/ml

Instrument :
ECD_S
ClientSampleId :

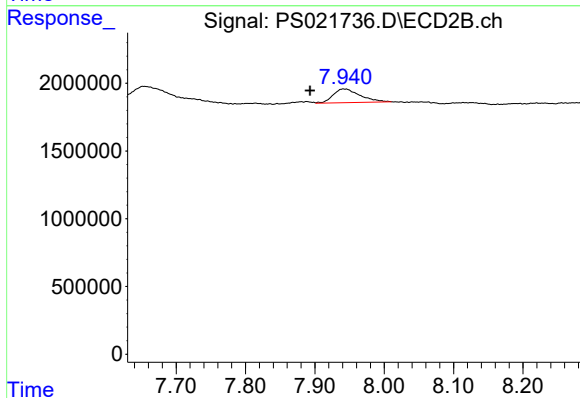


#9 2,4-D

R.T.: 7.941 min
Delta R.T.: 0.048 min
Response: 2757203
Conc: 1.09 ng/ml

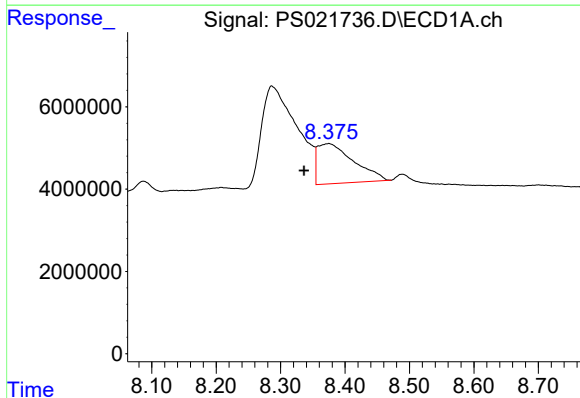


#12 2,4,5-T

R.T.: 8.374 min
Delta R.T.: 0.038 min
Response: 37762550
Conc: 1.96 ng/ml

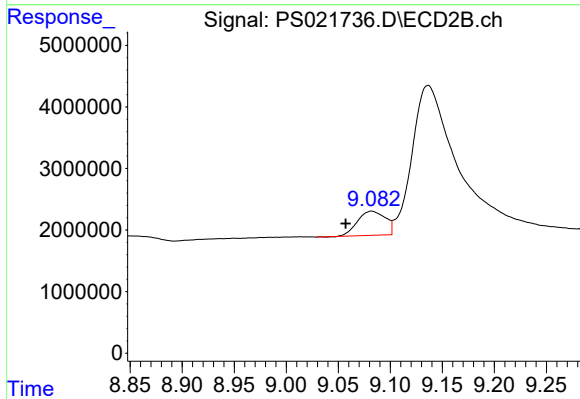

#12 2,4,5-T


R.T.: 9.082 min
Delta R.T.: 0.025 min
Response: 7323988
Conc: N.D.

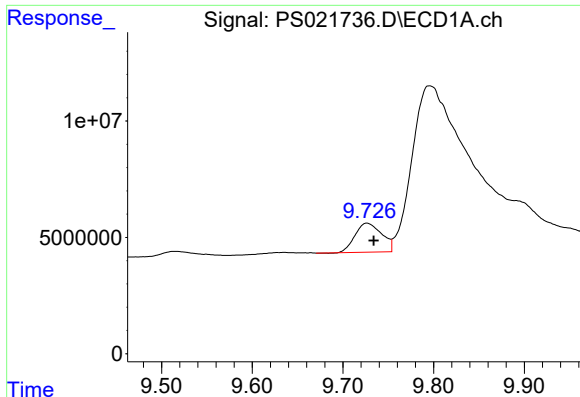

#15 Picloram


R.T.: 9.727 min
Delta R.T.: -0.007 min
Response: 25518997
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

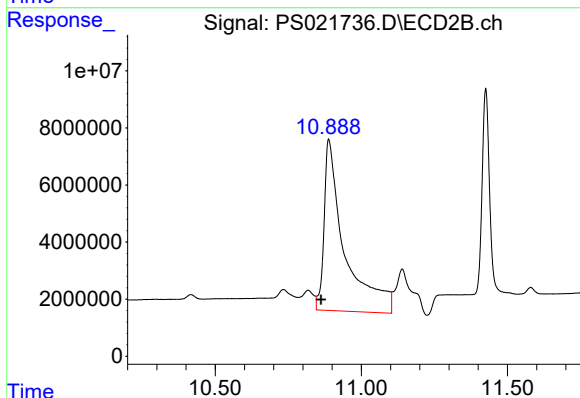


#15 Picloram

R.T.: 10.889 min
Delta R.T.: 0.027 min
Response: 290653551
Conc: 16.41 ng/ml

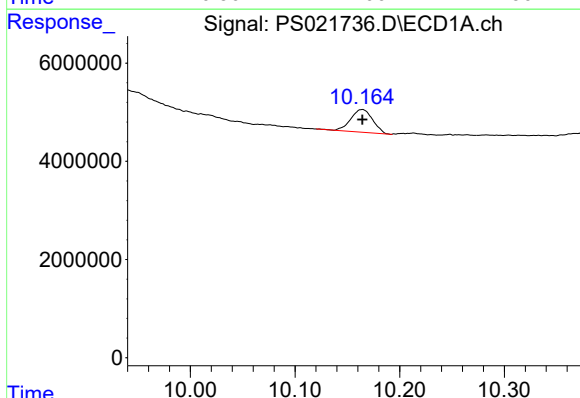

#16 DCPA

R.T.: 10.164 min
Delta R.T.: 0.000 min
Response: 6788361
Conc: N.D.

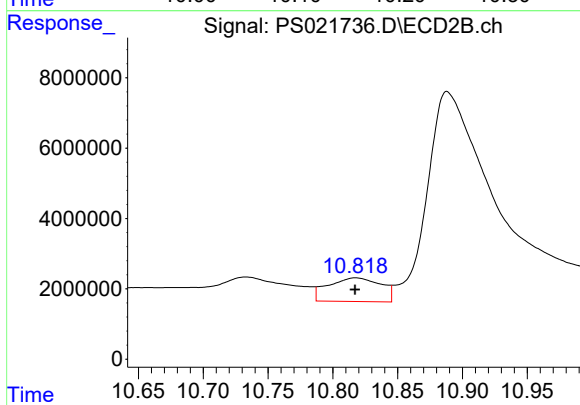

#16 DCPA

R.T.: 10.818 min
Delta R.T.: 0.000 min
Response: 19117683
Conc: 1.37 ng/ml