

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS011224\
 Data File : PS025504.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Jan 2024 09:08
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 13 20:13:55 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS011124.M
 Quant Title : 8080.M
 QLast Update : Thu Jan 11 16:45:24 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds						
1) T	Dalapon	0.000	2.562	0	3215556	N.D. 2.737
2) T	3,5-DICHL...	5.693	0.000	5751508	0	2.513 N.D. #
3) T	4-Nitroph...	0.000	6.362	0	458484	N.D. <MDL
5) T	DICAMBA	0.000	6.959	0	7701836	N.D. 2.314
6) T	MCP	0.000	6.959f	0	7701836	N.D. 3.320
7) T	MCPA	0.000	7.223	0	1627384	N.D. <MDL
8) T	DICHLORPROP	0.000	7.568	0	3147567	N.D. 3.641
9) T	2,4-D	7.249	0.000	26478938	0	14.380 N.D. #
11) T	2,4,5-TP ...	0.000	8.603	0	221714	N.D. <MDL
12) T	2,4,5-T	0.000	8.988	0	981689	N.D. <MDL
13) T	2,4-DB	0.000	9.478	0	815467	N.D. 1.562
14) T	DINOSEB	0.000	9.795	0	517563	N.D. <MDL
15) T	Picloram	9.661	10.782	11198500	5984355	1.082 1.126
16) T	DCPA	0.000	10.718	0	663977	N.D. <MDL



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS011224\
Data File : PS025504.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Jan 2024 09:08
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 13 20:13:55 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS011124.M
Quant Title : 8080.M
QLast Update : Thu Jan 11 16:45:24 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

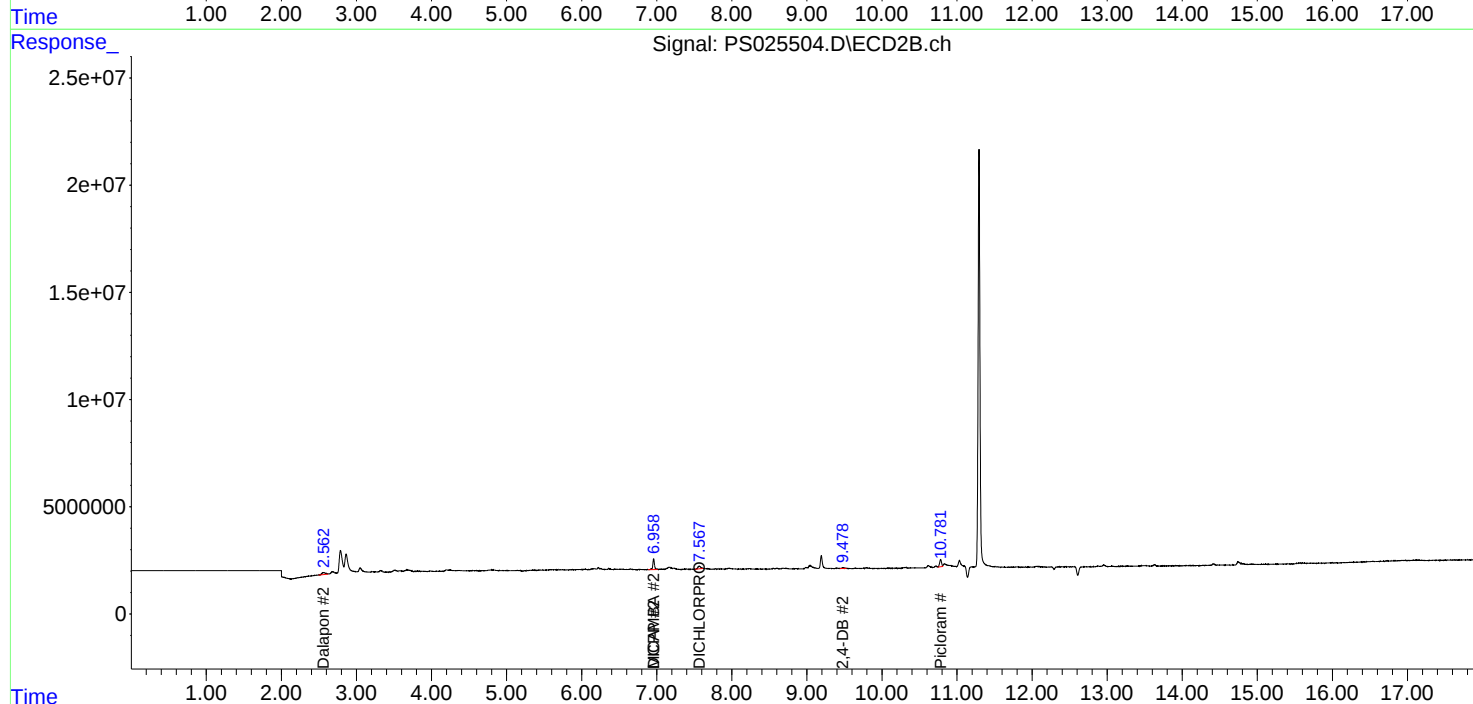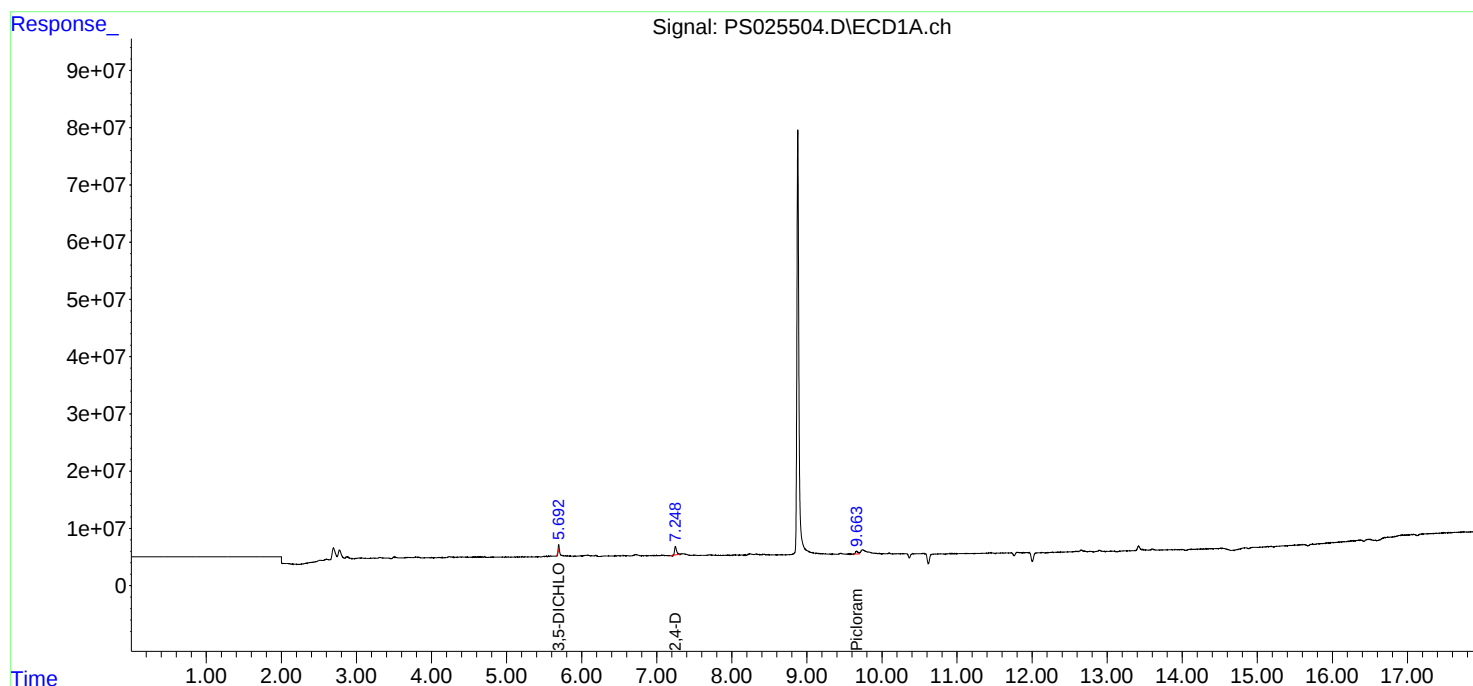


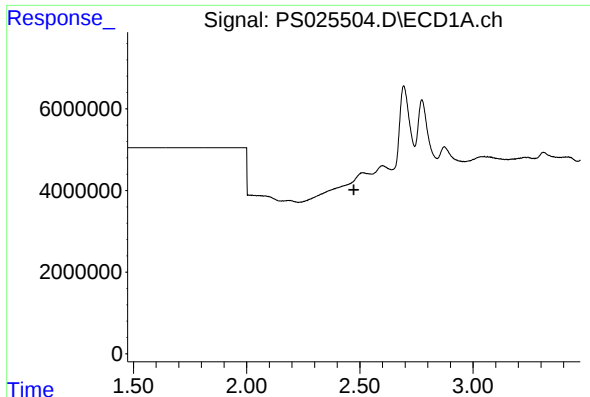

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.474 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

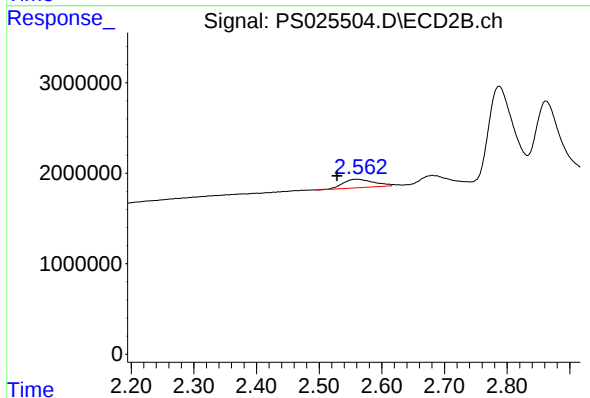


#1 Dalapon

R.T.: 2.562 min
Delta R.T.: 0.034 min
Response: 3215556
Conc: 2.74 ng/ml

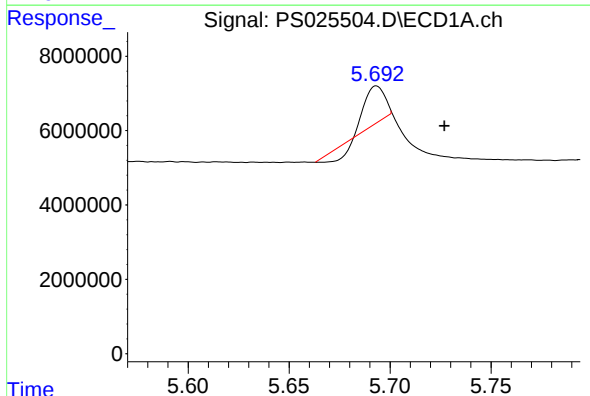


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 5.693 min
Delta R.T.: -0.033 min
Response: 5751508
Conc: 2.51 ng/ml

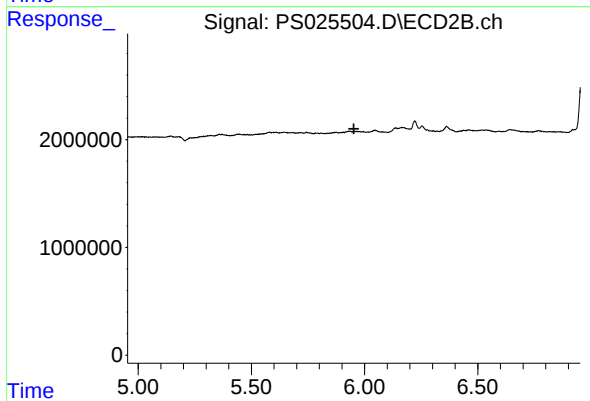

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 5.953 min
Response: 0
Conc: N.D.

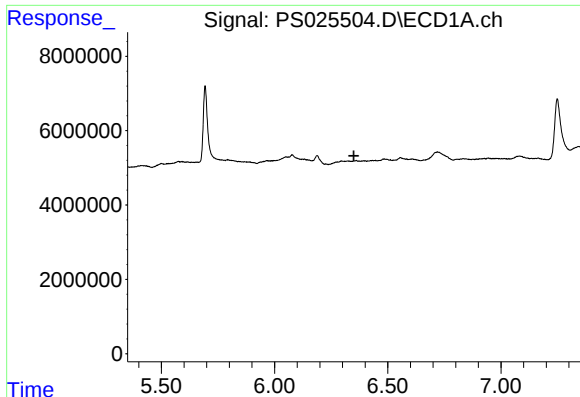

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T. : 6.350 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

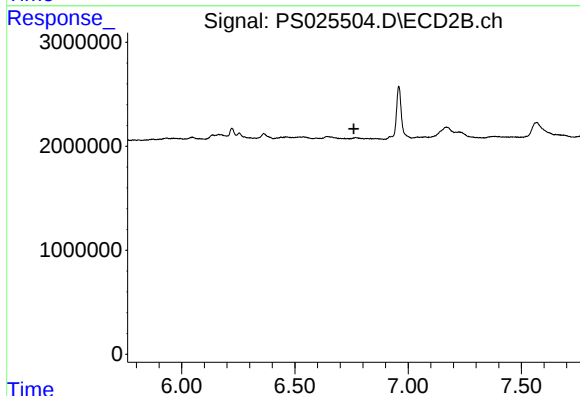


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 6.761 min
Response: 0
Conc: N.D.

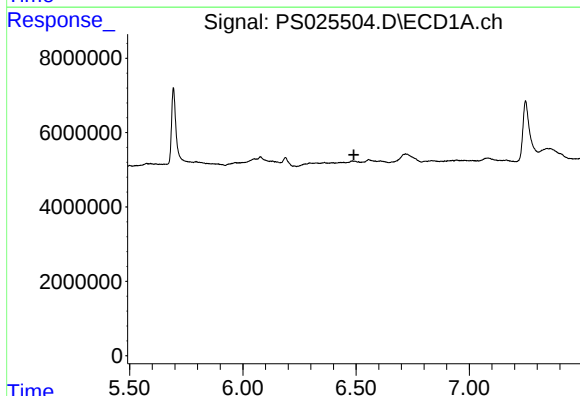


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 6.491 min
Response: 0
Conc: N.D.

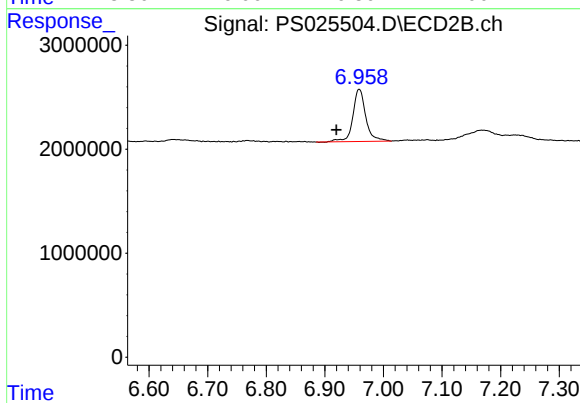

#5 DICAMBA


R.T.: 6.959 min
Delta R.T.: 0.039 min
Response: 7701836
Conc: 2.31 ng/ml

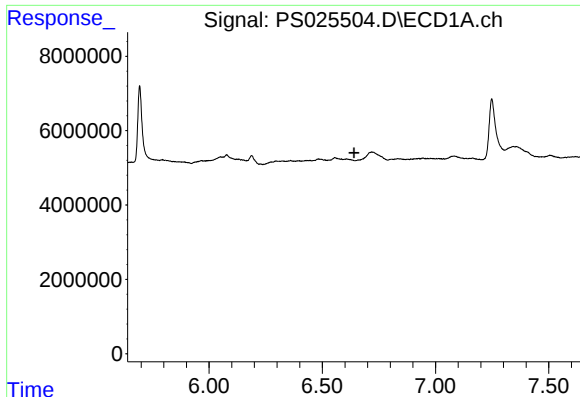

#6 MCP


R.T.: 0.000 min
Exp R.T.: 6.640 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

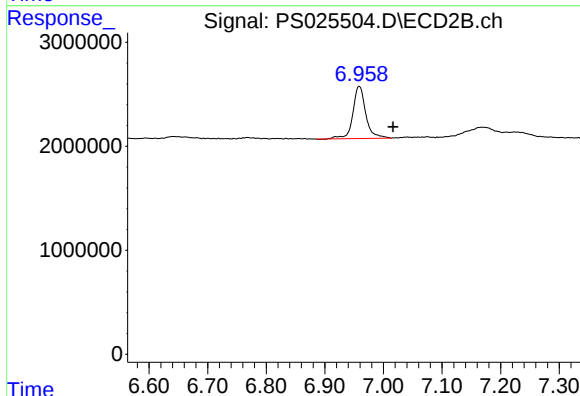


#6 MCP

R.T.: 6.959 min
Delta R.T.: -0.058 min
Response: 7701836
Conc: 3.32 ug/ml

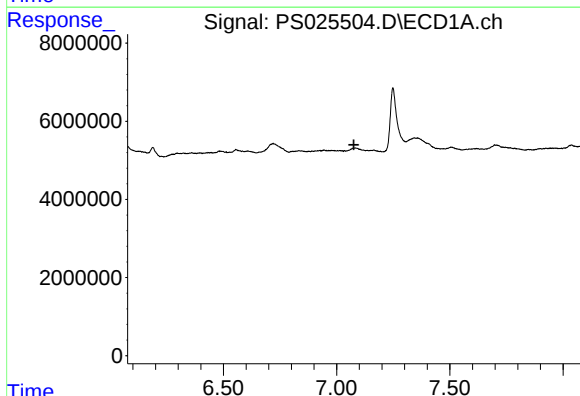


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 7.077 min
Response: 0
Conc: N.D.

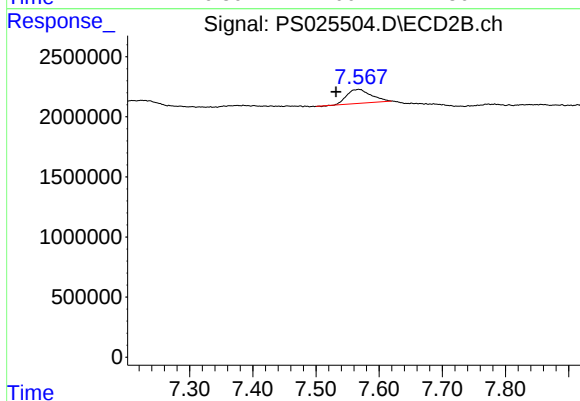

#8 DICHLORPROP


R.T.: 7.568 min
Delta R.T.: 0.036 min
Response: 3147567
Conc: 3.64 ng/ml

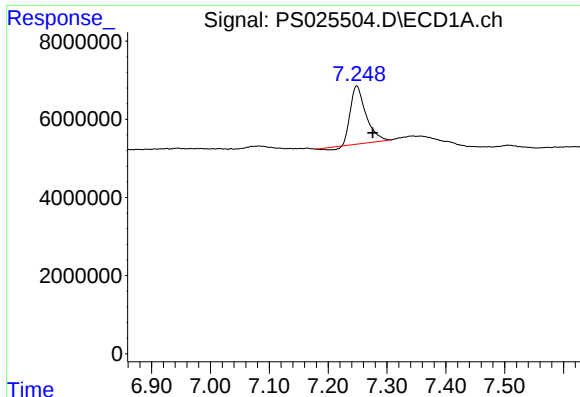

#9 2,4-D


R.T.: 7.249 min
Delta R.T.: -0.027 min
Response: 26478938
Conc: 14.38 ng/ml

Instrument :
ECD_S
ClientSampleId :
HEXANE

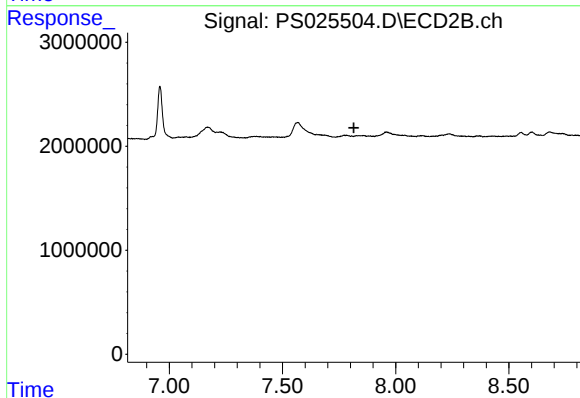


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 7.815 min
Response: 0
Conc: N.D.

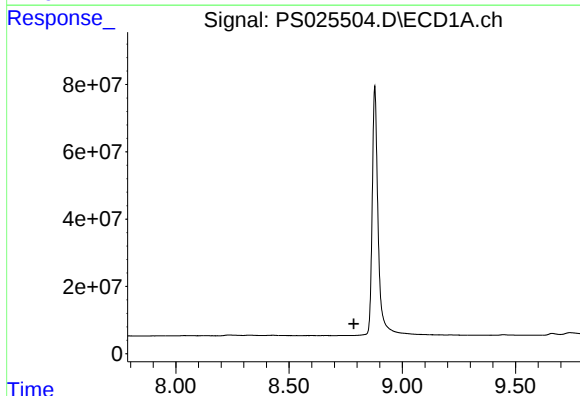


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 8.786 min
Response: 0
Conc: N.D.

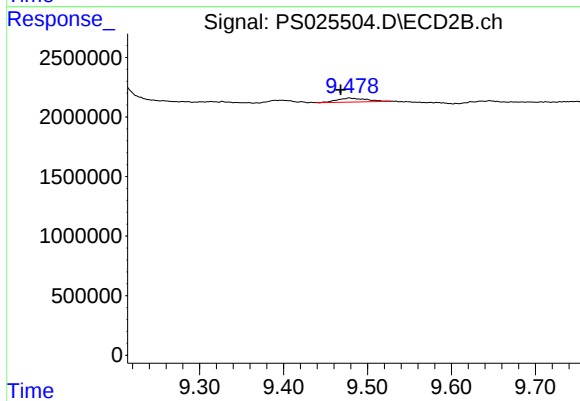

#13 2,4-DB


R.T.: 9.478 min
Delta R.T.: 0.010 min
Response: 815467
Conc: 1.56 ng/ml

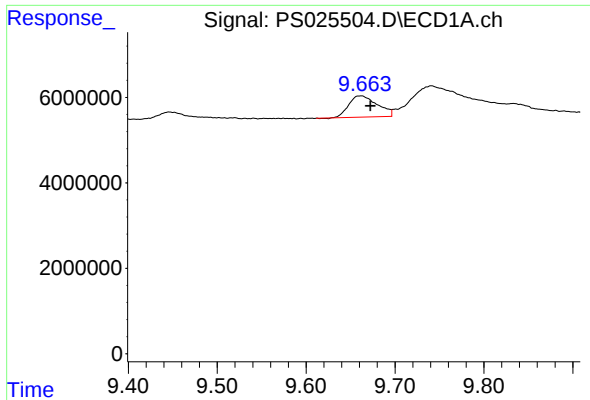

#15 Picloram

R.T.: 9.661 min
Delta R.T.: -0.011 min
Response: 11198500
Conc: 1.08 ng/ml

Instrument :
ECD_S
ClientSampleId :
HEXANE

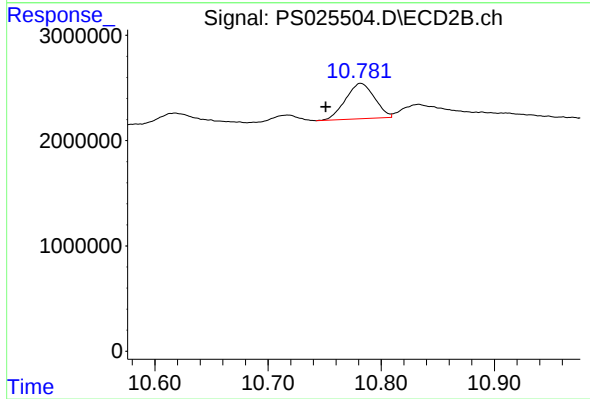

#15 Picloram

R.T.: 10.782 min
Delta R.T.: 0.031 min
Response: 5984355
Conc: 1.13 ng/ml