

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS011224\
 Data File : PS025508.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Jan 2024 11:09
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 13 20:15:28 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS011124.M
 Quant Title : 8080.M
 QLast Update : Thu Jan 11 16:45:24 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.352	6.761	775.5E6	407.4E6	520.656	530.639
Target Compounds							
1) T	Dalapon	0.000	2.561	0	2867223	N.D.	2.441
2) T	3,5-DICHL...	5.694	0.000	1944701	0	<MDL	N.D. #
5) T	DICAMBA	0.000	6.958	0	1532201	N.D.	<MDL
6) T	MCP	0.000	6.958f	0	1532201	N.D.	<MDL
7) T	MCPA	0.000	7.229	0	3032477	N.D.	<MDL
8) T	DICHLORPROP	0.000	7.567	0	1824852	N.D.	2.111
12) T	2,4,5-T	0.000	8.997	0	514205	N.D.	<MDL
13) T	2,4-DB	0.000	9.491	0	507254	N.D.	<MDL
14) T	DINOSEB	0.000	9.801	0	458738	N.D.	<MDL
15) T	Picloram	0.000	10.718	0	590571	N.D.	<MDL
16) T	DCPA	0.000	10.718	0	590571	N.D.	<MDL



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS011224\
Data File : PS025508.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Jan 2024 11:09
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 13 20:15:28 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS011224.M
Quant Title : 8080.M
QLast Update : Thu Jan 11 16:45:24 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

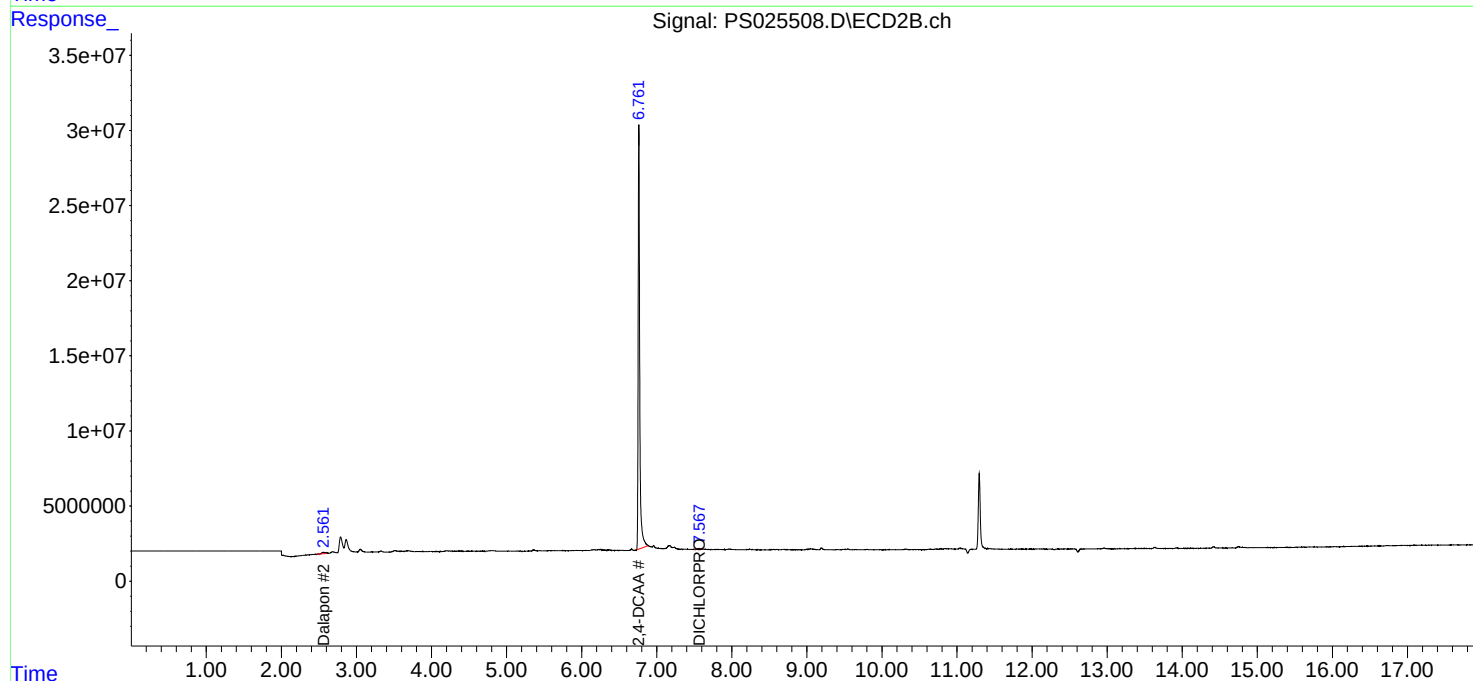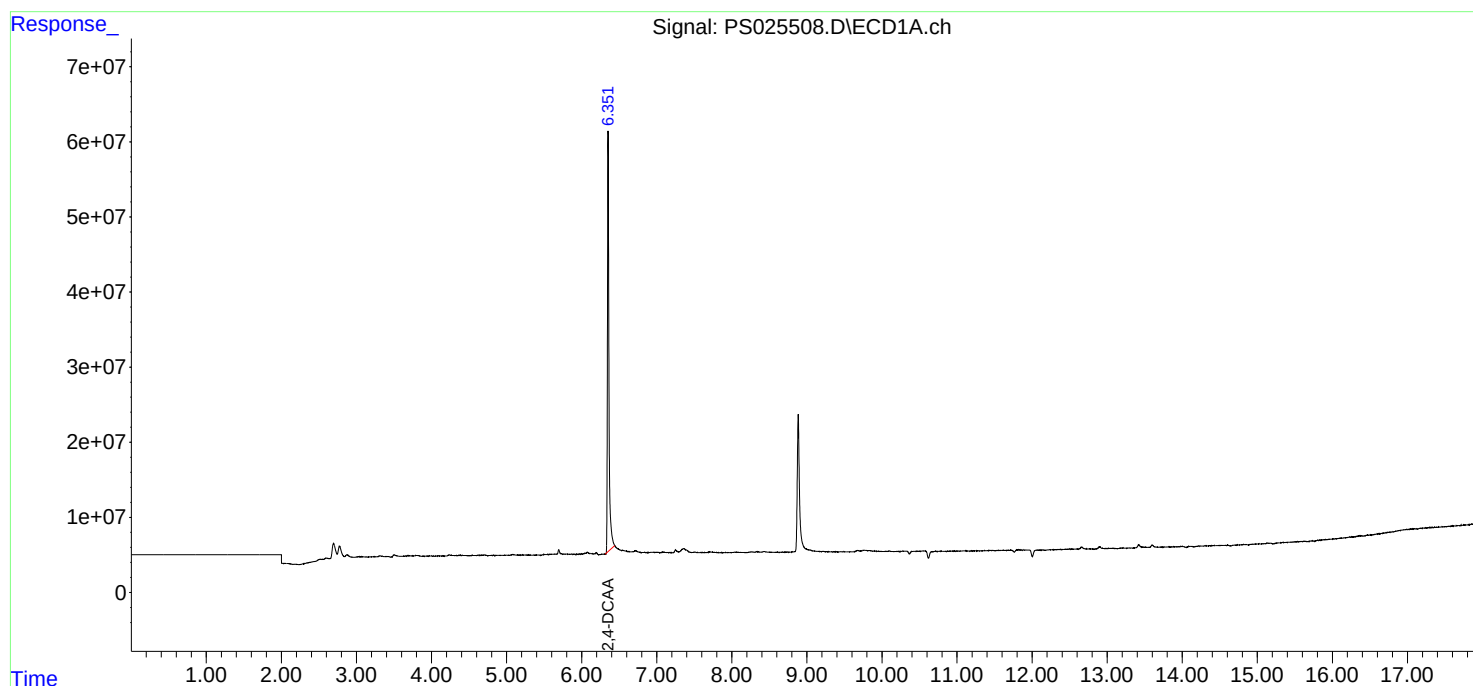


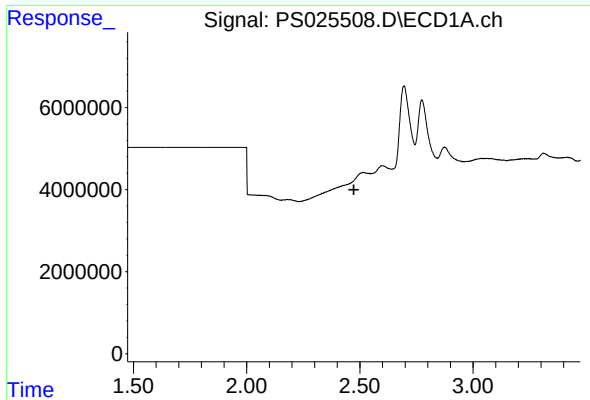

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.474 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

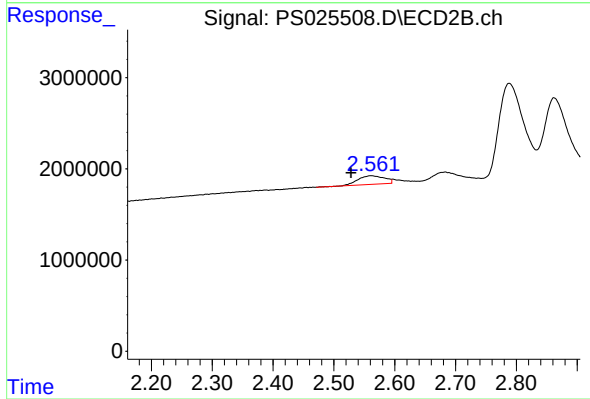


#1 Dalapon

R.T.: 2.561 min
Delta R.T.: 0.032 min
Response: 2867223
Conc: 2.44 ng/ml

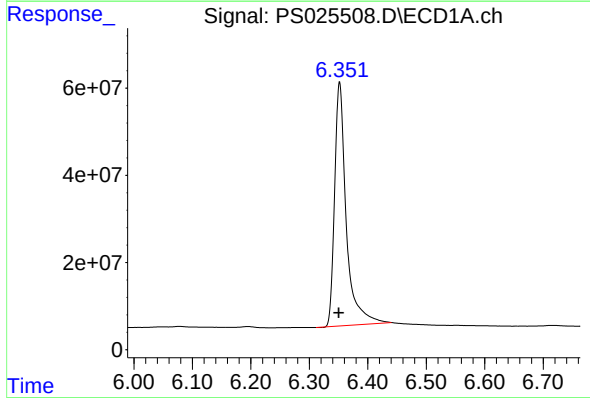


#4 2,4-DCAA

R.T.: 6.352 min
Delta R.T.: 0.002 min
Response: 775497399
Conc: 520.66 ng/ml

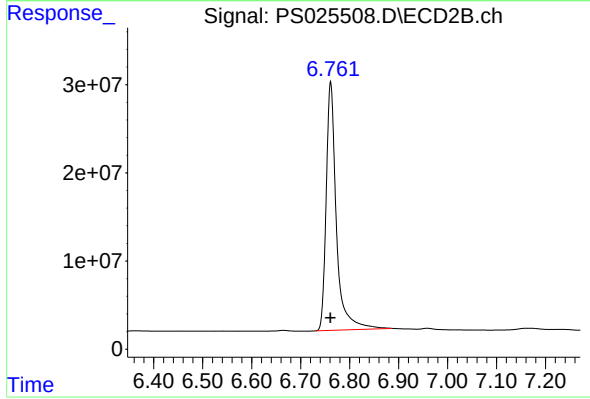

#4 2,4-DCAA


R.T.: 6.761 min
Delta R.T.: 0.000 min
Response: 407424562
Conc: 530.64 ng/ml

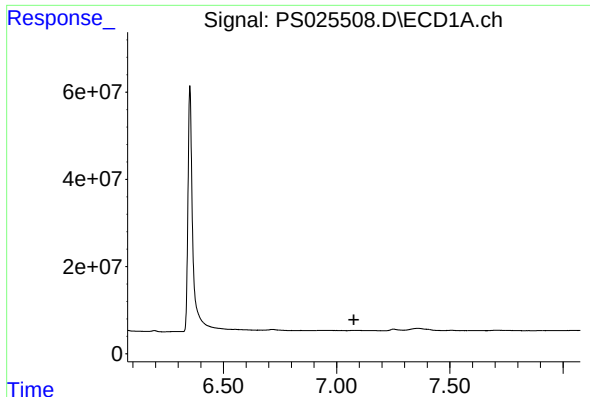

#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 7.077 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

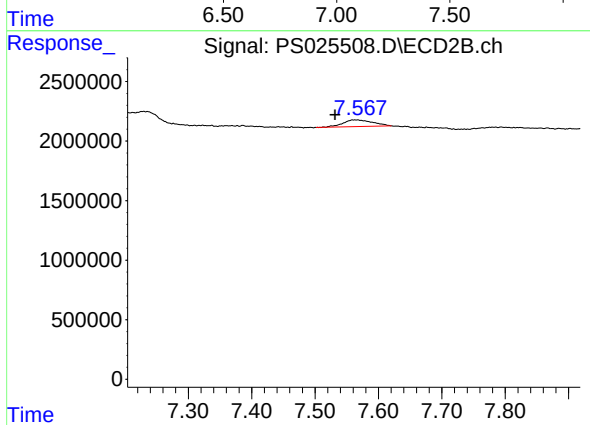

#8 DICHLORPROP

R.T.: 7.567 min
Delta R.T.: 0.036 min
Response: 1824852
Conc: 2.11 ng/ml