

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS011224\
 Data File : PS025517.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Jan 2024 20:02
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 13 20:19:06 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS011124.M
 Quant Title : 8080.M
 QLast Update : Thu Jan 11 16:45:24 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.352	6.761	772.4E6	408.7E6	518.567	532.291
Target Compounds							
1) T	Dalapon	0.000	2.559	0	2027118	N.D.	1.725
3) T	4-Nitroph...	0.000	6.367	0	999188	N.D.	2.099
5) T	DICAMBA	0.000	6.959	0	1634314	N.D.	<MDL
6) T	MCP	0.000	6.959f	0	1634314	N.D.	<MDL
7) T	MCPA	0.000	7.237	0	1976015	N.D.	<MDL
8) T	DICHLORPROP	0.000	7.560	0	4413249	N.D.	5.105
9) T	2,4-D	7.250	0.000	9817153	0	5.331	N.D. #
10) T	Pentachlo...	0.000	8.237	0	888888	N.D.	<MDL
12) T	2,4,5-T	0.000	8.993	0	611224	N.D.	<MDL
13) T	2,4-DB	0.000	9.478	0	795888	N.D.	1.525
15) T	Picloram	0.000	10.782	0	1946085	N.D.	<MDL
16) T	DCPA	0.000	10.717	0	1406116	N.D.	<MDL



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS011224\
Data File : PS025517.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Jan 2024 20:02
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 13 20:19:06 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS011124.M
Quant Title : 8080.M
QLast Update : Thu Jan 11 16:45:24 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

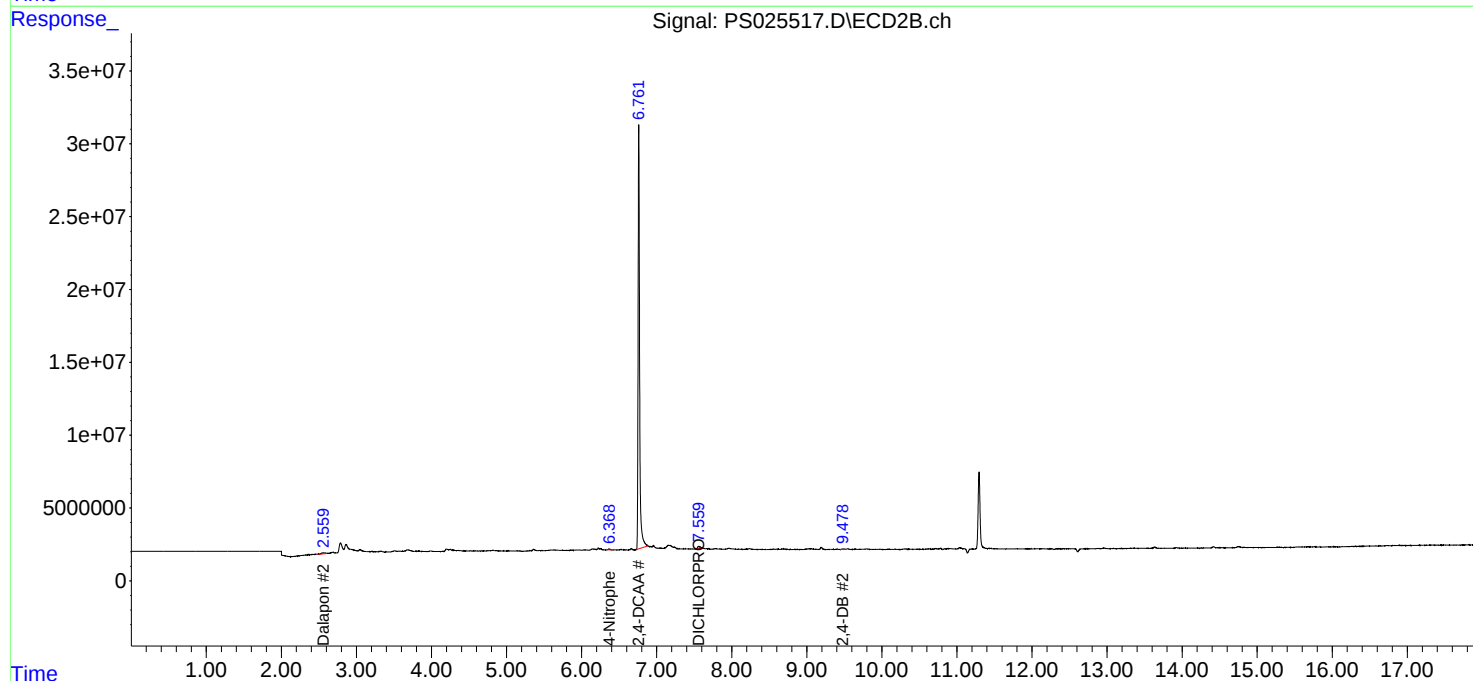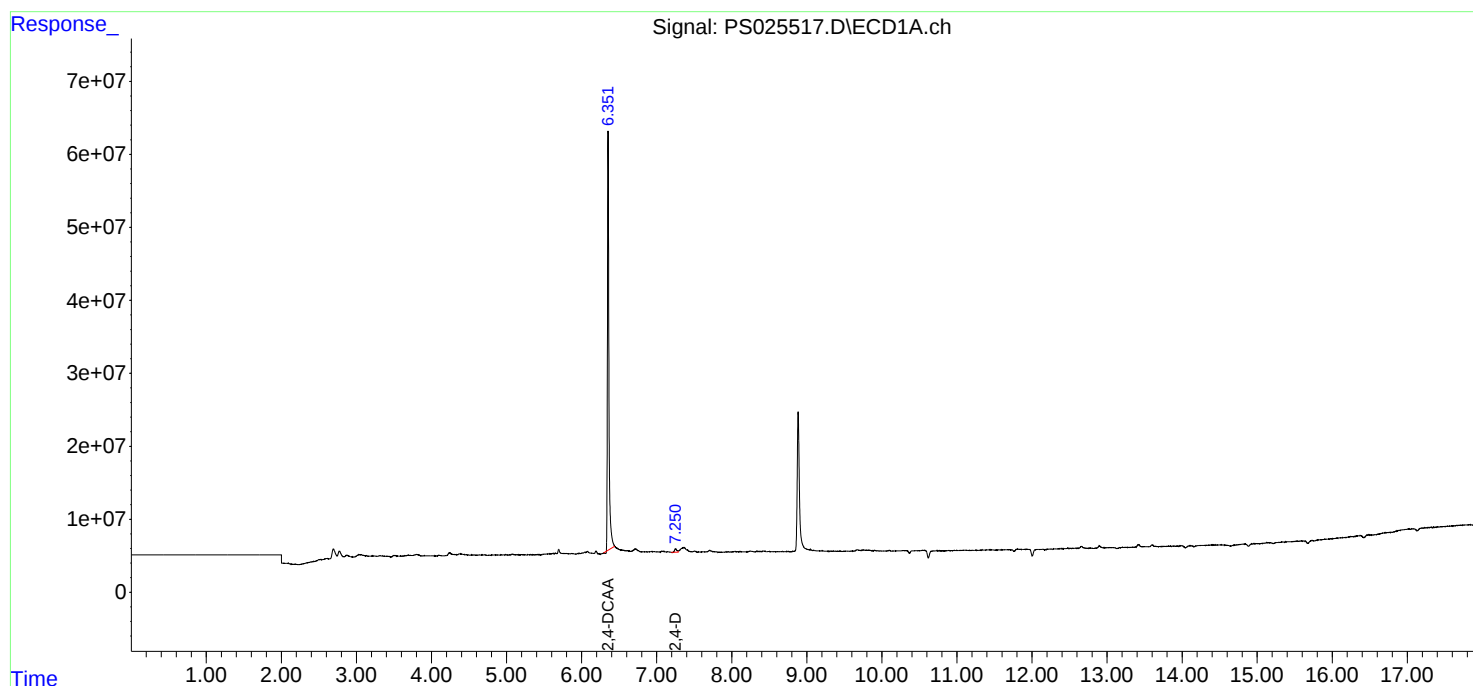


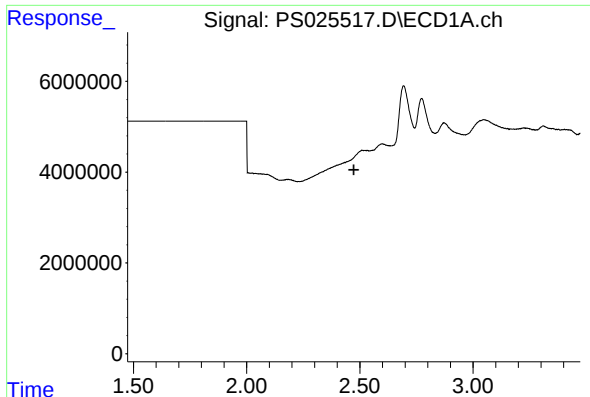

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.474 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

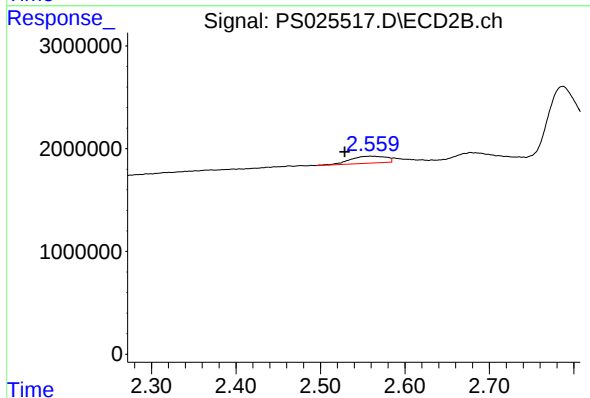


#1 Dalapon

R.T.: 2.559 min
Delta R.T.: 0.031 min
Response: 2027118
Conc: 1.73 ng/ml

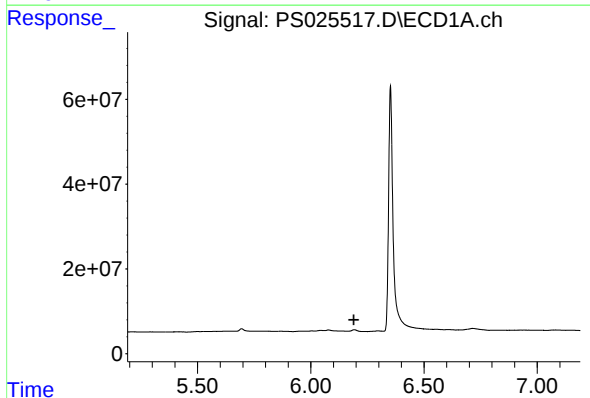


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T.: 6.191 min
Response: 0
Conc: N.D.

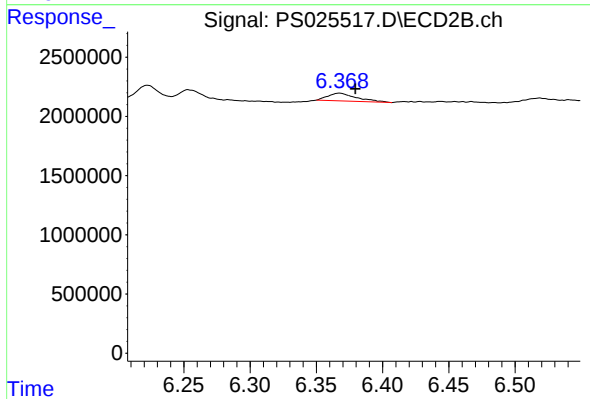

#3 4-Nitrophenol


R.T.: 6.367 min
Delta R.T.: -0.012 min
Response: 999188
Conc: 2.10 ng/ml

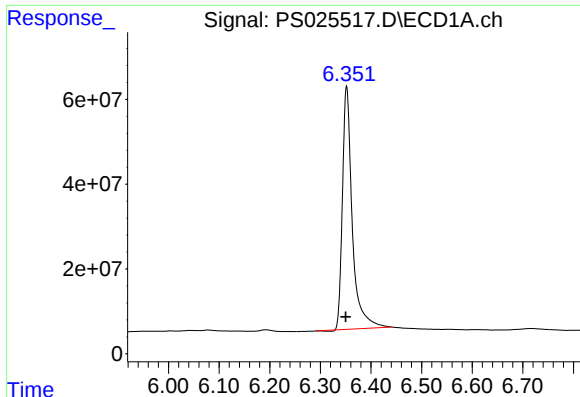

#4 2,4-DCAA


R.T.: 6.352 min
Delta R.T.: 0.002 min
Response: 772386298
Conc: 518.57 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

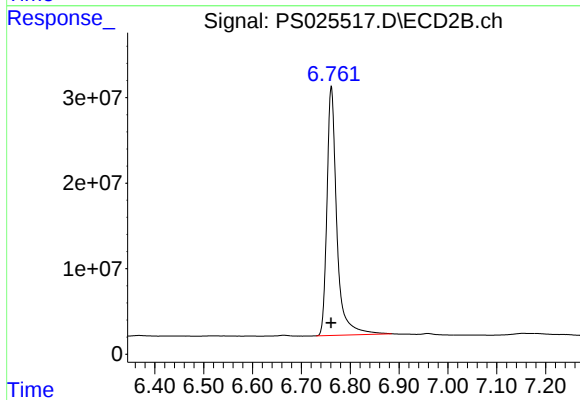


#4 2,4-DCAA

R.T.: 6.761 min
Delta R.T.: 0.000 min
Response: 408693173
Conc: 532.29 ng/ml

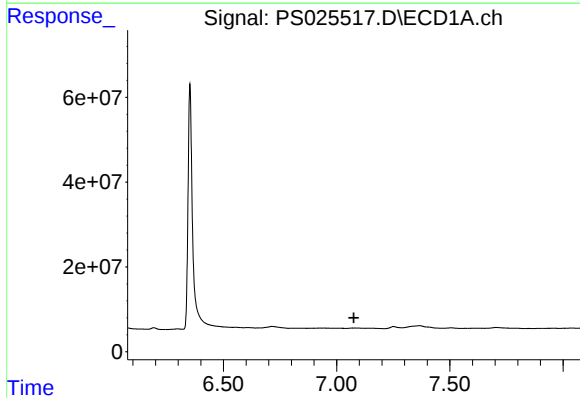


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 7.077 min
Response: 0
Conc: N.D.

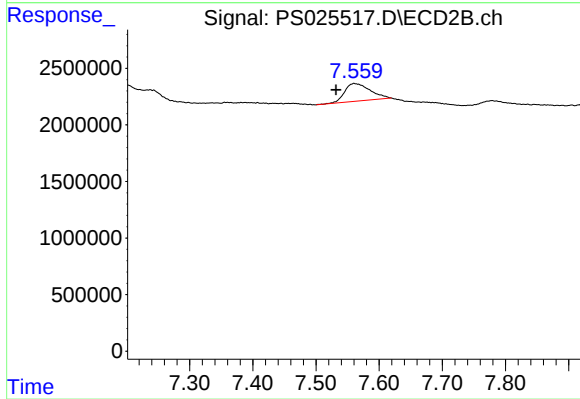

#8 DICHLORPROP


R.T.: 7.560 min
Delta R.T.: 0.029 min
Response: 4413249
Conc: 5.11 ng/ml

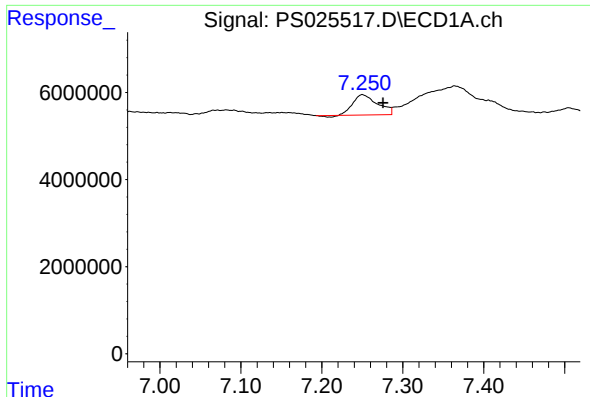

#9 2,4-D


R.T.: 7.250 min
Delta R.T.: -0.025 min
Response: 9817153
Conc: 5.33 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

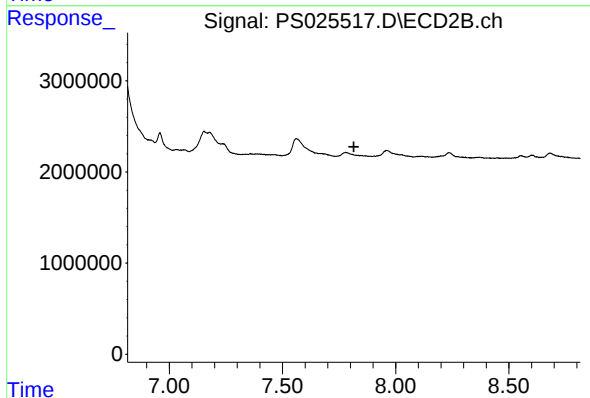


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 7.815 min
Response: 0
Conc: N.D.

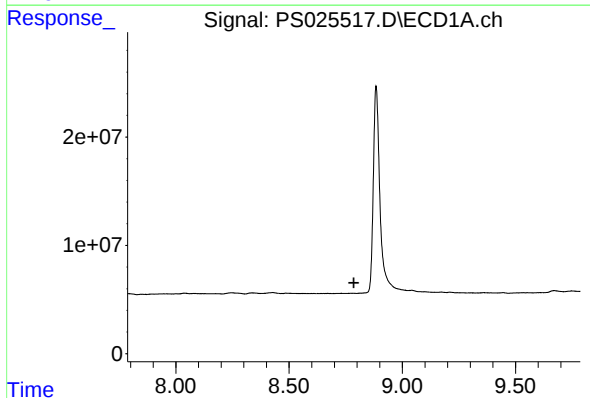

#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 8.786 min
Response: 0
Conc: N.D.

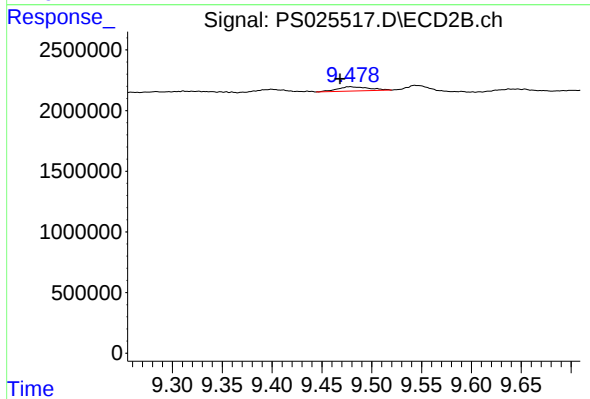

#13 2,4-DB

R.T.: 9.478 min
Delta R.T.: 0.010 min
Response: 795888
Conc: 1.52 ng/ml