

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS011320\
 Data File : PS008388.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Jan 2020 09:58
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 13 13:10:12 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010820.M
 Quant Title : 8080.M
 QLast Update : Wed Jan 08 11:00:59 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.275	5.969	991.5E6	501.4E6	561.512	529.198
Target Compounds							
6) T	MCP	0.000	6.232	0	8088069	N.D.	2.660
9) T	2,4-D	7.442	0.000	142.7E6	0	78.461	N.D. #
12) T	2,4,5-T	0.000	8.283	0	19154955	N.D.	3.622
15) T	Picloram	10.059	10.056	137.3E6	79353255	11.001	10.681
16) T	DCPA	0.000	10.056	0	79353255	N.D.	12.177



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS011320\
Data File : PS008388.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Jan 2020 09:58
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 13 13:10:12 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010820.M
Quant Title : 8080.M
QLast Update : Wed Jan 08 11:00:59 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

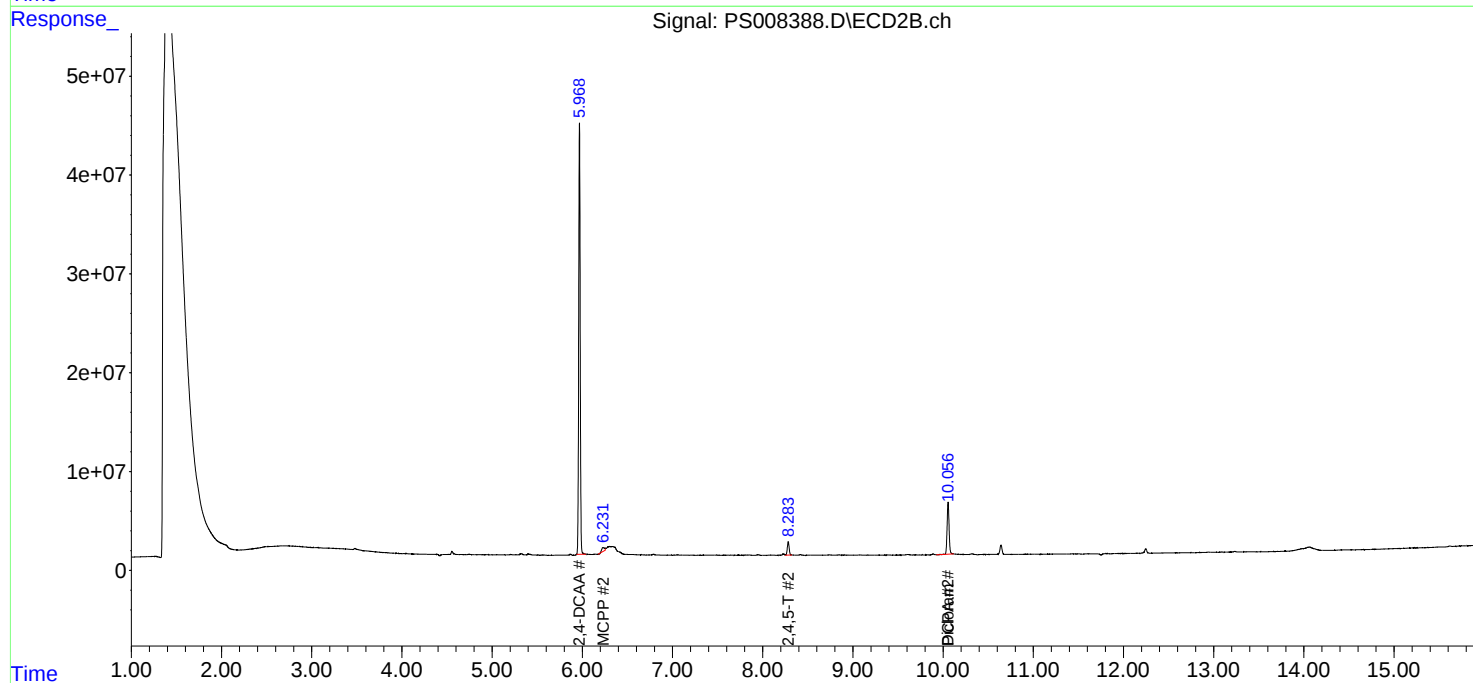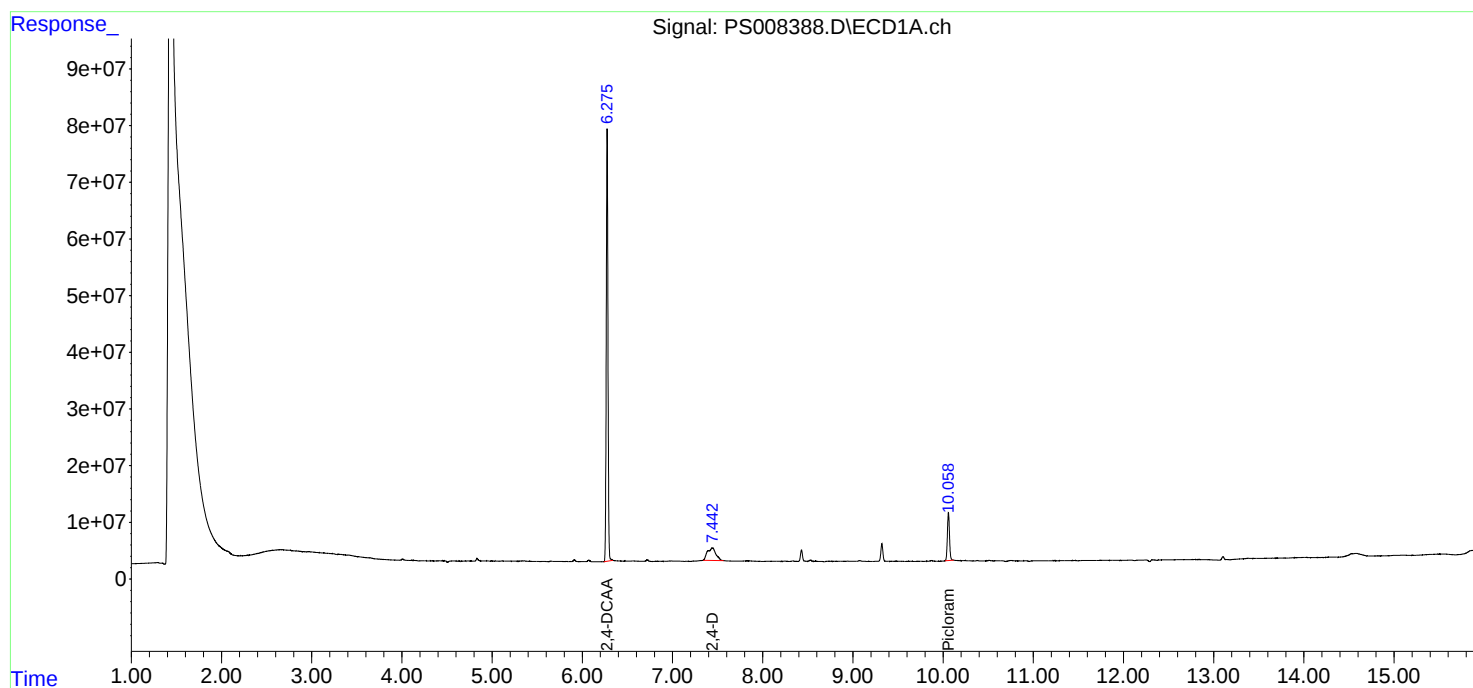


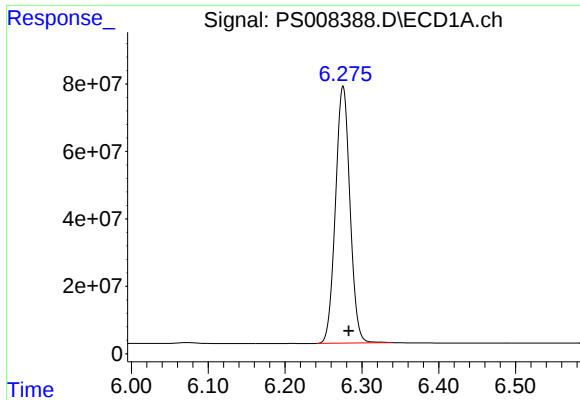

#4 2,4-DCAA


R.T.: 6.275 min
Delta R.T.: -0.007 min
Response: 991462962
Conc: 561.51 ng/ml

Instrument :
ECD_S
ClientSampleId :

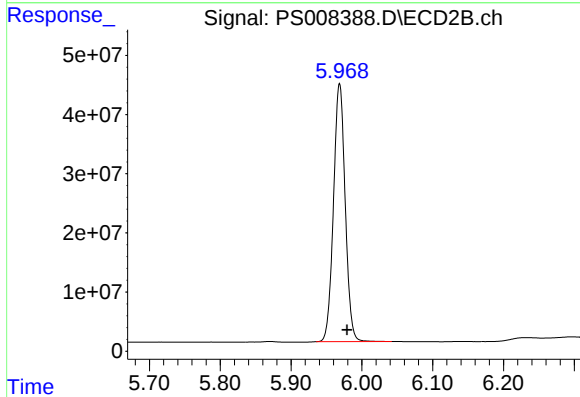


#4 2,4-DCAA

R.T.: 5.969 min
Delta R.T.: -0.011 min
Response: 501395631
Conc: 529.20 ng/ml

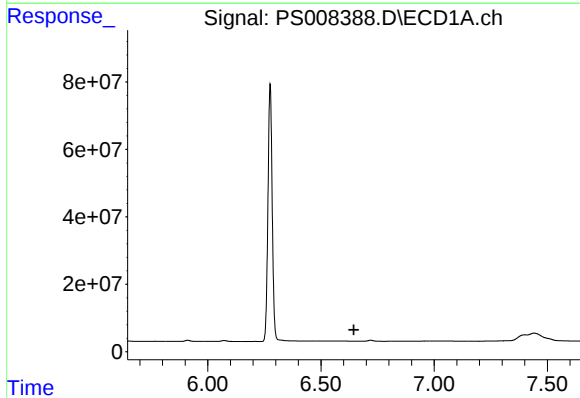


#6 MCP

R.T.: 0.000 min
Exp R.T. : 6.645 min
Response: 0
Conc: N.D.

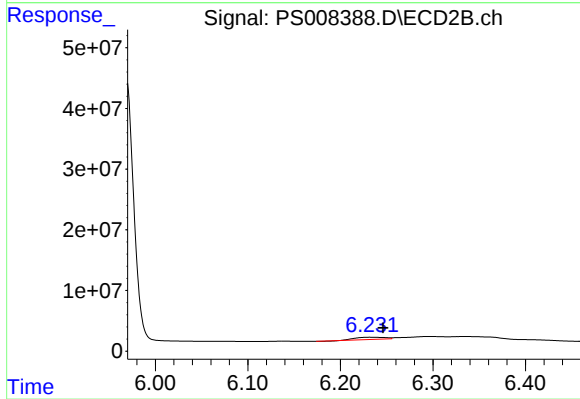

#6 MCP


R.T.: 6.232 min
Delta R.T.: -0.014 min
Response: 8088069
Conc: 2.66 ug/ml

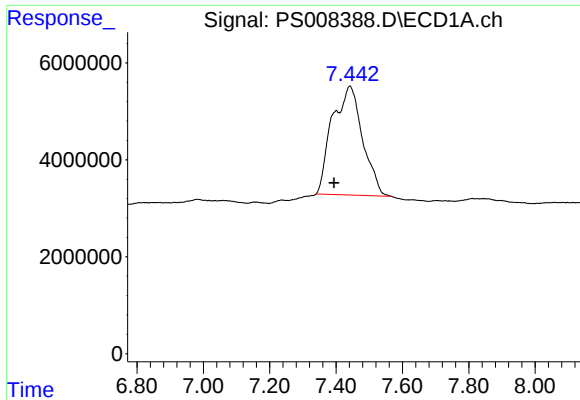

#9 2,4-D


R.T.: 7.442 min
Delta R.T.: 0.048 min
Response: 142728977
Conc: 78.46 ng/ml

Instrument :
ECD_S
ClientSampleId :

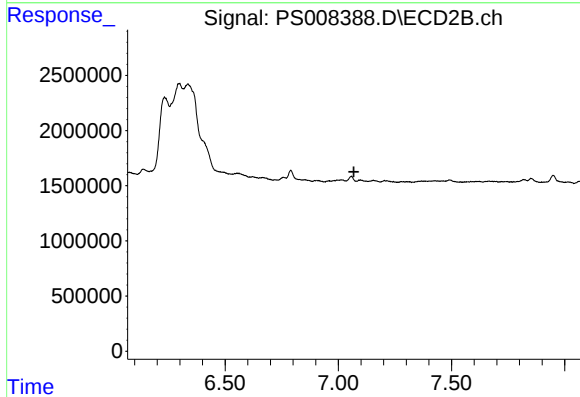


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 7.069 min
Response: 0
Conc: N.D.

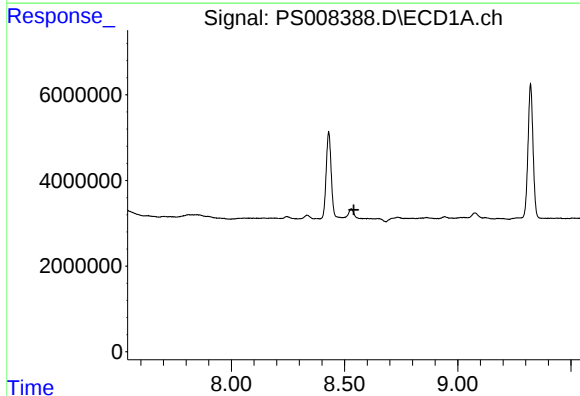


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 8.541 min
Response: 0
Conc: N.D.

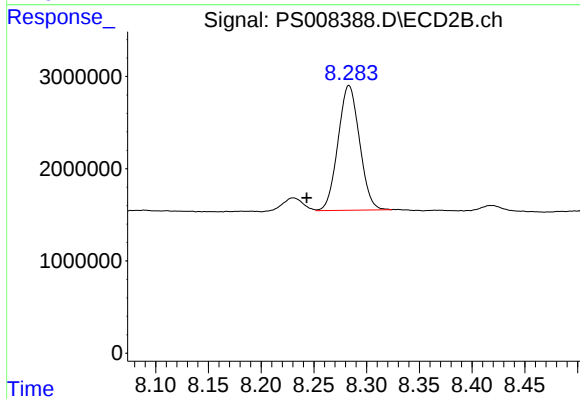

#12 2,4,5-T


R.T.: 8.283 min
Delta R.T.: 0.040 min
Response: 19154955
Conc: 3.62 ng/ml

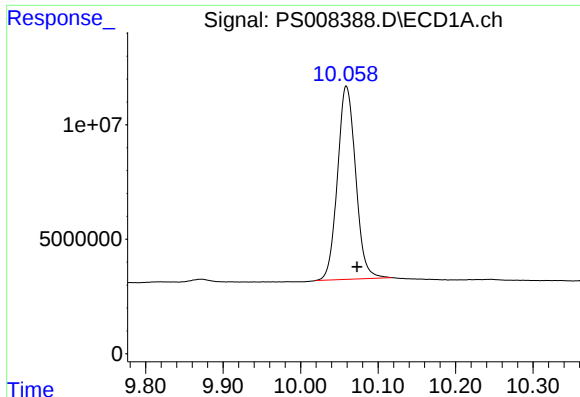

#15 Picloram


R.T.: 10.059 min
Delta R.T.: -0.014 min
Response: 137306090
Conc: 11.00 ng/ml

Instrument :
ECD_S
ClientSampleId :

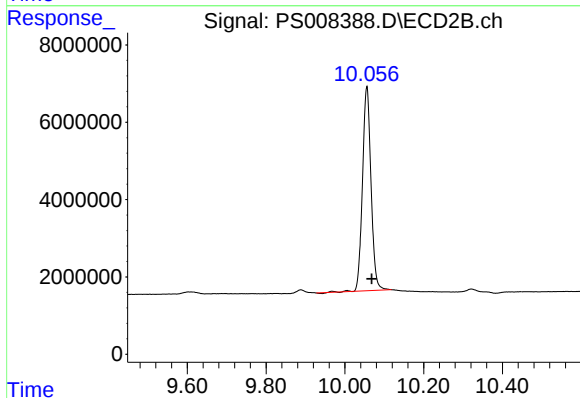


#15 Picloram

R.T.: 10.056 min
Delta R.T.: -0.012 min
Response: 79353255
Conc: 10.68 ng/ml

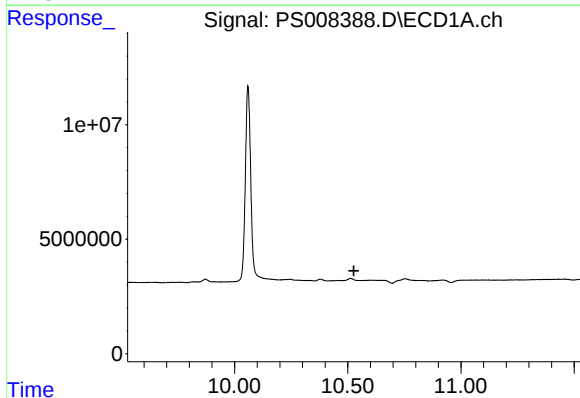

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 10.527 min
Response: 0
Conc: N.D.

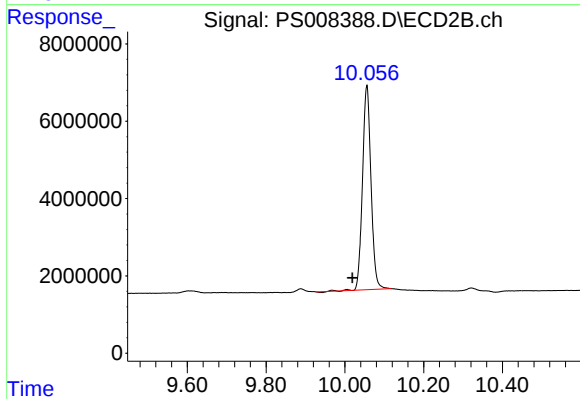

#16 DCPA

R.T.: 10.056 min
Delta R.T.: 0.037 min
Response: 79353255
Conc: 12.18 ng/ml