

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS011320\
 Data File : PS008391.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Jan 2020 12:28
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 13 13:37:03 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010820.M
 Quant Title : 8080.M
 QLast Update : Wed Jan 08 11:00:59 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.285	5.975	970.7E6	482.3E6	549.773	509.014
Target Compounds							
9) T	2,4-D	7.463	0.000	97508148	0	53.602	N.D. #
10) T	Pentachlo...	7.711	7.498	22986681	12877841	<MDL	<MDL #
12) T	2,4,5-T	0.000	8.237	0	9373743	N.D.	1.773
15) T	Picloram	10.066	10.061	347.1E6	195.8E6	27.806	26.349
16) T	DCPA	0.000	10.061	0	195.8E6	N.D.	30.039



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS011320\
Data File : PS008391.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Jan 2020 12:28
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 13 13:37:03 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010820.M
Quant Title : 8080.M
QLast Update : Wed Jan 08 11:00:59 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

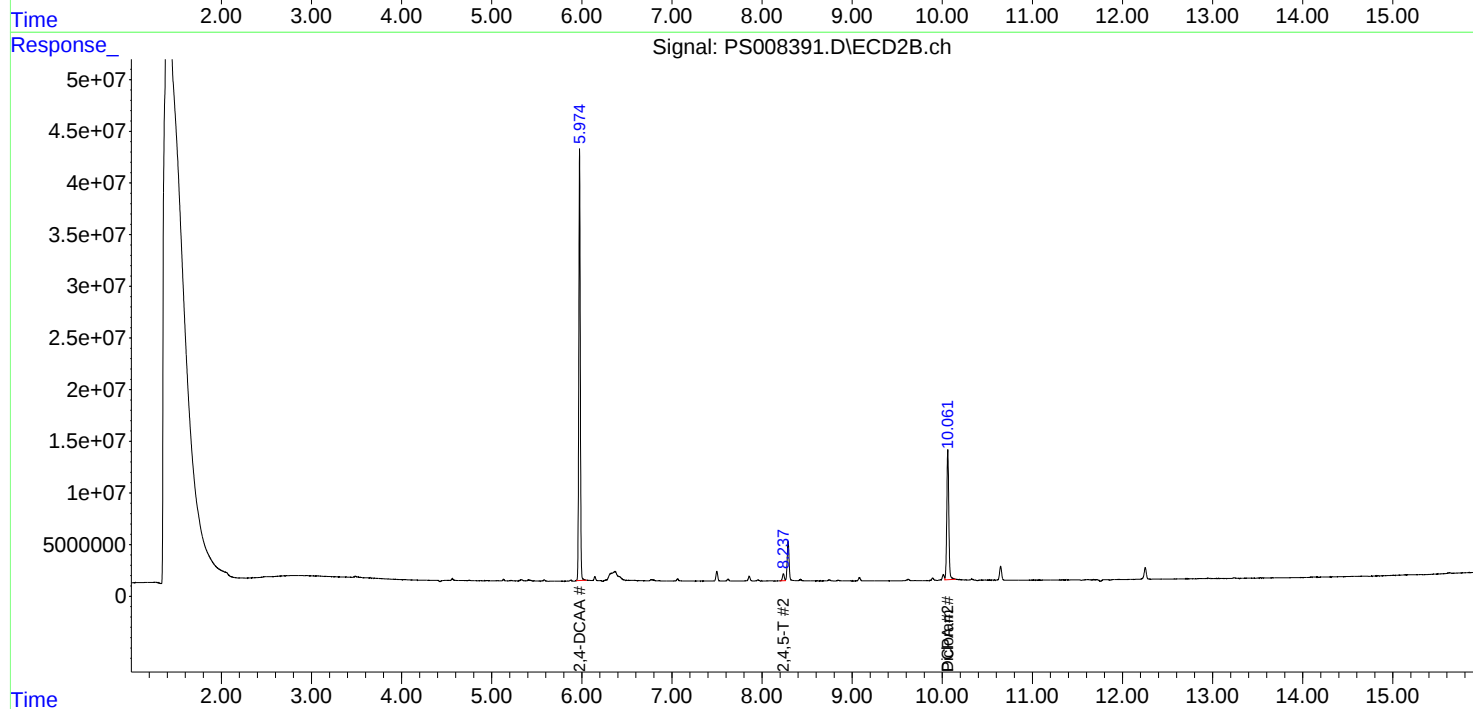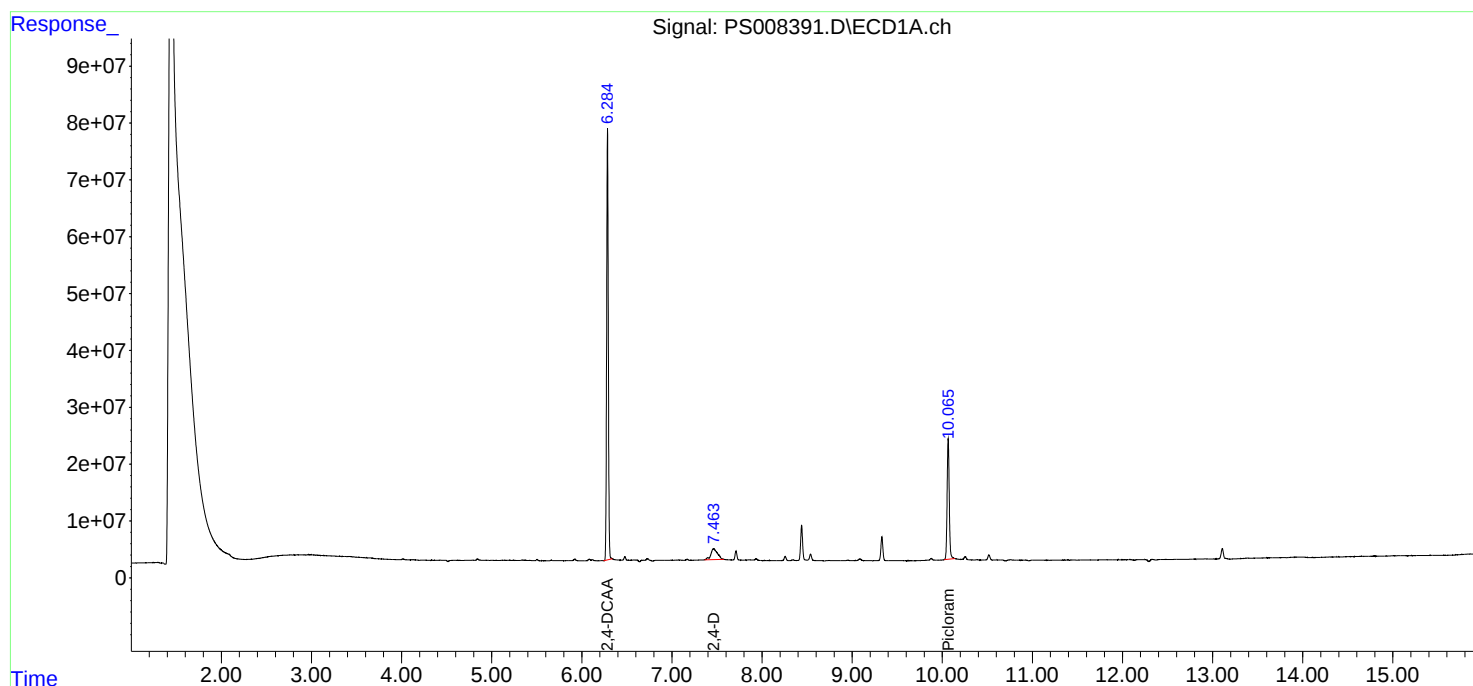


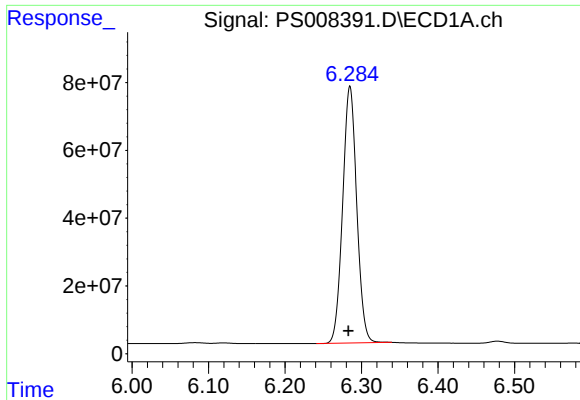

#4 2,4-DCAA


R.T.: 6.285 min
Delta R.T.: 0.002 min
Response: 970737048
Conc: 549.77 ng/ml

Instrument :
ECD_S
ClientSampleId :

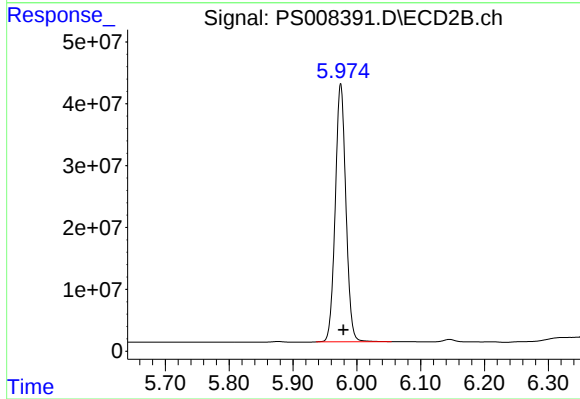


#4 2,4-DCAA

R.T.: 5.975 min
Delta R.T.: -0.004 min
Response: 482271793
Conc: 509.01 ng/ml

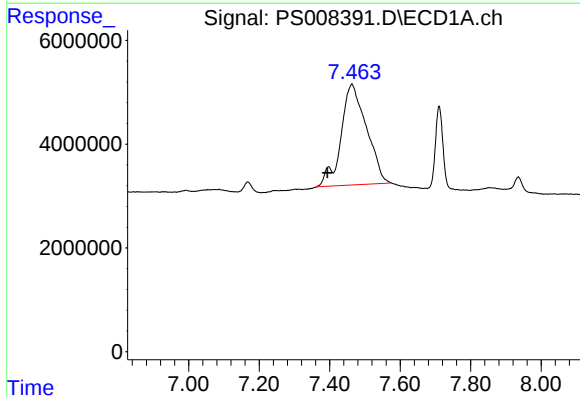


#9 2,4-D

R.T.: 7.463 min
Delta R.T.: 0.069 min
Response: 97508148
Conc: 53.60 ng/ml

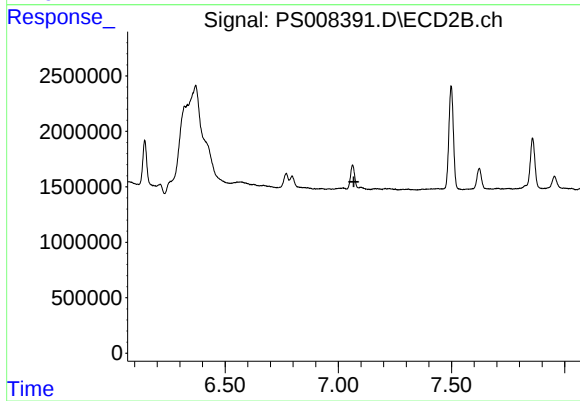

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 7.069 min
Response: 0
Conc: N.D.

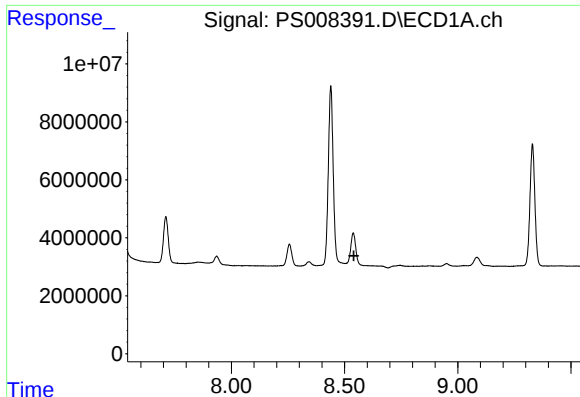

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 8.541 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

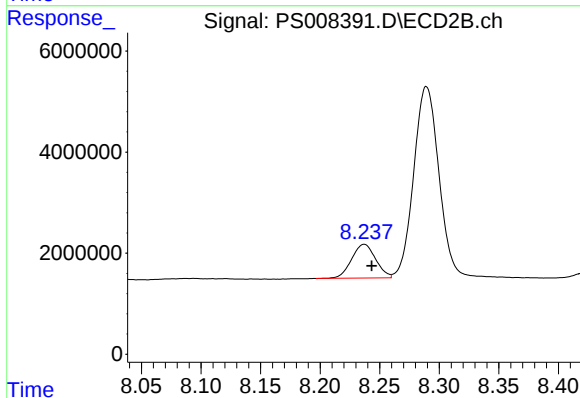


#12 2,4,5-T

R.T.: 8.237 min
Delta R.T.: -0.006 min
Response: 9373743
Conc: 1.77 ng/ml

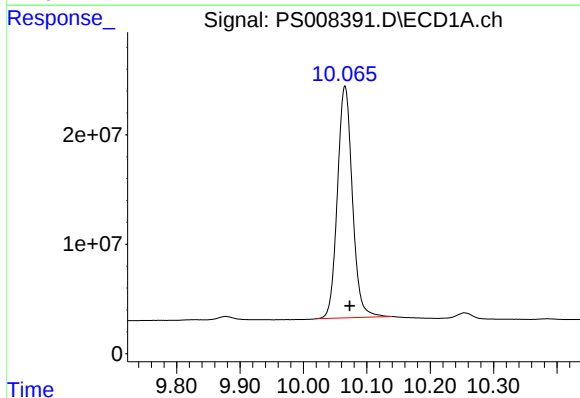


#15 Picloram

R.T.: 10.066 min
Delta R.T.: -0.007 min
Response: 347064981
Conc: 27.81 ng/ml

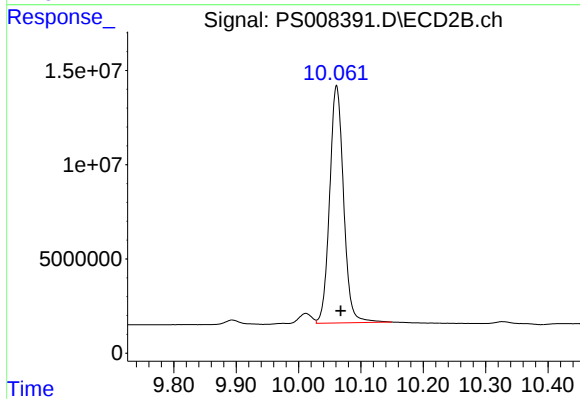

#15 Picloram


R.T.: 10.061 min
Delta R.T.: -0.007 min
Response: 195754987
Conc: 26.35 ng/ml

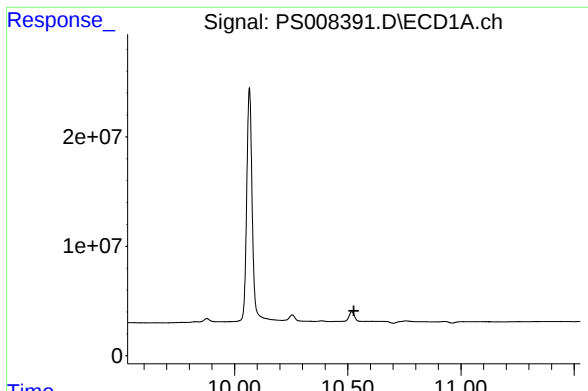

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 10.527 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

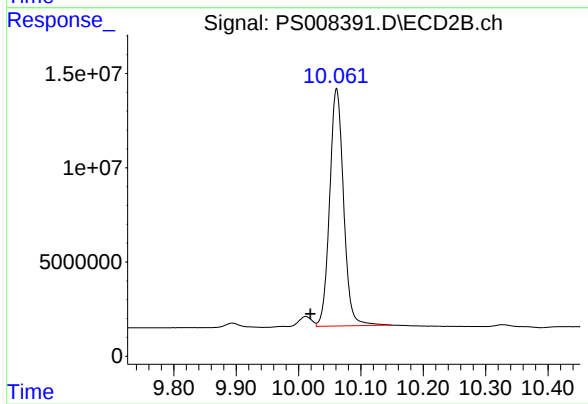

#16 DCPA

R.T.: 10.061 min
Delta R.T.: 0.042 min
Response: 195754987
Conc: 30.04 ng/ml