

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS011322\
 Data File : PS017980.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Jan 2022 08:49
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 13 15:09:27 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010522.M
 Quant Title : 8080.M
 QLast Update : Thu Jan 06 10:21:08 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.048	6.644	654.2E6	295.3E6	452.594	508.962
Target Compounds							
7) T	MCPA	7.493f	0.000	3809396	0	<MDL	N.D. #
11) T	2,4,5-TP ...	0.000	8.436f	0	8584645	N.D.	2.408
12) T	2,4,5-T	9.285	8.915f	13389484	12101150	1.511	3.700 #
13) T	2,4-DB	9.830	0.000	13093931	0	7.921	N.D. #
14) T	DINOSEB	10.924f	0.000	11474812	0	1.747	N.D. #
15) T	Picloram	10.804	10.660	363.7E6	129.4E6	30.469	27.678
16) T	DCPA	11.241	10.660f	6047171	129.4E6	<MDL	29.312 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS011322\
Data File : PS017980.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Jan 2022 08:49
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 13 15:09:27 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010522.M
Quant Title : 8080.M
QLast Update : Thu Jan 06 10:21:08 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

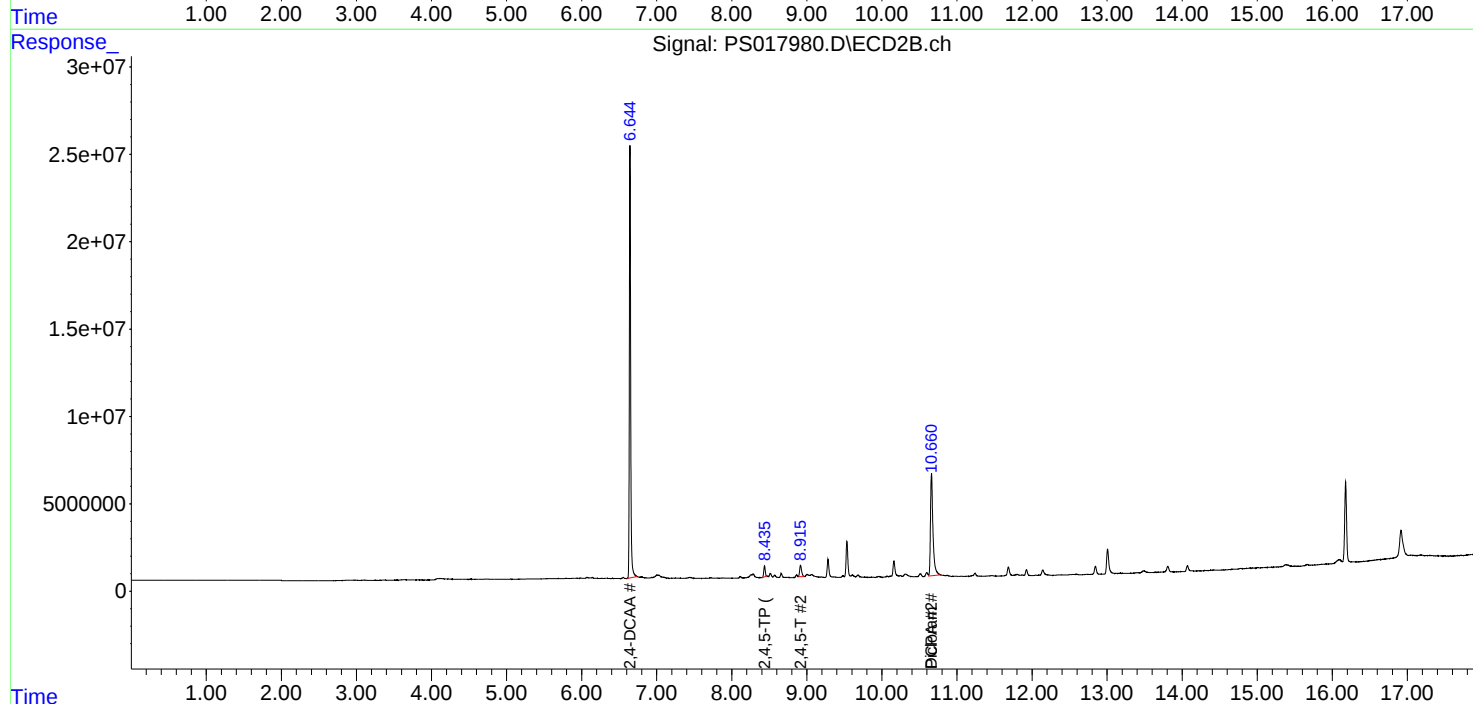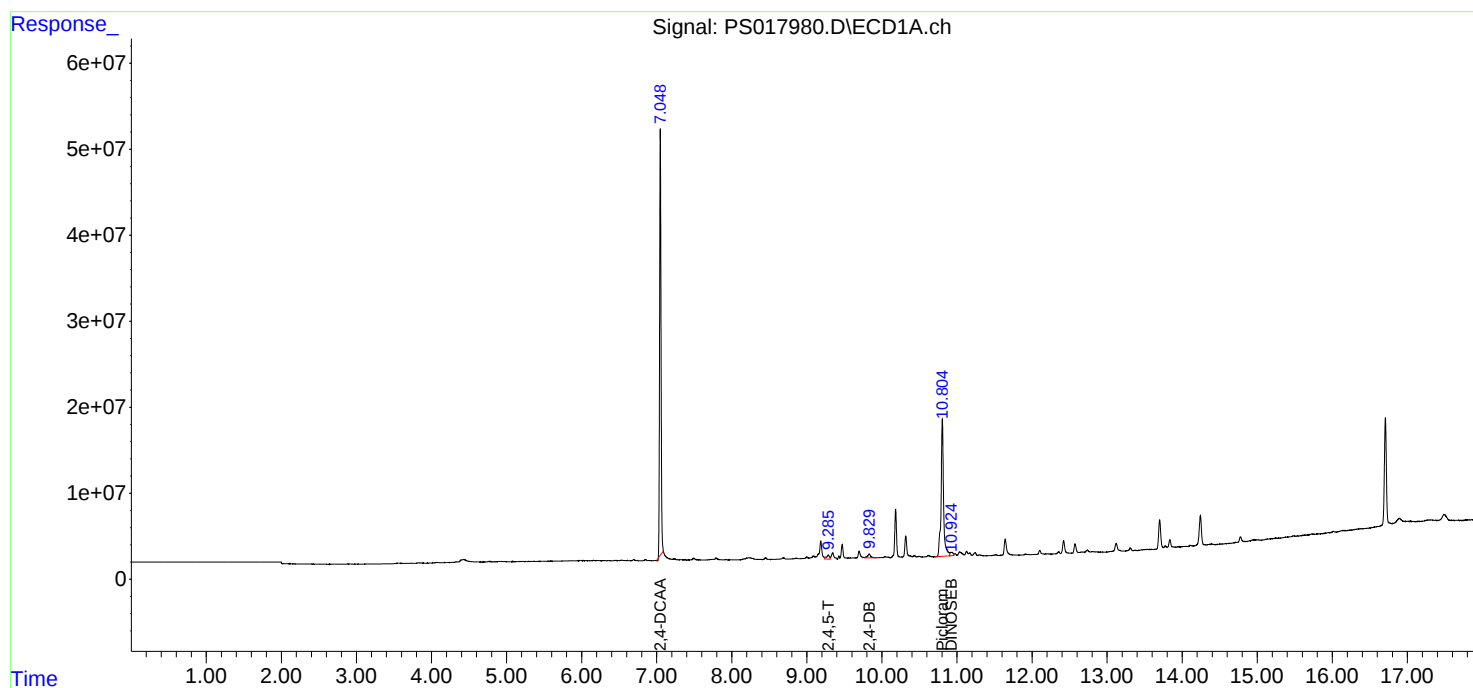


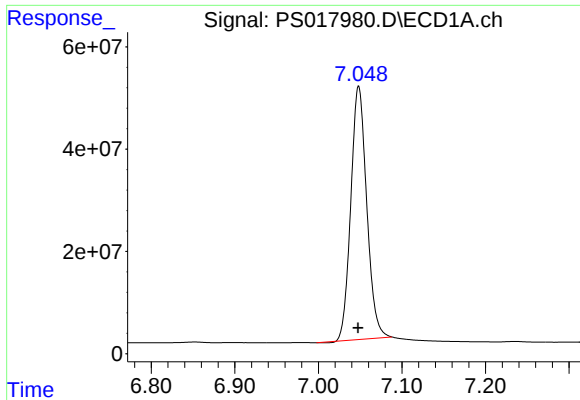

#4 2,4-DCAA


R.T.: 7.048 min
Delta R.T.: 0.000 min
Response: 654218679
Conc: 452.59 ng/ml

Instrument :
ECD_S
ClientSampleId :

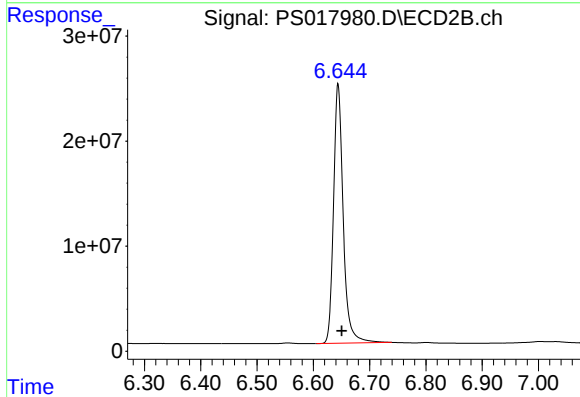


#4 2,4-DCAA

R.T.: 6.644 min
Delta R.T.: -0.007 min
Response: 295324646
Conc: 508.96 ng/ml

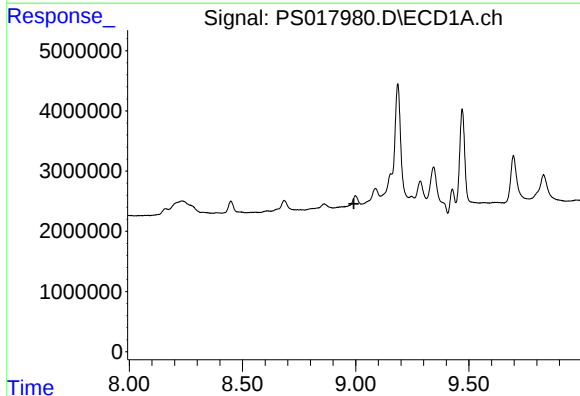


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 8.992 min
Response: 0
Conc: N.D.

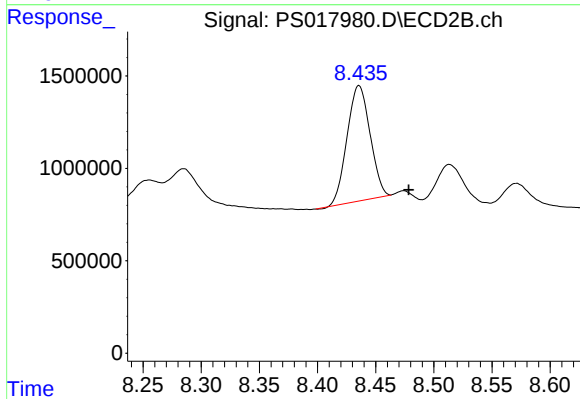

#11 2,4,5-TP (SILVEX)


R.T.: 8.436 min
Delta R.T.: -0.043 min
Response: 8584645
Conc: 2.41 ng/ml

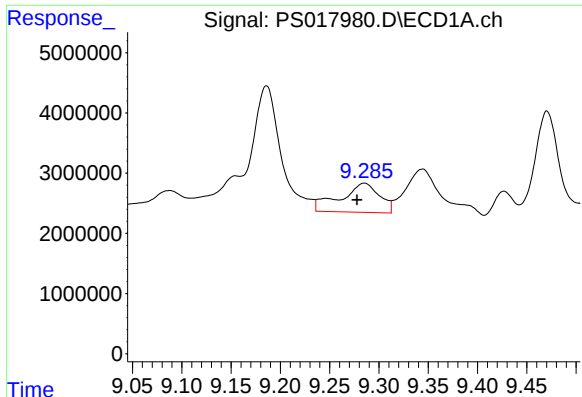

#12 2,4,5-T


R.T.: 9.285 min
Delta R.T.: 0.007 min
Response: 13389484
Conc: 1.51 ng/ml

Instrument :
ECD_S
ClientSampleId :

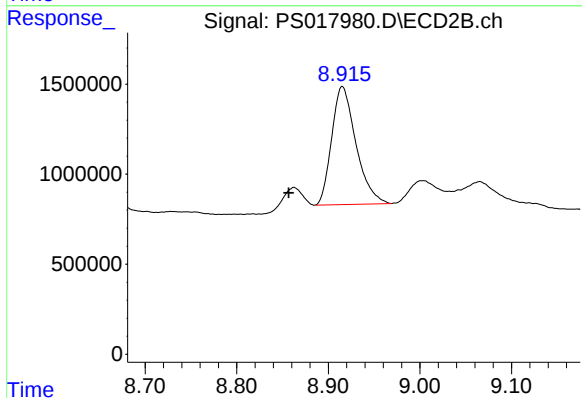


#12 2,4,5-T

R.T.: 8.915 min
Delta R.T.: 0.059 min
Response: 12101150
Conc: 3.70 ng/ml

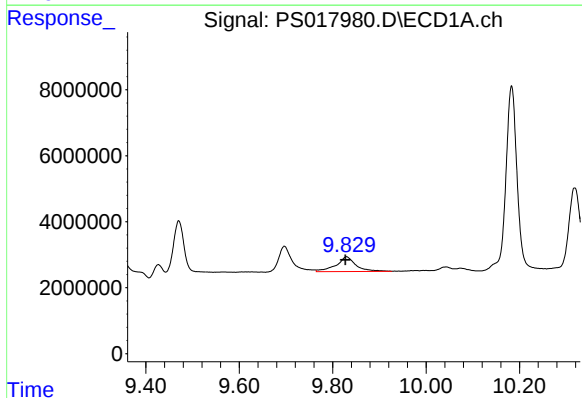


#13 2,4-DB

R.T.: 9.830 min
Delta R.T.: 0.003 min
Response: 13093931
Conc: 7.92 ng/ml

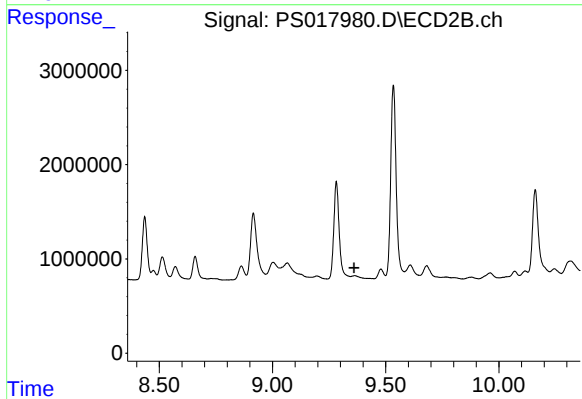

#13 2,4-DB


R.T.: 0.000 min
Exp R.T. : 9.360 min
Response: 0
Conc: N.D.

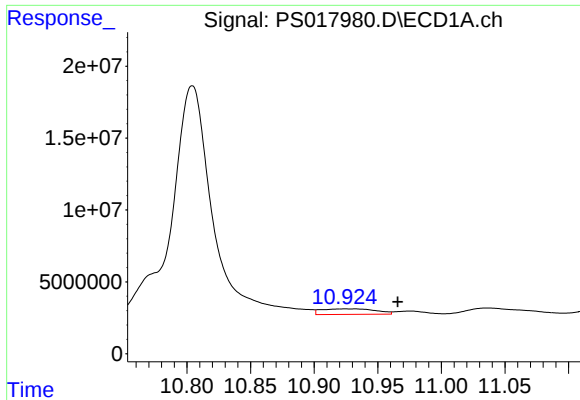

#14 DINOSEB


R.T.: 10.924 min
Delta R.T.: -0.041 min
Response: 11474812
Conc: 1.75 ng/ml

Instrument :
ECD_S
ClientSampleId :

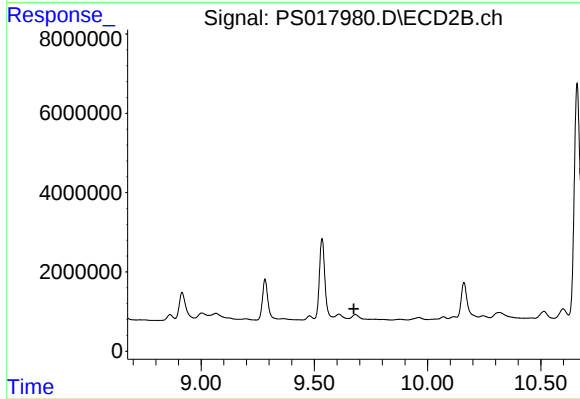


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 9.675 min
Response: 0
Conc: N.D.

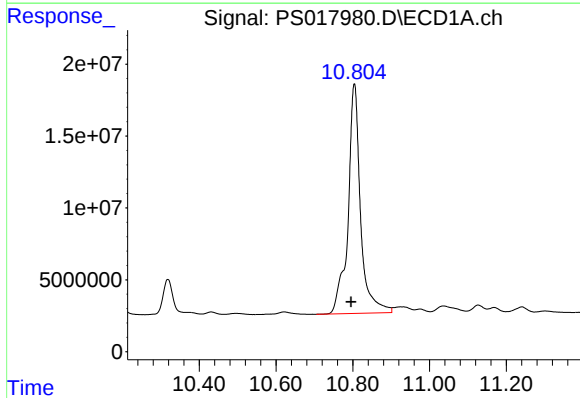


#15 Picloram

R.T.: 10.804 min
Delta R.T.: 0.008 min
Response: 363675697
Conc: 30.47 ng/ml

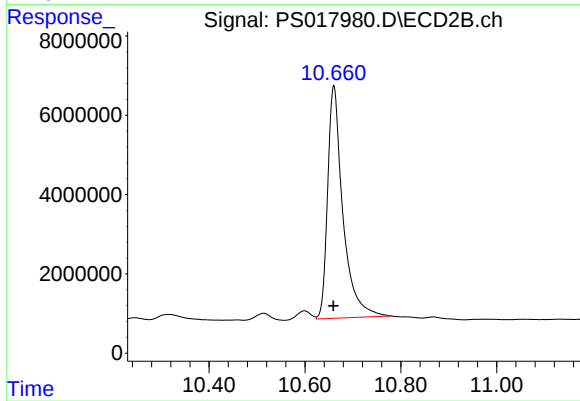

#15 Picloram


R.T.: 10.660 min
Delta R.T.: 0.001 min
Response: 129426230
Conc: 27.68 ng/ml

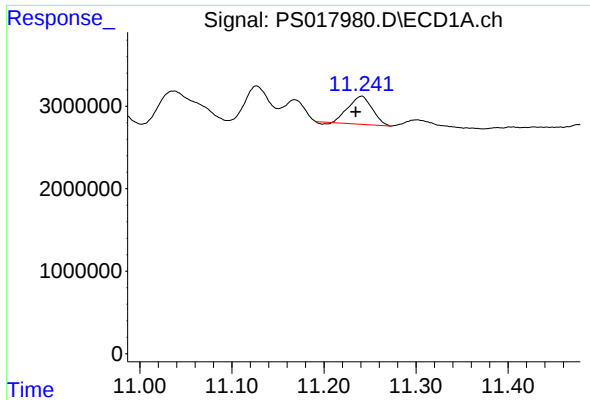

#16 DCPA

R.T.: 11.241 min
Delta R.T.: 0.007 min
Response: 6047171
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

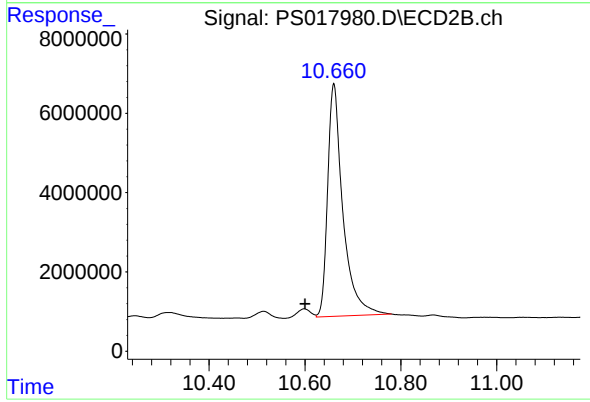

#16 DCPA

R.T.: 10.660 min
Delta R.T.: 0.061 min
Response: 129426230
Conc: 29.31 ng/ml