

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS011322\
 Data File : PS017986.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Jan 2022 13:27
 Operator : AJ\MA
 Sample : HSTDCCC750
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HSTDCCC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 13 15:10:38 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010522.M
 Quant Title : 8080.M
 QLast Update : Thu Jan 06 10:21:08 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.048	6.645	1070.5E6	422.7E6	740.560	728.424
Target Compounds							
1) T	Dalapon	2.908	2.419	1576.3E6	485.6E6	642.531	635.047
2) T	3,5-DICHL...	6.288	5.861	1417.5E6	598.2E6	658.919	676.248
3) T	4-Nitroph...	6.875	6.279	604.2E6	227.3E6	748.019	741.488
5) T	DICAMBA	7.235	6.800	4126.2E6	1743.3E6	660.777	663.085
6) T	MCPD	7.405	6.894	307.3E6	140.0E6	65.808	65.095
7) T	MCPA	7.553	7.104	439.8E6	196.0E6	65.919	65.682
8) T	DICHLORPROP	7.922	7.410	1030.2E6	440.1E6	654.893	659.409
9) T	2,4-D	8.148	7.699	1240.0E6	523.2E6	680.943	710.865
10) T	Pentachlo...	8.448	8.113	14265.7E6	5609.7E6	675.265	666.043
11) T	2,4,5-TP ...	8.999	8.475	5683.1E6	2408.8E6	671.587	675.728
12) T	2,4,5-T	9.281	8.851	5960.2E6	2325.9E6	672.399	711.059
13) T	2,4-DB	9.827	9.354	1249.0E6	307.1E6	755.596	694.089
14) T	DINOSEB	10.977	9.675	4305.7E6	1659.0E6	655.665	664.907
15) T	Picloram	10.797	10.651	8827.6E6	3432.8E6	739.586	734.100
16) T	DCPA	11.246	10.602	7327.6E6	2979.9E6	678.178	674.884



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS011322\
Data File : PS017986.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Jan 2022 13:27
Operator : AJ\MA
Sample : HSTDCCC750
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 13 15:10:38 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010522.M
Quant Title : 8080.M
QLast Update : Thu Jan 06 10:21:08 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

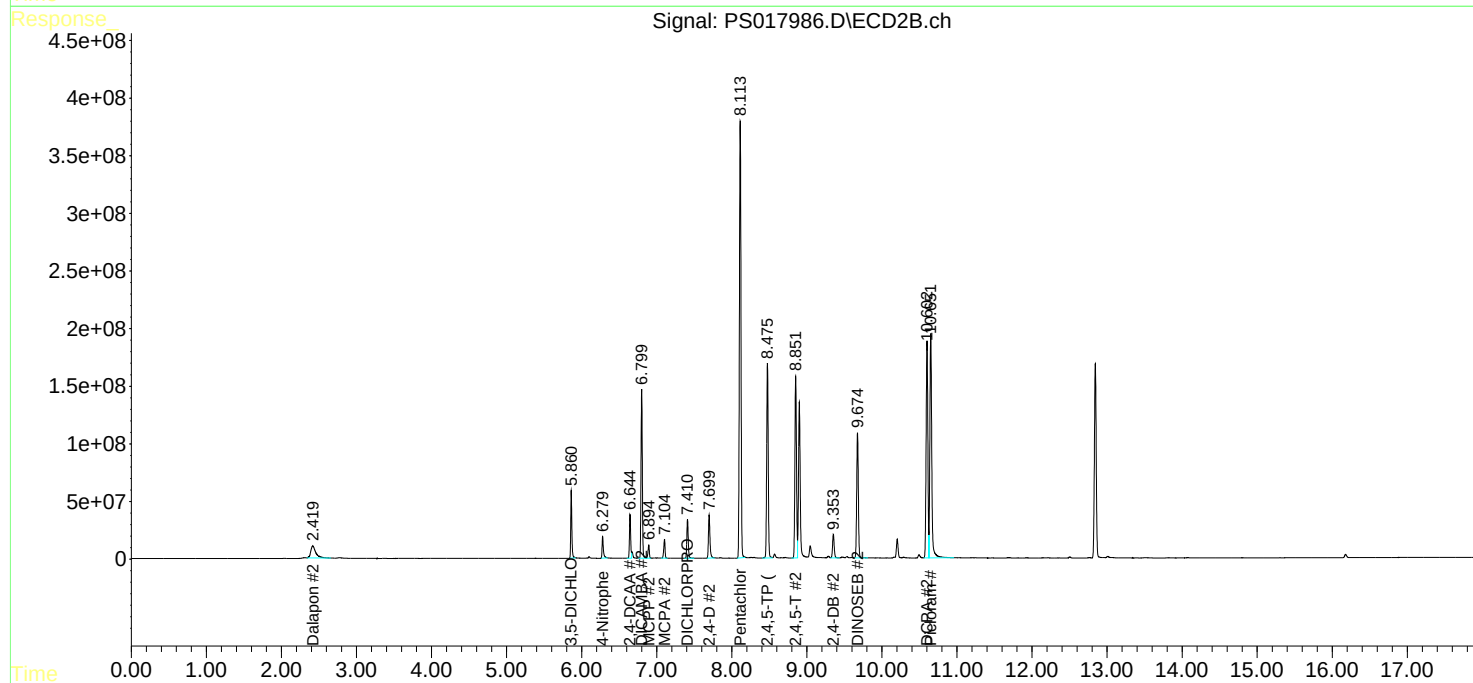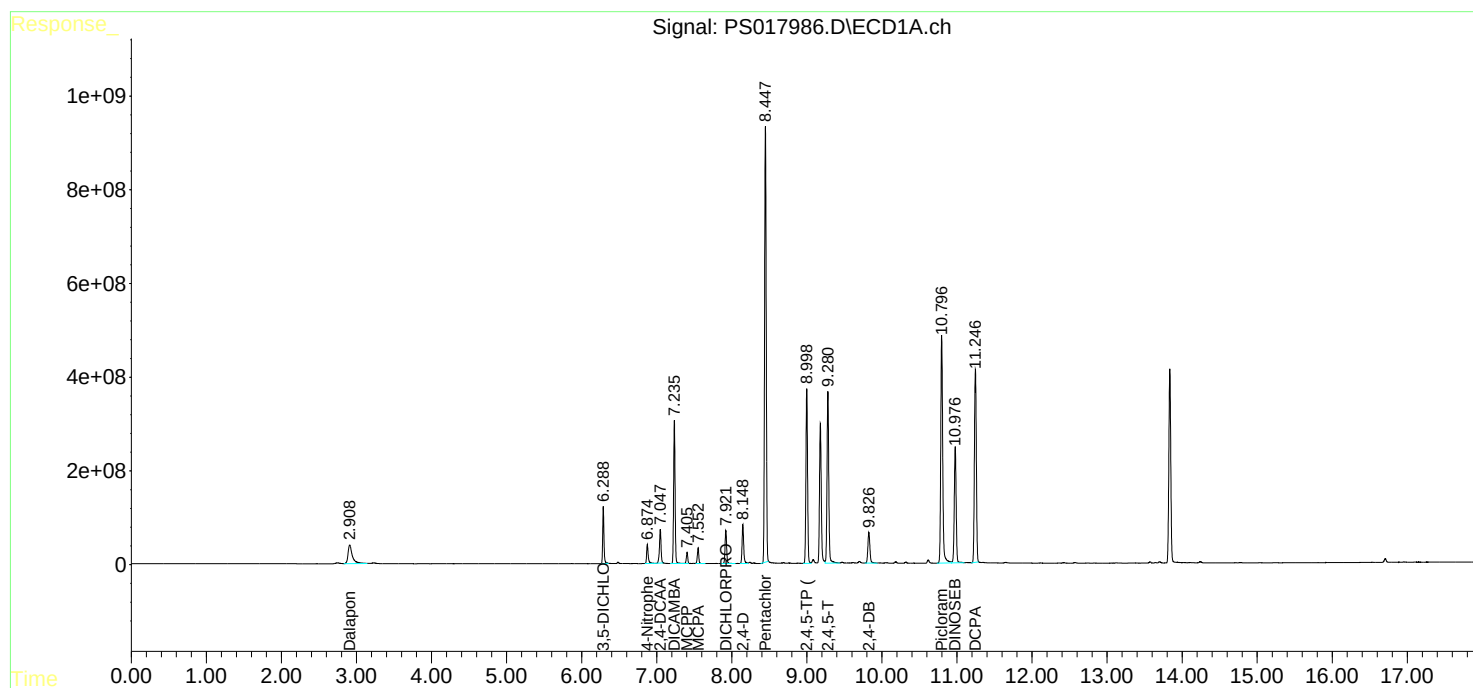


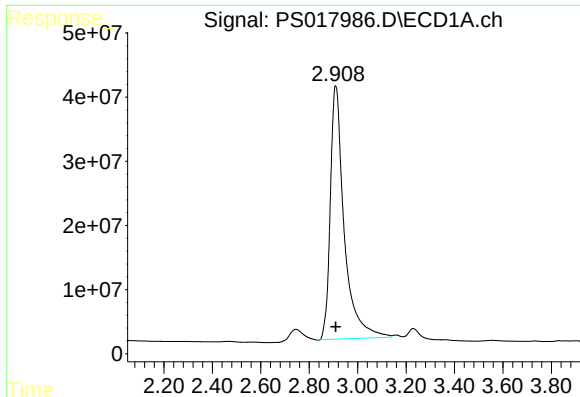

#1 Dalapon


R.T.: 2.908 min
Delta R.T.: 0.000 min
Response: 1576272226
Conc: 642.53 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

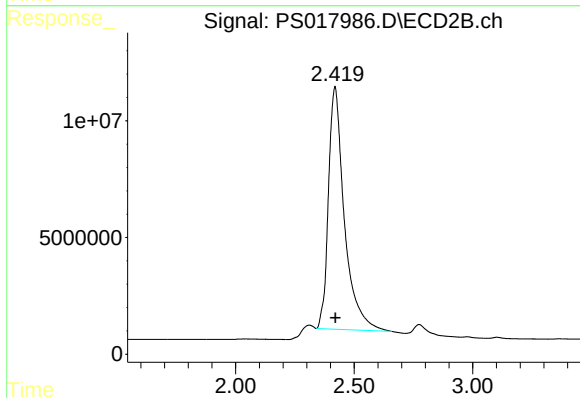


#1 Dalapon

R.T.: 2.419 min
Delta R.T.: -0.002 min
Response: 485612809
Conc: 635.05 ng/ml

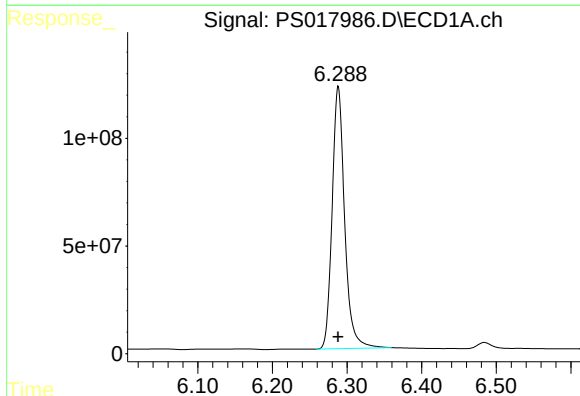


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.288 min
Delta R.T.: 0.000 min
Response: 1417495366
Conc: 658.92 ng/ml

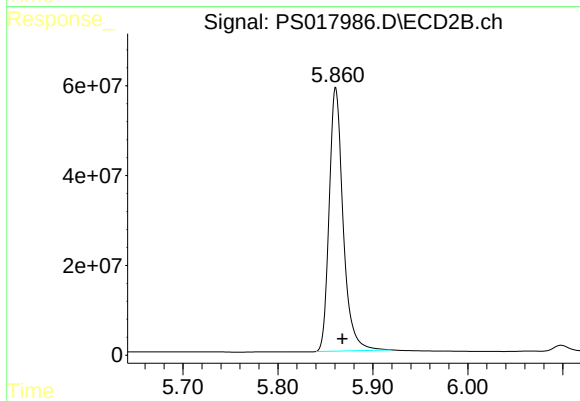

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 5.861 min
Delta R.T.: -0.007 min
Response: 598229572
Conc: 676.25 ng/ml

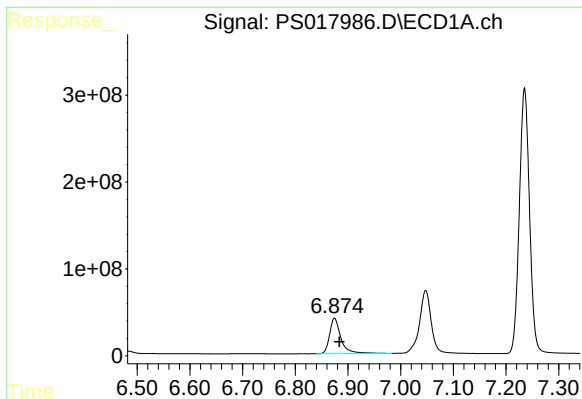

#3 4-Nitrophenol


R.T.: 6.875 min
Delta R.T.: -0.009 min
Response: 604162944
Conc: 748.02 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

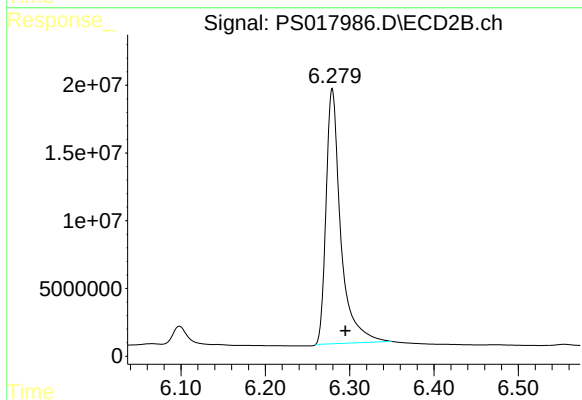


#3 4-Nitrophenol

R.T.: 6.279 min
Delta R.T.: -0.015 min
Response: 227282422
Conc: 741.49 ng/ml

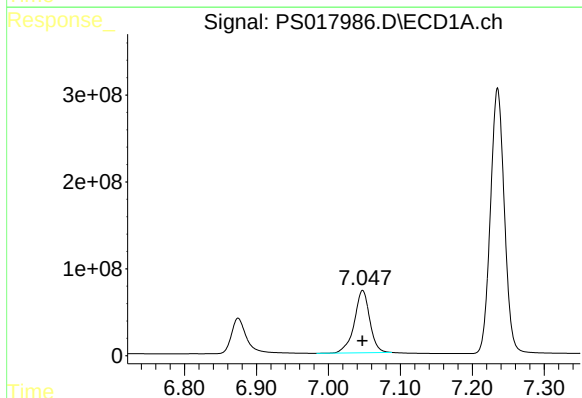


#4 2,4-DCAA

R.T.: 7.048 min
Delta R.T.: 0.000 min
Response: 1070469685
Conc: 740.56 ng/ml

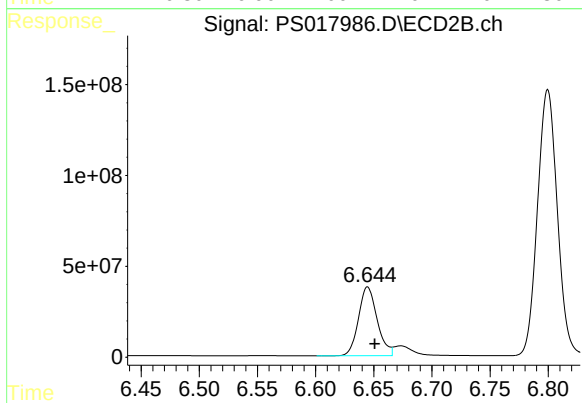

#4 2,4-DCAA


R.T.: 6.645 min
Delta R.T.: -0.006 min
Response: 422666966
Conc: 728.42 ng/ml

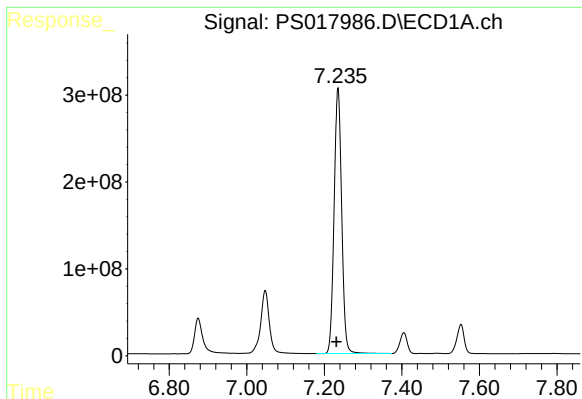

#5 DICAMBA


R.T.: 7.235 min
Delta R.T.: 0.004 min
Response: 4126166119
Conc: 660.78 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

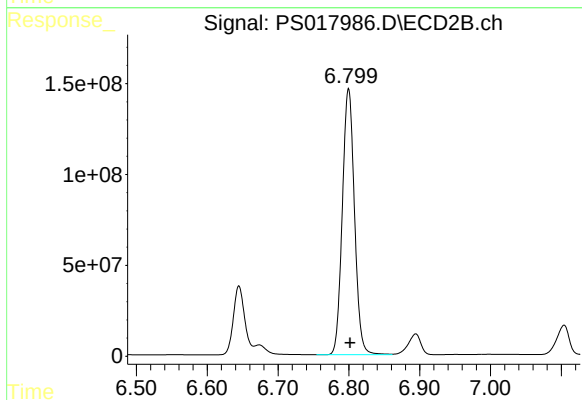


#5 DICAMBA

R.T.: 6.800 min
Delta R.T.: -0.002 min
Response: 1743286345
Conc: 663.09 ng/ml

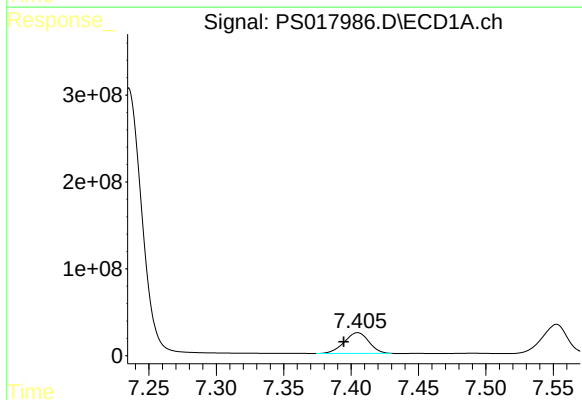


#6 MCP

R.T.: 7.405 min
Delta R.T.: 0.010 min
Response: 307252922
Conc: 65.81 ug/ml

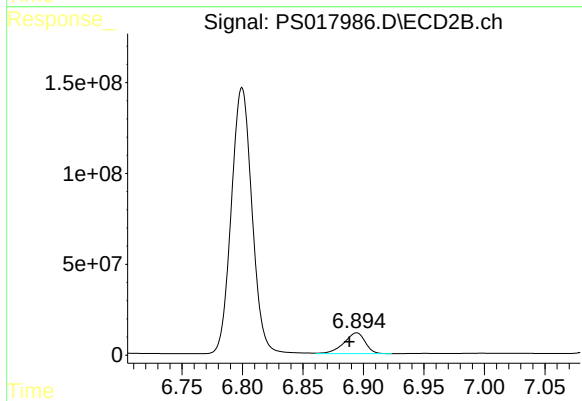

#6 MCP


R.T.: 6.894 min
Delta R.T.: 0.006 min
Response: 140014706
Conc: 65.09 ug/ml

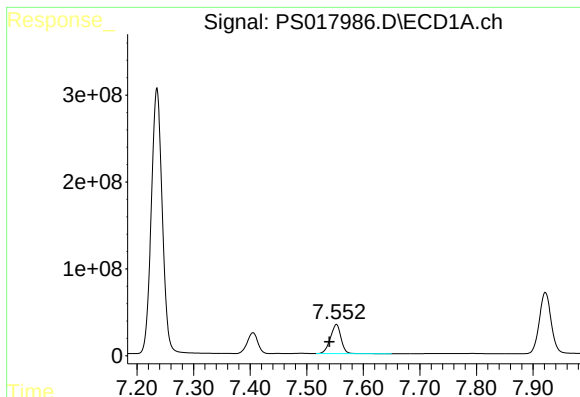

#7 MCPA


R.T.: 7.553 min
Delta R.T.: 0.012 min
Response: 439794953
Conc: 65.92 ug/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

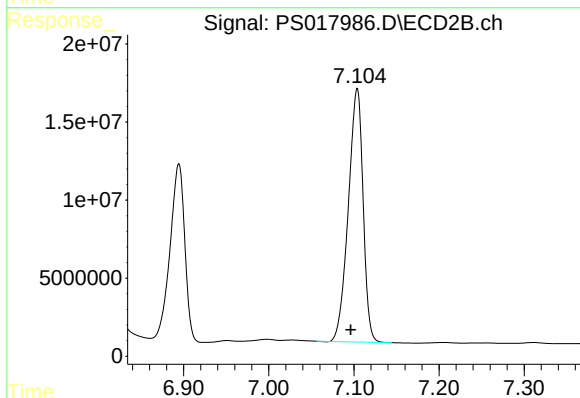


#7 MCPA

R.T.: 7.104 min
Delta R.T.: 0.008 min
Response: 195989850
Conc: 65.68 ug/ml

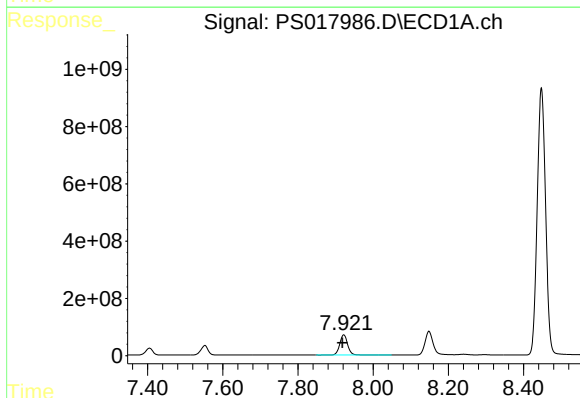


#8 DICHLORPROP

R.T.: 7.922 min
Delta R.T.: 0.004 min
Response: 1030176693
Conc: 654.89 ng/ml

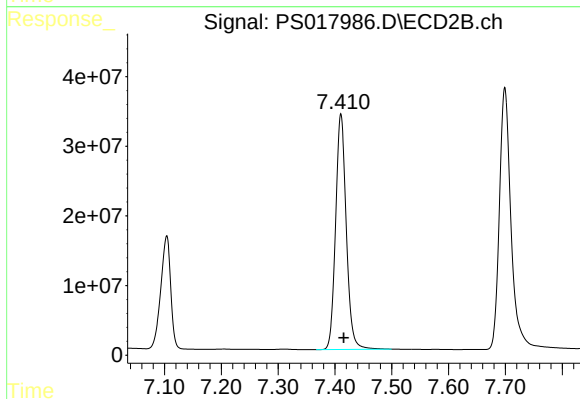

#8 DICHLORPROP


R.T.: 7.410 min
Delta R.T.: -0.005 min
Response: 440105314
Conc: 659.41 ng/ml

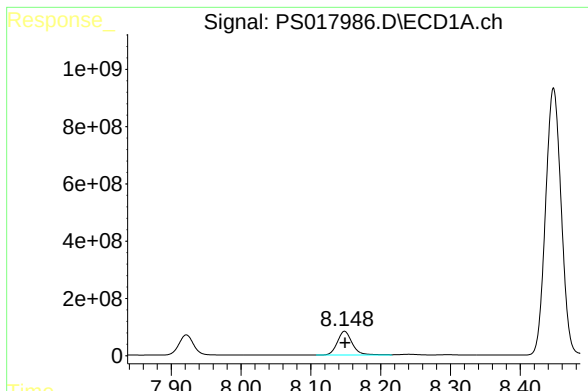

#9 2,4-D


R.T.: 8.148 min
Delta R.T.: 0.000 min
Response: 1239952636
Conc: 680.94 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

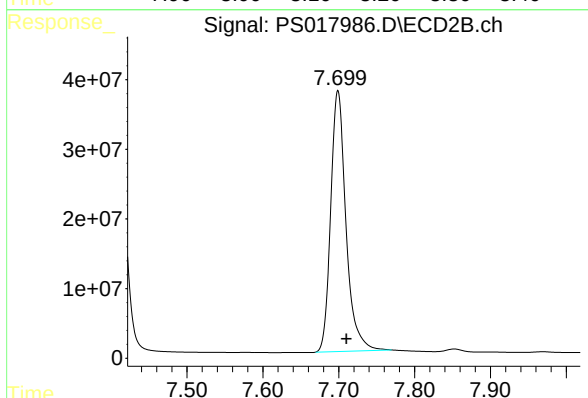


#9 2,4-D

R.T.: 7.699 min
Delta R.T.: -0.011 min
Response: 523158056
Conc: 710.87 ng/ml

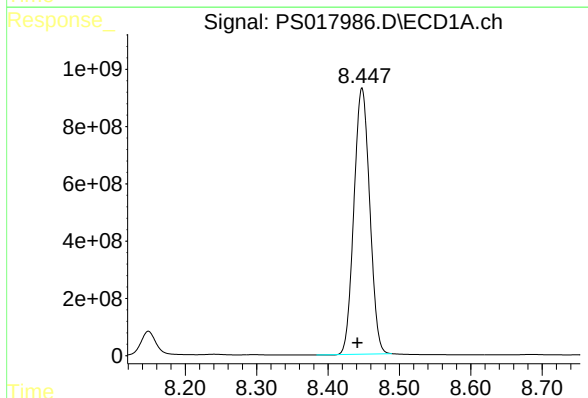


#10 Pentachlorophenol

R.T.: 8.448 min
Delta R.T.: 0.006 min
Response: 14265678379
Conc: 675.26 ng/ml

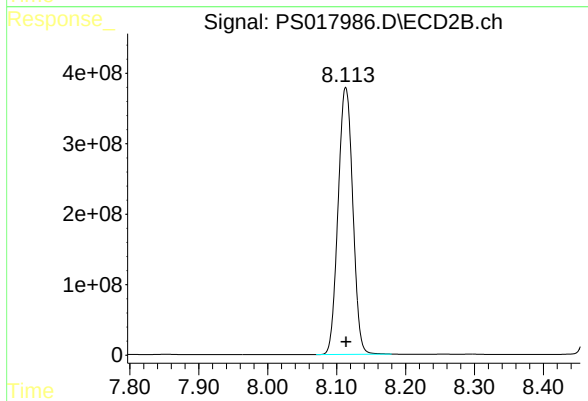

#10 Pentachlorophenol


R.T.: 8.113 min
Delta R.T.: 0.000 min
Response: 5609655922
Conc: 666.04 ng/ml

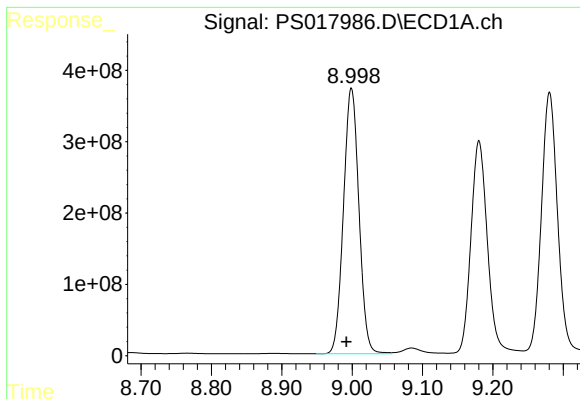

#11 2,4,5-TP (SILVEX)


R.T.: 8.999 min
Delta R.T.: 0.007 min
Response: 5683059858
Conc: 671.59 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

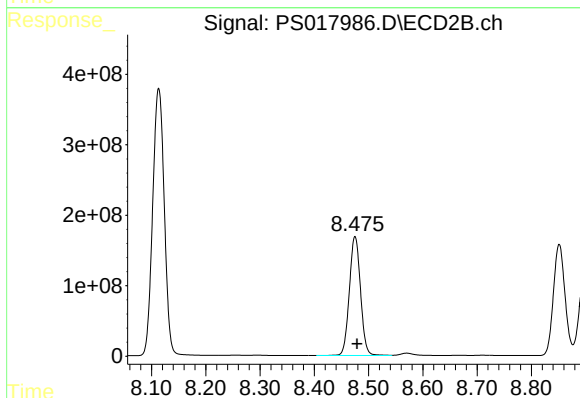


#11 2,4,5-TP (SILVEX)

R.T.: 8.475 min
Delta R.T.: -0.003 min
Response: 2408763266
Conc: 675.73 ng/ml

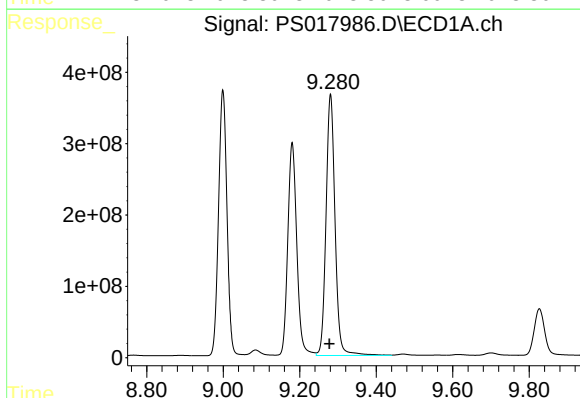


#12 2,4,5-T

R.T.: 9.281 min
Delta R.T.: 0.003 min
Response: 5960235290
Conc: 672.40 ng/ml

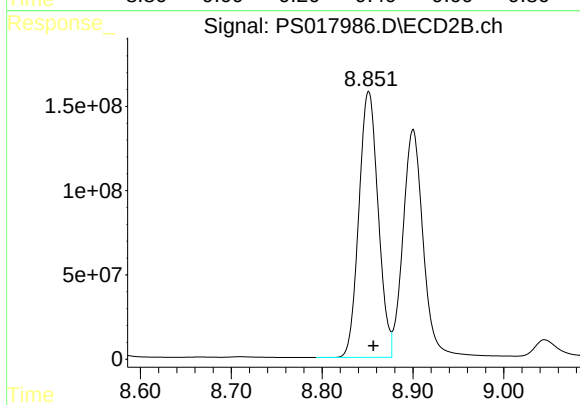

#12 2,4,5-T


R.T.: 8.851 min
Delta R.T.: -0.005 min
Response: 2325884746
Conc: 711.06 ng/ml

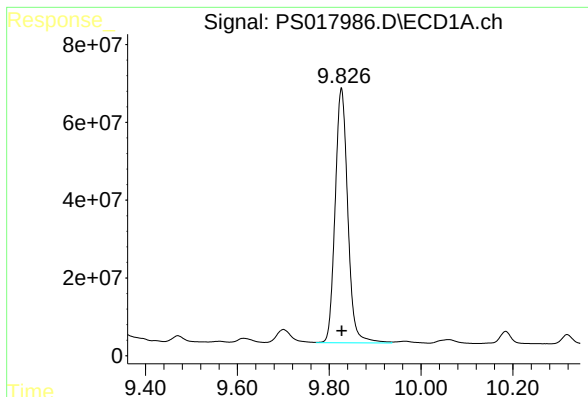

#13 2,4-DB


R.T.: 9.827 min
Delta R.T.: 0.000 min
Response: 1249025806
Conc: 755.60 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

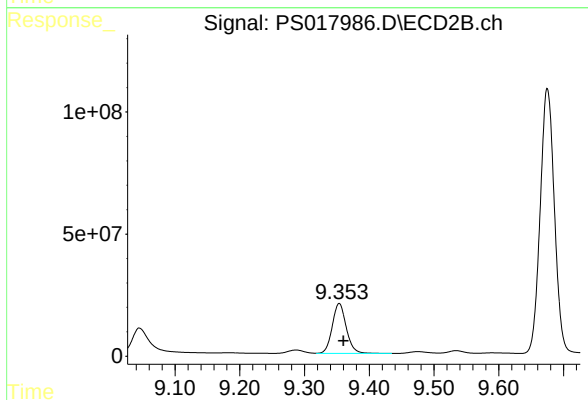


#13 2,4-DB

R.T.: 9.354 min
Delta R.T.: -0.006 min
Response: 307104708
Conc: 694.09 ng/ml

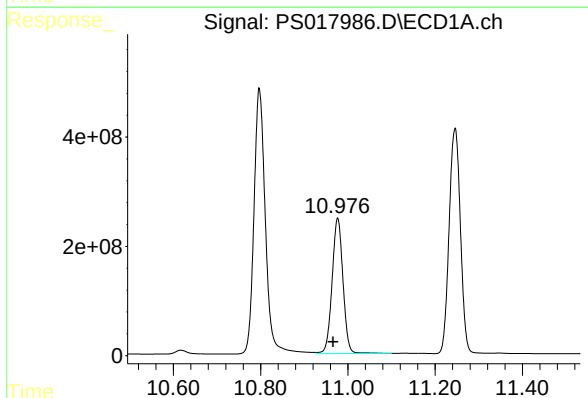


#14 DINOSEB

R.T.: 10.977 min
Delta R.T.: 0.011 min
Response: 4305716410
Conc: 655.67 ng/ml

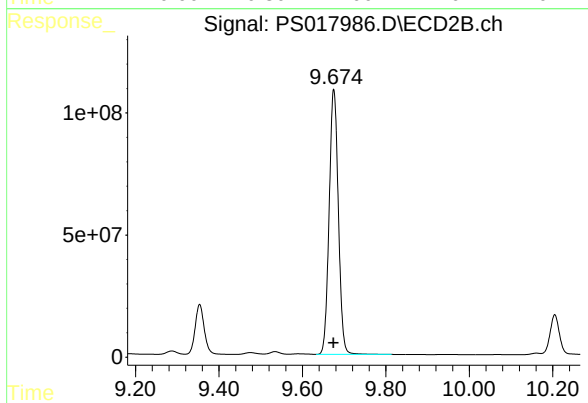

#14 DINOSEB


R.T.: 9.675 min
Delta R.T.: 0.000 min
Response: 1658954415
Conc: 664.91 ng/ml

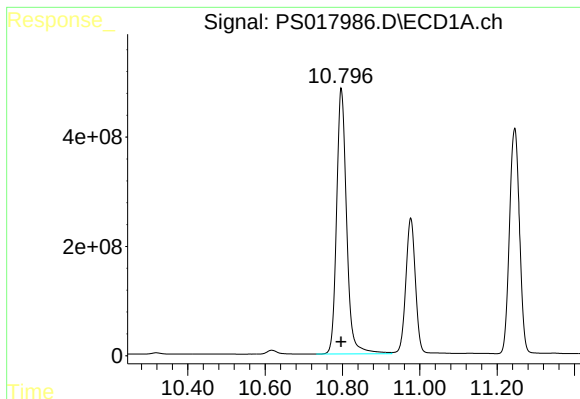

#15 Picloram


R.T.: 10.797 min
Delta R.T.: 0.000 min
Response: 8827632610
Conc: 739.59 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

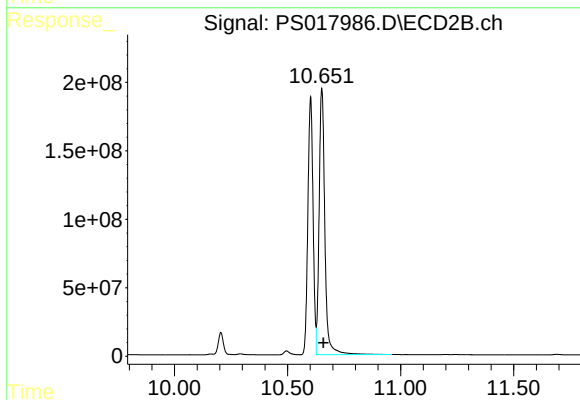


#15 Picloram

R.T.: 10.651 min
Delta R.T.: -0.008 min
Response: 3432761796
Conc: 734.10 ng/ml

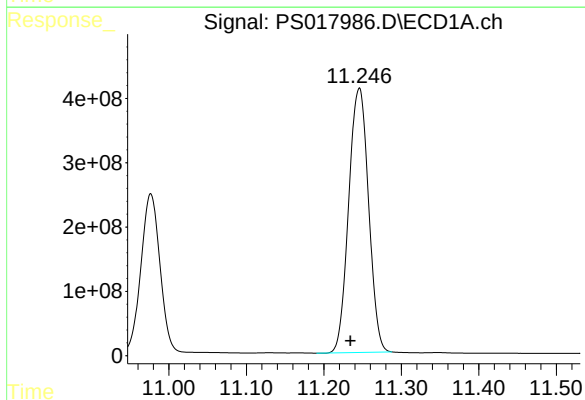

#16 DCPA

R.T.: 11.246 min
Delta R.T.: 0.011 min
Response: 7327565417
Conc: 678.18 ng/ml

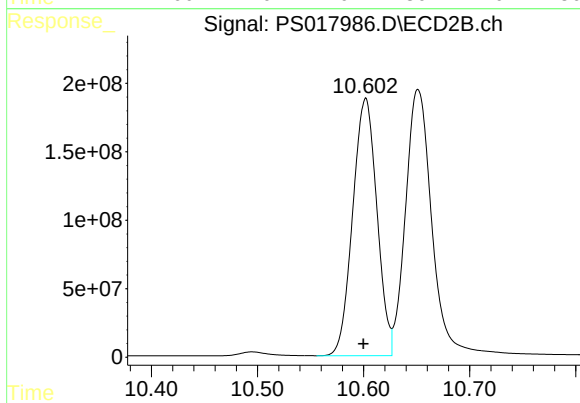

#16 DCPA

R.T.: 10.602 min
Delta R.T.: 0.002 min
Response: 2979941116
Conc: 674.88 ng/ml