

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS011323\
 Data File : PS021741.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Jan 2023 08:26
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 15 20:18:13 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010923.M
 Quant Title : 8080.M
 QLast Update : Tue Jan 10 10:34:52 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.354	6.809	25793077	7266520	9.266	4.044 #
Target Compounds							
1) T	Dalapon	2.480	0.000	3287648	0	1.162	N.D. #
3) T	4-Nitroph...	6.211	6.388f	6994973	342805	4.799	<MDL #
5) T	DICAMBA	6.520	7.023f	915374	2608.7E6	<MDL	306.806 #
6) T	MCP	0.000	7.023f	0	2608.7E6	N.D.	393.375
7) T	MCPA	6.842f	0.000	2931193	0	<MDL	N.D. #
8) T	DICHLORPROP	7.114	7.618	6974823	15722767	2.163	7.369 #
9) T	2,4-D	7.282	7.926	5693.6E6	3461647	1465.994	1.370 #
10) T	Pentachlo...	7.545	8.317	5297737	2879448	<MDL	<MDL #
11) T	2,4,5-TP ...	8.096	8.678	18245671	9149440	<MDL	<MDL #
14) T	DINOSEB	9.833f	9.839f	45730152	5900313	2.786	<MDL #
15) T	Picloram	9.712	10.861	1303.4E6	77423931	45.949	4.372 #
16) T	DCPA	10.159	10.829	6922579	65143374	<MDL	4.673 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS011323\
Data File : PS021741.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Jan 2023 08:26
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 15 20:18:13 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010923.M
Quant Title : 8080.M
QLast Update : Tue Jan 10 10:34:52 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

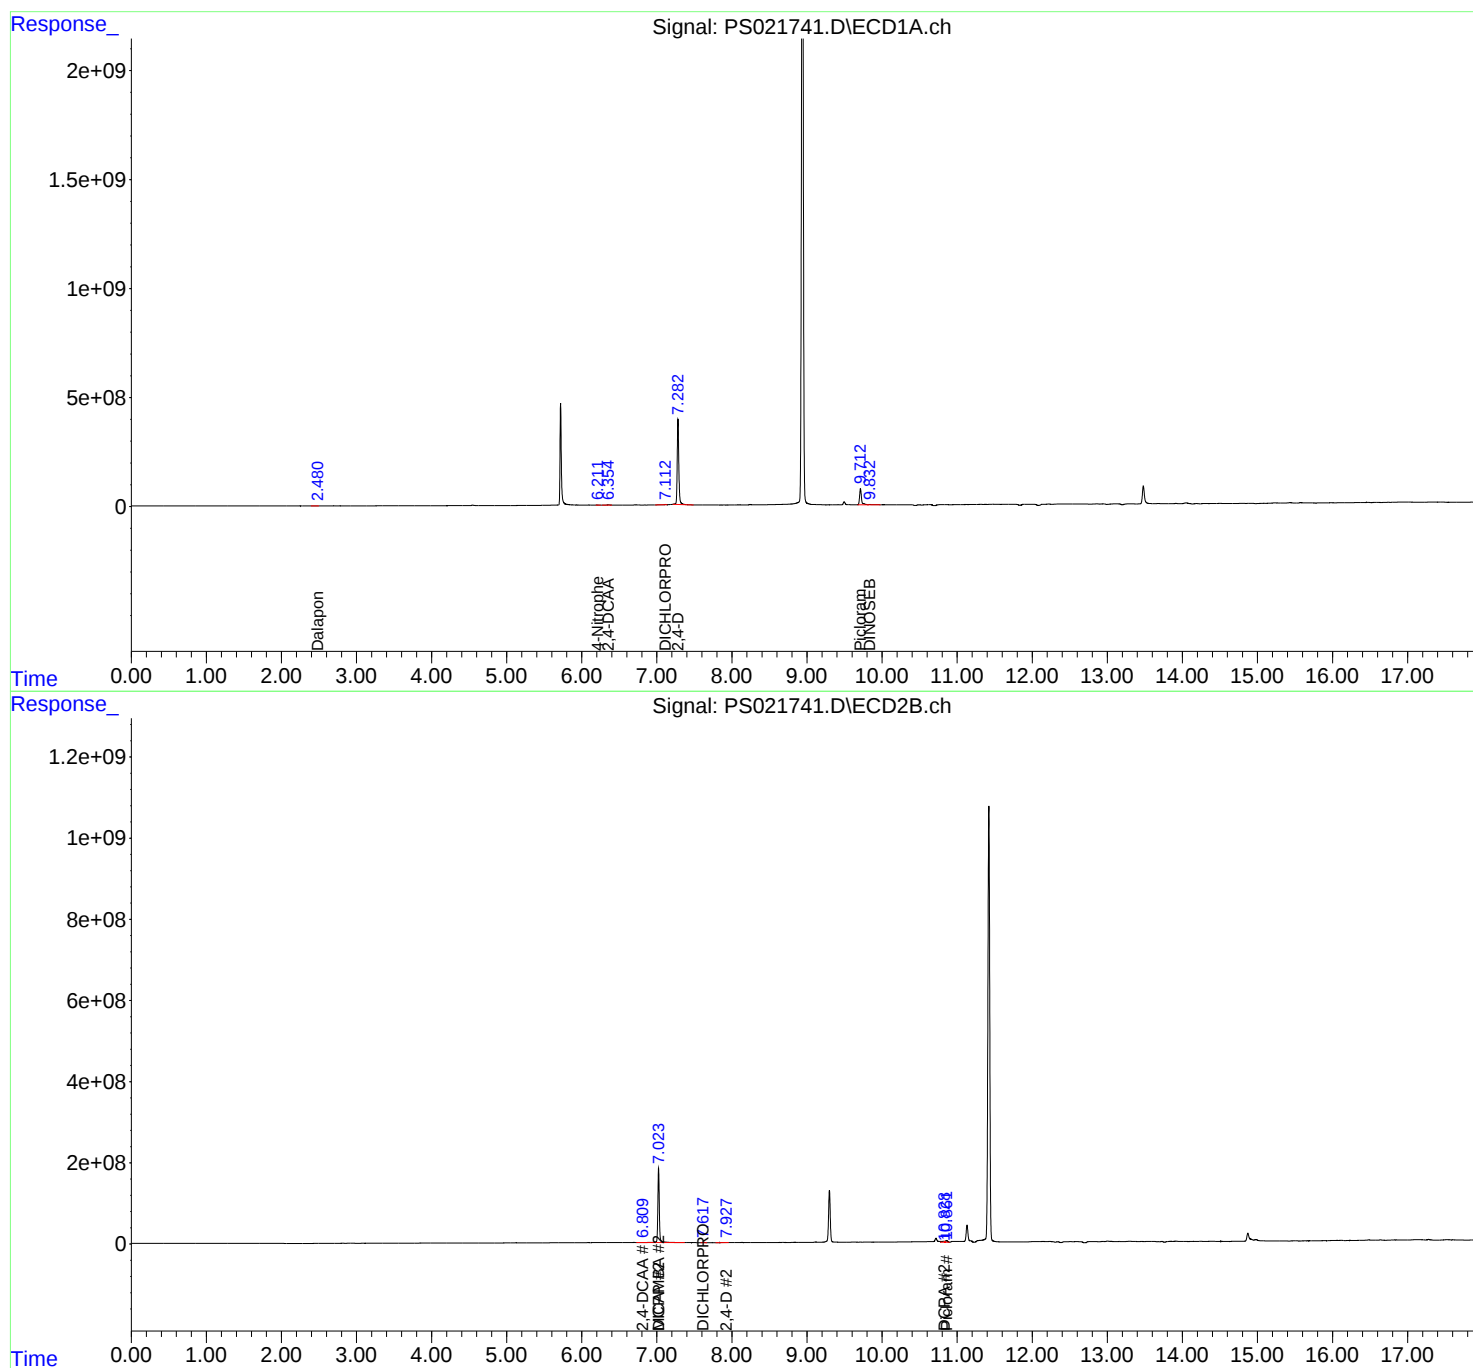


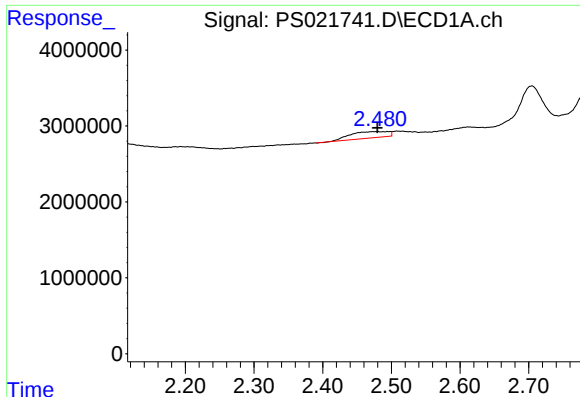

#1 Dalapon


R.T.: 2.480 min
Delta R.T.: 0.000 min
Response: 3287648
Conc: 1.16 ng/ml

Instrument :
ECD_S
ClientSampleId :

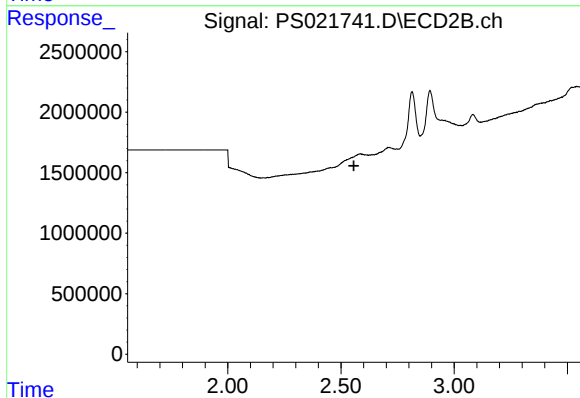


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 2.557 min
Response: 0
Conc: N.D.

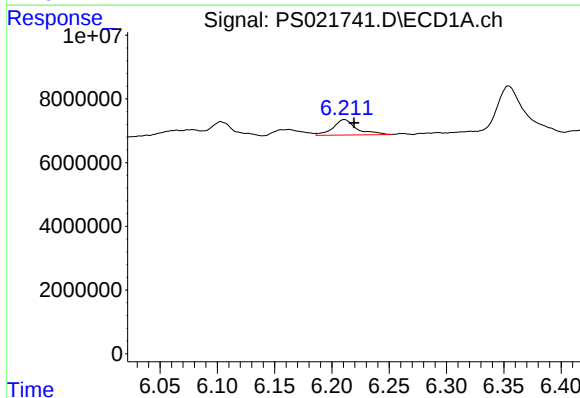


#3 4-Nitrophenol

R.T.: 6.211 min
Delta R.T.: -0.008 min
Response: 6994973
Conc: 4.80 ng/ml

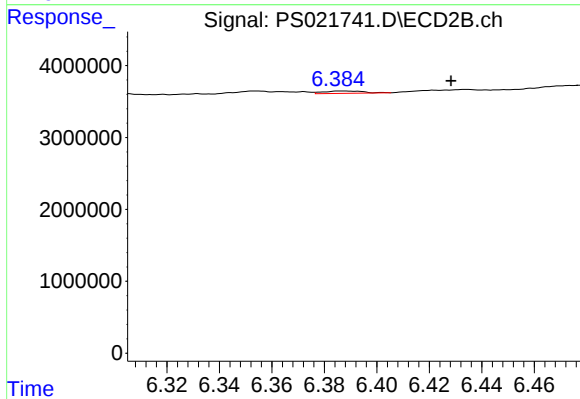

#3 4-Nitrophenol


R.T.: 6.388 min
Delta R.T.: -0.040 min
Response: 342805
Conc: N.D.

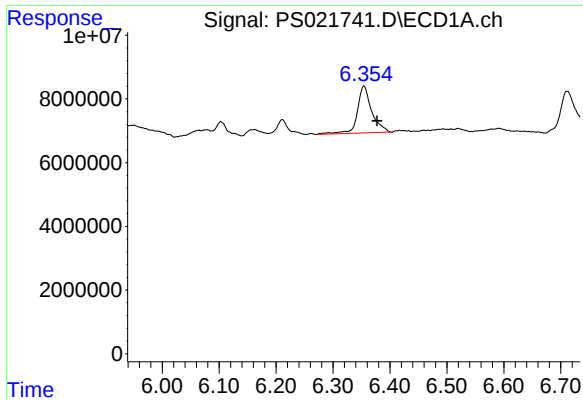

#4 2,4-DCAA


R.T.: 6.354 min
Delta R.T.: -0.023 min
Response: 25793077
Conc: 9.27 ng/ml

Instrument :
ECD_S
ClientSampleId :

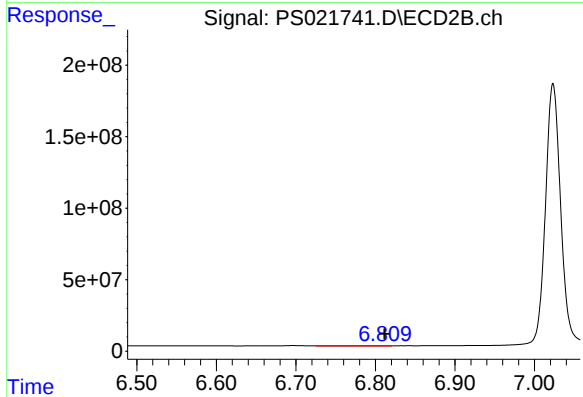


#4 2,4-DCAA

R.T.: 6.809 min
Delta R.T.: -0.002 min
Response: 7266520
Conc: 4.04 ng/ml

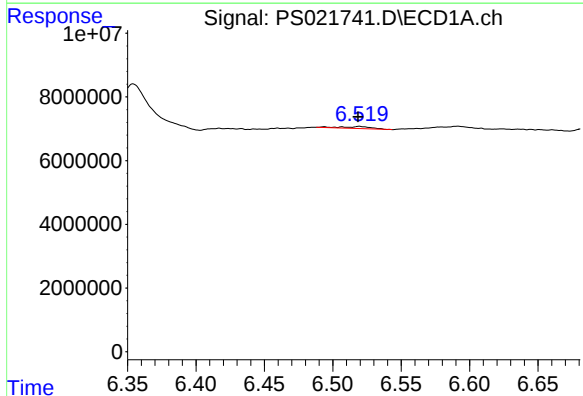


#5 DICAMBA

R.T.: 6.520 min
Delta R.T.: 0.001 min
Response: 915374
Conc: N.D.

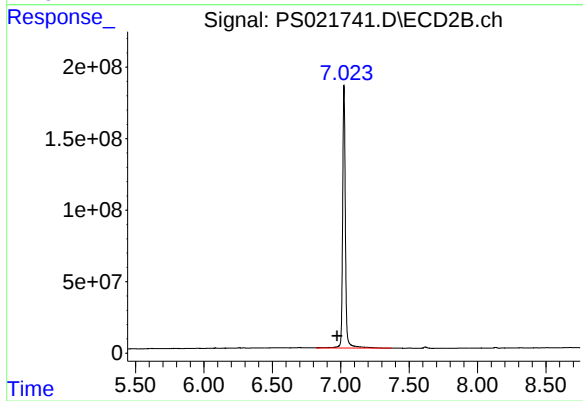

#5 DICAMBA


R.T.: 7.023 min
Delta R.T.: 0.049 min
Response: 2608694850
Conc: 306.81 ng/ml

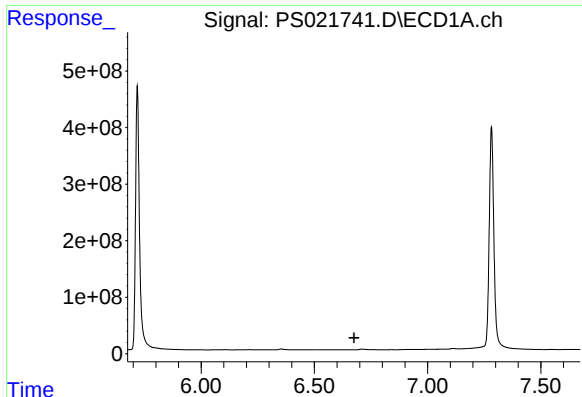

#6 MCP


R.T.: 0.000 min
Exp R.T.: 6.675 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

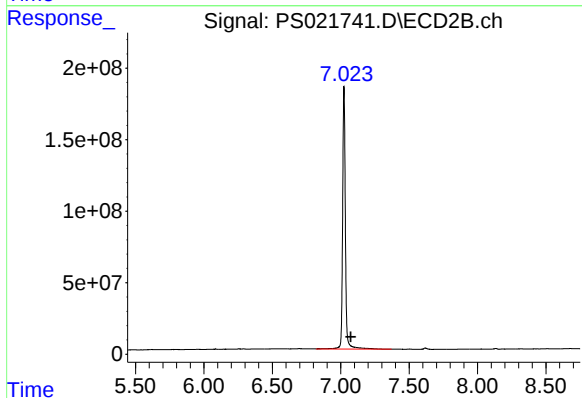


#6 MCP

R.T.: 7.023 min
Delta R.T.: -0.051 min
Response: 2608694850
Conc: 393.37 ug/ml

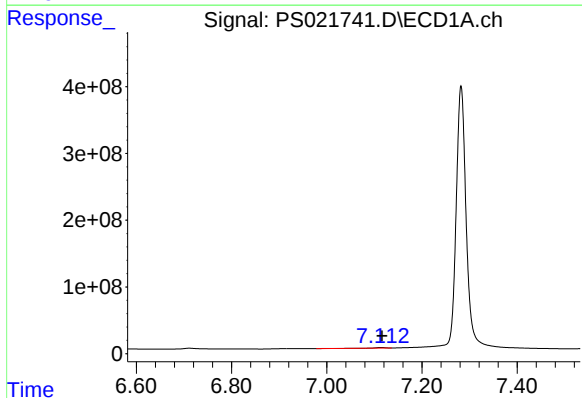


#8 DICHLORPROP

R.T.: 7.114 min
Delta R.T.: -0.003 min
Response: 6974823
Conc: 2.16 ng/ml

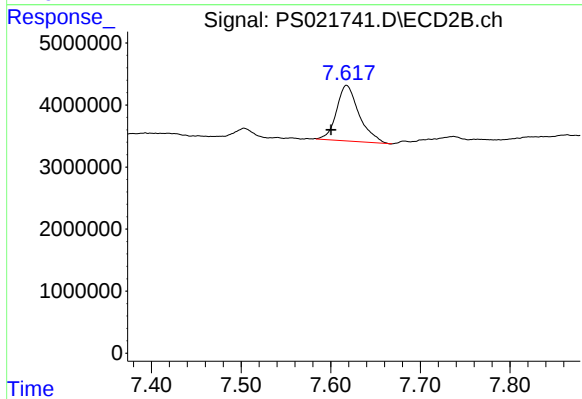

#8 DICHLORPROP


R.T.: 7.618 min
Delta R.T.: 0.017 min
Response: 15722767
Conc: 7.37 ng/ml

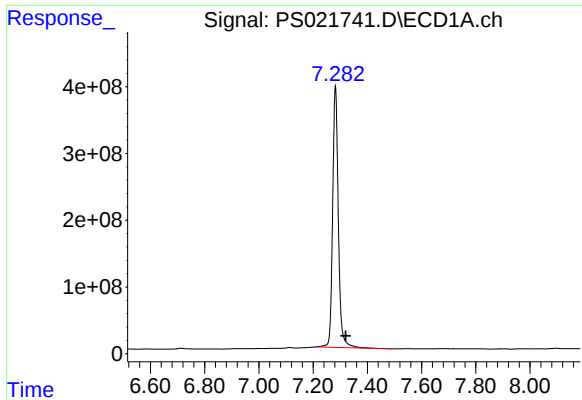

#9 2,4-D


R.T.: 7.282 min
Delta R.T.: -0.039 min
Response: 5693631162
Conc: 1465.99 ng/m

Instrument :
ECD_S
ClientSampleId :

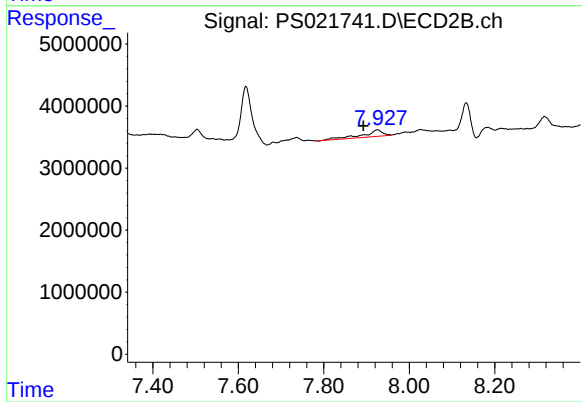


#9 2,4-D

R.T.: 7.926 min
Delta R.T.: 0.033 min
Response: 3461647
Conc: 1.37 ng/ml

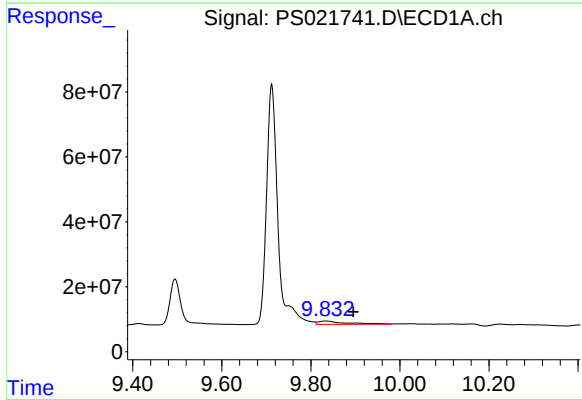


#14 DINOSEB

R.T.: 9.833 min
Delta R.T.: -0.063 min
Response: 45730152
Conc: 2.79 ng/ml

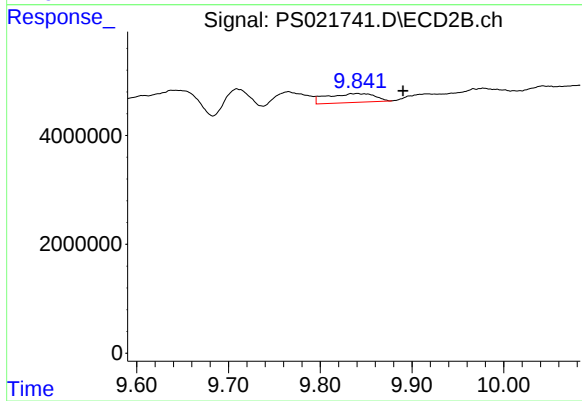

#14 DINOSEB


R.T.: 9.839 min
Delta R.T.: -0.051 min
Response: 5900313
Conc: N.D.

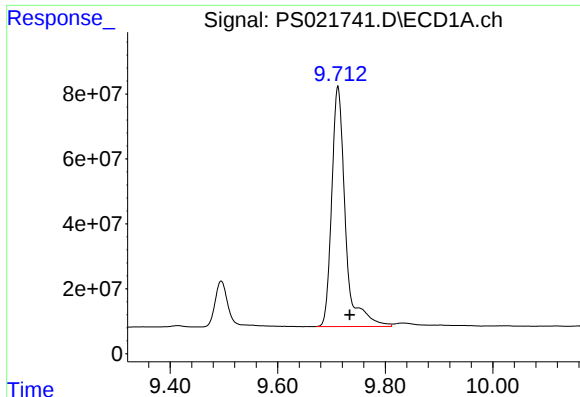

#15 Picloram


R.T.: 9.712 min
Delta R.T.: -0.022 min
Response: 1303446607
Conc: 45.95 ng/ml

Instrument :
ECD_S
ClientSampleId :

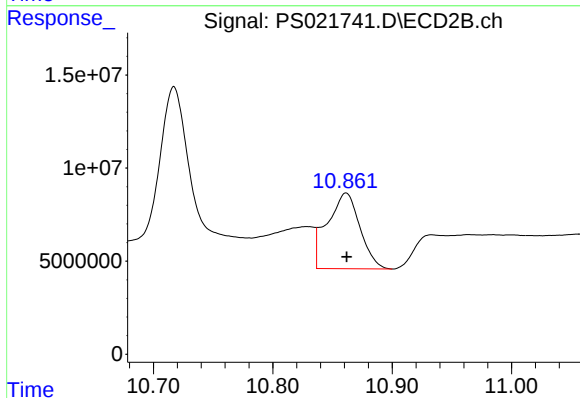


#15 Picloram

R.T.: 10.861 min
Delta R.T.: 0.000 min
Response: 77423931
Conc: 4.37 ng/ml

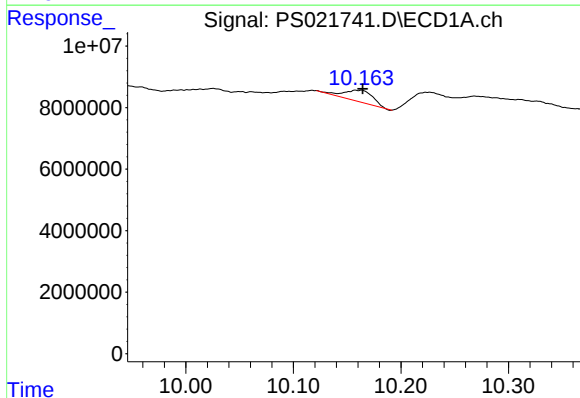

#16 DCPA

R.T.: 10.159 min
Delta R.T.: -0.006 min
Response: 6922579
Conc: N.D.

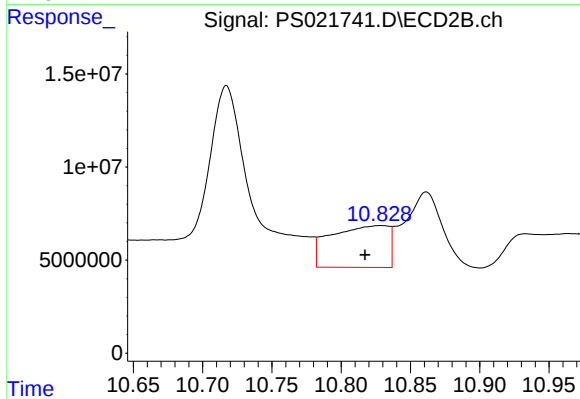

#16 DCPA

R.T.: 10.829 min
Delta R.T.: 0.011 min
Response: 65143374
Conc: 4.67 ng/ml