

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS011323\
 Data File : PS021742.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Jan 2023 08:50
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 15 20:18:53 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010923.M
 Quant Title : 8080.M
 QLast Update : Tue Jan 10 10:34:52 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.377	6.810	1537.4E6	1117.8E6	552.301	622.119
Target Compounds							
1) T	Dalapon	2.519	2.596	663610	534774	<MDL	<MDL #
3) T	4-Nitroph...	6.220	0.000	7739274	0	5.310	N.D. #
5) T	DICAMBA	0.000	7.030f	0	4063756	N.D.	<MDL
6) T	MCP	0.000	7.030f	0	4063756	N.D.	<MDL
7) T	MCPA	6.754f	0.000	6017244	0	<MDL	N.D. #
8) T	DICHLORPROP	7.135	7.648f	543394	2301882	<MDL	1.079 #
9) T	2,4-D	7.305	0.000	12007134	0	3.092	N.D. #
10) T	Pentachlo...	7.548	8.319	2560457	1174058	<MDL	<MDL #
11) T	2,4,5-TP ...	8.082	8.684	6249425	1263123	<MDL	<MDL #
12) T	2,4,5-T	8.368	9.080	7685745	2597430	<MDL	<MDL #
13) T	2,4-DB	8.824	0.000	511968	0	<MDL	N.D. #
14) T	DINOSEB	0.000	9.894	0	1113542	N.D.	<MDL
15) T	Picloram	9.723	10.819f	31729890	21120833	1.119	1.193
16) T	DCPA	10.161	10.819	2797242	21120833	<MDL	1.515 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS011323\
Data File : PS021742.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Jan 2023 08:50
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 15 20:18:53 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010923.M
Quant Title : 8080.M
QLast Update : Tue Jan 10 10:34:52 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

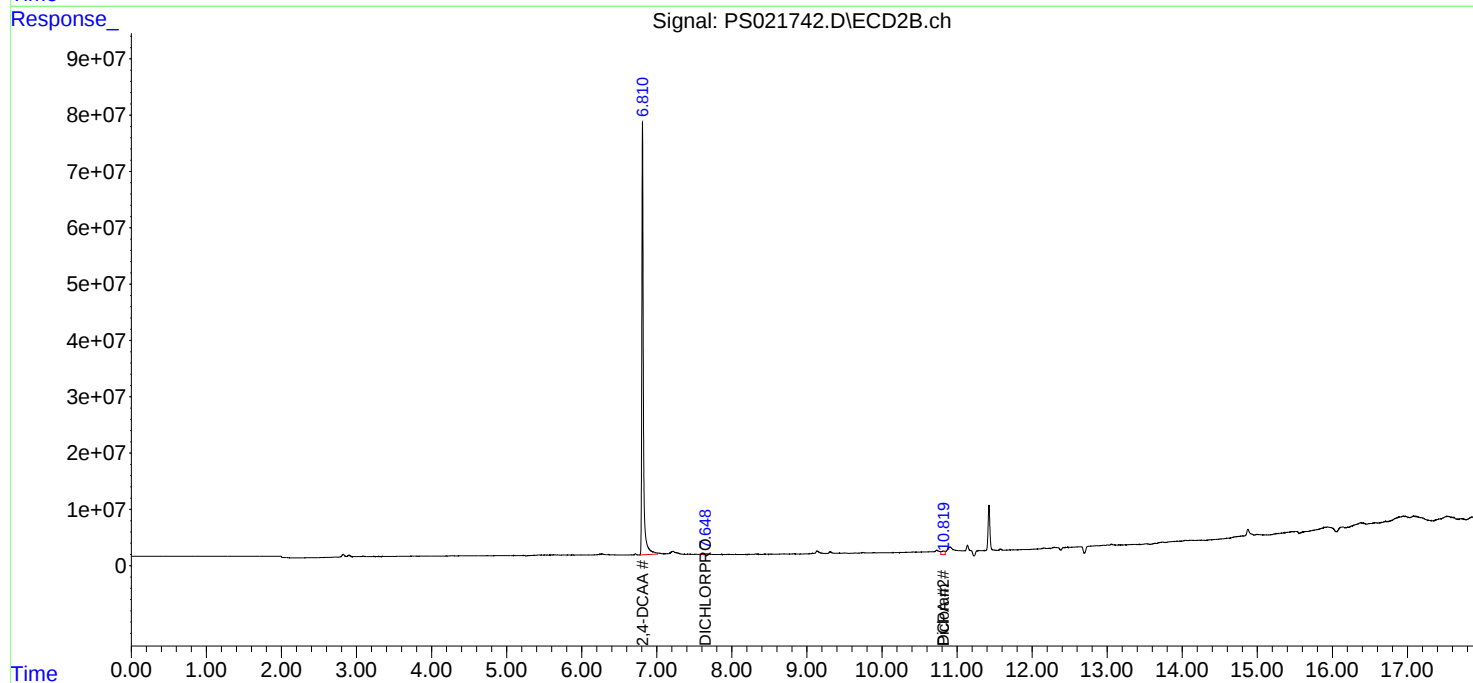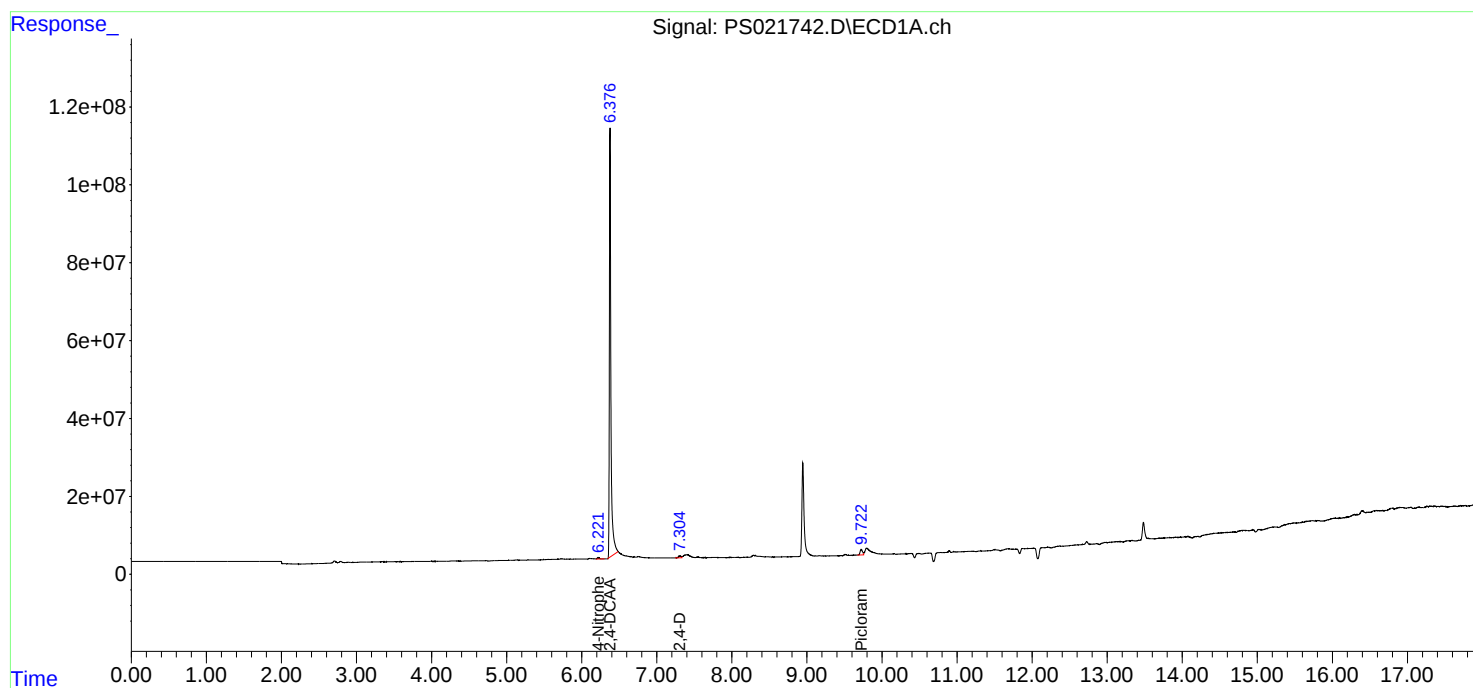


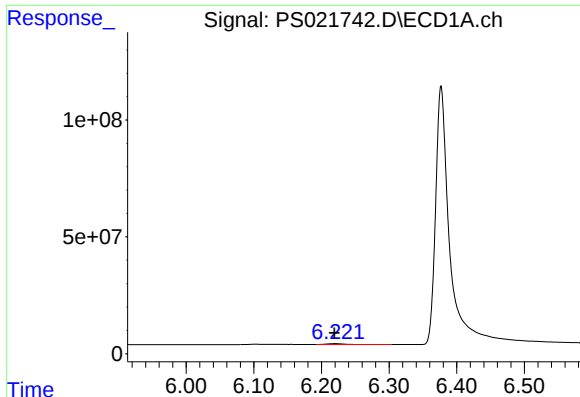

#3 4-Nitrophenol


R.T.: 6.220 min
Delta R.T.: 0.001 min
Response: 7739274
Conc: 5.31 ng/ml

Instrument :
ECD_S
ClientSampleId :

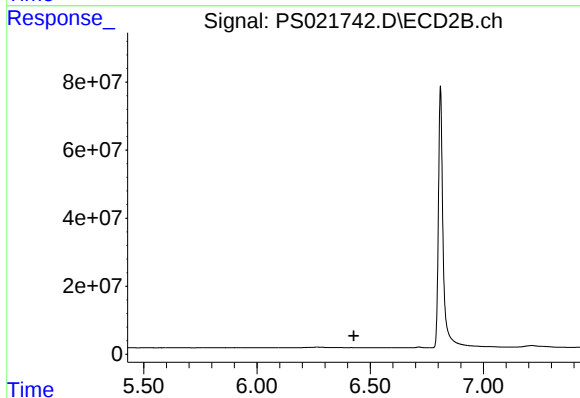


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.428 min
Response: 0
Conc: N.D.

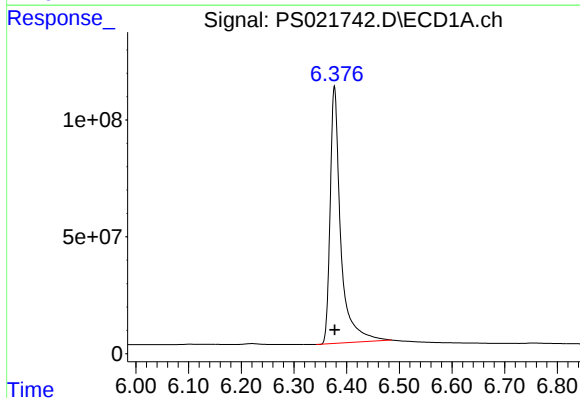


#4 2,4-DCAA

R.T.: 6.377 min
Delta R.T.: 0.000 min
Response: 1537365243
Conc: 552.30 ng/ml

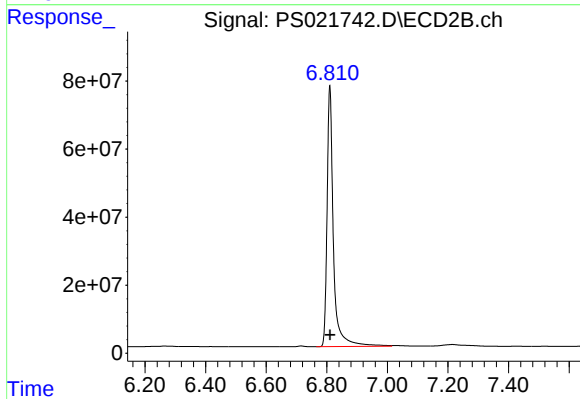

#4 2,4-DCAA


R.T.: 6.810 min
Delta R.T.: -0.001 min
Response: 1117754582
Conc: 622.12 ng/ml

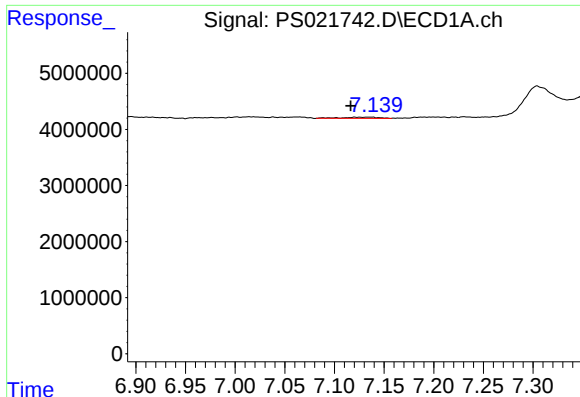

#8 DICHLORPROP


R.T.: 7.135 min
Delta R.T.: 0.019 min
Response: 543394
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

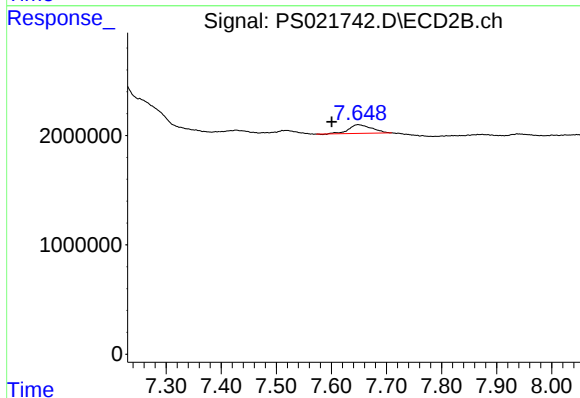


#8 DICHLORPROP

R.T.: 7.648 min
Delta R.T.: 0.048 min
Response: 2301882
Conc: 1.08 ng/ml

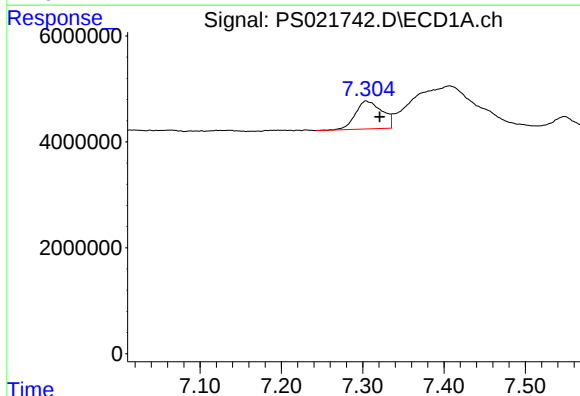


#9 2,4-D

R.T.: 7.305 min
Delta R.T.: -0.016 min
Response: 12007134
Conc: 3.09 ng/ml

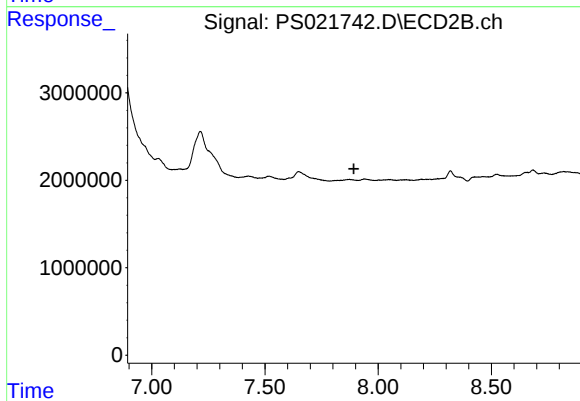

#9 2,4-D


R.T.: 0.000 min
Exp R.T. : 7.893 min
Response: 0
Conc: N.D.

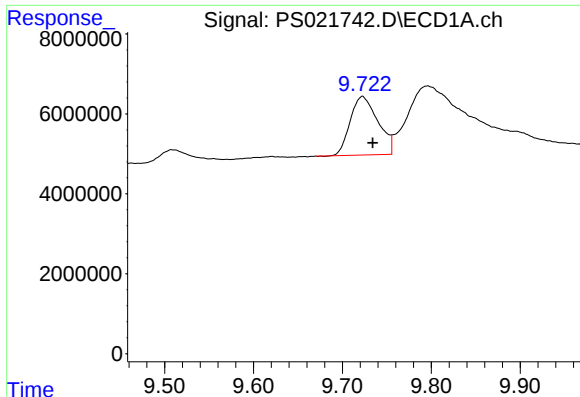

#15 Picloram


R.T.: 9.723 min
Delta R.T.: -0.011 min
Response: 31729890
Conc: 1.12 ng/ml

Instrument :
ECD_S
ClientSampleId :

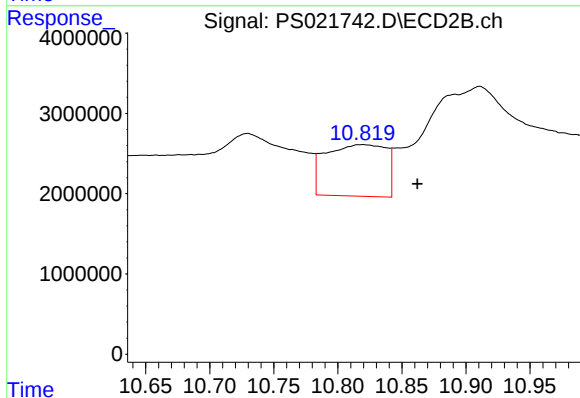


#15 Picloram

R.T.: 10.819 min
Delta R.T.: -0.043 min
Response: 21120833
Conc: 1.19 ng/ml

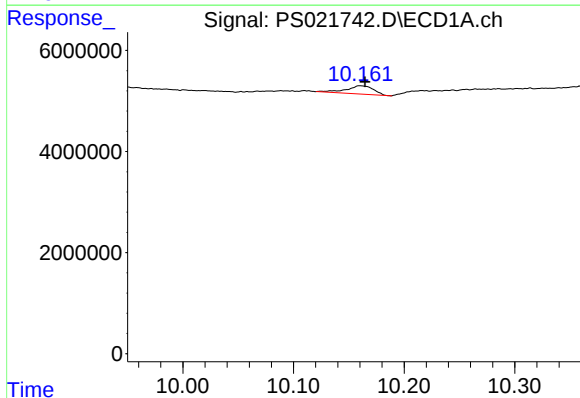

#16 DCPA

R.T.: 10.161 min
Delta R.T.: -0.003 min
Response: 2797242
Conc: N.D.

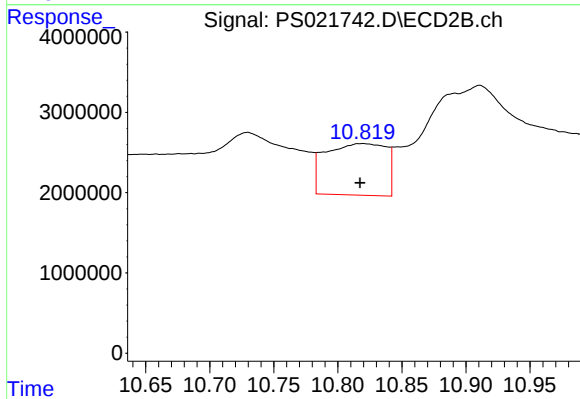

#16 DCPA

R.T.: 10.819 min
Delta R.T.: 0.002 min
Response: 21120833
Conc: 1.52 ng/ml