

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS011323\
 Data File : PS021750.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Jan 2023 18:50
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 15 20:25:43 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010923.M
 Quant Title : 8080.M
 QLast Update : Tue Jan 10 10:34:52 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.377	6.811	1579.8E6	1139.7E6	567.553	634.312
Target Compounds							
1) T	Dalapon	2.527f	0.000	717414	0	<MDL	N.D. #
3) T	4-Nitroph...	6.220	0.000	8706200	0	5.973	N.D. #
5) T	DICAMBA	0.000	7.032f	0	7399134	N.D.	<MDL
6) T	MCP	0.000	7.032f	0	7399134	N.D.	1.116
7) T	MCPA	6.756f	7.257	8707732	12116124	<MDL	1.336 #
8) T	DICHLORPROP	7.129	7.650f	580730	5262420	<MDL	2.467 #
9) T	2,4-D	7.307	0.000	10395040	0	2.677	N.D. #
10) T	Pentachlo...	7.547	8.319	2931700	3525924	<MDL	<MDL #
11) T	2,4,5-TP ...	8.085	8.684	11376180	2506145	<MDL	<MDL #
12) T	2,4,5-T	8.371	9.078	20385083	6031169	1.058	<MDL #
13) T	2,4-DB	8.825	9.591	397972	1347990	<MDL	<MDL #
14) T	DINOSEB	9.893	9.895	6594857	1344916	<MDL	<MDL #
15) T	Picloram	9.721	10.858	35066662	18538807	1.236	1.047
16) T	DCPA	10.161	10.817	3895497	35187393	<MDL	2.524 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS011323\
Data File : PS021750.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Jan 2023 18:50
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 15 20:25:43 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010923.M
Quant Title : 8080.M
QLast Update : Tue Jan 10 10:34:52 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

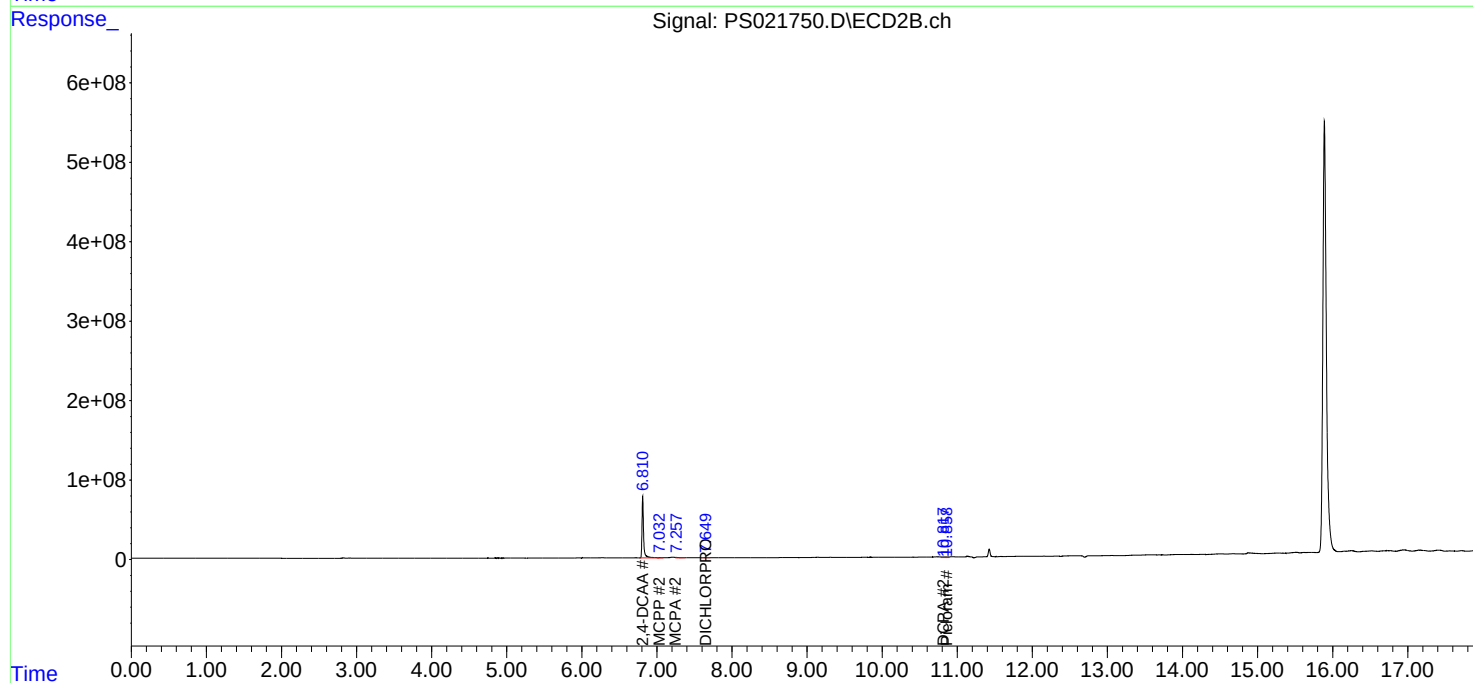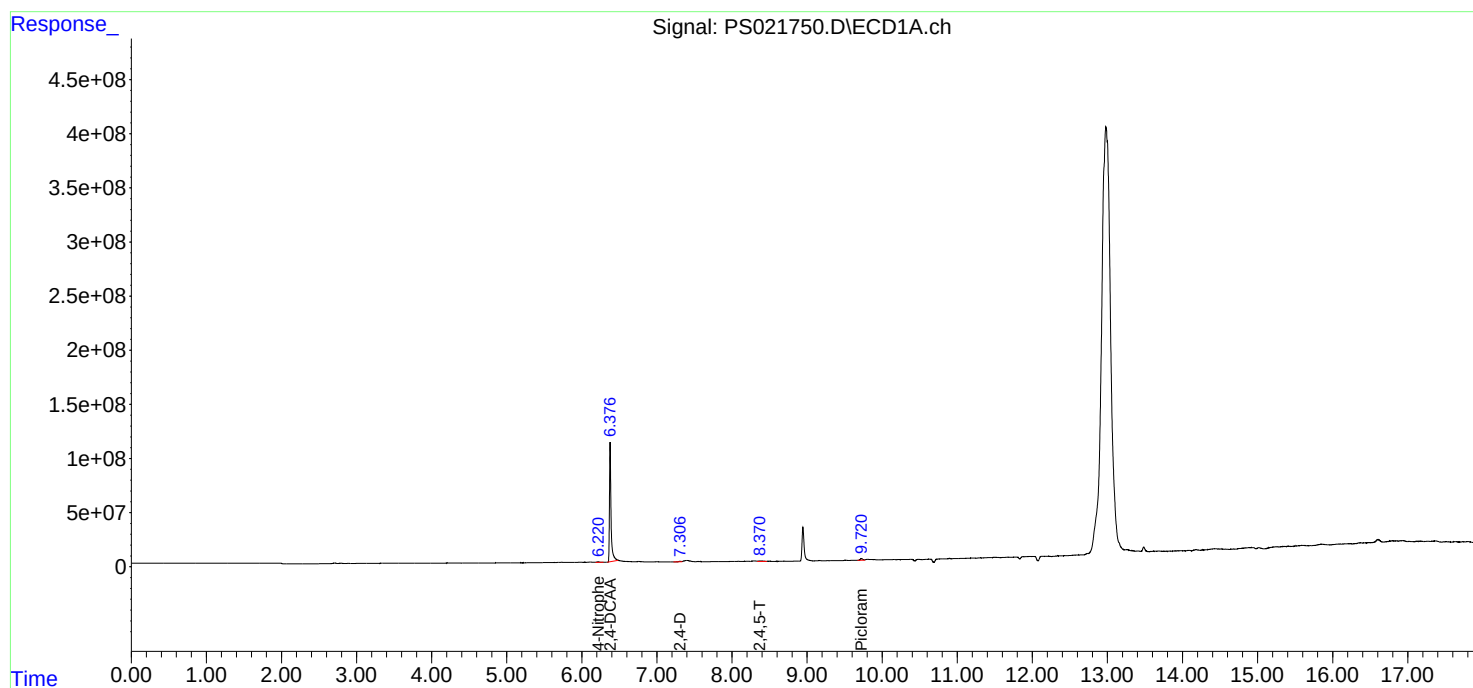


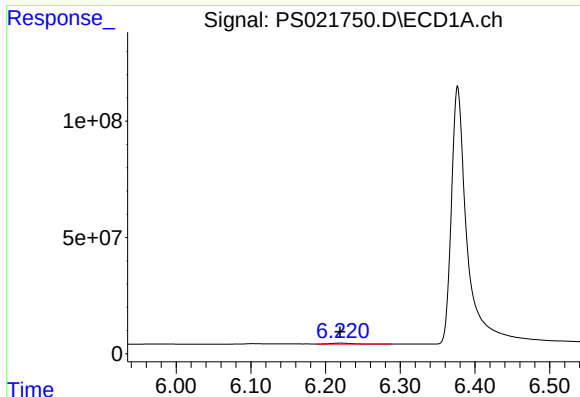

#3 4-Nitrophenol


R.T.: 6.220 min
Delta R.T.: 0.000 min
Response: 8706200
Conc: 5.97 ng/ml

Instrument :
ECD_S
ClientSampleId :

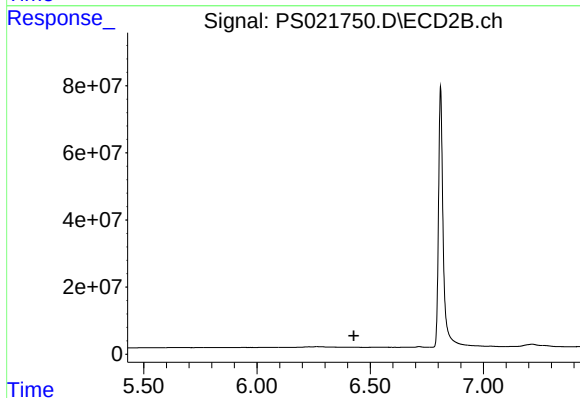


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.428 min
Response: 0
Conc: N.D.

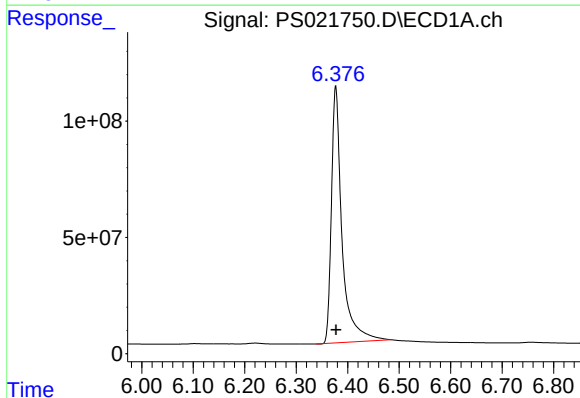


#4 2,4-DCAA

R.T.: 6.377 min
Delta R.T.: 0.000 min
Response: 1579821753
Conc: 567.55 ng/ml

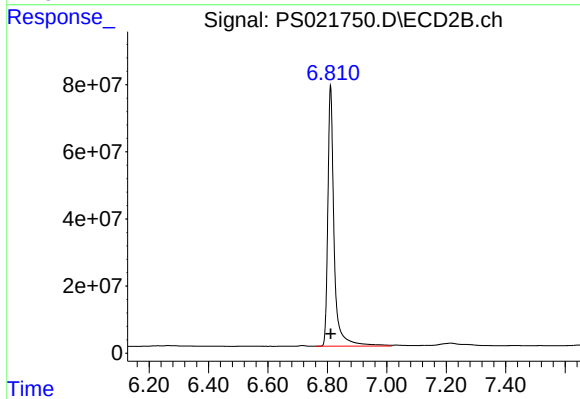

#4 2,4-DCAA


R.T.: 6.811 min
Delta R.T.: 0.000 min
Response: 1139661712
Conc: 634.31 ng/ml

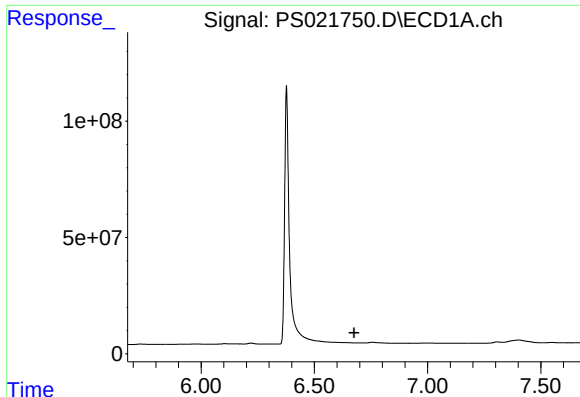

#6 MCPP


R.T.: 0.000 min
Exp R.T.: 6.675 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

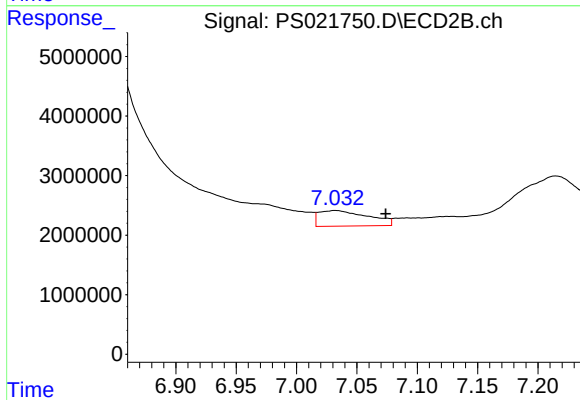


#6 MCPP

R.T.: 7.032 min
Delta R.T.: -0.042 min
Response: 7399134
Conc: 1.12 ug/ml

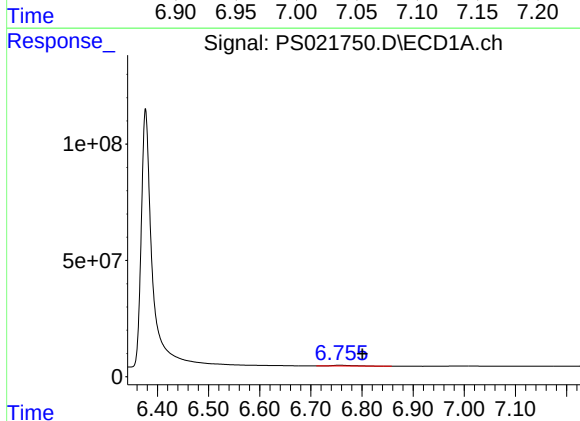


#7 MCPA

R.T.: 6.756 min
Delta R.T.: -0.045 min
Response: 8707732
Conc: N.D.

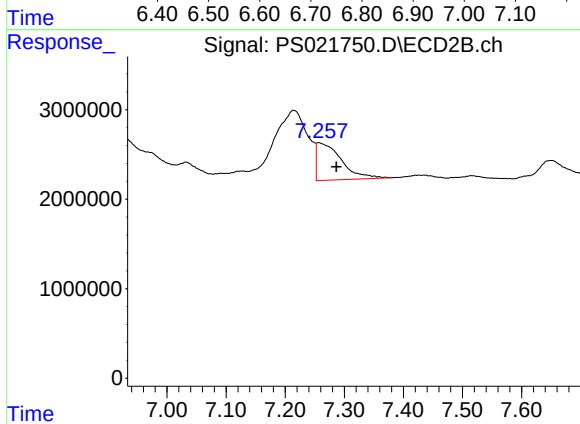

#7 MCPA


R.T.: 7.257 min
Delta R.T.: -0.030 min
Response: 12116124
Conc: 1.34 ug/ml

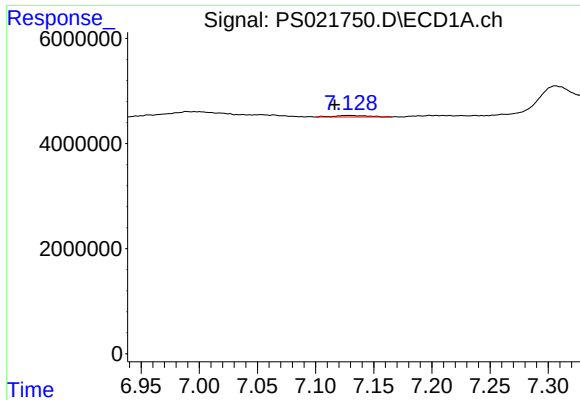

#8 DICHLORPROP


R.T.: 7.129 min
Delta R.T.: 0.012 min
Response: 580730
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

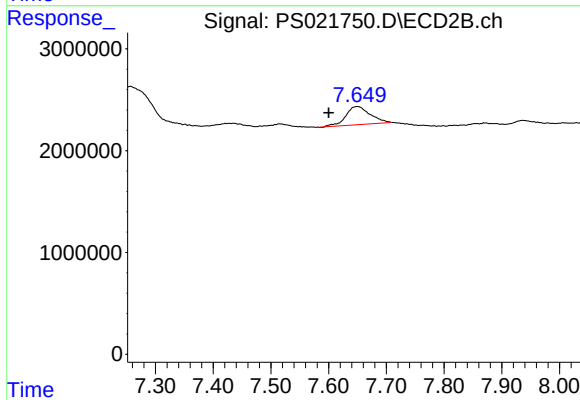


#8 DICHLORPROP

R.T.: 7.650 min
Delta R.T.: 0.050 min
Response: 5262420
Conc: 2.47 ng/ml

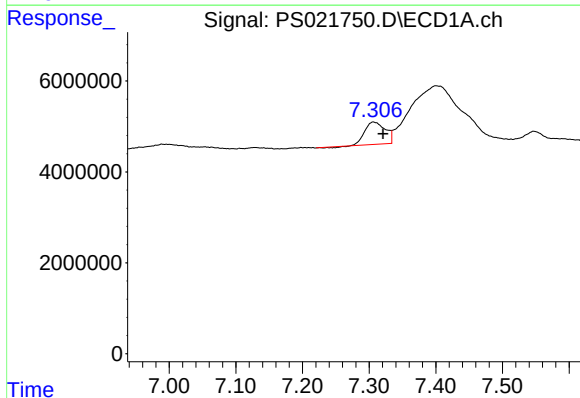


#9 2,4-D

R.T.: 7.307 min
Delta R.T.: -0.014 min
Response: 10395040
Conc: 2.68 ng/ml

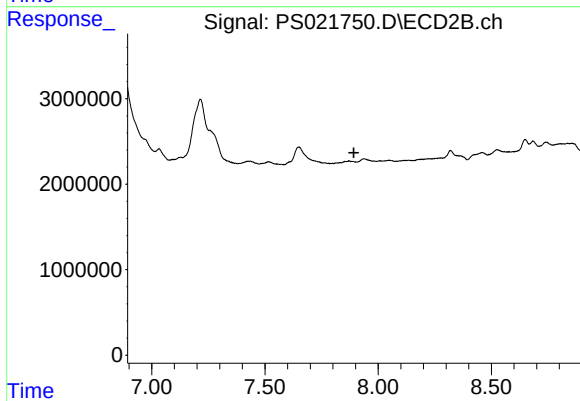

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 7.893 min
Response: 0
Conc: N.D.

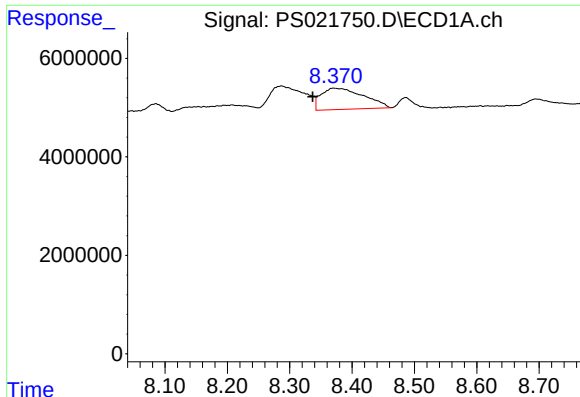

#12 2,4,5-T


R.T.: 8.371 min
Delta R.T.: 0.034 min
Response: 20385083
Conc: 1.06 ng/ml

Instrument :
ECD_S
ClientSampleId :

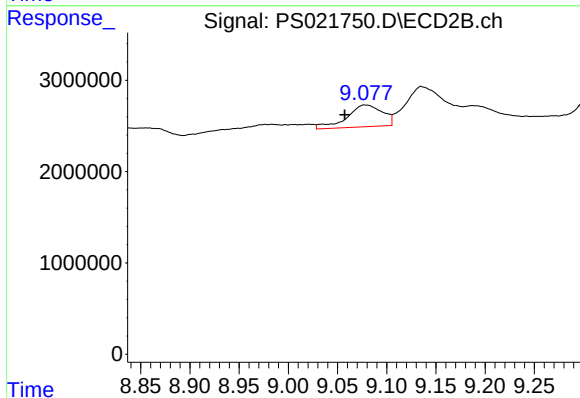


#12 2,4,5-T

R.T.: 9.078 min
Delta R.T.: 0.020 min
Response: 6031169
Conc: N.D.

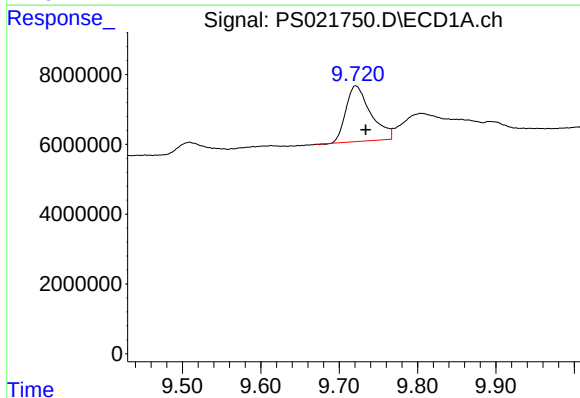


#15 Picloram

R.T.: 9.721 min
Delta R.T.: -0.013 min
Response: 35066662
Conc: 1.24 ng/ml

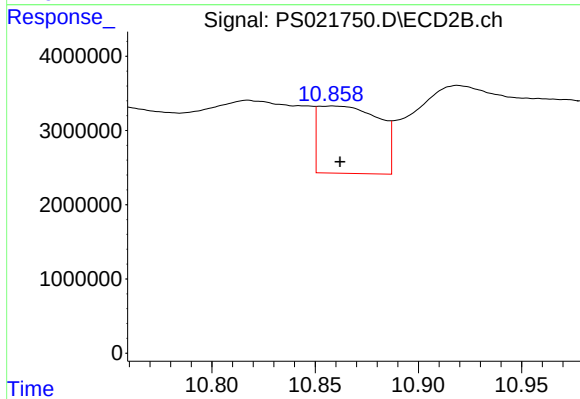

#15 Picloram


R.T.: 10.858 min
Delta R.T.: -0.004 min
Response: 18538807
Conc: 1.05 ng/ml

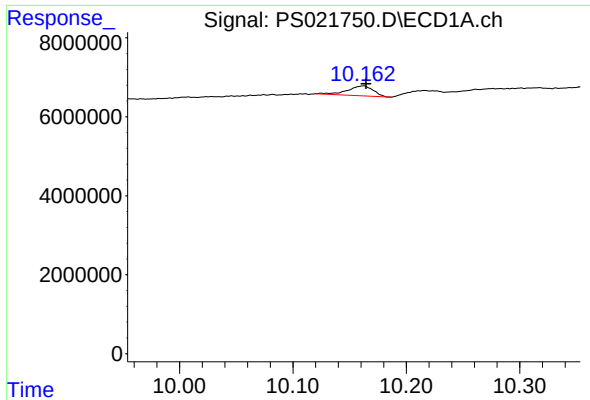

#16 DCPA

R.T.: 10.161 min
Delta R.T.: -0.003 min
Response: 3895497
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

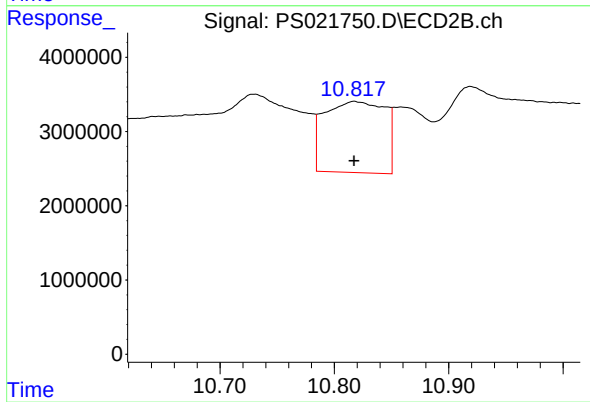

#16 DCPA

R.T.: 10.817 min
Delta R.T.: 0.000 min
Response: 35187393
Conc: 2.52 ng/ml