

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS011420\
 Data File : PS008402.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Jan 2020 11:08
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 14 23:46:54 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010820.M
 Quant Title : 8080.M
 QLast Update : Wed Jan 08 11:00:59 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.275	5.967	919.9E6	464.2E6	521.005	489.897
Target Compounds							
12) T	2,4,5-T	0.000	8.281	0	28854187	N.D.	5.456
15) T	Picloram	10.060	10.052	178.2E6	104.8E6	14.277	14.111
16) T	DCPA	0.000	10.052	0	104.8E6	N.D.	16.087



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS011420\
Data File : PS008402.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Jan 2020 11:08
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 14 23:46:54 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010820.M
Quant Title : 8080.M
QLast Update : Wed Jan 08 11:00:59 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

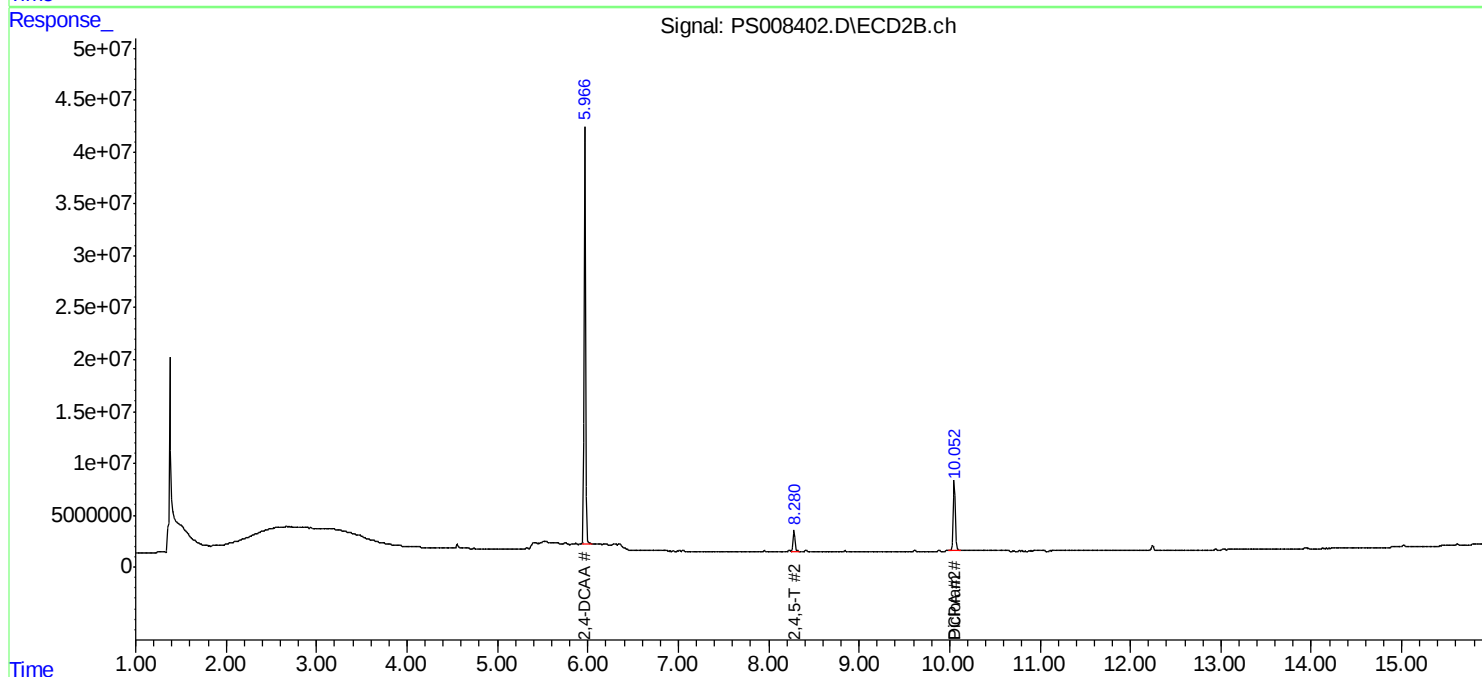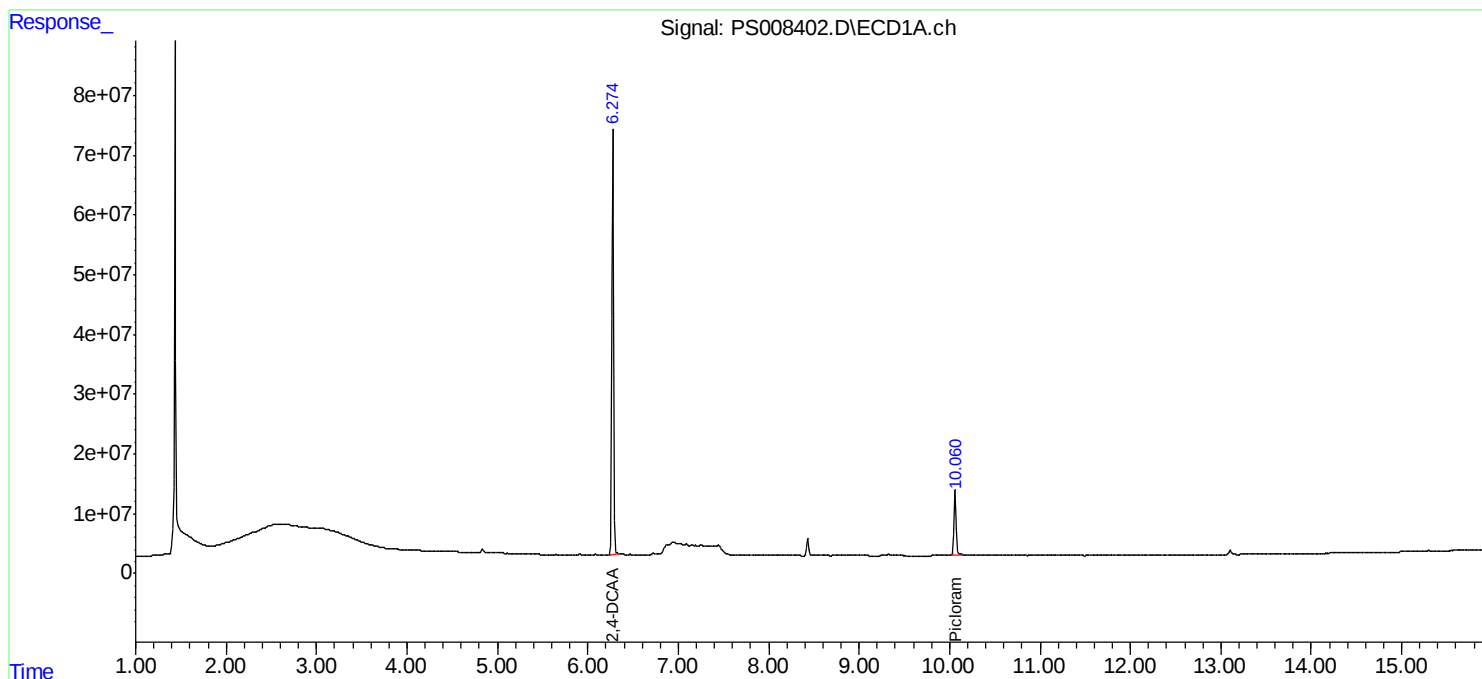


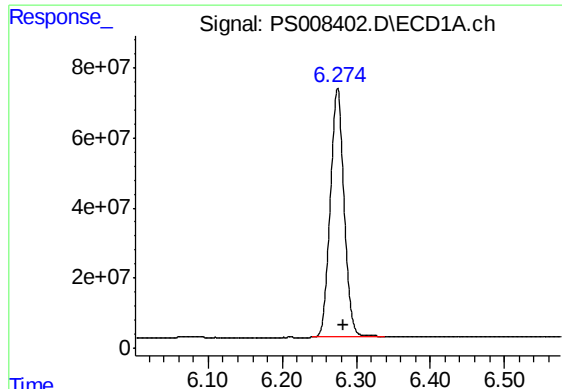

#4 2,4-DCAA


R.T.: 6.275 min
Delta R.T.: -0.008 min
Response: 919939770
Conc: 521.00 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

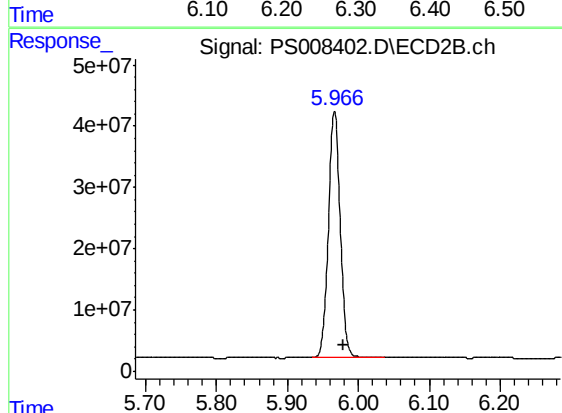


#4 2,4-DCAA

R.T.: 5.967 min
Delta R.T.: -0.013 min
Response: 464159357
Conc: 489.90 ng/ml

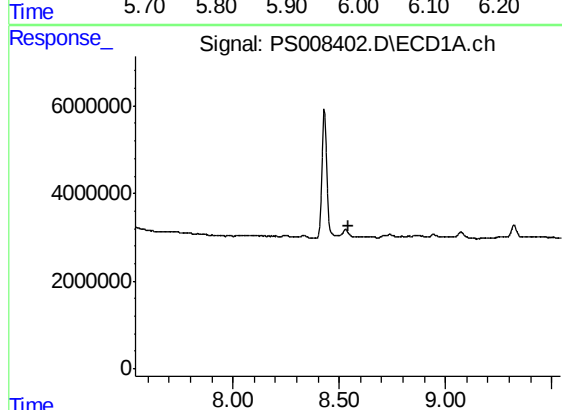


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 8.541 min
Response: 0
Conc: N.D.

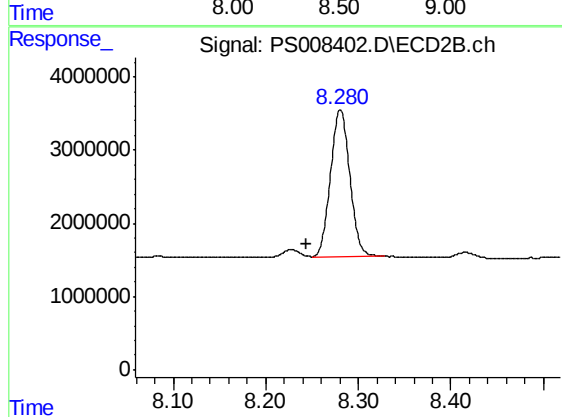

#12 2,4,5-T


R.T.: 8.281 min
Delta R.T.: 0.037 min
Response: 28854187
Conc: 5.46 ng/ml

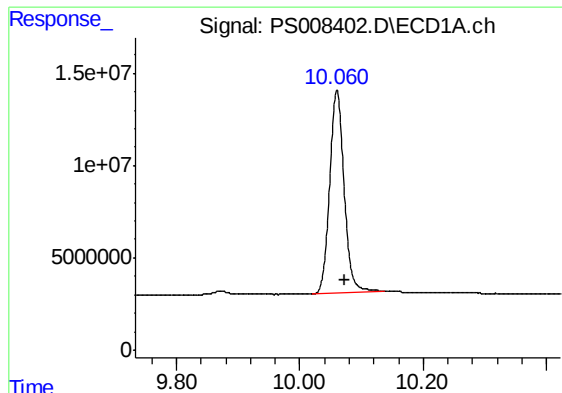

#15 Picloram


R.T.: 10.060 min
Delta R.T.: -0.013 min
Response: 178203497
Conc: 14.28 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

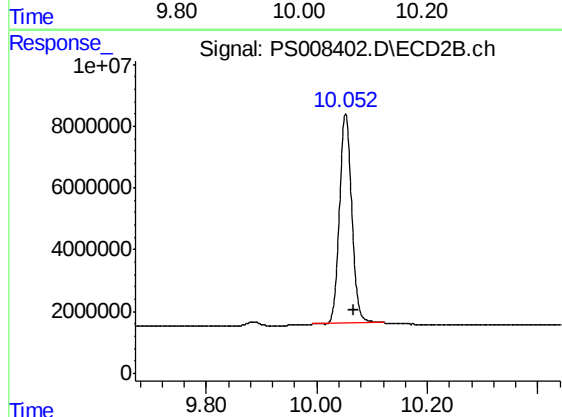


#15 Picloram

R.T.: 10.052 min
Delta R.T.: -0.016 min
Response: 104835230
Conc: 14.11 ng/ml

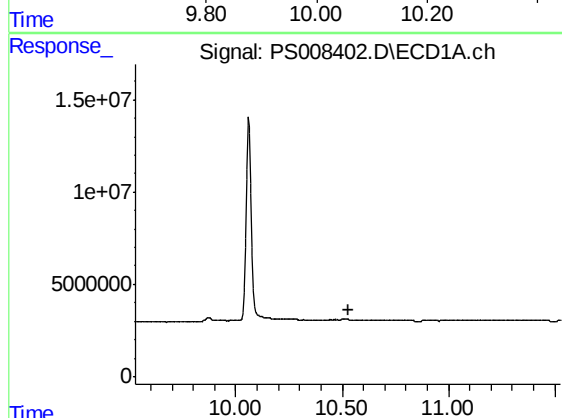

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 10.527 min
Response: 0
Conc: N.D.

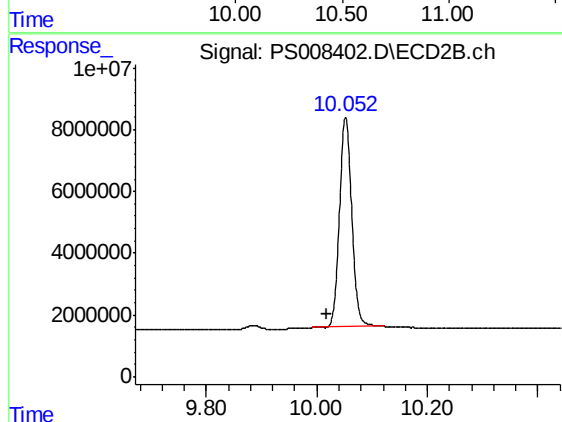

#16 DCPA

R.T.: 10.052 min
Delta R.T.: 0.033 min
Response: 104835230
Conc: 16.09 ng/ml