

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS011421\
 Data File : PS013774.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Jan 2021 22:12
 Operator : DD\AJ
 Sample : HSTDCCC750
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 15 00:31:48 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010421.M
 Quant Title : 8080.M
 QLast Update : Tue Jan 05 01:51:07 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.206	6.908	780.1E6	299.7E6	816.386	745.371
Target Compounds							
1) T	Dalapon	3.030	2.622	774.3E6	337.4E6	711.953	648.838
2) T	3,5-DICHL...	6.423	6.064	1005.0E6	437.4E6	759.949	694.318
3) T	4-Nitroph...	7.041	6.522	355.0E6	176.3E6	746.671	695.330
5) T	DICAMBA	7.396	7.074	3022.8E6	1225.7E6	784.917	713.700
6) T	MCPD	7.563	7.169	226.1E6	99994375	78.917	70.760
7) T	MCPA	7.712	7.384	318.7E6	140.7E6	77.544	69.605
8) T	DICHLORPROP	8.086	7.700	747.9E6	315.2E6	772.681	707.757
9) T	2,4-D	8.319	7.997	863.2E6	388.2E6	814.841	700.147
10) T	Pentachlo...	8.625	8.421	10975.6E6	4122.8E6	774.715	713.209
11) T	2,4,5-TP ...	9.173	8.782	4386.9E6	1713.8E6	787.811	717.427
12) T	2,4,5-T	9.461	9.164	4407.9E6	1649.2E6	779.521	720.407
13) T	2,4-DB	10.015	9.670	745.5E6	217.3E6	762.991	714.434
14) T	DINOSEB	11.166	9.997	3381.2E6	1188.8E6	766.397	710.464
15) T	Picloram	11.003	10.993	5278.1E6	2252.4E6	730.768	648.074
16) T	DCPA	11.431	10.924	5598.7E6	2237.1E6	792.424	722.809



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS011421\
Data File : PS013774.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Jan 2021 22:12
Operator : DD\AJ
Sample : HSTDCCC750
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 15 00:31:48 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010421.M
Quant Title : 8080.M
QLast Update : Tue Jan 05 01:51:07 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

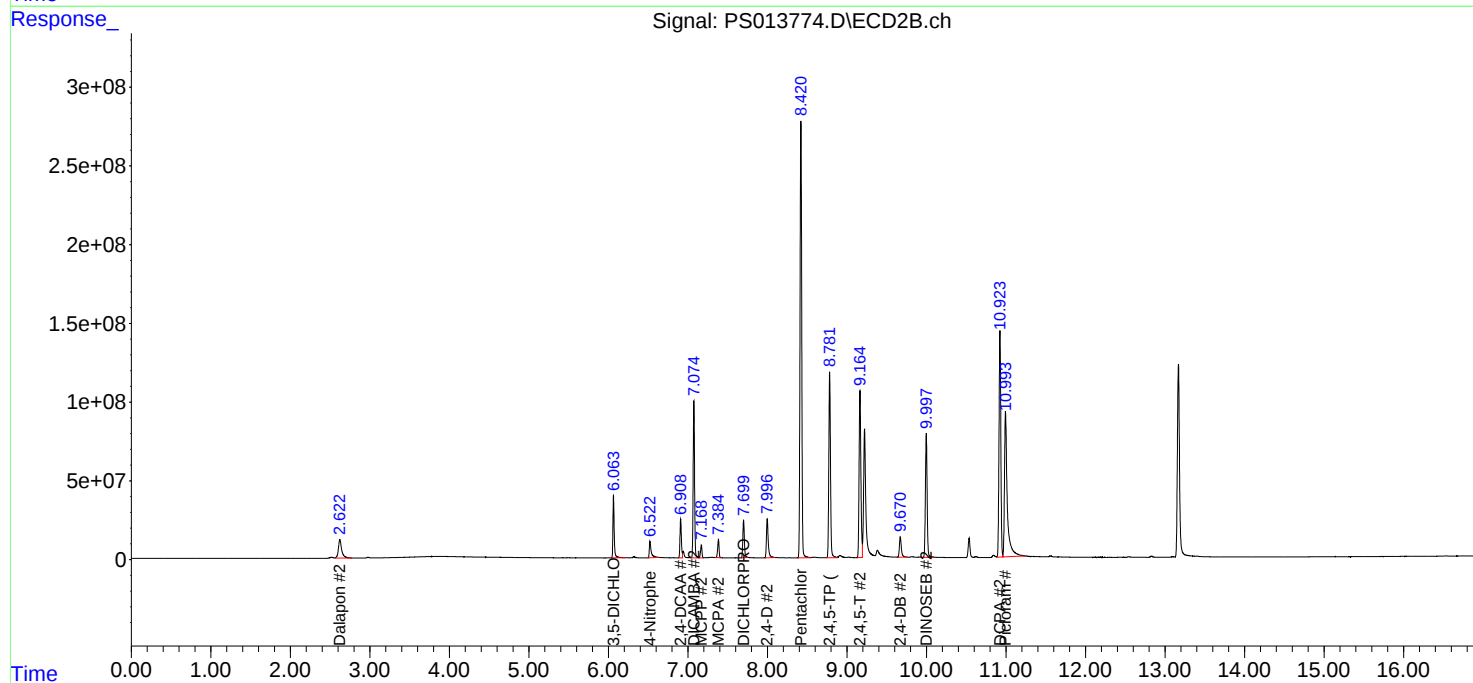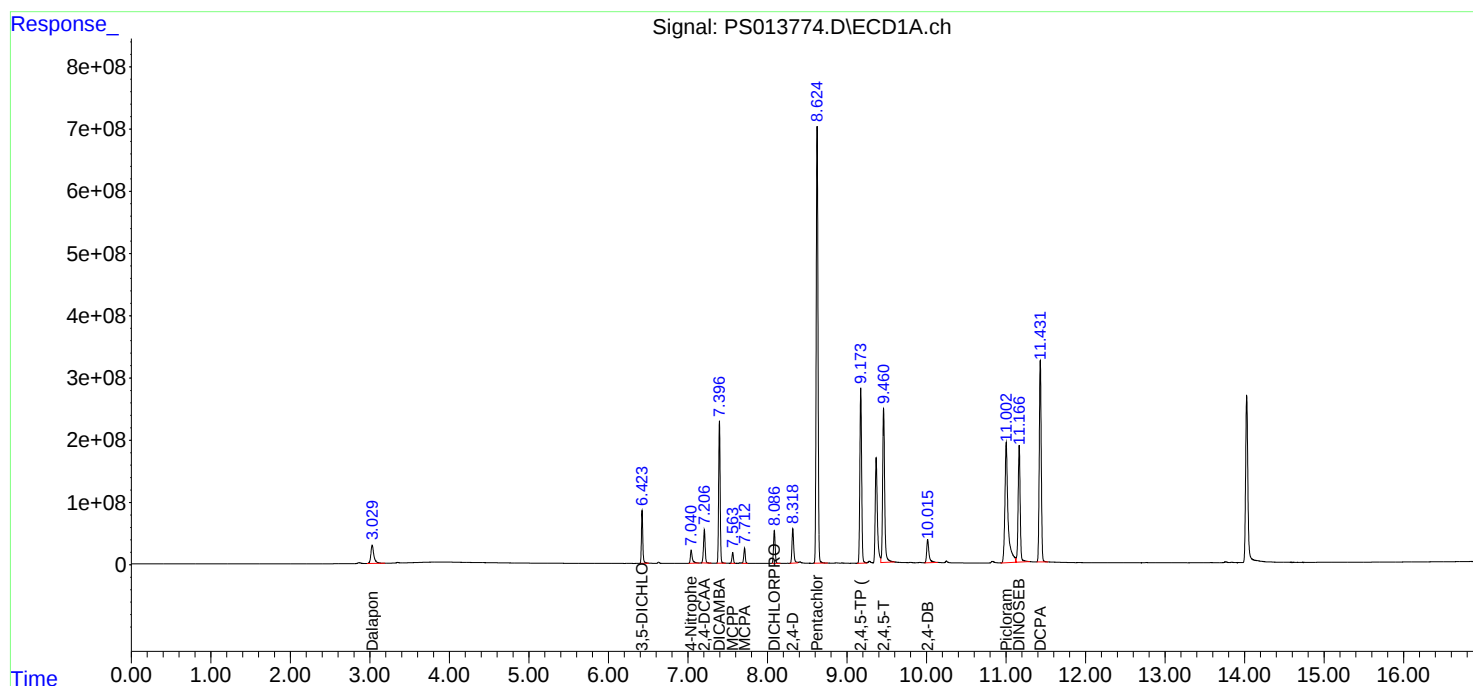


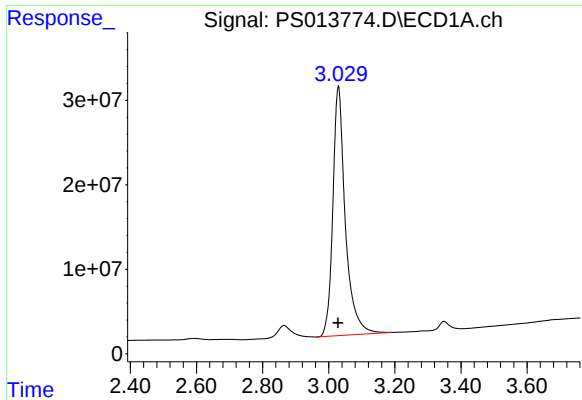

#1 Dalapon


R.T.: 3.030 min
Delta R.T.: 0.000 min
Response: 774337452
Conc: 711.95 ng/ml

Instrument :
ECD_S
ClientSampleId :

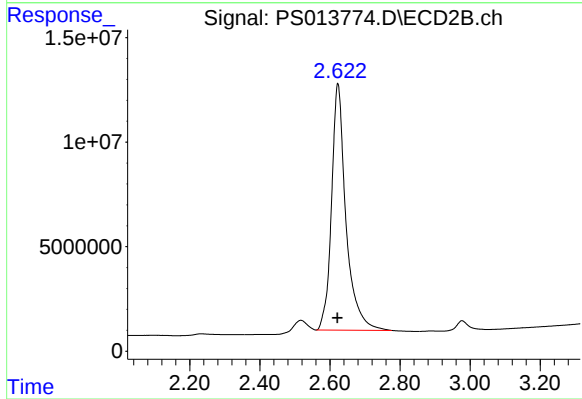


#1 Dalapon

R.T.: 2.622 min
Delta R.T.: 0.001 min
Response: 337362977
Conc: 648.84 ng/ml

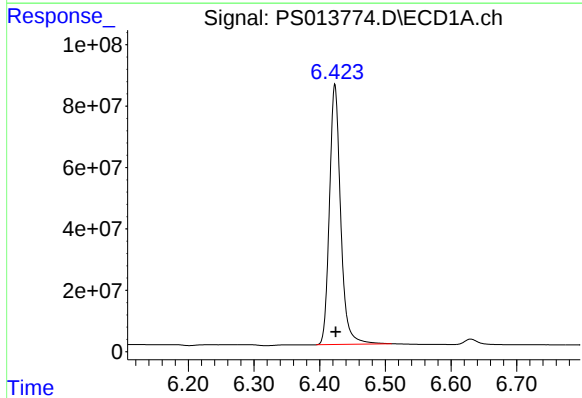


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.423 min
Delta R.T.: -0.001 min
Response: 1004967114
Conc: 759.95 ng/ml

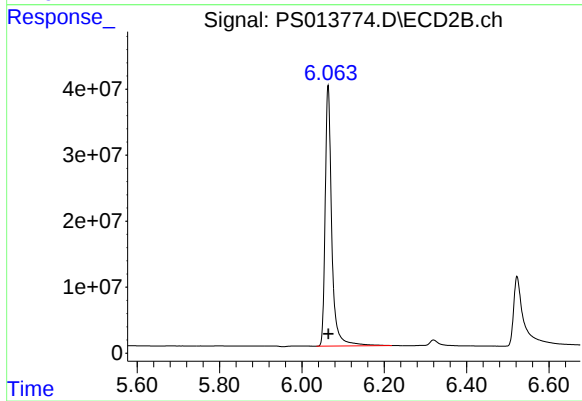

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.064 min
Delta R.T.: 0.000 min
Response: 437422179
Conc: 694.32 ng/ml

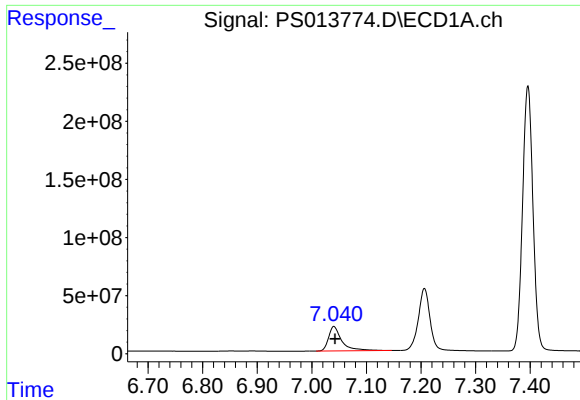

#3 4-Nitrophenol


R.T.: 7.041 min
Delta R.T.: -0.002 min
Response: 354992652
Conc: 746.67 ng/ml

Instrument :
ECD_S
ClientSampleId :

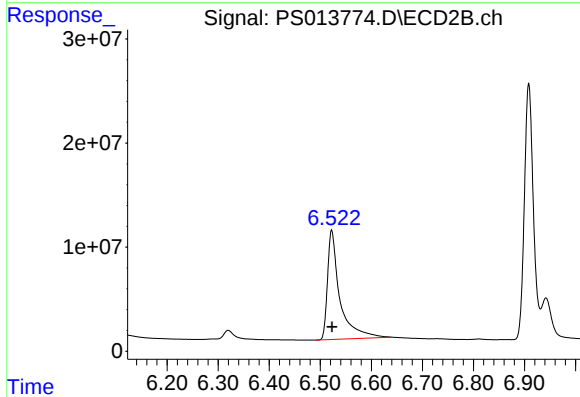


#3 4-Nitrophenol

R.T.: 6.522 min
Delta R.T.: 0.000 min
Response: 176342882
Conc: 695.33 ng/ml

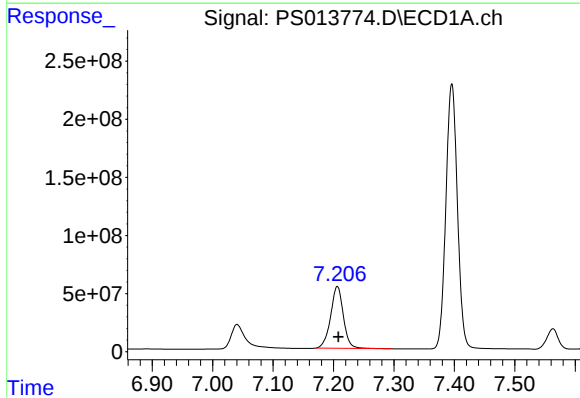


#4 2,4-DCAA

R.T.: 7.206 min
Delta R.T.: -0.002 min
Response: 780132960
Conc: 816.39 ng/ml

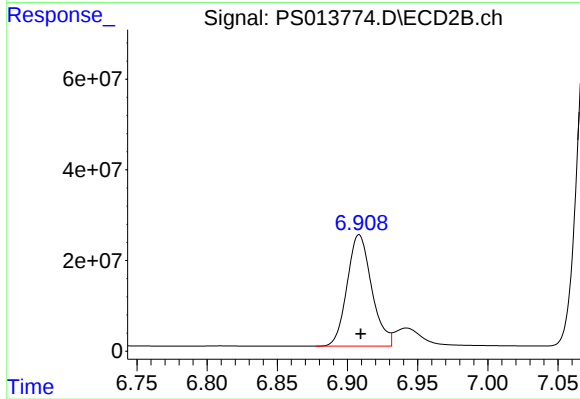

#4 2,4-DCAA


R.T.: 6.908 min
Delta R.T.: -0.001 min
Response: 299724887
Conc: 745.37 ng/ml

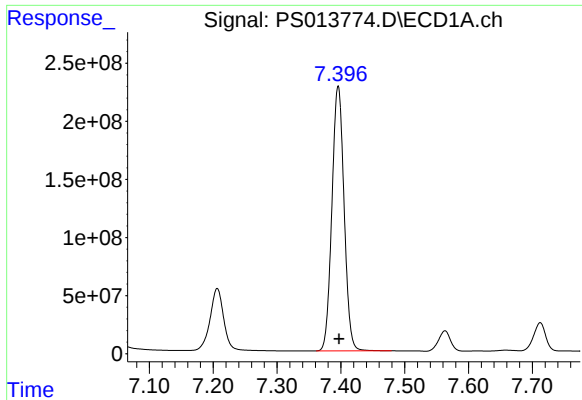

#5 DICAMBA


R.T.: 7.396 min
Delta R.T.: -0.002 min
Response: 3022754829
Conc: 784.92 ng/ml

Instrument :
ECD_S
ClientSampleId :

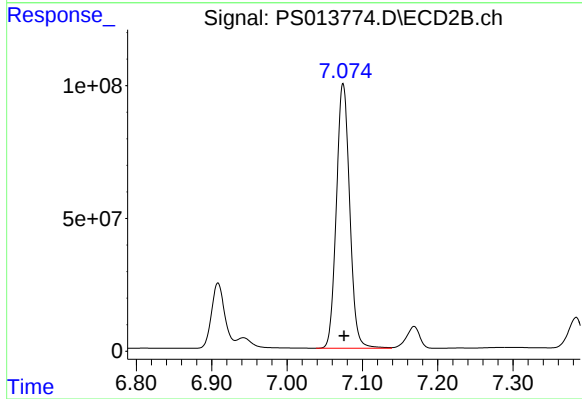


#5 DICAMBA

R.T.: 7.074 min
Delta R.T.: -0.001 min
Response: 1225676717
Conc: 713.70 ng/ml

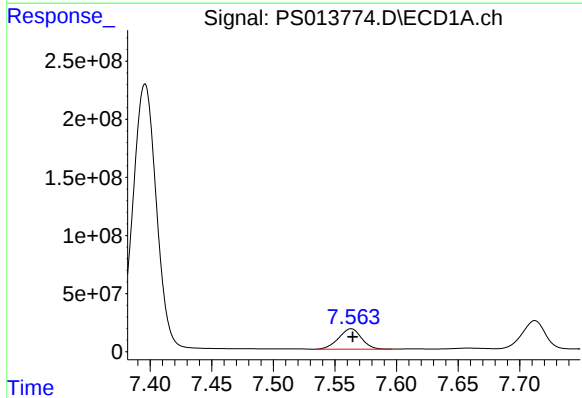


#6 MCP

R.T.: 7.563 min
Delta R.T.: -0.001 min
Response: 226065209
Conc: 78.92 ug/ml

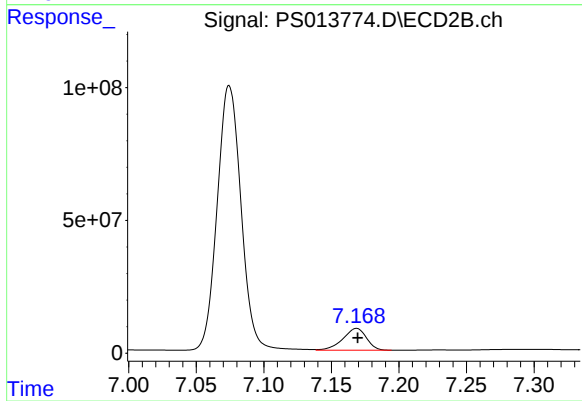

#6 MCP


R.T.: 7.169 min
Delta R.T.: 0.000 min
Response: 99994375
Conc: 70.76 ug/ml

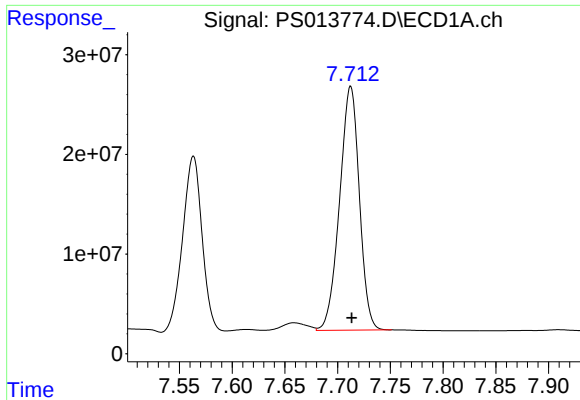

#7 MCPA


R.T.: 7.712 min
Delta R.T.: -0.001 min
Response: 318722206
Conc: 77.54 ug/ml

Instrument :
ECD_S
ClientSampleId :

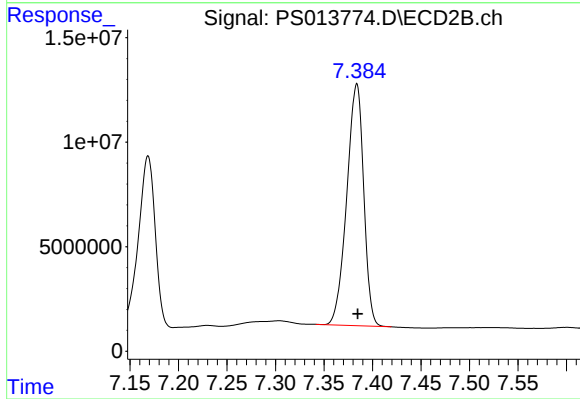


#7 MCPA

R.T.: 7.384 min
Delta R.T.: 0.000 min
Response: 140719080
Conc: 69.60 ug/ml

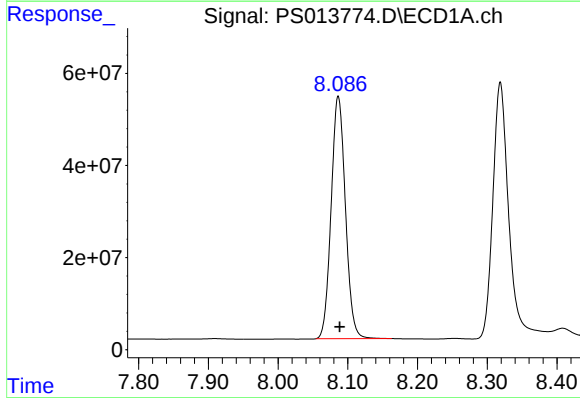


#8 DICHLORPROP

R.T.: 8.086 min
Delta R.T.: -0.002 min
Response: 747937111
Conc: 772.68 ng/ml

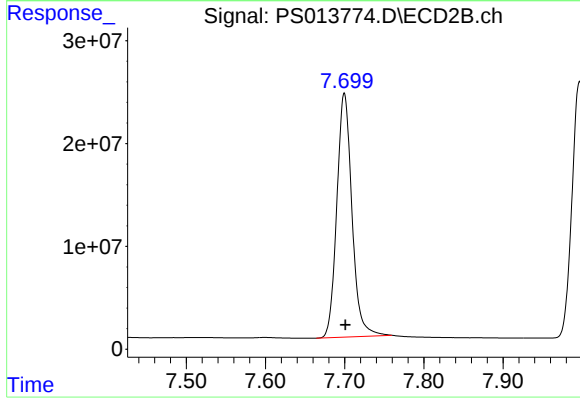

#8 DICHLORPROP


R.T.: 7.700 min
Delta R.T.: -0.001 min
Response: 315180204
Conc: 707.76 ng/ml

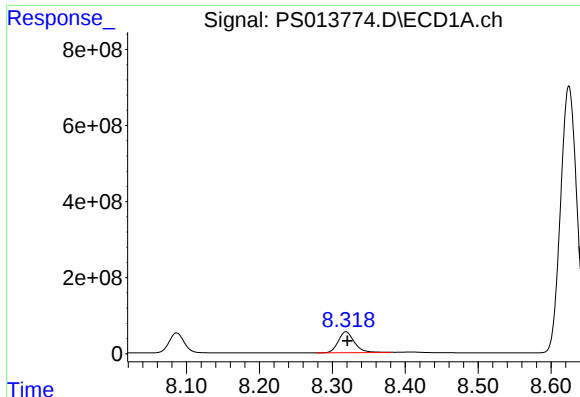

#9 2,4-D


R.T.: 8.319 min
Delta R.T.: -0.002 min
Response: 863162753
Conc: 814.84 ng/ml

Instrument :
ECD_S
ClientSampleId :

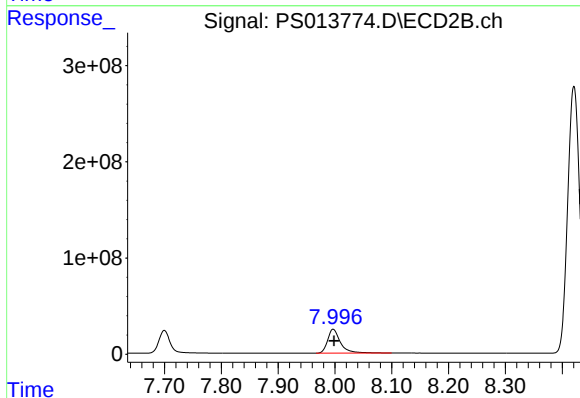


#9 2,4-D

R.T.: 7.997 min
Delta R.T.: -0.002 min
Response: 388161645
Conc: 700.15 ng/ml

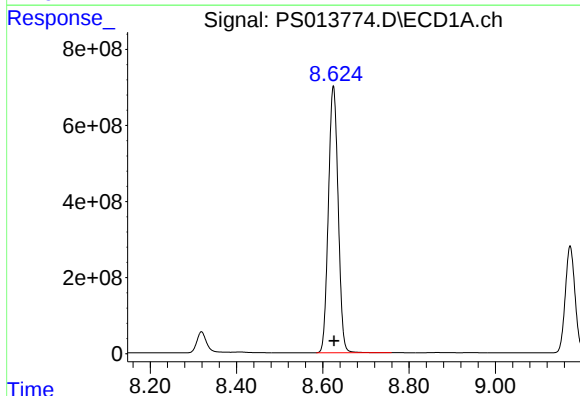


#10 Pentachlorophenol

R.T.: 8.625 min
Delta R.T.: -0.002 min
Response: 10975561842
Conc: 774.72 ng/ml

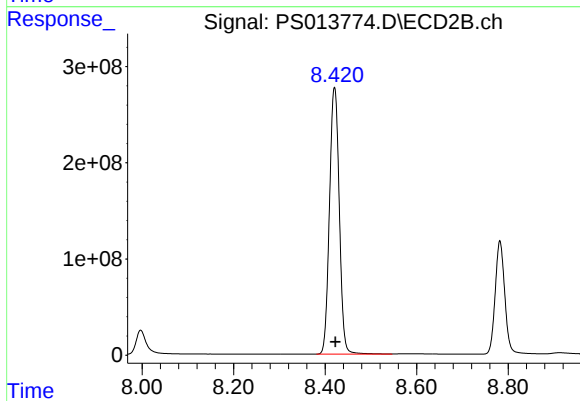

#10 Pentachlorophenol


R.T.: 8.421 min
Delta R.T.: -0.002 min
Response: 4122827480
Conc: 713.21 ng/ml

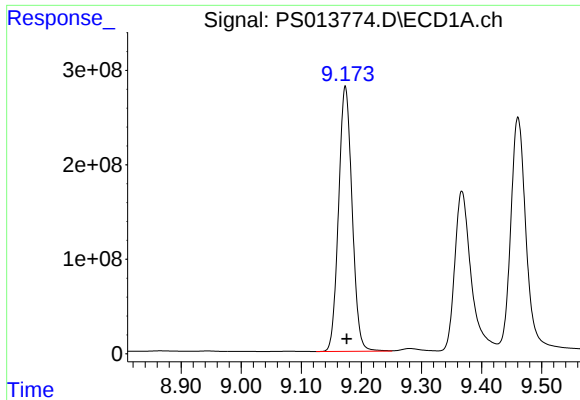

#11 2,4,5-TP (SILVEX)


R.T.: 9.173 min
Delta R.T.: -0.002 min
Response: 4386913643
Conc: 787.81 ng/ml

Instrument :
ECD_S
ClientSampleId :

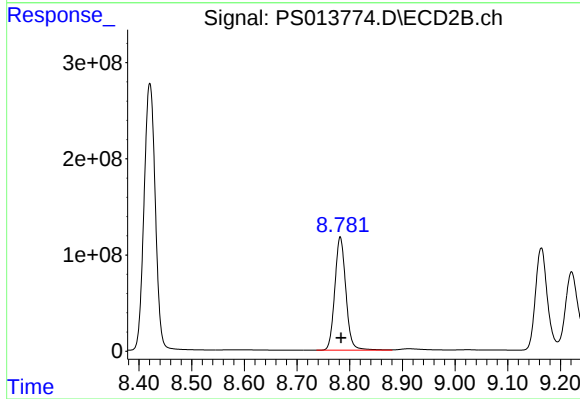


#11 2,4,5-TP (SILVEX)

R.T.: 8.782 min
Delta R.T.: -0.002 min
Response: 1713757101
Conc: 717.43 ng/ml

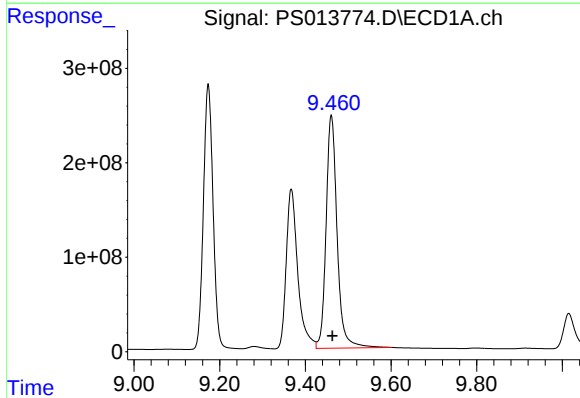


#12 2,4,5-T

R.T.: 9.461 min
Delta R.T.: -0.003 min
Response: 4407914576
Conc: 779.52 ng/ml

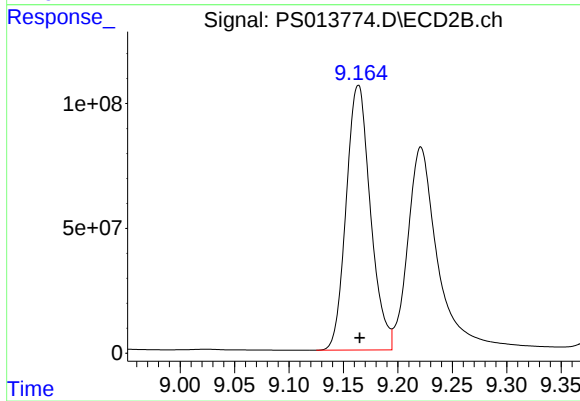

#12 2,4,5-T


R.T.: 9.164 min
Delta R.T.: -0.001 min
Response: 1649249991
Conc: 720.41 ng/ml

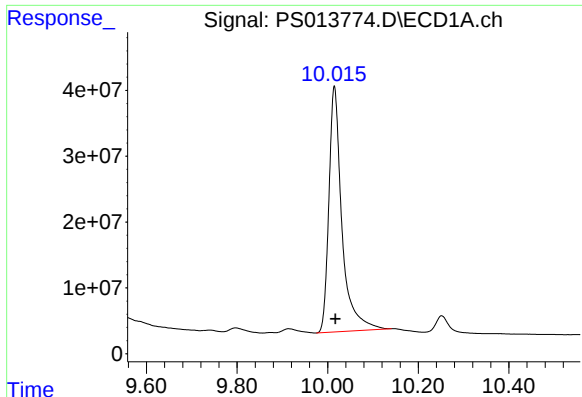

#13 2,4-DB


R.T.: 10.015 min
Delta R.T.: -0.002 min
Response: 745547725
Conc: 762.99 ng/ml

Instrument :
ECD_S
ClientSampleId :

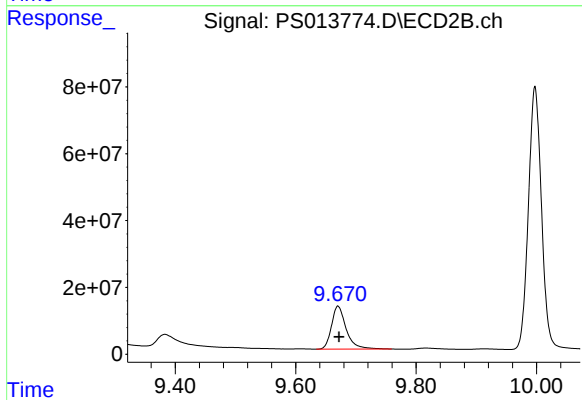


#13 2,4-DB

R.T.: 9.670 min
Delta R.T.: -0.002 min
Response: 217292216
Conc: 714.43 ng/ml

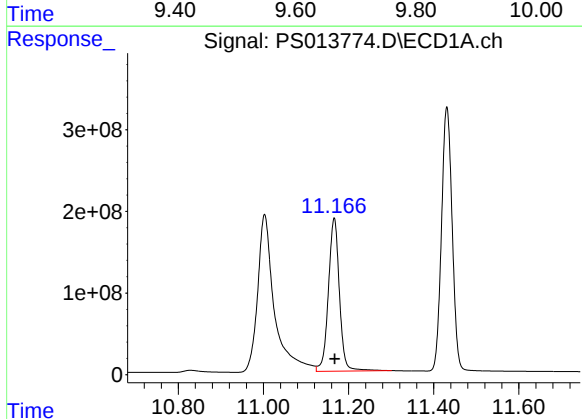


#14 DINOSEB

R.T.: 11.166 min
Delta R.T.: -0.001 min
Response: 3381233487
Conc: 766.40 ng/ml

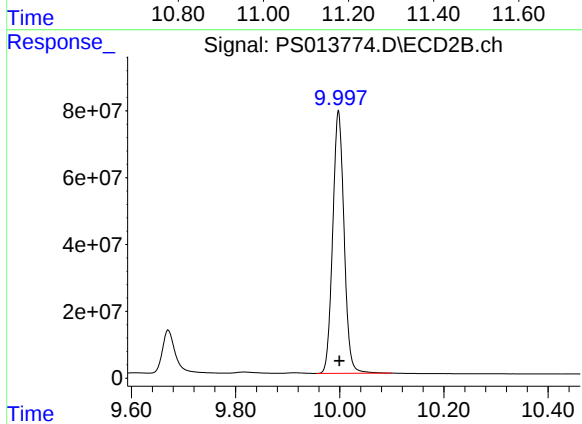

#14 DINOSEB


R.T.: 9.997 min
Delta R.T.: -0.002 min
Response: 1188833294
Conc: 710.46 ng/ml

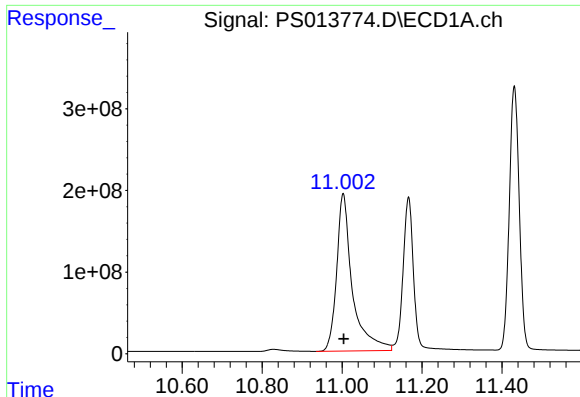

#15 Picloram


R.T.: 11.003 min
Delta R.T.: -0.001 min
Response: 5278060268
Conc: 730.77 ng/ml

Instrument :
ECD_S
ClientSampleId :

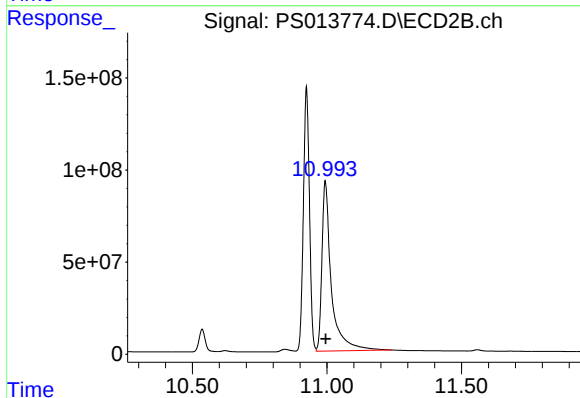


#15 Picloram

R.T.: 10.993 min
Delta R.T.: -0.002 min
Response: 2252408156
Conc: 648.07 ng/ml

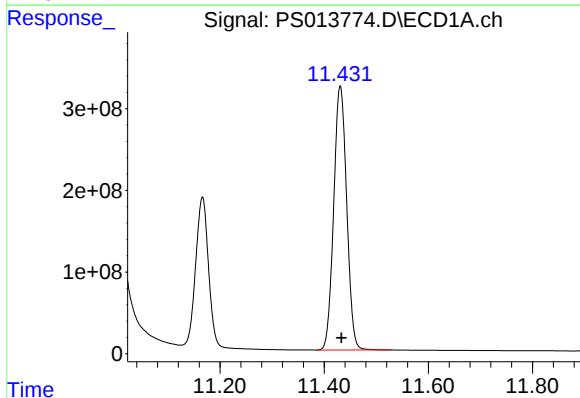

#16 DCPA

R.T.: 11.431 min
Delta R.T.: -0.003 min
Response: 5598654386
Conc: 792.42 ng/ml

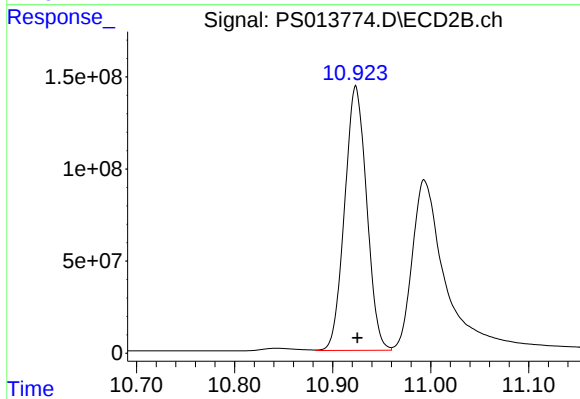

#16 DCPA

R.T.: 10.924 min
Delta R.T.: -0.002 min
Response: 2237116756
Conc: 722.81 ng/ml