

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS011422\
 Data File : PS017987.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Jan 2022 10:27
 Operator : AJ\MA
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 14 18:48:06 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010522.M
 Quant Title : 8080.M
 QLast Update : Thu Jan 06 10:21:08 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.056	0.000	3429314	0	2.372	N.D. #
Target Compounds							
2) T	3,5-DICHL...	6.296	0.000	3974068	0	1.847	N.D. #
5) T	DICAMBA	7.236	0.000	12029807	0	1.926	N.D. #
8) T	DICHLORPROP	7.925	0.000	3904798	0	2.482	N.D. #
9) T	2,4-D	8.166	0.000	1272660	0	<MDL	N.D. #
10) T	Pentachlo...	8.448	8.117	29904346	12669928	1.416	1.504
11) T	2,4,5-TP ...	9.000	8.477	15335886	6340991	1.812	1.779
12) T	2,4,5-T	9.287	8.866	30185974	8848977	3.405	2.705
13) T	2,4-DB	9.837	0.000	20183114	0	12.210	N.D. #
14) T	DINOSEB	10.977	0.000	17063401	0	2.598	N.D. #
15) T	Picloram	10.809	10.667	354.4E6	128.9E6	29.696	27.567
16) T	DCPA	11.246	10.603	22363458	8623427	2.070	1.953



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS011422\
Data File : PS017987.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Jan 2022 10:27
Operator : AJ\MA
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 14 18:48:06 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010522.M
Quant Title : 8080.M
QLast Update : Thu Jan 06 10:21:08 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

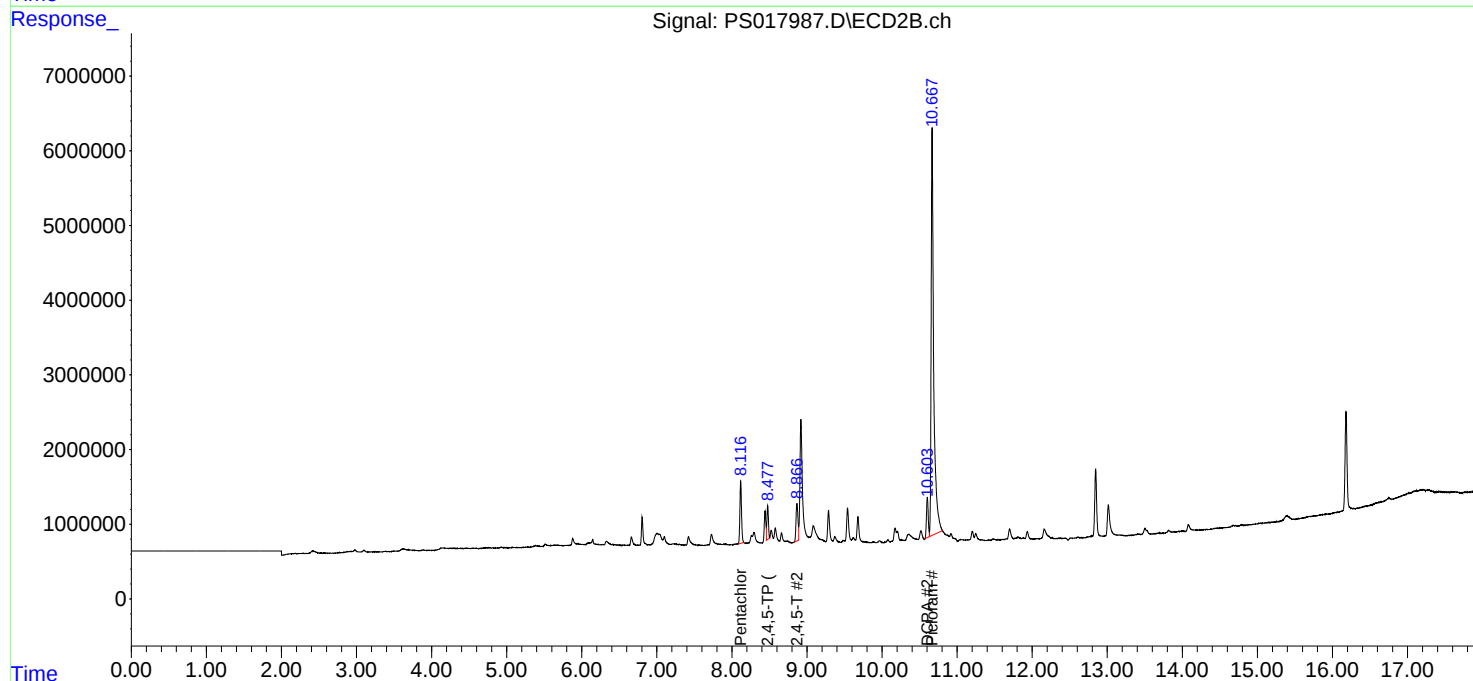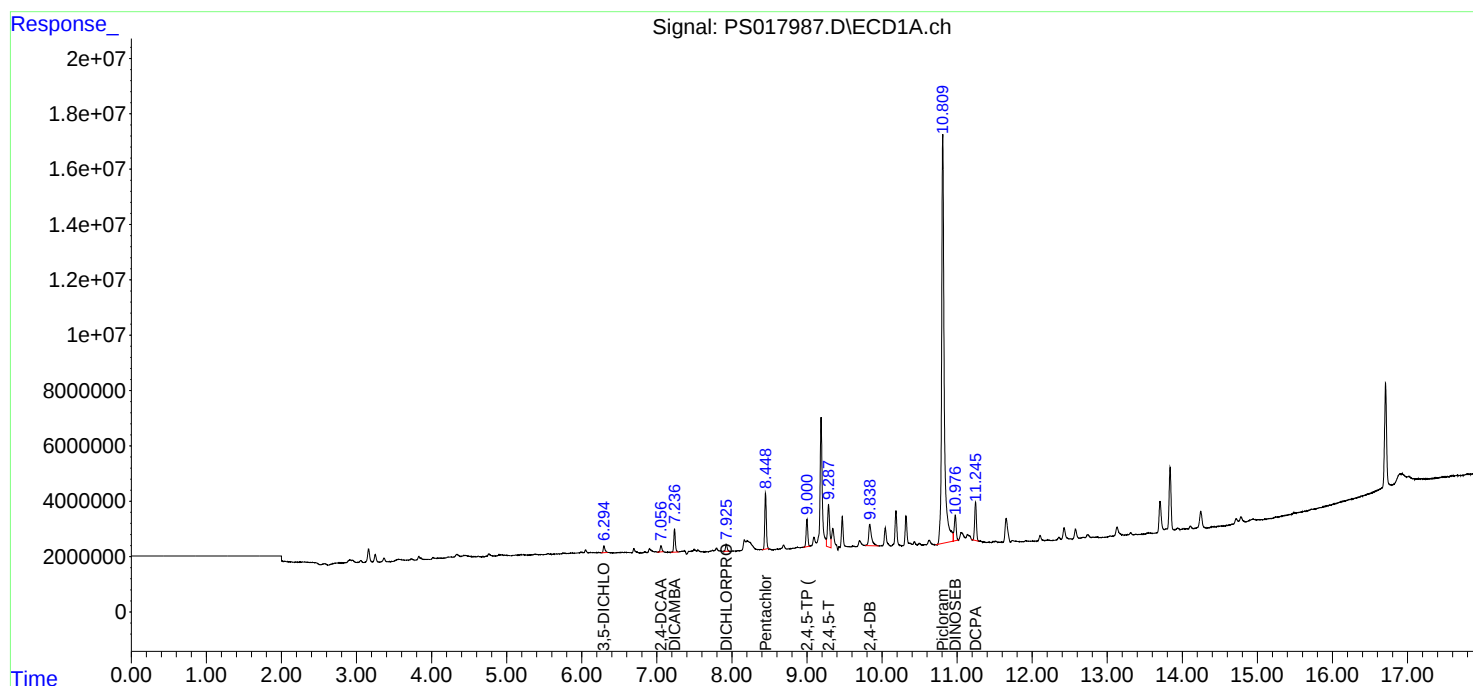


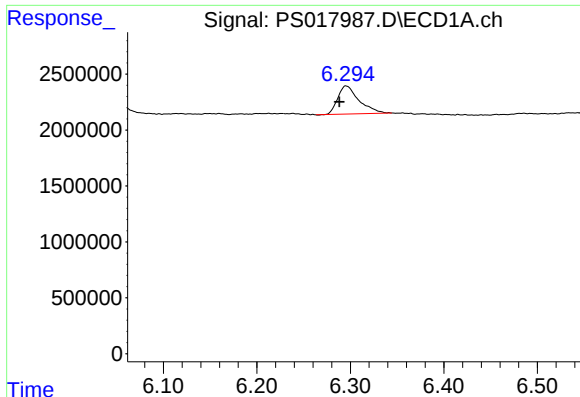

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.296 min
Delta R.T.: 0.007 min
Response: 3974068
Conc: 1.85 ng/ml

Instrument :
ECD_S
ClientSampleId :

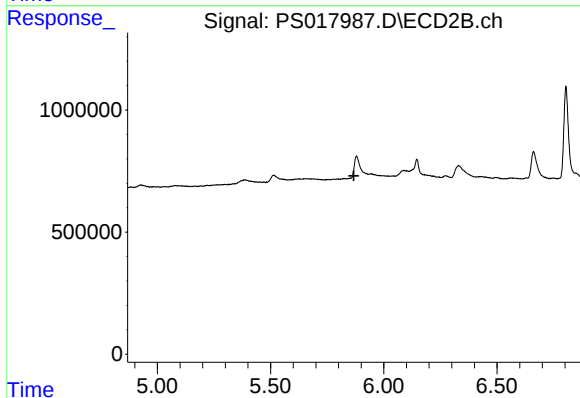


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 5.868 min
Response: 0
Conc: N.D.

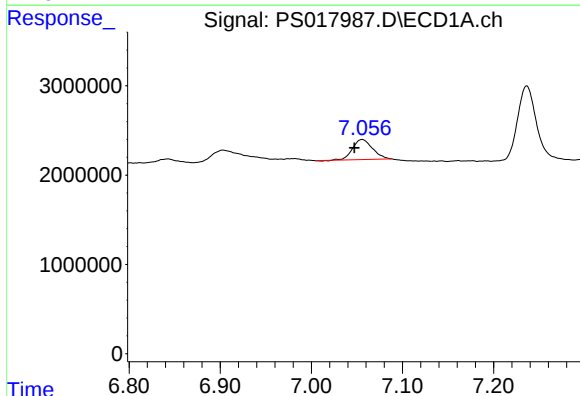


#4 2,4-DCAA

R.T.: 7.056 min
Delta R.T.: 0.008 min
Response: 3429314
Conc: 2.37 ng/ml

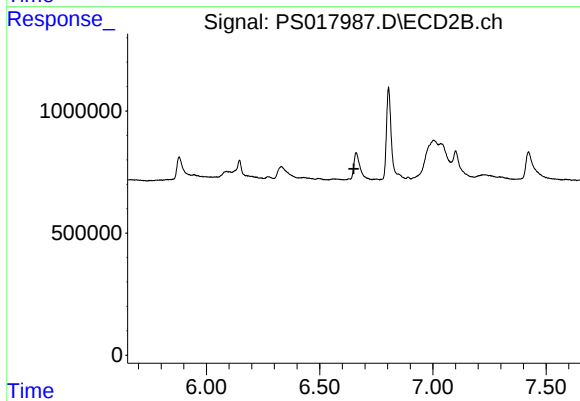

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T. : 6.651 min
Response: 0
Conc: N.D.

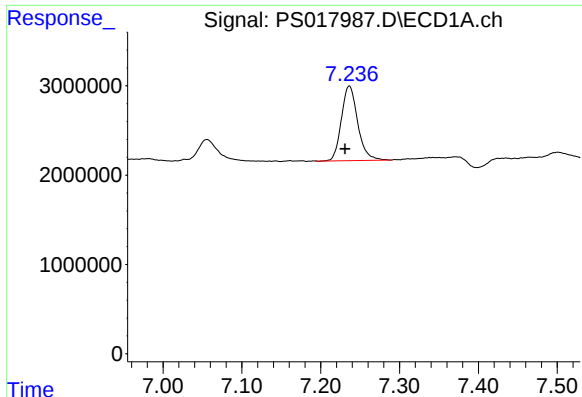

#5 DICAMBA


R.T.: 7.236 min
Delta R.T.: 0.005 min
Response: 12029807
Conc: 1.93 ng/ml

Instrument :
ECD_S
ClientSampleId :

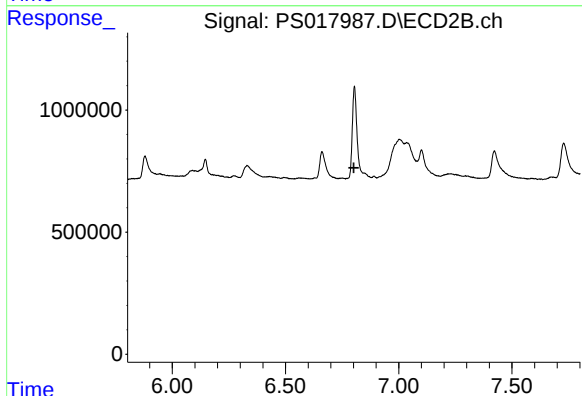


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 6.802 min
Response: 0
Conc: N.D.

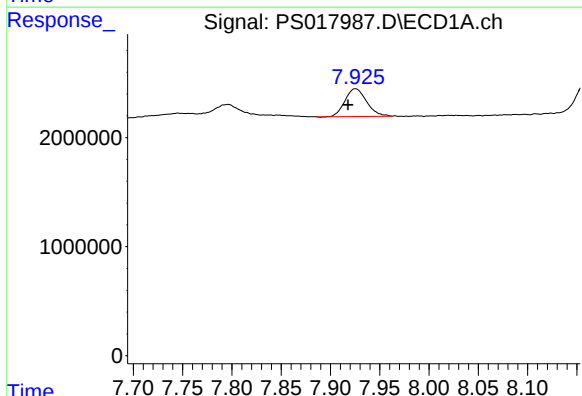


#8 DICHLORPROP

R.T.: 7.925 min
Delta R.T.: 0.007 min
Response: 3904798
Conc: 2.48 ng/ml

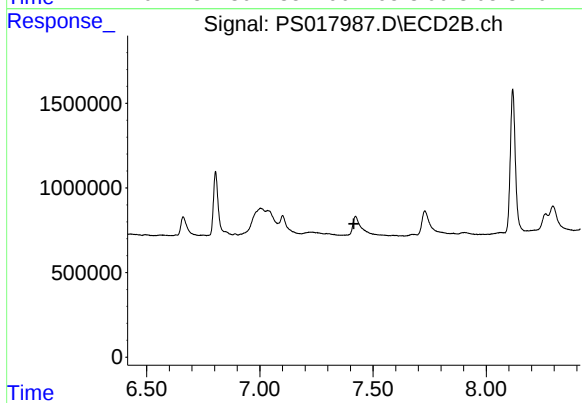

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T. : 7.415 min
Response: 0
Conc: N.D.

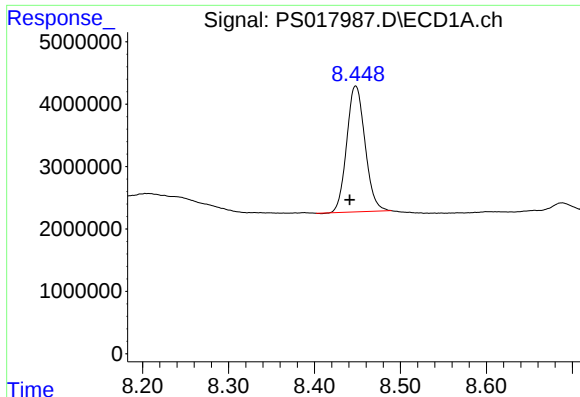

#10 Pentachlorophenol


R.T.: 8.448 min
Delta R.T.: 0.007 min
Response: 29904346
Conc: 1.42 ng/ml

Instrument :
ECD_S
ClientSampleId :

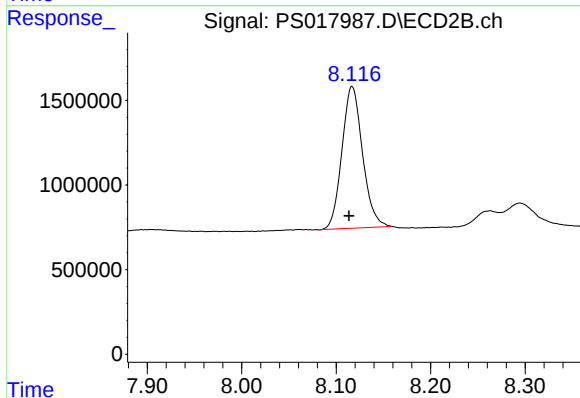


#10 Pentachlorophenol

R.T.: 8.117 min
Delta R.T.: 0.003 min
Response: 12669928
Conc: 1.50 ng/ml

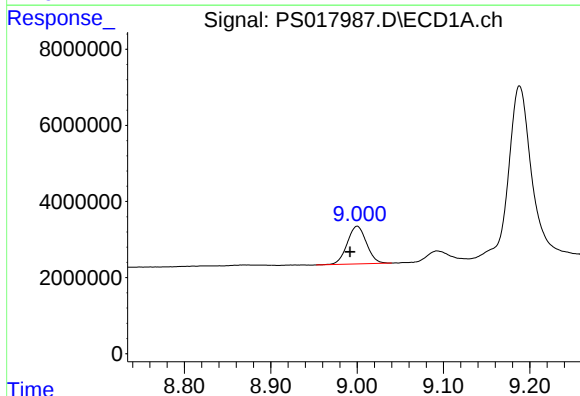


#11 2,4,5-TP (SILVEX)

R.T.: 9.000 min
Delta R.T.: 0.008 min
Response: 15335886
Conc: 1.81 ng/ml

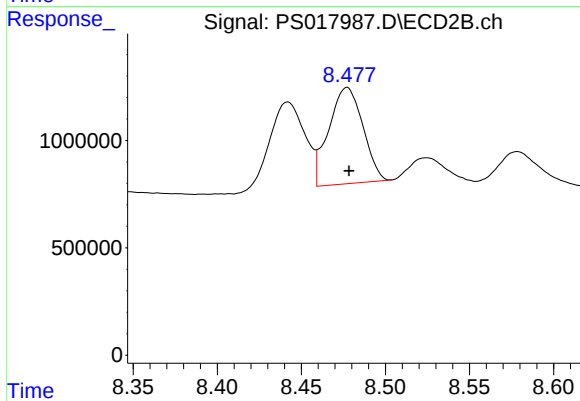

#11 2,4,5-TP (SILVEX)


R.T.: 8.477 min
Delta R.T.: -0.001 min
Response: 6340991
Conc: 1.78 ng/ml

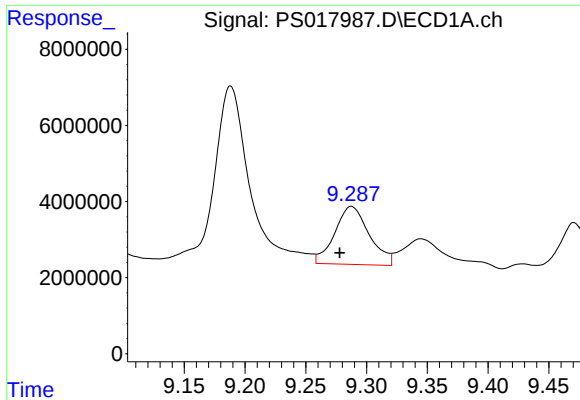

#12 2,4,5-T


R.T.: 9.287 min
Delta R.T.: 0.010 min
Response: 30185974
Conc: 3.41 ng/ml

Instrument :
ECD_S
ClientSampleId :

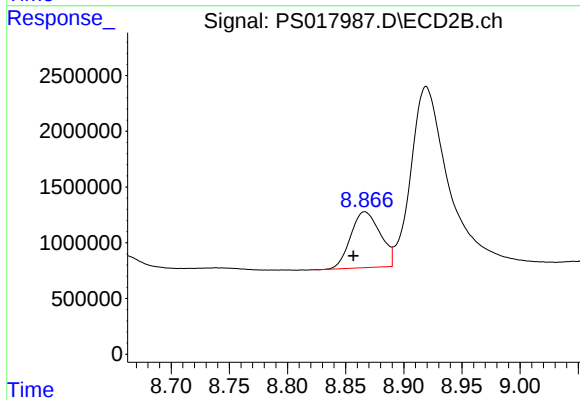


#12 2,4,5-T

R.T.: 8.866 min
Delta R.T.: 0.010 min
Response: 8848977
Conc: 2.71 ng/ml

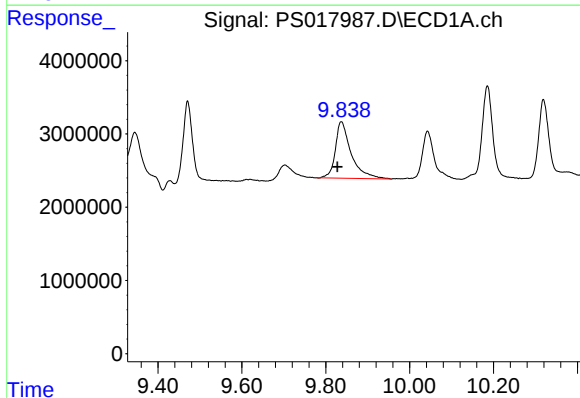


#13 2,4-DB

R.T.: 9.837 min
Delta R.T.: 0.010 min
Response: 20183114
Conc: 12.21 ng/ml

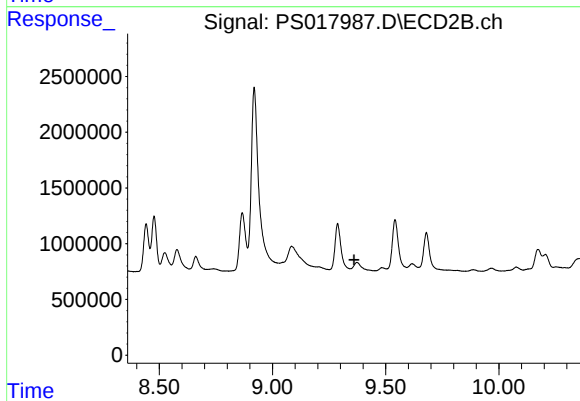

#13 2,4-DB


R.T.: 0.000 min
Exp R.T. : 9.360 min
Response: 0
Conc: N.D.

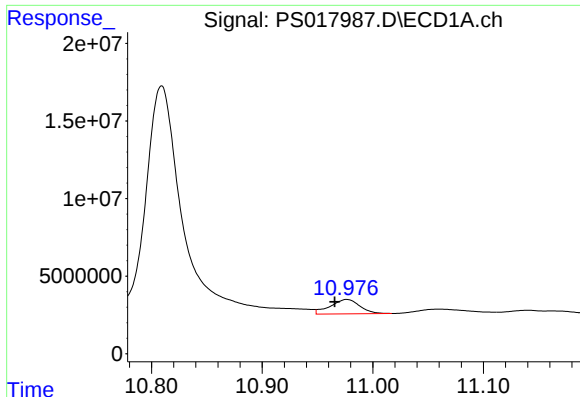

#14 DINOSEB


R.T.: 10.977 min
Delta R.T.: 0.011 min
Response: 17063401
Conc: 2.60 ng/ml

Instrument :
ECD_S
ClientSampleId :

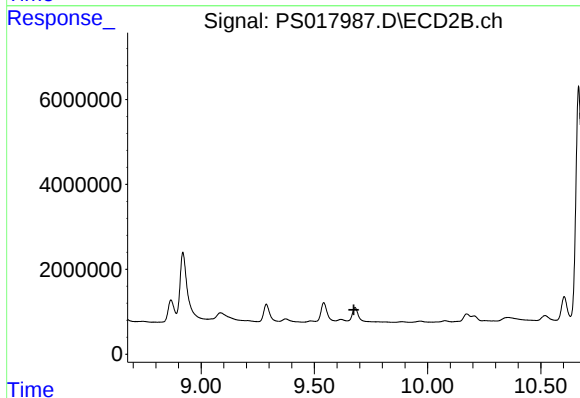


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 9.675 min
Response: 0
Conc: N.D.

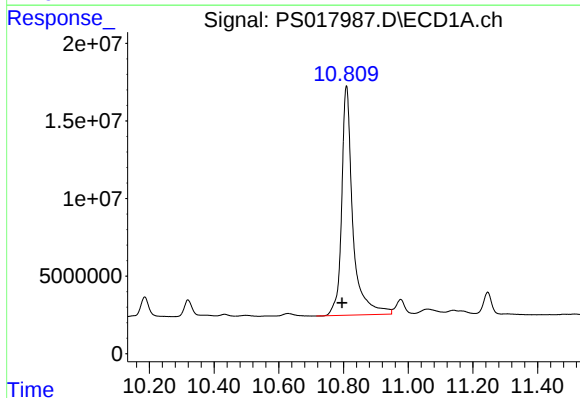


#15 Picloram

R.T.: 10.809 min
Delta R.T.: 0.013 min
Response: 354447502
Conc: 29.70 ng/ml

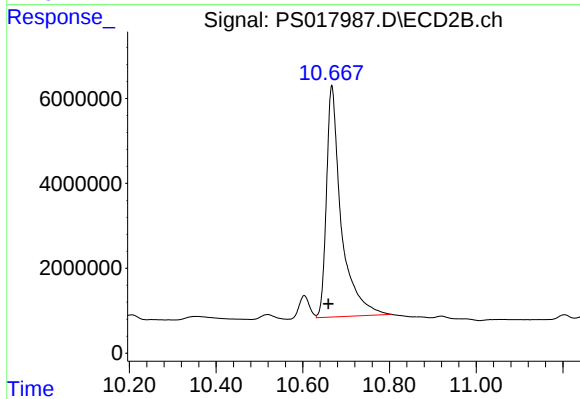

#15 Picloram


R.T.: 10.667 min
Delta R.T.: 0.008 min
Response: 128909230
Conc: 27.57 ng/ml

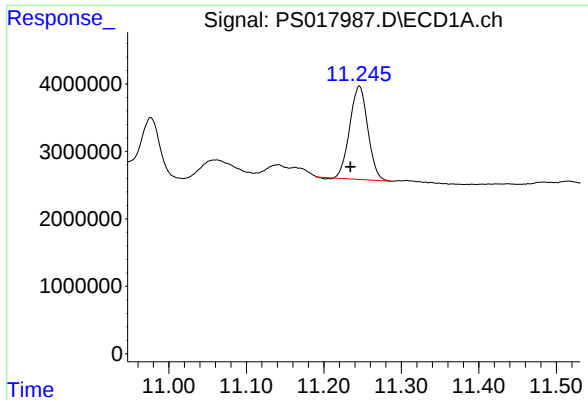

#16 DCPA

R.T.: 11.246 min
Delta R.T.: 0.011 min
Response: 22363458
Conc: 2.07 ng/ml

Instrument :
ECD_S
ClientSampleId :

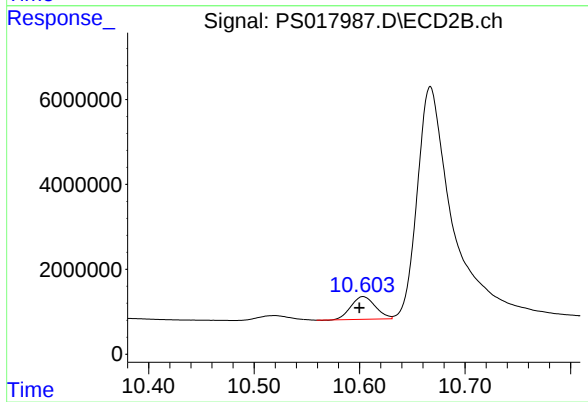

#16 DCPA

R.T.: 10.603 min
Delta R.T.: 0.003 min
Response: 8623427
Conc: 1.95 ng/ml