

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS011422\
 Data File : PS018002.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Jan 2022 17:40
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 14 18:54:50 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010522.M
 Quant Title : 8080.M
 QLast Update : Thu Jan 06 10:21:08 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.047	6.644	675.4E6	301.0E6	467.279	518.746
Target Compounds							
7) T	MCPA	7.491f	0.000	5689479	0	<MDL	N.D. #
9) T	2,4-D	8.203f	0.000	18209075	0	10.000	N.D. #
11) T	2,4,5-TP ...	9.056f	8.435f	8058934	6054319	<MDL	1.698 #
12) T	2,4,5-T	9.247	0.000	1506293	0	<MDL	N.D. #
14) T	DINOSEB	10.926f	0.000	12640475	0	1.925	N.D. #
15) T	Picloram	10.808	0.000	24755069	0	2.074	N.D. #
16) T	DCPA	11.232	0.000	5182311	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS011422\
Data File : PS018002.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Jan 2022 17:40
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 14 18:54:50 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010522.M
Quant Title : 8080.M
QLast Update : Thu Jan 06 10:21:08 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

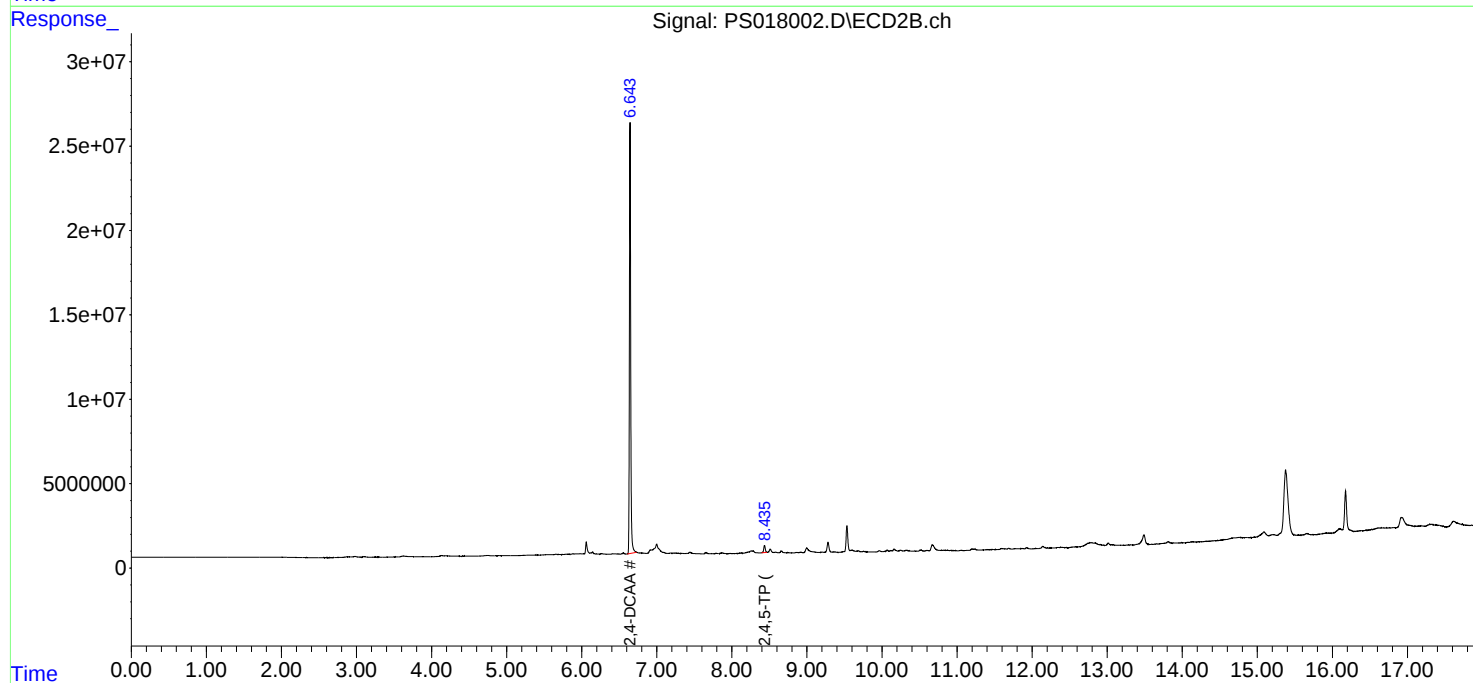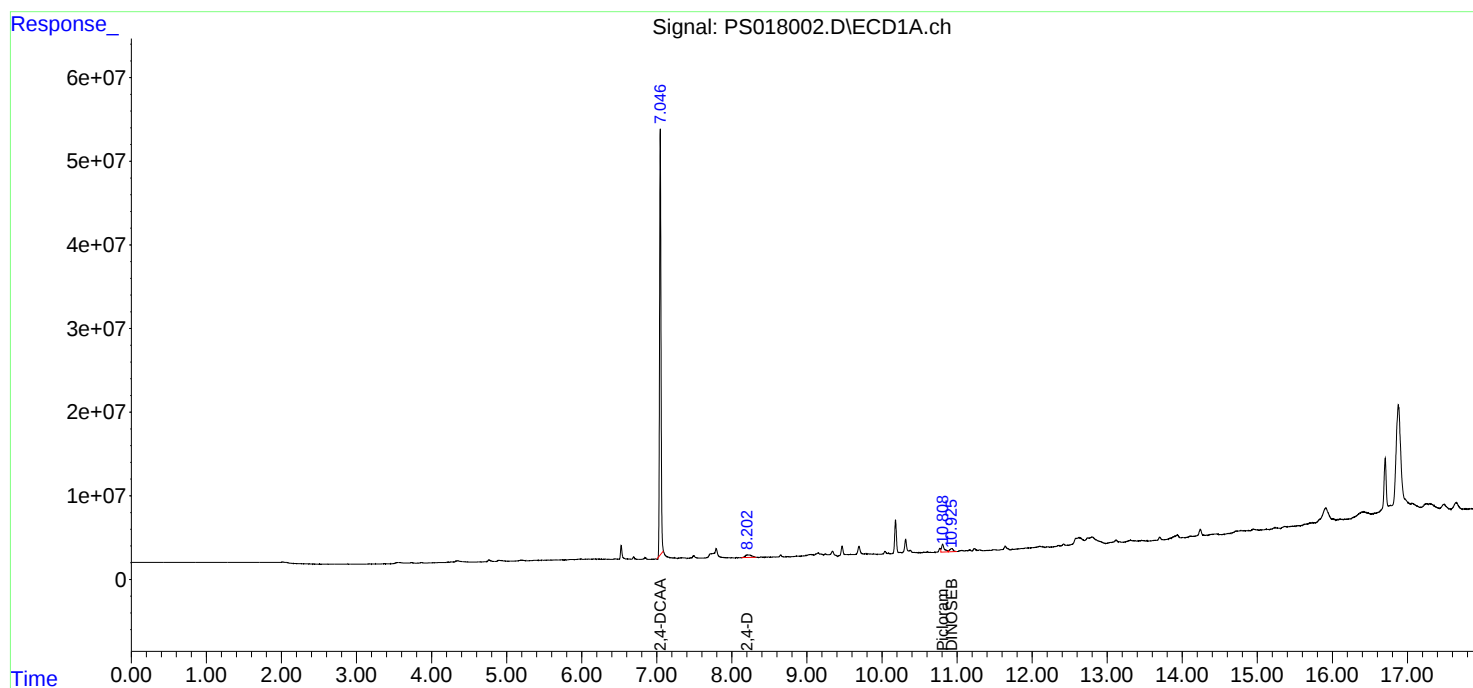


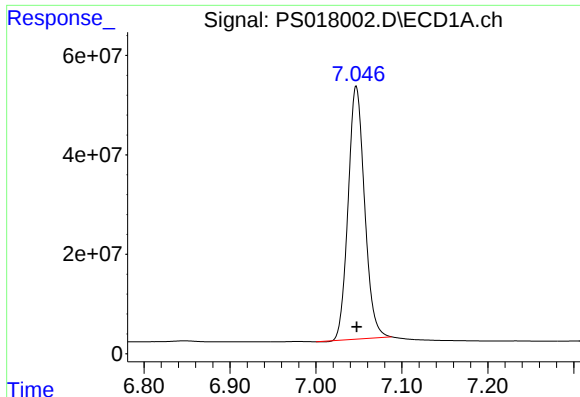

#4 2,4-DCAA


R.T.: 7.047 min
Delta R.T.: 0.000 min
Response: 675446042
Conc: 467.28 ng/ml

Instrument :
ECD_S
ClientSampleId :

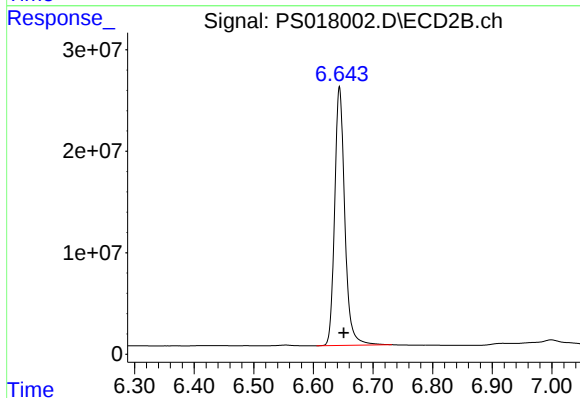


#4 2,4-DCAA

R.T.: 6.644 min
Delta R.T.: -0.007 min
Response: 301001857
Conc: 518.75 ng/ml

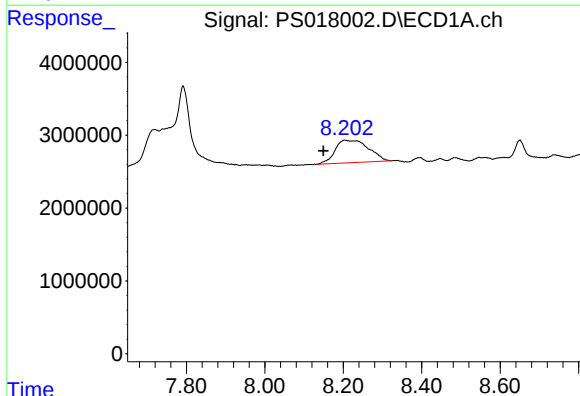


#9 2,4-D

R.T.: 8.203 min
Delta R.T.: 0.054 min
Response: 18209075
Conc: 10.00 ng/ml

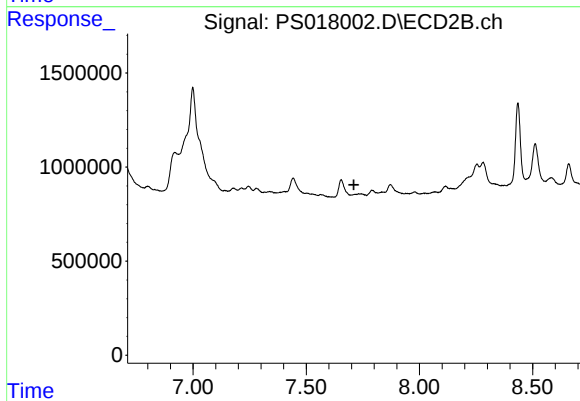

#9 2,4-D


R.T.: 0.000 min
Exp R.T. : 7.710 min
Response: 0
Conc: N.D.

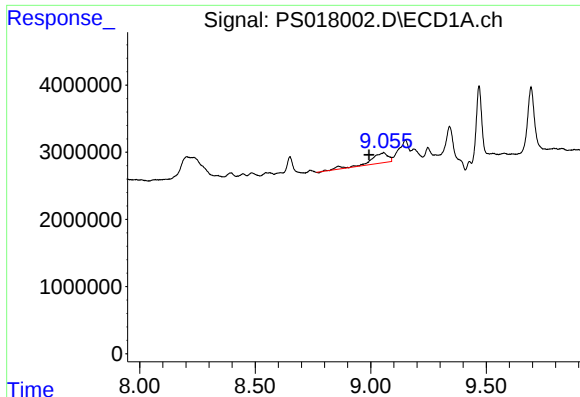

#11 2,4,5-TP (SILVEX)


R.T.: 9.056 min
Delta R.T.: 0.064 min
Response: 8058934
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

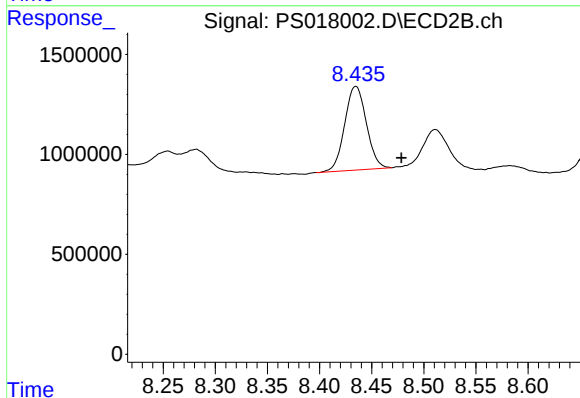


#11 2,4,5-TP (SILVEX)

R.T.: 8.435 min
Delta R.T.: -0.044 min
Response: 6054319
Conc: 1.70 ng/ml

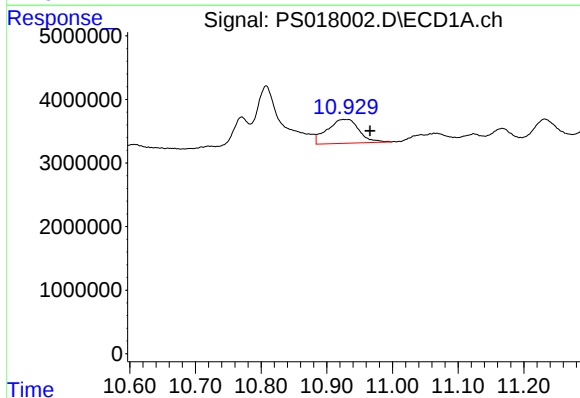


#14 DINOSEB

R.T.: 10.926 min
Delta R.T.: -0.040 min
Response: 12640475
Conc: 1.92 ng/ml

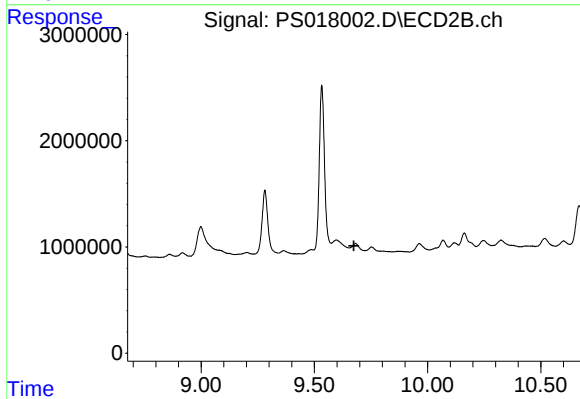

#14 DINOSEB


R.T.: 0.000 min
Exp R.T. : 9.675 min
Response: 0
Conc: N.D.

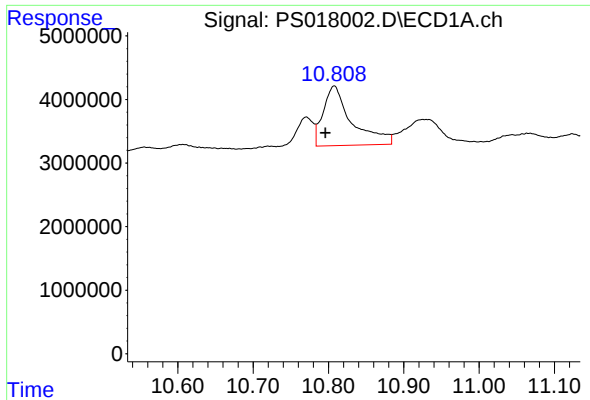

#15 Picloram

R.T.: 10.808 min
Delta R.T.: 0.012 min
Response: 24755069
Conc: 2.07 ng/ml

Instrument :
ECD_S
ClientSampleId :

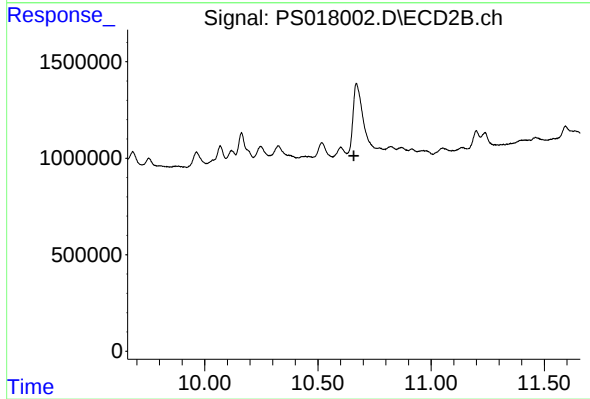

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 10.659 min
Response: 0
Conc: N.D.