

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS011422\
 Data File : PS018014.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Jan 2022 22:59
 Operator : AJ\MA
 Sample : N1121-01
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 WASTE-CLASS-LAUNDRY-PIT

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 01/17/2022
 Supervised By :Ankita Jodhani 01/17/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 15 00:17:34 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010522.M
 Quant Title : 8080.M
 QLast Update : Thu Jan 06 10:21:08 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
4) S 2,4-DCAA	7.048	6.644	532.0E6	200.7E6	368.043	345.883m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS011422\
Data File : PS018014.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Jan 2022 22:59
Operator : AJ\MA
Sample : N1121-01
Misc :
ALS Vial : 26 Sample Multiplier: 1



Instrument :
ECD_S
ClientSampleId :
WASTE-CLASS-LAUNDRY-PIT


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 01/17/2022
Supervised By : Ankita Jodhani 01/17/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 15 00:17:34 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010522.M
Quant Title : 8080.M
QLast Update : Thu Jan 06 10:21:08 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

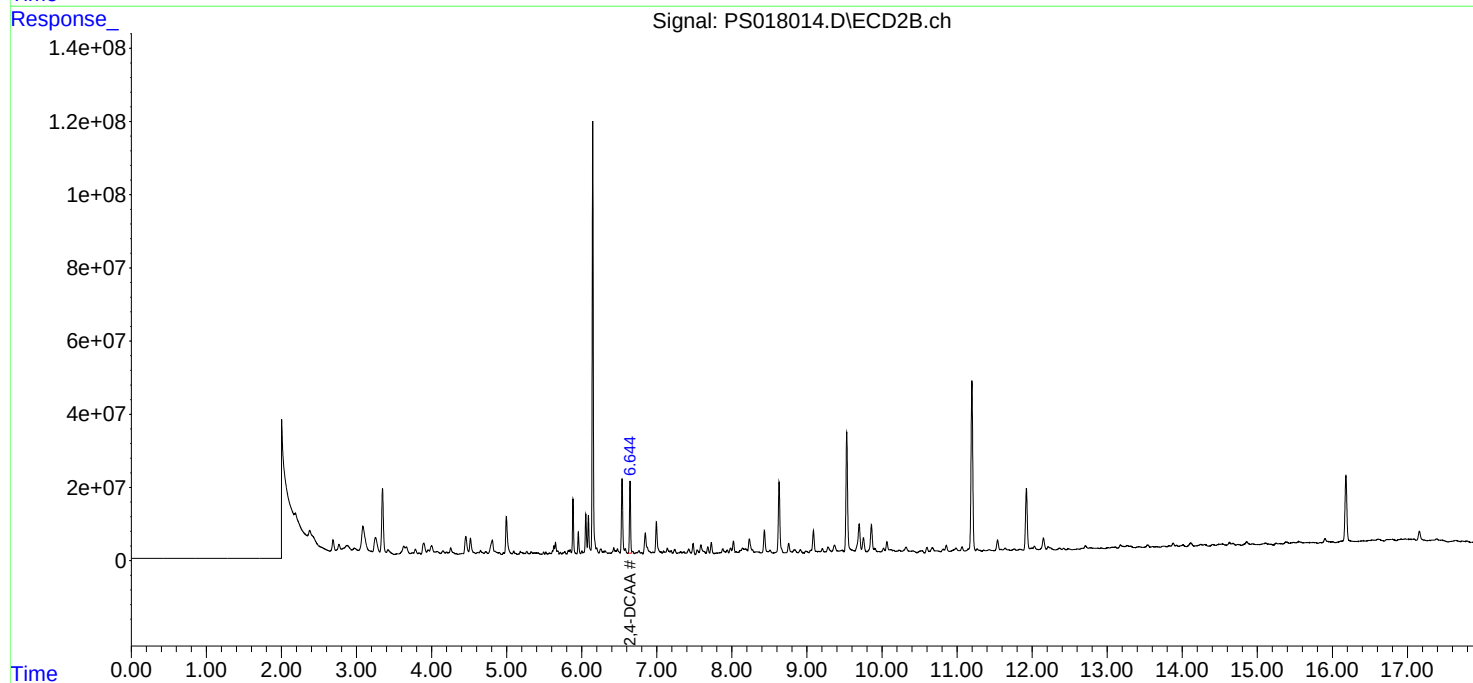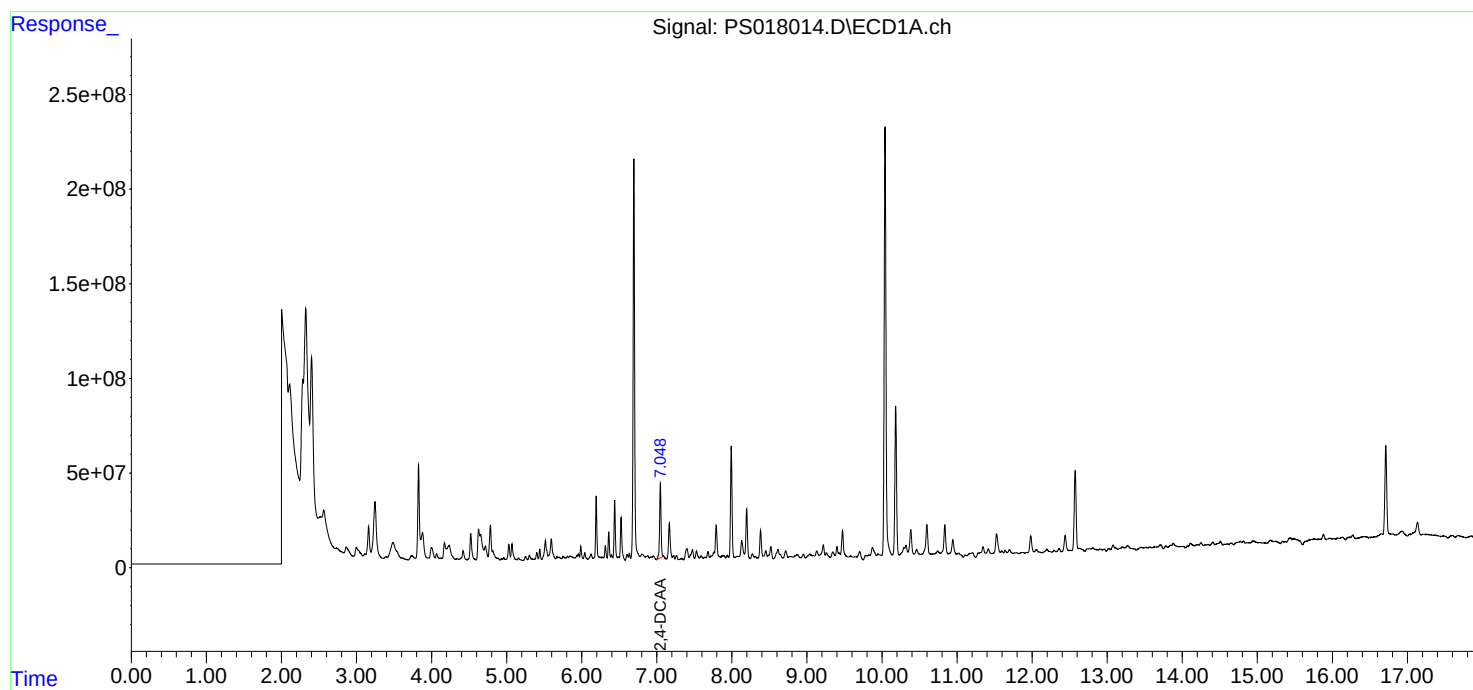

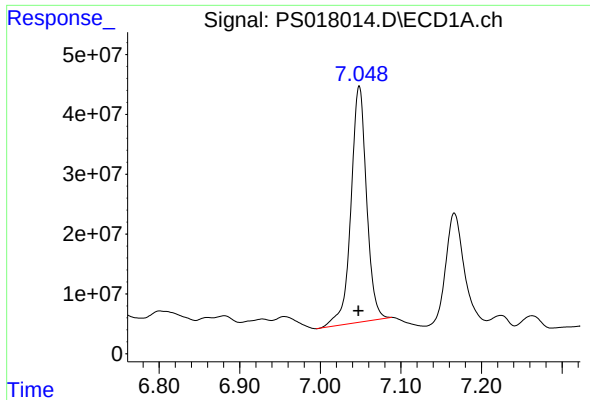

#4 2,4-DCAA

R.T.: 7.048 min
Delta R.T.: 0.000 min
Response: 532002010
Conc: 368.04 ng/ml

Instrument :

ECD_S

ClientSampleId :


WASTE-CLASS-LAUNDRY-PIT

Manual Integrations

APPROVED

Reviewed By :Abdul Mirza 01/17/2022

Supervised By :Ankita Jodhani 01/17/2022

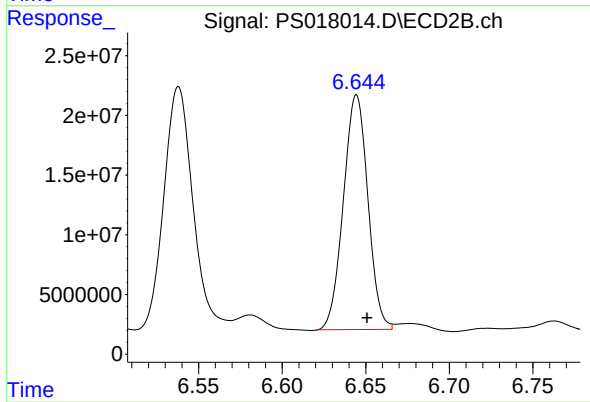

#4 2,4-DCAA

R.T.: 6.644 min
Delta R.T.: -0.007 min
Response: 200698020
Conc: 345.88 ng/ml m