

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS011522\
 Data File : PS018017.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Jan 2022 08:47
 Operator : AJ\MA
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 16 23:27:34 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010522.M
 Quant Title : 8080.M
 QLast Update : Thu Jan 06 10:21:08 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds						
11) T	2,4,5-TP ...	0.000	8.440	0	20850148	N.D. 5.849
12) T	2,4,5-T	9.288	8.922f	12867045	14520814	1.452 4.439 #
13) T	2,4-DB	9.839	0.000	13503557	0	8.169 N.D. #
14) T	DINOSEB	10.975	0.000	4892122	0	<MDL N.D. #
15) T	Picloram	10.808	10.664	363.8E6	128.8E6	30.482 27.550
16) T	DCPA	11.244	10.664f	4746967	128.8E6	<MDL 29.176 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS011522\
Data File : PS018017.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Jan 2022 08:47
Operator : AJ\MA
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 16 23:27:34 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010522.M
Quant Title : 8080.M
QLast Update : Thu Jan 06 10:21:08 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

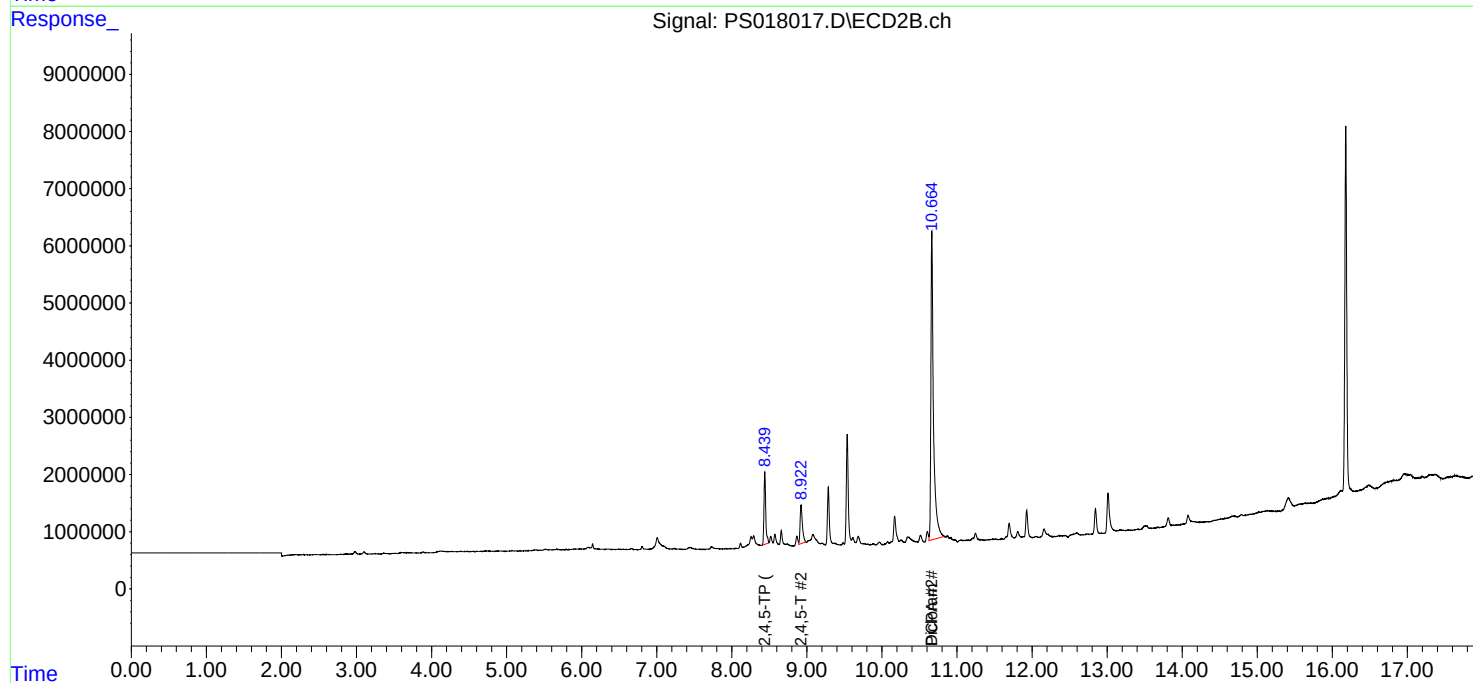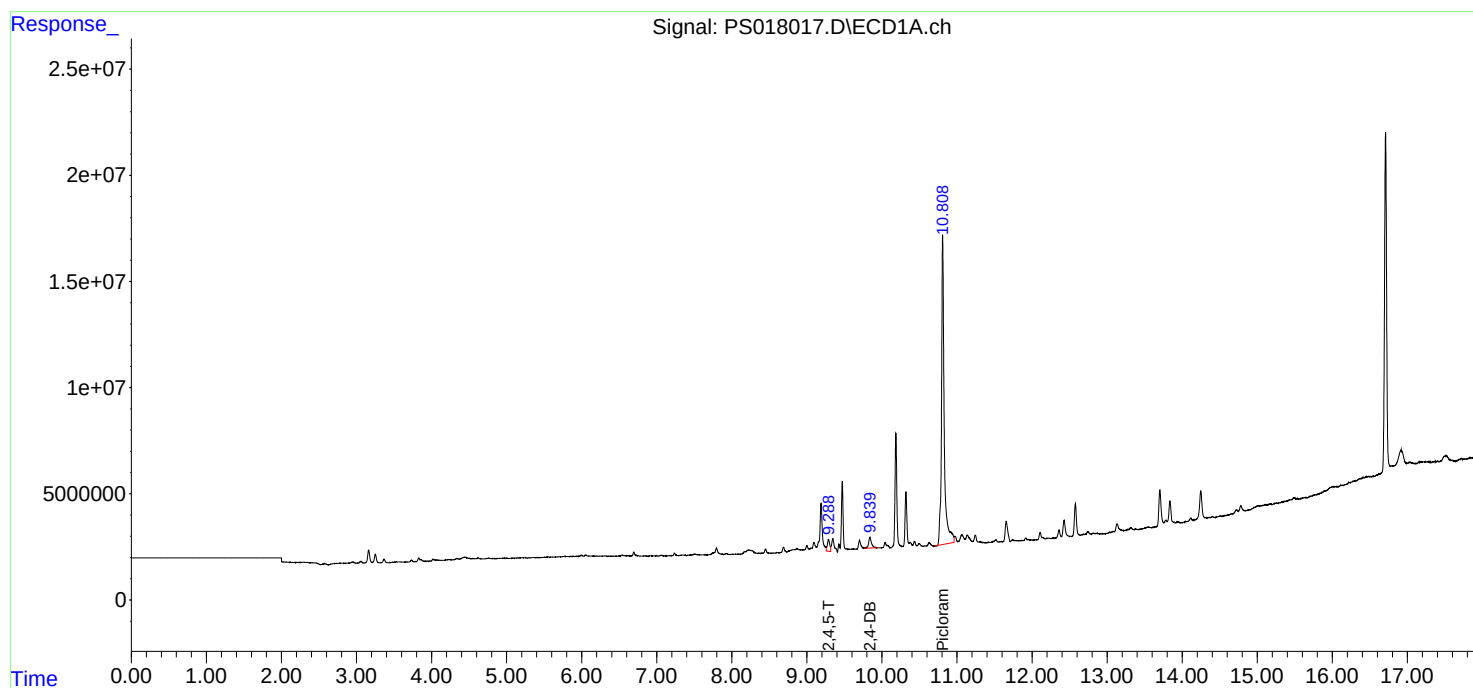


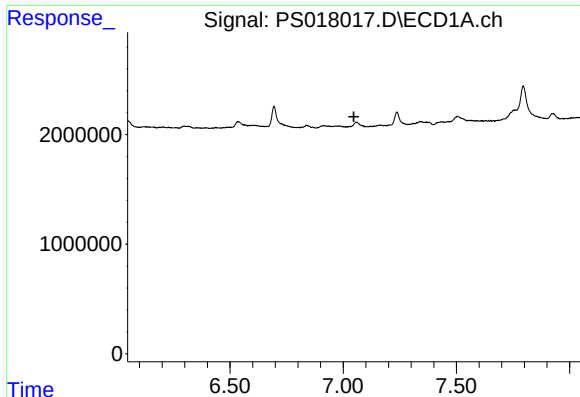

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T.: 7.047 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

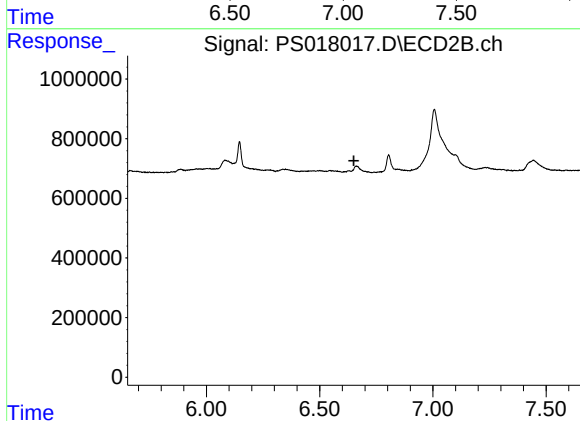


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T.: 6.651 min
Response: 0
Conc: N.D.

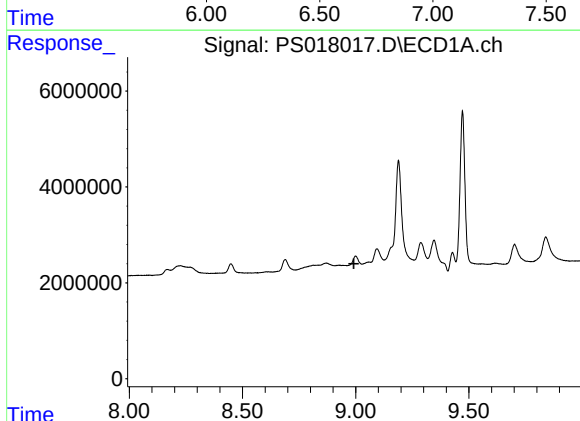


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 8.992 min
Response: 0
Conc: N.D.

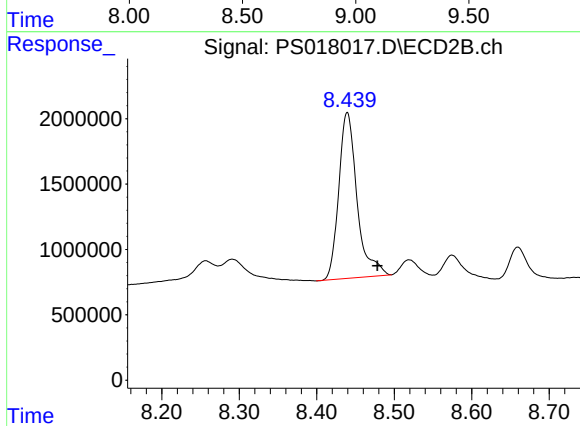

#11 2,4,5-TP (SILVEX)


R.T.: 8.440 min
Delta R.T.: -0.039 min
Response: 20850148
Conc: 5.85 ng/ml

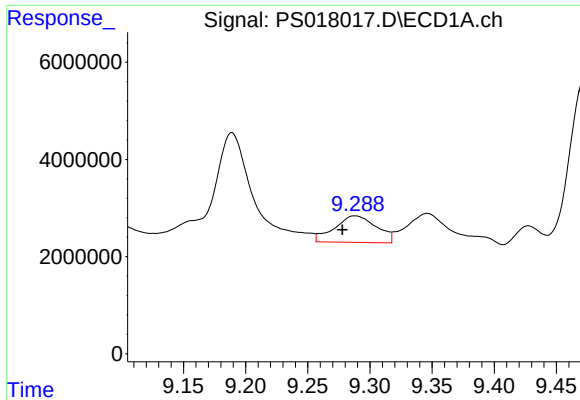

#12 2,4,5-T


R.T.: 9.288 min
Delta R.T.: 0.010 min
Response: 12867045
Conc: 1.45 ng/ml

Instrument :
ECD_S
ClientSampleId :
HEXANE

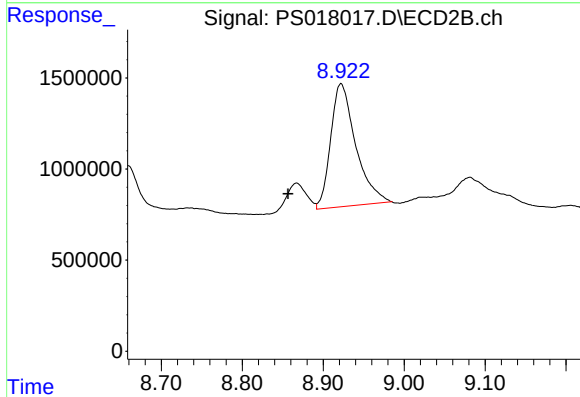


#12 2,4,5-T

R.T.: 8.922 min
Delta R.T.: 0.065 min
Response: 14520814
Conc: 4.44 ng/ml

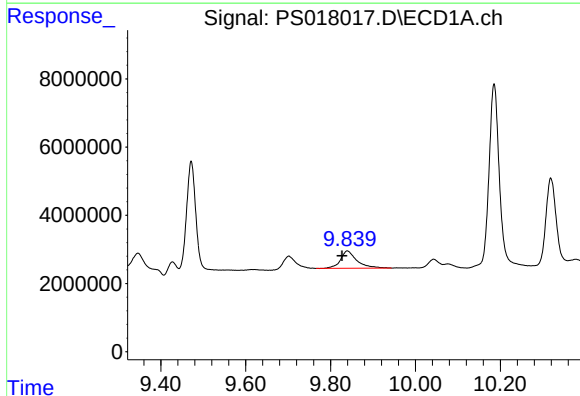


#13 2,4-DB

R.T.: 9.839 min
Delta R.T.: 0.012 min
Response: 13503557
Conc: 8.17 ng/ml

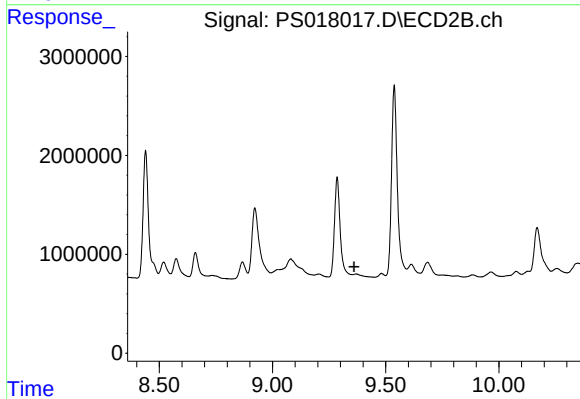

#13 2,4-DB


R.T.: 0.000 min
Exp R.T. : 9.360 min
Response: 0
Conc: N.D.

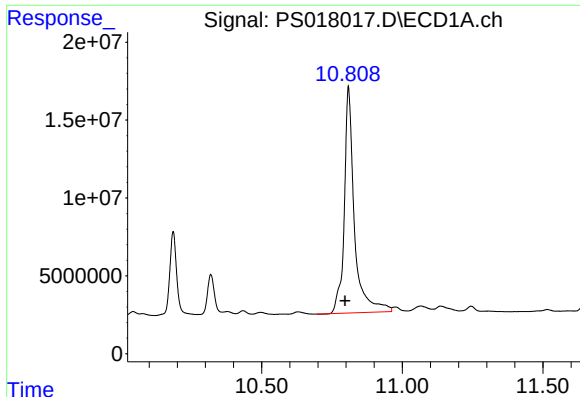

#15 Picloram


R.T.: 10.808 min
Delta R.T.: 0.012 min
Response: 363826298
Conc: 30.48 ng/ml

Instrument :
ECD_S
ClientSampleId :
HEXANE

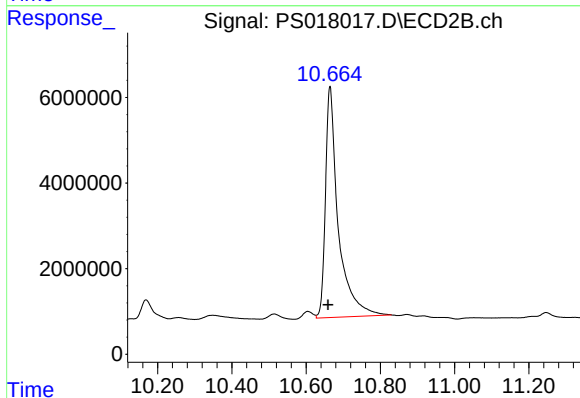


#15 Picloram

R.T.: 10.664 min
Delta R.T.: 0.005 min
Response: 128828329
Conc: 27.55 ng/ml

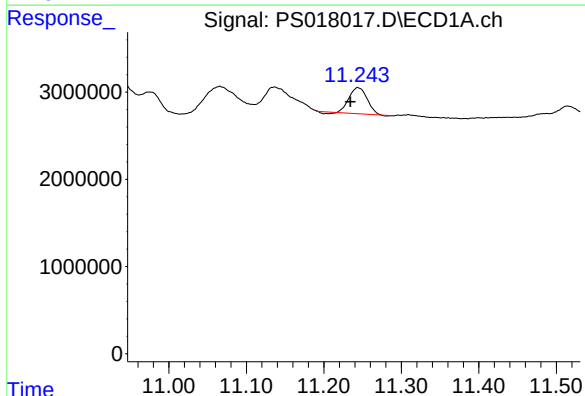

#16 DCPA

R.T.: 11.244 min
Delta R.T.: 0.010 min
Response: 4746967
Conc: N.D.

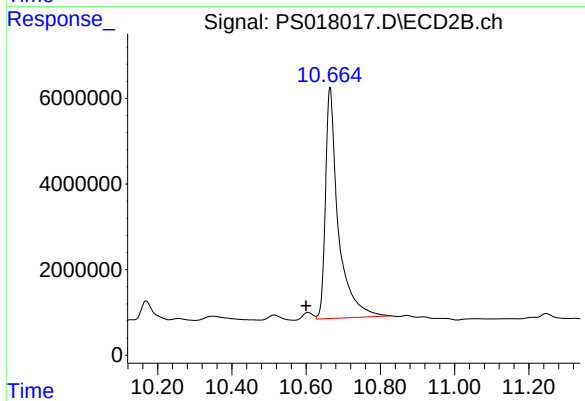

#16 DCPA

R.T.: 10.664 min
Delta R.T.: 0.065 min
Response: 128828329
Conc: 29.18 ng/ml