

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS011522\
 Data File : PS018018.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Jan 2022 09:14
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 16 23:27:58 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010522.M
 Quant Title : 8080.M
 QLast Update : Thu Jan 06 10:21:08 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.049	6.646	631.9E6	294.7E6	437.125	507.828
Target Compounds							
11) T	2,4,5-TP ...	0.000	8.441	0	12706897	N.D.	3.565
12) T	2,4,5-T	9.348f	0.000	10817262	0	1.220	N.D. #
13) T	2,4-DB	9.842	0.000	7479933	0	4.525	N.D. #
15) T	Picloram	10.812	10.669	264.0E6	89659871	22.114	19.174
16) T	DCPA	0.000	10.669f	0	89659871	N.D.	20.306



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS011522\
Data File : PS018018.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Jan 2022 09:14
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 16 23:27:58 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010522.M
Quant Title : 8080.M
QLast Update : Thu Jan 06 10:21:08 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

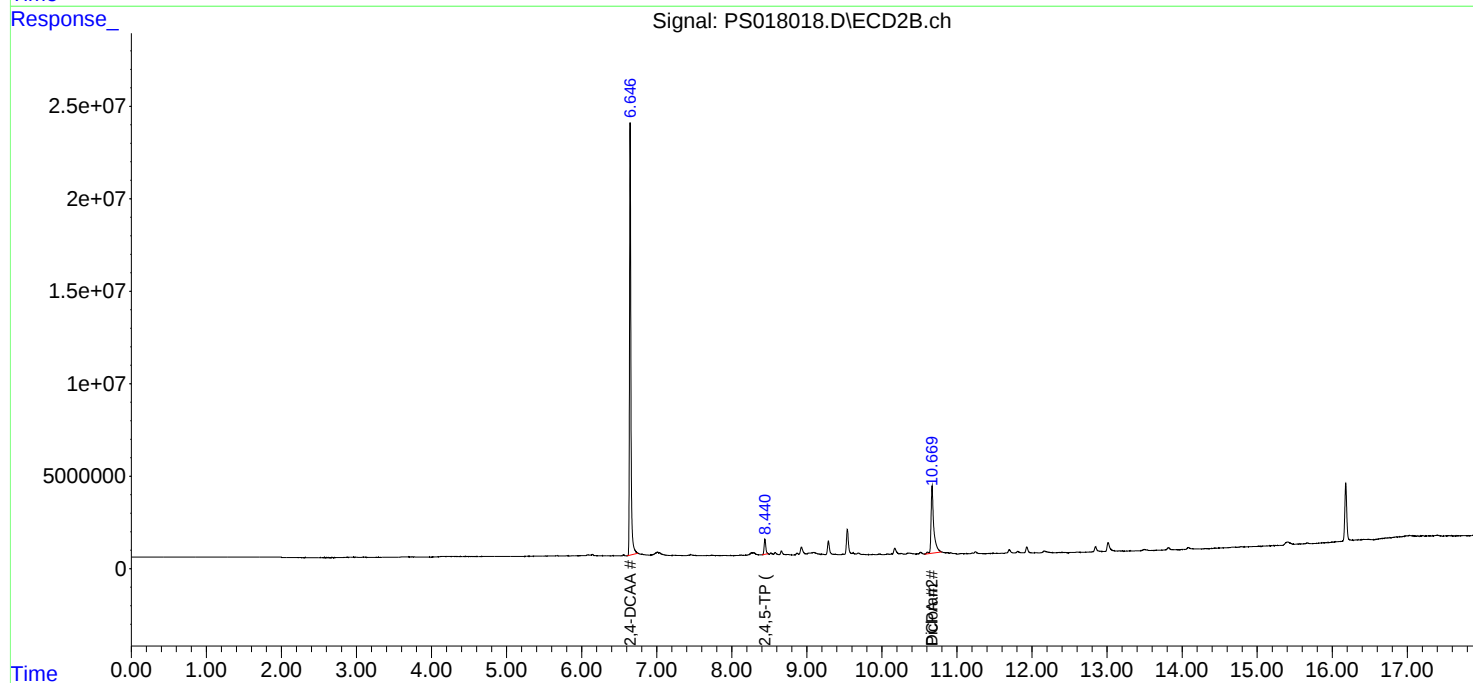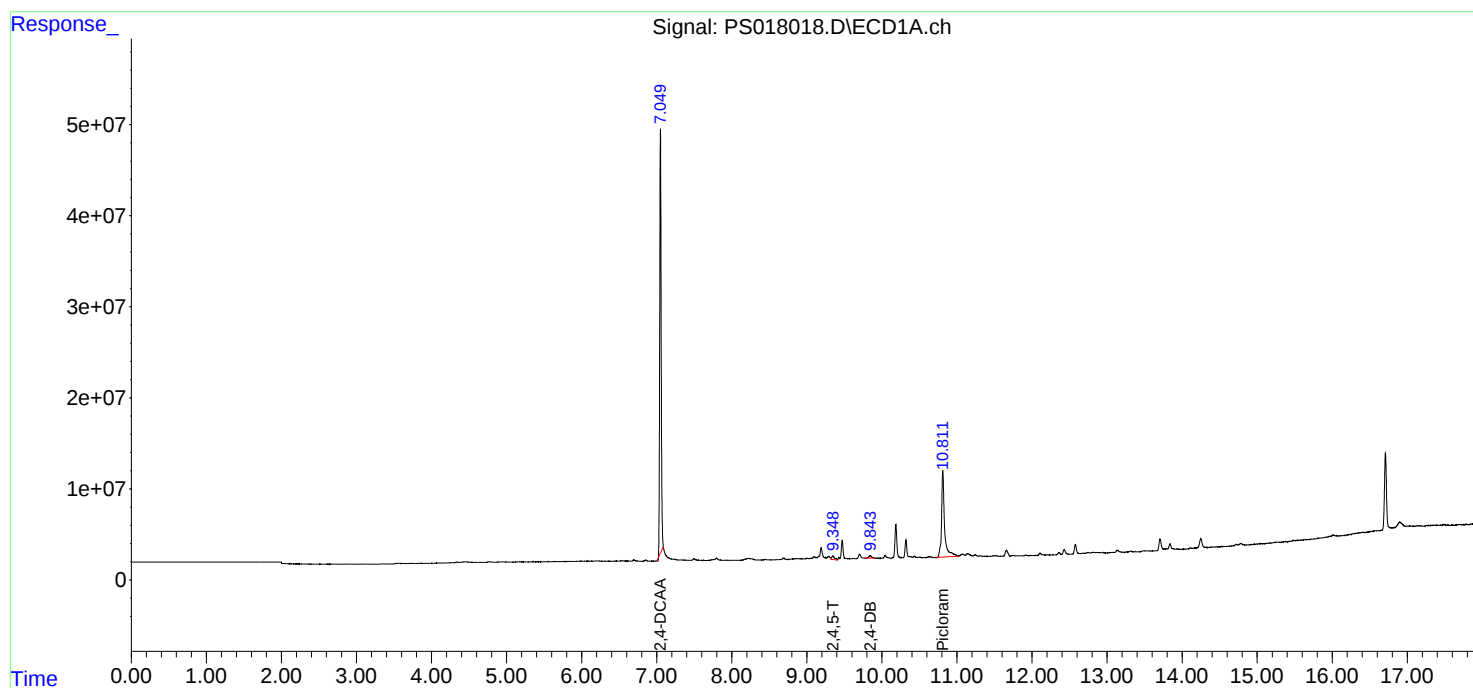


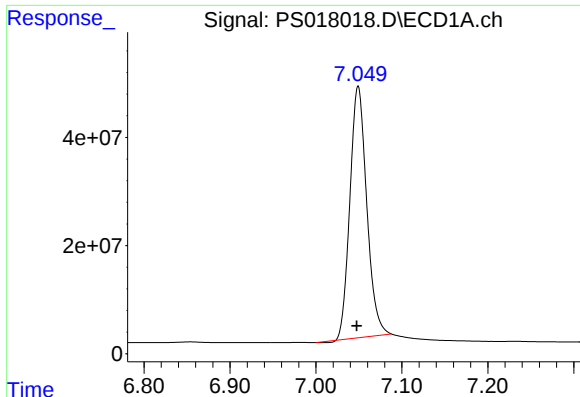

#4 2,4-DCAA


R.T.: 7.049 min
Delta R.T.: 0.002 min
Response: 631858576
Conc: 437.12 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

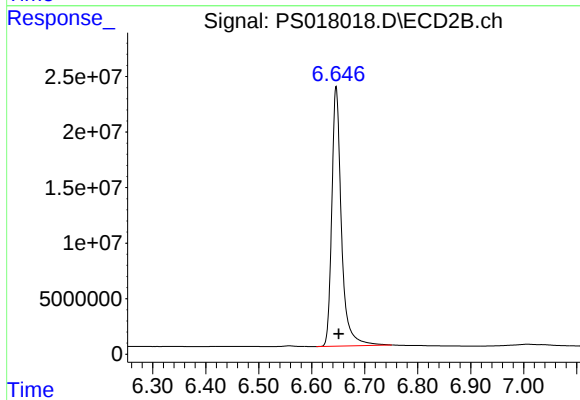


#4 2,4-DCAA

R.T.: 6.646 min
Delta R.T.: -0.005 min
Response: 294666781
Conc: 507.83 ng/ml

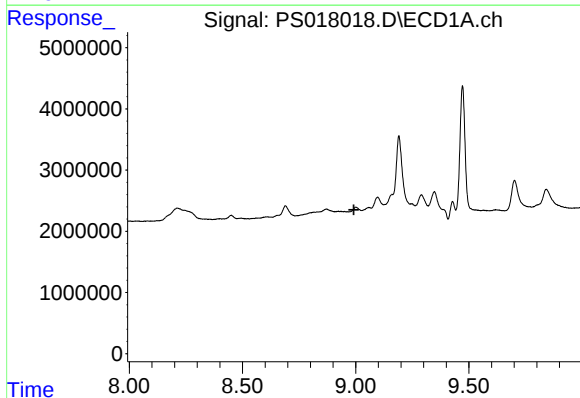


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 8.992 min
Response: 0
Conc: N.D.

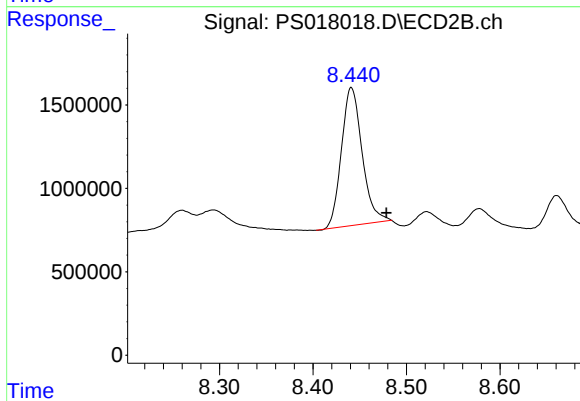

#11 2,4,5-TP (SILVEX)


R.T.: 8.441 min
Delta R.T.: -0.038 min
Response: 12706897
Conc: 3.56 ng/ml

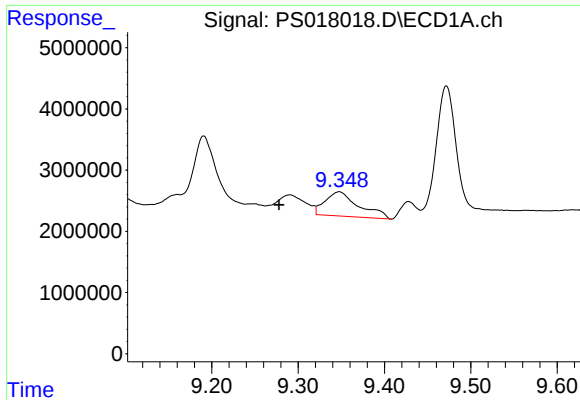

#12 2,4,5-T


R.T.: 9.348 min
Delta R.T.: 0.070 min
Response: 10817262
Conc: 1.22 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

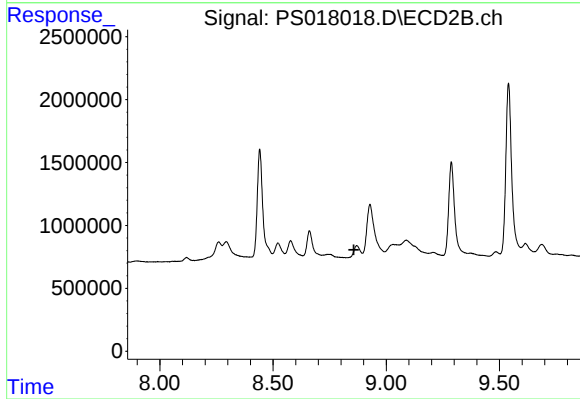


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 8.857 min
Response: 0
Conc: N.D.

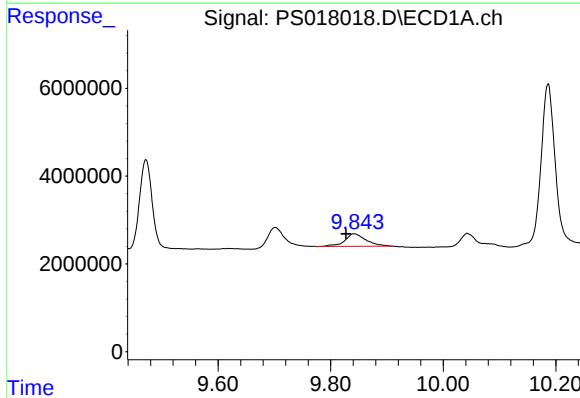


#13 2,4-DB

R.T.: 9.842 min
Delta R.T.: 0.015 min
Response: 7479933
Conc: 4.52 ng/ml

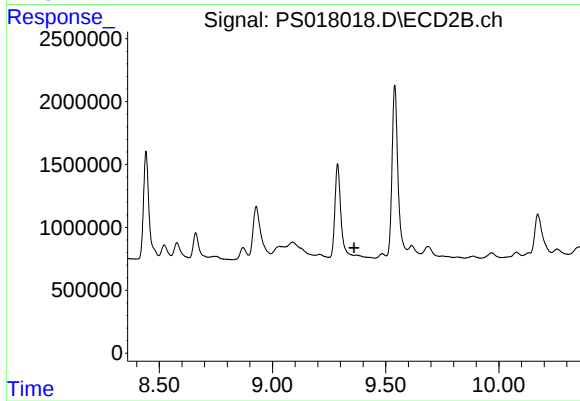

#13 2,4-DB


R.T.: 0.000 min
Exp R.T. : 9.360 min
Response: 0
Conc: N.D.

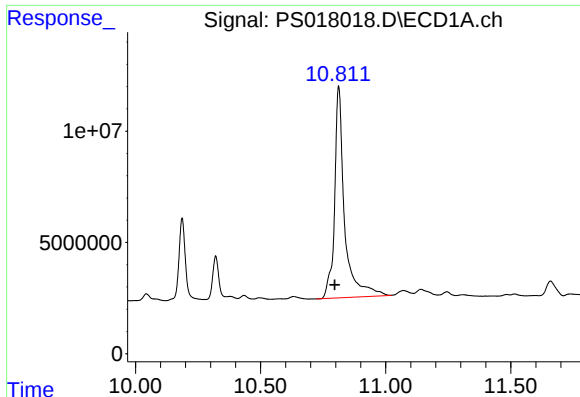

#15 Picloram


R.T.: 10.812 min
Delta R.T.: 0.016 min
Response: 263951022
Conc: 22.11 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

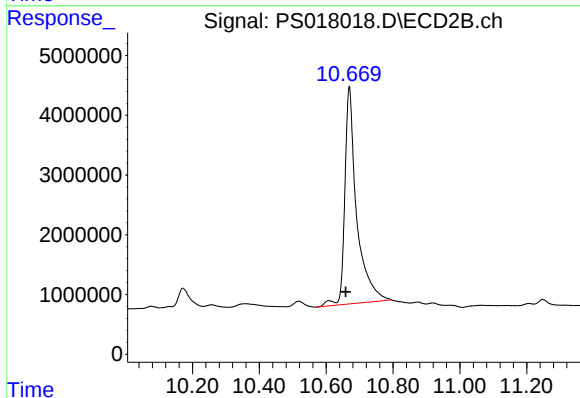


#15 Picloram

R.T.: 10.669 min
Delta R.T.: 0.010 min
Response: 89659871
Conc: 19.17 ng/ml

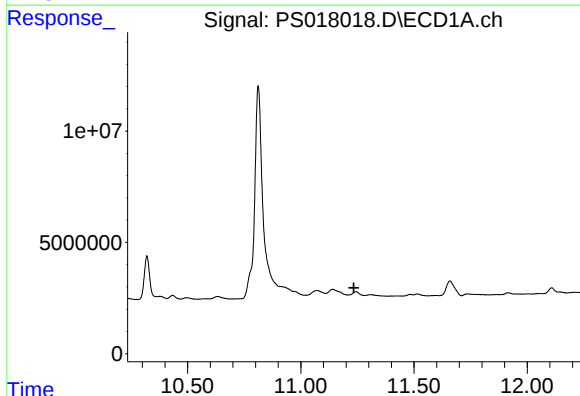

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 11.234 min
Response: 0
Conc: N.D.

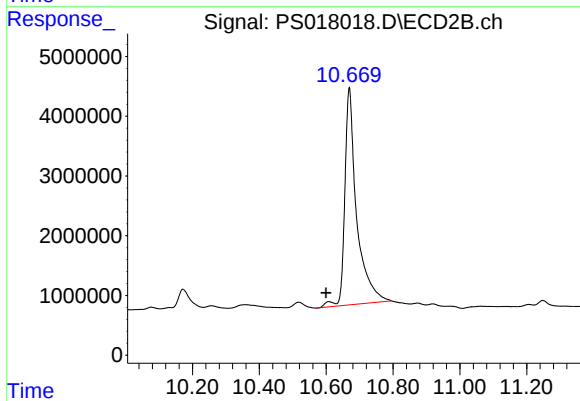

#16 DCPA

R.T.: 10.669 min
Delta R.T.: 0.069 min
Response: 89659871
Conc: 20.31 ng/ml