

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS011522\
 Data File : PS018030.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Jan 2022 14:30
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 16 23:33:54 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010522.M
 Quant Title : 8080.M
 QLast Update : Thu Jan 06 10:21:08 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.050	6.645	652.3E6	296.9E6	451.270	511.687
Target Compounds							
7) T	MCPA	7.496f	0.000	4324667	0	<MDL	N.D. #
9) T	2,4-D	8.215f	0.000	2246248	0	1.234	N.D. #
11) T	2,4,5-TP ...	0.000	8.438f	0	7510829	N.D.	2.107
12) T	2,4,5-T	9.347f	0.000	16856670	0	1.902	N.D. #
14) T	DINOSEB	10.939	0.000	12810451	0	1.951	N.D. #
15) T	Picloram	10.778	0.000	9111083	0	<MDL	N.D. #
16) T	DCPA	11.240	0.000	3846806	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS011522\
Data File : PS018030.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Jan 2022 14:30
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 16 23:33:54 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010522.M
Quant Title : 8080.M
QLast Update : Thu Jan 06 10:21:08 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

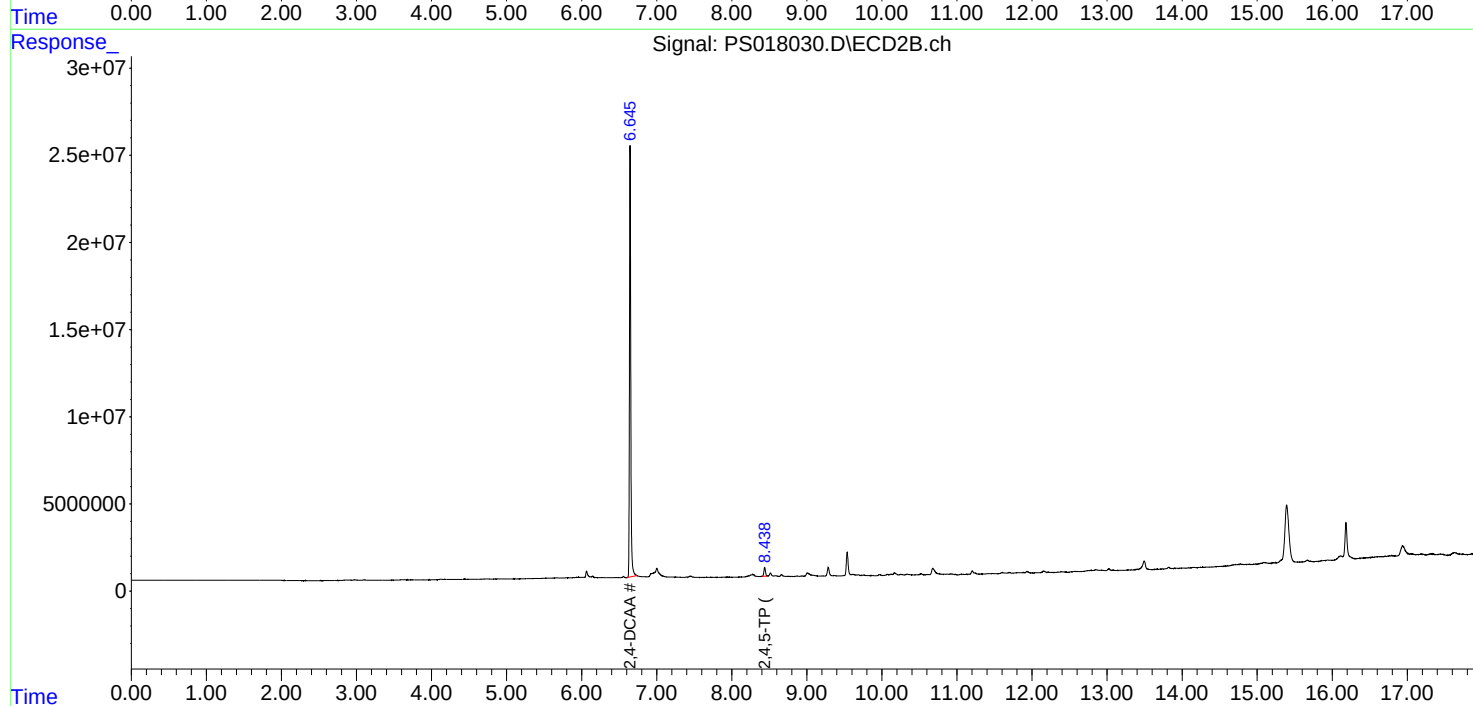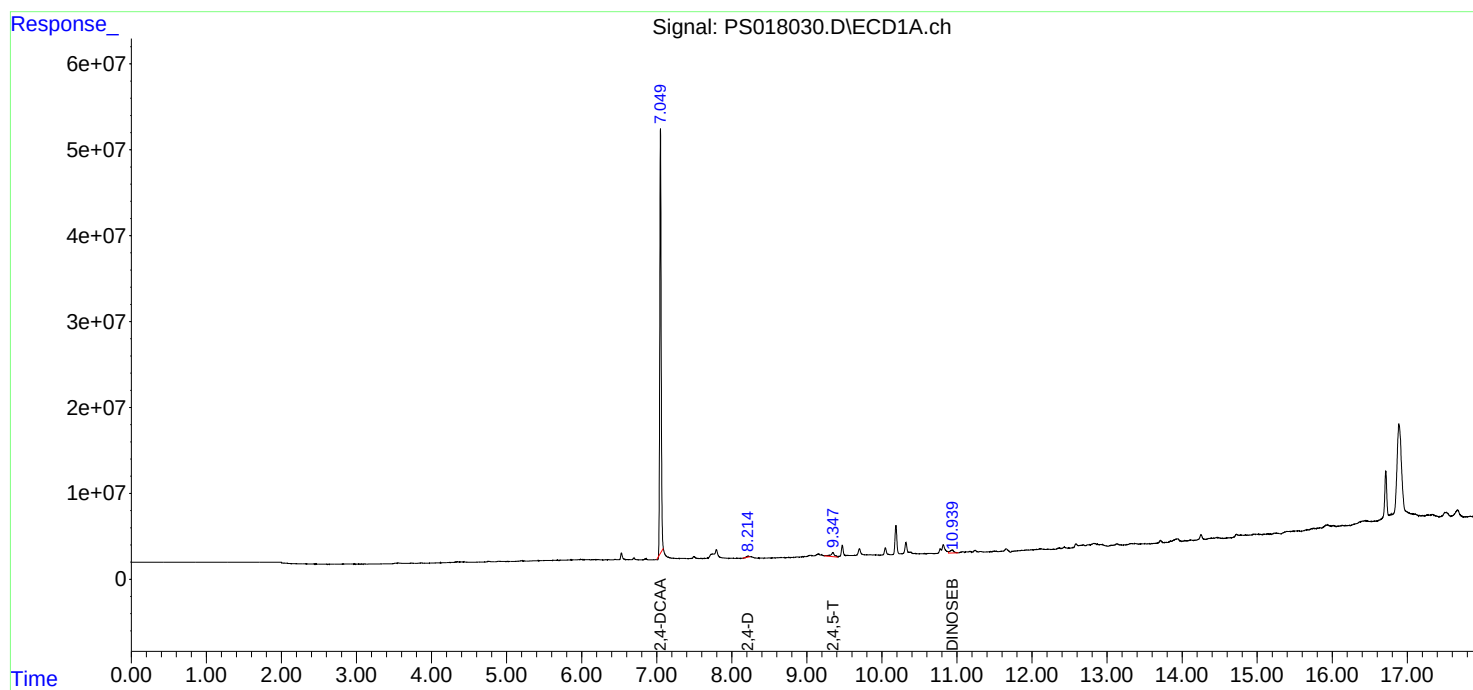


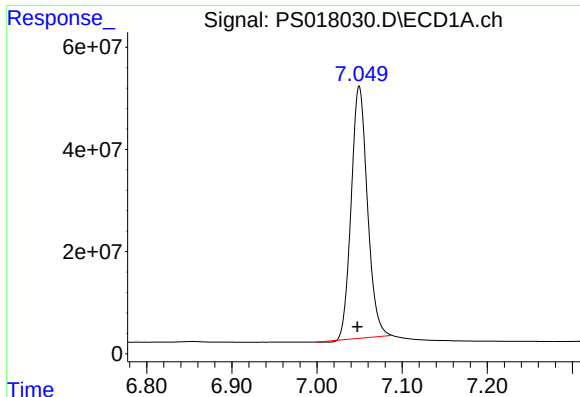

#4 2,4-DCAA


R.T.: 7.050 min
Delta R.T.: 0.002 min
Response: 652305795
Conc: 451.27 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

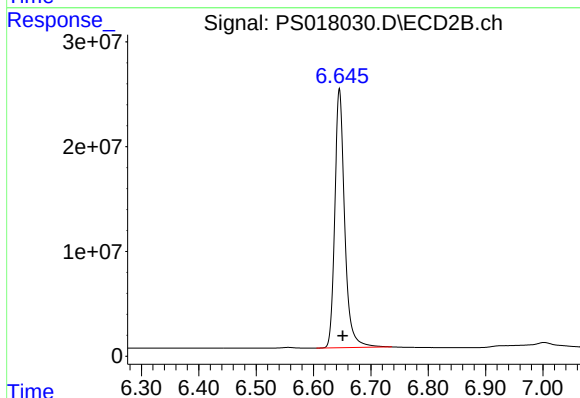


#4 2,4-DCAA

R.T.: 6.645 min
Delta R.T.: -0.006 min
Response: 296905881
Conc: 511.69 ng/ml

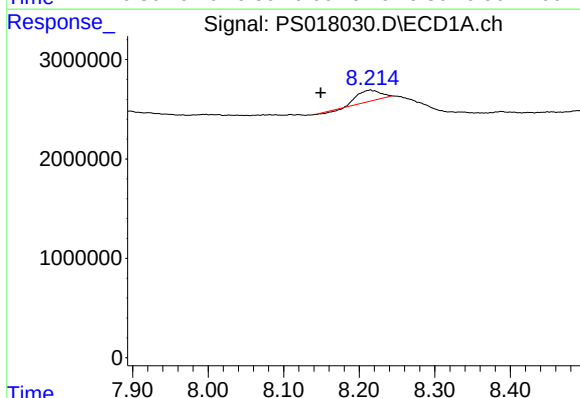


#9 2,4-D

R.T.: 8.215 min
Delta R.T.: 0.065 min
Response: 2246248
Conc: 1.23 ng/ml

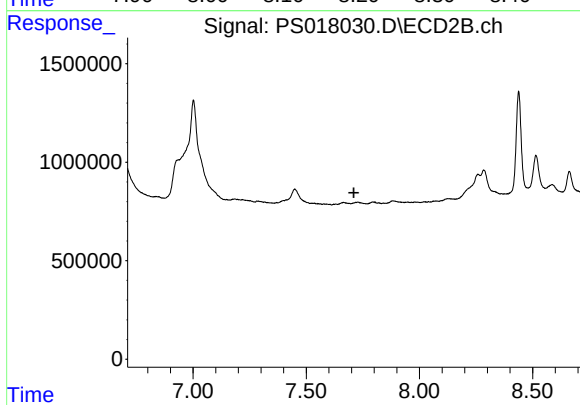

#9 2,4-D


R.T.: 0.000 min
Exp R.T. : 7.710 min
Response: 0
Conc: N.D.

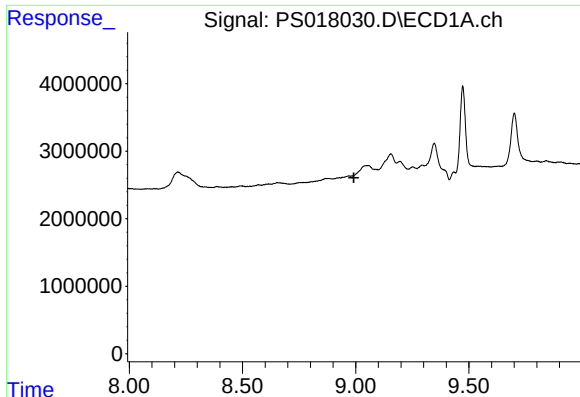

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 8.992 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

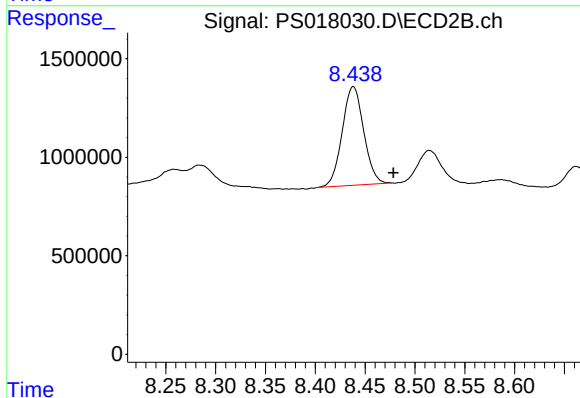


#11 2,4,5-TP (SILVEX)

R.T.: 8.438 min
Delta R.T.: -0.040 min
Response: 7510829
Conc: 2.11 ng/ml

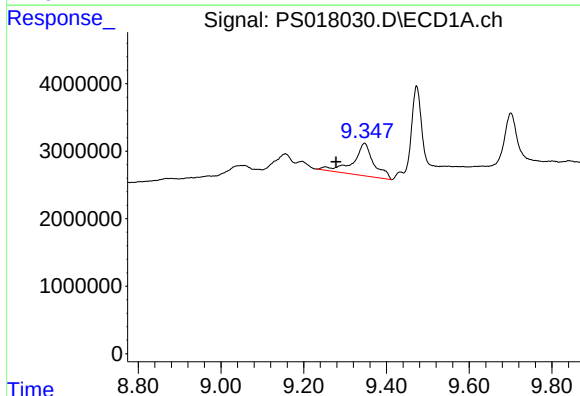


#12 2,4,5-T

R.T.: 9.347 min
Delta R.T.: 0.069 min
Response: 16856670
Conc: 1.90 ng/ml

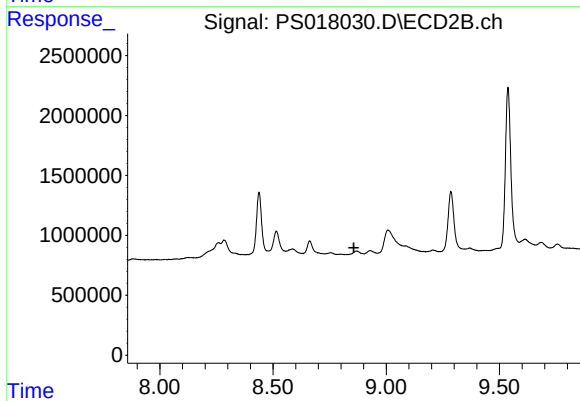

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 8.857 min
Response: 0
Conc: N.D.

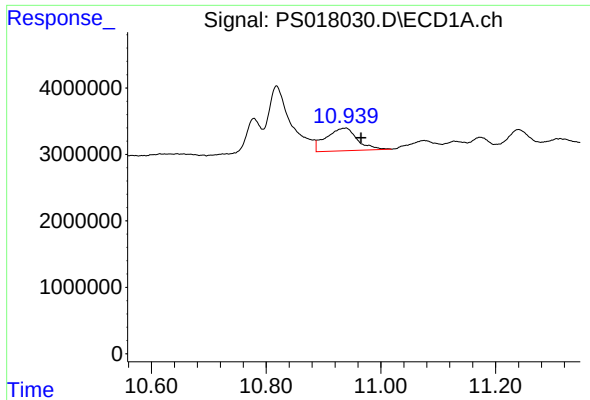

#14 DINOSEB

R.T.: 10.939 min
Delta R.T.: -0.026 min
Response: 12810451
Conc: 1.95 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

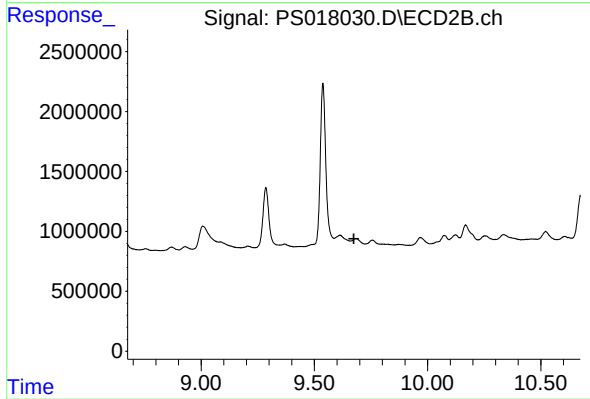

#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 9.675 min
Response: 0
Conc: N.D.