

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS011522\  
 Data File : PS018035.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 15 Jan 2022 16:42  
 Operator : AJ\MA  
 Sample : N1099-10  
 Misc :  
 ALS Vial : 23 Sample Multiplier: 1

Instrument :  
 ECD\_S  
 ClientSampleId :  
 VACLOT-BACKFILL-TILCON-10

Manual Integrations  
 APPROVED

Reviewed By :Abdul Mirza 01/17/2022  
 Supervised By :Ankita Jodhani 01/17/2022

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Jan 16 23:36:30 2022  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS010522.M  
 Quant Title : 8080.M  
 QLast Update : Thu Jan 06 10:21:08 2022  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2 µl  
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

| Compound                    | RT#1  | RT#2  | Resp#1  | Resp#2  | ng/ml   | ng/ml    |
|-----------------------------|-------|-------|---------|---------|---------|----------|
| -----                       |       |       |         |         |         |          |
| System Monitoring Compounds |       |       |         |         |         |          |
| 4) S 2,4-DCAA               | 7.047 | 6.643 | 935.6E6 | 371.2E6 | 647.244 | 639.725m |

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS011522\  
Data File : PS018035.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 15 Jan 2022 16:42  
Operator : AJ\MA  
Sample : N1099-10  
Misc :  
ALS Vial : 23 Sample Multiplier: 1



Instrument :  
ECD\_S  
ClientSampleId :  
VACLOT-BACKFILL-TILCON-10


Manual Integrations  
APPROVED

Reviewed By : Abdul Mirza 01/17/2022  
Supervised By : Ankita Jodhani 01/17/2022

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Jan 16 23:36:30 2022  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS010522.M  
Quant Title : 8080.M  
QLast Update : Thu Jan 06 10:21:08 2022  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 2 µl  
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2  
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

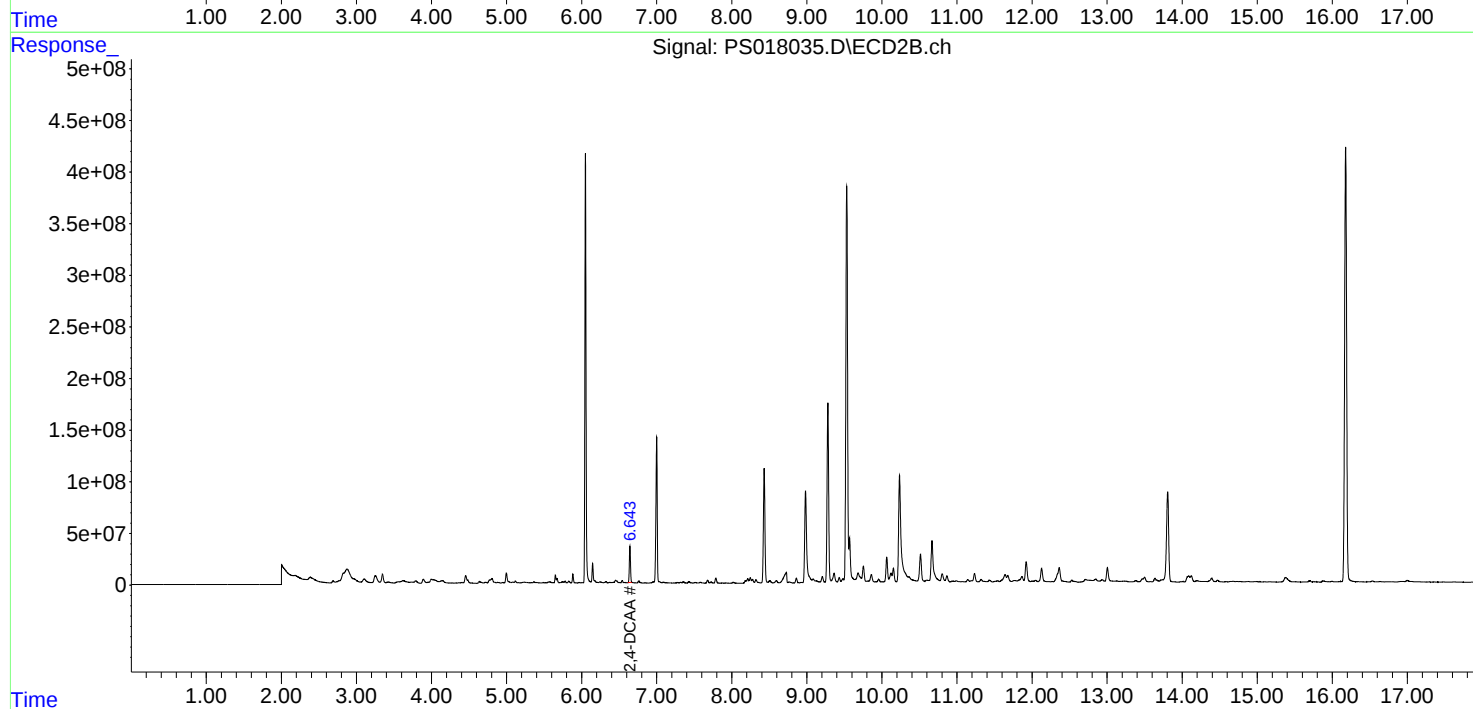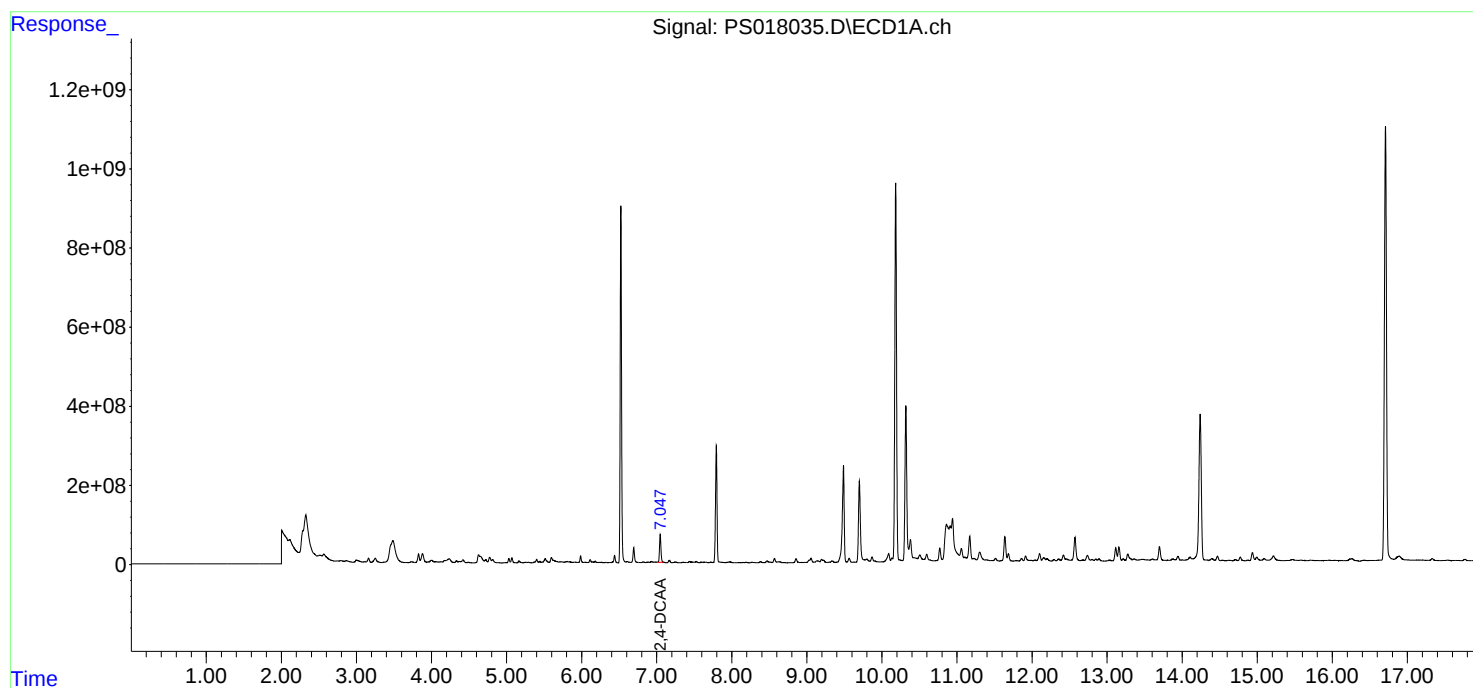

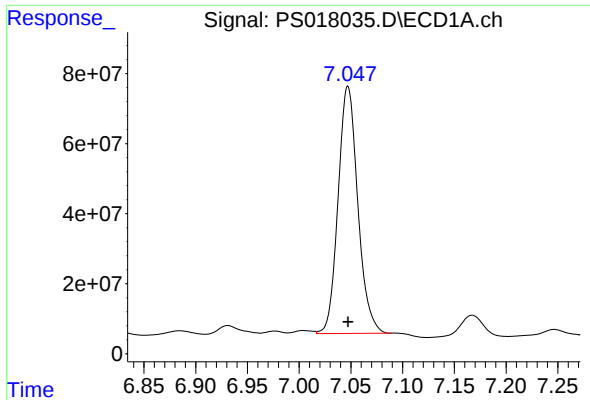


#4 2,4-DCAA

R.T.: 7.047 min  
Delta R.T.: 0.000 min  
Response: 935582820  
Conc: 647.24 ng/ml

Instrument :  
ECD\_S  
ClientSampleId :  
VACLOT-BACKFILL-TILCON-10

Manual Integrations  
APPROVED

Reviewed By :Abdul Mirza 01/17/2022  
Supervised By :Ankita Jodhani 01/17/2022

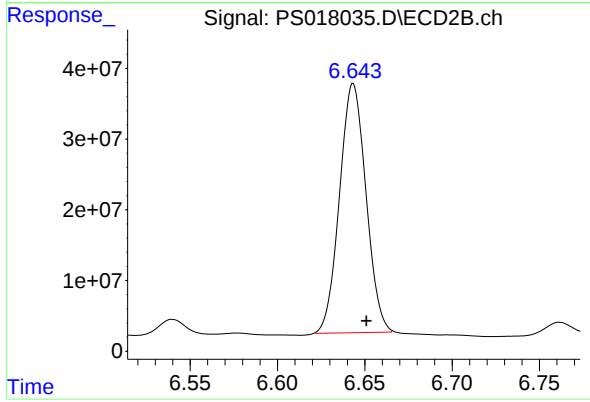

#4 2,4-DCAA

R.T.: 6.643 min  
Delta R.T.: -0.008 min  
Response: 371199468  
Conc: 639.72 ng/ml m