

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS011524\
 Data File : PS025536.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Jan 2024 09:39
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 16 03:41:54 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS011124.M
 Quant Title : 8080.M
 QLast Update : Thu Jan 11 16:45:24 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds						
1) T	Dalapon	0.000	2.557	0	1156682	N.D. <MDL
3) T	4-Nitroph...	0.000	6.363	0	629377	N.D. 1.322
5) T	DICAMBA	0.000	6.959	0	45929310	N.D. 13.801
6) T	MCP	0.000	6.959f	0	45929310	N.D. 19.799
7) T	MCPA	0.000	7.174f	0	7462451	N.D. 2.154
8) T	DICHLORPROP	0.000	7.583f	0	705087	N.D. <MDL
9) T	2,4-D	7.244	0.000	310.1E6	0	168.385 N.D. #
13) T	2,4-DB	0.000	9.480	0	388839	N.D. <MDL
15) T	Picloram	0.000	10.784	0	2153451	N.D. <MDL
16) T	DCPA	0.000	10.784f	0	2153451	N.D. <MDL



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS011524\
Data File : PS025536.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Jan 2024 09:39
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 16 03:41:54 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS011124.M
Quant Title : 8080.M
QLast Update : Thu Jan 11 16:45:24 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

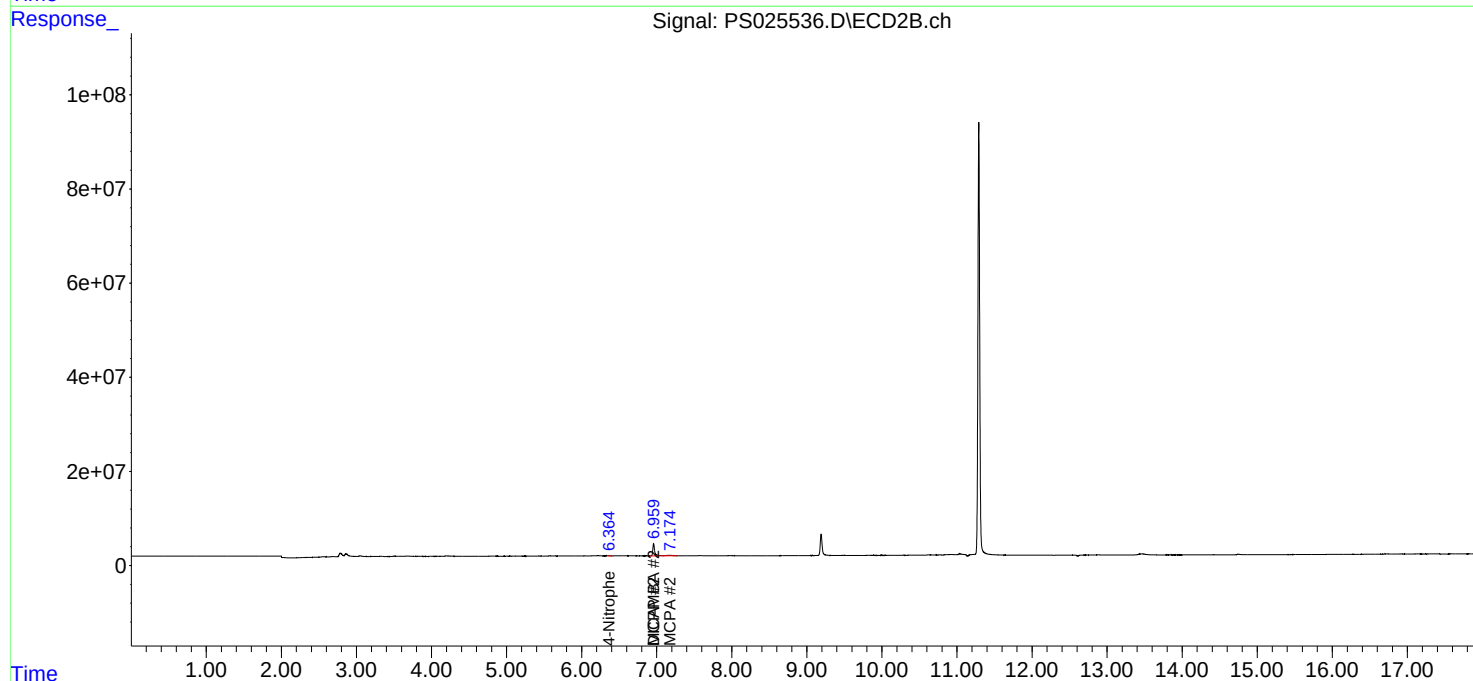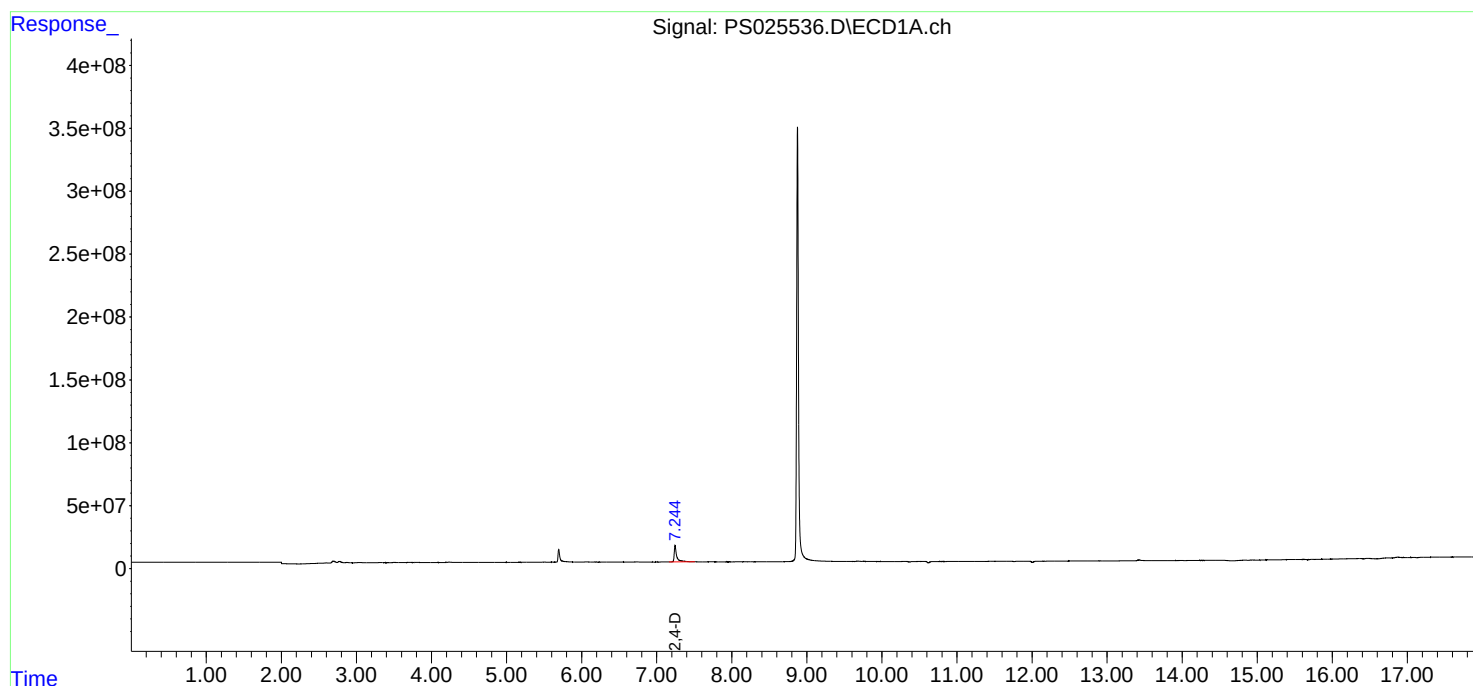


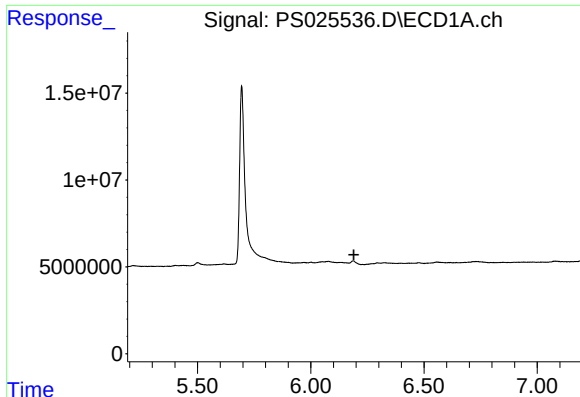

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 6.191 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

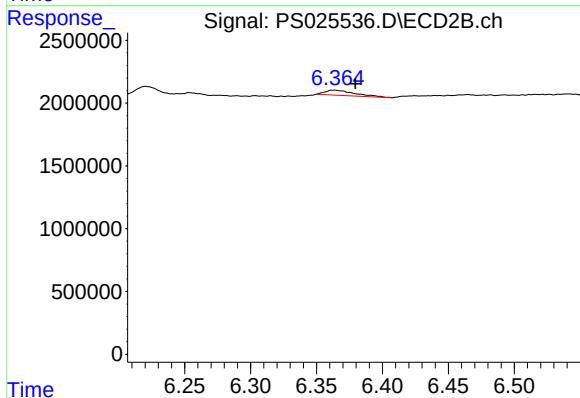


#3 4-Nitrophenol

R.T.: 6.363 min
Delta R.T.: -0.016 min
Response: 629377
Conc: 1.32 ng/ml

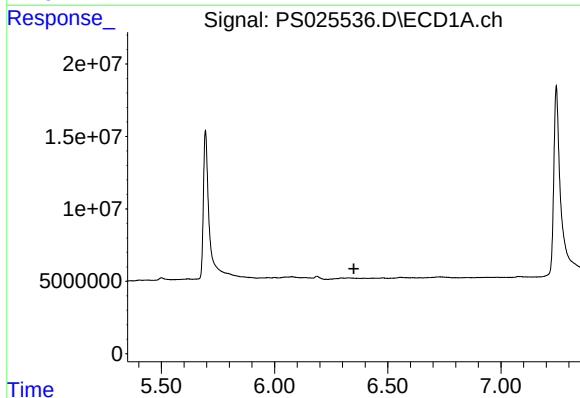


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T.: 6.350 min
Response: 0
Conc: N.D.

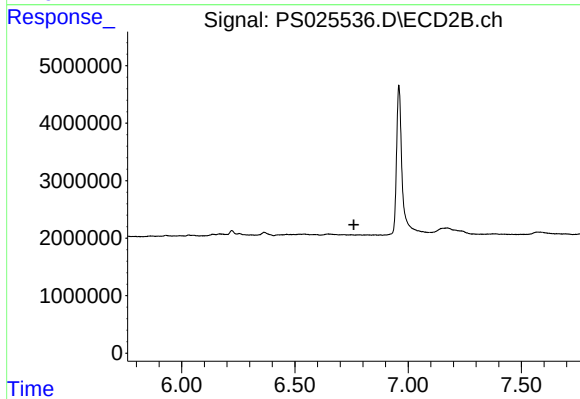

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T.: 6.761 min
Response: 0
Conc: N.D.

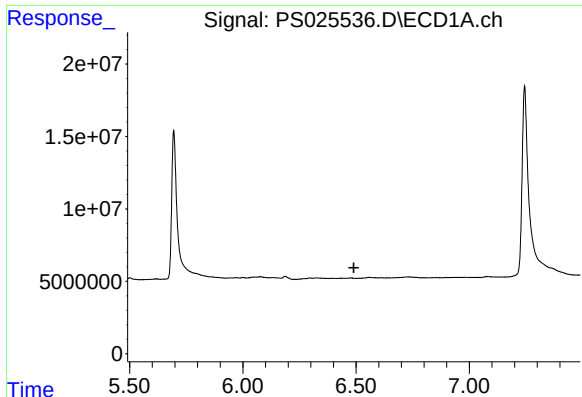

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 6.491 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

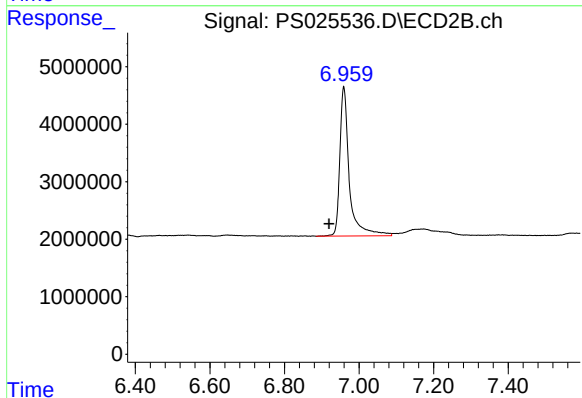


#5 DICAMBA

R.T.: 6.959 min
Delta R.T.: 0.039 min
Response: 45929310
Conc: 13.80 ng/ml

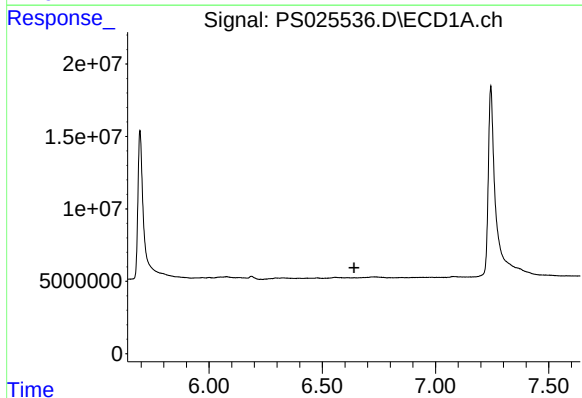


#6 MCP

R.T.: 0.000 min
Exp R.T.: 6.640 min
Response: 0
Conc: N.D.

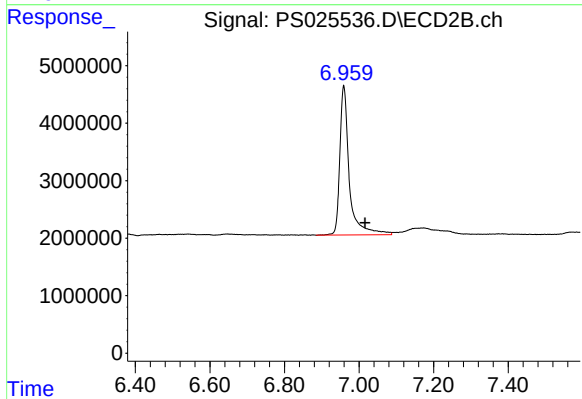

#6 MCP


R.T.: 6.959 min
Delta R.T.: -0.057 min
Response: 45929310
Conc: 19.80 ug/ml

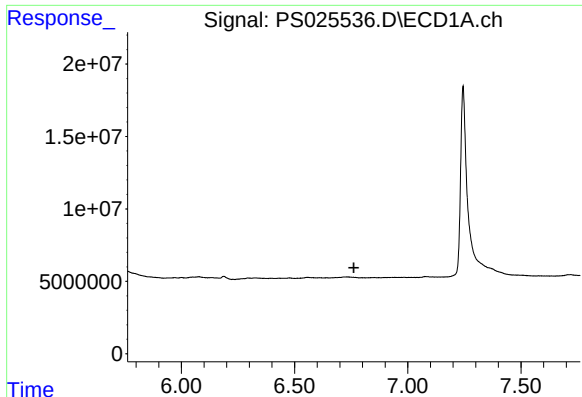

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 6.762 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

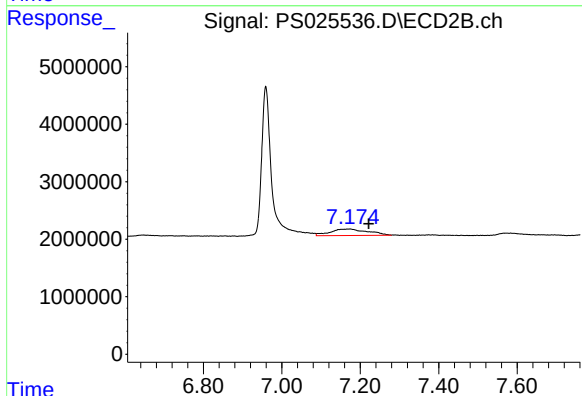


#7 MCPA

R.T.: 7.174 min
Delta R.T.: -0.047 min
Response: 7462451
Conc: 2.15 ug/ml

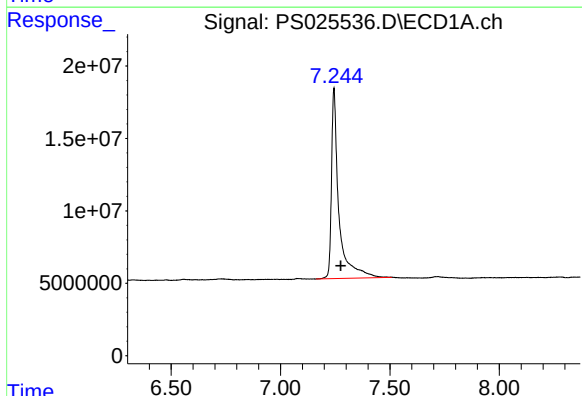

#9 2,4-D

R.T.: 7.244 min
Delta R.T.: -0.031 min
Response: 310056103
Conc: 168.39 ng/ml

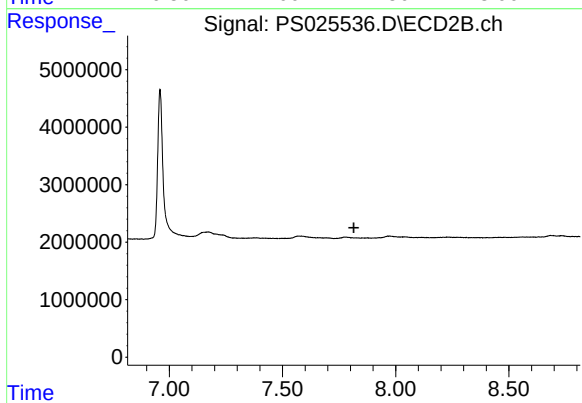

#9 2,4-D

R.T.: 0.000 min
Exp R.T.: 7.815 min
Response: 0
Conc: N.D.