

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS011525\
 Data File : PS028909.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Jan 2025 09:08
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 15 20:36:35 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS011425.M
 Quant Title : 8080.M
 QLast Update : Tue Jan 14 12:25:39 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.199	0.000	140847	0	<MDL	N.D. #
Target Compounds							
1) T	Dalapon	2.588f	0.000	108128	0	<MDL	N.D. #
2) T	3,5-DICHL...	6.360	0.000	1609883	0	<MDL	N.D. #
3) T	4-Nitroph...	6.983	0.000	5122711	0	2.891	N.D. #
5) T	DICAMBA	7.378	7.880	89538	3209973	<MDL	<MDL #
6) T	MCPD	7.521f	0.000	1241558	0	<MDL	N.D. #
7) T	MCPA	7.713	8.202	190342	3844965	<MDL	<MDL #
8) T	DICHLORPROP	8.091	8.635f	153372	2861898	<MDL	2.036 #
10) T	Pentachlo...	8.616	0.000	398792	0	<MDL	N.D. #
11) T	2,4,5-TP ...	9.157f	0.000	2362328	0	<MDL	N.D. #
13) T	2,4-DB	10.058	0.000	765012	0	<MDL	N.D. #
15) T	Picloram	11.086	12.266	59085927	8274160	1.873	<MDL #
16) T	DCPA	11.532	0.000	10438341	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS011525\
Data File : PS028909.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Jan 2025 09:08
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 15 20:36:35 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS011425.M
Quant Title : 8080.M
QLast Update : Tue Jan 14 12:25:39 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

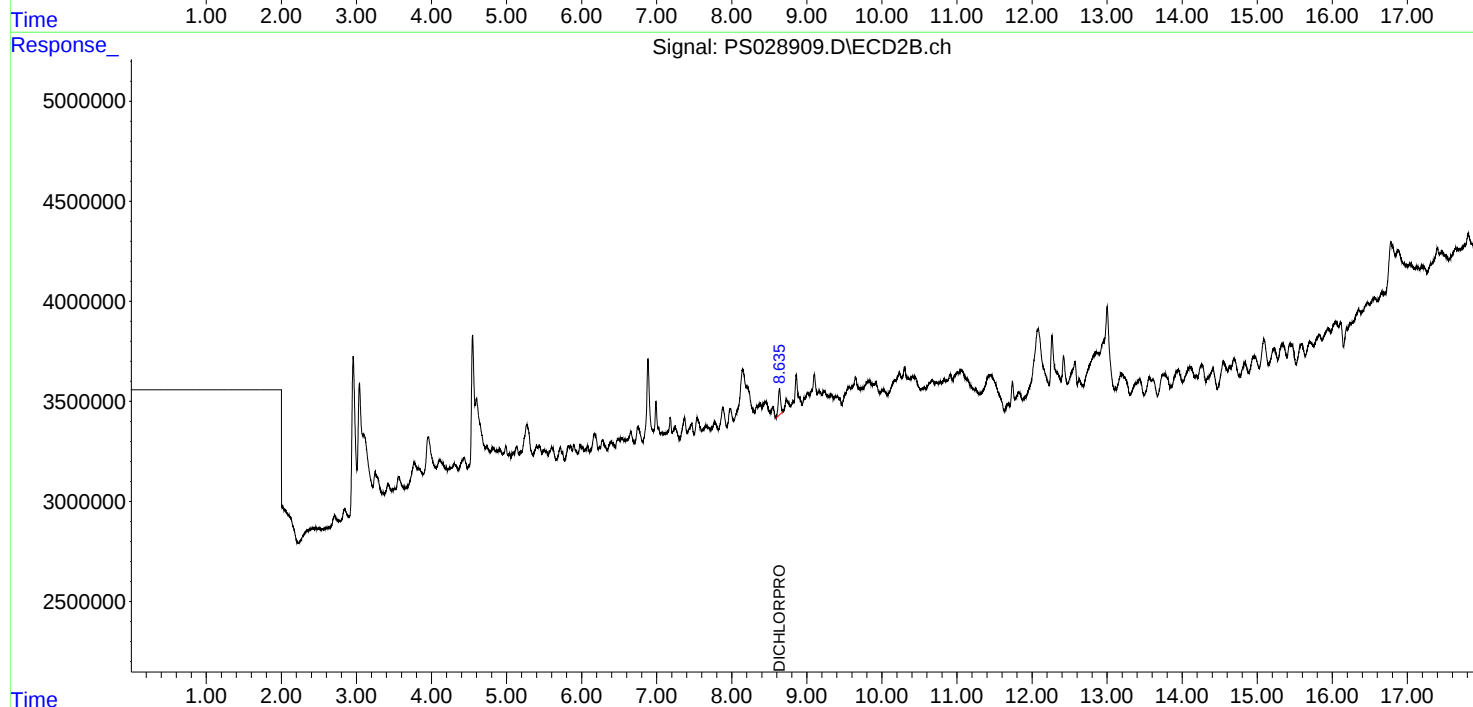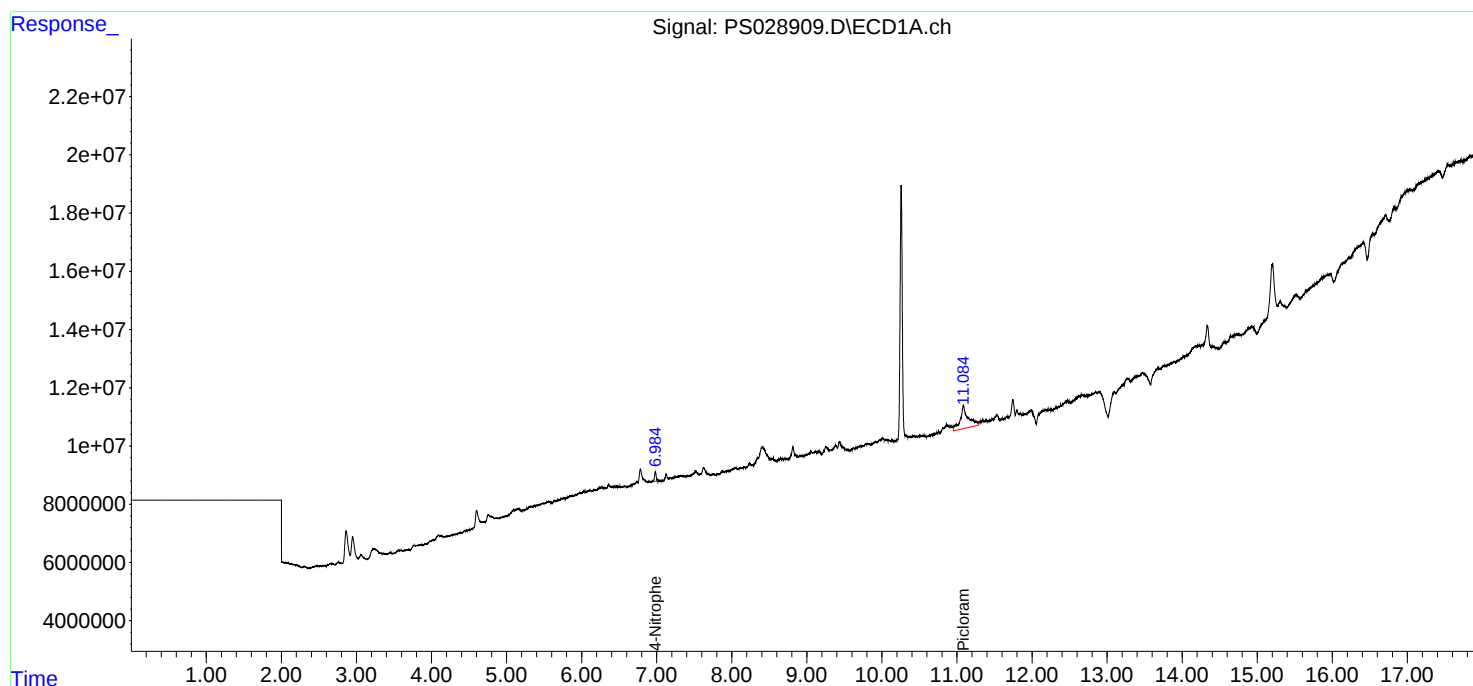


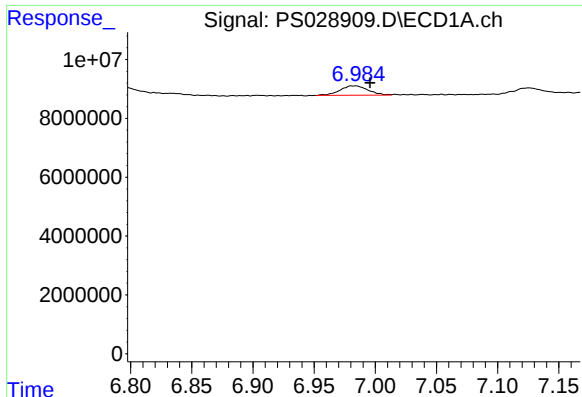

#3 4-Nitrophenol


R.T.: 6.983 min
Delta R.T.: -0.013 min
Response: 5122711
Conc: 2.89 ng/ml

Instrument :
ECD_S
ClientSampleId :
HEXANE

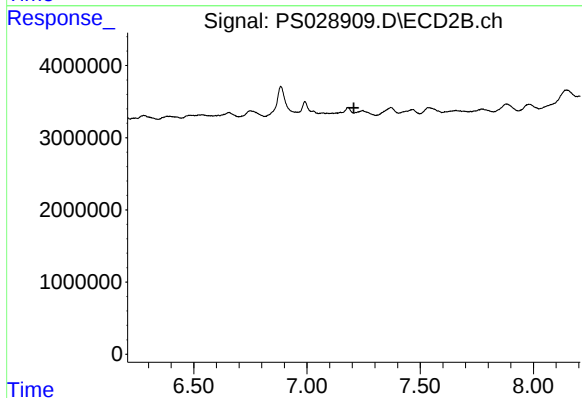


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 7.207 min
Response: 0
Conc: N.D.

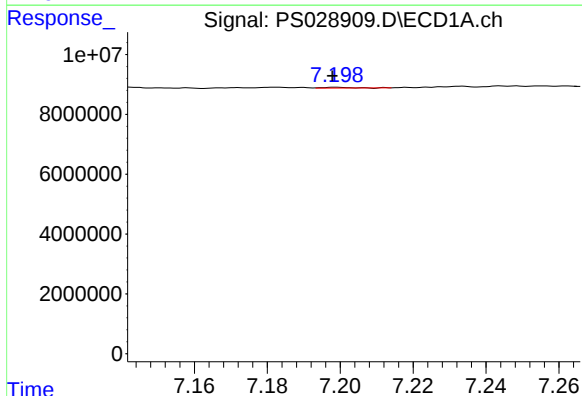


#4 2,4-DCAA

R.T.: 7.199 min
Delta R.T.: 0.001 min
Response: 140847
Conc: N.D.

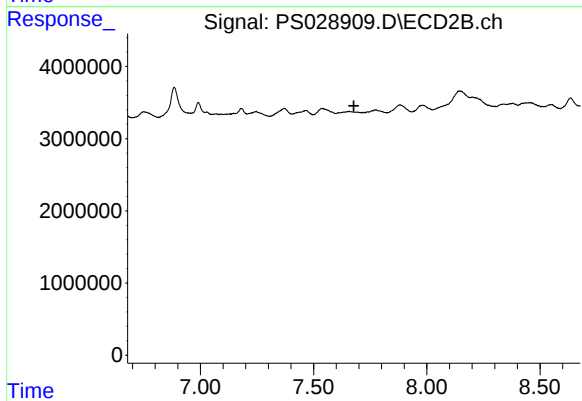

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T. : 7.678 min
Response: 0
Conc: N.D.

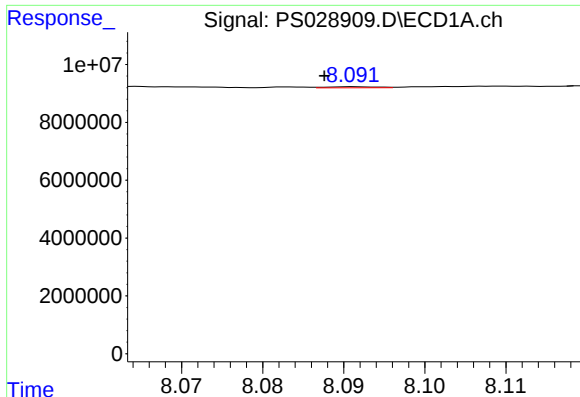

#8 DICHLORPROP


R.T.: 8.091 min
Delta R.T.: 0.004 min
Response: 153372
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

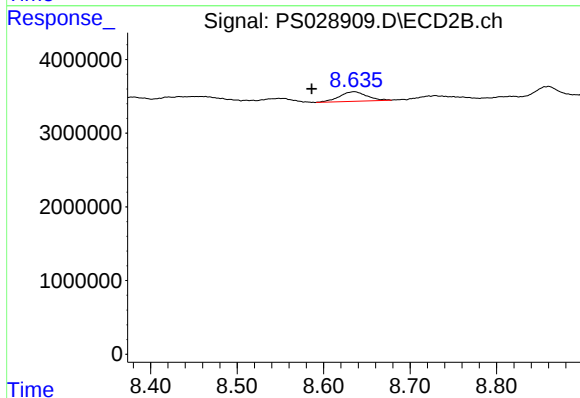


#8 DICHLORPROP

R.T.: 8.635 min
Delta R.T.: 0.049 min
Response: 2861898
Conc: 2.04 ng/ml

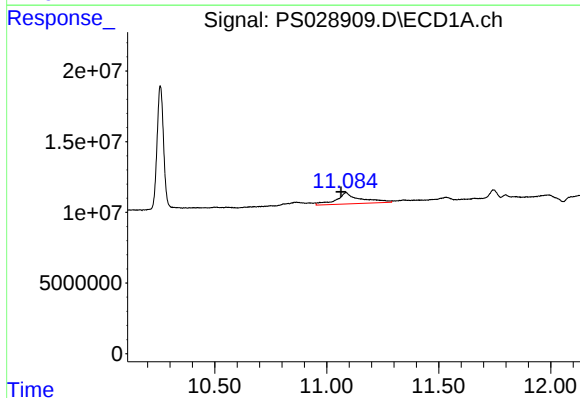

#15 Picloram

R.T.: 11.086 min
Delta R.T.: 0.021 min
Response: 59085927
Conc: 1.87 ng/ml

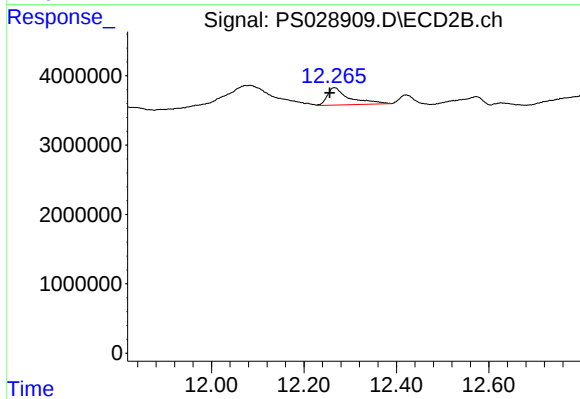

#15 Picloram

R.T.: 12.266 min
Delta R.T.: 0.010 min
Response: 8274160
Conc: N.D.