

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS011623\
 Data File : PS021762.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Jan 2023 08:22
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 17 02:28:16 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010923.M
 Quant Title : 8080.M
 QLast Update : Tue Jan 10 10:34:52 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml	

System Monitoring Compounds								
4) S	2,4-DCAA	6.354	0.000	28981223	0	10.412	N.D.	#
Target Compounds								
1) T	Dalapon	2.510	2.586	2555156	477845	<MDL	<MDL	#
3) T	4-Nitroph...	6.211	6.468f	7574842	1348795	5.197	1.230	#
5) T	DICAMBA	0.000	7.023f	0	2912.9E6	N.D.	342.579	
6) T	MCP	6.640	7.023f	160444	2912.9E6	<MDL	439.242	#
7) T	MCPA	6.839	0.000	1080487	0	<MDL	N.D.	#
8) T	DICHLORPROP	7.114	7.618	1261631	17867411	<MDL	8.375	#
9) T	2,4-D	7.282	7.923	6083.0E6	3543403	1566.244	1.402	#
10) T	Pentachlo...	7.542	8.316	4481151	2282586	<MDL	<MDL	#
11) T	2,4,5-TP ...	8.097	8.676	37366725	4263755	2.028	<MDL	#
14) T	DINOSEB	9.944f	9.836f	3692024	7139611	<MDL	<MDL	#
15) T	Picloram	9.711	10.829	1159.6E6	92210257	40.878	5.207	#
16) T	DCPA	10.157	10.829	5035613	92210257	<MDL	6.615	#



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS011623\
Data File : PS021762.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Jan 2023 08:22
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 17 02:28:16 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010923.M
Quant Title : 8080.M
QLast Update : Tue Jan 10 10:34:52 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

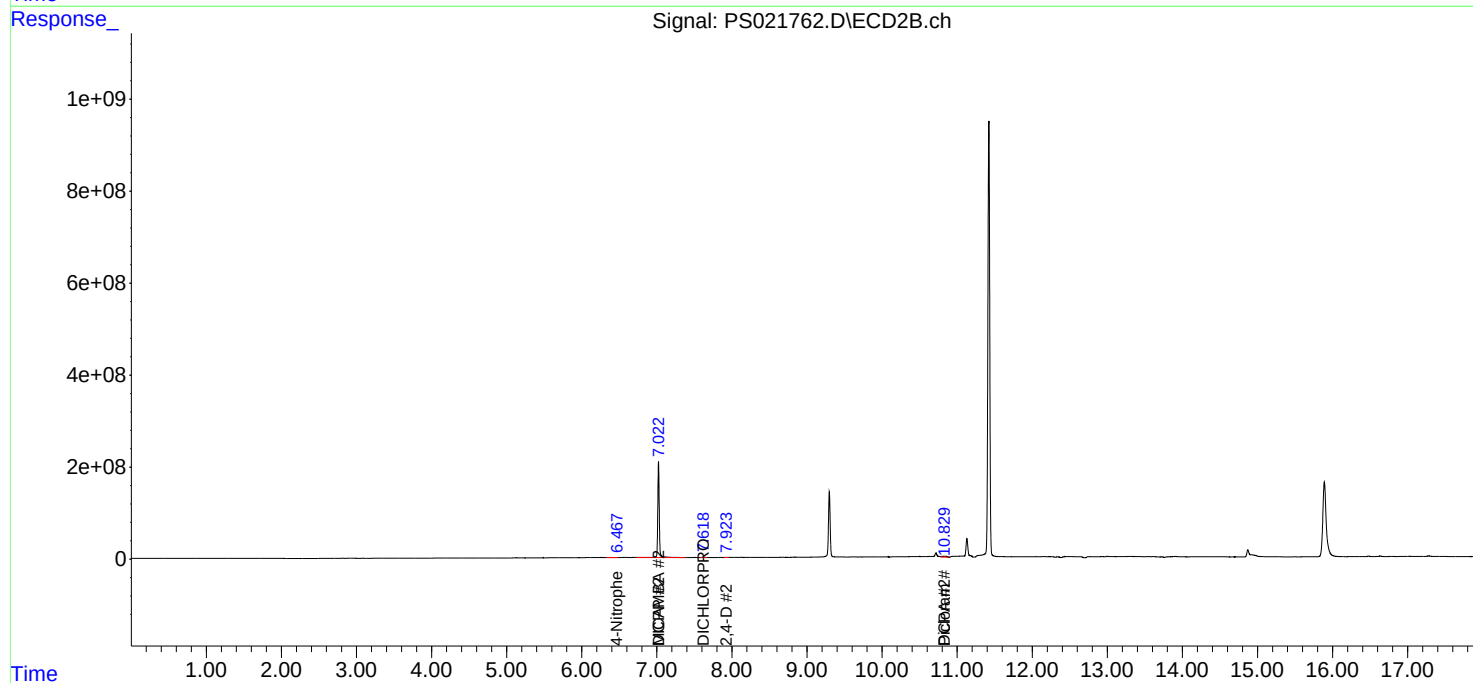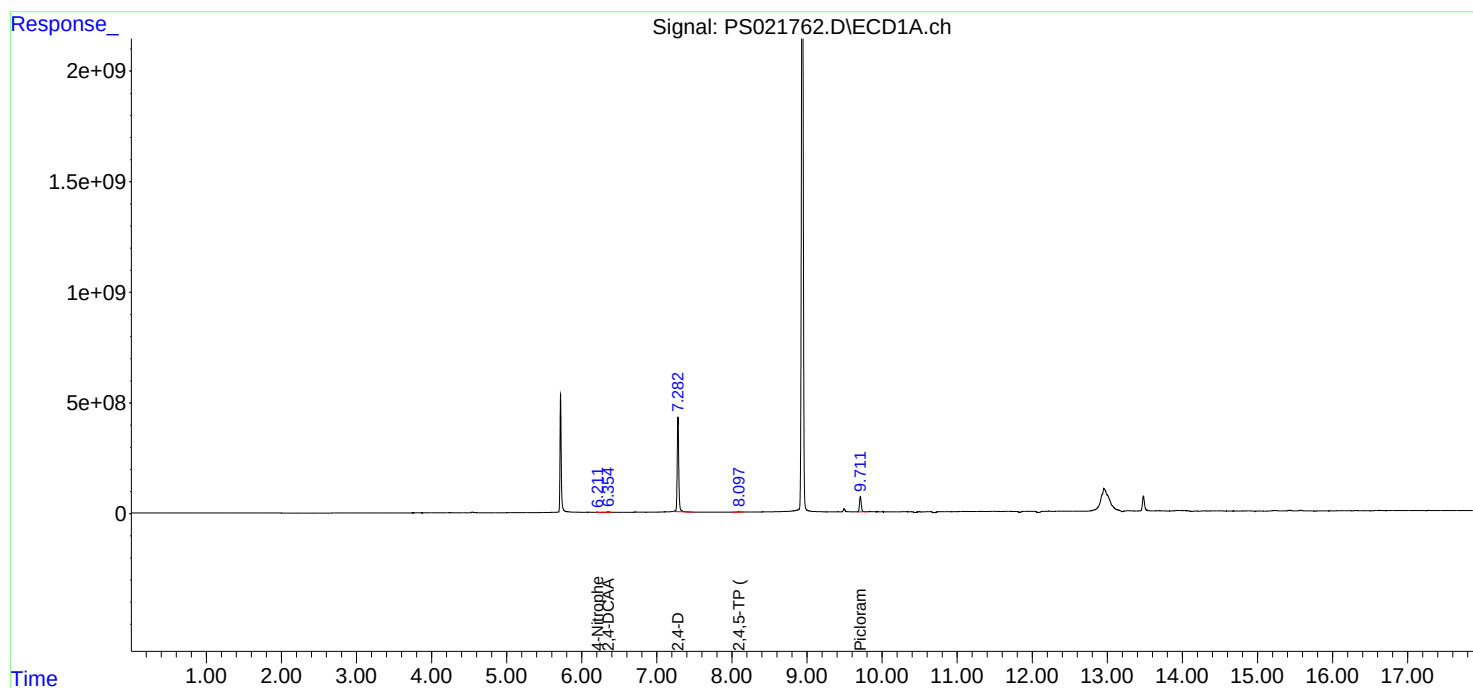


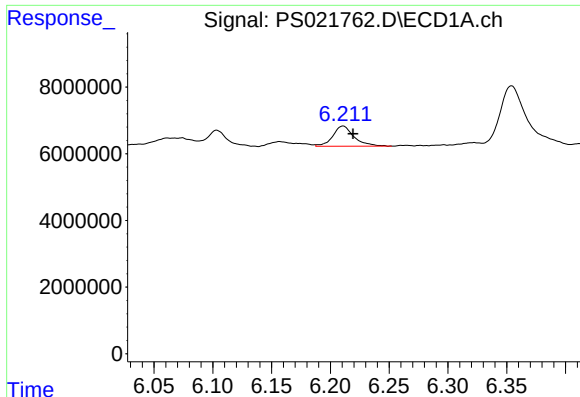

#3 4-Nitrophenol


R.T.: 6.211 min
Delta R.T.: -0.009 min
Response: 7574842
Conc: 5.20 ng/ml

Instrument :
ECD_S
ClientSampleId :

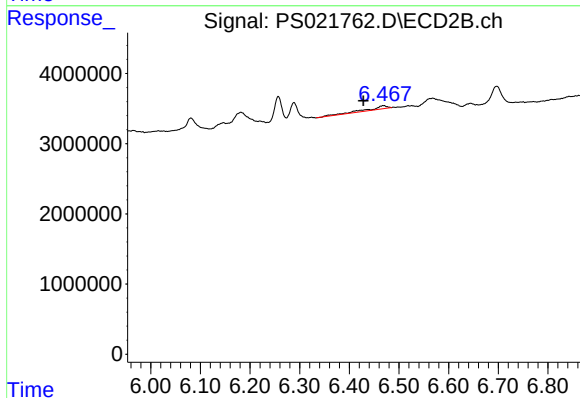


#3 4-Nitrophenol

R.T.: 6.468 min
Delta R.T.: 0.040 min
Response: 1348795
Conc: 1.23 ng/ml

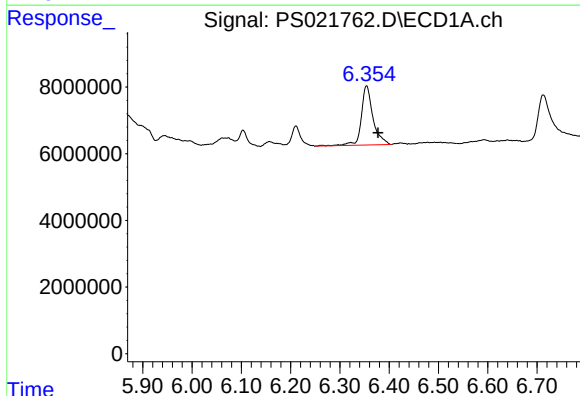


#4 2,4-DCAA

R.T.: 6.354 min
Delta R.T.: -0.023 min
Response: 28981223
Conc: 10.41 ng/ml

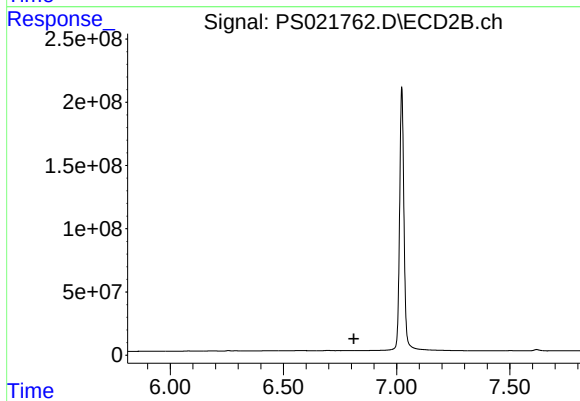

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T. : 6.811 min
Response: 0
Conc: N.D.

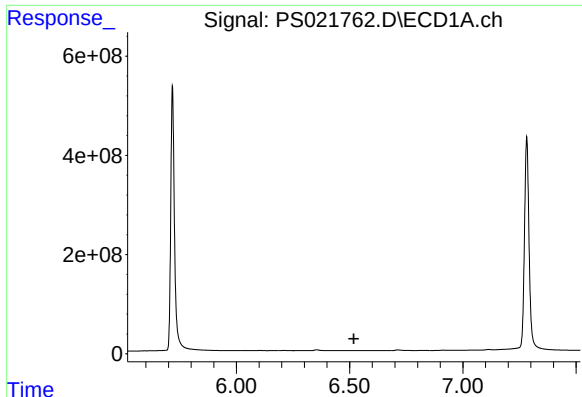

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 6.518 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

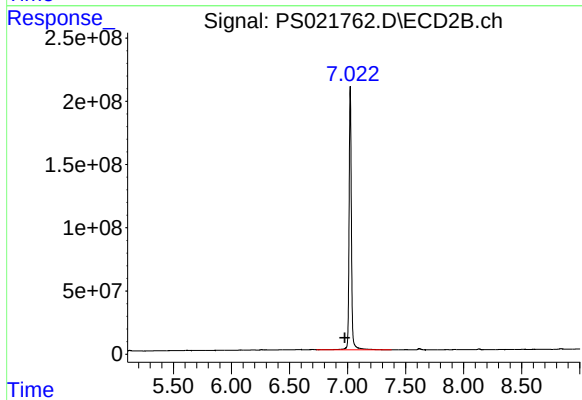


#5 DICAMBA

R.T.: 7.023 min
Delta R.T.: 0.048 min
Response: 2912865526
Conc: 342.58 ng/ml

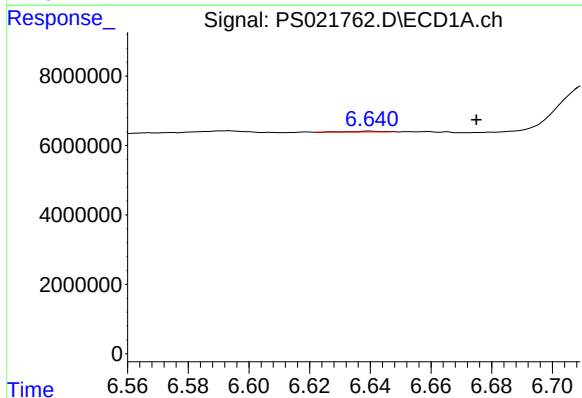


#6 MCPP

R.T.: 6.640 min
Delta R.T.: -0.035 min
Response: 160444
Conc: N.D.

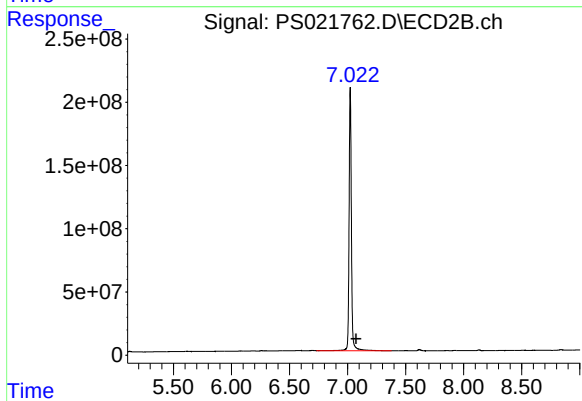

#6 MCPP


R.T.: 7.023 min
Delta R.T.: -0.051 min
Response: 2912865526
Conc: 439.24 ug/ml

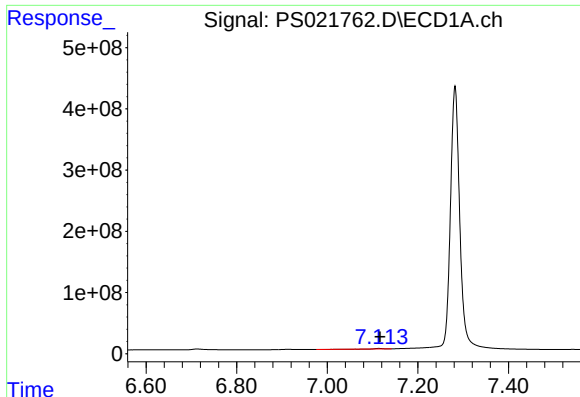

#8 DICHLORPROP


R.T.: 7.114 min
Delta R.T.: -0.003 min
Response: 1261631
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

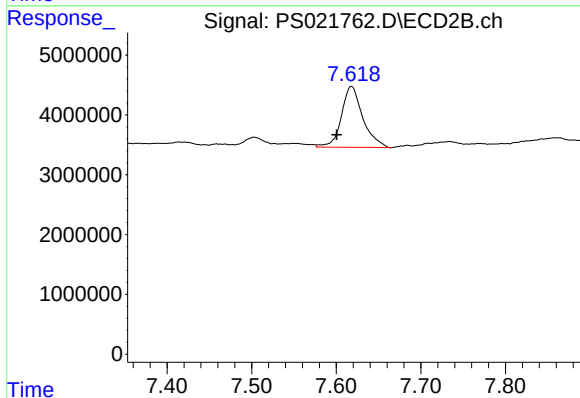


#8 DICHLORPROP

R.T.: 7.618 min
Delta R.T.: 0.018 min
Response: 17867411
Conc: 8.37 ng/ml

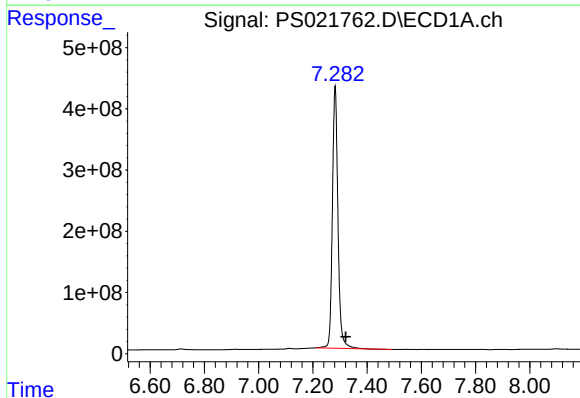


#9 2,4-D

R.T.: 7.282 min
Delta R.T.: -0.039 min
Response: 6082982233
Conc: 1566.24 ng/ml

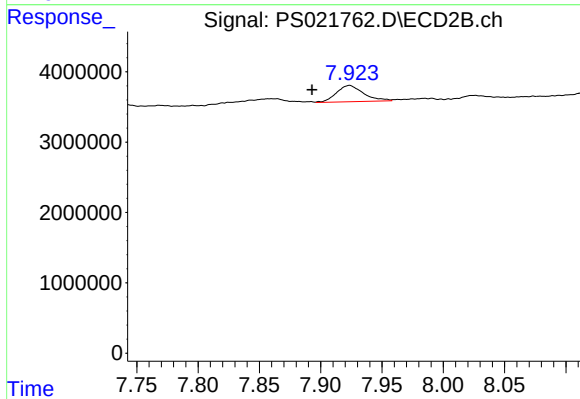

#9 2,4-D


R.T.: 7.923 min
Delta R.T.: 0.030 min
Response: 3543403
Conc: 1.40 ng/ml

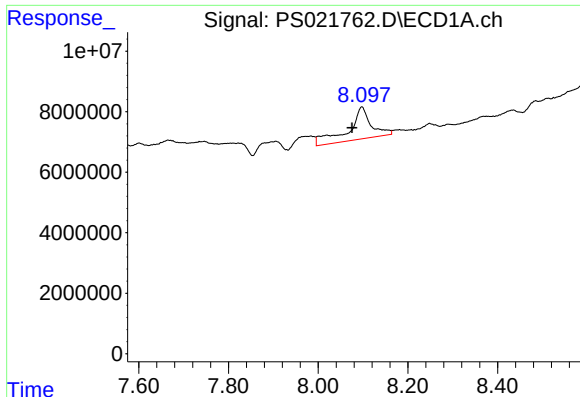

#11 2,4,5-TP (SILVEX)


R.T.: 8.097 min
Delta R.T.: 0.022 min
Response: 37366725
Conc: 2.03 ng/ml

Instrument :
ECD_S
ClientSampleId :

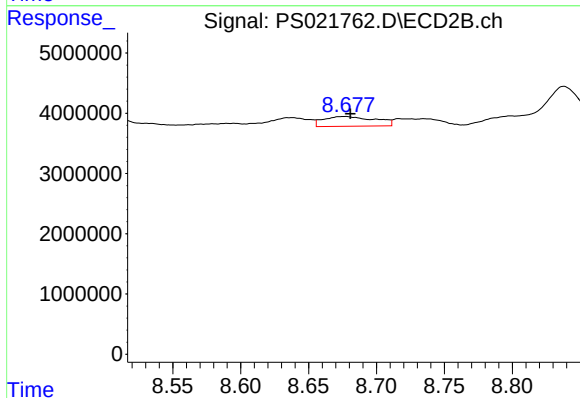


#11 2,4,5-TP (SILVEX)

R.T.: 8.676 min
Delta R.T.: -0.005 min
Response: 4263755
Conc: N.D.

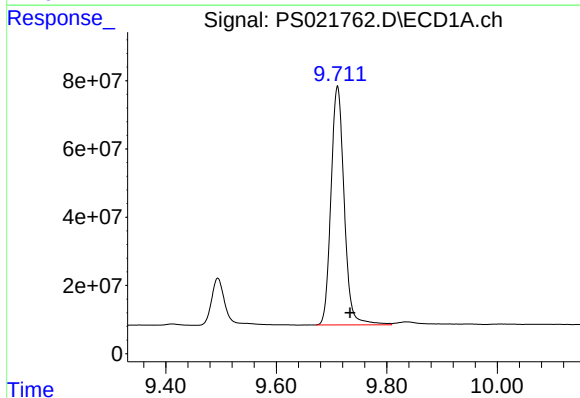


#15 Picloram

R.T.: 9.711 min
Delta R.T.: -0.023 min
Response: 1159613206
Conc: 40.88 ng/ml

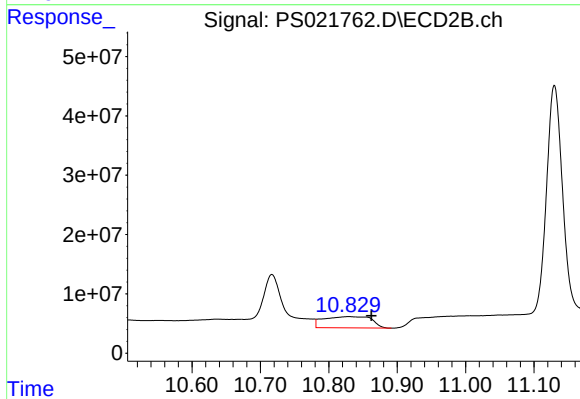

#15 Picloram


R.T.: 10.829 min
Delta R.T.: -0.033 min
Response: 92210257
Conc: 5.21 ng/ml

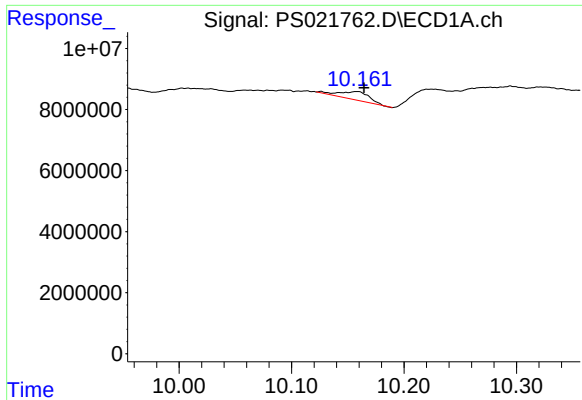

#16 DCPA

R.T.: 10.157 min
Delta R.T.: -0.007 min
Response: 5035613
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

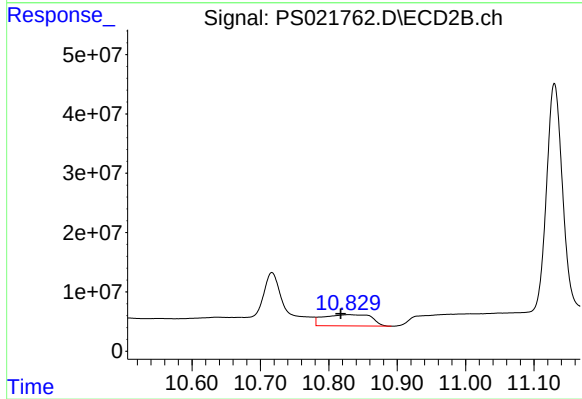

#16 DCPA

R.T.: 10.829 min
Delta R.T.: 0.012 min
Response: 92210257
Conc: 6.61 ng/ml