

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS011623\
 Data File : PS021787.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Jan 2023 19:58
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 17 02:47:25 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010923.M
 Quant Title : 8080.M
 QLast Update : Tue Jan 10 10:34:52 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.377	6.810	1472.0E6	1071.7E6	528.835	596.466
Target Compounds							
1) T	Dalapon	2.516	0.000	671865	0	<MDL	N.D. #
2) T	3,5-DICHL...	5.801f	0.000	255015	0	<MDL	N.D. #
3) T	4-Nitroph...	6.223	0.000	6615204	0	4.538	N.D. #
7) T	MCPA	6.758f	0.000	6899389	0	<MDL	N.D. #
8) T	DICHLORPROP	7.135	7.653f	598369	4773357	<MDL	2.237 #
10) T	Pentachlo...	7.539	0.000	1297212	0	<MDL	N.D. #
11) T	2,4,5-TP ...	8.088	8.683	2837813	1028829	<MDL	<MDL #
12) T	2,4,5-T	8.316	9.082	2578959	4421002	<MDL	<MDL #
13) T	2,4-DB	8.827	9.593	598709	691398	<MDL	<MDL #
14) T	DINOSEB	9.894	9.893	3070303	1171304	<MDL	<MDL #
15) T	Picloram	9.756	10.819f	6087707	1861502	<MDL	<MDL #
16) T	DCPA	10.166	10.819	2391973	1861502	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS011623\
Data File : PS021787.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Jan 2023 19:58
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 17 02:47:25 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010923.M
Quant Title : 8080.M
QLast Update : Tue Jan 10 10:34:52 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

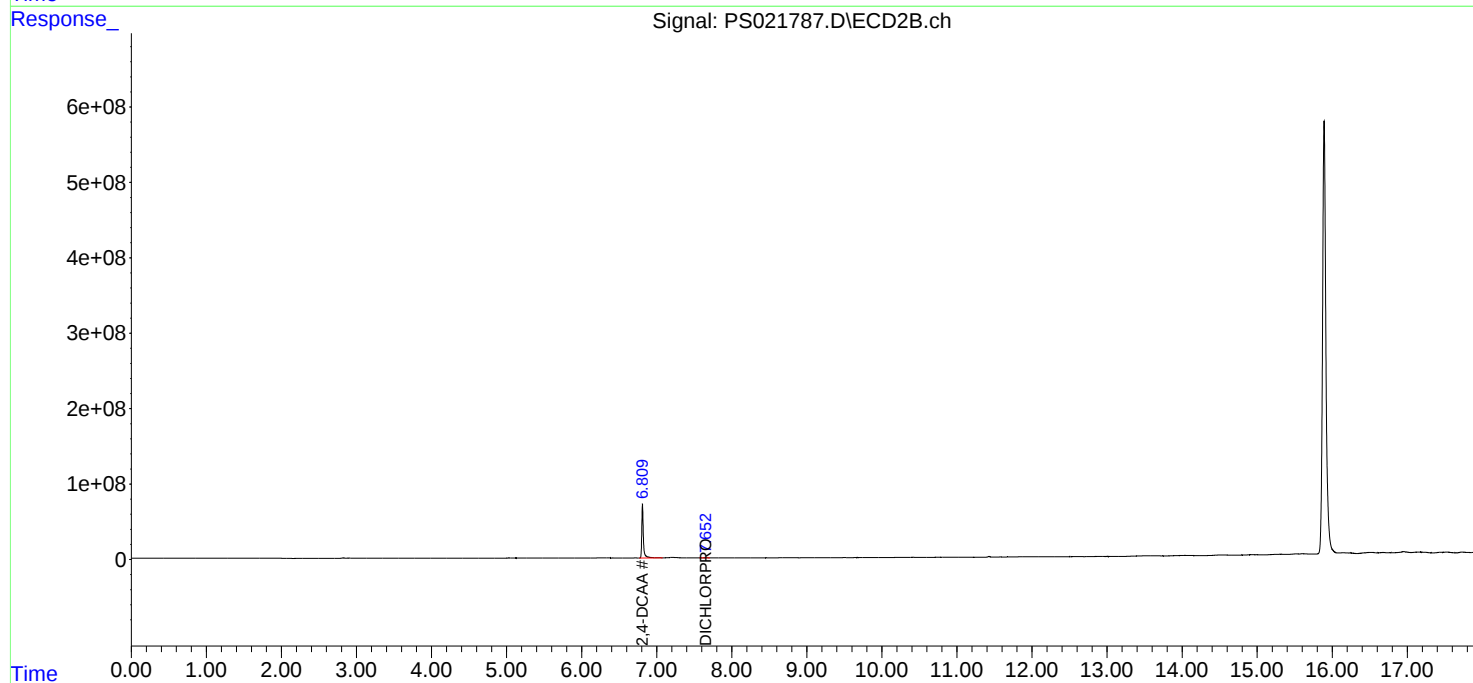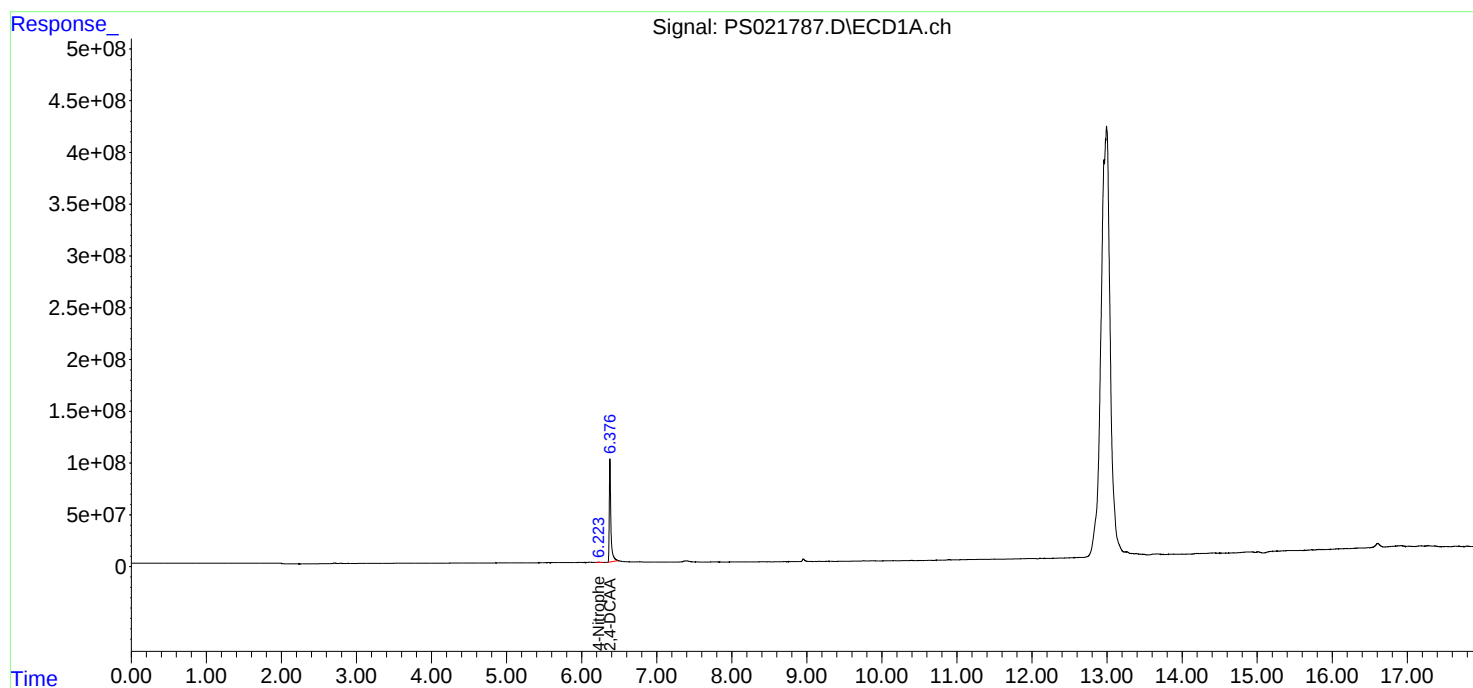


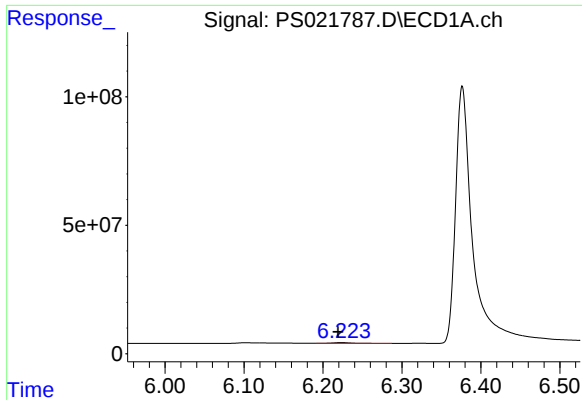

#3 4-Nitrophenol


R.T.: 6.223 min
Delta R.T.: 0.004 min
Response: 6615204
Conc: 4.54 ng/ml

Instrument :
ECD_S
ClientSampleId :

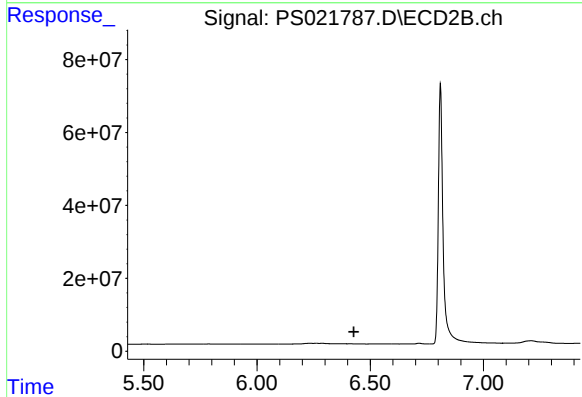


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.428 min
Response: 0
Conc: N.D.

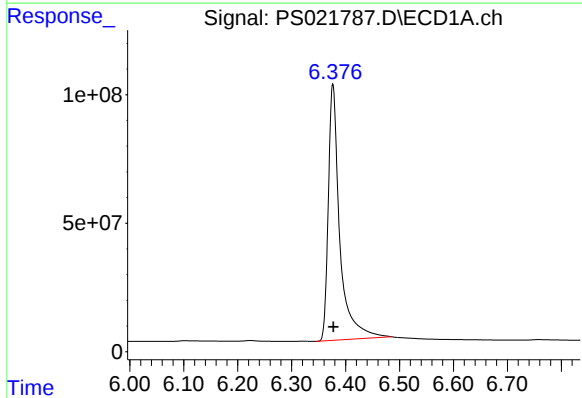


#4 2,4-DCAA

R.T.: 6.377 min
Delta R.T.: 0.000 min
Response: 1472046081
Conc: 528.83 ng/ml

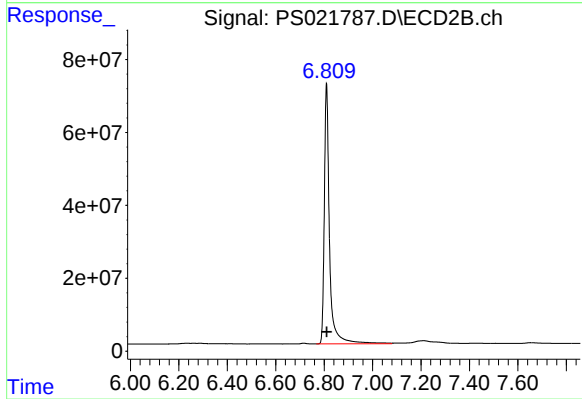

#4 2,4-DCAA


R.T.: 6.810 min
Delta R.T.: -0.002 min
Response: 1071664984
Conc: 596.47 ng/ml

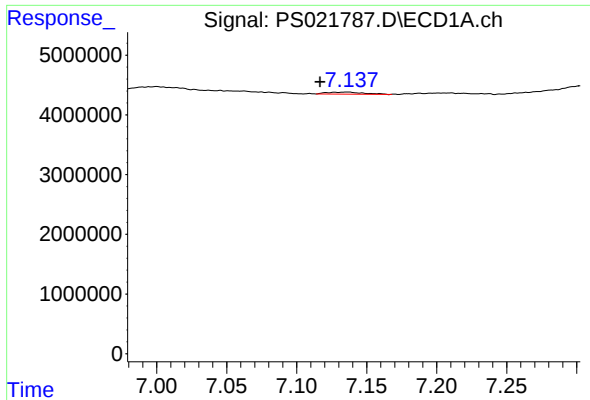

#8 DICHLORPROP

R.T.: 7.135 min
Delta R.T.: 0.019 min
Response: 598369
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

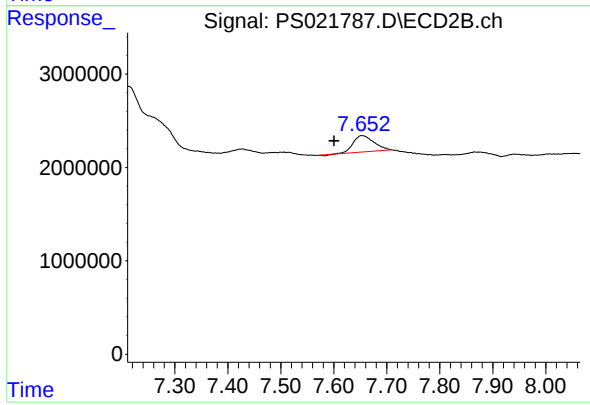

#8 DICHLORPROP

R.T.: 7.653 min
Delta R.T.: 0.053 min
Response: 4773357
Conc: 2.24 ng/ml