

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS011719\
 Data File : PS002821.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Jan 2019 15:33
 Operator : EI\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 18 03:07:21 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS011719.M
 Quant Title : 8080.M
 QLast Update : Thu Jan 17 13:42:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.296	10.787	186.0E6	172.5E6	515.802	427.606
Target Compounds							
3) T	4-Nitroph...	10.927	0.000	640572	0	3.034	N.D. #
7) T	MCPA	0.000	11.675	0	6383913	N.D.	3.653 #
10) T	Pentachlo...	13.522	13.199	1187683	901985	0.216	0.162
11) T	2,4,5-TP ...	14.405	0.000	458327	0	0.220	N.D. #
12) T	2,4,5-T	0.000	14.411	0	5461389	N.D.	3.233 #
15) T	Picloram	16.778	16.713	529787	1367662	0.197	0.467 #
16) T	DCPA	0.000	16.642	0	774506	N.D.	0.270 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS011719\
Data File : PS002821.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Jan 2019 15:33
Operator : EI\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 18 03:07:21 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS011719.M
Quant Title : 8080.M
QLast Update : Thu Jan 17 13:42:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

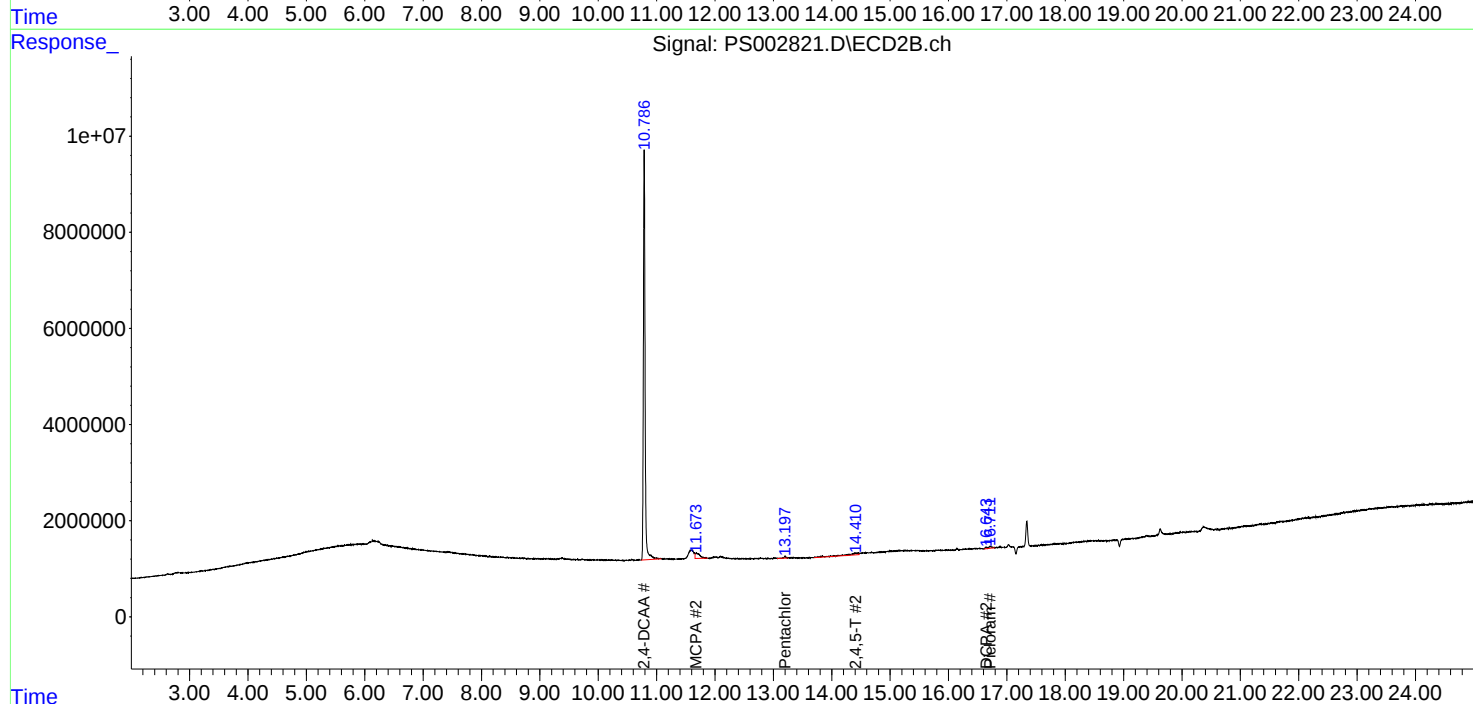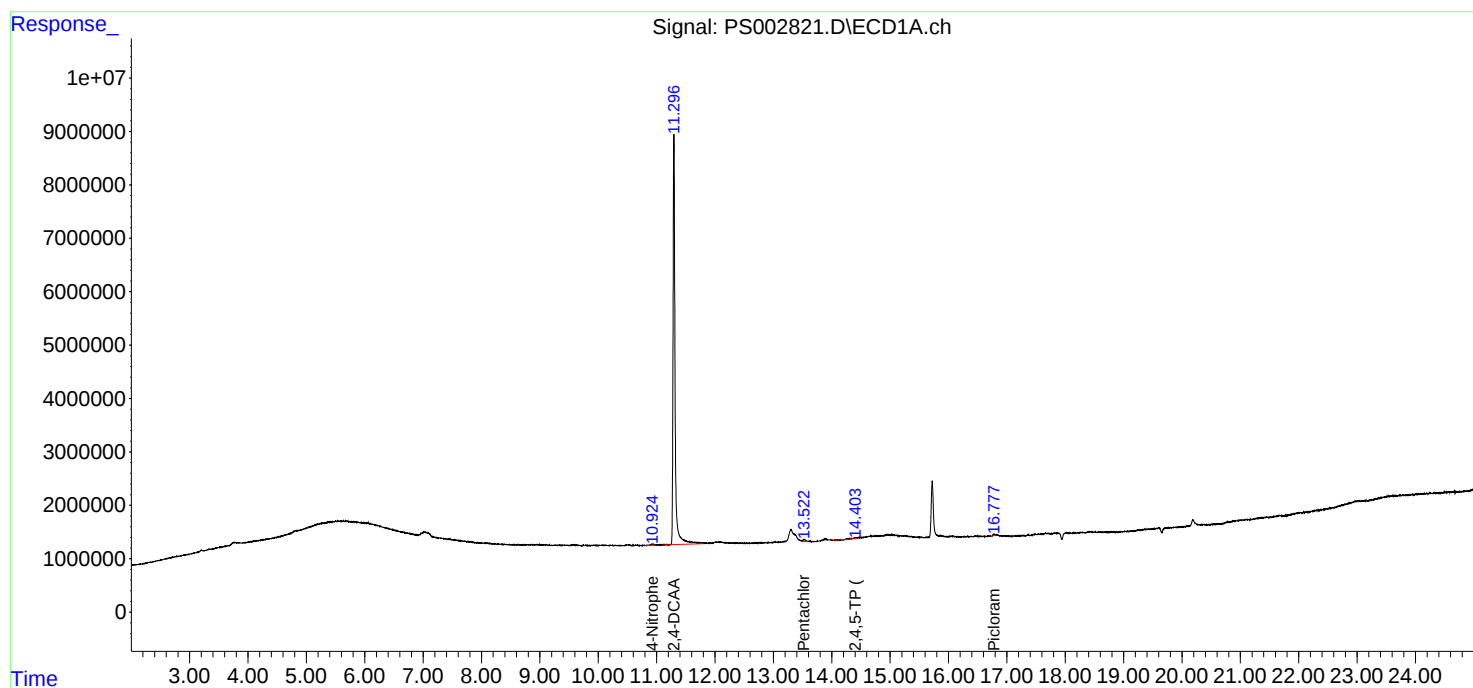


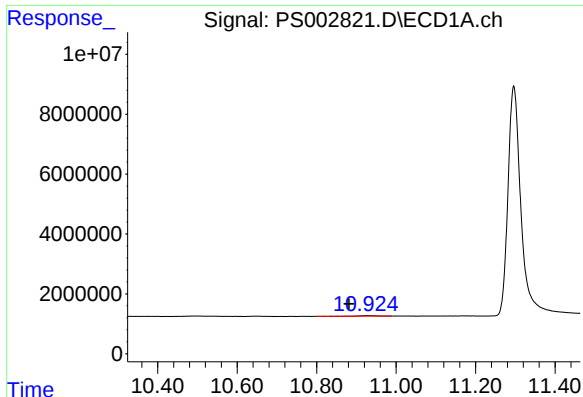

#3 4-Nitrophenol


R.T.: 10.927 min
Delta R.T.: 0.045 min
Response: 640572
Conc: 3.03 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

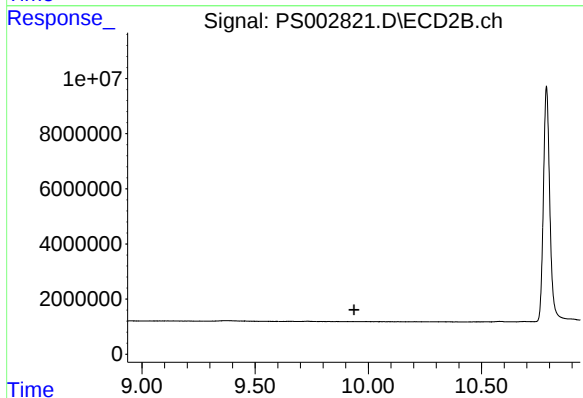


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 9.937 min
Response: 0
Conc: N.D.

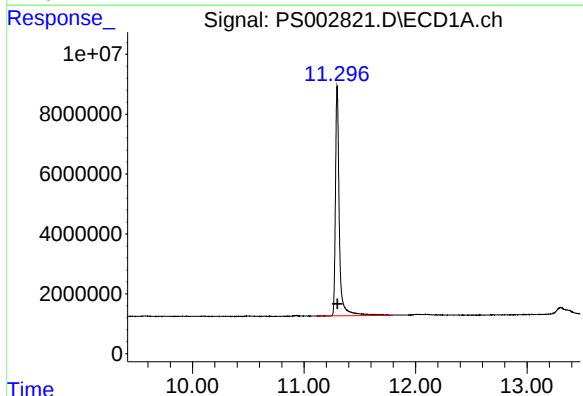


#4 2,4-DCAA

R.T.: 11.296 min
Delta R.T.: -0.003 min
Response: 186042352
Conc: 515.80 ng/ml

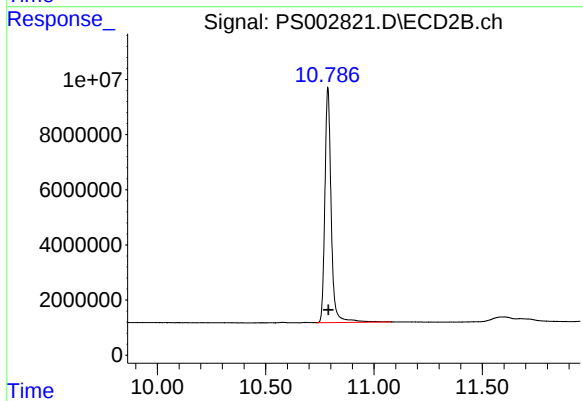

#4 2,4-DCAA


R.T.: 10.787 min
Delta R.T.: -0.003 min
Response: 172461500
Conc: 427.61 ng/ml

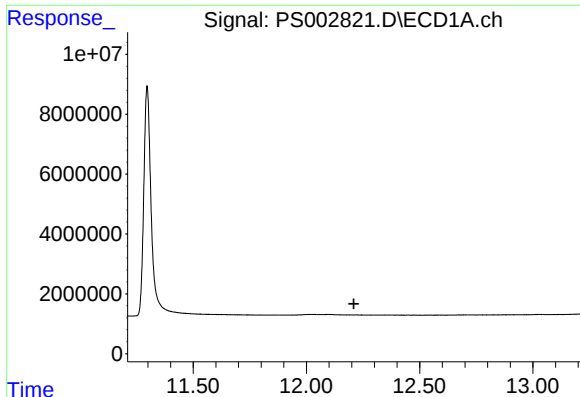

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 12.210 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

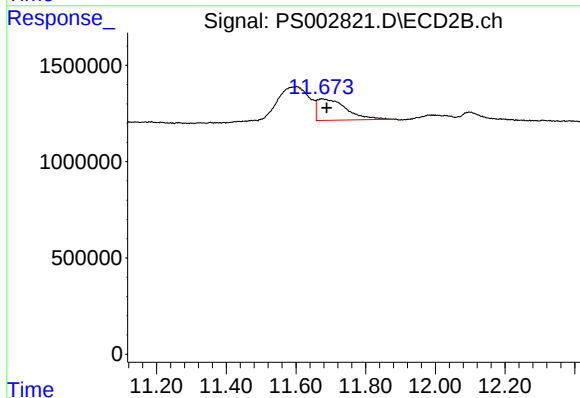


#7 MCPA

R.T.: 11.675 min
Delta R.T.: -0.014 min
Response: 6383913
Conc: 3.65 ug/ml

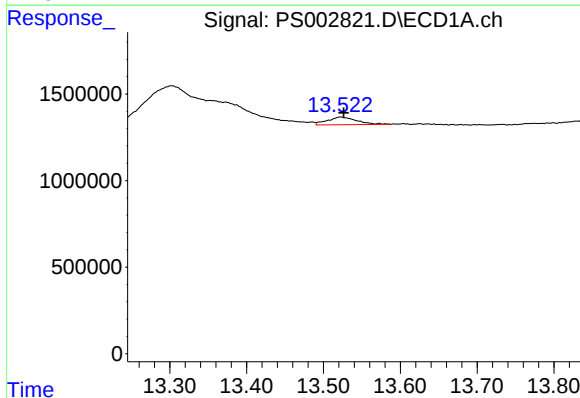


#10 Pentachlorophenol

R.T.: 13.522 min
Delta R.T.: -0.004 min
Response: 1187683
Conc: 0.22 ng/ml

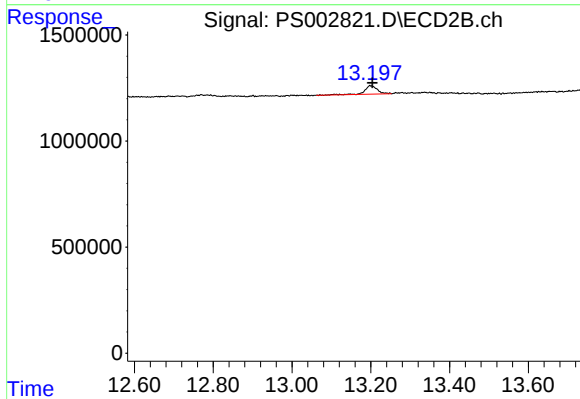

#10 Pentachlorophenol


R.T.: 13.199 min
Delta R.T.: -0.005 min
Response: 901985
Conc: 0.16 ng/ml

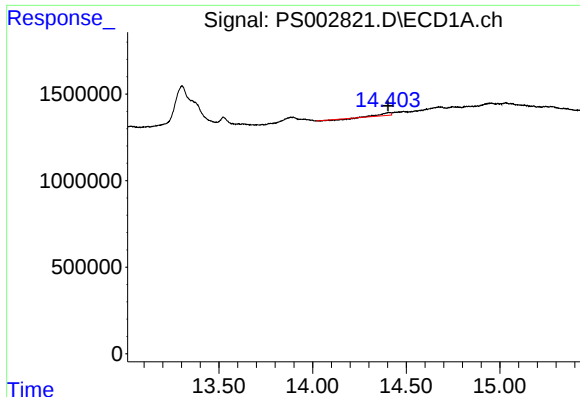

#11 2,4,5-TP (SILVEX)


R.T.: 14.405 min
Delta R.T.: 0.002 min
Response: 458327
Conc: 0.22 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

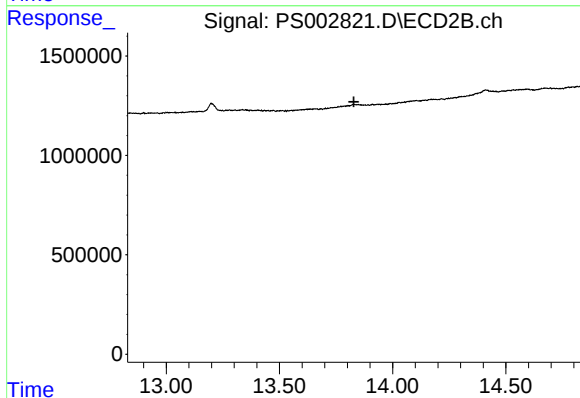


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 13.829 min
Response: 0
Conc: N.D.

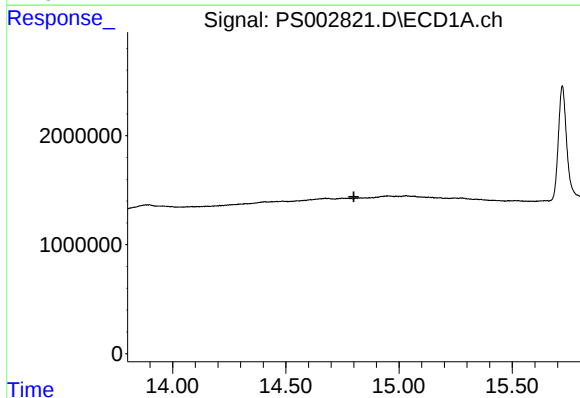


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 14.800 min
Response: 0
Conc: N.D.

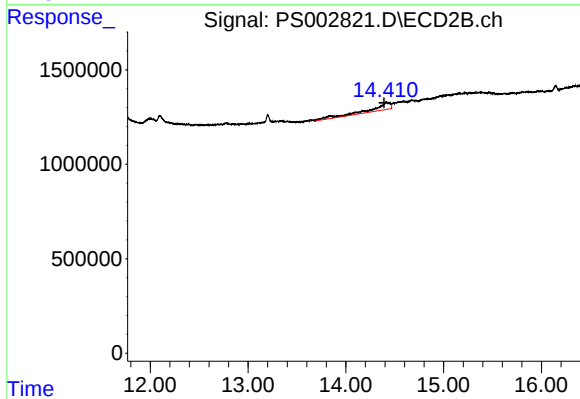

#12 2,4,5-T


R.T.: 14.411 min
Delta R.T.: 0.020 min
Response: 5461389
Conc: 3.23 ng/ml

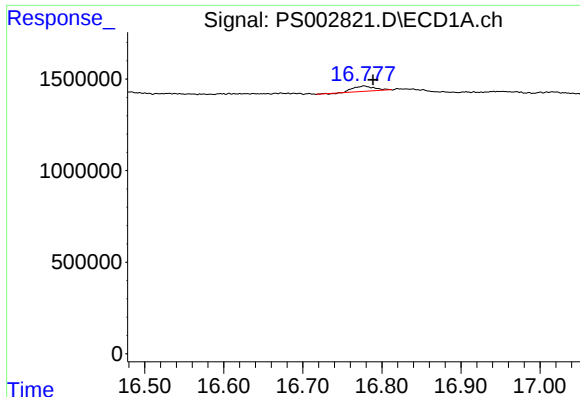

#15 Picloram


R.T.: 16.778 min
Delta R.T.: -0.011 min
Response: 529787
Conc: 0.20 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

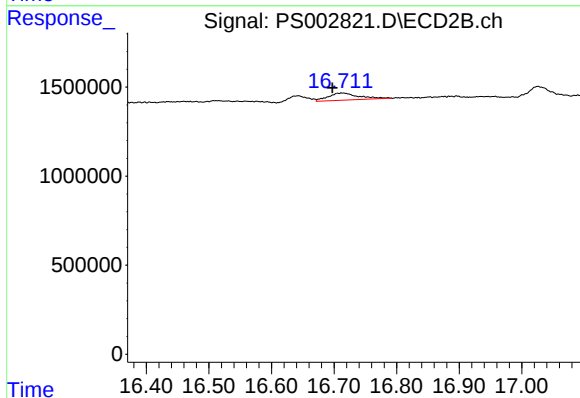


#15 Picloram

R.T.: 16.713 min
Delta R.T.: 0.016 min
Response: 1367662
Conc: 0.47 ng/ml

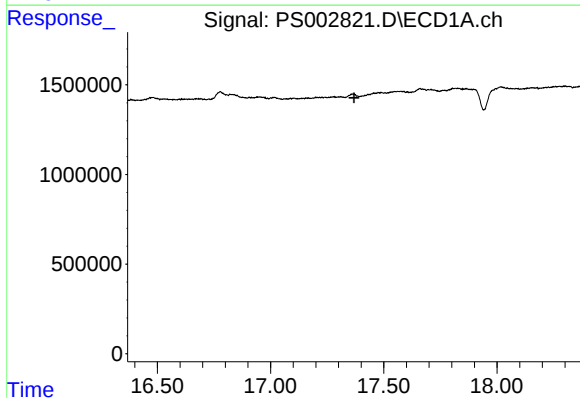

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.368 min
Response: 0
Conc: N.D.

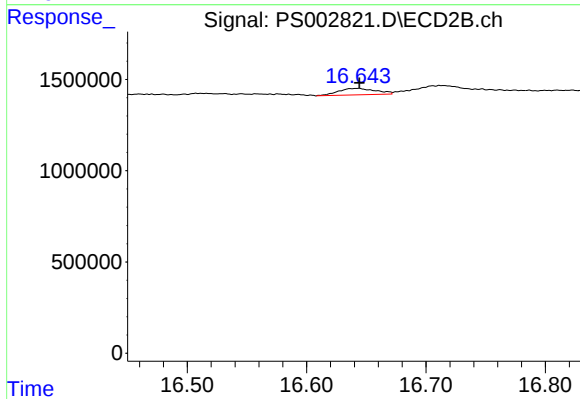

#16 DCPA

R.T.: 16.642 min
Delta R.T.: -0.002 min
Response: 774506
Conc: 0.27 ng/ml