

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS011719\
 Data File : PS002841.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Jan 2019 01:56
 Operator : EI\SJ
 Sample : K1159-01
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 SSSI-0115-S-TCLP-7

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 18 04:15:24 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS011719.M
 Quant Title : 8080.M
 QLast Update : Thu Jan 17 13:42:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.349	10.842	189.8E6	177.7E6	526.287	440.514
Target Compounds							
1) T	Dalapon	2.858	2.337	101.3E6	328.9E6	204.417	654.144 #
5) T	DICAMBA	0.000	11.083	0	7244609	N.D.	4.976 #
6) T	MCPD	11.932	0.000	931863	0	0.901	N.D. #
7) T	MCPA	12.203	11.620	28696125	18702950	17.094	10.701 #
8) T	DICHLORPROP	12.736	12.246	9622917	16782998	25.141	44.654 #
10) T	Pentachlo...	13.596	0.000	6826609	0	1.243	N.D. #
11) T	2,4,5-TP ...	0.000	13.790	0	19435802	N.D.	8.967 #
12) T	2,4,5-T	0.000	14.405	0	12855387	N.D.	7.611 #
13) T	2,4-DB	15.560	15.079	2803850	5146533	10.873	18.790 #
14) T	DINOSEB	17.013	15.501	25696129	15187096	15.409	9.195 #
15) T	Picloram	16.800	0.000	6361867	0	2.361	N.D. #
16) T	DCPA	0.000	16.576	0	16047691	N.D.	5.588 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS011719\
Data File : PS002841.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Jan 2019 01:56
Operator : EI\SJ
Sample : K1159-01
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
SSSI-0115-S-TCLP-7

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 18 04:15:24 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS011719.M
Quant Title : 8080.M
QLast Update : Thu Jan 17 13:42:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

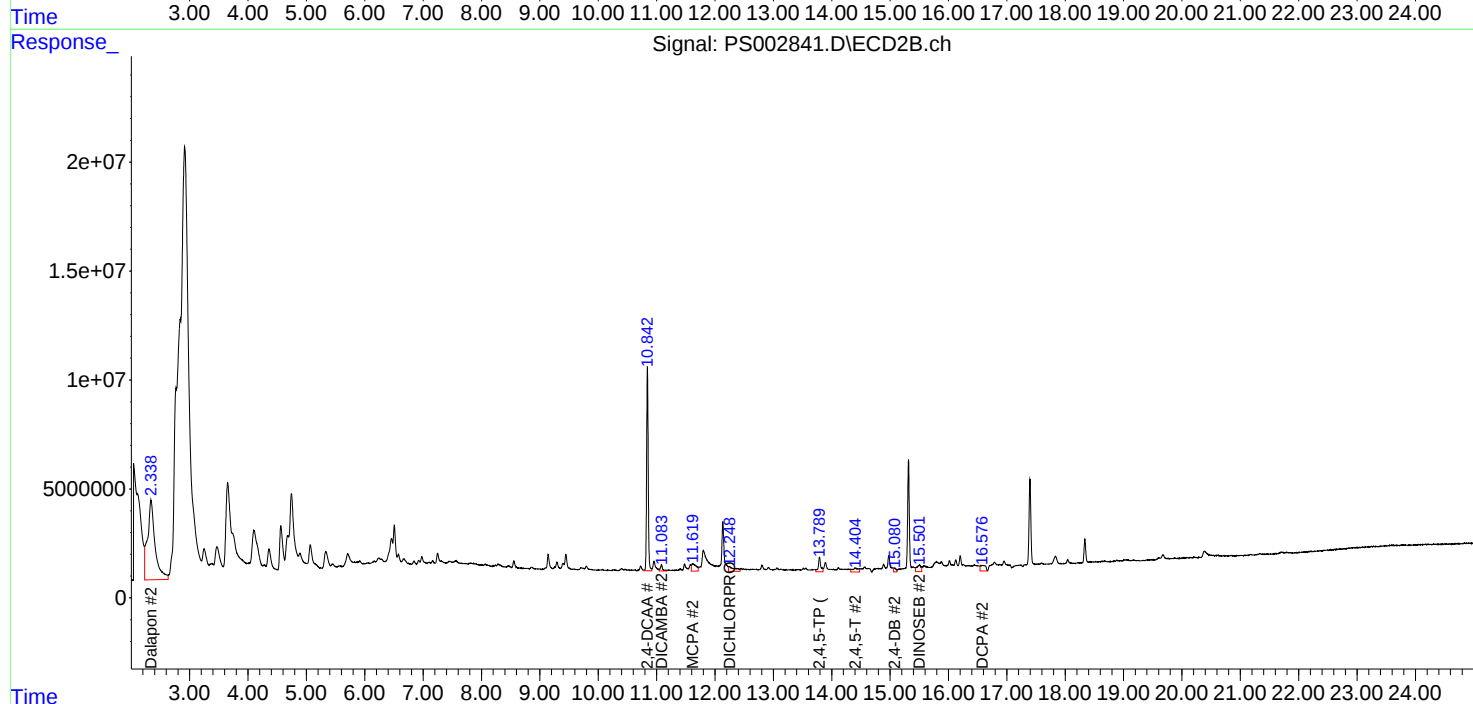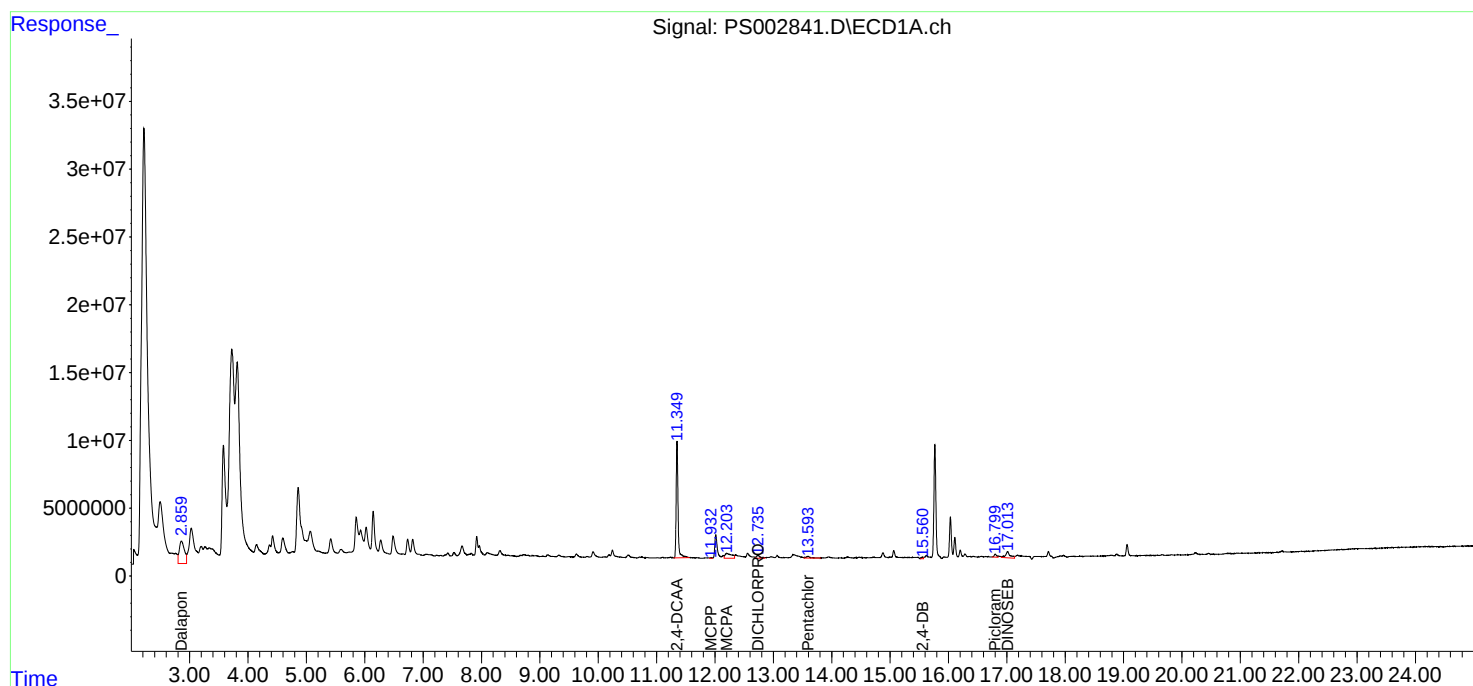


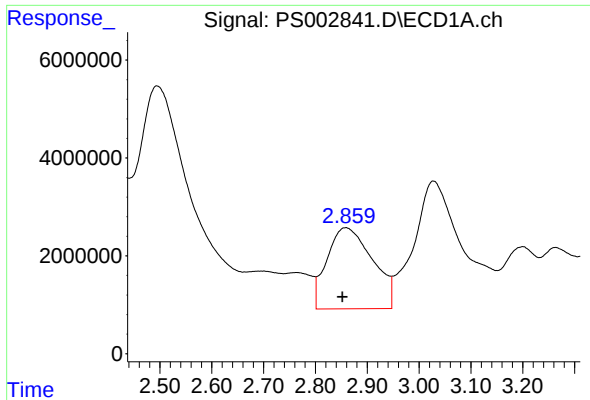

#1 Dalapon


R.T.: 2.858 min
Delta R.T.: 0.006 min
Response: 101349571
Conc: 204.42 ng/ml

Instrument :
ECD_S
ClientSampleId :
SSSI-0115-S-TCLP-7

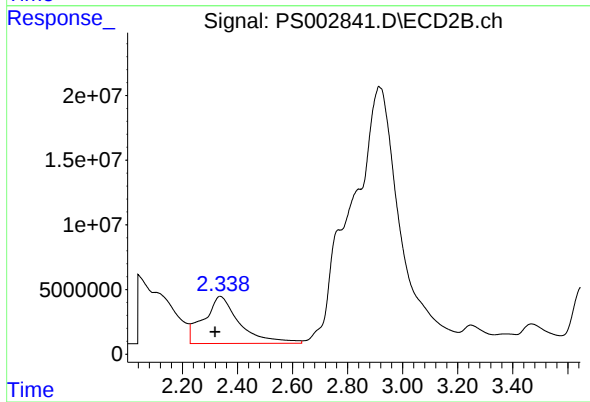


#1 Dalapon

R.T.: 2.337 min
Delta R.T.: 0.018 min
Response: 328944709
Conc: 654.14 ng/ml

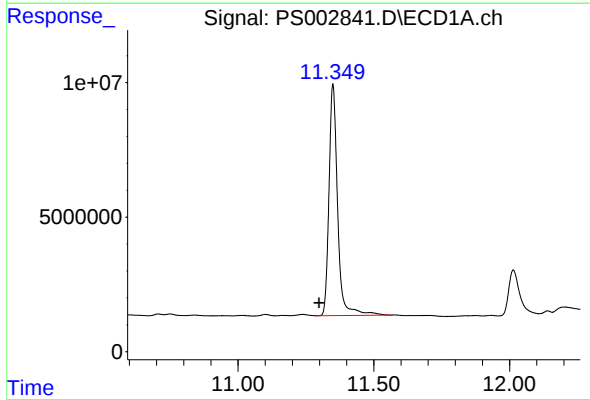


#4 2,4-DCAA

R.T.: 11.349 min
Delta R.T.: 0.050 min
Response: 189824152
Conc: 526.29 ng/ml

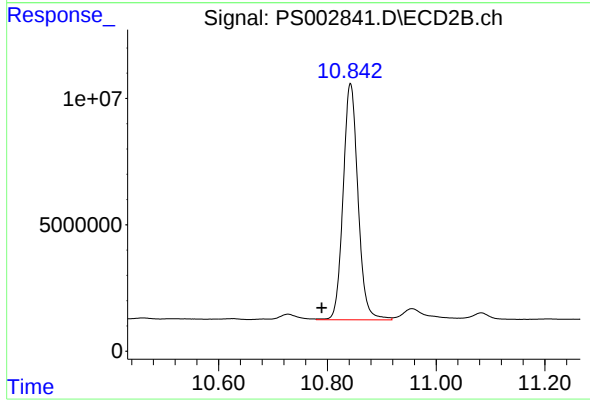

#4 2,4-DCAA


R.T.: 10.842 min
Delta R.T.: 0.053 min
Response: 177667762
Conc: 440.51 ng/ml

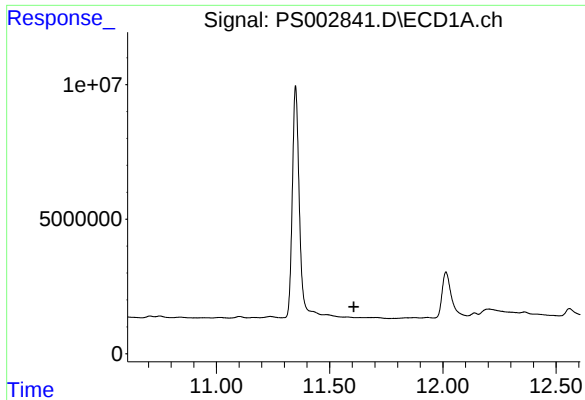

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 11.607 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
SSSI-0115-S-TCLP-7

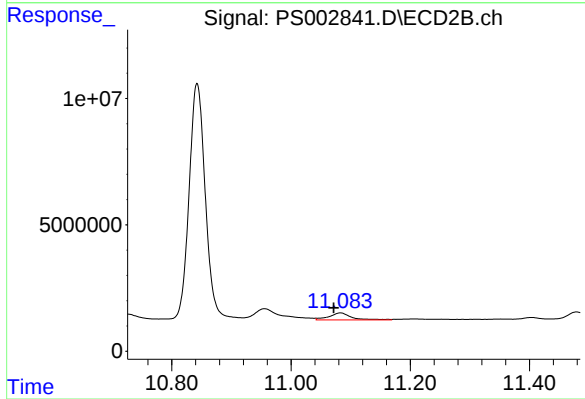


#5 DICAMBA

R.T.: 11.083 min
Delta R.T.: 0.011 min
Response: 7244609
Conc: 4.98 ng/ml

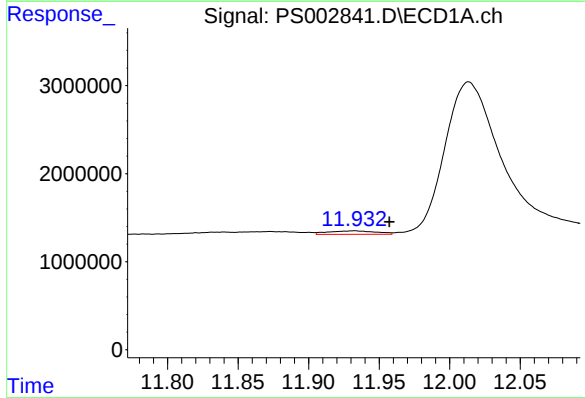


#6 MCP

R.T.: 11.932 min
Delta R.T.: -0.025 min
Response: 931863
Conc: 0.90 ug/ml

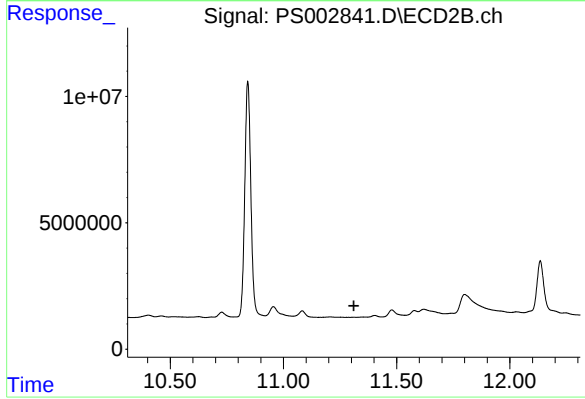

#6 MCP


R.T.: 0.000 min
Exp R.T.: 11.312 min
Response: 0
Conc: N.D.

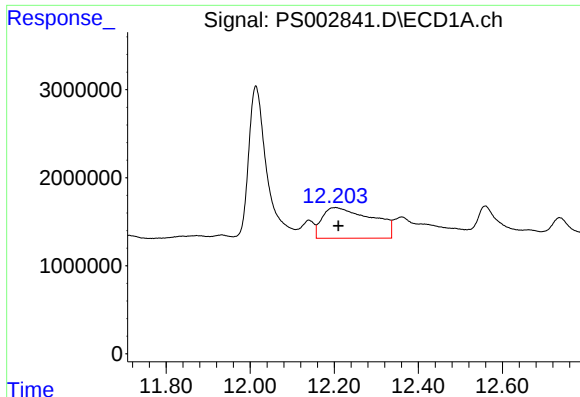

#7 MCPA


R.T.: 12.203 min
Delta R.T.: -0.007 min
Response: 28696125
Conc: 17.09 ug/ml

Instrument :
ECD_S
ClientSampleId :
SSSI-0115-S-TCLP-7

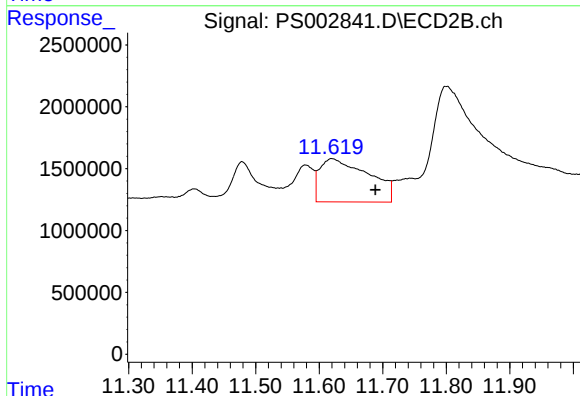


#7 MCPA

R.T.: 11.620 min
Delta R.T.: -0.068 min
Response: 18702950
Conc: 10.70 ug/ml

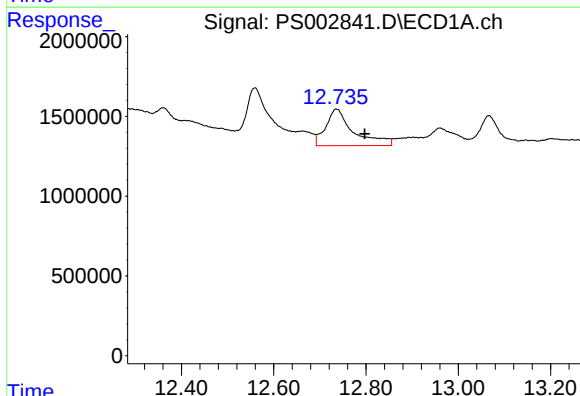


#8 DICHLORPROP

R.T.: 12.736 min
Delta R.T.: -0.061 min
Response: 9622917
Conc: 25.14 ng/ml

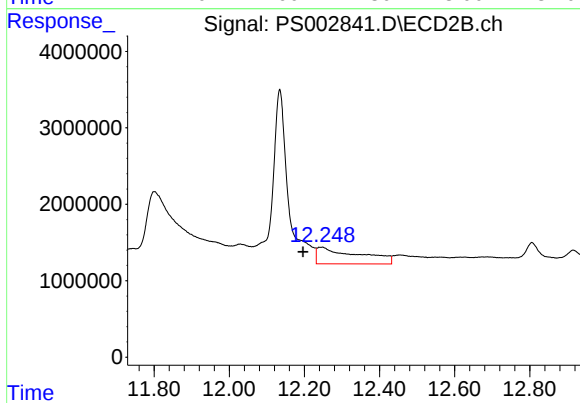

#8 DICHLORPROP


R.T.: 12.246 min
Delta R.T.: 0.049 min
Response: 16782998
Conc: 44.65 ng/ml

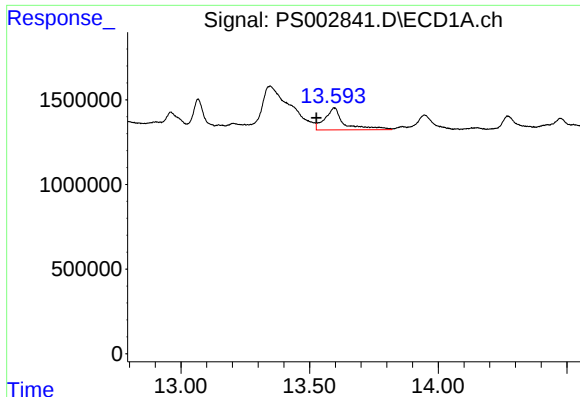

#10 Pentachlorophenol


R.T.: 13.596 min
Delta R.T.: 0.069 min
Response: 6826609
Conc: 1.24 ng/ml

Instrument :
ECD_S
ClientSampleId :
SSSI-0115-S-TCLP-7

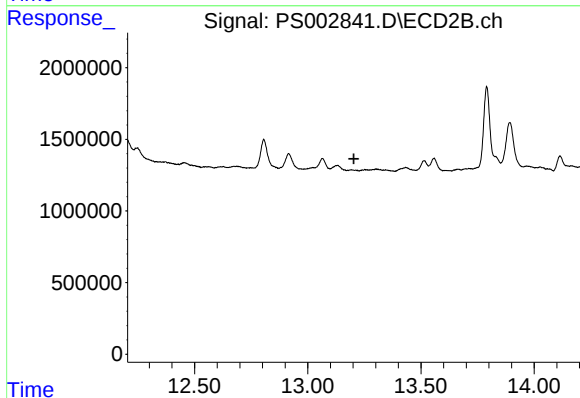


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T. : 13.204 min
Response: 0
Conc: N.D.

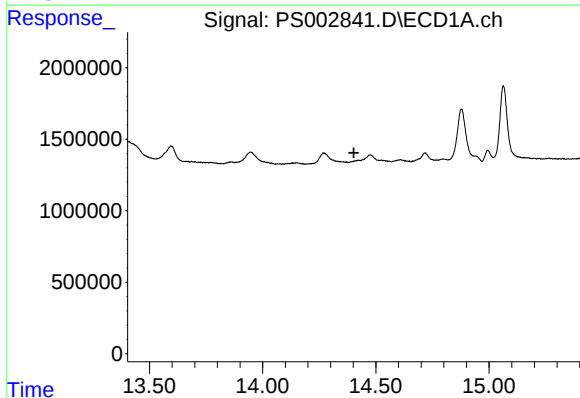


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 14.403 min
Response: 0
Conc: N.D.

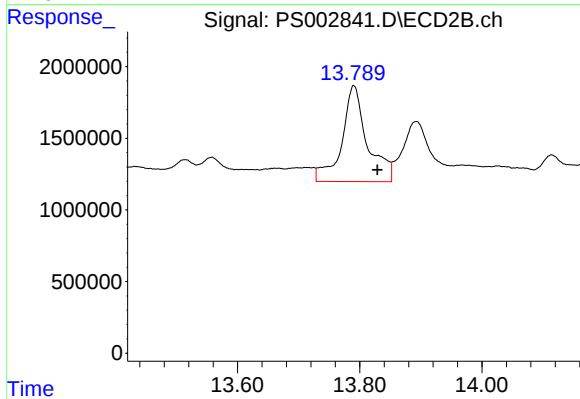

#11 2,4,5-TP (SILVEX)


R.T.: 13.790 min
Delta R.T.: -0.039 min
Response: 19435802
Conc: 8.97 ng/ml

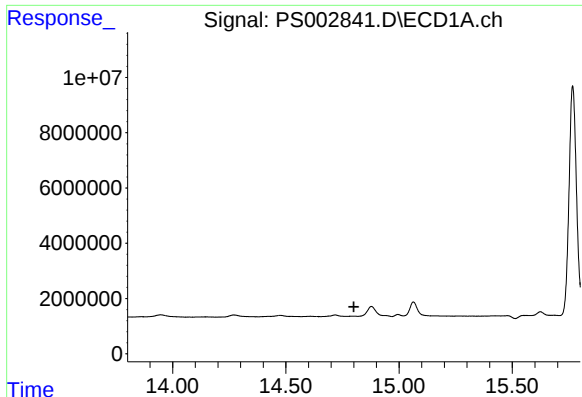

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 14.800 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
SSSI-0115-S-TCLP-7

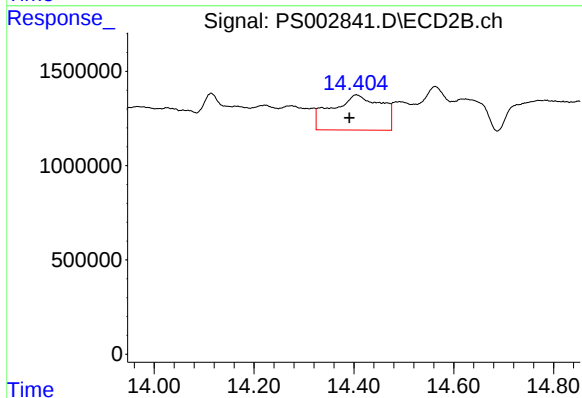


#12 2,4,5-T

R.T.: 14.405 min
Delta R.T.: 0.014 min
Response: 12855387
Conc: 7.61 ng/ml

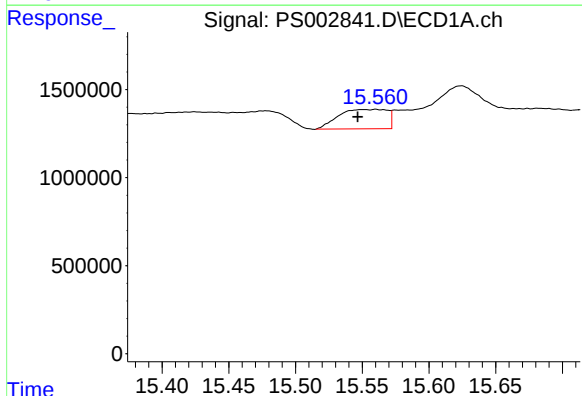


#13 2,4-DB

R.T.: 15.560 min
Delta R.T.: 0.014 min
Response: 2803850
Conc: 10.87 ng/ml

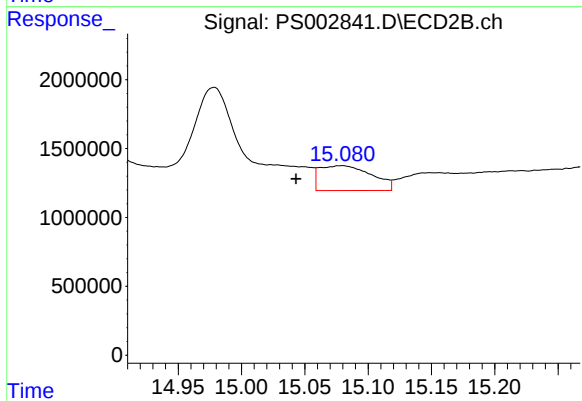

#13 2,4-DB


R.T.: 15.079 min
Delta R.T.: 0.036 min
Response: 5146533
Conc: 18.79 ng/ml

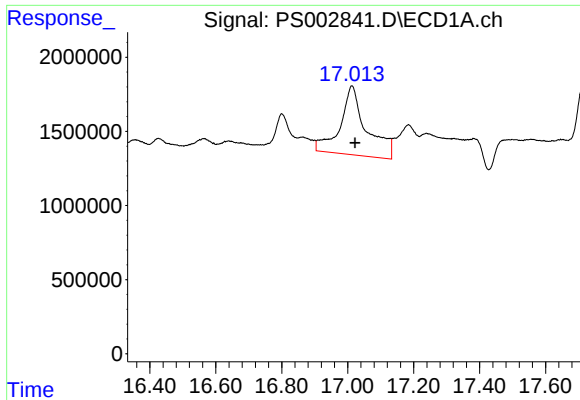

#14 DINOSEB


R.T.: 17.013 min
Delta R.T.: -0.010 min
Response: 25696129
Conc: 15.41 ng/ml

Instrument :
ECD_S
ClientSampleId :
SSSI-0115-S-TCLP-7

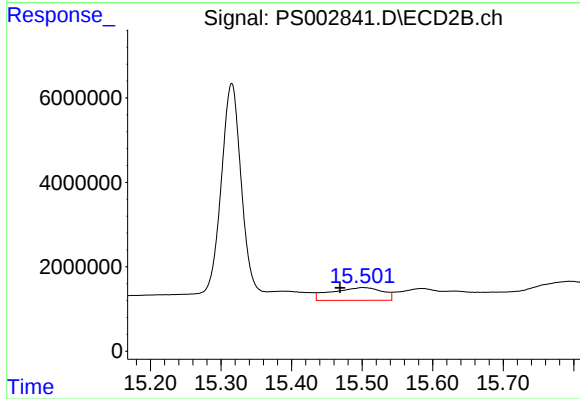


#14 DINOSEB

R.T.: 15.501 min
Delta R.T.: 0.032 min
Response: 15187096
Conc: 9.19 ng/ml

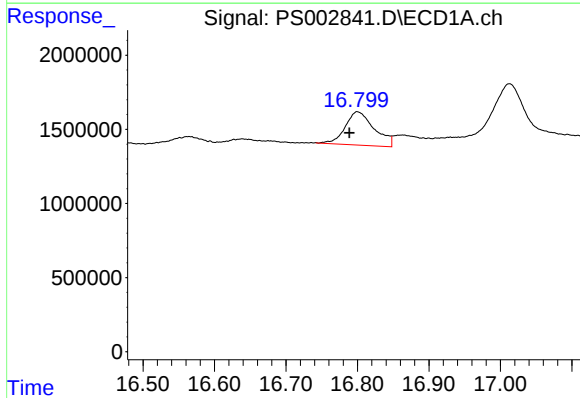


#15 Picloram

R.T.: 16.800 min
Delta R.T.: 0.011 min
Response: 6361867
Conc: 2.36 ng/ml

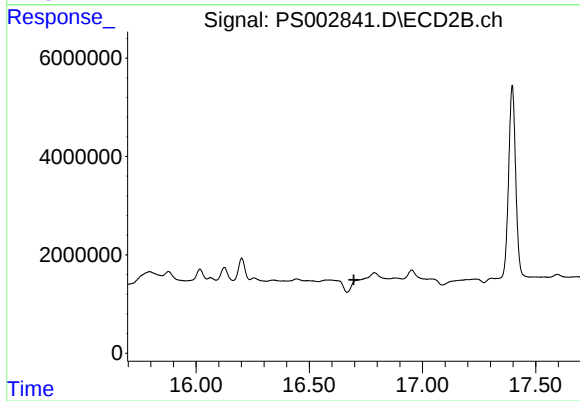

#15 Picloram


R.T.: 0.000 min
Exp R.T. : 16.697 min
Response: 0
Conc: N.D.

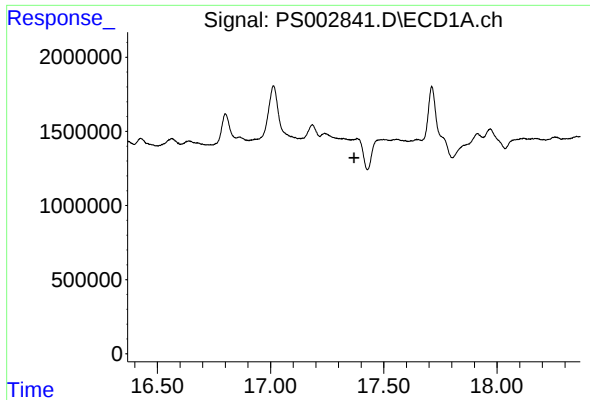

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.368 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
SSSI-0115-S-TCLP-7

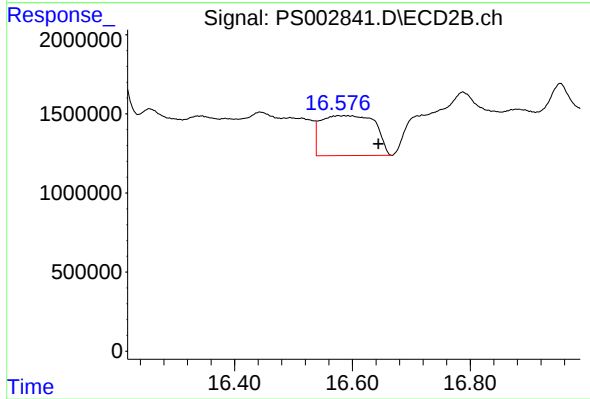

#16 DCPA

R.T.: 16.576 min
Delta R.T.: -0.068 min
Response: 16047691
Conc: 5.59 ng/ml