

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS011719\
 Data File : PS002813.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Jan 2019 11:16
 Operator : EI\SJ
 Sample : HSTDICC750
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HSTDICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 17 13:35:24 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS011719.M
 Quant Title : 8080.M
 QLast Update : Thu Jan 17 13:34:15 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.326	10.816	263.7E6	294.7E6	750.000	750.000
Target Compounds							
1) T	Dalapon	2.877	2.343	320.7E6	333.8E6	682.500	682.500
2) T	3,5-DICHL...	9.753	8.975	364.4E6	342.2E6	697.500	697.500
3) T	4-Nitroph...	10.911	9.964	142.1E6	128.0E6	682.500	682.500
5) T	DICAMBA	11.633	11.097	1046.8E6	1013.3E6	705.000	705.000
6) T	MCPD	11.977	11.329	72353091	66377497	70.500	70.500
7) T	MCPA	12.227	11.705	112.9E6	113.2E6	69.750	69.750
8) T	DICHLORPROP	12.824	12.222	257.0E6	256.4E6	705.000	705.000
9) T	2,4-D	13.182	12.694	276.0E6	305.7E6	705.000	705.000
10) T	Pentachlo...	13.553	13.230	3879.7E6	3942.1E6	712.500	712.500
11) T	2,4,5-TP ...	14.429	13.854	1466.9E6	1529.2E6	712.500	712.500
12) T	2,4,5-T	14.827	14.417	1510.2E6	1204.0E6	712.500	712.500
13) T	2,4-DB	15.574	15.069	181.7E6	193.2E6	712.500	712.500
14) T	DINOSEB	17.047	15.494	1158.8E6	1145.0E6	705.000	705.000
15) T	Picloram	16.816	16.723	1927.0E6	2105.3E6	712.500	712.500
16) T	DCPA	17.393	16.669	1914.0E6	2050.0E6	720.000	720.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS011719\
Data File : PS002813.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Jan 2019 11:16
Operator : EI\SJ
Sample : HSTDICC750
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 17 13:35:24 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS011719.M
Quant Title : 8080.M
QLast Update : Thu Jan 17 13:34:15 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

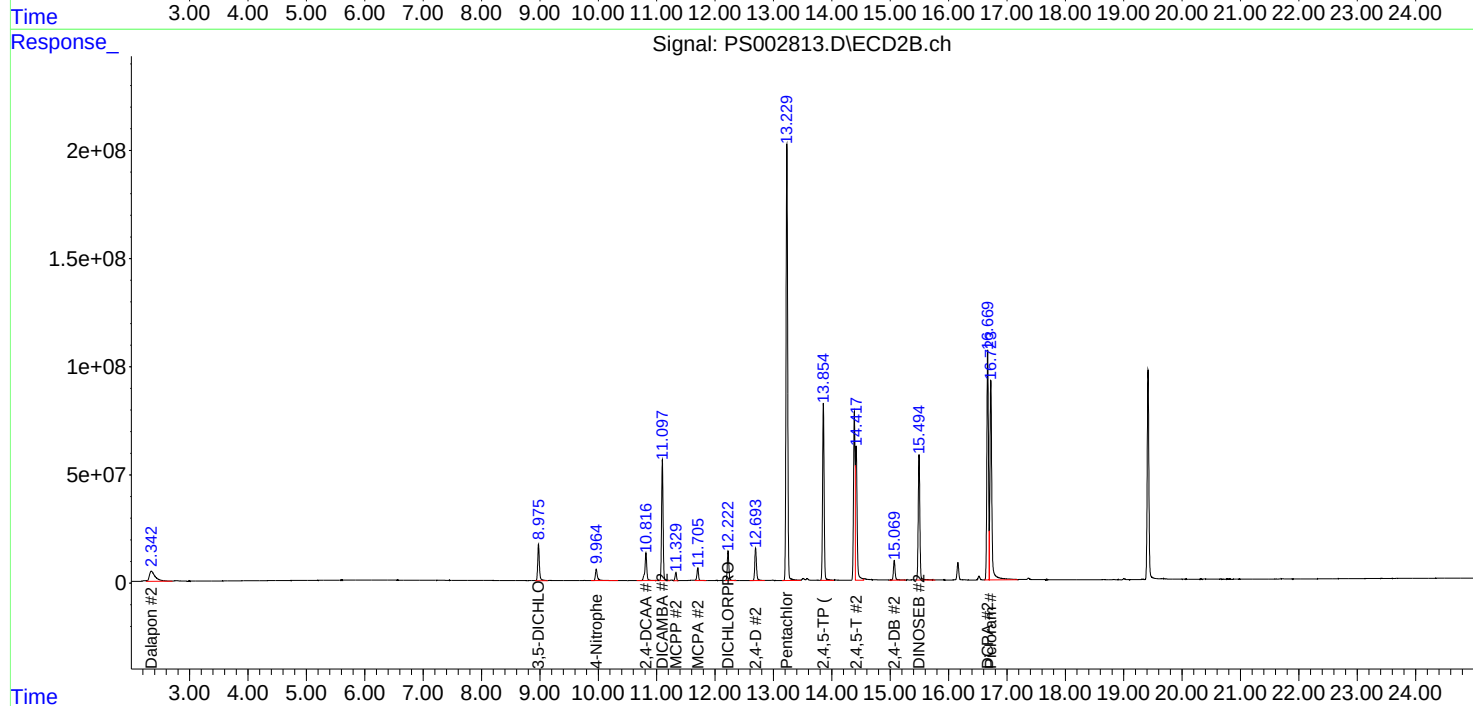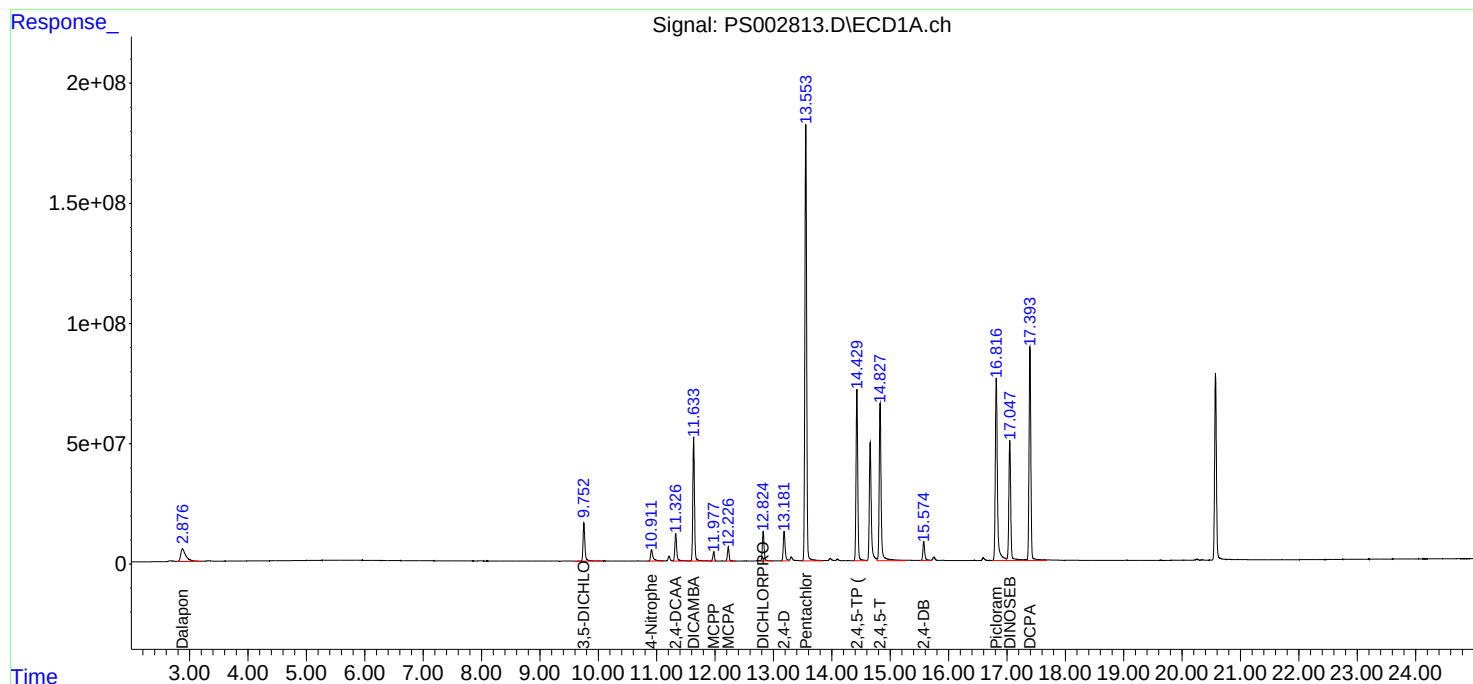


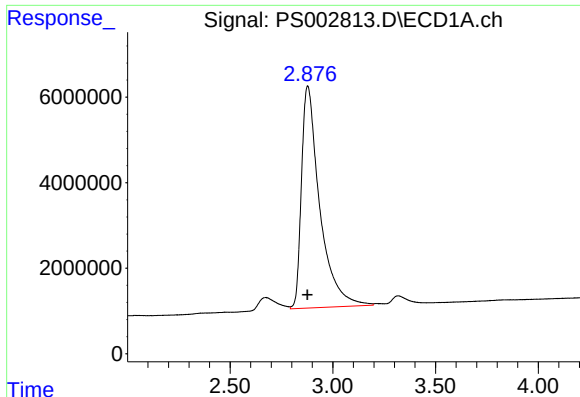

#1 Dalapon


R.T.: 2.877 min
Delta R.T.: 0.000 min
Response: 320719686
Conc: 682.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

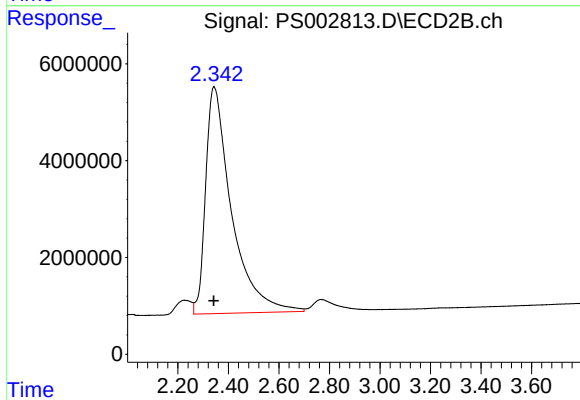


#1 Dalapon

R.T.: 2.343 min
Delta R.T.: 0.000 min
Response: 333786390
Conc: 682.50 ng/ml

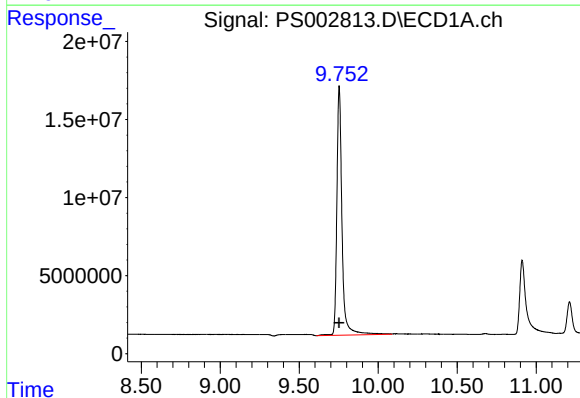


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 9.753 min
Delta R.T.: 0.000 min
Response: 364392417
Conc: 697.50 ng/ml

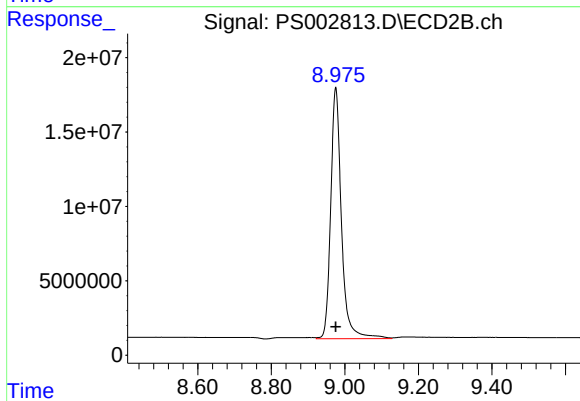

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 8.975 min
Delta R.T.: 0.000 min
Response: 342158651
Conc: 697.50 ng/ml

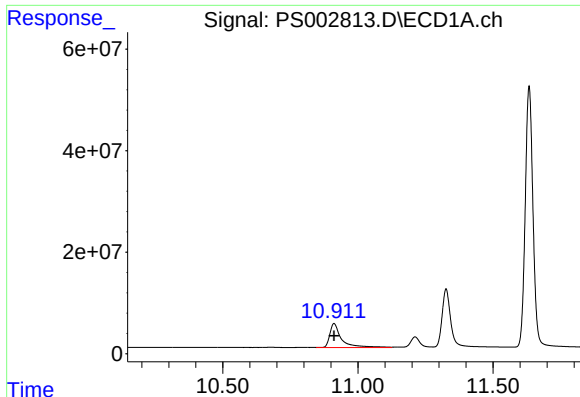

#3 4-Nitrophenol


R.T.: 10.911 min
Delta R.T.: 0.000 min
Response: 142118964
Conc: 682.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

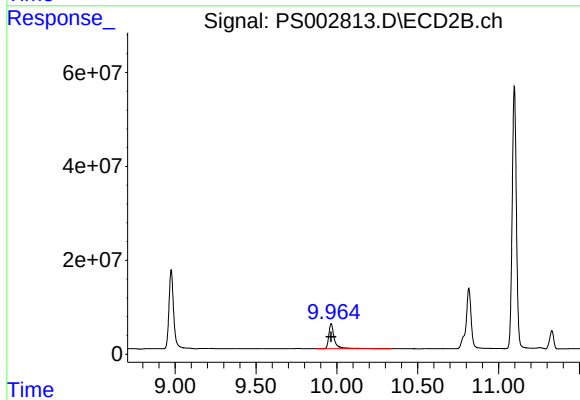


#3 4-Nitrophenol

R.T.: 9.964 min
Delta R.T.: 0.000 min
Response: 128034155
Conc: 682.50 ng/ml

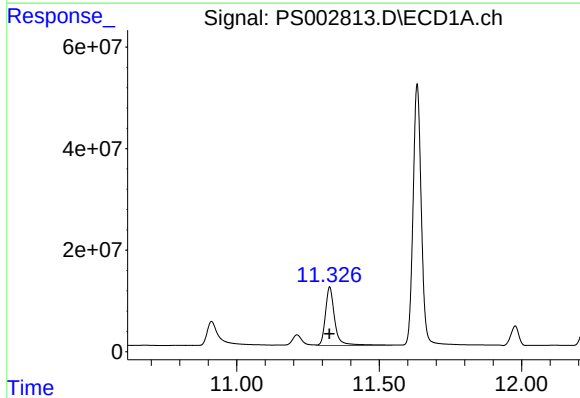


#4 2,4-DCAA

R.T.: 11.326 min
Delta R.T.: 0.000 min
Response: 263698200
Conc: 750.00 ng/ml

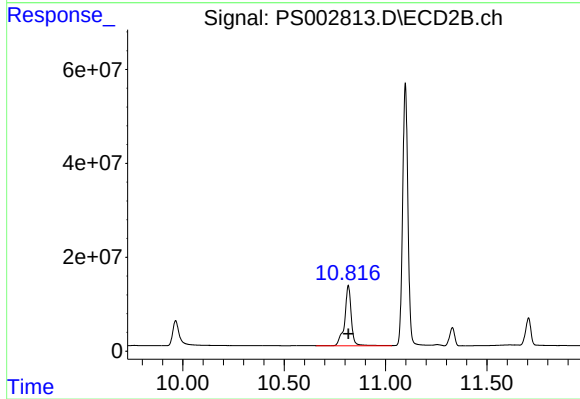

#4 2,4-DCAA


R.T.: 10.816 min
Delta R.T.: 0.000 min
Response: 294724034
Conc: 750.00 ng/ml

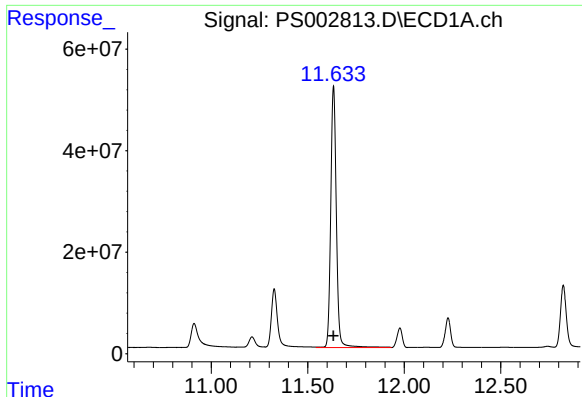

#5 DICAMBA


R.T.: 11.633 min
Delta R.T.: 0.000 min
Response: 1046780833
Conc: 705.00 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

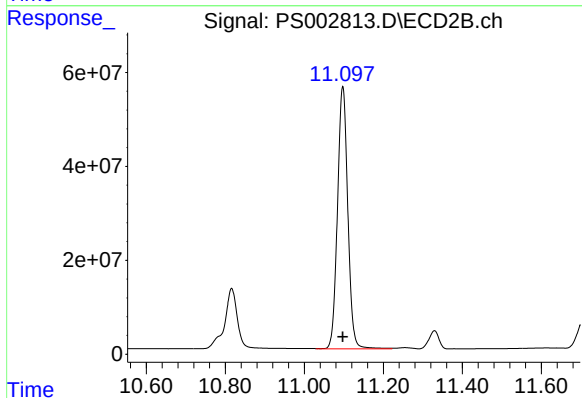


#5 DICAMBA

R.T.: 11.097 min
Delta R.T.: 0.000 min
Response: 1013297105
Conc: 705.00 ng/ml

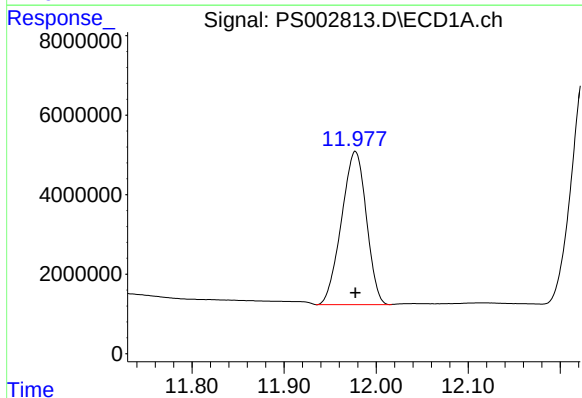


#6 MCP

R.T.: 11.977 min
Delta R.T.: 0.000 min
Response: 72353091
Conc: 70.50 ug/ml

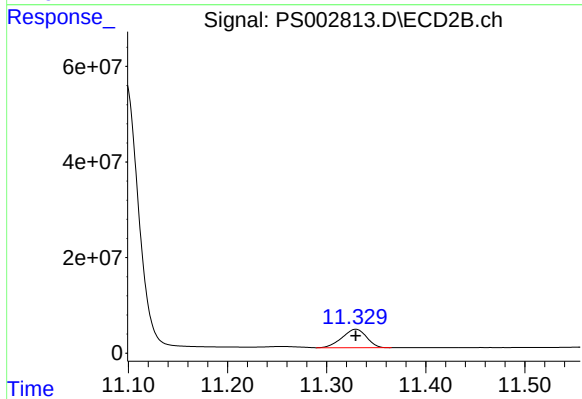

#6 MCP


R.T.: 11.329 min
Delta R.T.: 0.000 min
Response: 66377497
Conc: 70.50 ug/ml

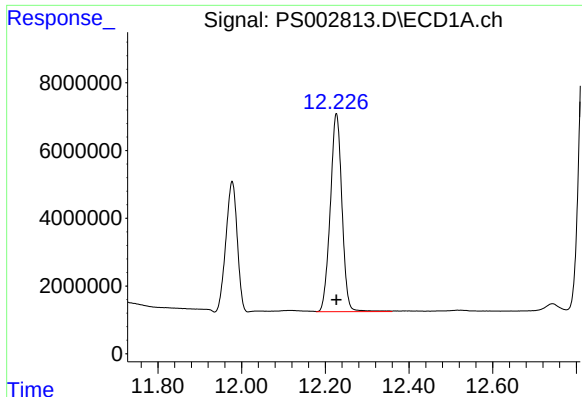

#7 MCPA


R.T.: 12.227 min
Delta R.T.: 0.000 min
Response: 112915702
Conc: 69.75 ug/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

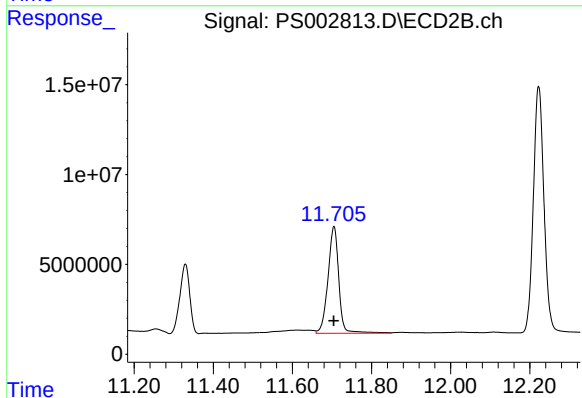


#7 MCPA

R.T.: 11.705 min
Delta R.T.: 0.000 min
Response: 113167425
Conc: 69.75 ug/ml

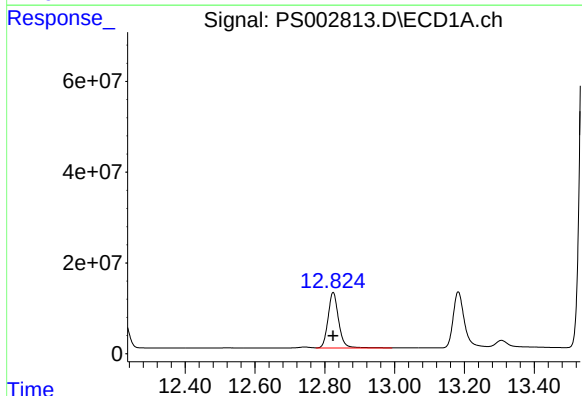


#8 DICHLORPROP

R.T.: 12.824 min
Delta R.T.: 0.000 min
Response: 257024220
Conc: 705.00 ng/ml

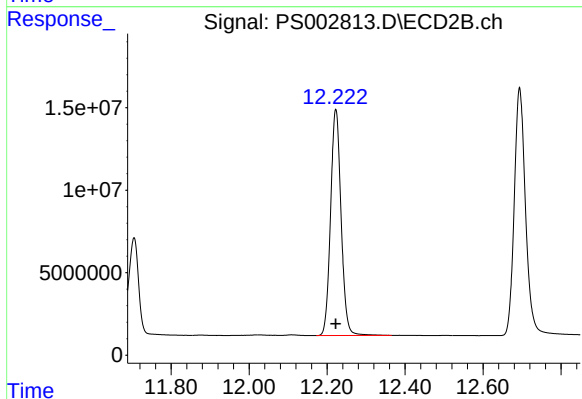

#8 DICHLORPROP


R.T.: 12.222 min
Delta R.T.: 0.000 min
Response: 256356478
Conc: 705.00 ng/ml

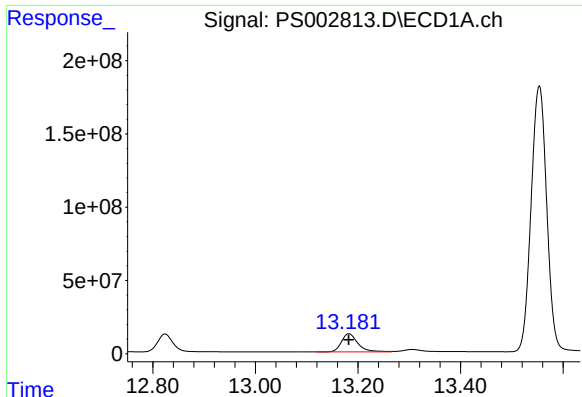

#9 2,4-D


R.T.: 13.182 min
Delta R.T.: 0.000 min
Response: 275976008
Conc: 705.00 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

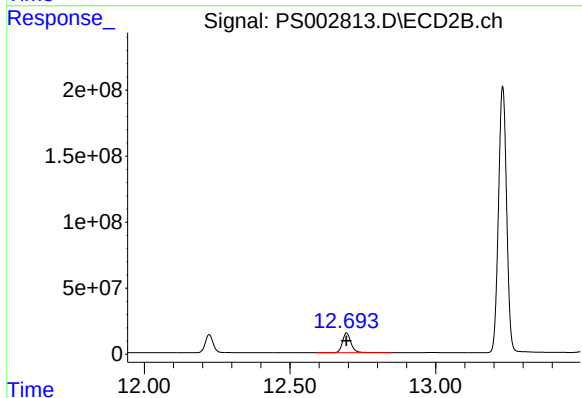


#9 2,4-D

R.T.: 12.694 min
Delta R.T.: 0.000 min
Response: 305680136
Conc: 705.00 ng/ml

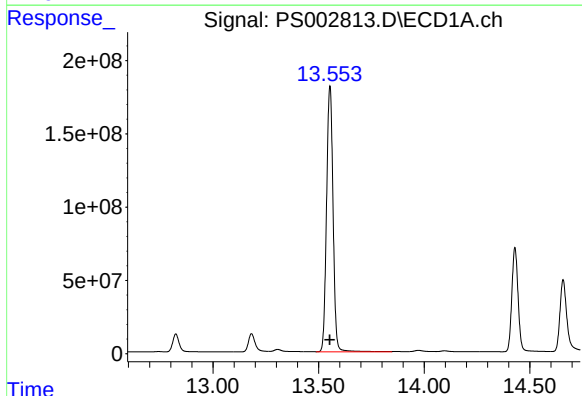


#10 Pentachlorophenol

R.T.: 13.553 min
Delta R.T.: 0.000 min
Response: 3879684468
Conc: 712.50 ng/ml

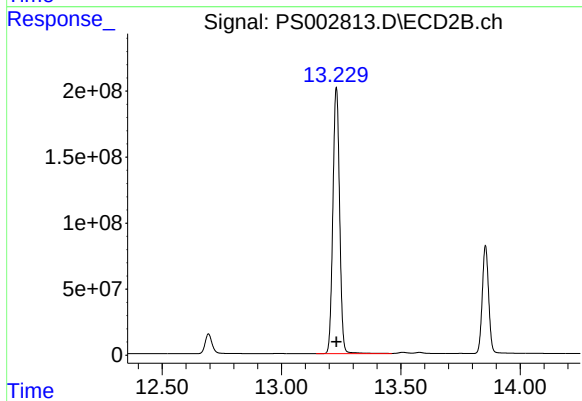

#10 Pentachlorophenol


R.T.: 13.230 min
Delta R.T.: 0.000 min
Response: 3942102538
Conc: 712.50 ng/ml

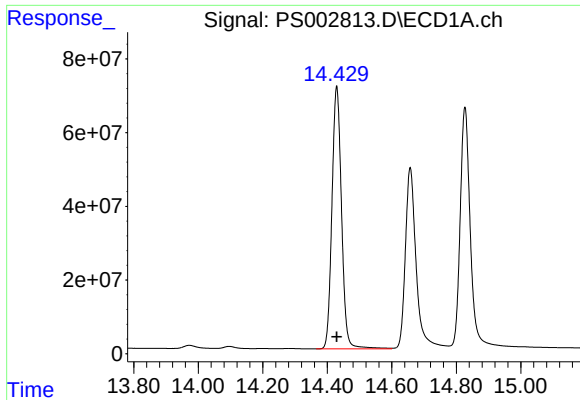

#11 2,4,5-TP (SILVEX)


R.T.: 14.429 min
Delta R.T.: 0.000 min
Response: 1466899024
Conc: 712.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

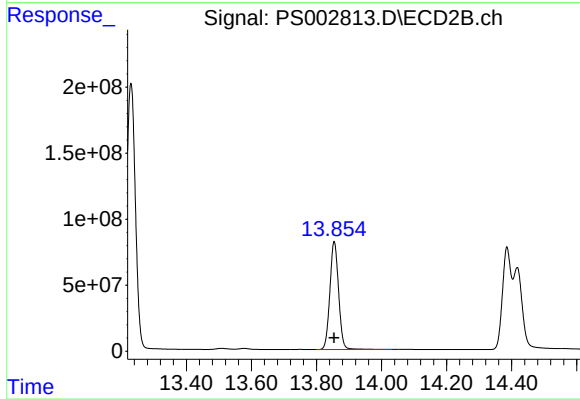


#11 2,4,5-TP (SILVEX)

R.T.: 13.854 min
Delta R.T.: 0.000 min
Response: 1529200224
Conc: 712.50 ng/ml

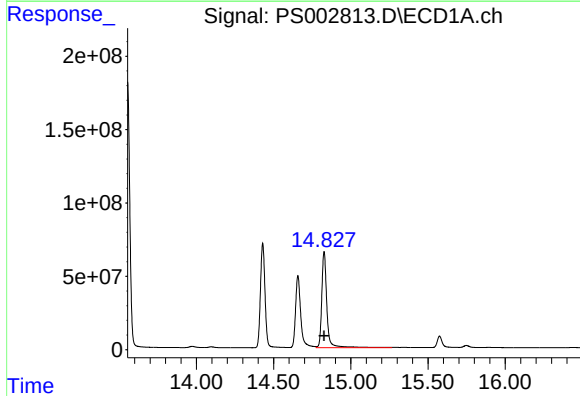


#12 2,4,5-T

R.T.: 14.827 min
Delta R.T.: 0.000 min
Response: 1510179013
Conc: 712.50 ng/ml

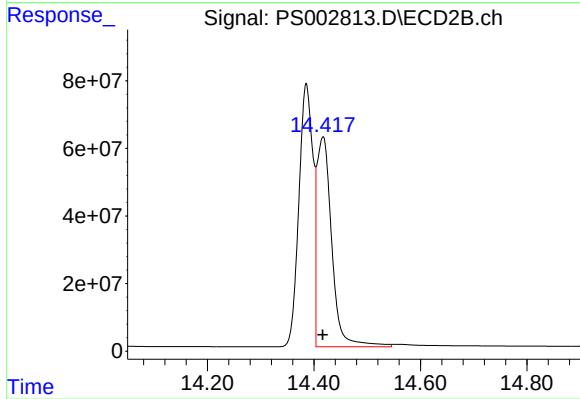

#12 2,4,5-T


R.T.: 14.417 min
Delta R.T.: 0.000 min
Response: 1204009349
Conc: 712.50 ng/ml

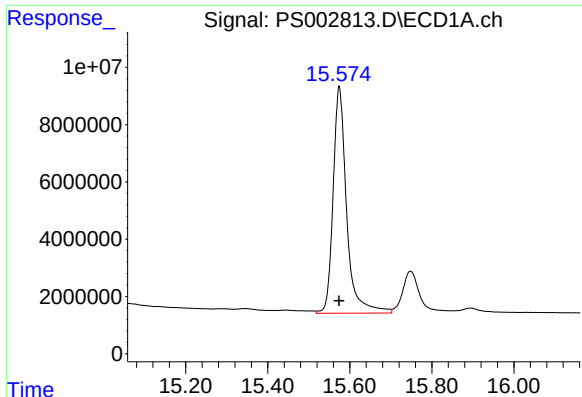

#13 2,4-DB


R.T.: 15.574 min
Delta R.T.: 0.000 min
Response: 181652723
Conc: 712.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

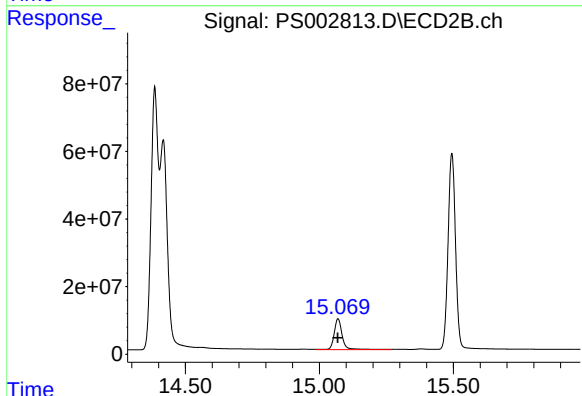


#13 2,4-DB

R.T.: 15.069 min
Delta R.T.: 0.000 min
Response: 193236908
Conc: 712.50 ng/ml

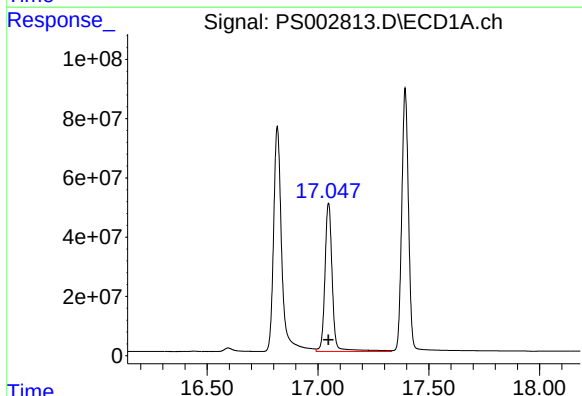


#14 DINOSEB

R.T.: 17.047 min
Delta R.T.: 0.000 min
Response: 1158779086
Conc: 705.00 ng/ml

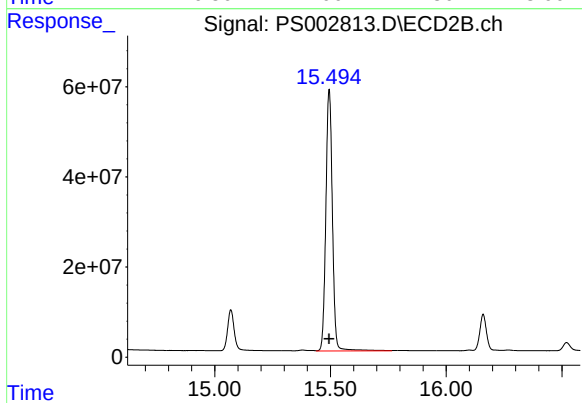

#14 DINOSEB


R.T.: 15.494 min
Delta R.T.: 0.000 min
Response: 1145041085
Conc: 705.00 ng/ml

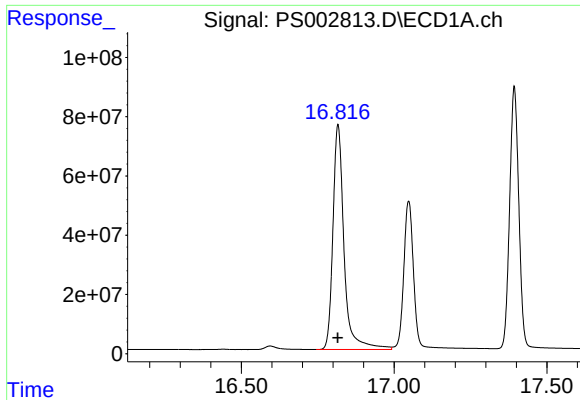

#15 Picloram


R.T.: 16.816 min
Delta R.T.: 0.000 min
Response: 1926968559
Conc: 712.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

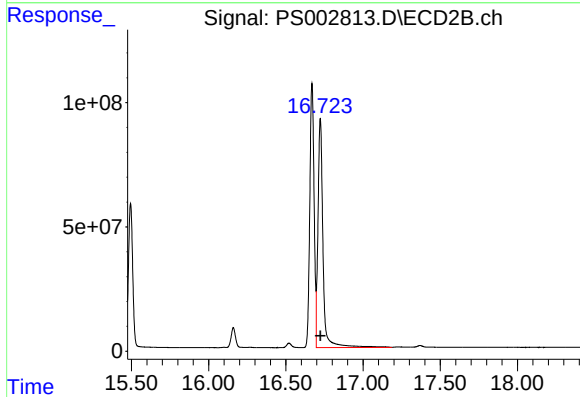


#15 Picloram

R.T.: 16.723 min
Delta R.T.: 0.000 min
Response: 2105330355
Conc: 712.50 ng/ml

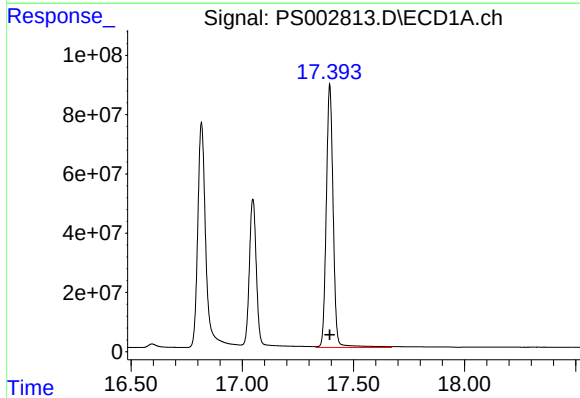

#16 DCPA

R.T.: 17.393 min
Delta R.T.: 0.000 min
Response: 1914019750
Conc: 720.00 ng/ml

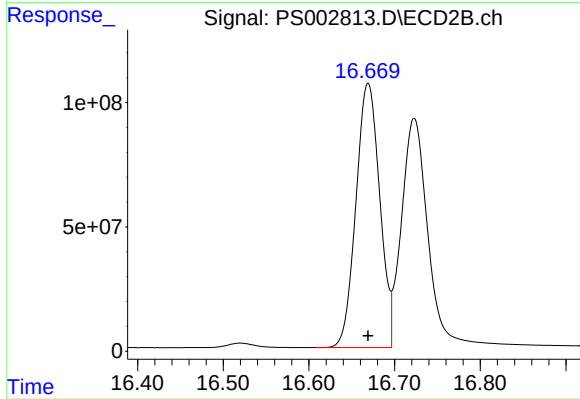

#16 DCPA

R.T.: 16.669 min
Delta R.T.: 0.000 min
Response: 2049999265
Conc: 720.00 ng/ml