

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS011720\
 Data File : PS008446.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Jan 2020 17:32
 Operator : DD\AJ
 Sample : PB126160TB
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 17 17:56:52 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010820.M
 Quant Title : 8080.M
 QLast Update : Wed Jan 08 11:00:59 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds

1) T	Dalapon	2.578	2.170	175.4E6	15370225	68.423	12.124 #
2) T	3,5-DICHL...	5.566	5.133	15216034	128.6E6	6.353	92.042 #
3) T	4-Nitroph...	6.122	5.649	30950578	14732291	31.778	24.812
5) T	DICAMBA	6.516	6.081	25774932	122.8E6	3.750	30.702 #
6) T	MCP	6.667	0.000	12320977	0	2.417	N.D. #
8) T	DICHLORPROP	0.000	6.766	0	33497310	N.D.	34.671
9) T	2,4-D	7.433	0.000	53182940	0	29.236	N.D. #
10) T	Pentachlo...	7.735	0.000	21700386	0	<MDL	N.D. #
15) T	Picloram	0.000	10.031	0	19556013	N.D.	2.632
16) T	DCPA	0.000	10.031	0	19556013	N.D.	3.001



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS011720\
Data File : PS008446.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Jan 2020 17:32
Operator : DD\AJ
Sample : PB126160TB
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 17 17:56:52 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010820.M
Quant Title : 8080.M
QLast Update : Wed Jan 08 11:00:59 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

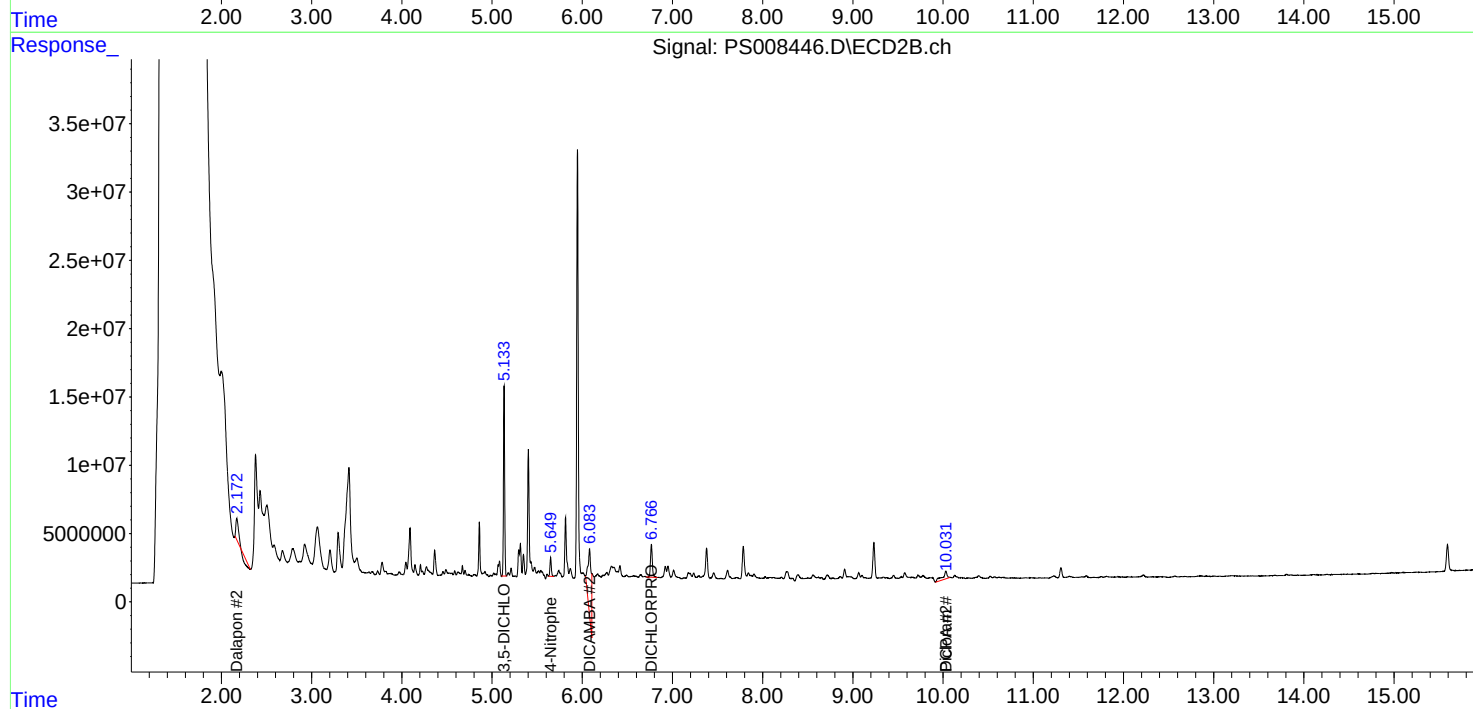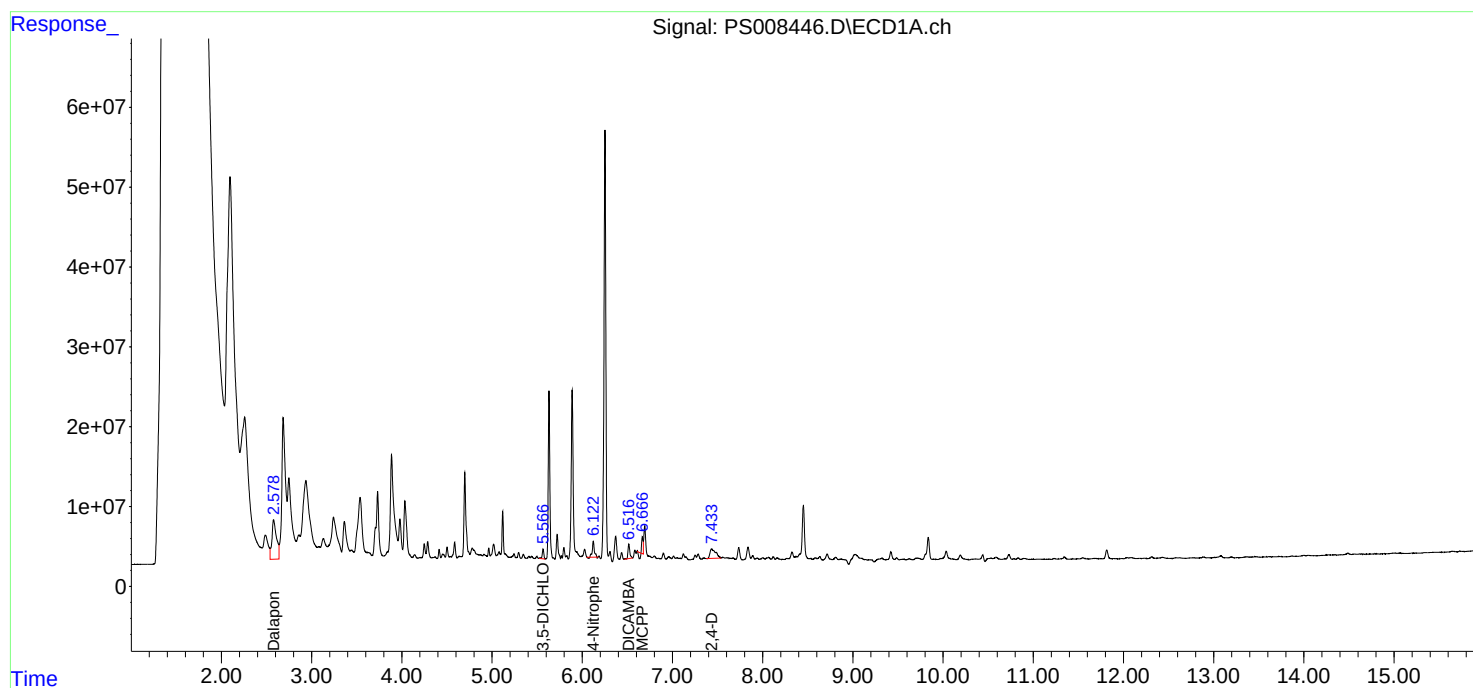


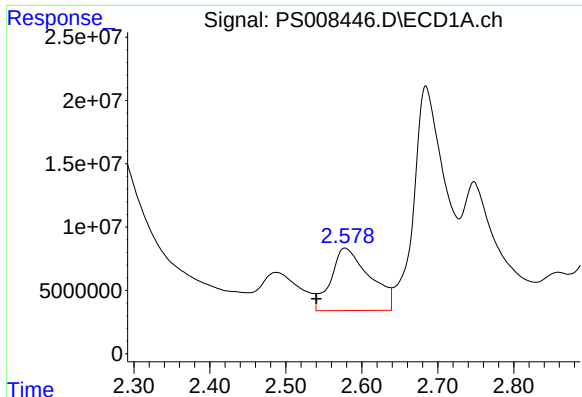

#1 Dalapon


R.T.: 2.578 min
Delta R.T.: 0.038 min
Response: 175426821
Conc: 68.42 ng/ml

Instrument :
ECD_S
ClientSampleId :

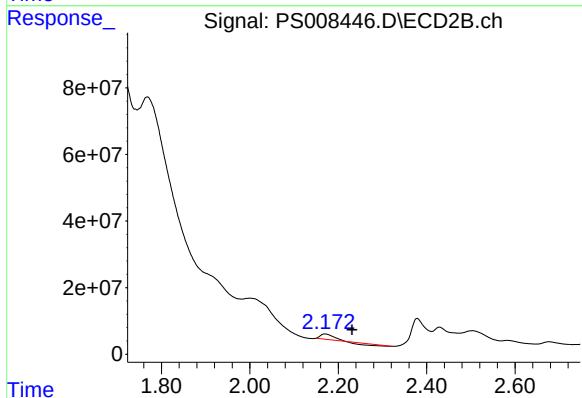


#1 Dalapon

R.T.: 2.170 min
Delta R.T.: -0.061 min
Response: 15370225
Conc: 12.12 ng/ml

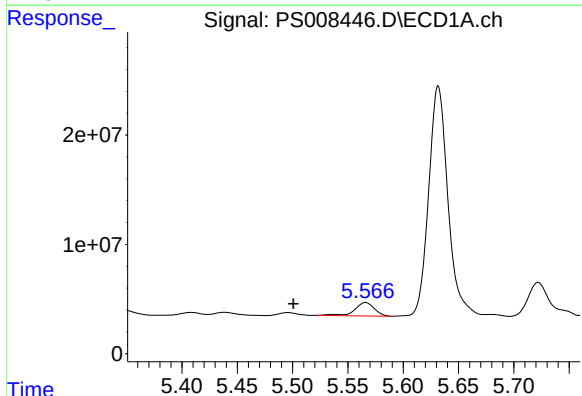


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 5.566 min
Delta R.T.: 0.065 min
Response: 15216034
Conc: 6.35 ng/ml

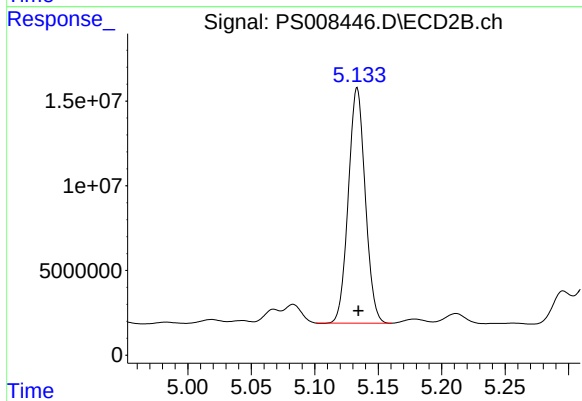

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 5.133 min
Delta R.T.: 0.000 min
Response: 128599096
Conc: 92.04 ng/ml

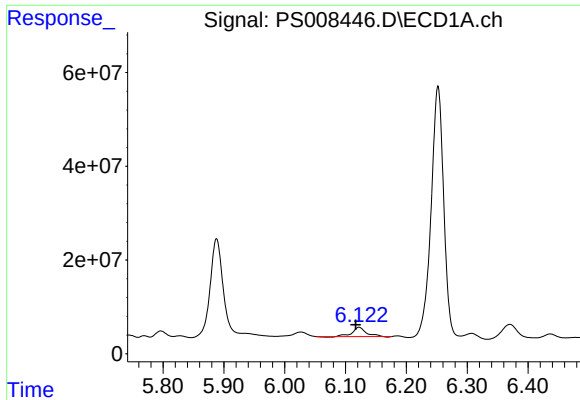

#3 4-Nitrophenol


R.T.: 6.122 min
Delta R.T.: 0.006 min
Response: 30950578
Conc: 31.78 ng/ml

Instrument :
ECD_S
ClientSampleId :

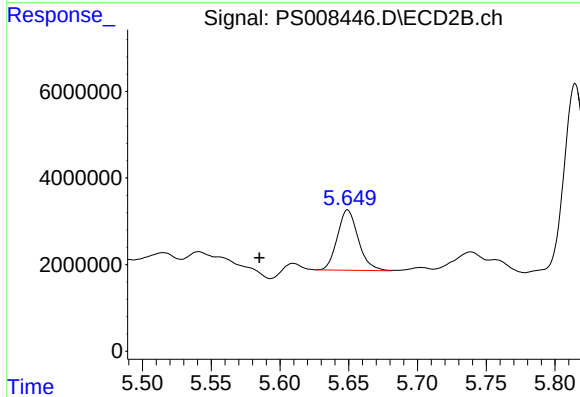


#3 4-Nitrophenol

R.T.: 5.649 min
Delta R.T.: 0.064 min
Response: 14732291
Conc: 24.81 ng/ml

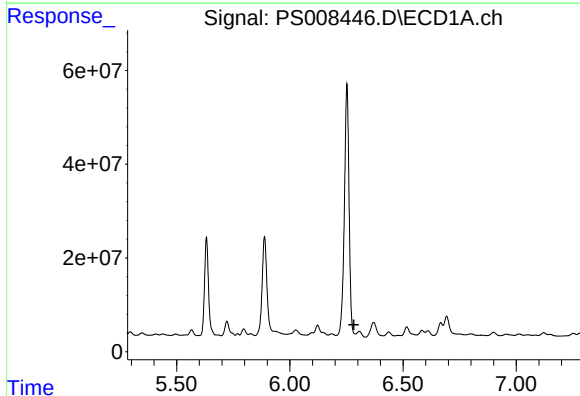


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 6.283 min
Response: 0
Conc: N.D.

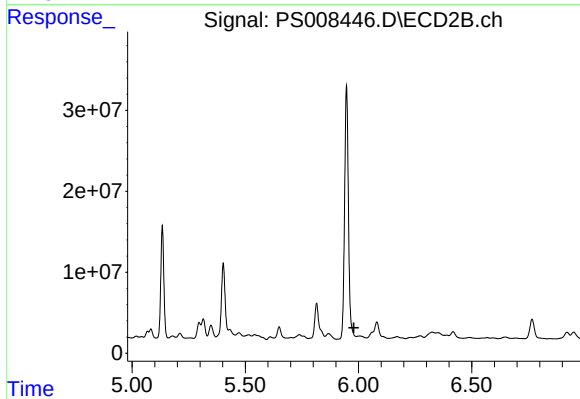

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T. : 5.979 min
Response: 0
Conc: N.D.

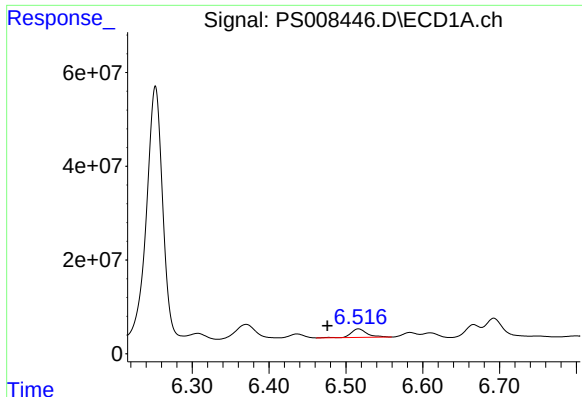

#5 DICAMBA


R.T.: 6.516 min
Delta R.T.: 0.040 min
Response: 25774932
Conc: 3.75 ng/ml

Instrument :
ECD_S
ClientSampleId :

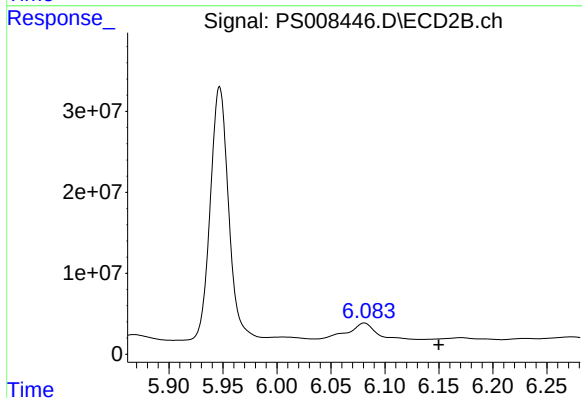


#5 DICAMBA

R.T.: 6.081 min
Delta R.T.: -0.069 min
Response: 122776772
Conc: 30.70 ng/ml

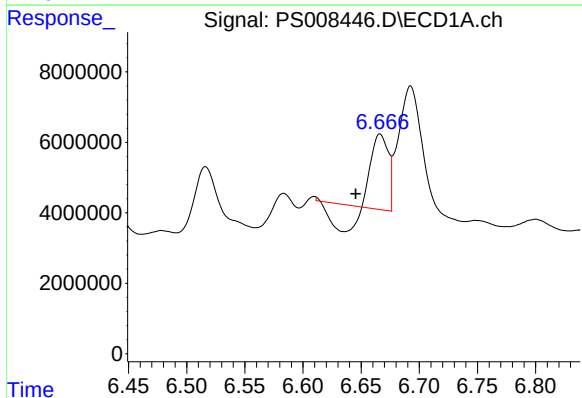


#6 MCP

R.T.: 6.667 min
Delta R.T.: 0.021 min
Response: 12320977
Conc: 2.42 ug/ml

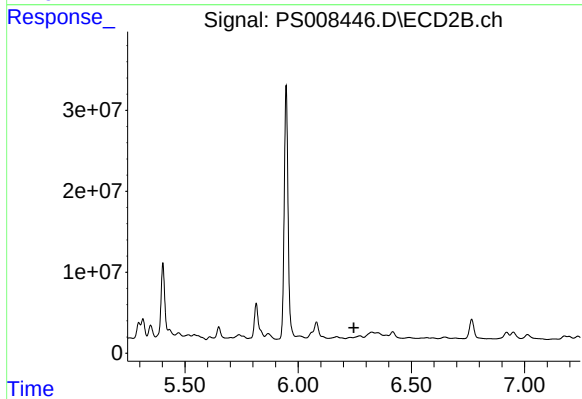

#6 MCP


R.T.: 0.000 min
Exp R.T.: 6.246 min
Response: 0
Conc: N.D.

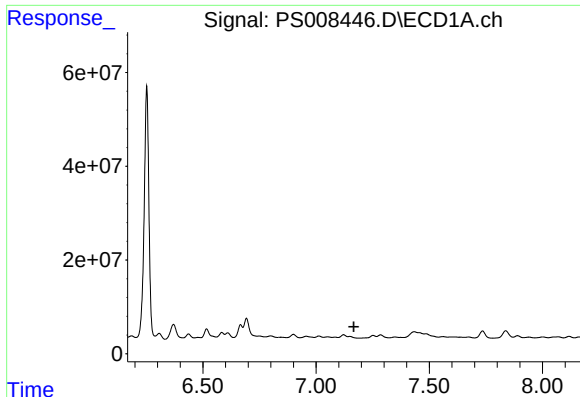

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 7.167 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

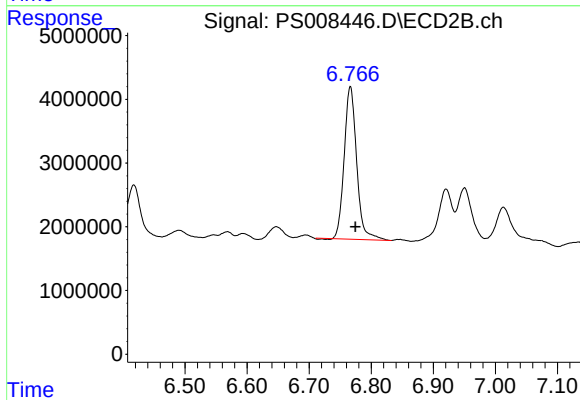


#8 DICHLORPROP

R.T.: 6.766 min
Delta R.T.: -0.008 min
Response: 33497310
Conc: 34.67 ng/ml

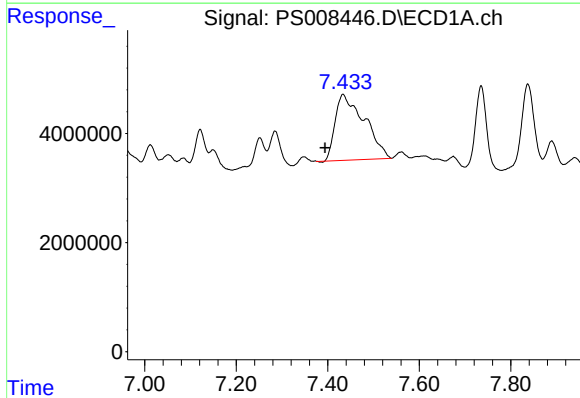


#9 2,4-D

R.T.: 7.433 min
Delta R.T.: 0.040 min
Response: 53182940
Conc: 29.24 ng/ml

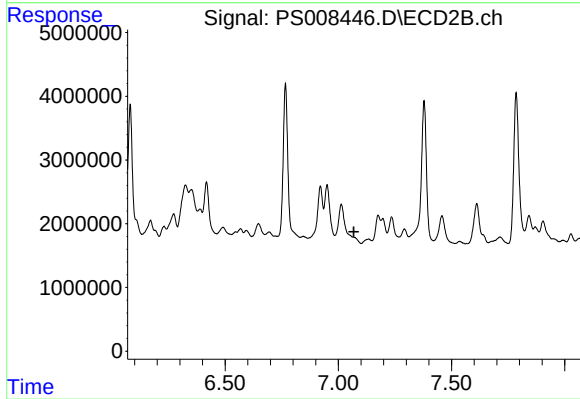

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 7.069 min
Response: 0
Conc: N.D.

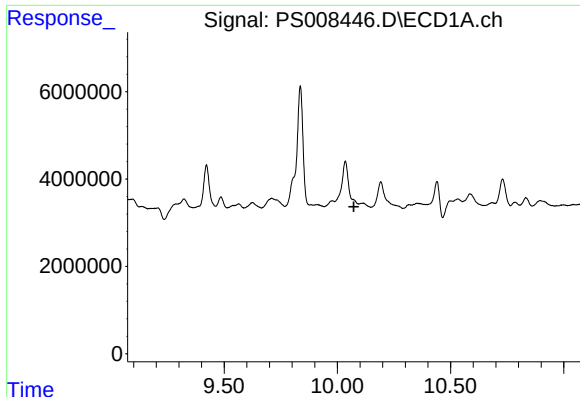

#15 Picloram


R.T.: 0.000 min
Exp R.T. : 10.073 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

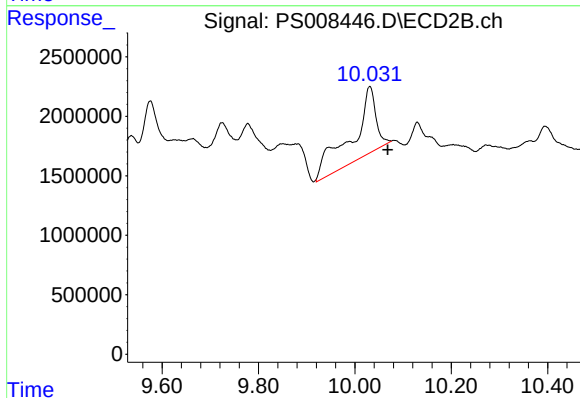


#15 Picloram

R.T.: 10.031 min
Delta R.T.: -0.037 min
Response: 19556013
Conc: 2.63 ng/ml

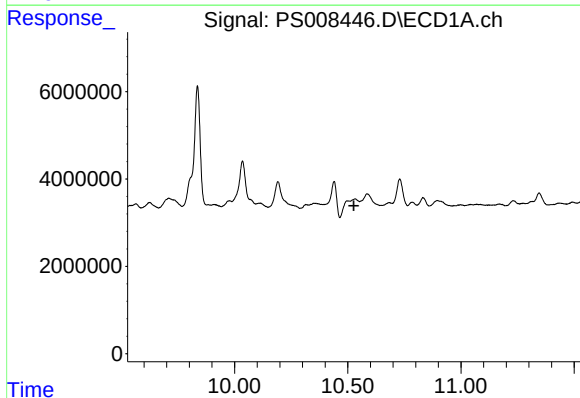

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 10.527 min
Response: 0
Conc: N.D.

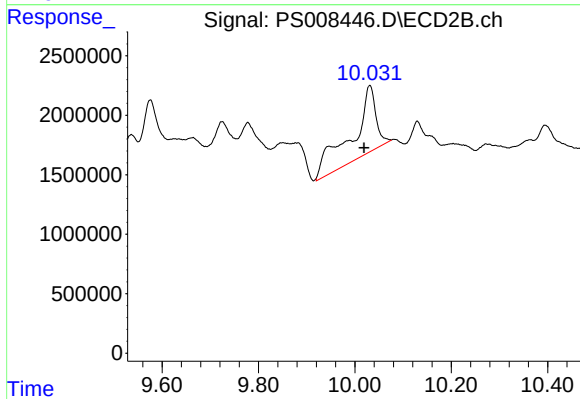

#16 DCPA

R.T.: 10.031 min
Delta R.T.: 0.012 min
Response: 19556013
Conc: 3.00 ng/ml