

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS011720\
 Data File : PS008450.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Jan 2020 18:59
 Operator : DD\AJ
 Sample : L1006-04
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HD-01-011520

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 17 22:31:42 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010820.M
 Quant Title : 8080.M
 QLast Update : Wed Jan 08 11:00:59 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.286	5.982	797.4E6	391.5E6	451.603	413.189
Target Compounds							
1) T	Dalapon	2.521	2.205	132.0E6	25346409	51.472	19.993 #
2) T	3,5-DICHL...	0.000	5.168	0	141.0E6	N.D.	100.909
3) T	4-Nitroph...	6.156	0.000	15979346	0	16.406	N.D. #
6) T	MCP	6.593	0.000	11692329	0	2.294	N.D. #
7) T	MCPA	6.727	0.000	69192533	0	9.469	N.D. #
8) T	DICHLORPROP	0.000	6.801	0	20348561	N.D.	21.062
10) T	Pentachlo...	7.768	0.000	22244413	0	<MDL	N.D. #
11) T	2,4,5-TP ...	0.000	7.842	0	12945318	N.D.	2.477
12) T	2,4,5-T	8.484	0.000	129.2E6	0	13.998	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS011720\
Data File : PS008450.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Jan 2020 18:59
Operator : DD\AJ
Sample : L1006-04
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HD-01-011520

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 17 22:31:42 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010820.M
Quant Title : 8080.M
QLast Update : Wed Jan 08 11:00:59 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

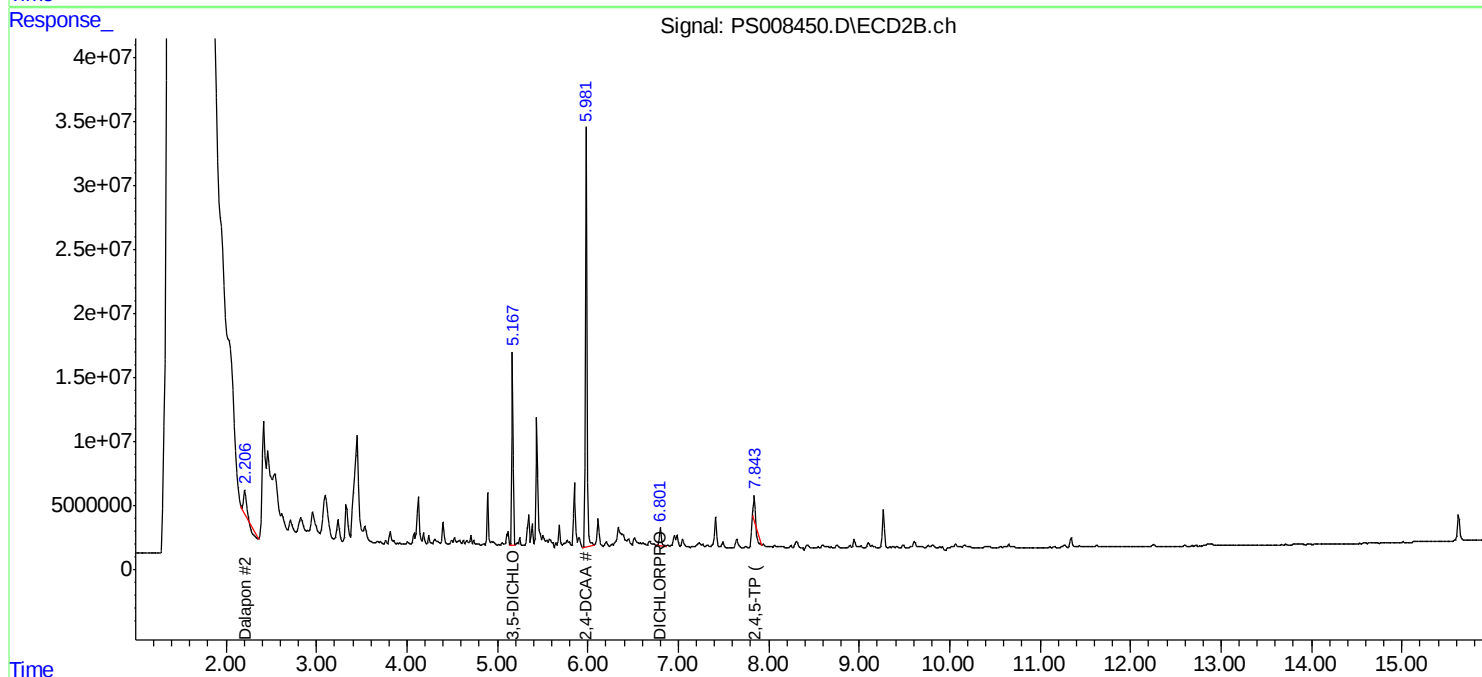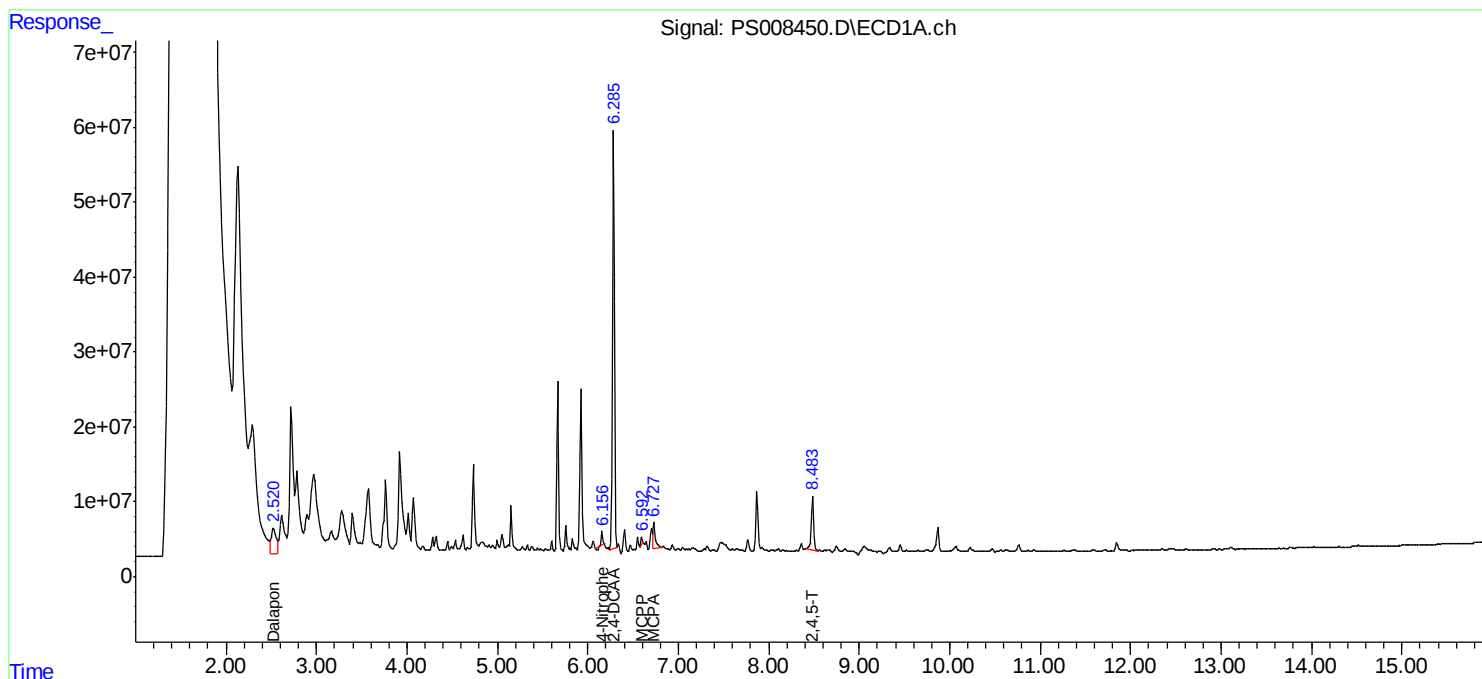


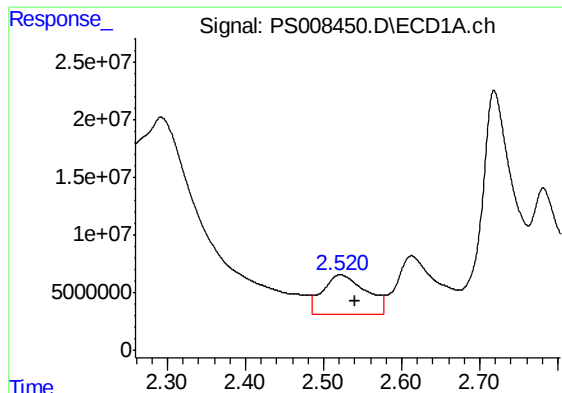

#1 Dalapon


R.T.: 2.521 min
Delta R.T.: -0.019 min
Response: 131965505
Conc: 51.47 ng/ml

Instrument :
ECD_S
ClientSampleId :
HD-01-011520

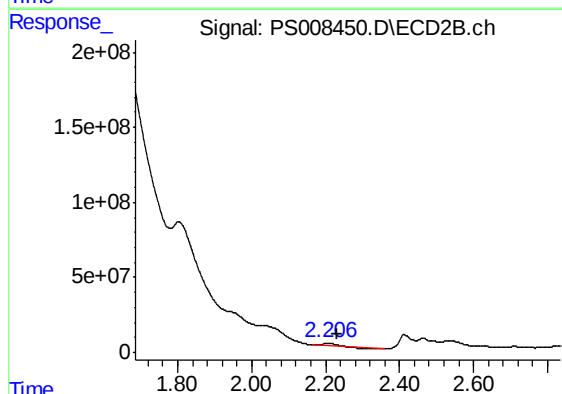


#1 Dalapon

R.T.: 2.205 min
Delta R.T.: -0.026 min
Response: 25346409
Conc: 19.99 ng/ml

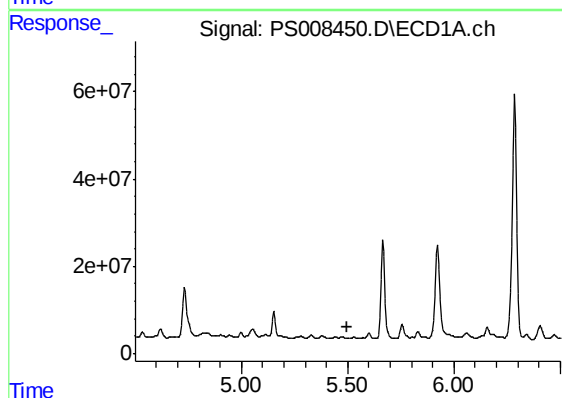


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 5.501 min
Response: 0
Conc: N.D.

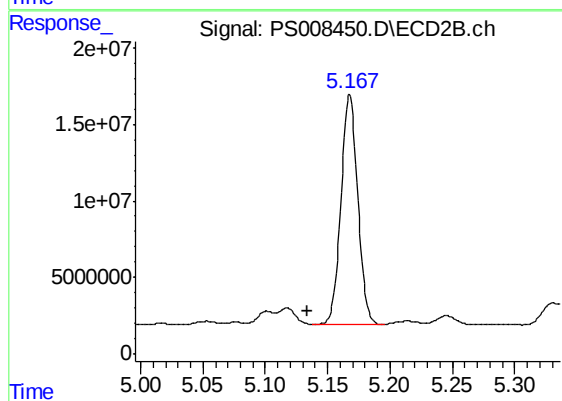

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 5.168 min
Delta R.T.: 0.033 min
Response: 140987521
Conc: 100.91 ng/ml

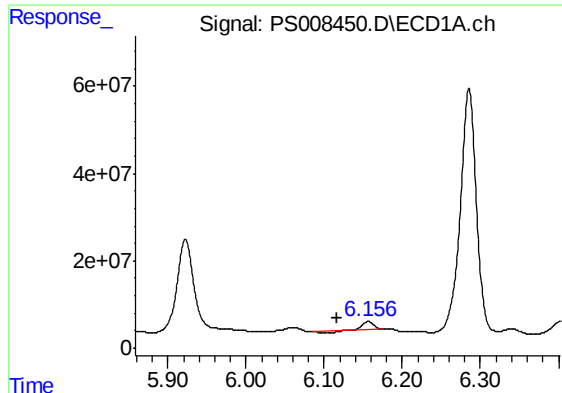

#3 4-Nitrophenol


R.T.: 6.156 min
Delta R.T.: 0.040 min
Response: 15979346
Conc: 16.41 ng/ml

Instrument :
ECD_S
ClientSampleId :
HD-01-011520

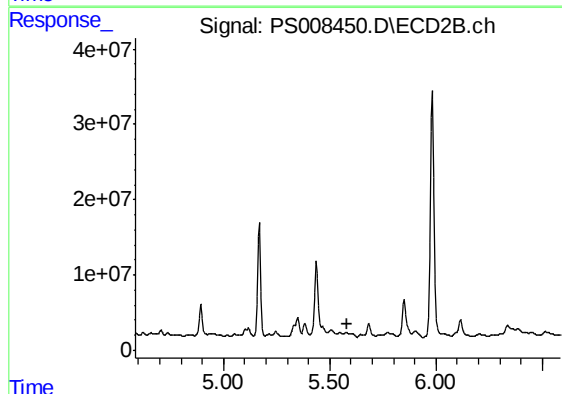


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 5.585 min
Response: 0
Conc: N.D.

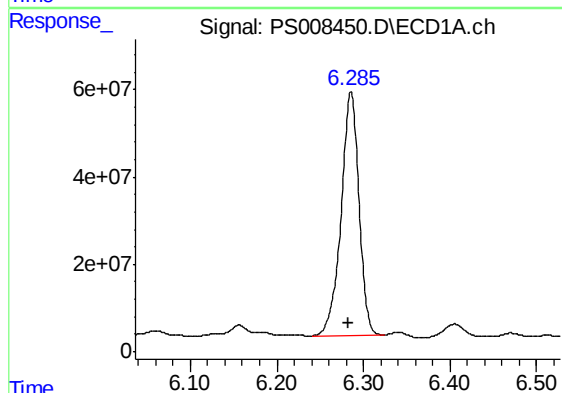


#4 2,4-DCAA

R.T.: 6.286 min
Delta R.T.: 0.003 min
Response: 797397035
Conc: 451.60 ng/ml

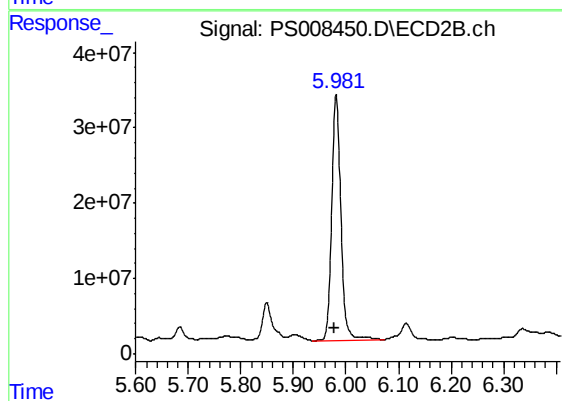

#4 2,4-DCAA


R.T.: 5.982 min
Delta R.T.: 0.002 min
Response: 391481547
Conc: 413.19 ng/ml

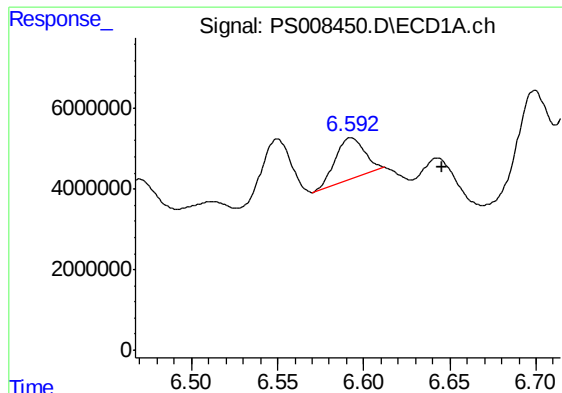

#6 MCPP


R.T.: 6.593 min
Delta R.T.: -0.053 min
Response: 11692329
Conc: 2.29 ug/ml

Instrument :
ECD_S
ClientSampleId :
HD-01-011520

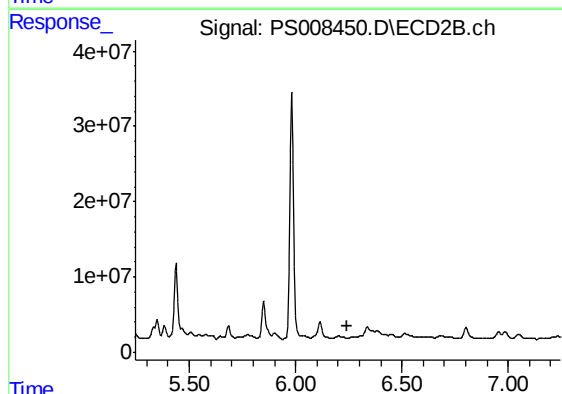


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 6.246 min
Response: 0
Conc: N.D.

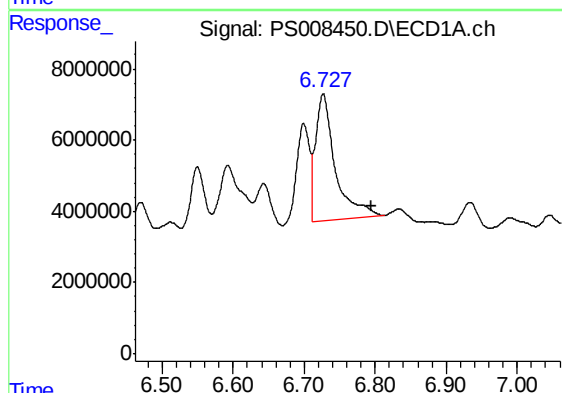


#7 MCPA

R.T.: 6.727 min
Delta R.T.: -0.067 min
Response: 69192533
Conc: 9.47 ug/ml

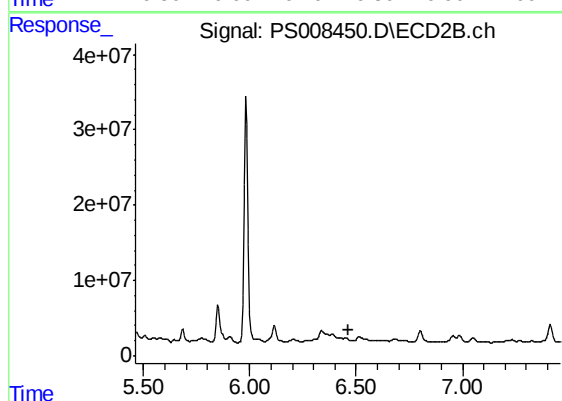

#7 MCPA


R.T.: 0.000 min
Exp R.T. : 6.462 min
Response: 0
Conc: N.D.

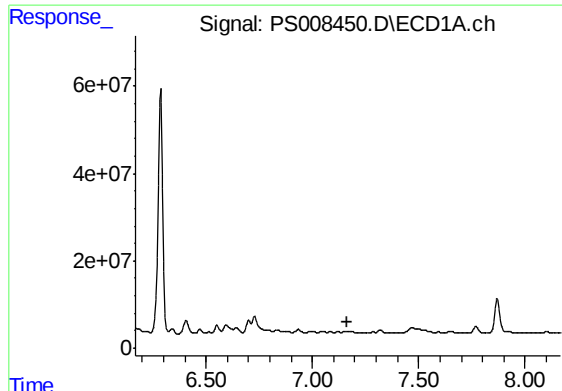

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 7.167 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HD-01-011520

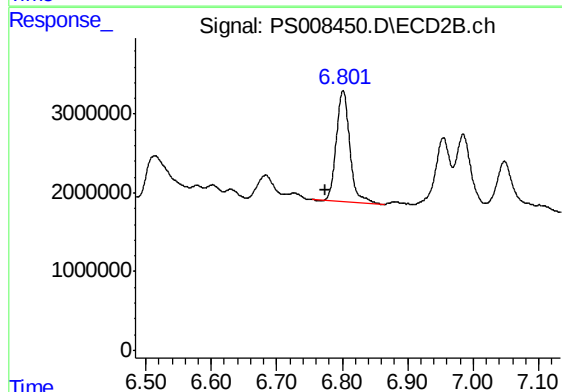


#8 DICHLORPROP

R.T.: 6.801 min
Delta R.T.: 0.027 min
Response: 20348561
Conc: 21.06 ng/ml

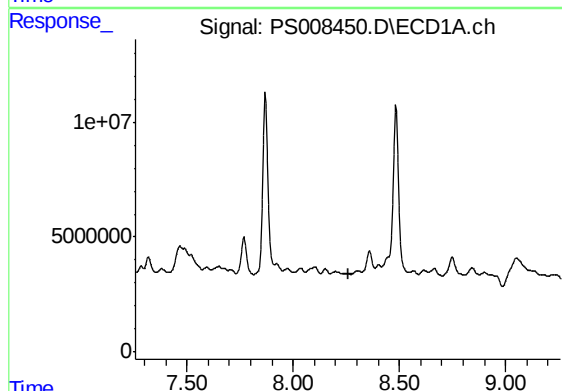


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 8.258 min
Response: 0
Conc: N.D.

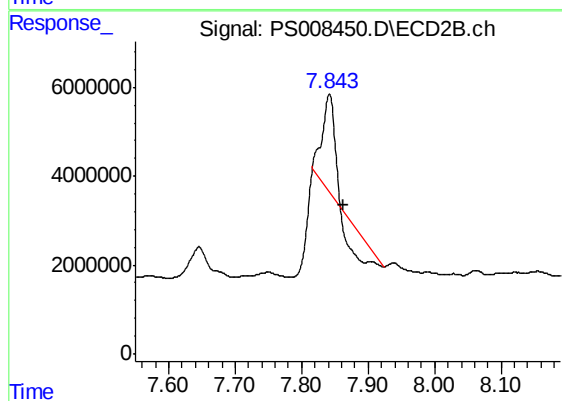

#11 2,4,5-TP (SILVEX)


R.T.: 7.842 min
Delta R.T.: -0.022 min
Response: 12945318
Conc: 2.48 ng/ml

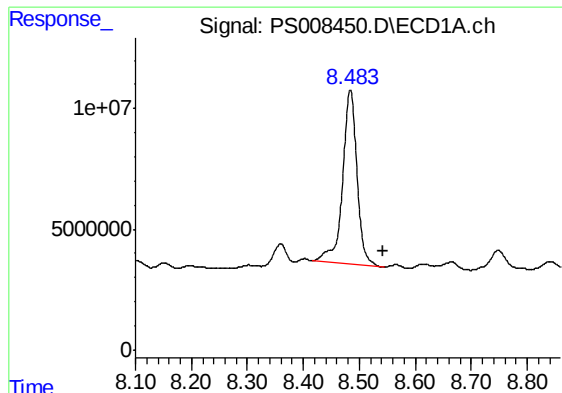

#12 2,4,5-T

R.T.: 8.484 min
Delta R.T.: -0.057 min
Response: 129154685
Conc: 14.00 ng/ml

Instrument :
ECD_S
ClientSampleId :
HD-01-011520

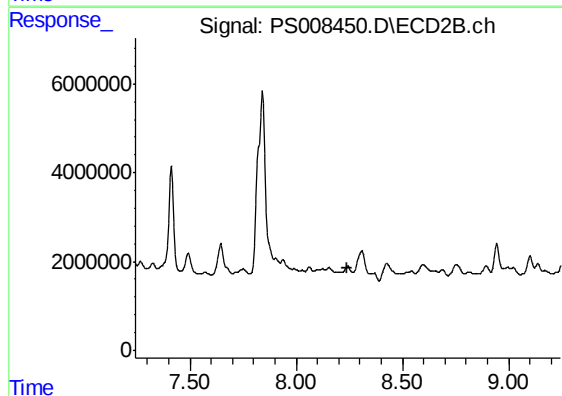

#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 8.243 min
Response: 0
Conc: N.D.