

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS011720\
 Data File : PS008453.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Jan 2020 20:05
 Operator : DD\AJ
 Sample : L1126-06
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 WASTE-CHARACTERIZATION

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 17 22:32:24 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010820.M
 Quant Title : 8080.M
 QLast Update : Wed Jan 08 11:00:59 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.270	5.966	743.7E6	389.8E6	421.219	411.407
Target Compounds							
1) T	Dalapon	2.506	2.189	124.8E6	33992985	48.689	26.814 #
2) T	3,5-DICHL...	0.000	5.152	0	111.1E6	N.D.	79.530
3) T	4-Nitroph...	6.140	0.000	24065499	0	24.709	N.D. #
6) T	MCP	6.684	0.000	31088435	0	6.100	N.D. #
8) T	DICHLORPROP	0.000	6.786	0	12488897	N.D.	12.926
10) T	Pentachlo...	7.752	0.000	24929022	0	1.025	N.D. #
11) T	2,4,5-TP ...	0.000	7.805	0	7957088	N.D.	1.522



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS011720\
Data File : PS008453.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Jan 2020 20:05
Operator : DD\AJ
Sample : L1126-06
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
WASTE-CHARACTERIZATION

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 17 22:32:24 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010820.M
Quant Title : 8080.M
QLast Update : Wed Jan 08 11:00:59 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

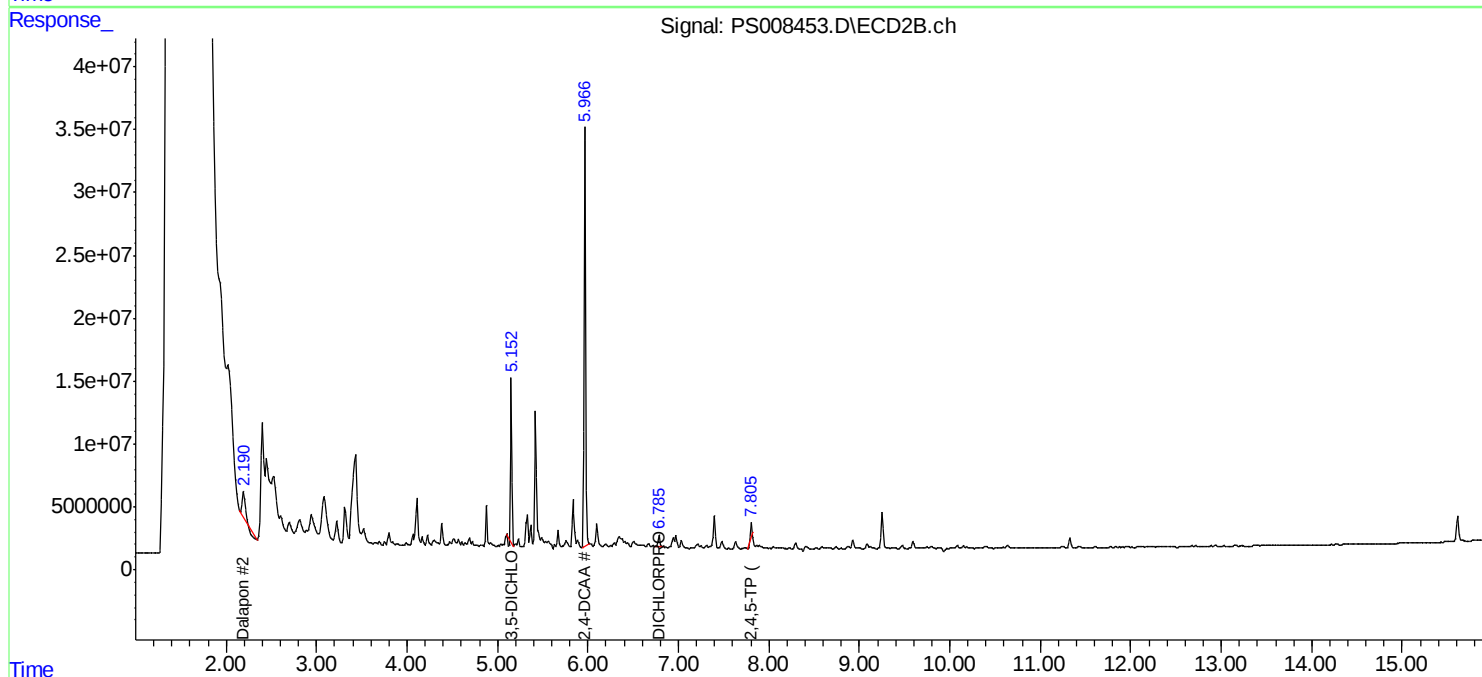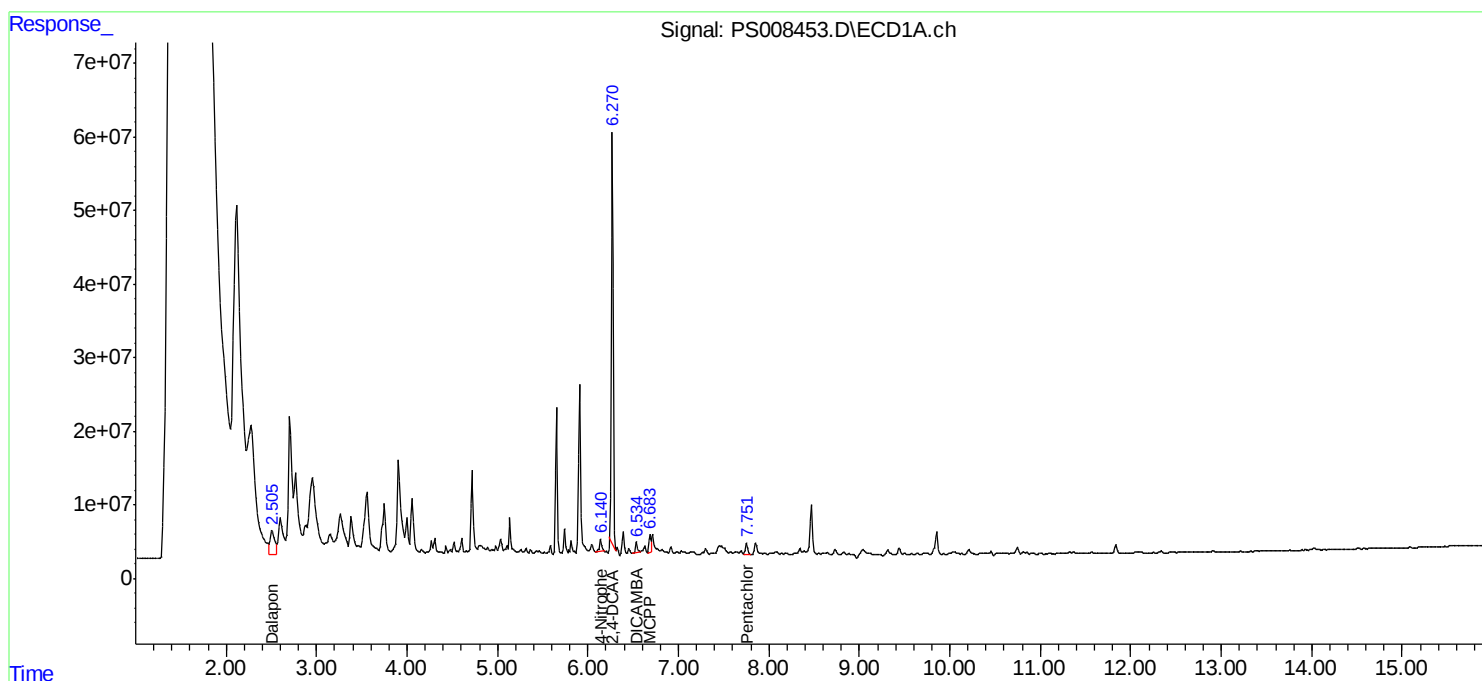


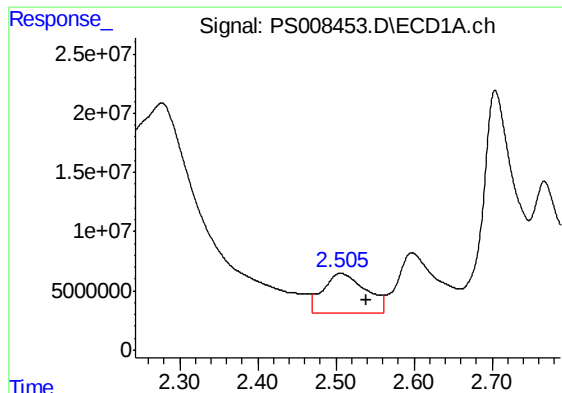

#1 Dalapon


R.T.: 2.506 min
Delta R.T.: -0.034 min
Response: 124832479
Conc: 48.69 ng/ml

Instrument :
ECD_S
ClientSampleId :
WASTE-CHARACTERIZATION

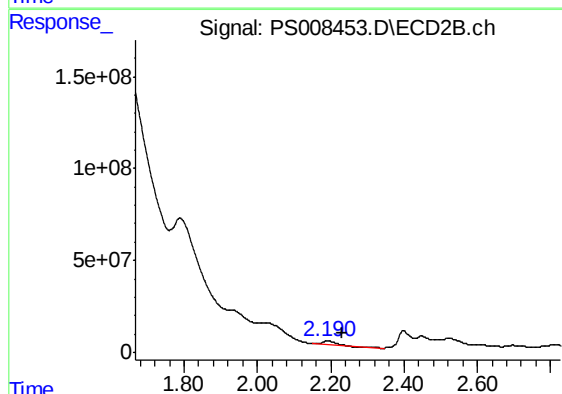


#1 Dalapon

R.T.: 2.189 min
Delta R.T.: -0.042 min
Response: 33992985
Conc: 26.81 ng/ml

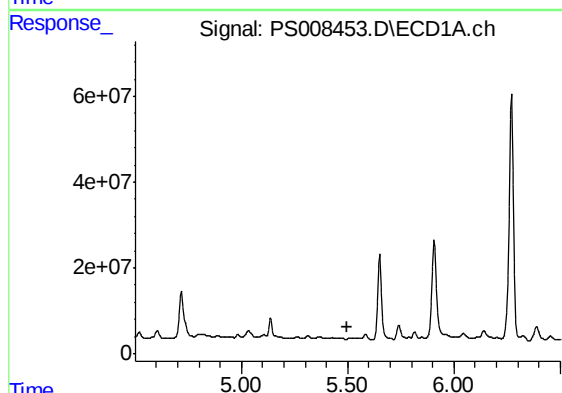


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 5.501 min
Response: 0
Conc: N.D.

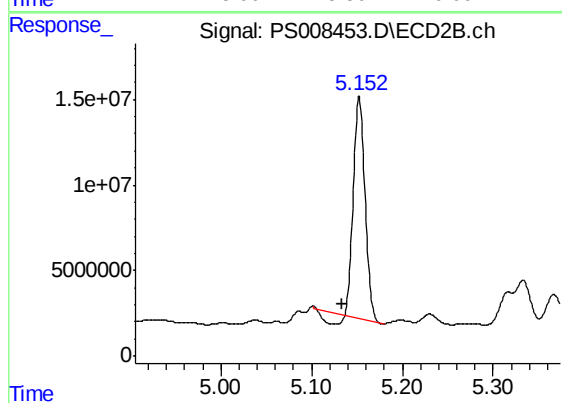

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 5.152 min
Delta R.T.: 0.018 min
Response: 111116839
Conc: 79.53 ng/ml

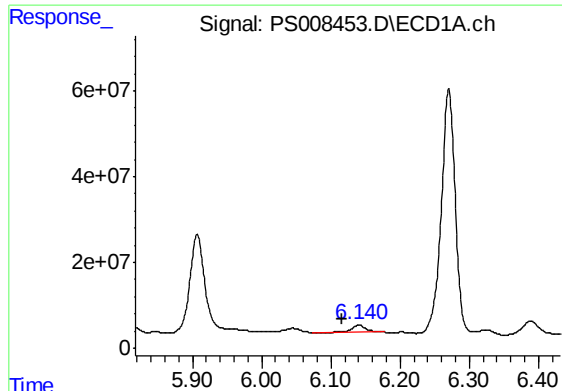

#3 4-Nitrophenol


R.T.: 6.140 min
Delta R.T.: 0.024 min
Response: 24065499
Conc: 24.71 ng/ml

Instrument :
ECD_S
ClientSampleId :
WASTE-CHARACTERIZATION

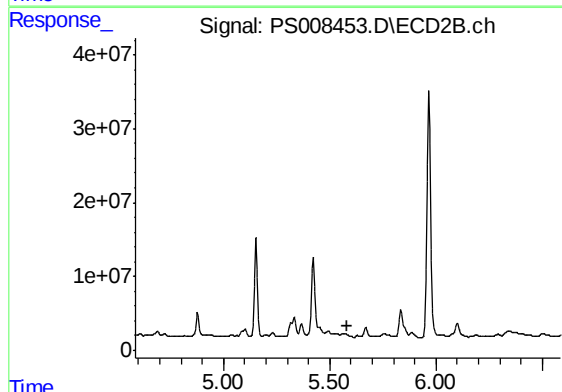


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 5.585 min
Response: 0
Conc: N.D.

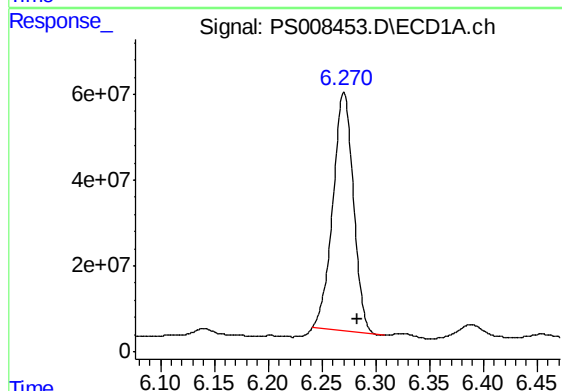


#4 2,4-DCAA

R.T.: 6.270 min
Delta R.T.: -0.012 min
Response: 743748118
Conc: 421.22 ng/ml

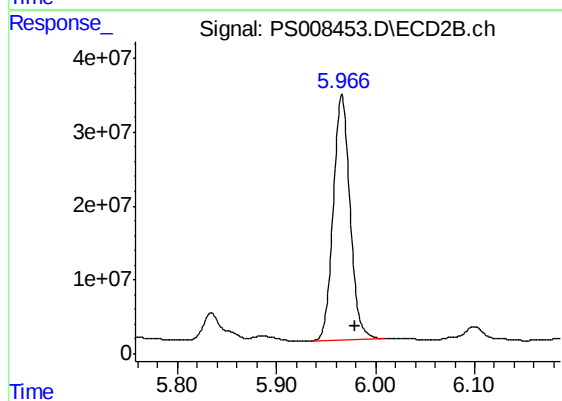

#4 2,4-DCAA


R.T.: 5.966 min
Delta R.T.: -0.013 min
Response: 389793279
Conc: 411.41 ng/ml

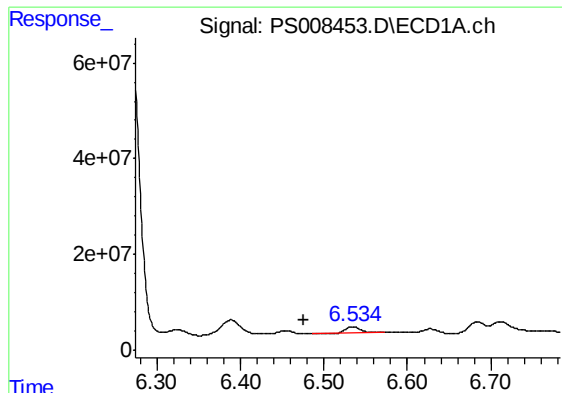

#5 DICAMBA


R.T.: 6.534 min
Delta R.T.: 0.058 min
Response: 16828763
Conc: 2.45 ng/ml

Instrument :
ECD_S
ClientSampleId :
WASTE-CHARACTERIZATION

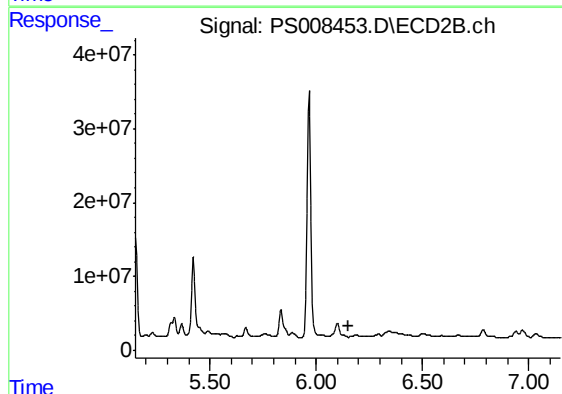


#5 DICAMBA

R.T.: 6.100 min
Delta R.T.: -0.050 min
Response: -12631523
Conc: N.D.

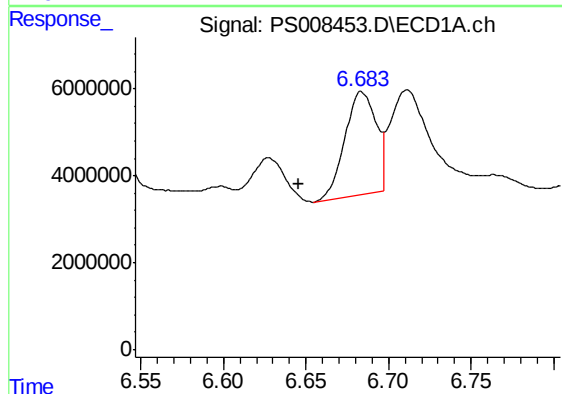


#6 MCPP

R.T.: 6.684 min
Delta R.T.: 0.038 min
Response: 31088435
Conc: 6.10 ug/ml

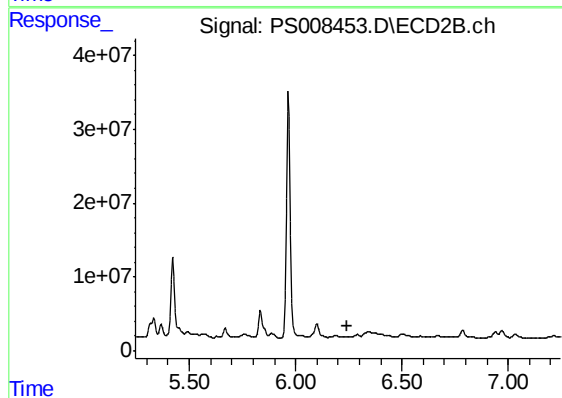

#6 MCPP


R.T.: 0.000 min
Exp R.T.: 6.246 min
Response: 0
Conc: N.D.

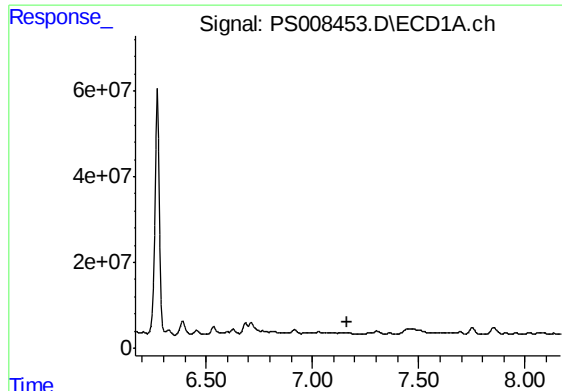

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T. : 7.167 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
WASTE-CHARACTERIZATION

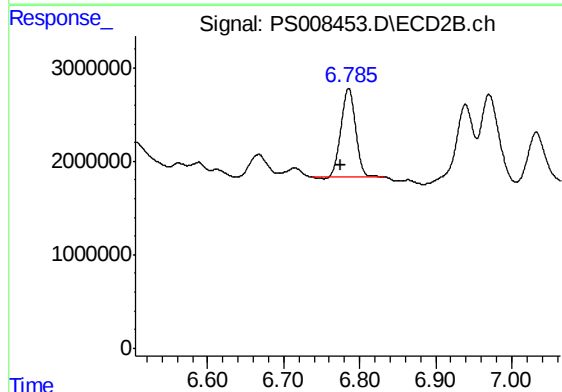


#8 DICHLORPROP

R.T.: 6.786 min
Delta R.T.: 0.011 min
Response: 12488897
Conc: 12.93 ng/ml

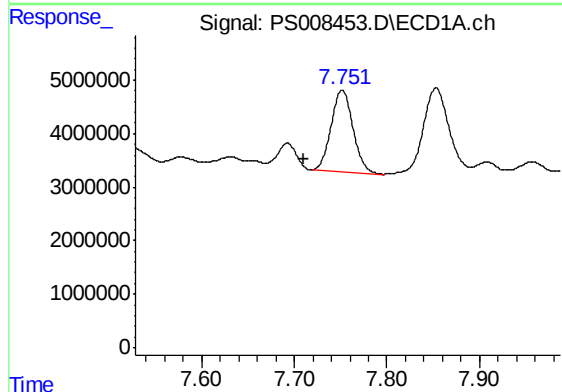


#10 Pentachlorophenol

R.T.: 7.752 min
Delta R.T.: 0.041 min
Response: 24929022
Conc: 1.03 ng/ml

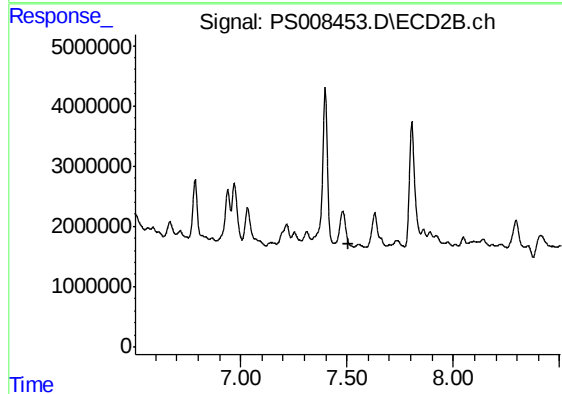

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T. : 7.505 min
Response: 0
Conc: N.D.

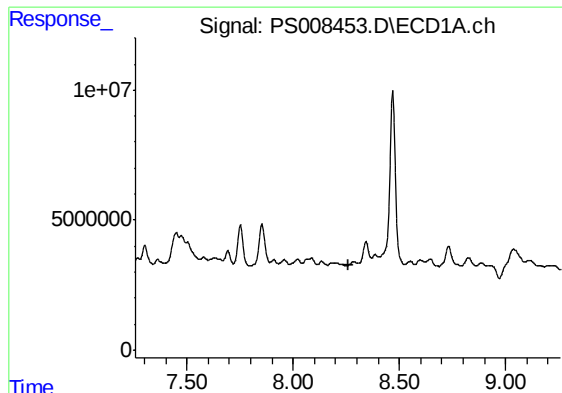

#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 8.258 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
WASTE-CHARACTERIZATION

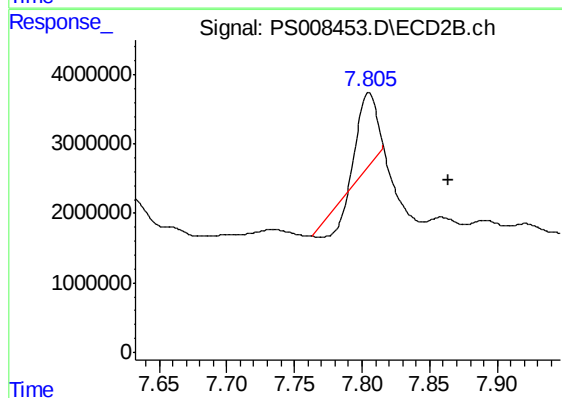

#11 2,4,5-TP (SILVEX)

R.T.: 7.805 min
Delta R.T.: -0.059 min
Response: 7957088
Conc: 1.52 ng/ml