

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS011720\
 Data File : PS008453.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Jan 2020 20:05
 Operator : DD\AJ
 Sample : L1126-06
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 WASTE-CHARACTERIZATION

Manual Integrations
 APPROVED

Ankita
 1/20/2020 9:32:06 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 17 22:32:24 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010820.M
 Quant Title : 8080.M
 QLast Update : Wed Jan 08 11:00:59 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
4) S 2,4-DCAA	6.270	5.966	790.4E6	389.8E6	447.650m	411.407

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS011720\
Data File : PS008453.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Jan 2020 20:05
Operator : DD\AJ
Sample : L1126-06
Misc :
ALS Vial : 13 Sample Multiplier: 1



Instrument :
ECD_S
ClientSampleId :
WASTE-CHARACTERIZATION


Manual Integrations
APPROVED

Ankita
1/20/2020 9:32:06 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 17 22:32:24 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010820.M
Quant Title : 8080.M
QLast Update : Wed Jan 08 11:00:59 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

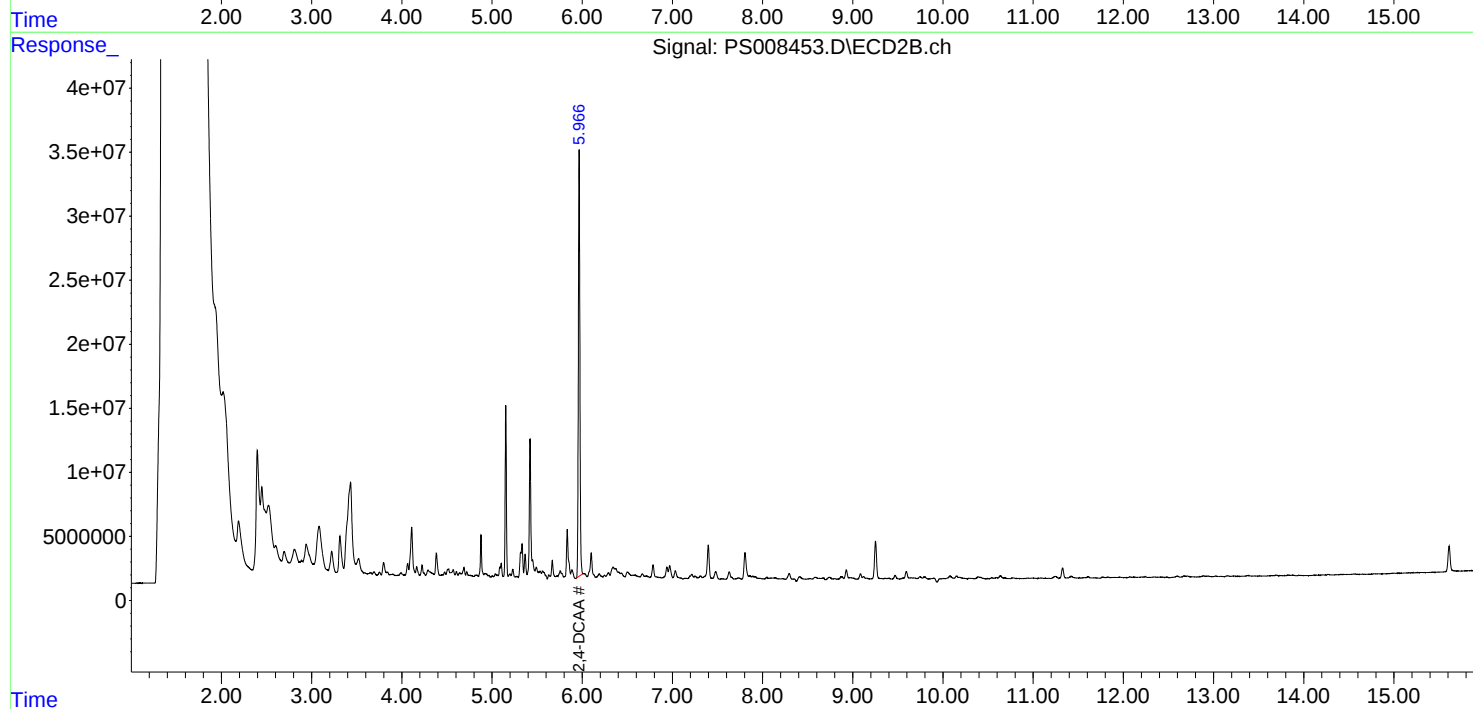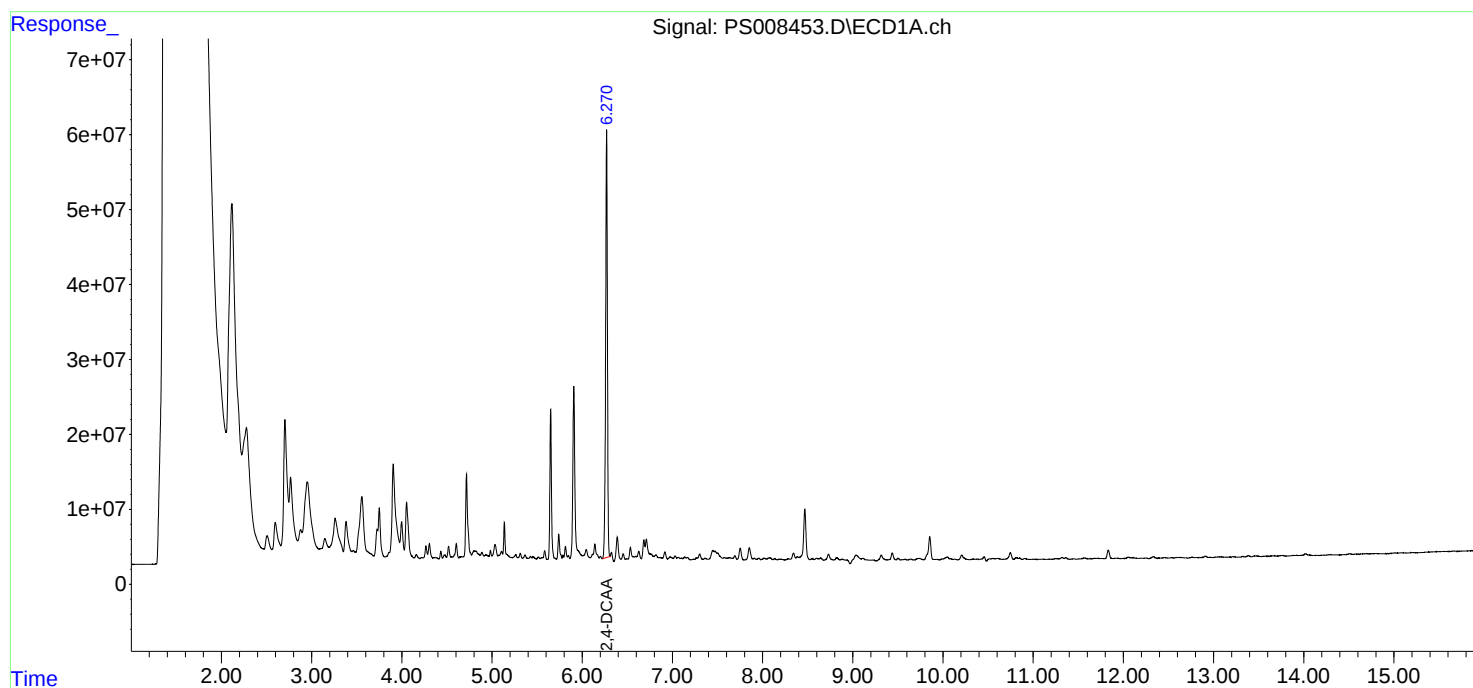

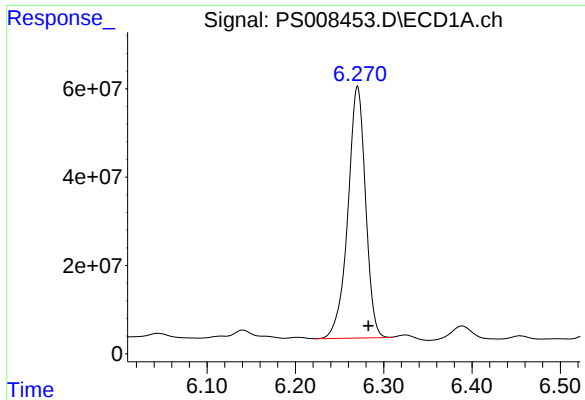


#4 2,4-DCAA

R.T.: 6.270 min
Delta R.T.: -0.013 min
Response: 790417874
Conc: 447.65 ng/ml m

Instrument :
ECD_S
ClientSampleId :
WASTE-CHARACTERIZATION

Manual Integrations
APPROVED

Ankita
1/20/2020 9:32:06 AM

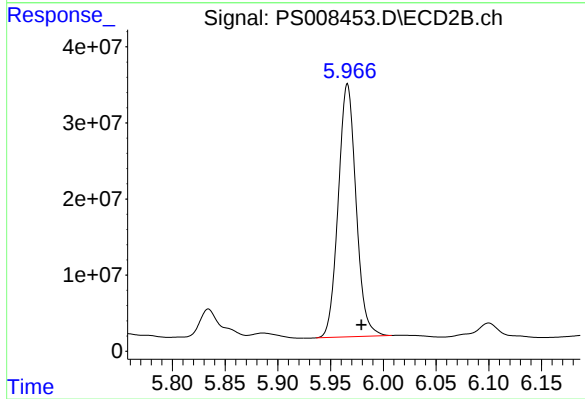

#4 2,4-DCAA

R.T.: 5.966 min
Delta R.T.: -0.013 min
Response: 389793279
Conc: 411.41 ng/ml